

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ061523\
 Data File : PQ061468.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jun 2023 20:41
 Operator : YP\AJ
 Sample : 03241-01
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 30852

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/16/2023
 Supervised By :Ankita Jodhani 06/16/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 16 05:22:56 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ060923.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 09 18:19:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.406	2.761	92530610	51151346	20.585	19.155m
2) SA Decachlor...	8.590	7.540	64513300	45089469	19.151	13.433 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ061523\
Data File : PQ061468.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jun 2023 20:41
Operator : YP\AJ
Sample : 03241-01
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
30852


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/16/2023
Supervised By :Ankita Jodhani 06/16/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 16 05:22:56 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ060923.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 09 18:19:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

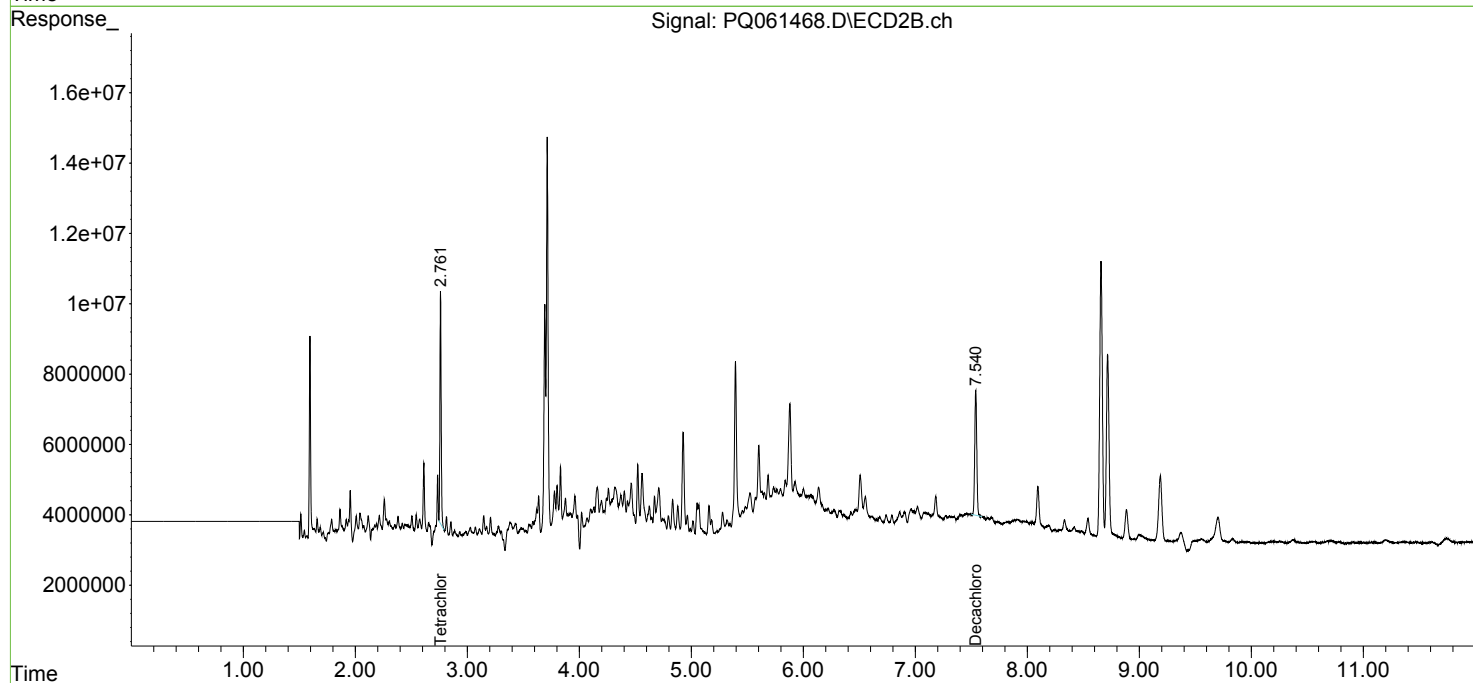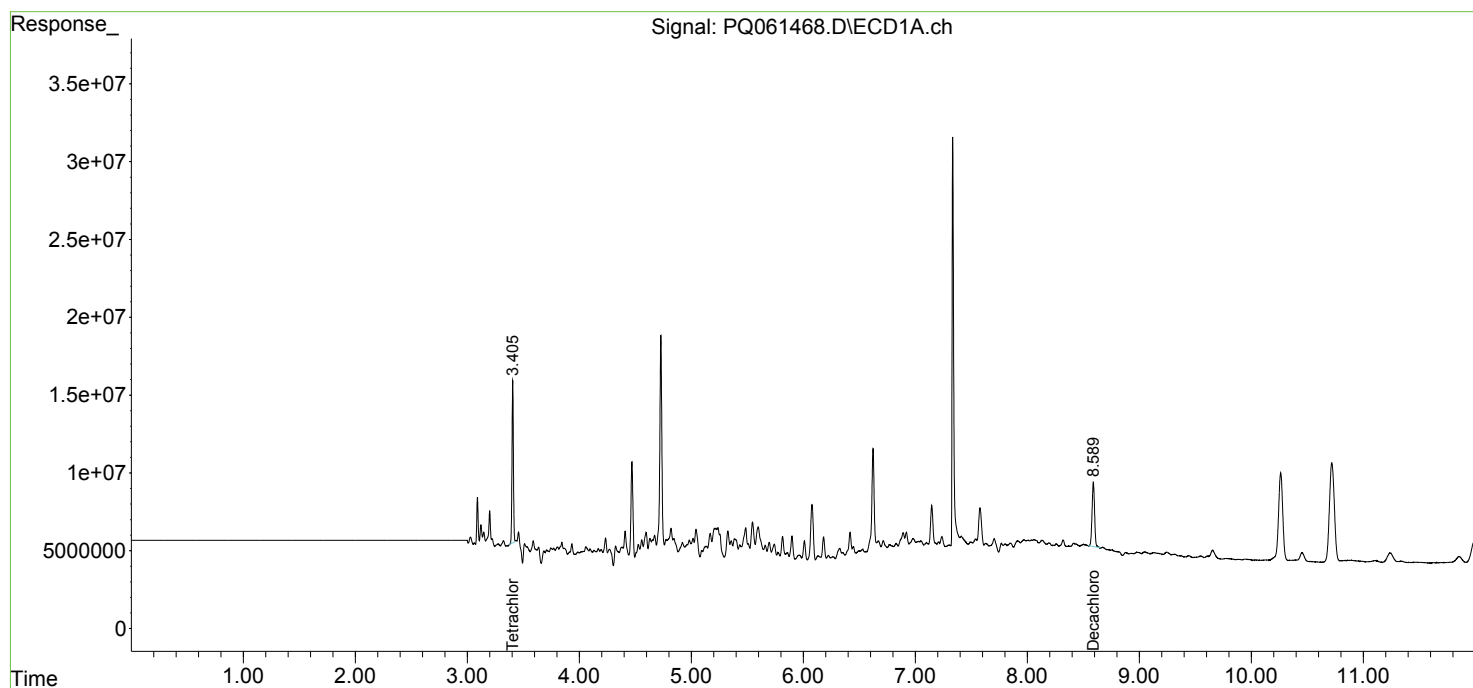

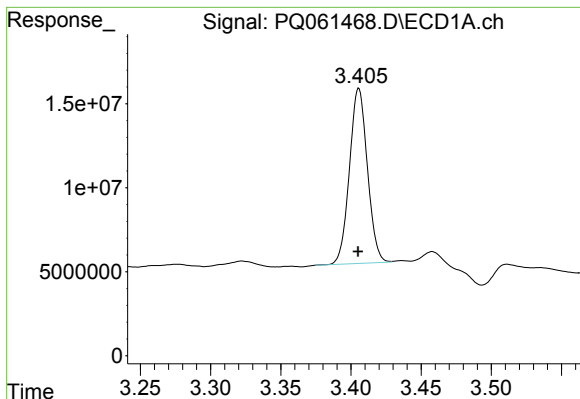


#1 Tetrachloro-m-xylene

R.T.: 3.406 min
Delta R.T.: 0.000 min
Response: 92530610
Conc: 20.59 ng/ml

Instrument :
ECD_Q
ClientSampleId :
30852


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/16/2023
Supervised By :Ankita Jodhani 06/16/2023

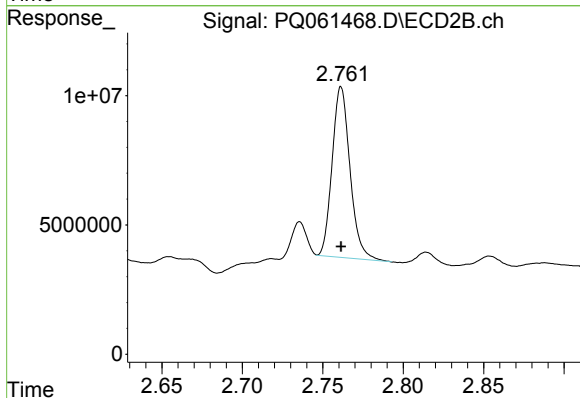


#1 Tetrachloro-m-xylene

R.T.: 2.761 min
Delta R.T.: 0.000 min
Response: 51151346
Conc: 19.16 ng/ml m

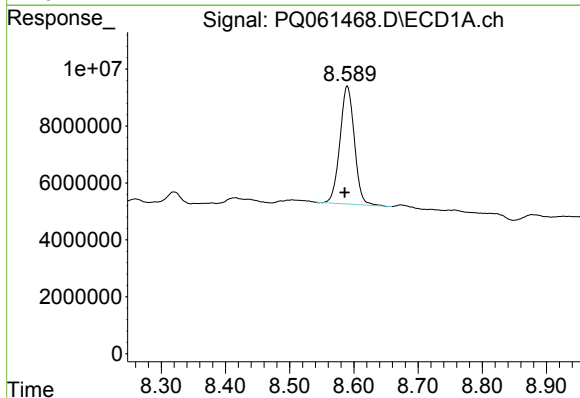

#2 Decachlorobiphenyl

R.T.: 8.590 min
Delta R.T.: 0.004 min
Response: 64513300
Conc: 19.15 ng/ml

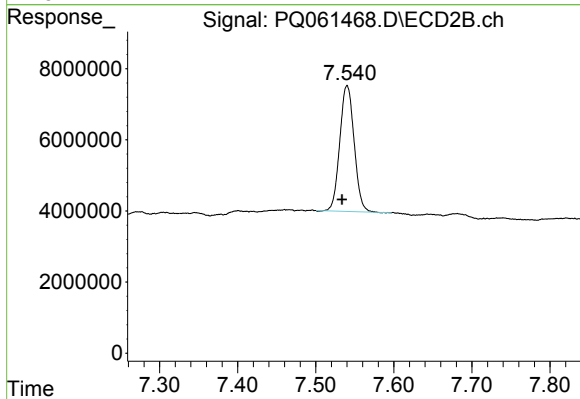

#2 Decachlorobiphenyl

R.T.: 7.540 min
Delta R.T.: 0.006 min
Response: 45089469
Conc: 13.43 ng/ml