

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ061623\
 Data File : PQ061486.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jun 2023 17:11
 Operator : YP\AJ
 Sample : 03251-01RE
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 MW-01RE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/19/2023
 Supervised By :Ankita Jodhani 06/19/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 16 17:37:31 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ060923.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 09 18:19:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.405	2.760	106.2E6	59412341	23.623	22.249m
2) SA Decachlor...	8.585	7.533	78426329	95687159	23.281	28.508

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ061623\
Data File : PQ061486.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jun 2023 17:11
Operator : YP\AJ
Sample : 03251-01RE
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
MW-01RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/19/2023
Supervised By :Ankita Jodhani 06/19/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 16 17:37:31 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ060923.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 09 18:19:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

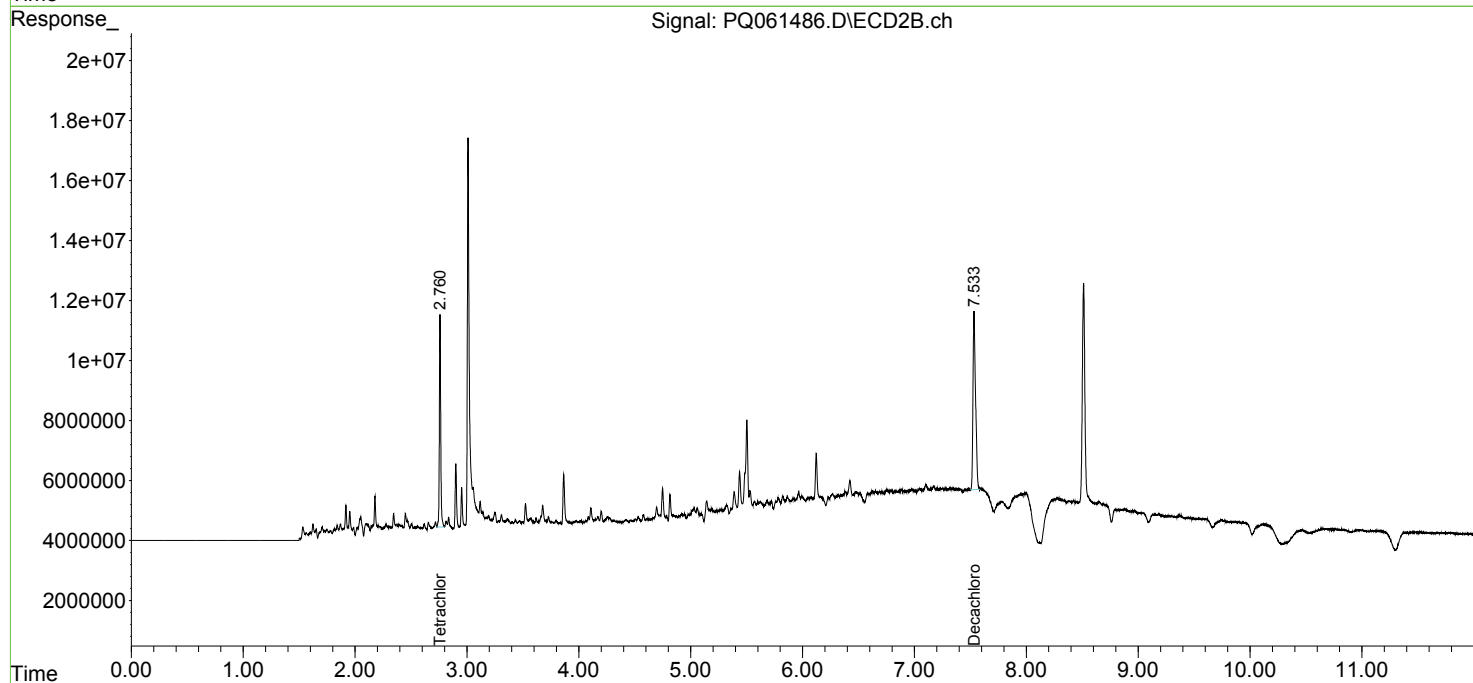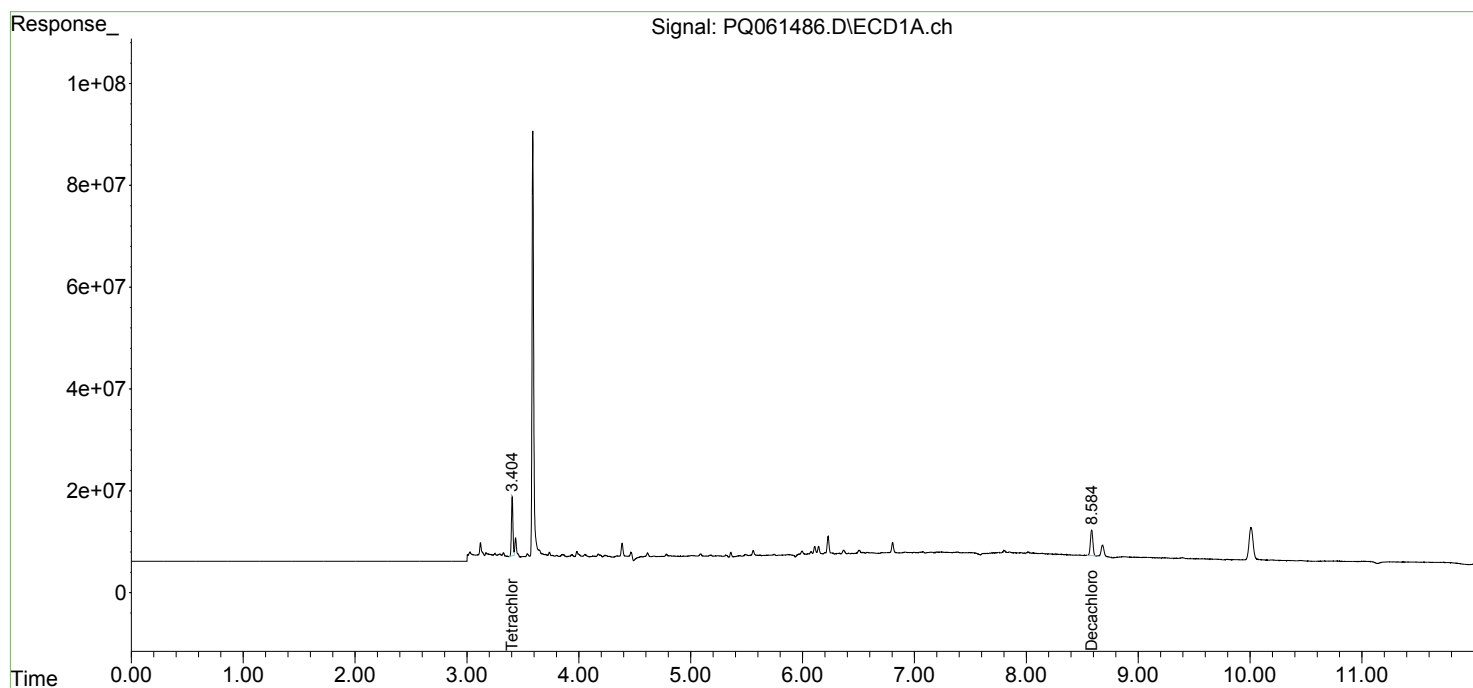

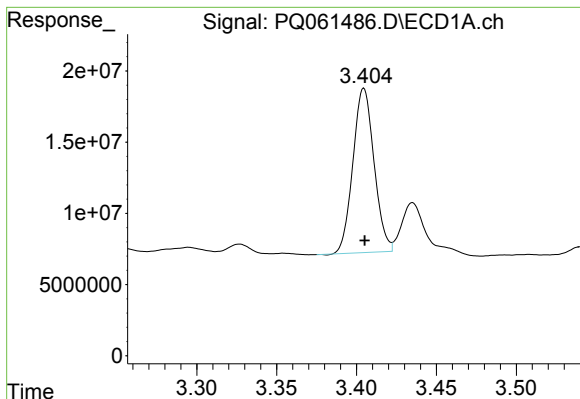


#1 Tetrachloro-m-xylene

R.T.: 3.405 min
Delta R.T.: 0.000 min
Response: 106188087
Conc: 23.62 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MW-01RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/19/2023
Supervised By :Ankita Jodhani 06/19/2023

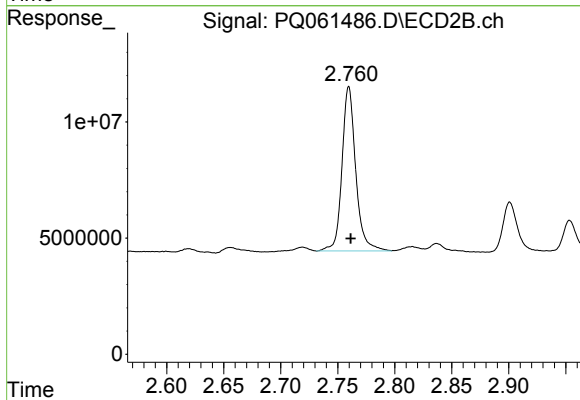


#1 Tetrachloro-m-xylene

R.T.: 2.760 min
Delta R.T.: -0.002 min
Response: 59412341
Conc: 22.25 ng/ml m

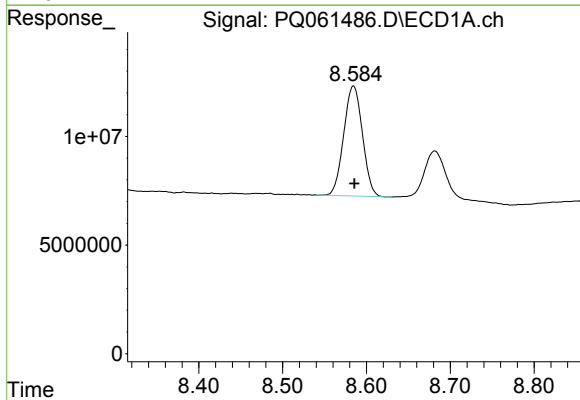

#2 Decachlorobiphenyl

R.T.: 8.585 min
Delta R.T.: -0.001 min
Response: 78426329
Conc: 23.28 ng/ml

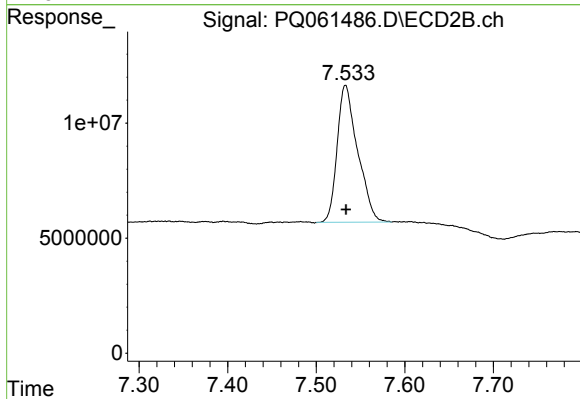

#2 Decachlorobiphenyl

R.T.: 7.533 min
Delta R.T.: 0.000 min
Response: 95687159
Conc: 28.51 ng/ml