

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ061923\
 Data File : PQ061495.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2023 10:55
 Operator : YP\AJ
 Sample : 03251-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 MW-01

Manual Integrations
 APPROVED

Reviewed By :Yogesh
 Patel

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 15:18:23 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ060923.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 09 18:19:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

06/20/2023
 Supervised By :Ankita
 Jodhani

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	06/20/2023
----------	------	------	--------	--------	-------	-------	------------

System Monitoring Compounds

1) SA Tetrachlo...	3.405	2.759	97447003	62806039	21.679	23.520m	
2) SA Decachlor...	8.586	7.533	73921163	100.0E6	21.944	29.799 #	

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ061923\
Data File : PQ061495.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2023 10:55
Operator : YP\AJ
Sample : 03251-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
MW-01



Manual Integrations
APPROVED


Reviewed By :Yogesh
Patel

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 15:18:23 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ060923.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 09 18:19:31 2023
Response via : Initial Calibration
Integrator: ChemStation

06/20/2023
Supervised By :Ankita
Jodhani

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

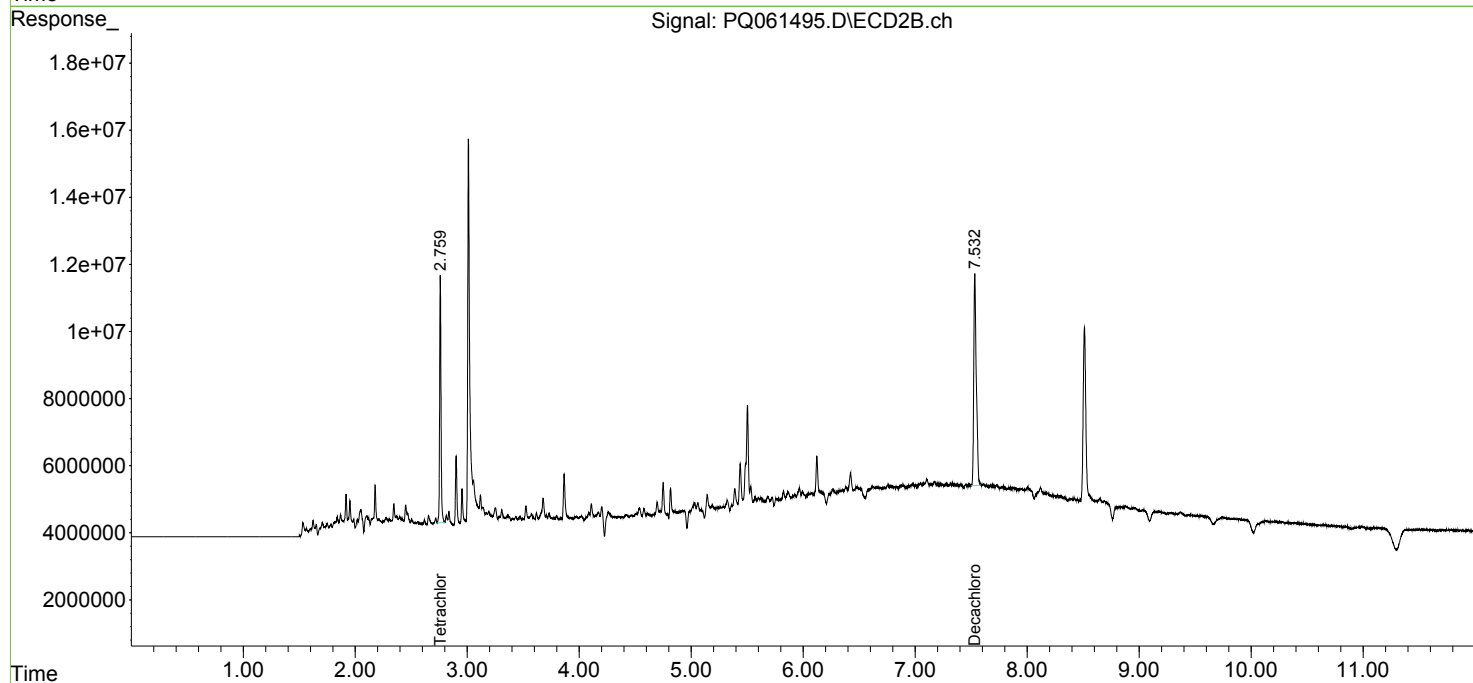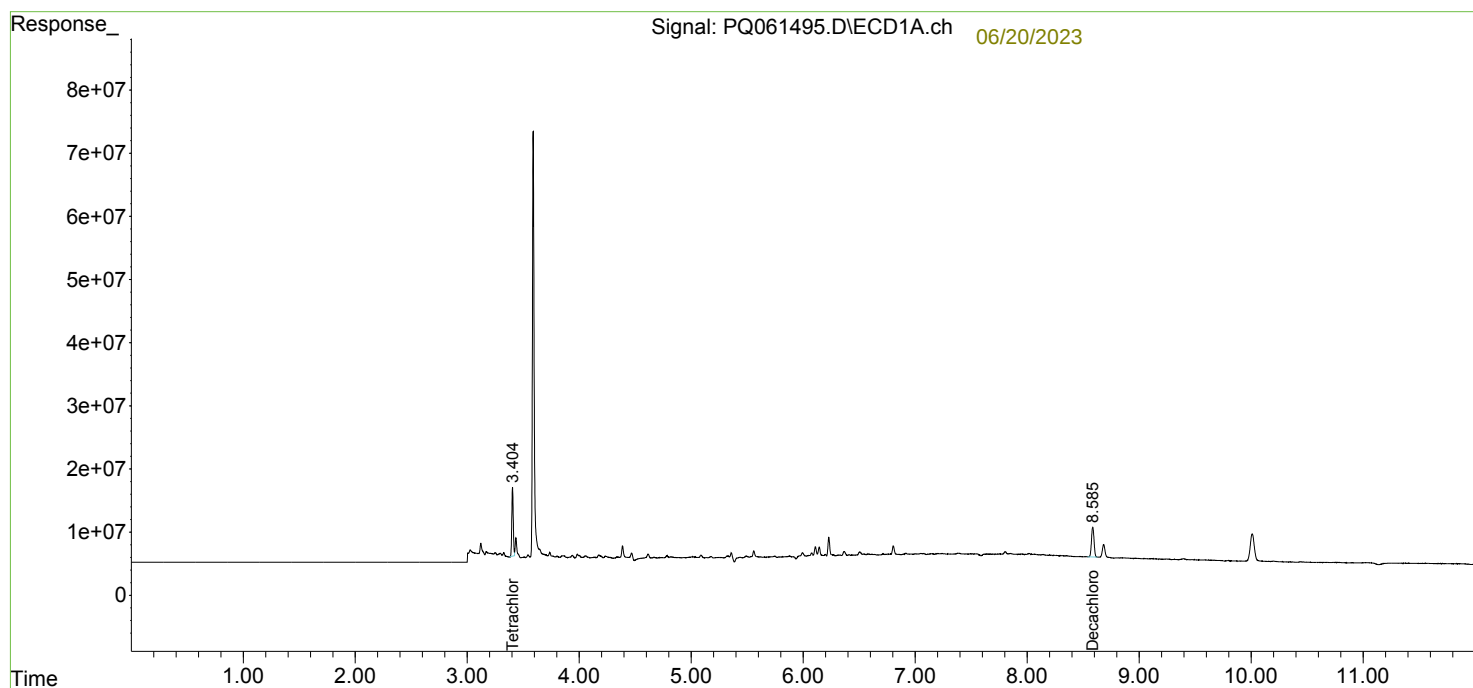

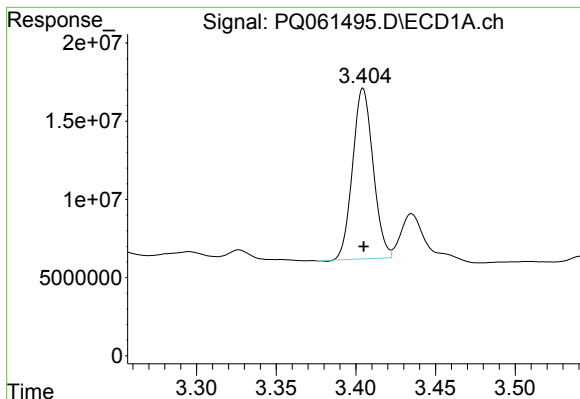


#1 Tetrachloro-m-xylene

R.T.: 3.405 min
Delta R.T.: 0.000 min
Response: 97447003
Conc: 21.68 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MW-01

Manual Integrations
APPROVED

Reviewed By :Yogesh
Patel

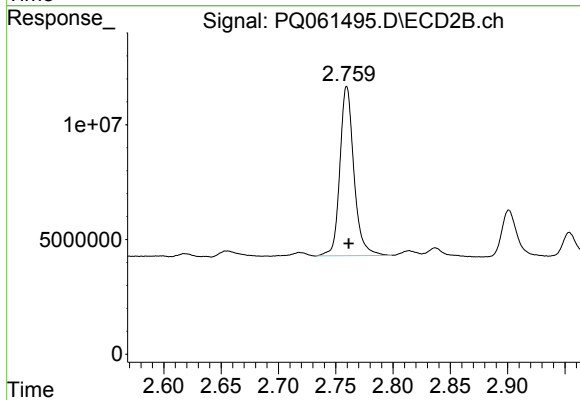


#1 Tetrachloro-m-xylene

R.T.: 2.759 min
Delta R.T.: -0.002 min
Response: 62806039
Conc: 23.52 ng/ml m


06/20/2023
Supervised By :Ankita
Jodhani

06/20/2023

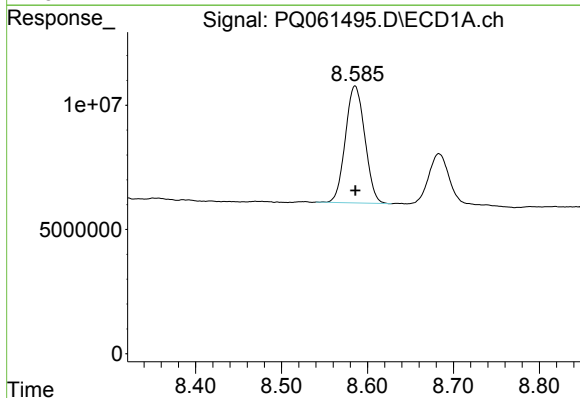

#2 Decachlorobiphenyl

R.T.: 8.586 min
Delta R.T.: 0.000 min
Response: 73921163
Conc: 21.94 ng/ml

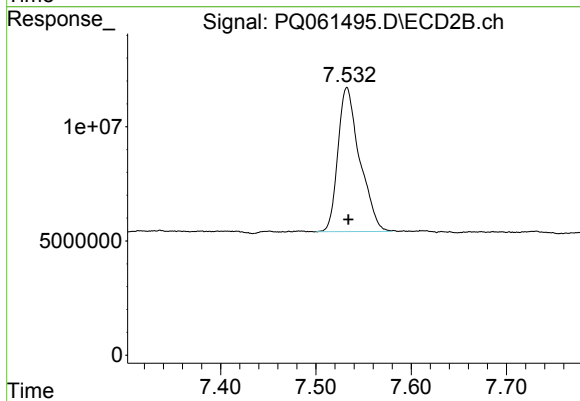

#2 Decachlorobiphenyl

R.T.: 7.533 min
Delta R.T.: -0.001 min
Response: 100020117
Conc: 29.80 ng/ml