

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ061923\
 Data File : PQ061500.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2023 14:10
 Operator : YP\AJ
 Sample : 03241-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 40508

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/20/2023
 Supervised By :Ankita Jodhani 06/20/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 15:20:41 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ060923.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 09 18:19:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.409	2.761	25472568	17328093	5.667m	6.489m
2) SA Decachlor...	8.601	7.547	26995997	19115053	8.014	5.695m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ061923\
Data File : PQ061500.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2023 14:10
Operator : YP\AJ
Sample : 03241-02
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
40508


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/20/2023
Supervised By :Ankita Jodhani 06/20/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 15:20:41 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ060923.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 09 18:19:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

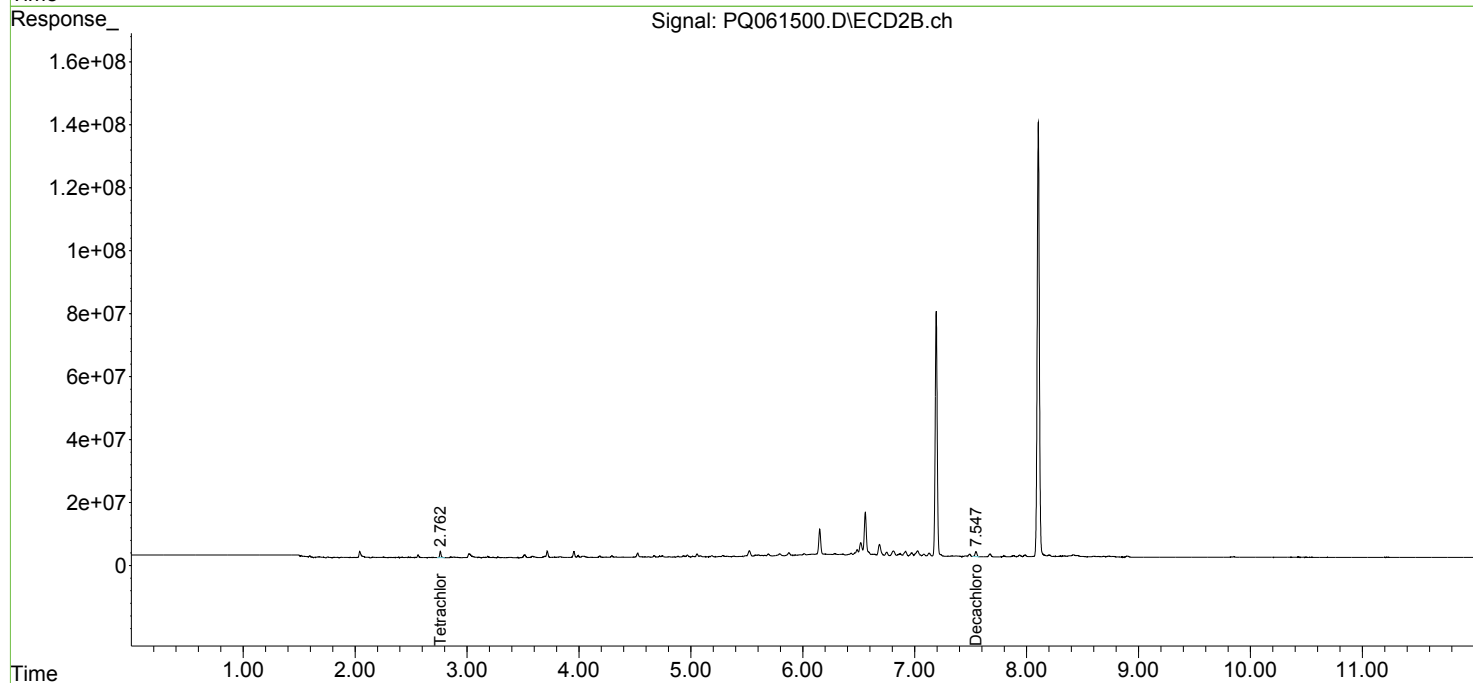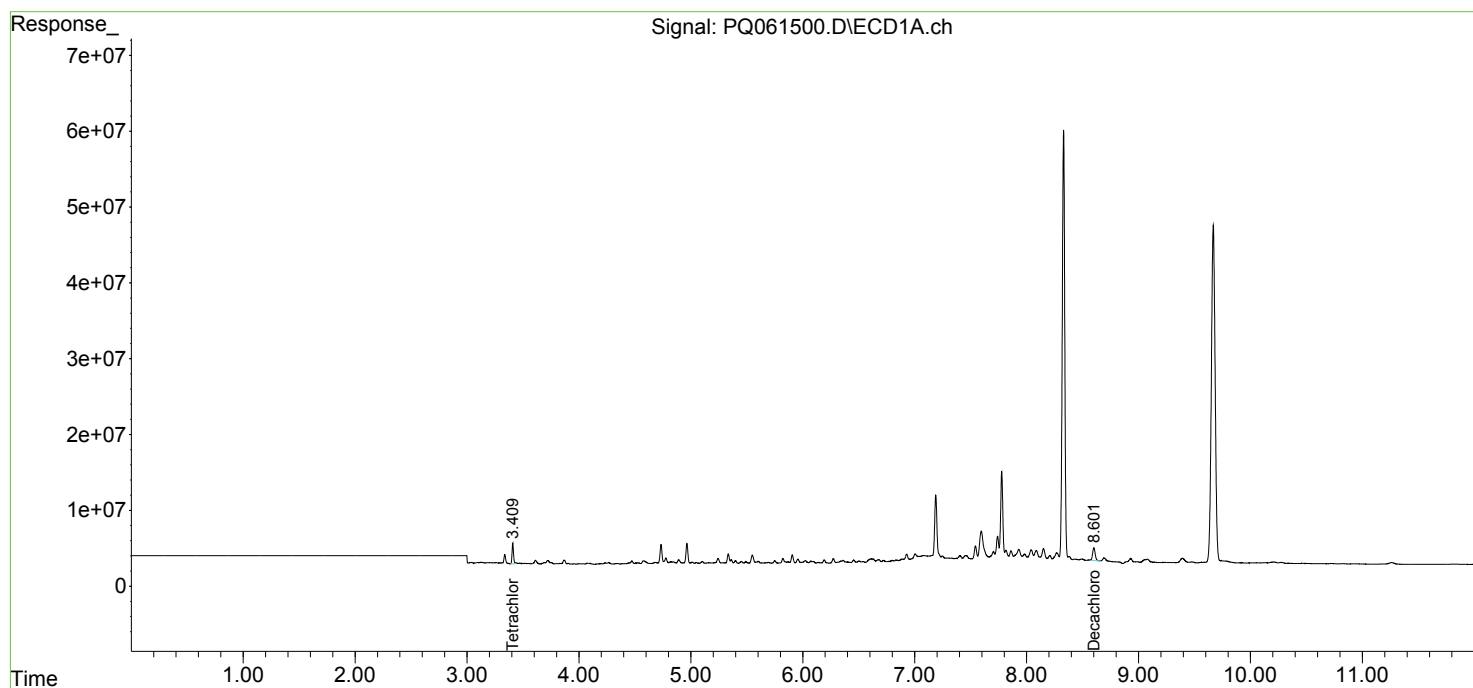

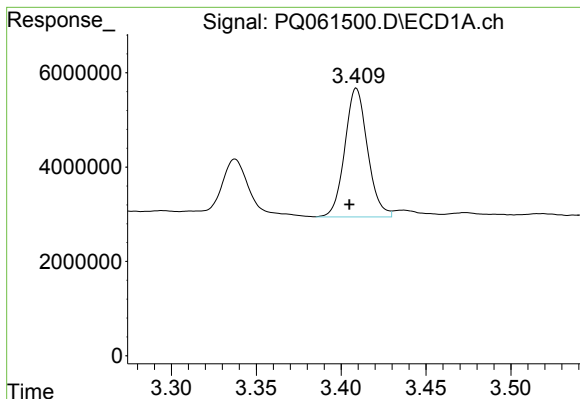


#1 Tetrachloro-m-xylene

R.T.: 3.409 min
Delta R.T.: 0.004 min
Response: 25472568
Conc: 5.67 ng/ml

Instrument :
ECD_Q
ClientSampleId :
40508


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/20/2023
Supervised By :Ankita Jodhani 06/20/2023

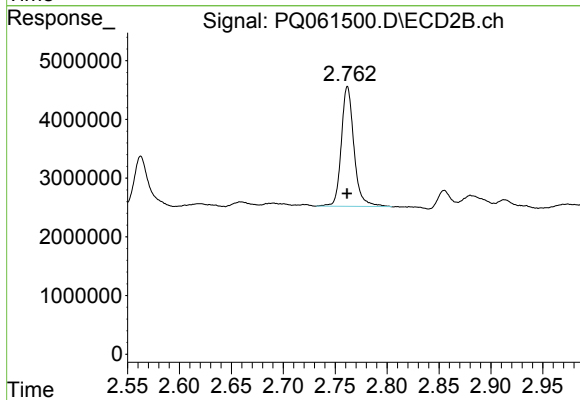


#1 Tetrachloro-m-xylene

R.T.: 2.761 min
Delta R.T.: 0.000 min
Response: 17328093
Conc: 6.49 ng/ml m

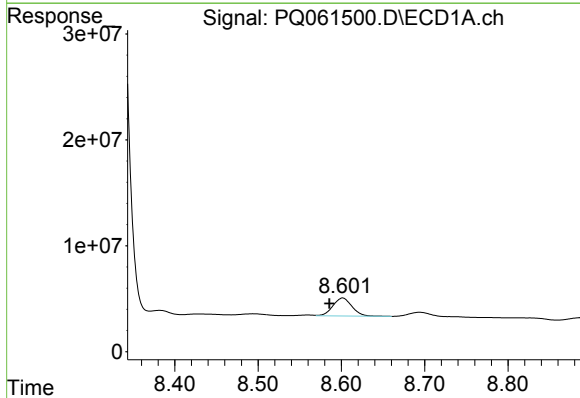

#2 Decachlorobiphenyl

R.T.: 8.601 min
Delta R.T.: 0.016 min
Response: 26995997
Conc: 8.01 ng/ml

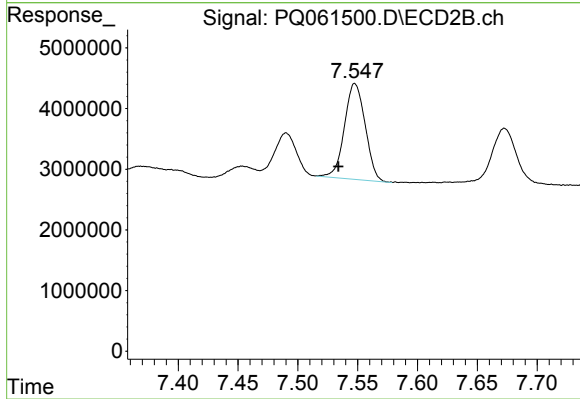

#2 Decachlorobiphenyl

R.T.: 7.547 min
Delta R.T.: 0.013 min
Response: 19115053
Conc: 5.69 ng/ml m