

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ061924\
 Data File : PQ067046.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2024 11:52
 Operator : YP\AJ
 Sample : P2937-15 10X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 BC274271-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/20/2024
 Supervised By :Ankita Jodhani 06/20/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 13:58:13 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ053124.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 03 10:00:54 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.447	2.824	6197617	9432440	1.119m	1.612m#
2) SA Decachlor...	8.705	7.611	5127153	6012183	1.352	1.047

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ061924\
Data File : PQ067046.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2024 11:52
Operator : YP\AJ
Sample : P2937-15 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
BC274271-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/20/2024
Supervised By :Ankita Jodhani 06/20/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 13:58:13 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ053124.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 03 10:00:54 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

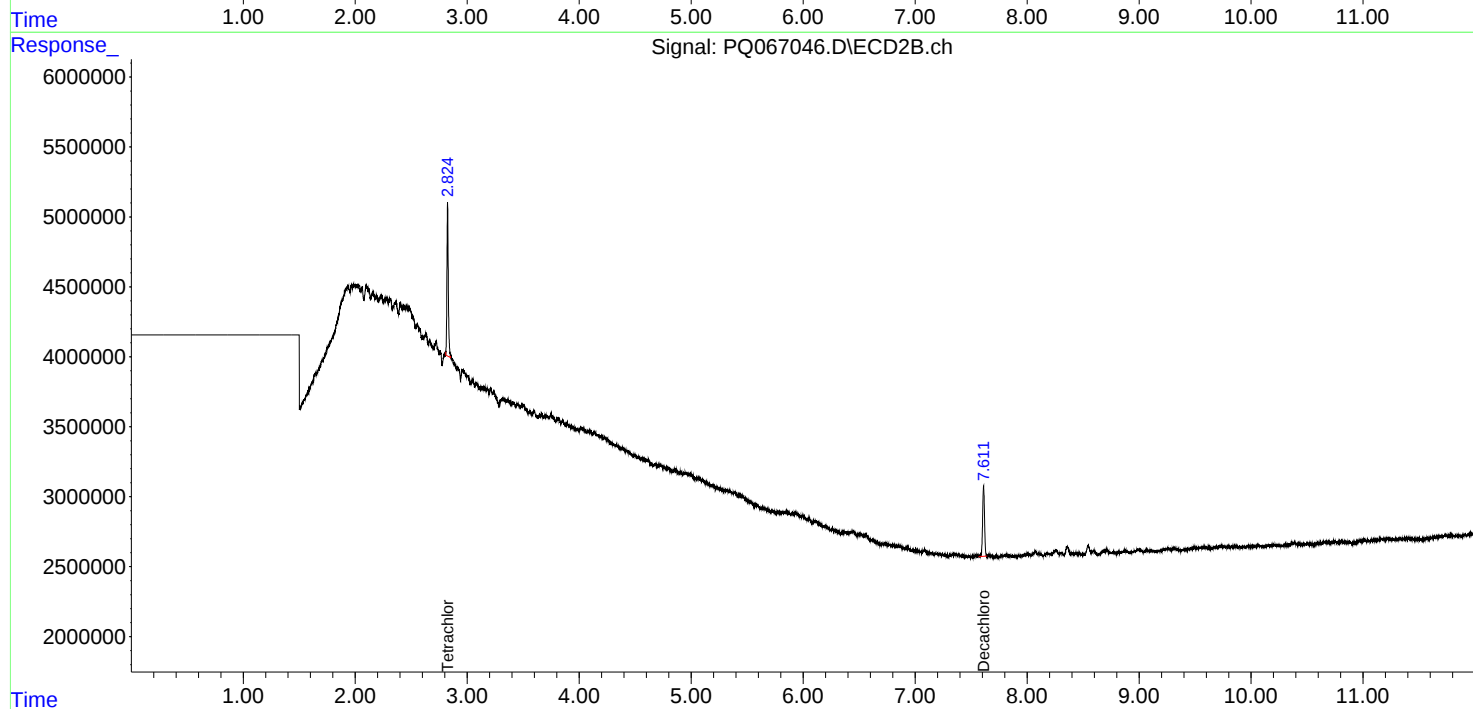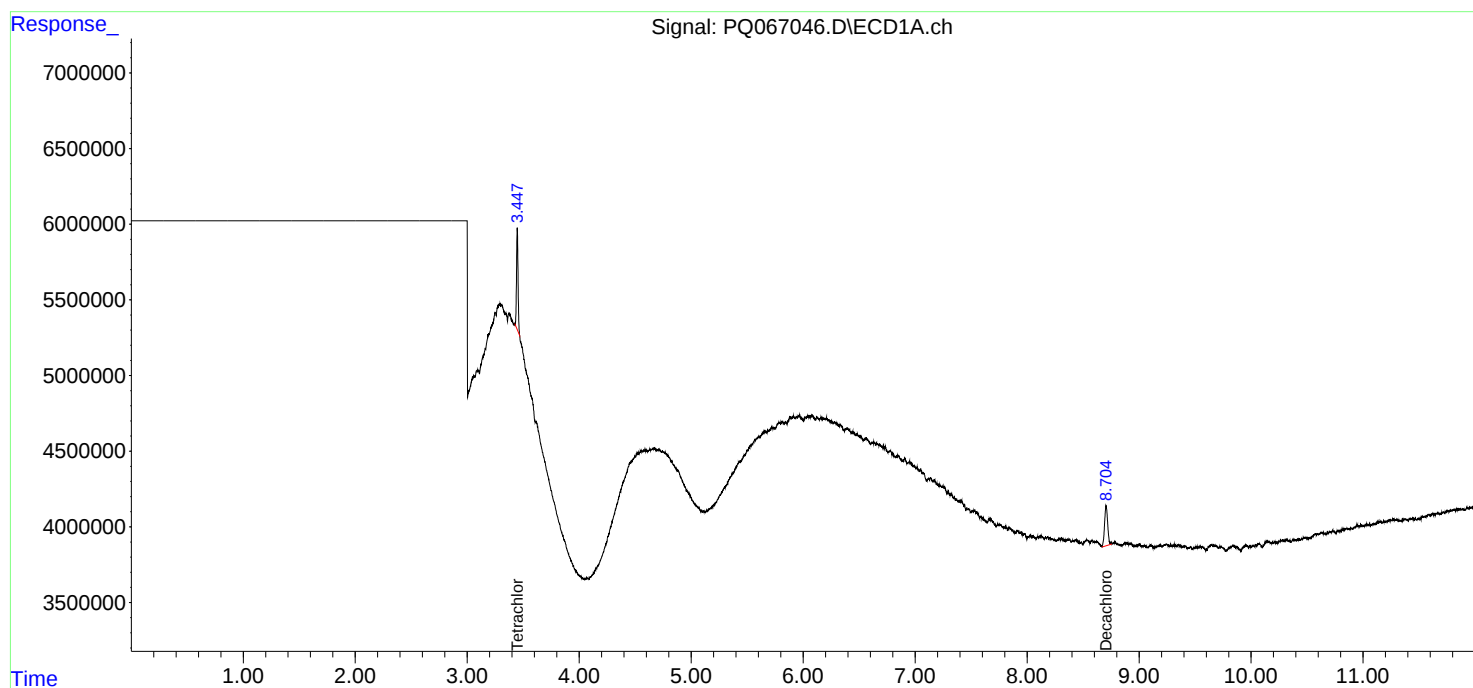

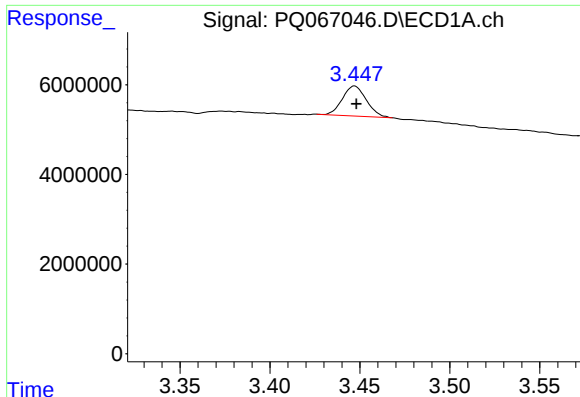


#1 Tetrachloro-m-xylene

R.T.: 3.447 min
Delta R.T.: -0.001 min
Response: 6197617
Conc: 1.12 ng/ml

Instrument :
ECD_Q
ClientSampleId :
BC274271-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/20/2024
Supervised By :Ankita Jodhani 06/20/2024

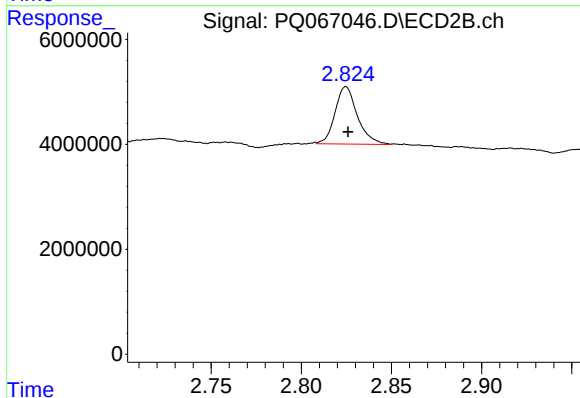


#1 Tetrachloro-m-xylene

R.T.: 2.824 min
Delta R.T.: -0.002 min
Response: 9432440
Conc: 1.61 ng/ml m

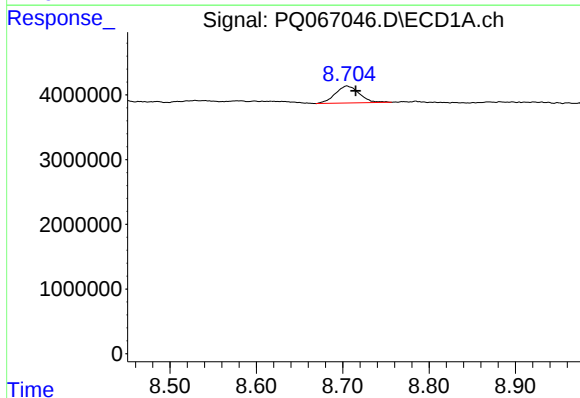

#2 Decachlorobiphenyl

R.T.: 8.705 min
Delta R.T.: -0.010 min
Response: 5127153
Conc: 1.35 ng/ml

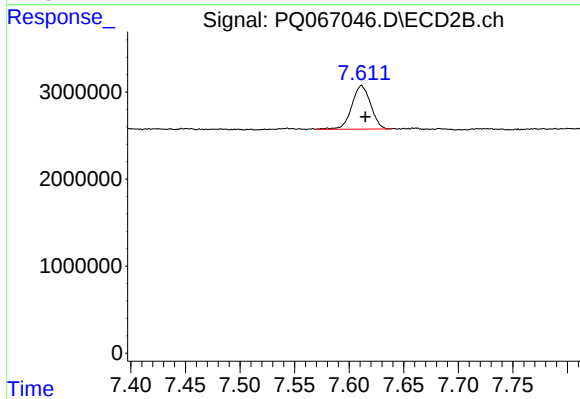

#2 Decachlorobiphenyl

R.T.: 7.611 min
Delta R.T.: -0.004 min
Response: 6012183
Conc: 1.05 ng/ml