

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ062023\
 Data File : PQ061571.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2023 21:01
 Operator : YP\AJ
 Sample : 03315-01 10X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 31263

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/21/2023
 Supervised By :Ankita Jodhani 06/21/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 02:33:53 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ060923.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 09 18:19:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.405	2.760	7644443	4978099	1.701	1.864
2) SA Decachlor...	8.582	7.532	10895834	9023560	3.234m	2.688

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ062023\
Data File : PQ061571.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2023 21:01
Operator : YP\AJ
Sample : 03315-01 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
31263


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/21/2023
Supervised By :Ankita Jodhani 06/21/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 02:33:53 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ060923.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 09 18:19:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

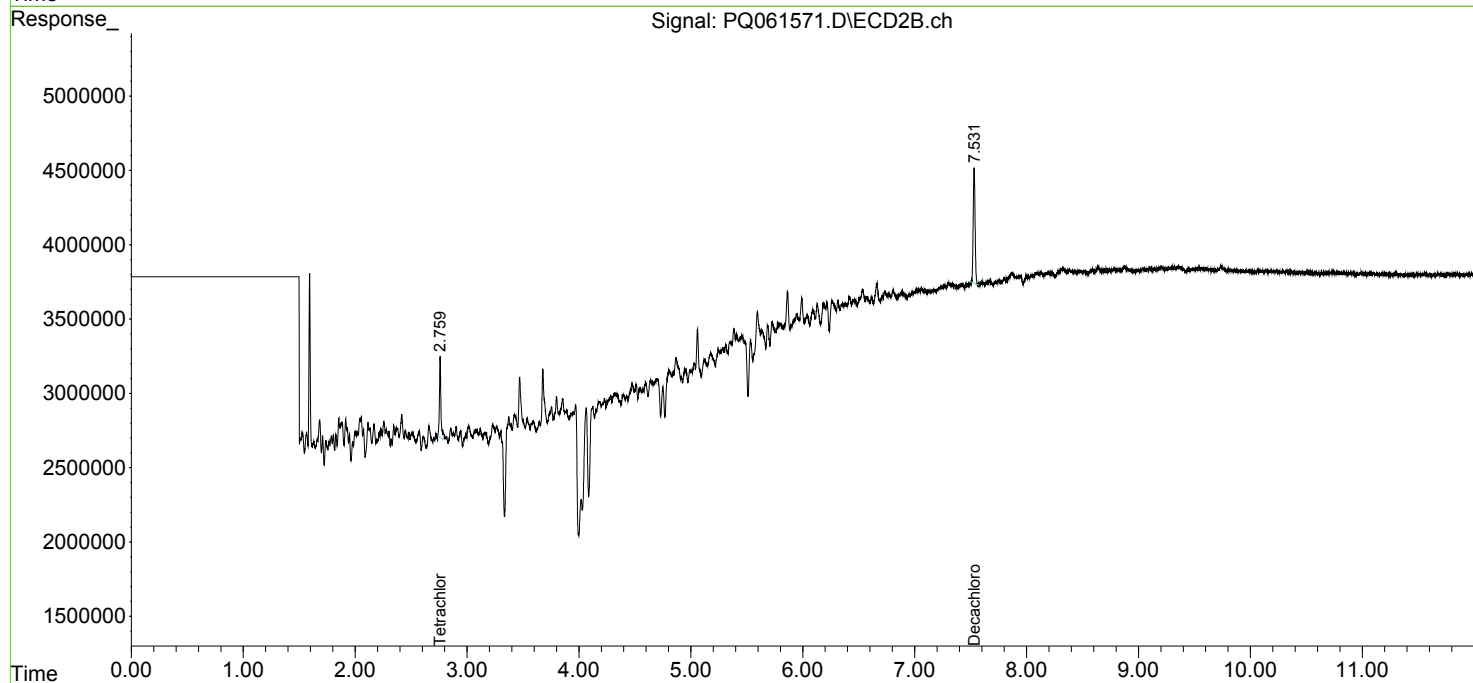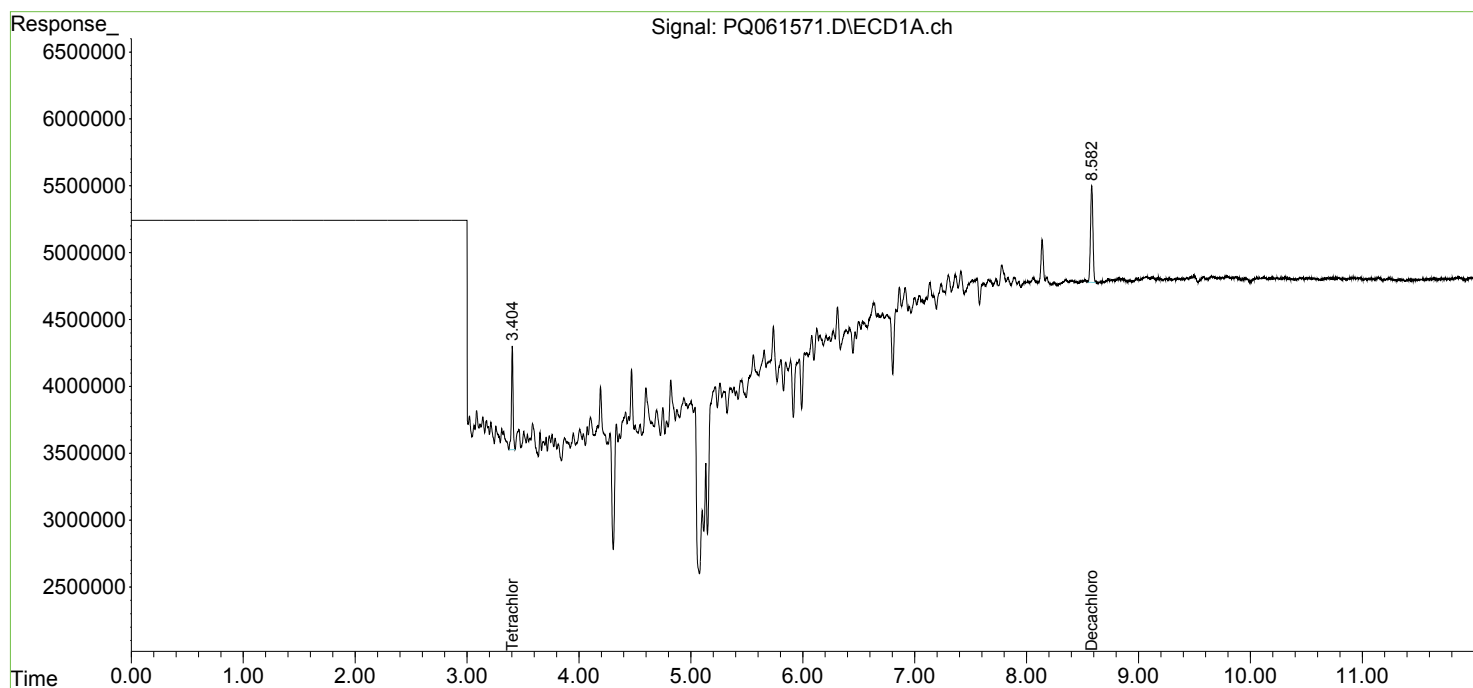

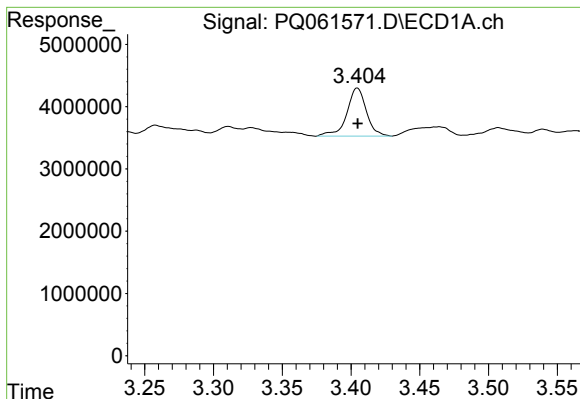

#1 Tetrachloro-m-xylene

R.T.: 3.405 min
Delta R.T.: 0.000 min
Response: 7644443
Conc: 1.70 ng/ml


Instrument :

ECD_Q

ClientSampleId :
31263


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/21/2023
Supervised By :Ankita Jodhani 06/21/2023

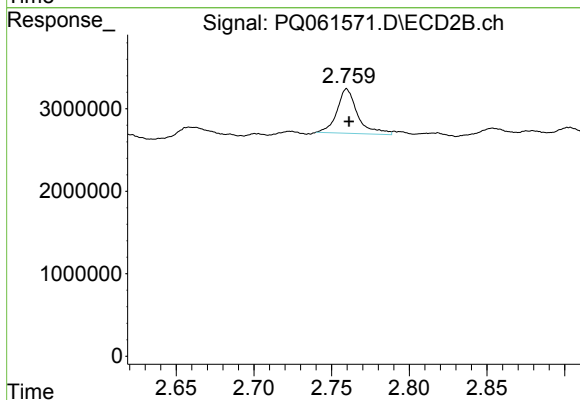


#1 Tetrachloro-m-xylene

R.T.: 2.760 min
Delta R.T.: -0.002 min
Response: 4978099
Conc: 1.86 ng/ml

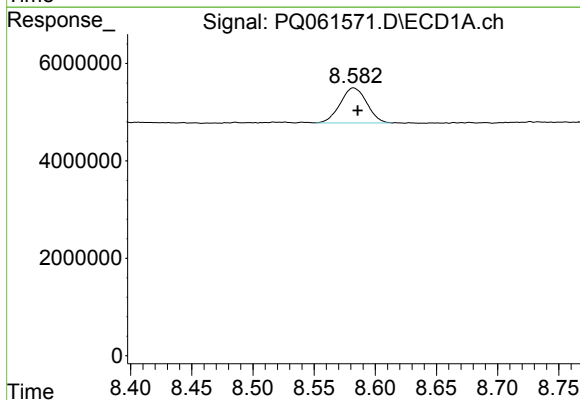

#2 Decachlorobiphenyl

R.T.: 8.582 min
Delta R.T.: -0.004 min
Response: 10895834
Conc: 3.23 ng/ml m

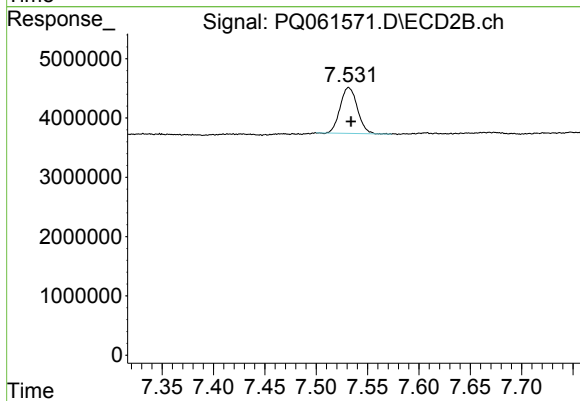

#2 Decachlorobiphenyl

R.T.: 7.532 min
Delta R.T.: -0.002 min
Response: 9023560
Conc: 2.69 ng/ml