

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ062525\
 Data File : PQ070457.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jun 2025 10:38
 Operator : YP\AJ
 Sample : Q2126-09
 Misc : AR1221 MDL 25 PPB
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 MDL-WATER-03-QT2-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 04:55:59 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ062425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jun 26 02:49:53 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.403	2.782	112.5E6	127.6E6	18.370	18.898
2)	SA Decachlor...	8.501	7.542	86067815	151.2E6	20.908	20.856
Target Compounds							
3)	L1 AR-1016-1	4.480	3.781	540526	908145	2.880	4.373 #
4)	L1 AR-1016-2	4.499	3.798	578956	1022895	1.870	3.024 #
5)	L1 AR-1016-3	4.557	3.960	595019	782998	2.957	4.173 #
6)	L1 AR-1016-4	4.647	4.042f	461283	690512	2.914	3.936 #
7)	L1 AR-1016-5	4.944	4.201	61349	6576	0.377	0.033 #
8)	L2 AR-1221-1	3.596	2.981	1397245	1862102	16.297	18.213
9)	L2 AR-1221-2	3.675	3.053	2659066	3176626	41.142	40.271
10)	L2 AR-1221-3	3.742	3.126	4046901	4527209	20.865	19.973
11)	L3 AR-1232-1	3.742	3.126	4046901	4527209	28.599	27.160
12)	L3 AR-1232-2	4.231	3.798	623132	1022895	7.690	6.411
13)	L3 AR-1232-3	4.499	3.960	578956	782998	4.057	8.909 #
14)	L3 AR-1232-4	4.647	4.042	461283	690512	6.415	8.951 #
15)	L3 AR-1232-5	4.777	4.201	166696	6576	2.789	0.079 #
16)	L4 AR-1242-1	4.480	3.781	540526	908145	3.493	5.176 #
17)	L4 AR-1242-2	4.499	3.798	578956	1022895	2.204	3.673 #
18)	L4 AR-1242-3	4.557	3.960	595019	782998	3.502	4.982 #
19)	L4 AR-1242-4	4.647	4.042	461283	690512	3.418	4.534 #
20)	L4 AR-1242-5	5.326f	4.539	2381866	691688	17.710	3.791 #
21)	L5 AR-1248-1	4.480	3.781	540526	908145	4.364	6.461 #
22)	L5 AR-1248-2	4.742	4.042f	174606	690512	0.946	2.958 #
23)	L5 AR-1248-3	4.944	4.042	61349	690512	0.278	3.067 #
24)	L5 AR-1248-4	5.326	4.201	2381866	6576	10.733	0.024 #
25)	L5 AR-1248-5	5.387f	4.591	361456	556608	1.564	2.223 #
26)	L6 AR-1254-1	5.295	4.539	668922	691688	2.704	1.707 #
27)	L6 AR-1254-2	5.512	4.687	446532	149002	1.189	0.413 #
28)	L6 AR-1254-3	5.864	5.077	223360	6622715	0.575	11.710 #
29)	L6 AR-1254-4	6.159	5.295	4401979	122306	17.684	0.401 #
30)	L6 AR-1254-5	6.537	5.660f	222629	63777	0.749	0.124 #
31)	L7 AR-1260-1	6.031	5.210	628362	171733	2.175	0.450 #
32)	L7 AR-1260-2	6.324f	5.374	252462	503176	0.792	1.149 #
33)	L7 AR-1260-3	6.614	5.533	99421	61120	0.383	0.142 #
34)	L7 AR-1260-4	6.866	5.959f	105253	180061	0.386	0.491 #
35)	L7 AR-1260-5	7.159	6.233	198167	600816	0.398	0.723 #
36)	L8 AR-1262-1	6.866	5.738	105253	1097696	0.299	2.006 #
37)	L8 AR-1262-2	7.159	5.959f	198167	180061	0.350	0.354
38)	L8 AR-1262-3	7.469f	6.544f	1015167	488625	2.606	1.245 #
39)	L8 AR-1262-4	7.499	6.579	349002	267856	1.091	0.382 #
40)	L8 AR-1262-5	0.000	7.077	0	228819	N.D.	0.722 #
41)	L9 AR-1268-1	7.469f	6.544f	1015167	488625	1.409	0.422 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ062525\
Data File : PQ070457.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jun 2025 10:38
Operator : YP\AJ
Sample : Q2126-09
Misc : AR1221 MDL 25 PPB
ALS Vial : 23 Sample Multiplier: 1


Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 04:55:59 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ062425.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 26 02:49:53 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	7.499	6.579	349002	267856	0.525	0.250 #
43) L9	AR-1268-3	7.681	6.772	255328	362231	0.450	0.379
44) L9	AR-1268-4	0.000	7.077	0	228819	N.D.	0.608 #
45) L9	AR-1268-5	8.275	7.324	441316	597522	0.276	0.227


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

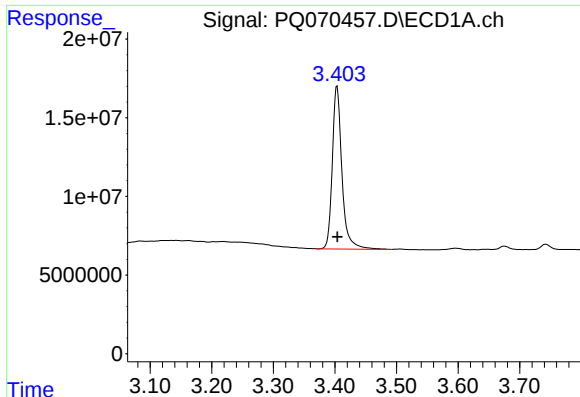

#1 Tetrachloro-m-xylene


R.T.: 3.403 min
Delta R.T.: 0.000 min
Response: 112458804
Conc: 18.37 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

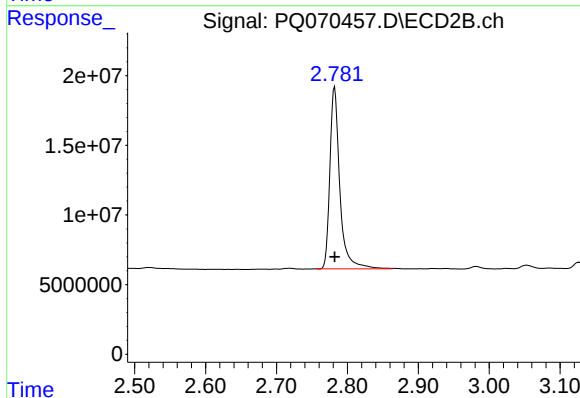


#1 Tetrachloro-m-xylene

R.T.: 2.782 min
Delta R.T.: 0.000 min
Response: 127623336
Conc: 18.90 ng/ml

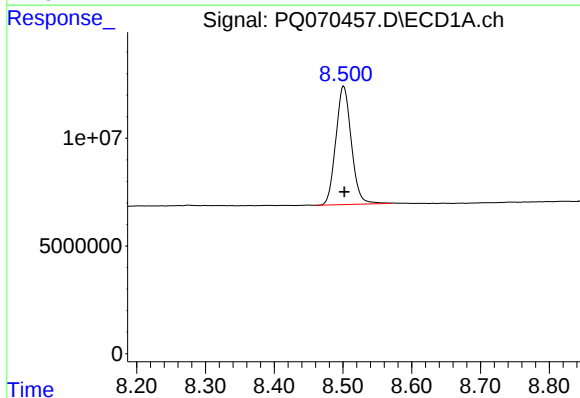


#2 Decachlorobiphenyl

R.T.: 8.501 min
Delta R.T.: 0.000 min
Response: 86067815
Conc: 20.91 ng/ml

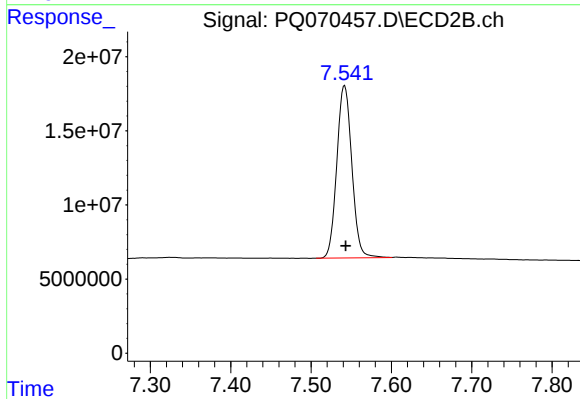

#2 Decachlorobiphenyl


R.T.: 7.542 min
Delta R.T.: -0.002 min
Response: 151193325
Conc: 20.86 ng/ml

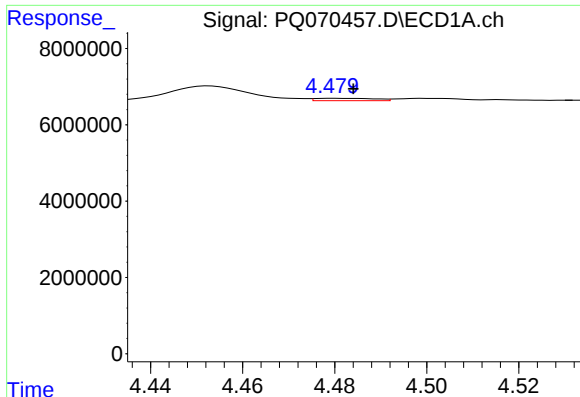

#3 AR-1016-1


R.T.: 4.480 min
Delta R.T.: -0.004 min
Response: 540526
Conc: 2.88 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

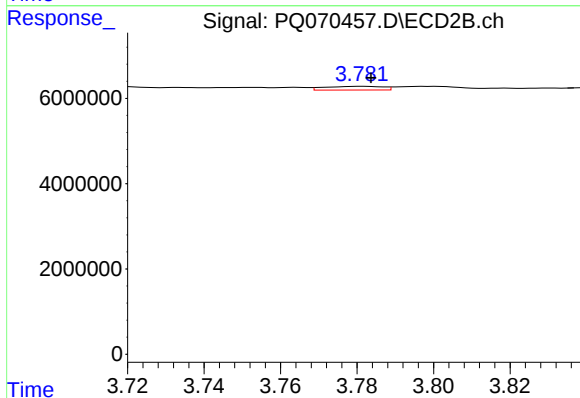


#3 AR-1016-1

R.T.: 3.781 min
Delta R.T.: -0.002 min
Response: 908145
Conc: 4.37 ng/ml

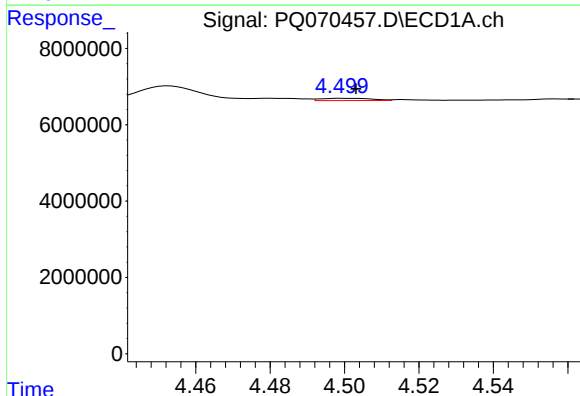


#4 AR-1016-2

R.T.: 4.499 min
Delta R.T.: -0.004 min
Response: 578956
Conc: 1.87 ng/ml

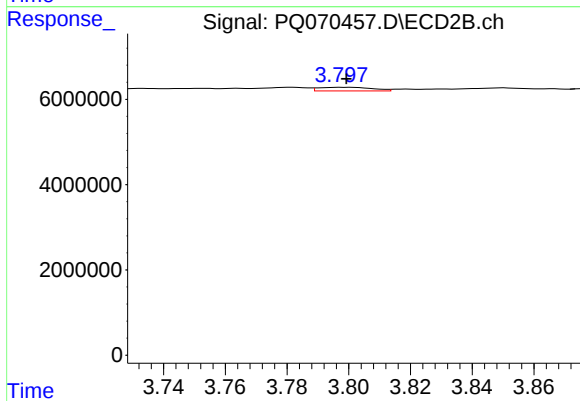

#4 AR-1016-2


R.T.: 3.798 min
Delta R.T.: -0.002 min
Response: 1022895
Conc: 3.02 ng/ml

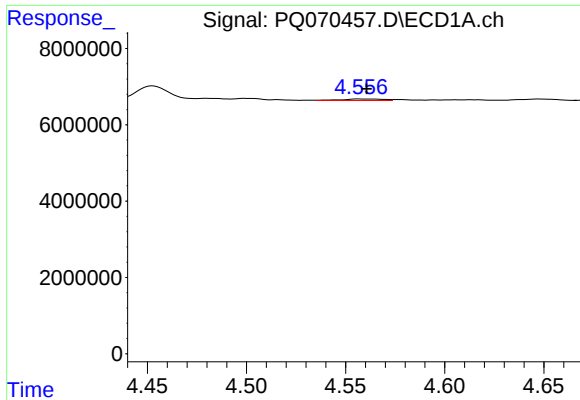

#5 AR-1016-3


R.T.: 4.557 min
Delta R.T.: -0.004 min
Response: 595019
Conc: 2.96 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

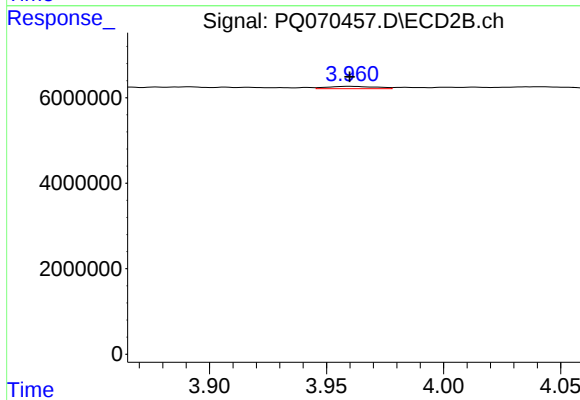


#5 AR-1016-3

R.T.: 3.960 min
Delta R.T.: 0.000 min
Response: 782998
Conc: 4.17 ng/ml

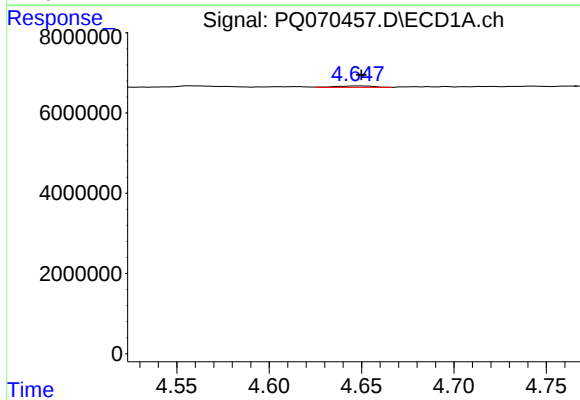


#6 AR-1016-4

R.T.: 4.647 min
Delta R.T.: -0.003 min
Response: 461283
Conc: 2.91 ng/ml

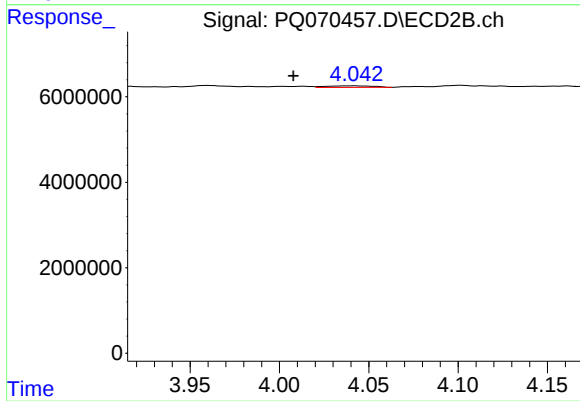

#6 AR-1016-4


R.T.: 4.042 min
Delta R.T.: 0.034 min
Response: 690512
Conc: 3.94 ng/ml

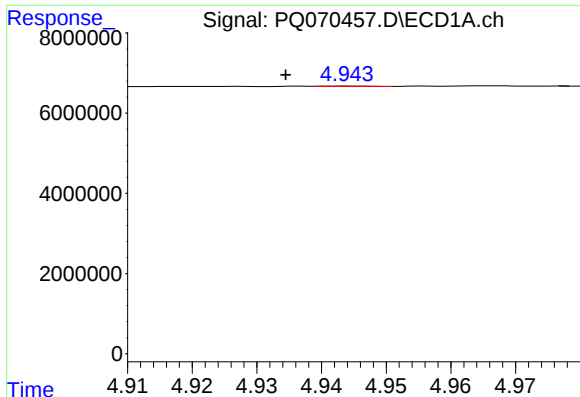

#7 AR-1016-5


R.T.: 4.944 min
Delta R.T.: 0.010 min
Response: 61349
Conc: 0.38 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

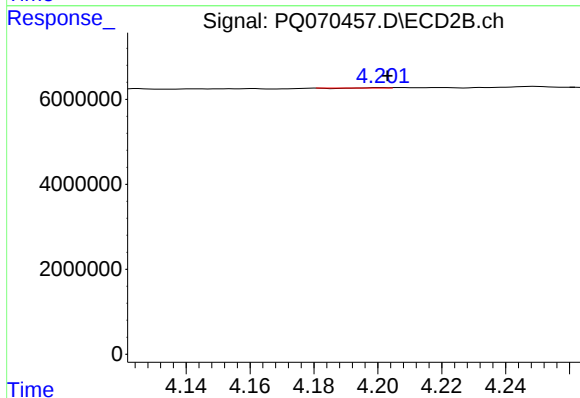


#7 AR-1016-5

R.T.: 4.201 min
Delta R.T.: -0.002 min
Response: 6576
Conc: 0.03 ng/ml

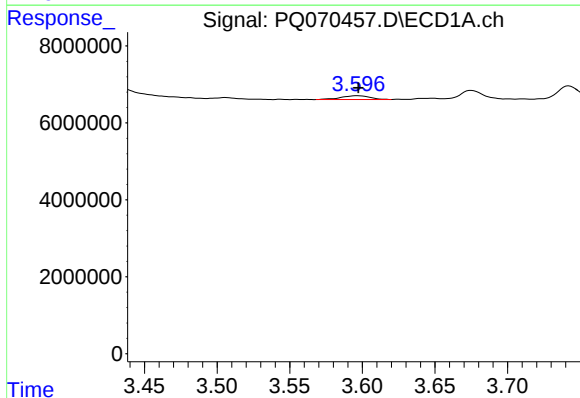


#8 AR-1221-1

R.T.: 3.596 min
Delta R.T.: -0.001 min
Response: 1397245
Conc: 16.30 ng/ml

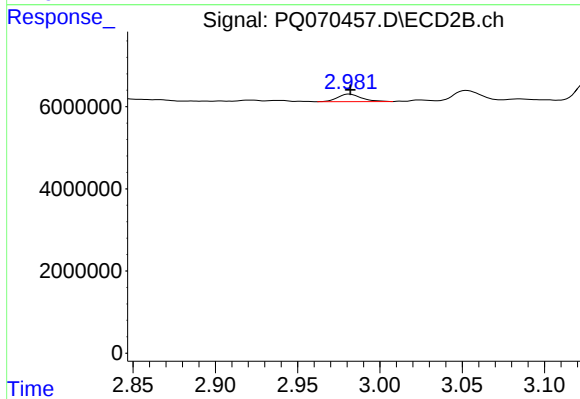

#8 AR-1221-1


R.T.: 2.981 min
Delta R.T.: 0.000 min
Response: 1862102
Conc: 18.21 ng/ml

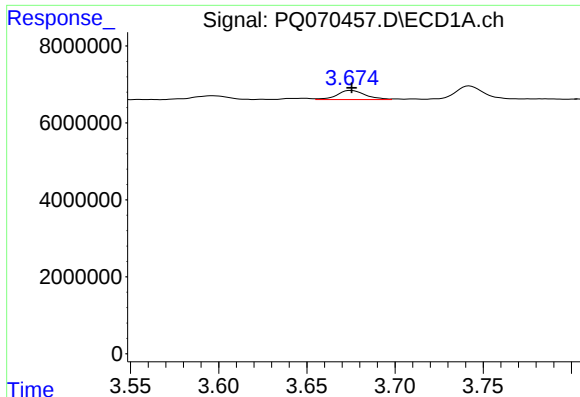

#9 AR-1221-2


R.T.: 3.675 min
Delta R.T.: 0.000 min
Response: 2659066
Conc: 41.14 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

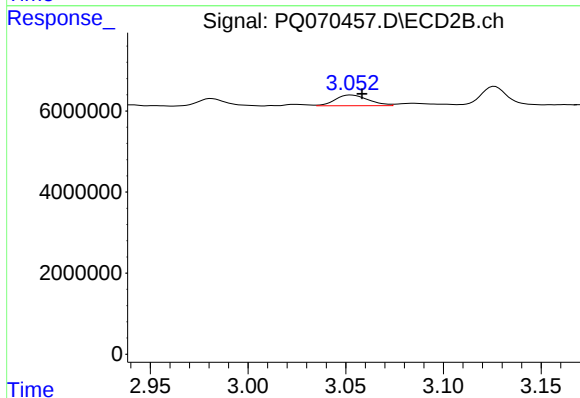


#9 AR-1221-2

R.T.: 3.053 min
Delta R.T.: -0.006 min
Response: 3176626
Conc: 40.27 ng/ml

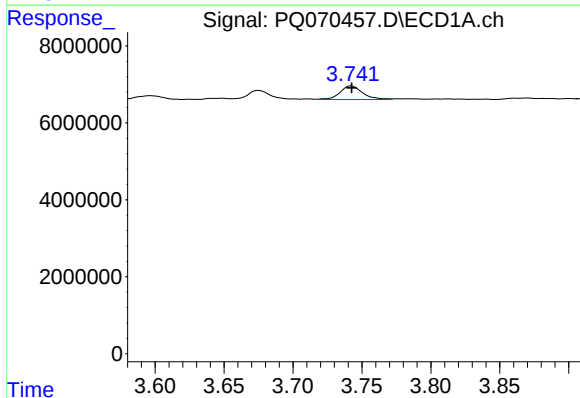


#10 AR-1221-3

R.T.: 3.742 min
Delta R.T.: 0.000 min
Response: 4046901
Conc: 20.87 ng/ml

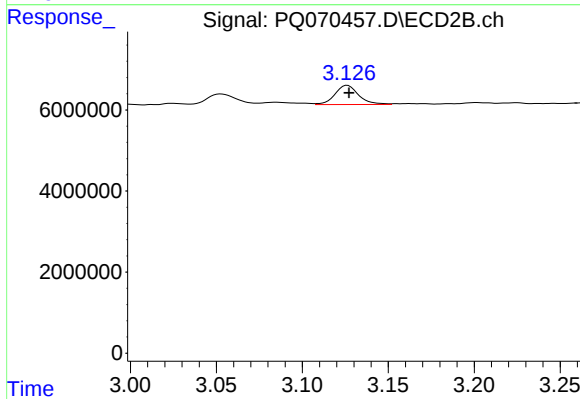

#10 AR-1221-3


R.T.: 3.126 min
Delta R.T.: 0.000 min
Response: 4527209
Conc: 19.97 ng/ml

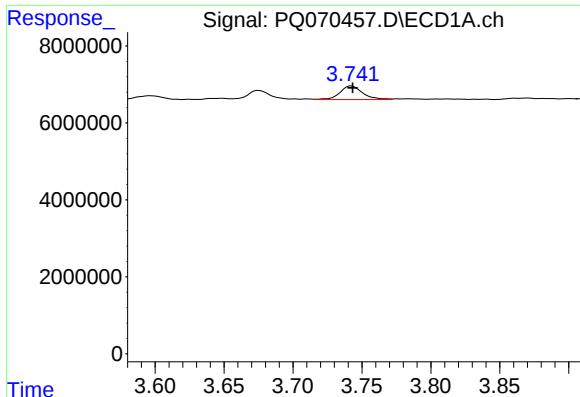

#11 AR-1232-1


R.T.: 3.742 min
Delta R.T.: -0.001 min
Response: 4046901
Conc: 28.60 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

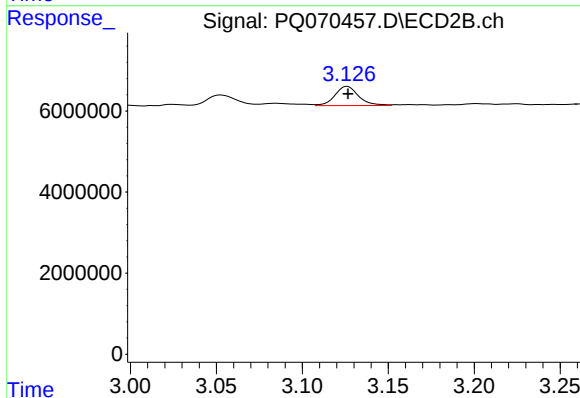


#11 AR-1232-1

R.T.: 3.126 min
Delta R.T.: 0.000 min
Response: 4527209
Conc: 27.16 ng/ml

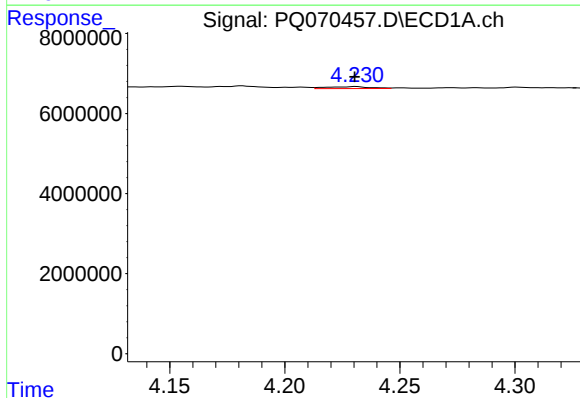


#12 AR-1232-2

R.T.: 4.231 min
Delta R.T.: 0.000 min
Response: 623132
Conc: 7.69 ng/ml

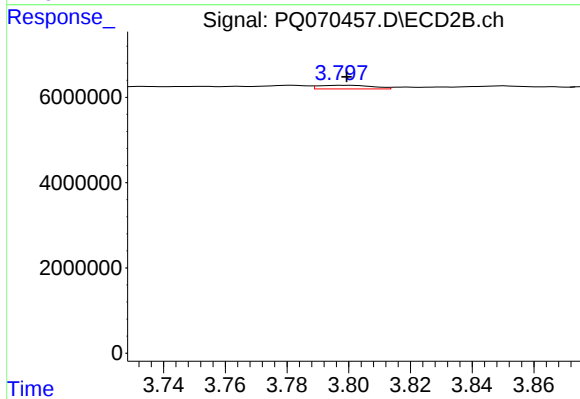

#12 AR-1232-2


R.T.: 3.798 min
Delta R.T.: -0.002 min
Response: 1022895
Conc: 6.41 ng/ml

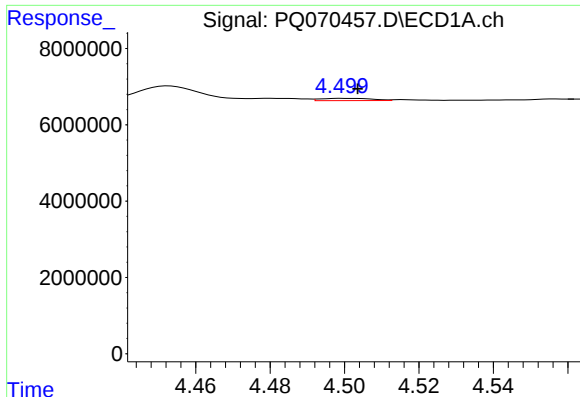

#13 AR-1232-3


R.T.: 4.499 min
Delta R.T.: -0.004 min
Response: 578956
Conc: 4.06 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

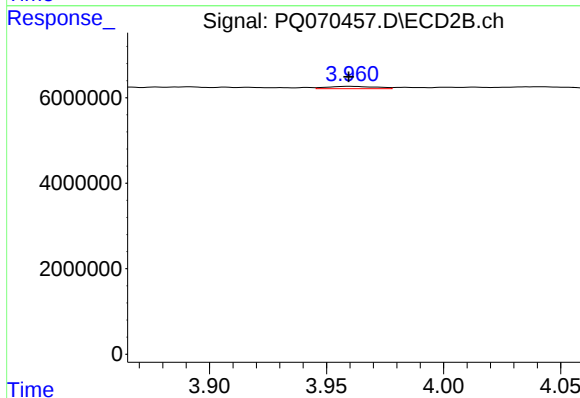


#13 AR-1232-3

R.T.: 3.960 min
Delta R.T.: 0.001 min
Response: 782998
Conc: 8.91 ng/ml

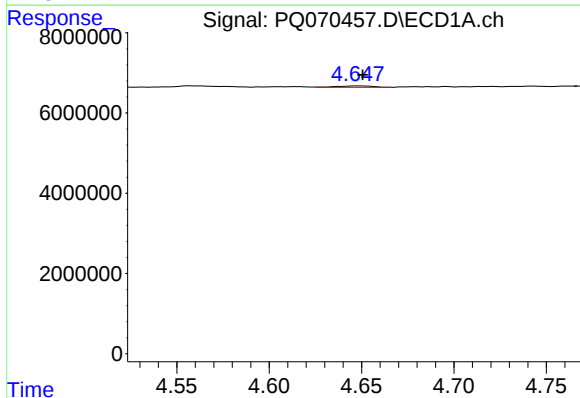


#14 AR-1232-4

R.T.: 4.647 min
Delta R.T.: -0.003 min
Response: 461283
Conc: 6.42 ng/ml

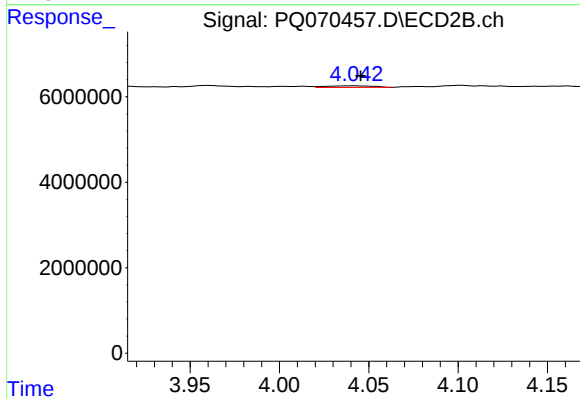

#14 AR-1232-4


R.T.: 4.042 min
Delta R.T.: -0.003 min
Response: 690512
Conc: 8.95 ng/ml

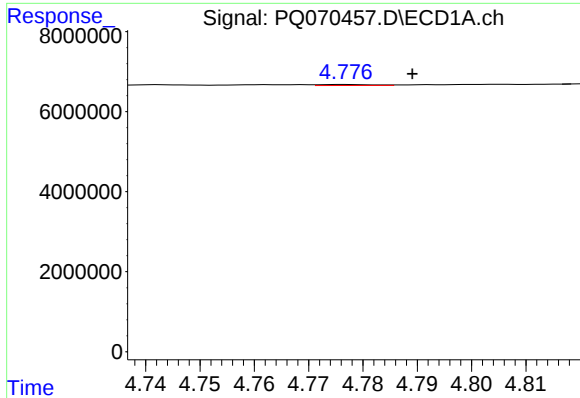

#15 AR-1232-5


R.T.: 4.777 min
Delta R.T.: -0.012 min
Response: 166696
Conc: 2.79 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

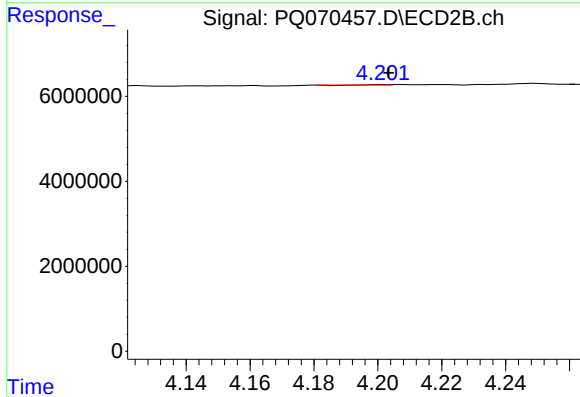


#15 AR-1232-5

R.T.: 4.201 min
Delta R.T.: -0.002 min
Response: 6576
Conc: 0.08 ng/ml

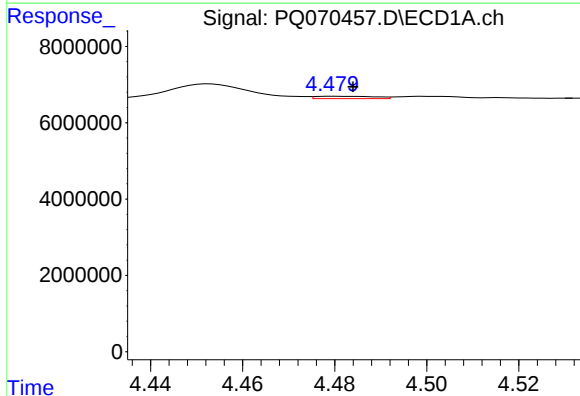


#16 AR-1242-1

R.T.: 4.480 min
Delta R.T.: -0.004 min
Response: 540526
Conc: 3.49 ng/ml

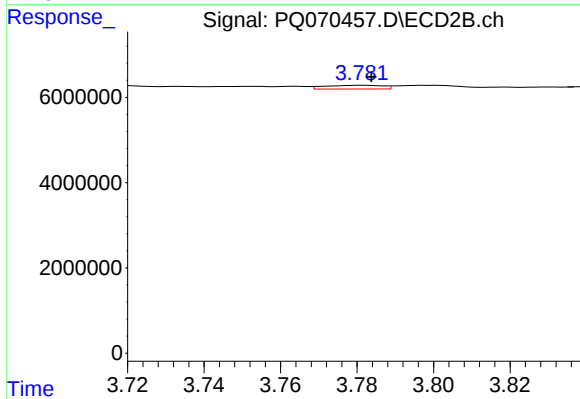

#16 AR-1242-1


R.T.: 3.781 min
Delta R.T.: -0.002 min
Response: 908145
Conc: 5.18 ng/ml

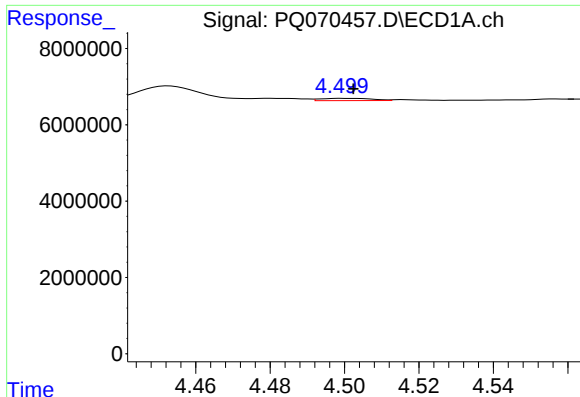

#17 AR-1242-2


R.T.: 4.499 min
Delta R.T.: -0.003 min
Response: 578956
Conc: 2.20 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

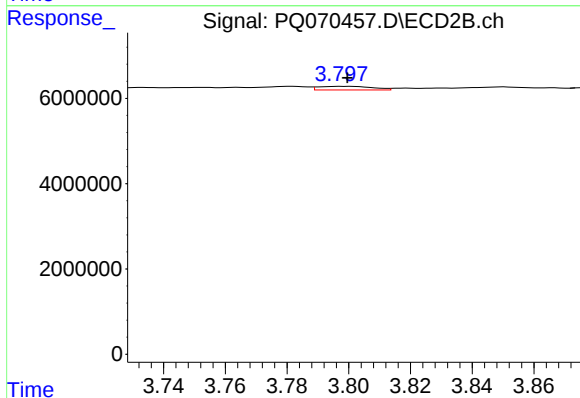


#17 AR-1242-2

R.T.: 3.798 min
Delta R.T.: -0.002 min
Response: 1022895
Conc: 3.67 ng/ml

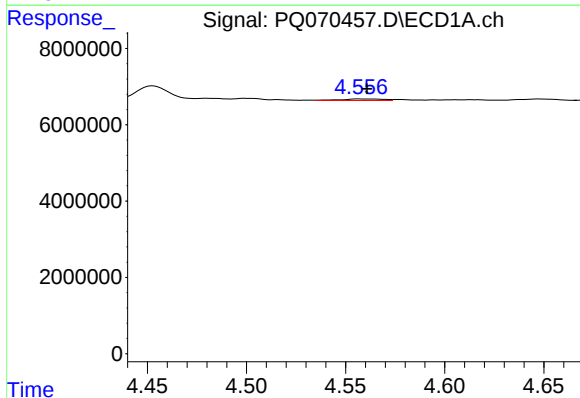


#18 AR-1242-3

R.T.: 4.557 min
Delta R.T.: -0.004 min
Response: 595019
Conc: 3.50 ng/ml

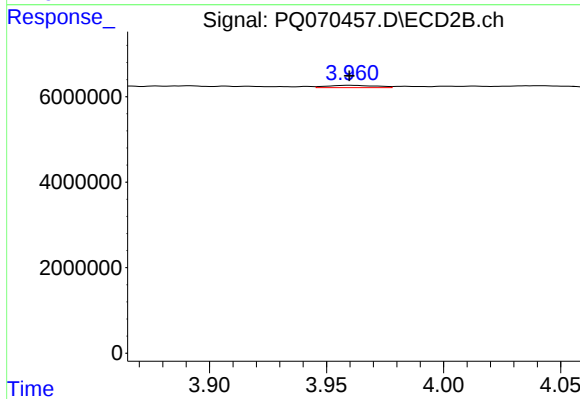

#18 AR-1242-3


R.T.: 3.960 min
Delta R.T.: 0.000 min
Response: 782998
Conc: 4.98 ng/ml

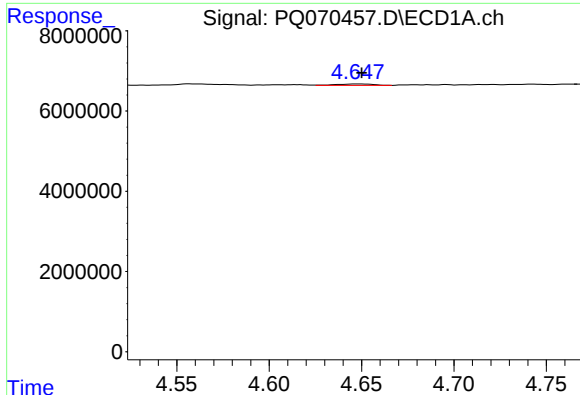

#19 AR-1242-4


R.T.: 4.647 min
Delta R.T.: -0.003 min
Response: 461283
Conc: 3.42 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

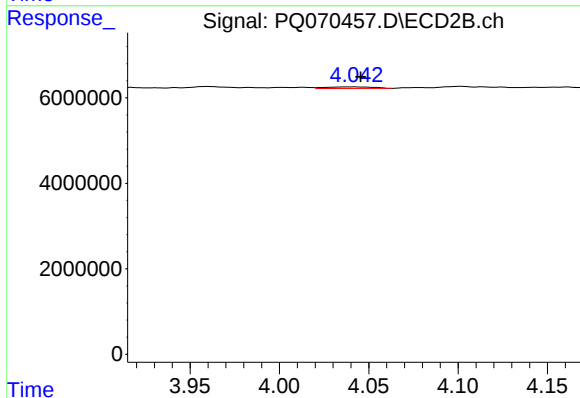


#19 AR-1242-4

R.T.: 4.042 min
Delta R.T.: -0.003 min
Response: 690512
Conc: 4.53 ng/ml

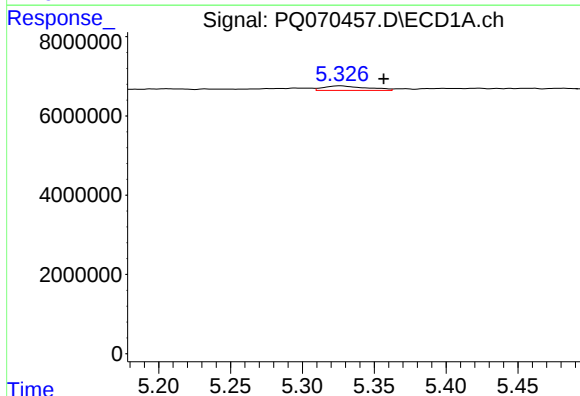


#20 AR-1242-5

R.T.: 5.326 min
Delta R.T.: -0.030 min
Response: 2381866
Conc: 17.71 ng/ml

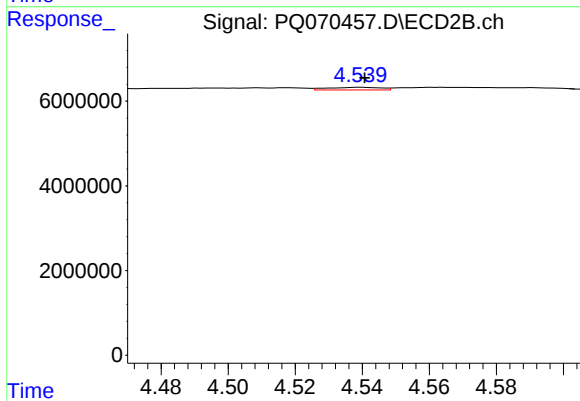

#20 AR-1242-5


R.T.: 4.539 min
Delta R.T.: -0.001 min
Response: 691688
Conc: 3.79 ng/ml

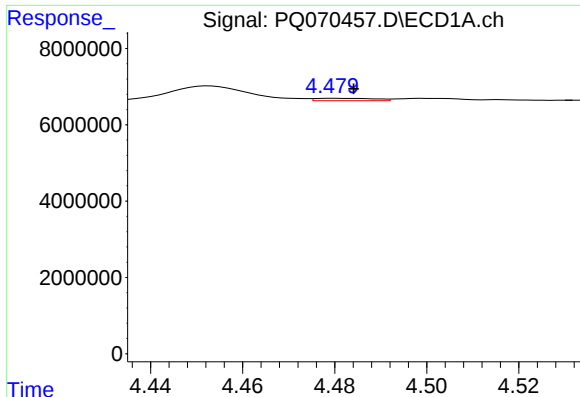

#21 AR-1248-1


R.T.: 4.480 min
Delta R.T.: -0.004 min
Response: 540526
Conc: 4.36 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

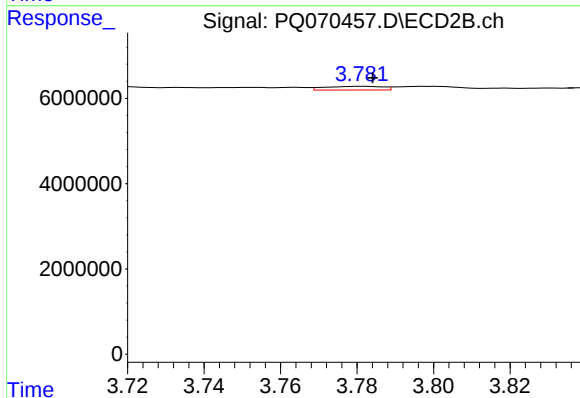


#21 AR-1248-1

R.T.: 3.781 min
Delta R.T.: -0.003 min
Response: 908145
Conc: 6.46 ng/ml

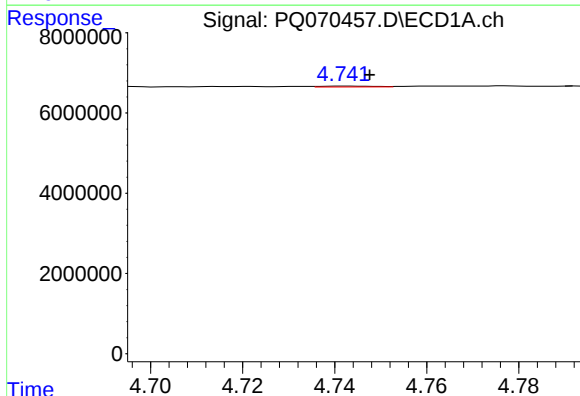


#22 AR-1248-2

R.T.: 4.742 min
Delta R.T.: -0.006 min
Response: 174606
Conc: 0.95 ng/ml

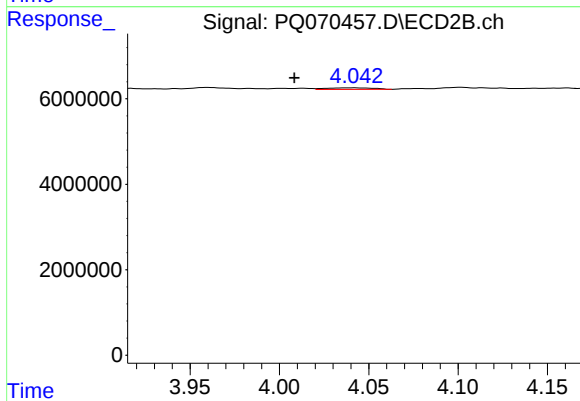

#22 AR-1248-2


R.T.: 4.042 min
Delta R.T.: 0.034 min
Response: 690512
Conc: 2.96 ng/ml

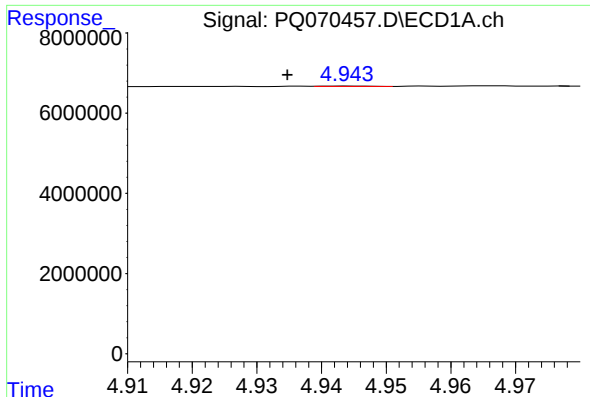

#23 AR-1248-3


R.T.: 4.944 min
Delta R.T.: 0.010 min
Response: 61349
Conc: 0.28 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

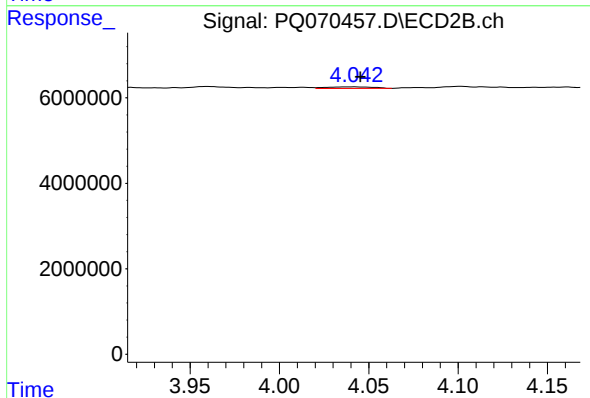


#23 AR-1248-3

R.T.: 4.042 min
Delta R.T.: -0.003 min
Response: 690512
Conc: 3.07 ng/ml

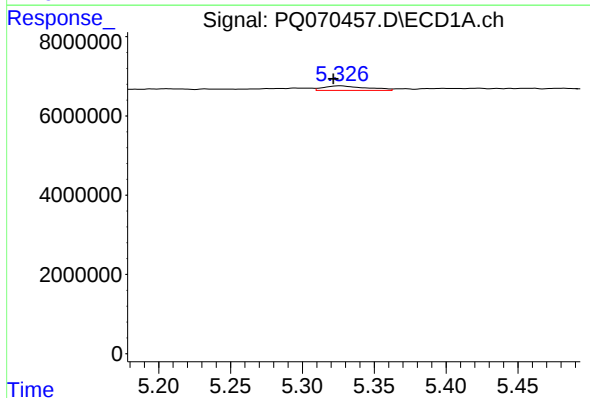


#24 AR-1248-4

R.T.: 5.326 min
Delta R.T.: 0.005 min
Response: 2381866
Conc: 10.73 ng/ml

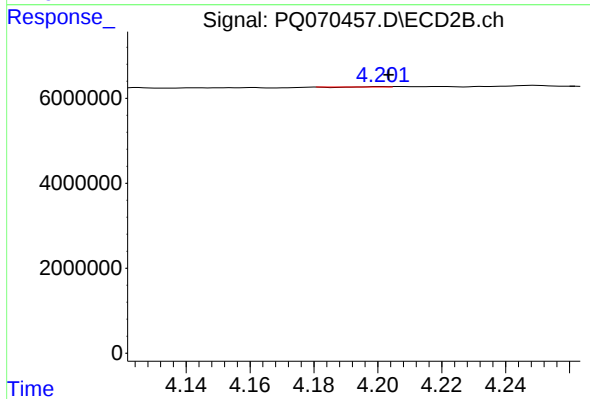

#24 AR-1248-4


R.T.: 4.201 min
Delta R.T.: -0.002 min
Response: 6576
Conc: 0.02 ng/ml

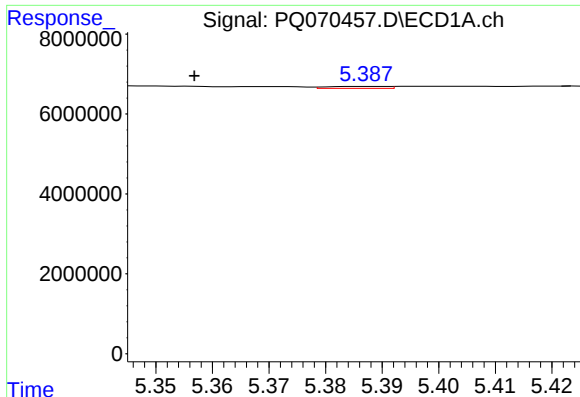

#25 AR-1248-5


R.T.: 5.387 min
Delta R.T.: 0.030 min
Response: 361456
Conc: 1.56 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

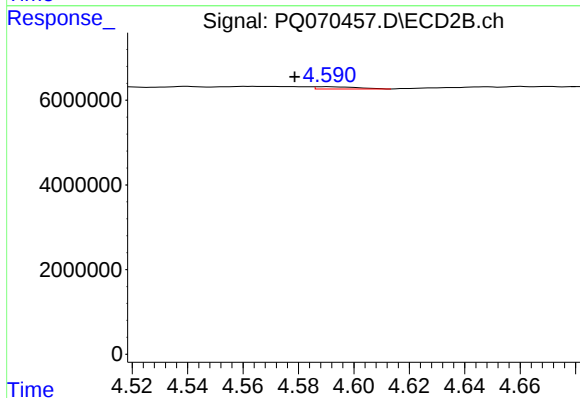


#25 AR-1248-5

R.T.: 4.591 min
Delta R.T.: 0.012 min
Response: 556608
Conc: 2.22 ng/ml

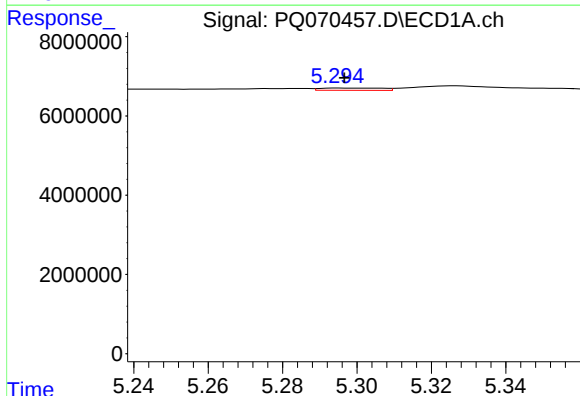


#26 AR-1254-1

R.T.: 5.295 min
Delta R.T.: -0.002 min
Response: 668922
Conc: 2.70 ng/ml

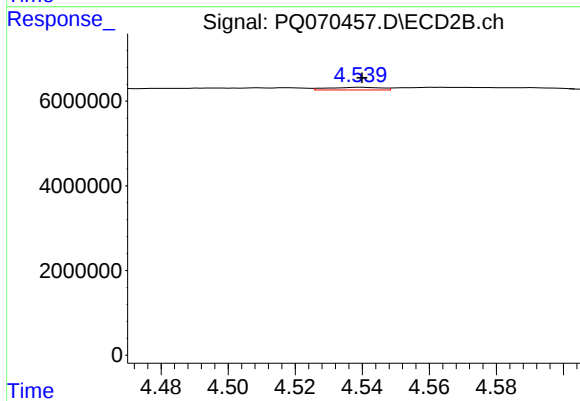

#26 AR-1254-1


R.T.: 4.539 min
Delta R.T.: 0.000 min
Response: 691688
Conc: 1.71 ng/ml

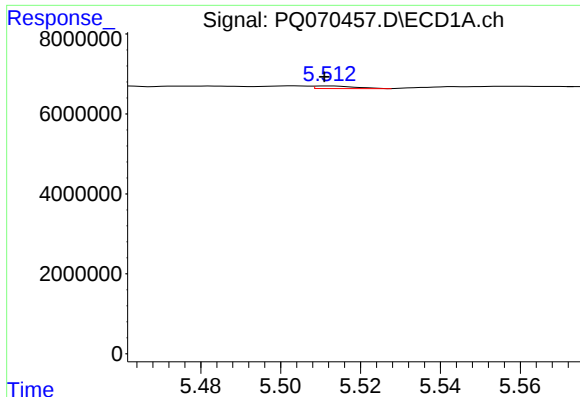

#27 AR-1254-2


R.T.: 5.512 min
Delta R.T.: 0.001 min
Response: 446532
Conc: 1.19 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

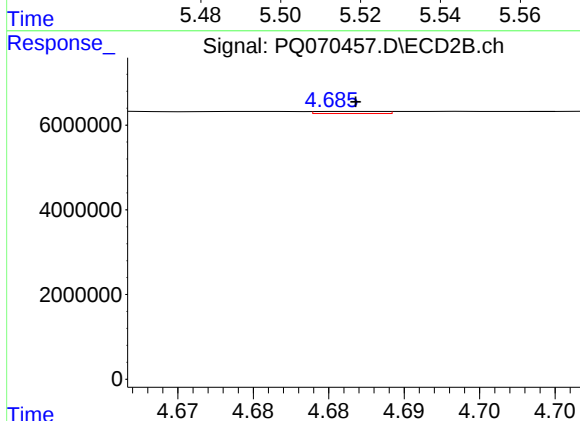


#27 AR-1254-2

R.T.: 4.687 min
Delta R.T.: 0.000 min
Response: 149002
Conc: 0.41 ng/ml

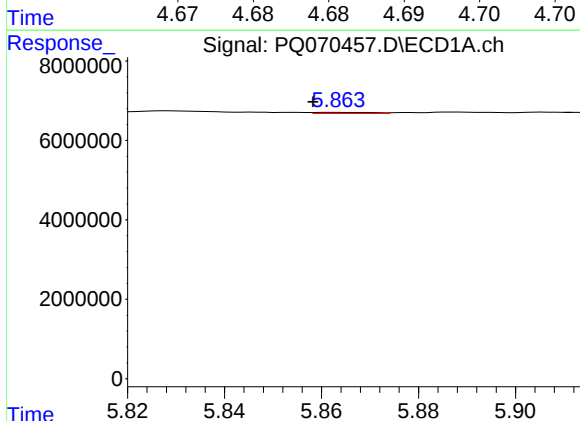


#28 AR-1254-3

R.T.: 5.864 min
Delta R.T.: 0.005 min
Response: 223360
Conc: 0.58 ng/ml

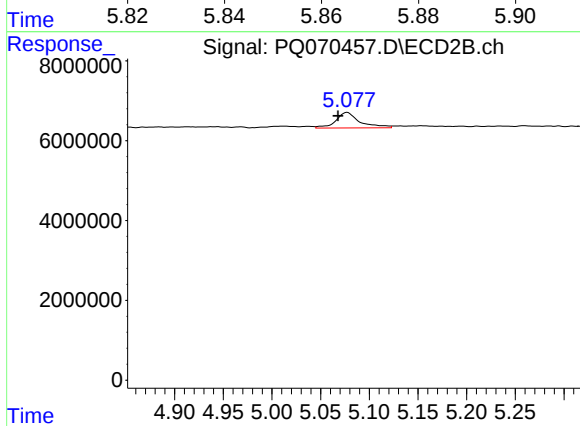

#28 AR-1254-3


R.T.: 5.077 min
Delta R.T.: 0.010 min
Response: 6622715
Conc: 11.71 ng/ml

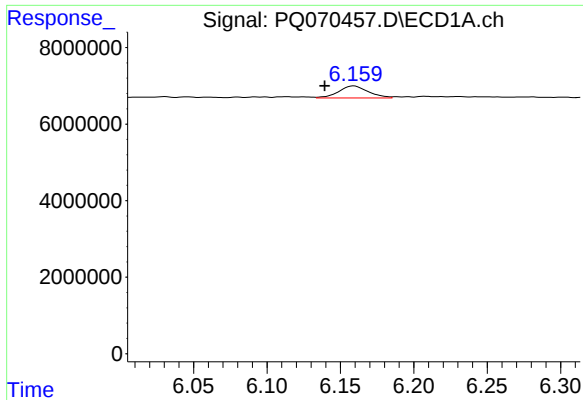

#29 AR-1254-4


R.T.: 6.159 min
Delta R.T.: 0.020 min
Response: 4401979
Conc: 17.68 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

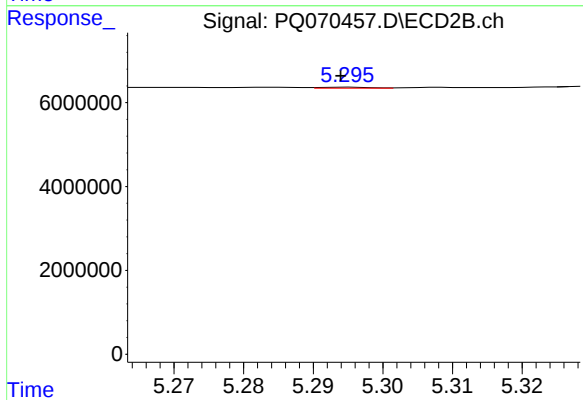


#29 AR-1254-4

R.T.: 5.295 min
Delta R.T.: 0.001 min
Response: 122306
Conc: 0.40 ng/ml

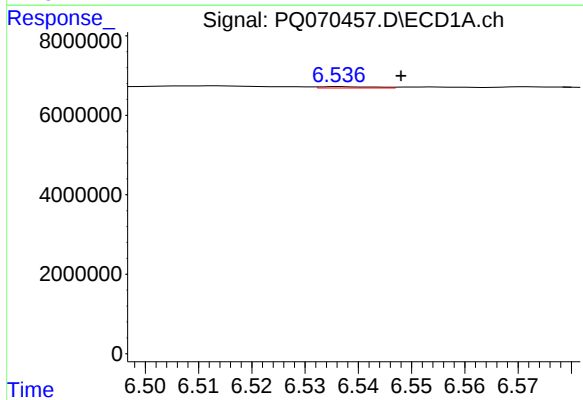


#30 AR-1254-5

R.T.: 6.537 min
Delta R.T.: -0.011 min
Response: 222629
Conc: 0.75 ng/ml

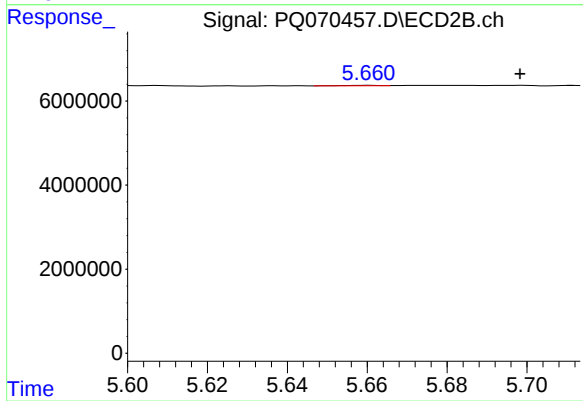

#30 AR-1254-5


R.T.: 5.660 min
Delta R.T.: -0.038 min
Response: 63777
Conc: 0.12 ng/ml

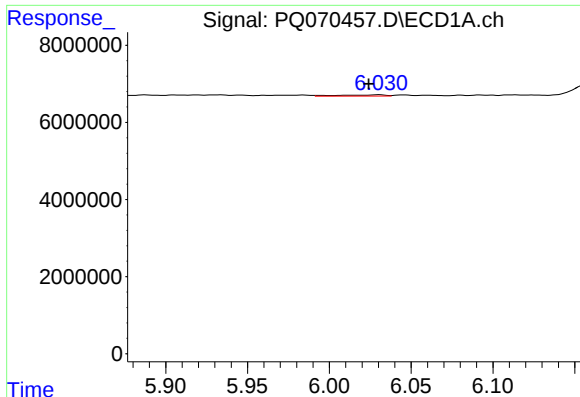

#31 AR-1260-1


R.T.: 6.031 min
Delta R.T.: 0.007 min
Response: 628362
Conc: 2.17 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

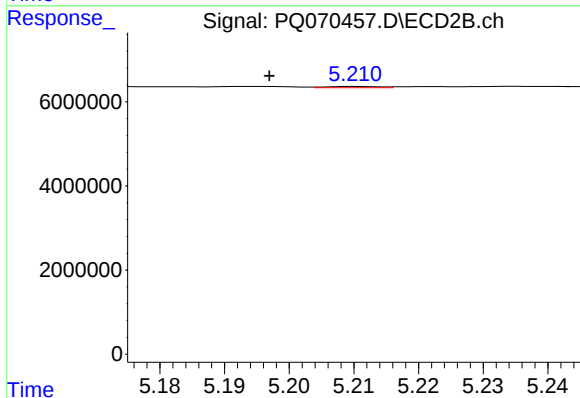


#31 AR-1260-1

R.T.: 5.210 min
Delta R.T.: 0.014 min
Response: 171733
Conc: 0.45 ng/ml

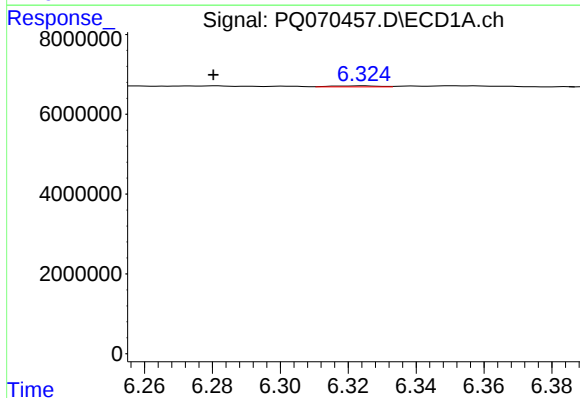


#32 AR-1260-2

R.T.: 6.324 min
Delta R.T.: 0.044 min
Response: 252462
Conc: 0.79 ng/ml

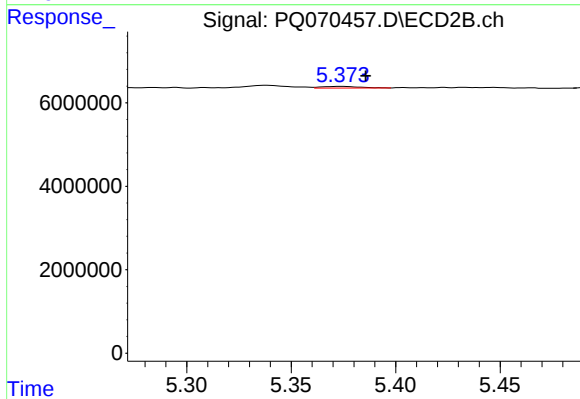

#32 AR-1260-2


R.T.: 5.374 min
Delta R.T.: -0.012 min
Response: 503176
Conc: 1.15 ng/ml

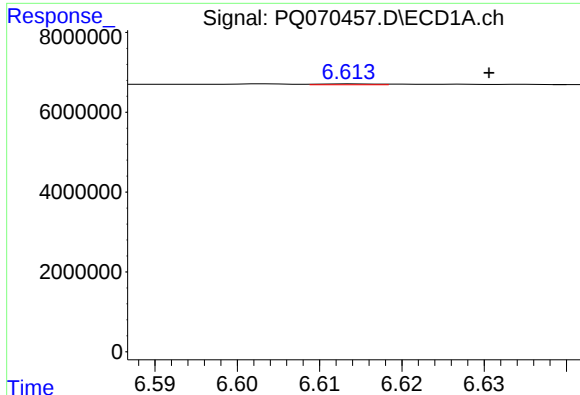

#33 AR-1260-3


R.T.: 6.614 min
Delta R.T.: -0.017 min
Response: 99421
Conc: 0.38 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

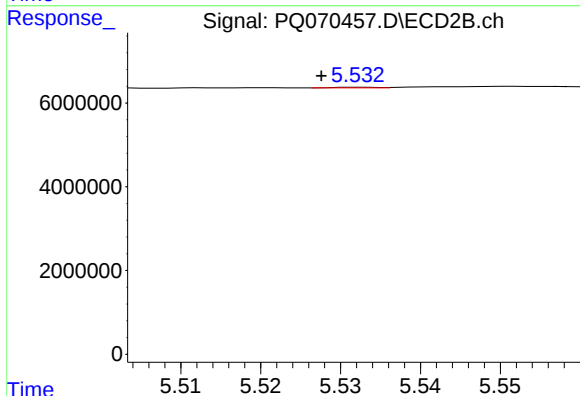


#33 AR-1260-3

R.T.: 5.533 min
Delta R.T.: 0.005 min
Response: 61120
Conc: 0.14 ng/ml

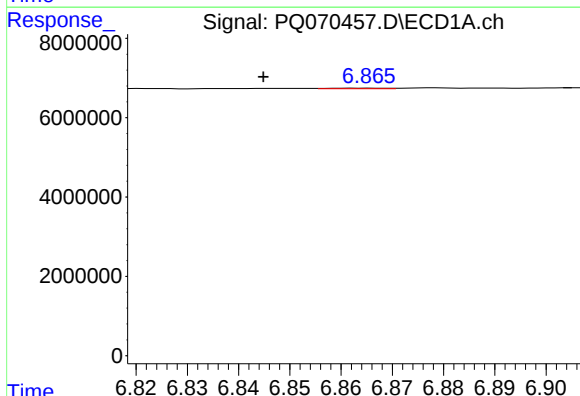


#34 AR-1260-4

R.T.: 6.866 min
Delta R.T.: 0.021 min
Response: 105253
Conc: 0.39 ng/ml

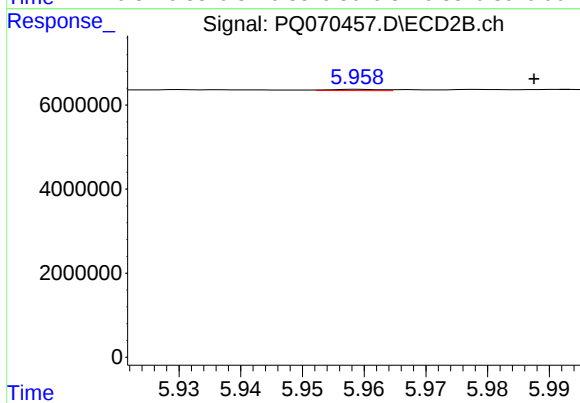

#34 AR-1260-4


R.T.: 5.959 min
Delta R.T.: -0.028 min
Response: 180061
Conc: 0.49 ng/ml

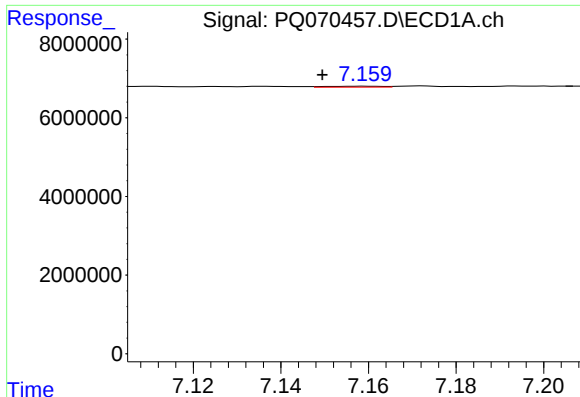

#35 AR-1260-5


R.T.: 7.159 min
Delta R.T.: 0.010 min
Response: 198167
Conc: 0.40 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

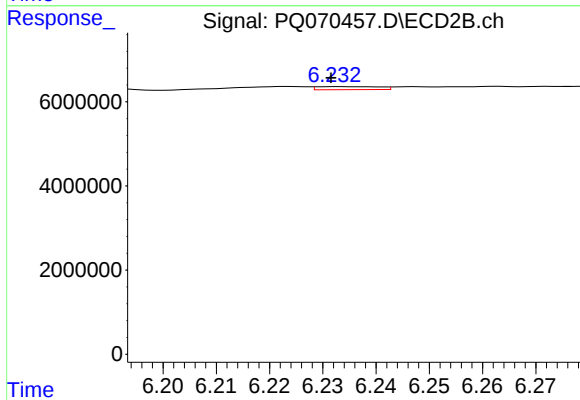


#35 AR-1260-5

R.T.: 6.233 min
Delta R.T.: 0.002 min
Response: 600816
Conc: 0.72 ng/ml

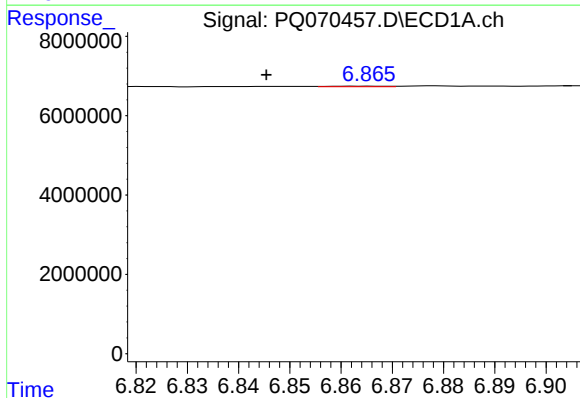


#36 AR-1262-1

R.T.: 6.866 min
Delta R.T.: 0.020 min
Response: 105253
Conc: 0.30 ng/ml

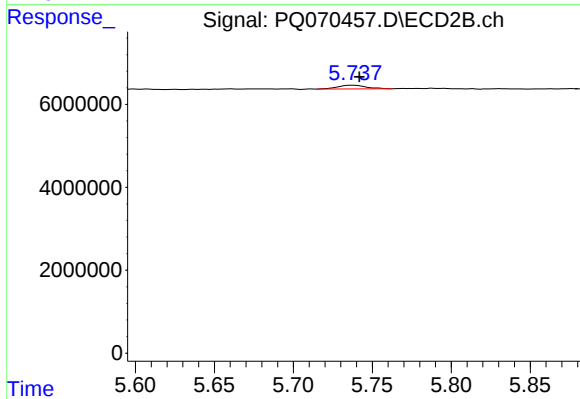

#36 AR-1262-1


R.T.: 5.738 min
Delta R.T.: -0.004 min
Response: 1097696
Conc: 2.01 ng/ml

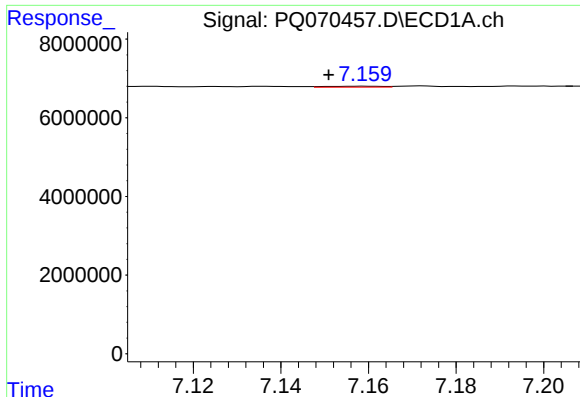

#37 AR-1262-2


R.T.: 7.159 min
Delta R.T.: 0.008 min
Response: 198167
Conc: 0.35 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

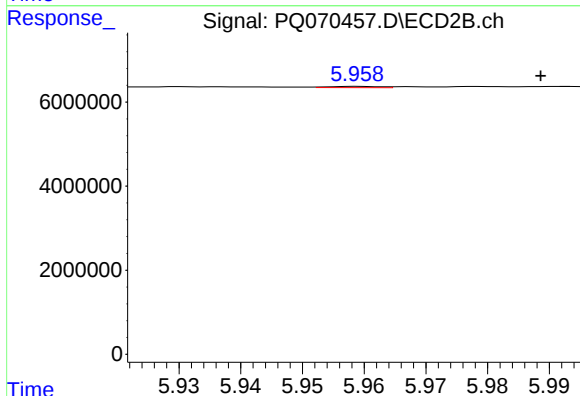


#37 AR-1262-2

R.T.: 5.959 min
Delta R.T.: -0.029 min
Response: 180061
Conc: 0.35 ng/ml

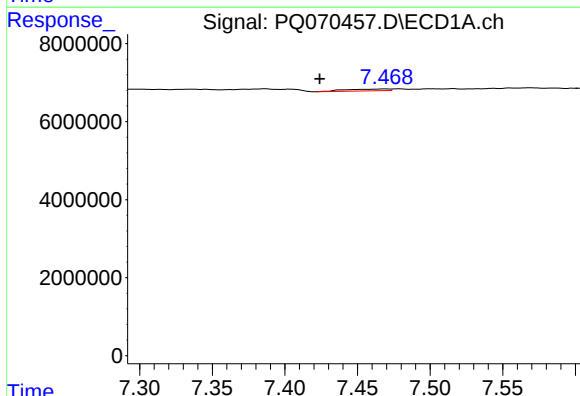


#38 AR-1262-3

R.T.: 7.469 min
Delta R.T.: 0.045 min
Response: 1015167
Conc: 2.61 ng/ml

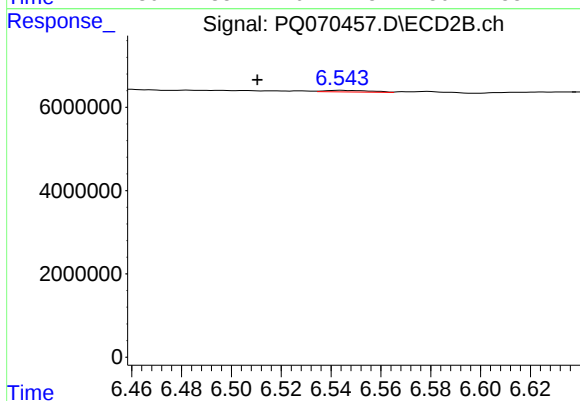

#38 AR-1262-3


R.T.: 6.544 min
Delta R.T.: 0.033 min
Response: 488625
Conc: 1.24 ng/ml

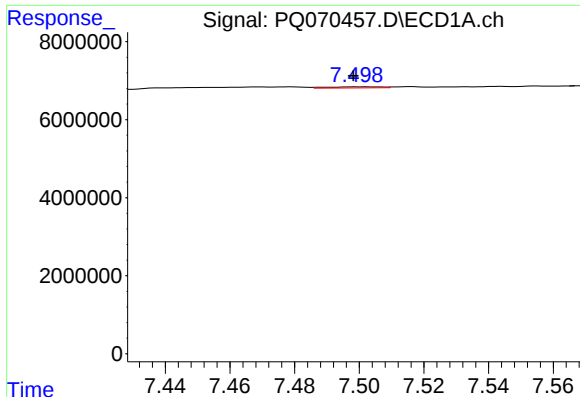

#39 AR-1262-4


R.T.: 7.499 min
Delta R.T.: 0.001 min
Response: 349002
Conc: 1.09 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

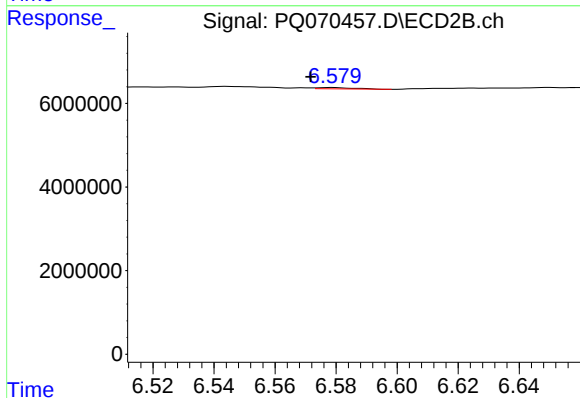


#39 AR-1262-4

R.T.: 6.579 min
Delta R.T.: 0.008 min
Response: 267856
Conc: 0.38 ng/ml

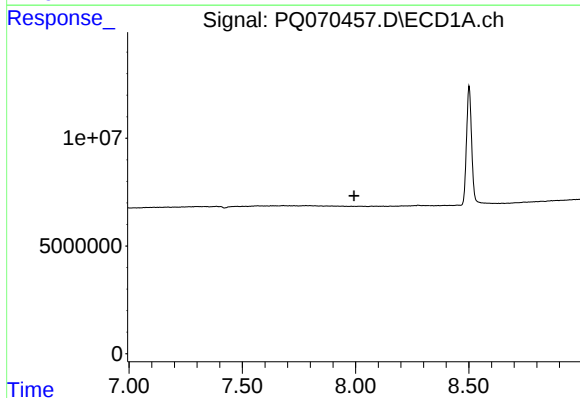


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T. : 7.993 min
Response: 0
Conc: N.D.

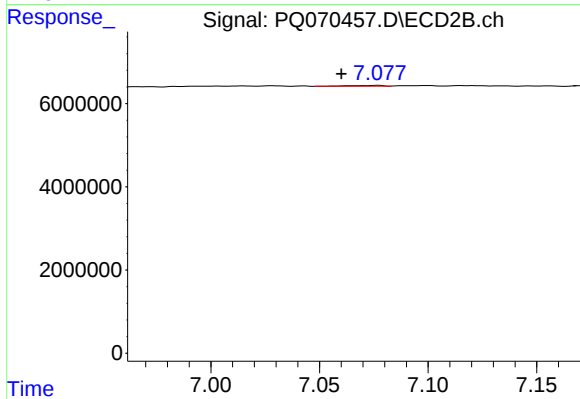

#40 AR-1262-5


R.T.: 7.077 min
Delta R.T.: 0.017 min
Response: 228819
Conc: 0.72 ng/ml

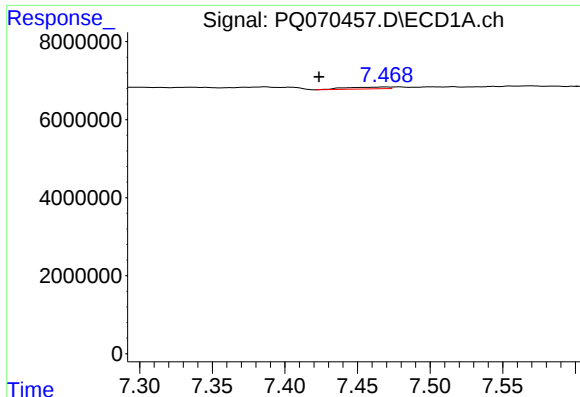

#41 AR-1268-1


R.T.: 7.469 min
Delta R.T.: 0.045 min
Response: 1015167
Conc: 1.41 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

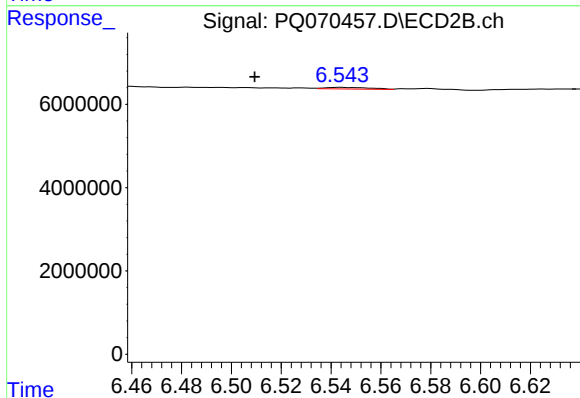


#41 AR-1268-1

R.T.: 6.544 min
Delta R.T.: 0.034 min
Response: 488625
Conc: 0.42 ng/ml

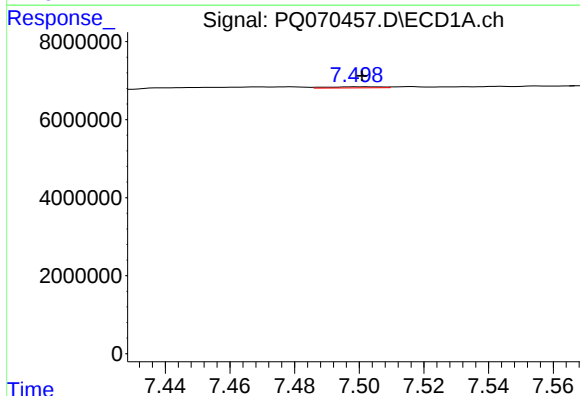


#42 AR-1268-2

R.T.: 7.499 min
Delta R.T.: -0.002 min
Response: 349002
Conc: 0.53 ng/ml

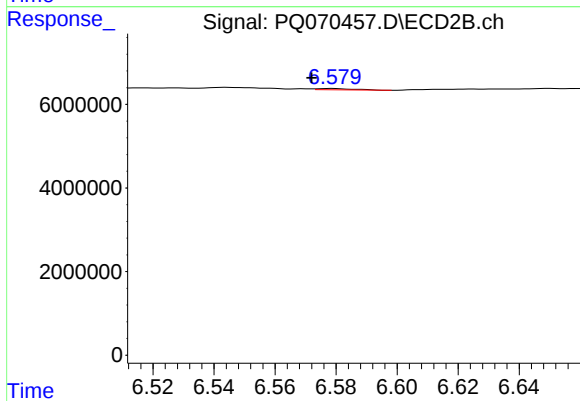

#42 AR-1268-2


R.T.: 6.579 min
Delta R.T.: 0.007 min
Response: 267856
Conc: 0.25 ng/ml

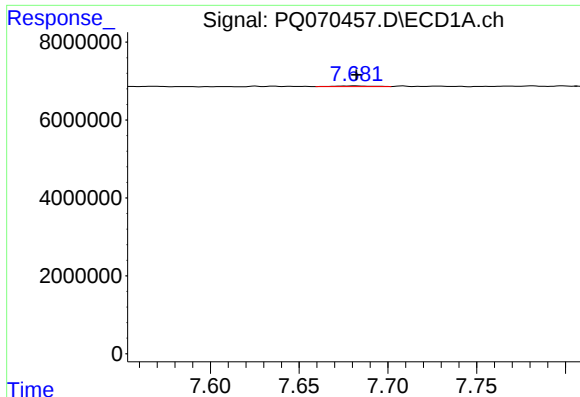

#43 AR-1268-3


R.T.: 7.681 min
Delta R.T.: 0.000 min
Response: 255328
Conc: 0.45 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

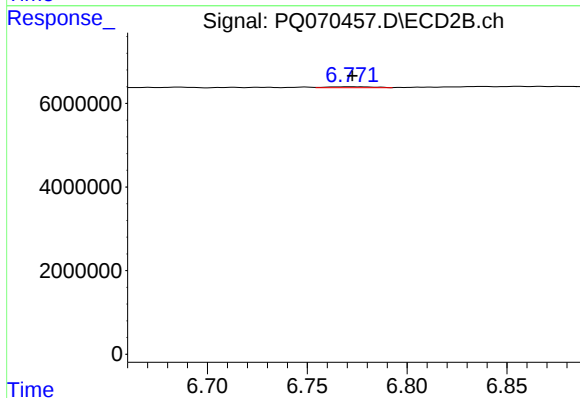


#43 AR-1268-3

R.T.: 6.772 min
Delta R.T.: 0.000 min
Response: 362231
Conc: 0.38 ng/ml

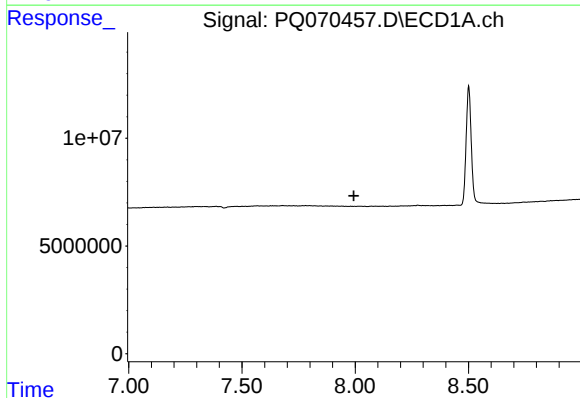


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 7.994 min
Response: 0
Conc: N.D.

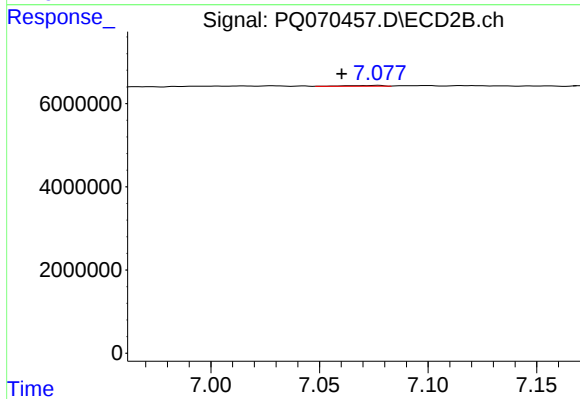

#44 AR-1268-4


R.T.: 7.077 min
Delta R.T.: 0.017 min
Response: 228819
Conc: 0.61 ng/ml

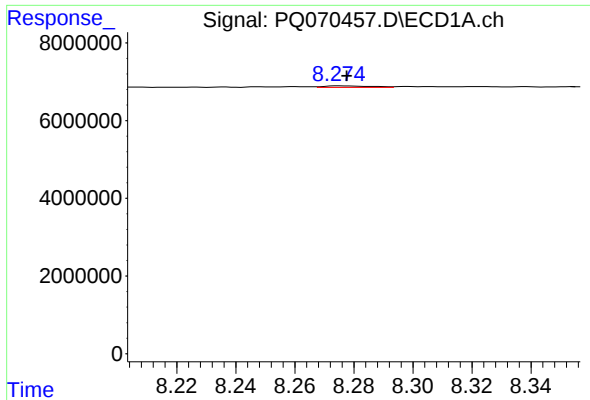

#45 AR-1268-5

R.T.: 8.275 min
Delta R.T.: -0.003 min
Response: 441316
Conc: 0.28 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

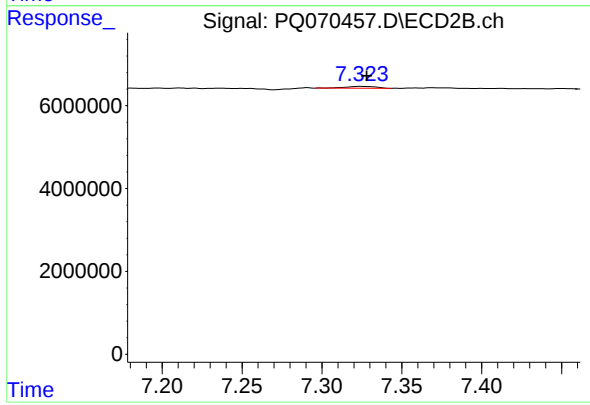

#45 AR-1268-5

R.T.: 7.324 min
Delta R.T.: -0.004 min
Response: 597522
Conc: 0.23 ng/ml