

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ062525\
 Data File : PQ070458.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jun 2025 10:53
 Operator : YP\AJ
 Sample : Q2126-09
 Misc : AR1232 MDL 25 PPB
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 MDL-WATER-03-QT2-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 04:56:14 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ062425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jun 26 02:49:53 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.403	2.781	114.9E6	127.4E6	18.764	18.865
2)	SA Decachlor...	8.502	7.543	87909565	153.9E6	21.355	21.222
Target Compounds							
3)	L1 AR-1016-1	4.483	3.783	2383073	2349265	12.696	11.312
4)	L1 AR-1016-2	4.502	3.798	3581883	3534923	11.567	10.451
5)	L1 AR-1016-3	4.560	3.959	2161597	1856165	10.744	9.891
6)	L1 AR-1016-4	4.649	4.007	1477163	1472990	9.332	8.397
7)	L1 AR-1016-5	4.934	4.202	1630798	1877628	10.027	9.303
8)	L2 AR-1221-1	3.598	2.982	914520	1327350	10.666	12.983
9)	L2 AR-1221-2	3.675	3.051	2576331	2809463	39.862	35.616
10)	L2 AR-1221-3	3.742	3.126	3385654	3351409	17.456	14.786
11)	L3 AR-1232-1	3.742	3.126	3385654	3351409	23.926	20.106
12)	L3 AR-1232-2	4.229	3.798	1838424	3534923	22.687	22.154
13)	L3 AR-1232-3	4.502	3.959	3581883	1856165	25.102	21.119
14)	L3 AR-1232-4	4.649	4.043	1477163	1940371	20.544	25.151
15)	L3 AR-1232-5	4.786	4.202	1190829	1877628	19.926	22.421
16)	L4 AR-1242-1	4.483	3.783	2383073	2349265	15.399	13.391
17)	L4 AR-1242-2	4.502	3.798	3581883	3534923	13.635	12.695
18)	L4 AR-1242-3	4.560	3.959	2161597	1856165	12.724	11.810
19)	L4 AR-1242-4	4.649	4.043	1477163	1940371	10.946	12.742
20)	L4 AR-1242-5	5.354	4.540	1826041	2900811	13.577	15.897
21)	L5 AR-1248-1	4.483	3.783	2383073	2349265	19.242	16.714
22)	L5 AR-1248-2	4.747	4.007	996530	1472990	5.402	6.310
23)	L5 AR-1248-3	4.934	4.043	1630798	1940371	7.385	8.619
24)	L5 AR-1248-4	5.321	4.202	2469838	1877628	11.129	6.886 #
25)	L5 AR-1248-5	5.354	4.578	1826041	3782510	7.901	15.104 #
26)	L6 AR-1254-1	5.294	4.540	1800160	2900811	7.277	7.160
27)	L6 AR-1254-2	5.506	4.682	2203701	1179341	5.867	3.266 #
28)	L6 AR-1254-3	5.857	5.076	454882	5150207	1.172	9.107 #
29)	L6 AR-1254-4	6.159	5.292	4768244	575467	19.155	1.887 #
30)	L6 AR-1254-5	6.509f	5.694	1414508	229514	4.762	0.446 #
31)	L7 AR-1260-1	6.022	5.193	392087	516385	1.357	1.352
32)	L7 AR-1260-2	6.255f	5.371	553871	274457	1.737	0.626 #
33)	L7 AR-1260-3	6.635	5.544	178589	347111	0.688	0.805
34)	L7 AR-1260-4	6.835	5.995	96013	414554	0.352	1.130 #
35)	L7 AR-1260-5	0.000	6.228	0	700051	N.D.	0.842 #
36)	L8 AR-1262-1	6.835	5.735	96013	1564435	0.273	2.859 #
37)	L8 AR-1262-2	0.000	5.995	0	414554	N.D.	0.815 #
38)	L8 AR-1262-3	7.435	6.529	135996	97121	0.349	0.247 #
39)	L8 AR-1262-4	7.486	6.529f	191502	97121	0.598	0.139 #
40)	L8 AR-1262-5	8.007	7.059	84193	63654	0.449	0.201 #
41)	L9 AR-1268-1	7.435	6.529	135996	97121	0.189	0.084 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ062525\
Data File : PQ070458.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jun 2025 10:53
Operator : YP\AJ
Sample : Q2126-09
Misc : AR1232 MDL 25 PPB
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 04:56:14 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ062425.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 26 02:49:53 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	7.486	6.529f	191502	97121	0.288	0.091 #
43)	L9 AR-1268-3	0.000	6.760	0	308093	N.D.	0.323 #
44)	L9 AR-1268-4	8.007	7.059	84193	63654	0.408	0.169 #
45)	L9 AR-1268-5	8.274	7.323	396898	613549	0.248	0.233



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ062525\
Data File : PQ070458.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jun 2025 10:53
Operator : YP\AJ
Sample : Q2126-09
Misc : AR1232 MDL 25 PPB
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 04:56:14 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ062425.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 26 02:49:53 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

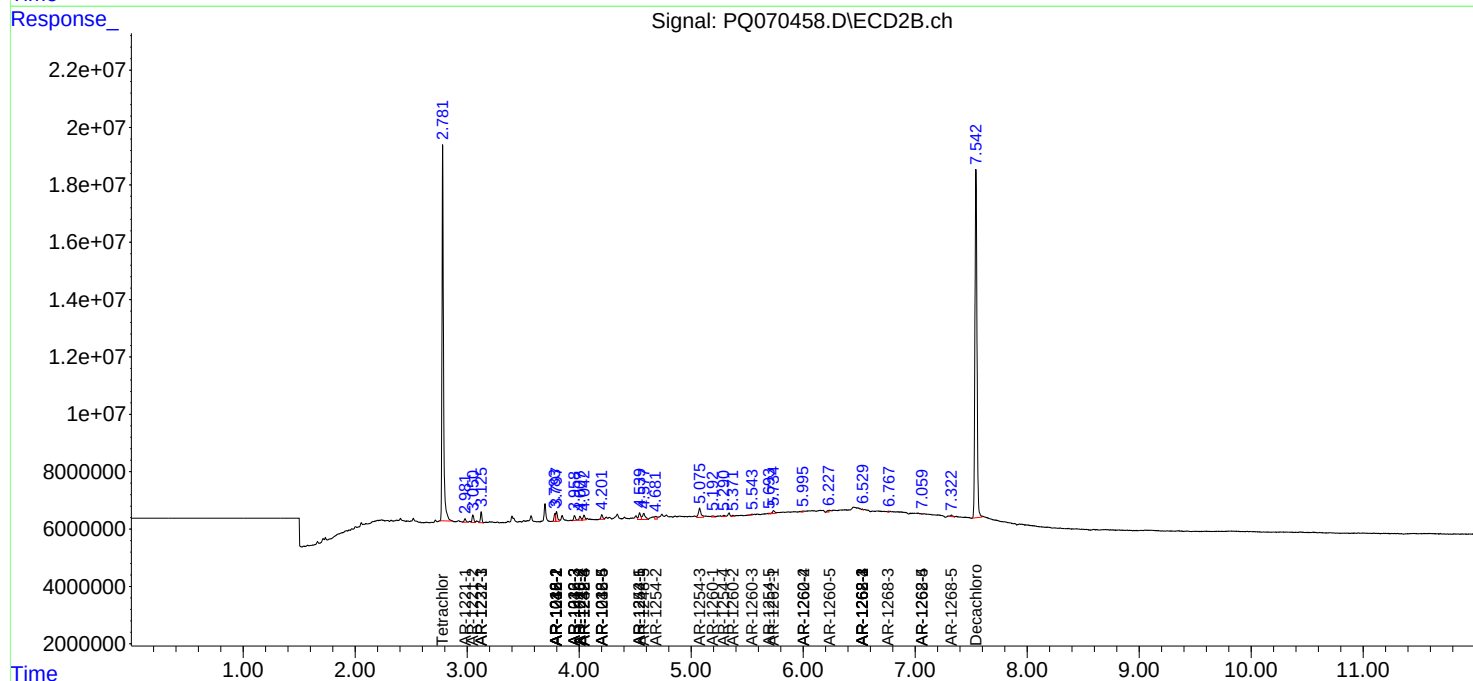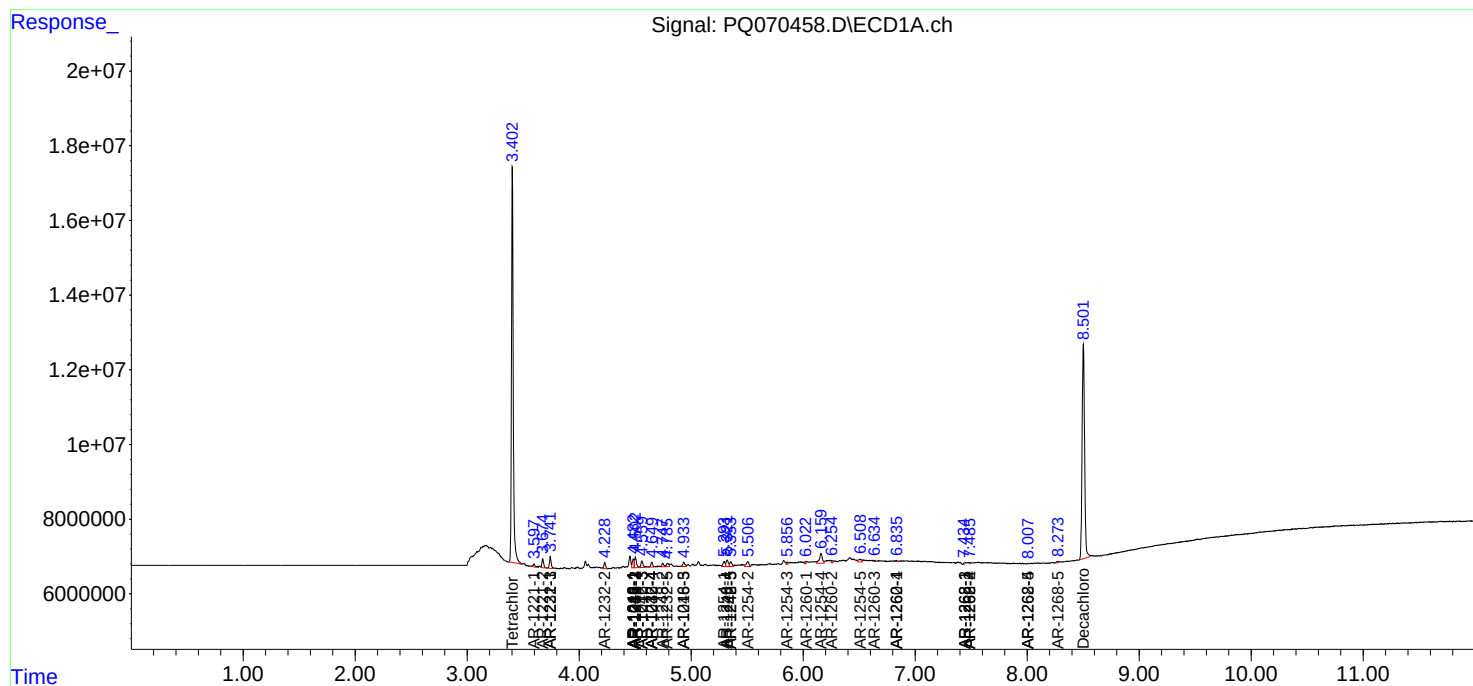


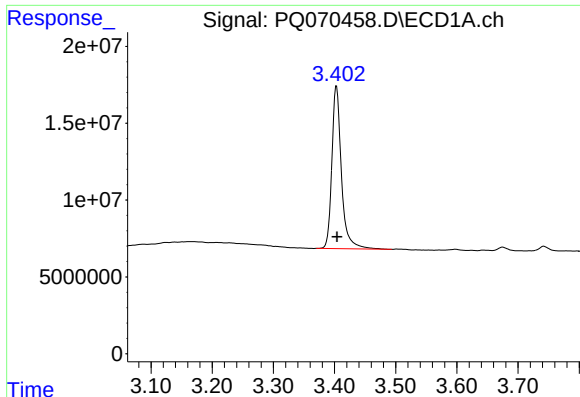

#1 Tetrachloro-m-xylene


R.T.: 3.403 min
Delta R.T.: 0.000 min
Response: 114868218
Conc: 18.76 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

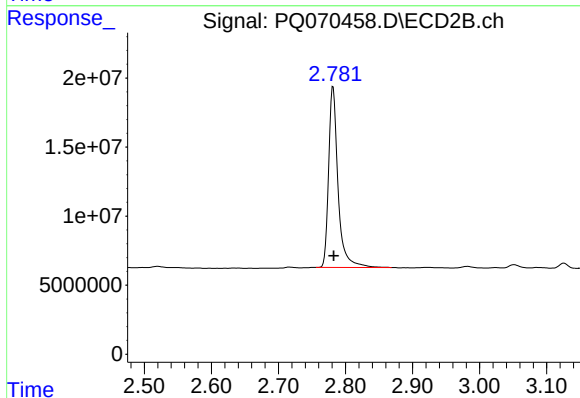


#1 Tetrachloro-m-xylene

R.T.: 2.781 min
Delta R.T.: 0.000 min
Response: 127395875
Conc: 18.86 ng/ml

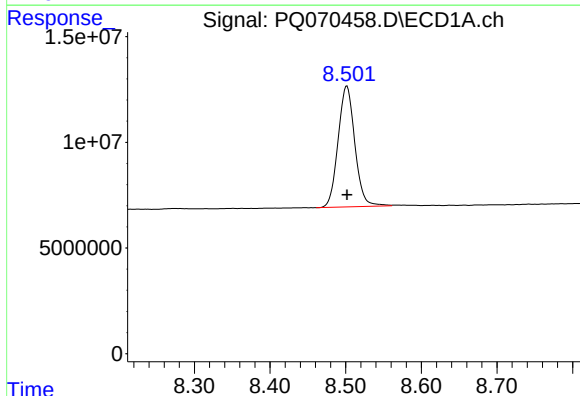


#2 Decachlorobiphenyl

R.T.: 8.502 min
Delta R.T.: 0.000 min
Response: 87909565
Conc: 21.36 ng/ml

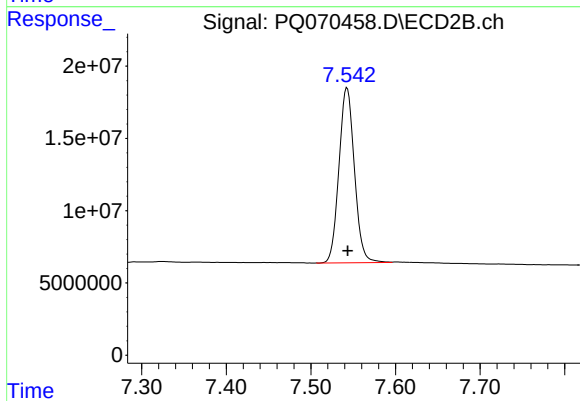

#2 Decachlorobiphenyl


R.T.: 7.543 min
Delta R.T.: 0.000 min
Response: 153850722
Conc: 21.22 ng/ml

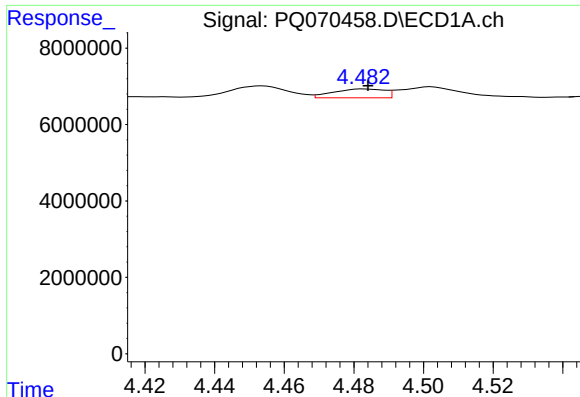

#3 AR-1016-1


R.T.: 4.483 min
Delta R.T.: -0.001 min
Response: 2383073
Conc: 12.70 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

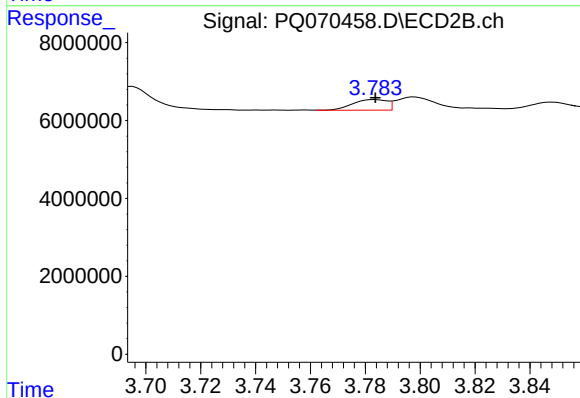


#3 AR-1016-1

R.T.: 3.783 min
Delta R.T.: 0.000 min
Response: 2349265
Conc: 11.31 ng/ml

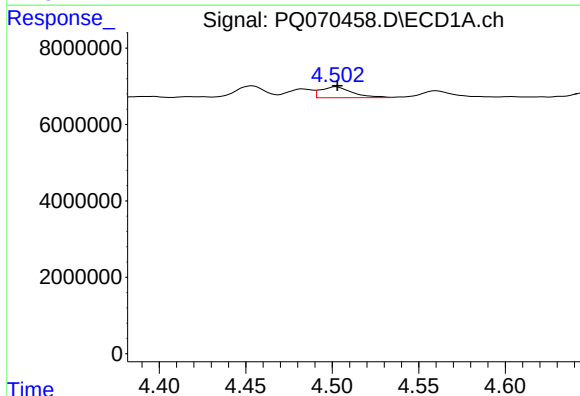


#4 AR-1016-2

R.T.: 4.502 min
Delta R.T.: 0.000 min
Response: 3581883
Conc: 11.57 ng/ml

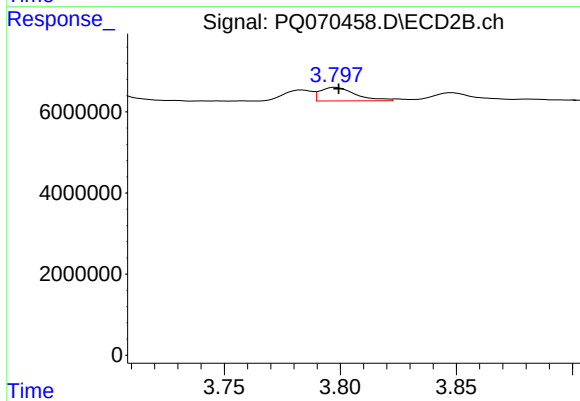

#4 AR-1016-2


R.T.: 3.798 min
Delta R.T.: -0.001 min
Response: 3534923
Conc: 10.45 ng/ml

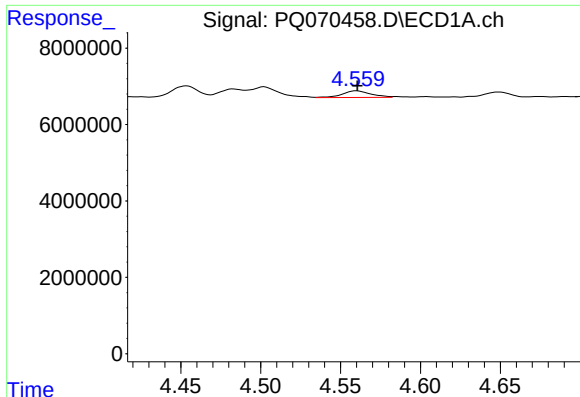

#5 AR-1016-3


R.T.: 4.560 min
Delta R.T.: 0.000 min
Response: 2161597
Conc: 10.74 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

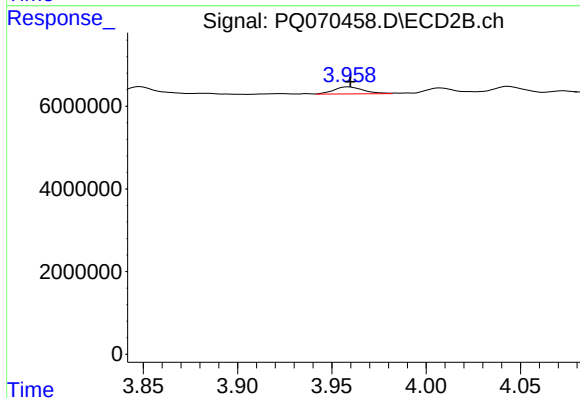


#5 AR-1016-3

R.T.: 3.959 min
Delta R.T.: -0.001 min
Response: 1856165
Conc: 9.89 ng/ml

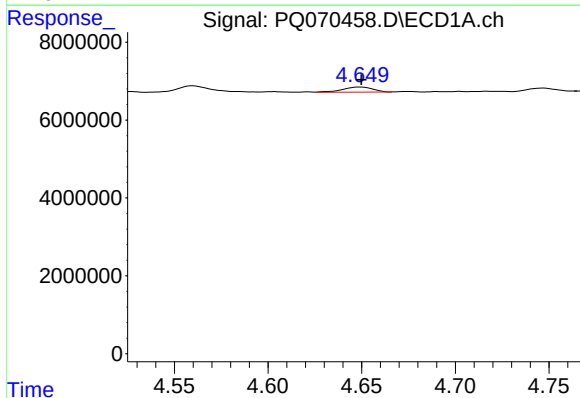


#6 AR-1016-4

R.T.: 4.649 min
Delta R.T.: 0.000 min
Response: 1477163
Conc: 9.33 ng/ml

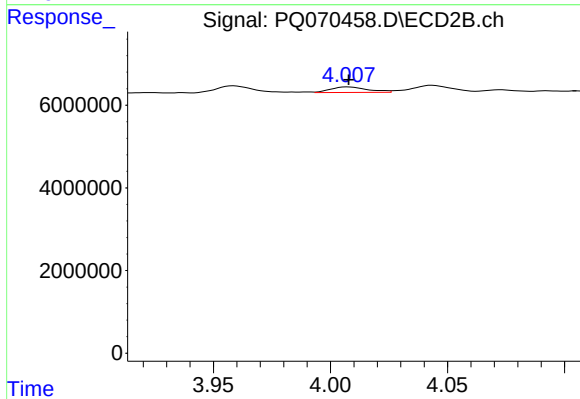

#6 AR-1016-4


R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 1472990
Conc: 8.40 ng/ml

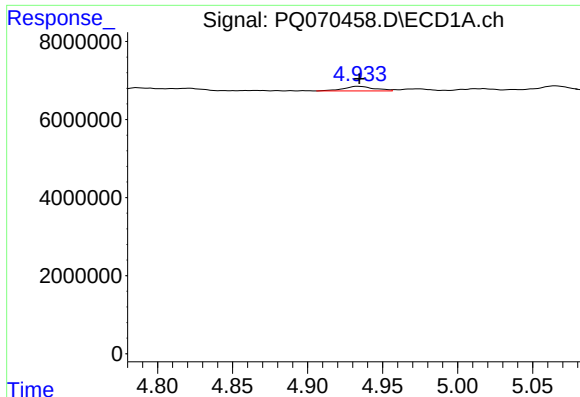

#7 AR-1016-5


R.T.: 4.934 min
Delta R.T.: 0.000 min
Response: 1630798
Conc: 10.03 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

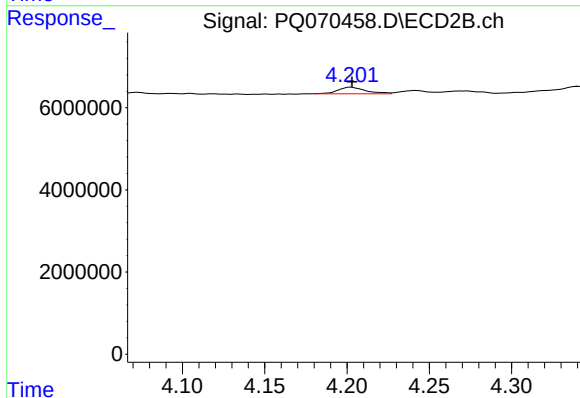


#7 AR-1016-5

R.T.: 4.202 min
Delta R.T.: 0.000 min
Response: 1877628
Conc: 9.30 ng/ml

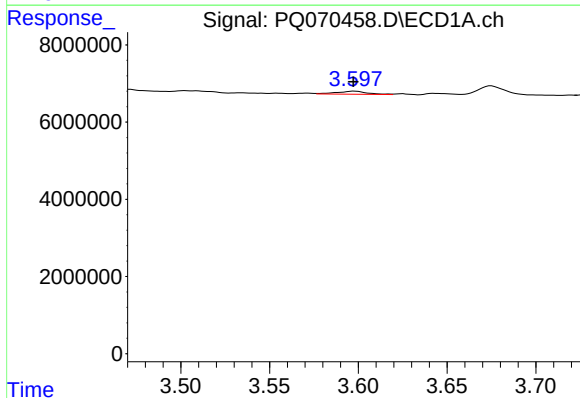


#8 AR-1221-1

R.T.: 3.598 min
Delta R.T.: 0.000 min
Response: 914520
Conc: 10.67 ng/ml

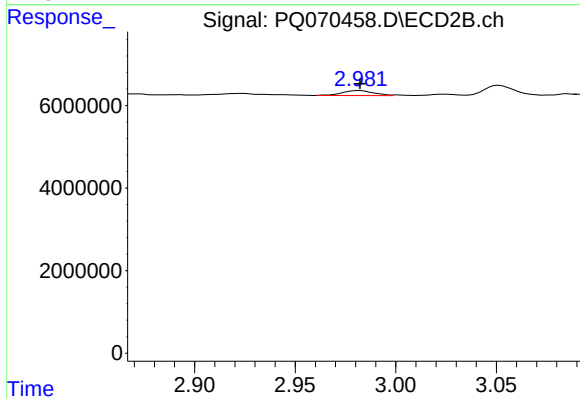

#8 AR-1221-1


R.T.: 2.982 min
Delta R.T.: 0.000 min
Response: 1327350
Conc: 12.98 ng/ml

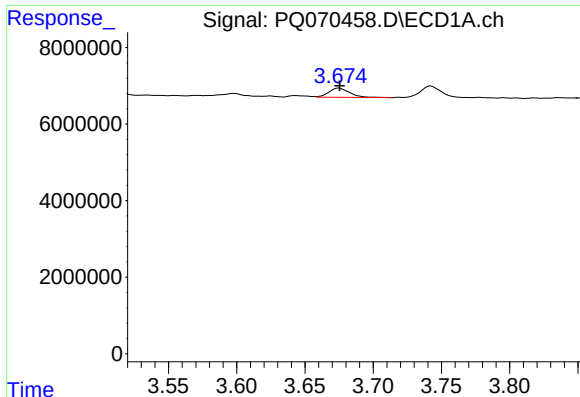

#9 AR-1221-2


R.T.: 3.675 min
Delta R.T.: 0.000 min
Response: 2576331
Conc: 39.86 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

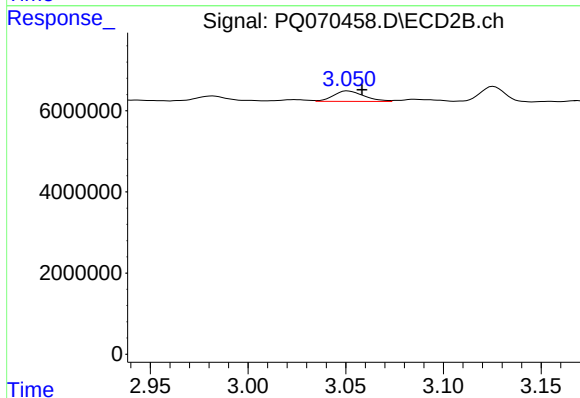


#9 AR-1221-2

R.T.: 3.051 min
Delta R.T.: -0.007 min
Response: 2809463
Conc: 35.62 ng/ml

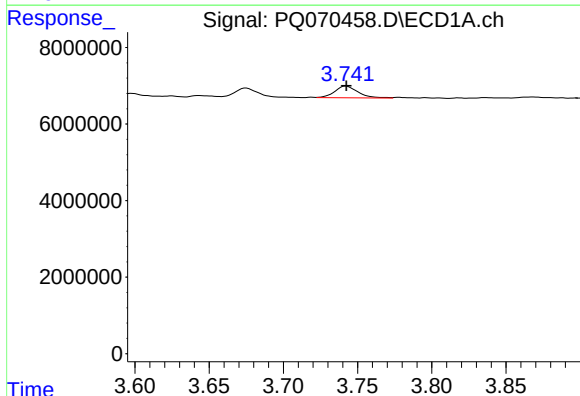


#10 AR-1221-3

R.T.: 3.742 min
Delta R.T.: 0.000 min
Response: 3385654
Conc: 17.46 ng/ml

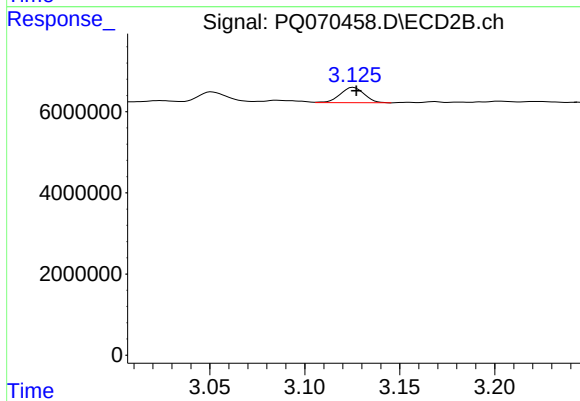

#10 AR-1221-3


R.T.: 3.126 min
Delta R.T.: -0.002 min
Response: 3351409
Conc: 14.79 ng/ml

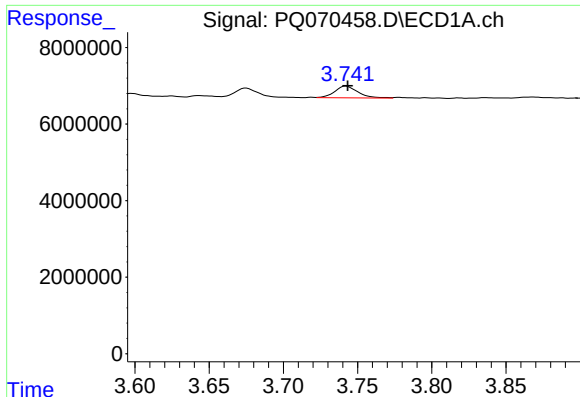

#11 AR-1232-1


R.T.: 3.742 min
Delta R.T.: -0.001 min
Response: 3385654
Conc: 23.93 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

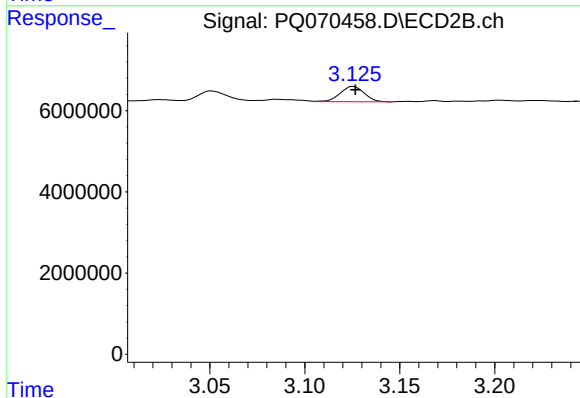


#11 AR-1232-1

R.T.: 3.126 min
Delta R.T.: 0.000 min
Response: 3351409
Conc: 20.11 ng/ml

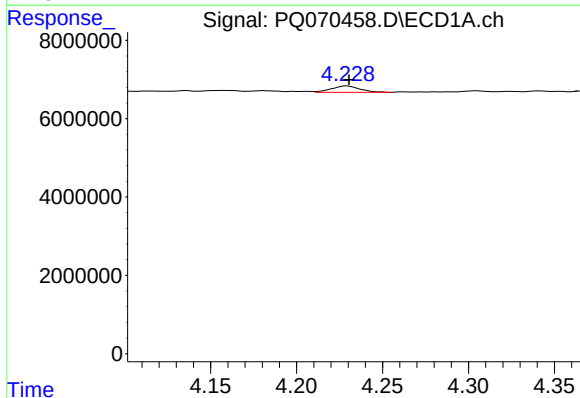


#12 AR-1232-2

R.T.: 4.229 min
Delta R.T.: -0.001 min
Response: 1838424
Conc: 22.69 ng/ml

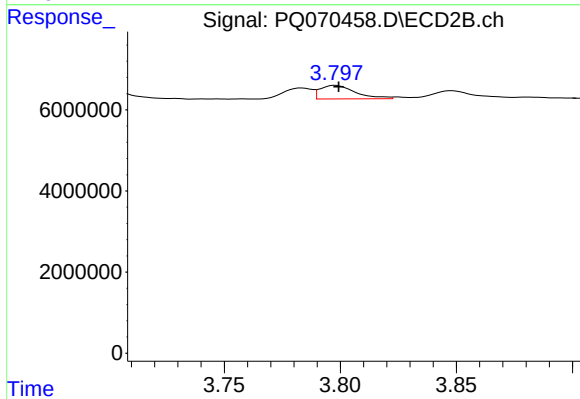

#12 AR-1232-2


R.T.: 3.798 min
Delta R.T.: -0.001 min
Response: 3534923
Conc: 22.15 ng/ml

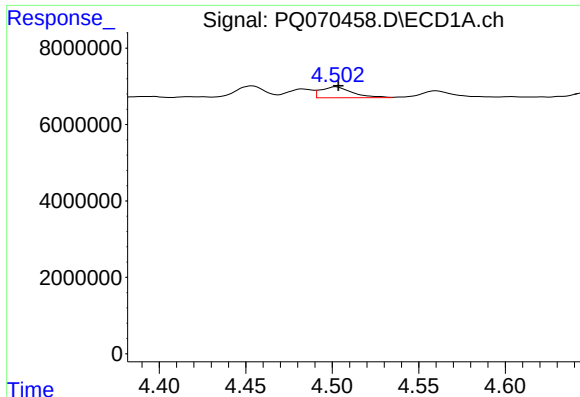

#13 AR-1232-3


R.T.: 4.502 min
Delta R.T.: -0.001 min
Response: 3581883
Conc: 25.10 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

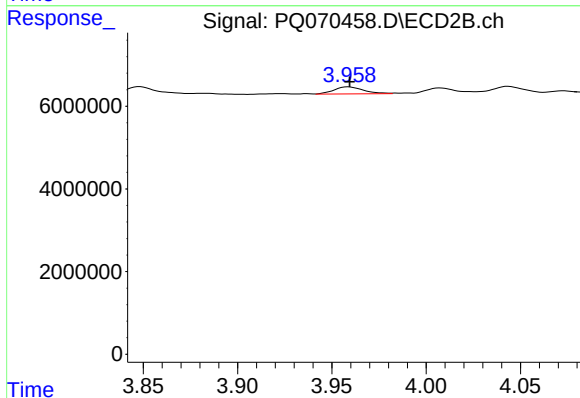


#13 AR-1232-3

R.T.: 3.959 min
Delta R.T.: 0.000 min
Response: 1856165
Conc: 21.12 ng/ml

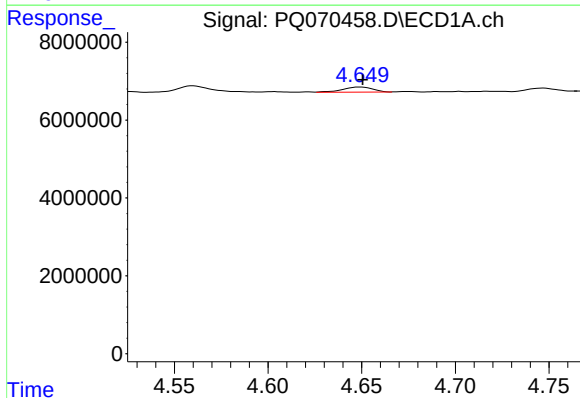


#14 AR-1232-4

R.T.: 4.649 min
Delta R.T.: -0.001 min
Response: 1477163
Conc: 20.54 ng/ml

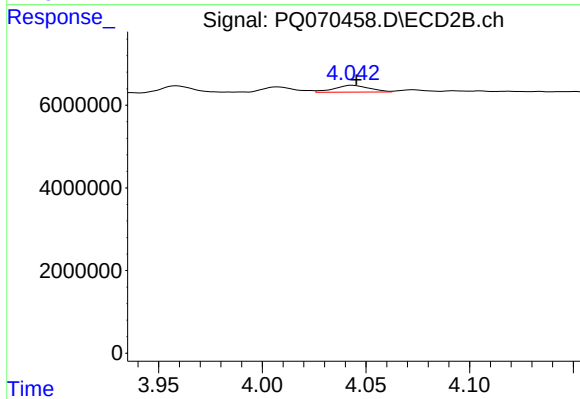

#14 AR-1232-4


R.T.: 4.043 min
Delta R.T.: -0.002 min
Response: 1940371
Conc: 25.15 ng/ml

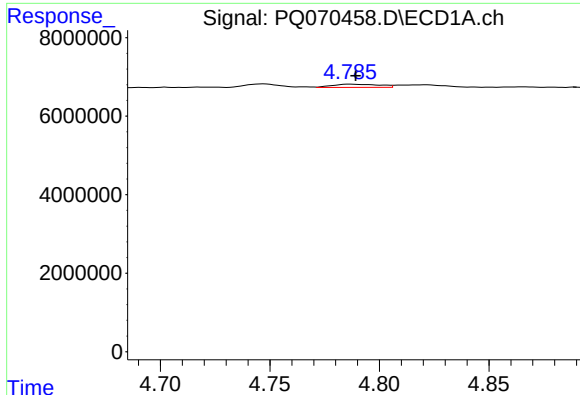

#15 AR-1232-5


R.T.: 4.786 min
Delta R.T.: -0.003 min
Response: 1190829
Conc: 19.93 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

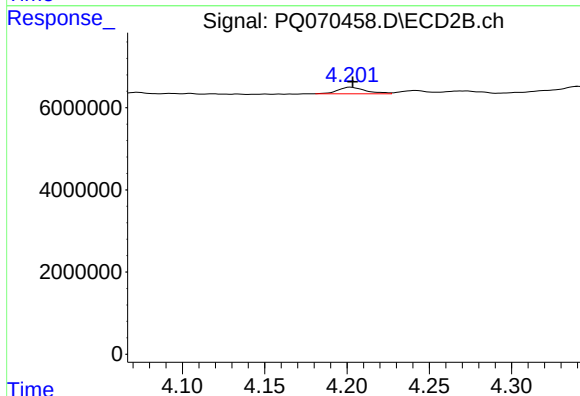


#15 AR-1232-5

R.T.: 4.202 min
Delta R.T.: -0.001 min
Response: 1877628
Conc: 22.42 ng/ml

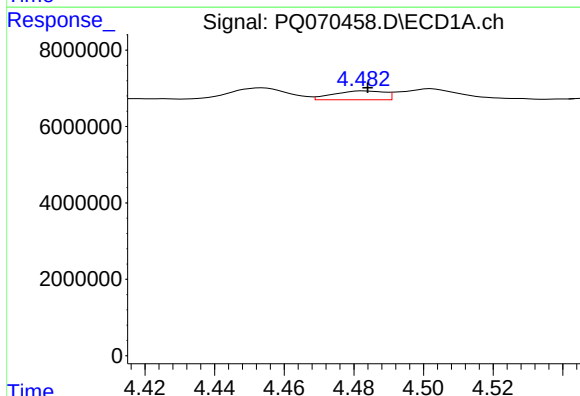


#16 AR-1242-1

R.T.: 4.483 min
Delta R.T.: -0.001 min
Response: 2383073
Conc: 15.40 ng/ml

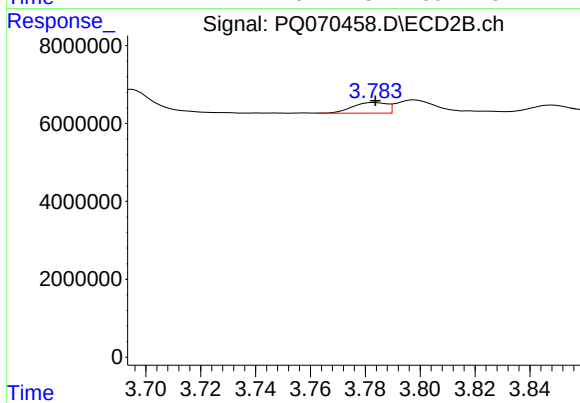

#16 AR-1242-1


R.T.: 3.783 min
Delta R.T.: 0.000 min
Response: 2349265
Conc: 13.39 ng/ml

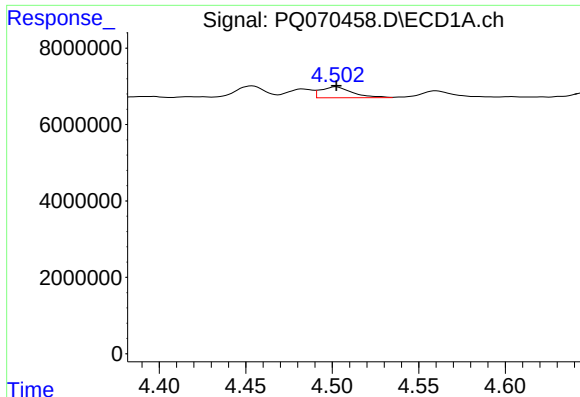

#17 AR-1242-2


R.T.: 4.502 min
Delta R.T.: 0.000 min
Response: 3581883
Conc: 13.64 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

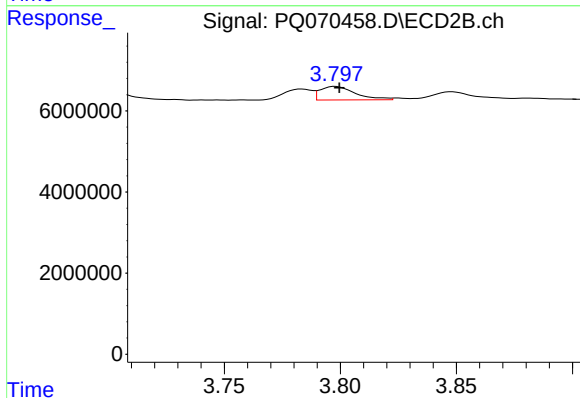


#17 AR-1242-2

R.T.: 3.798 min
Delta R.T.: -0.002 min
Response: 3534923
Conc: 12.69 ng/ml

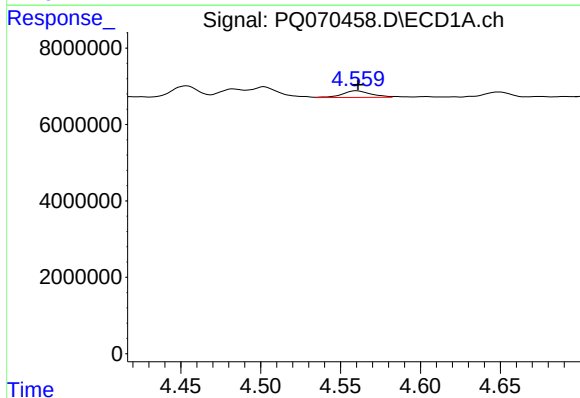


#18 AR-1242-3

R.T.: 4.560 min
Delta R.T.: 0.000 min
Response: 2161597
Conc: 12.72 ng/ml

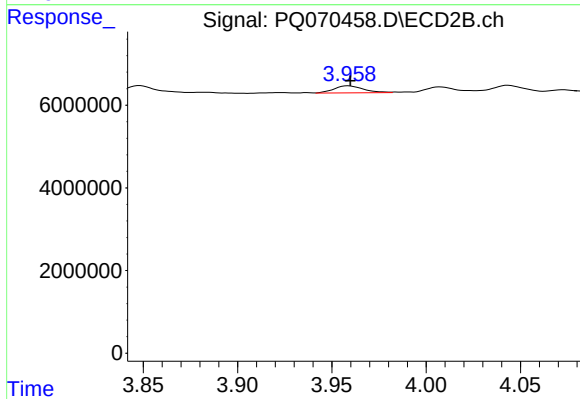

#18 AR-1242-3


R.T.: 3.959 min
Delta R.T.: -0.001 min
Response: 1856165
Conc: 11.81 ng/ml

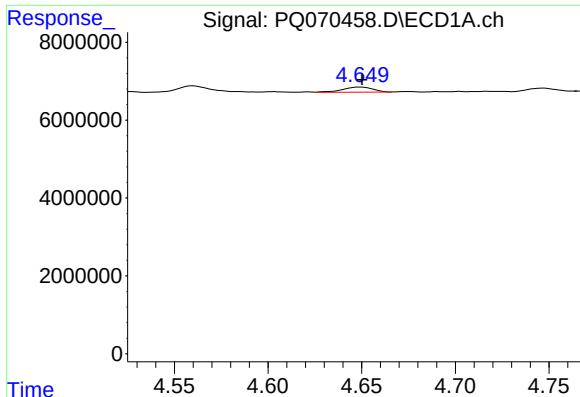

#19 AR-1242-4


R.T.: 4.649 min
Delta R.T.: 0.000 min
Response: 1477163
Conc: 10.95 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

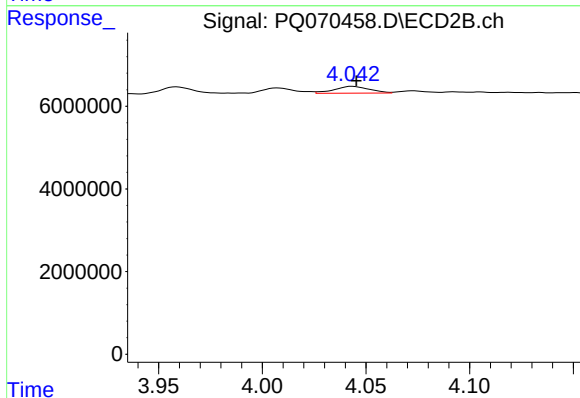


#19 AR-1242-4

R.T.: 4.043 min
Delta R.T.: -0.002 min
Response: 1940371
Conc: 12.74 ng/ml

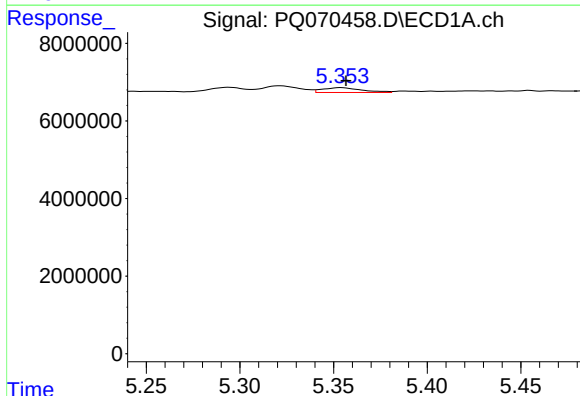


#20 AR-1242-5

R.T.: 5.354 min
Delta R.T.: -0.003 min
Response: 1826041
Conc: 13.58 ng/ml

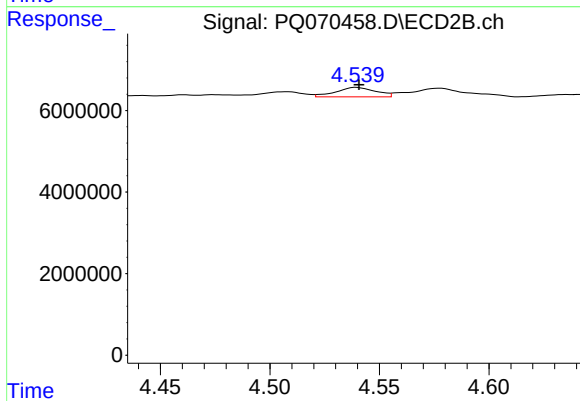

#20 AR-1242-5


R.T.: 4.540 min
Delta R.T.: -0.001 min
Response: 2900811
Conc: 15.90 ng/ml

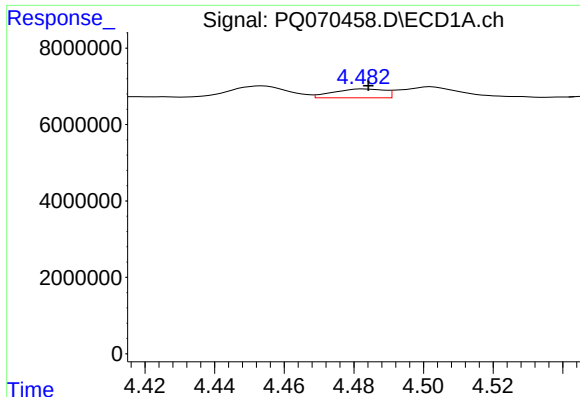

#21 AR-1248-1


R.T.: 4.483 min
Delta R.T.: -0.001 min
Response: 2383073
Conc: 19.24 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

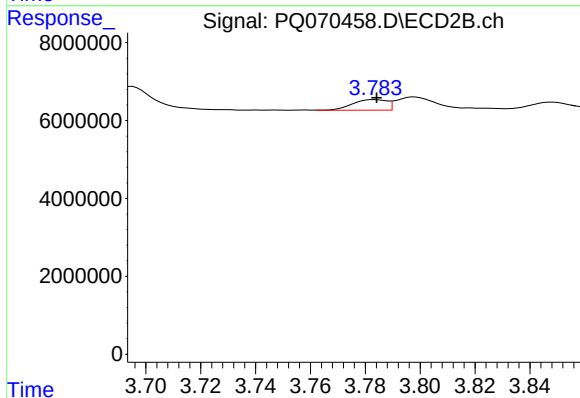


#21 AR-1248-1

R.T.: 3.783 min
Delta R.T.: 0.000 min
Response: 2349265
Conc: 16.71 ng/ml

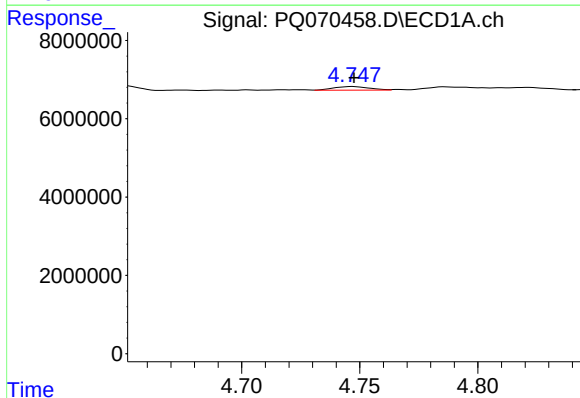


#22 AR-1248-2

R.T.: 4.747 min
Delta R.T.: 0.000 min
Response: 996530
Conc: 5.40 ng/ml

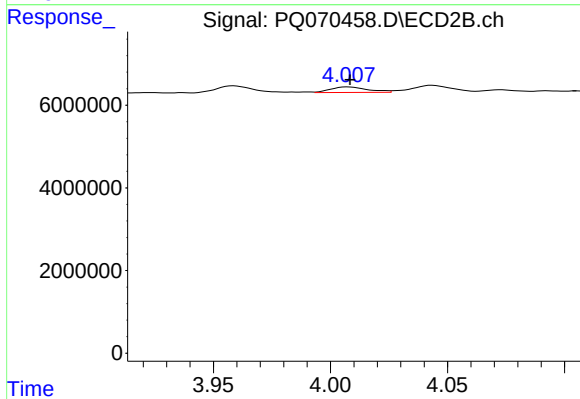

#22 AR-1248-2


R.T.: 4.007 min
Delta R.T.: -0.001 min
Response: 1472990
Conc: 6.31 ng/ml

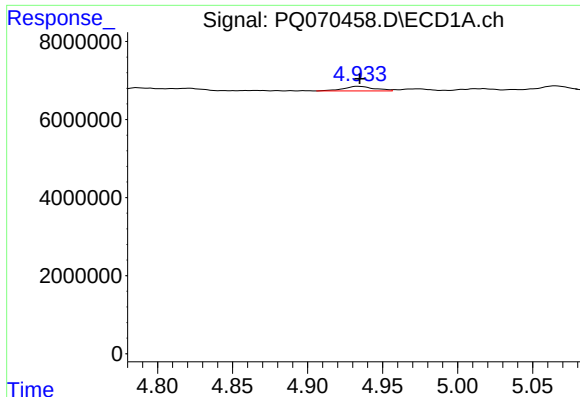

#23 AR-1248-3


R.T.: 4.934 min
Delta R.T.: 0.000 min
Response: 1630798
Conc: 7.38 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

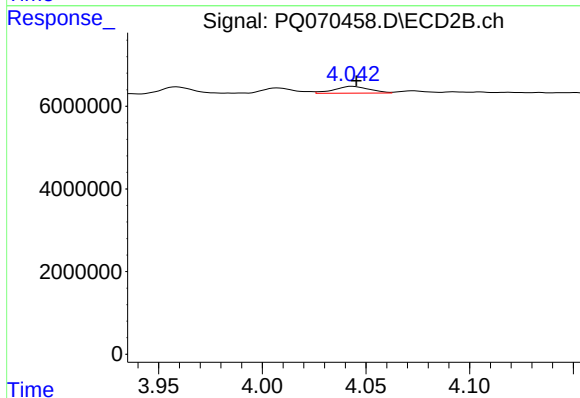


#23 AR-1248-3

R.T.: 4.043 min
Delta R.T.: -0.002 min
Response: 1940371
Conc: 8.62 ng/ml

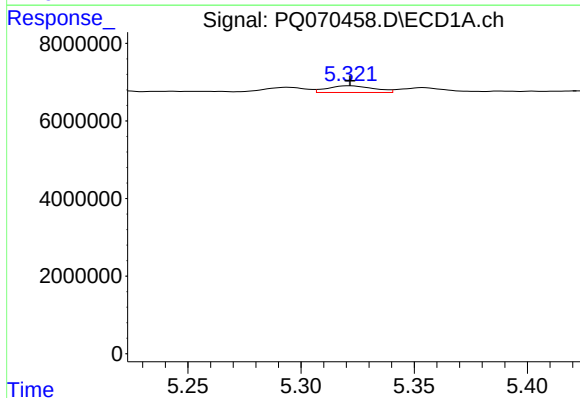


#24 AR-1248-4

R.T.: 5.321 min
Delta R.T.: 0.000 min
Response: 2469838
Conc: 11.13 ng/ml

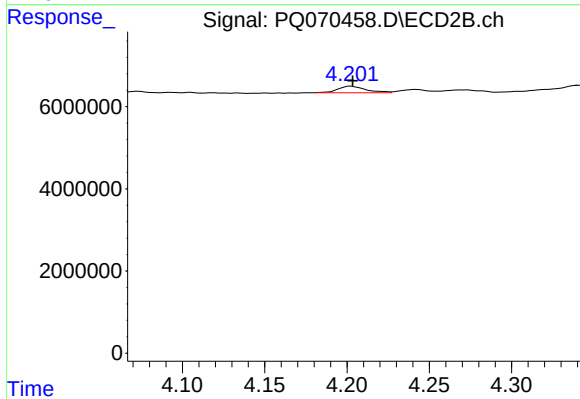

#24 AR-1248-4


R.T.: 4.202 min
Delta R.T.: -0.001 min
Response: 1877628
Conc: 6.89 ng/ml

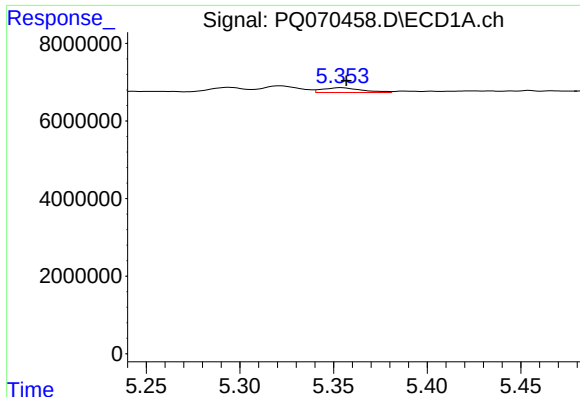

#25 AR-1248-5


R.T.: 5.354 min
Delta R.T.: -0.003 min
Response: 1826041
Conc: 7.90 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

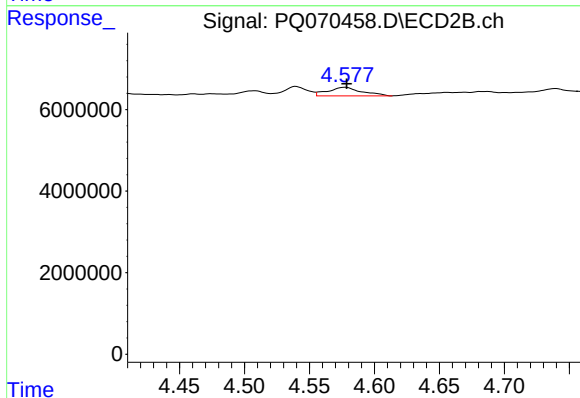


#25 AR-1248-5

R.T.: 4.578 min
Delta R.T.: 0.000 min
Response: 3782510
Conc: 15.10 ng/ml

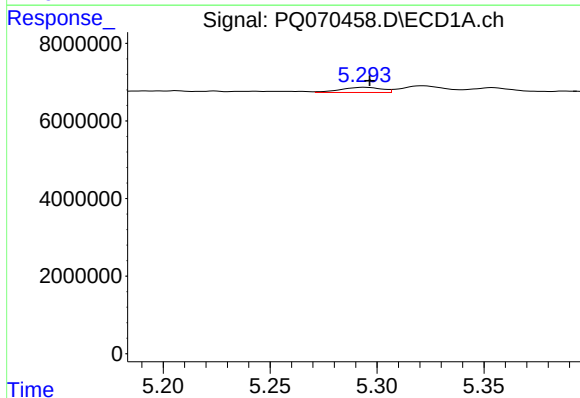


#26 AR-1254-1

R.T.: 5.294 min
Delta R.T.: -0.003 min
Response: 1800160
Conc: 7.28 ng/ml

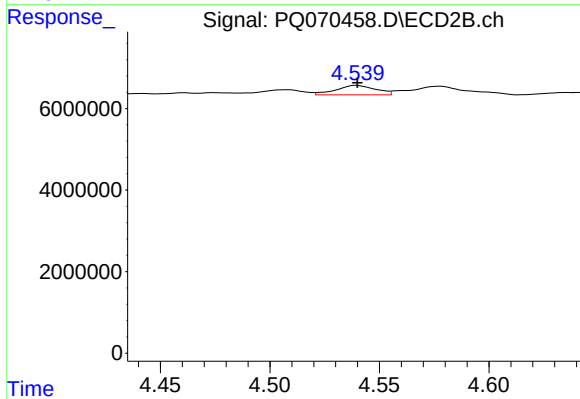

#26 AR-1254-1


R.T.: 4.540 min
Delta R.T.: 0.000 min
Response: 2900811
Conc: 7.16 ng/ml

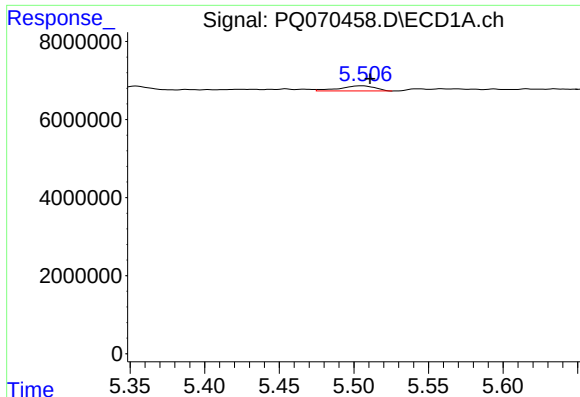

#27 AR-1254-2


R.T.: 5.506 min
Delta R.T.: -0.005 min
Response: 2203701
Conc: 5.87 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

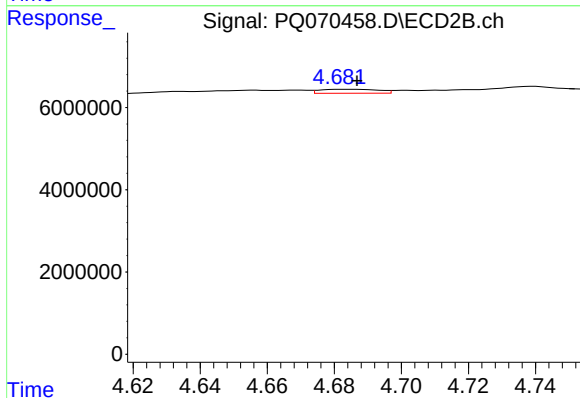


#27 AR-1254-2

R.T.: 4.682 min
Delta R.T.: -0.005 min
Response: 1179341
Conc: 3.27 ng/ml

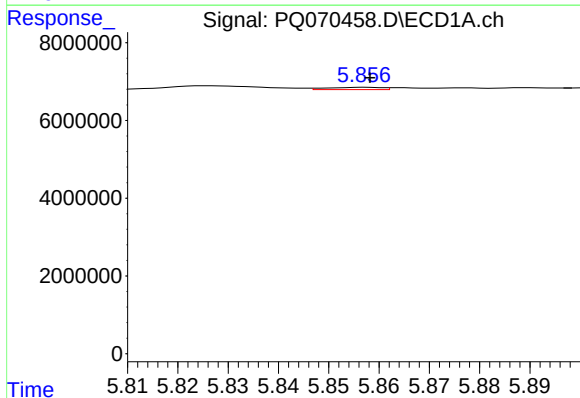


#28 AR-1254-3

R.T.: 5.857 min
Delta R.T.: -0.001 min
Response: 454882
Conc: 1.17 ng/ml

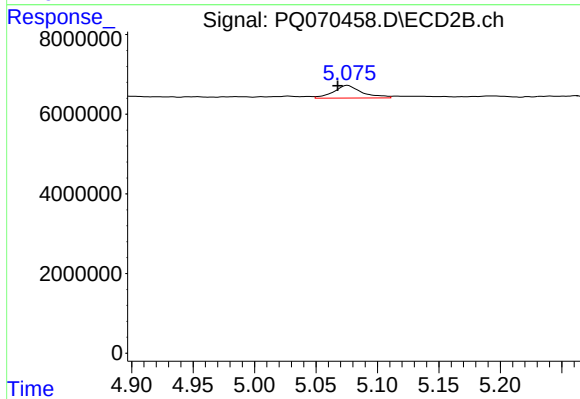

#28 AR-1254-3


R.T.: 5.076 min
Delta R.T.: 0.008 min
Response: 5150207
Conc: 9.11 ng/ml

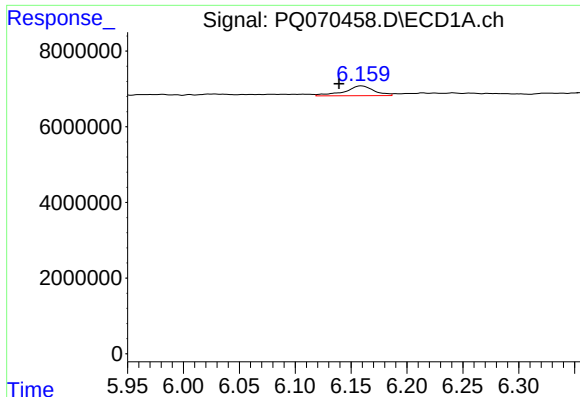

#29 AR-1254-4


R.T.: 6.159 min
Delta R.T.: 0.020 min
Response: 4768244
Conc: 19.15 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

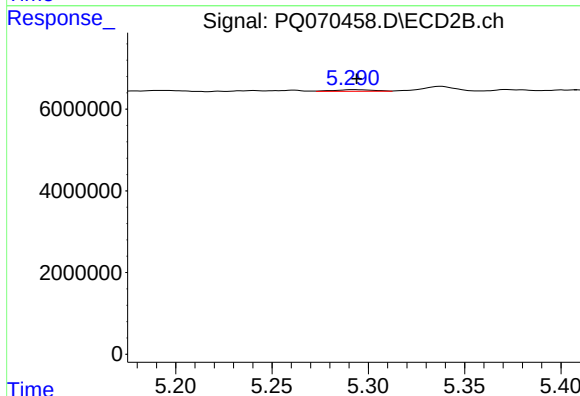


#29 AR-1254-4

R.T.: 5.292 min
Delta R.T.: -0.002 min
Response: 575467
Conc: 1.89 ng/ml

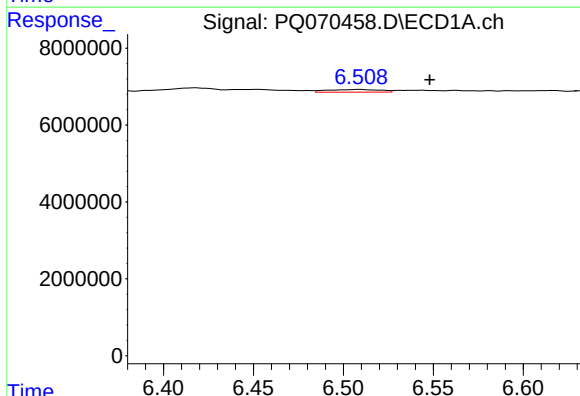


#30 AR-1254-5

R.T.: 6.509 min
Delta R.T.: -0.039 min
Response: 1414508
Conc: 4.76 ng/ml

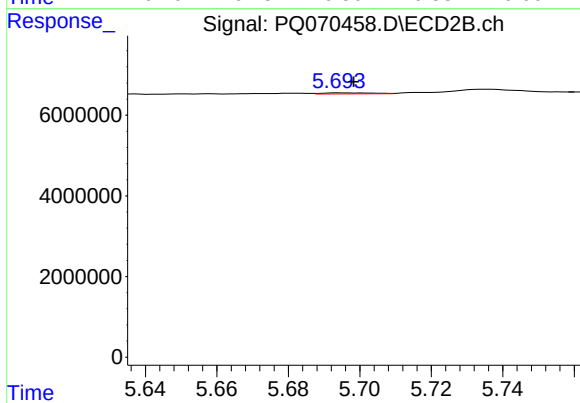

#30 AR-1254-5


R.T.: 5.694 min
Delta R.T.: -0.004 min
Response: 229514
Conc: 0.45 ng/ml

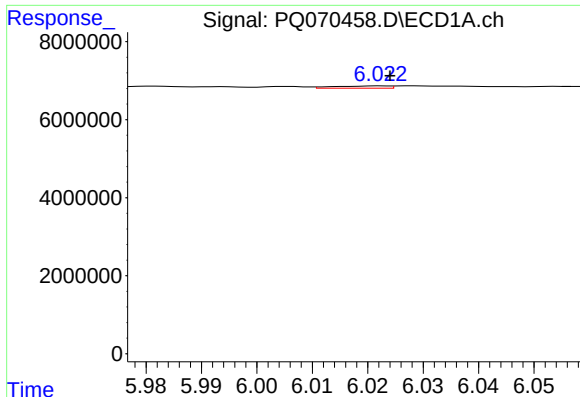

#31 AR-1260-1


R.T.: 6.022 min
Delta R.T.: -0.002 min
Response: 392087
Conc: 1.36 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

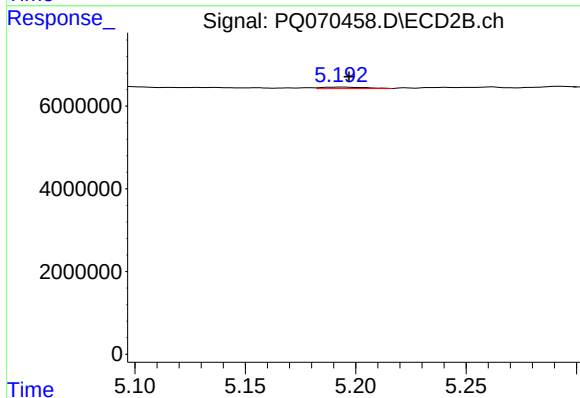


#31 AR-1260-1

R.T.: 5.193 min
Delta R.T.: -0.004 min
Response: 516385
Conc: 1.35 ng/ml

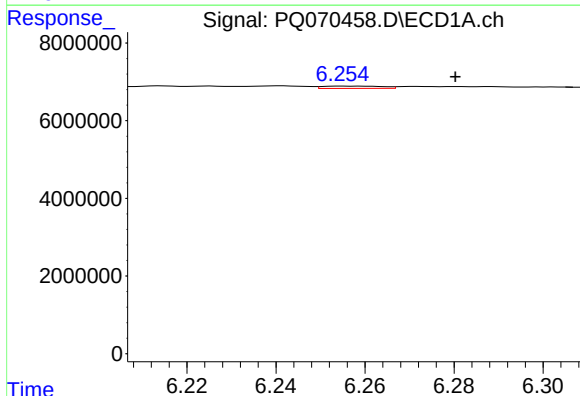


#32 AR-1260-2

R.T.: 6.255 min
Delta R.T.: -0.025 min
Response: 553871
Conc: 1.74 ng/ml

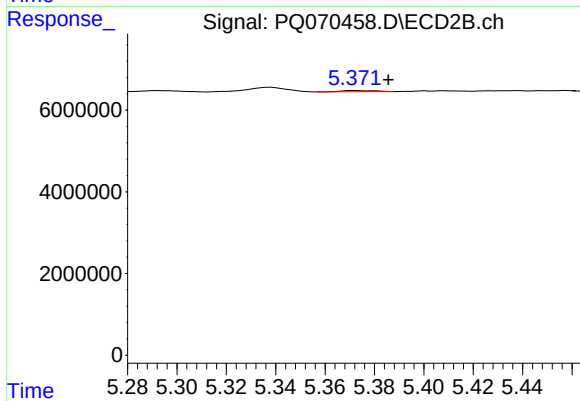

#32 AR-1260-2


R.T.: 5.371 min
Delta R.T.: -0.014 min
Response: 274457
Conc: 0.63 ng/ml

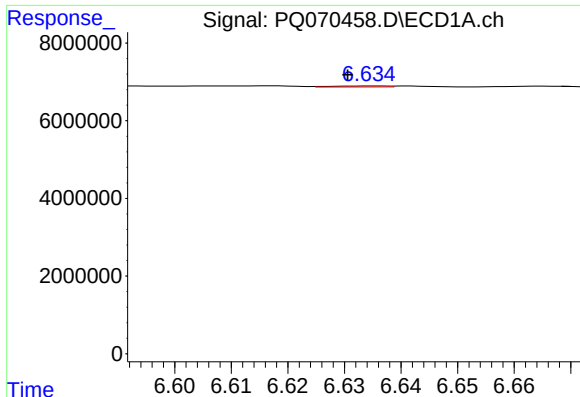

#33 AR-1260-3


R.T.: 6.635 min
Delta R.T.: 0.004 min
Response: 178589
Conc: 0.69 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

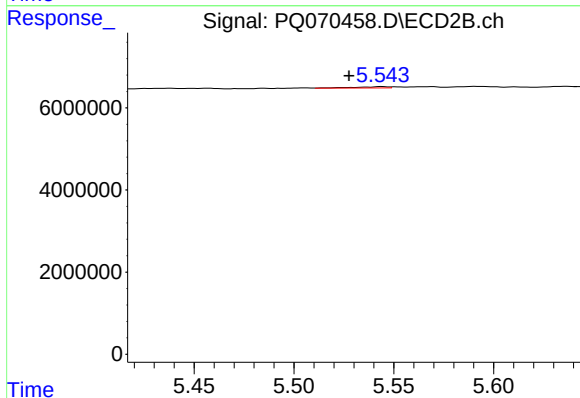


#33 AR-1260-3

R.T.: 5.544 min
Delta R.T.: 0.016 min
Response: 347111
Conc: 0.80 ng/ml

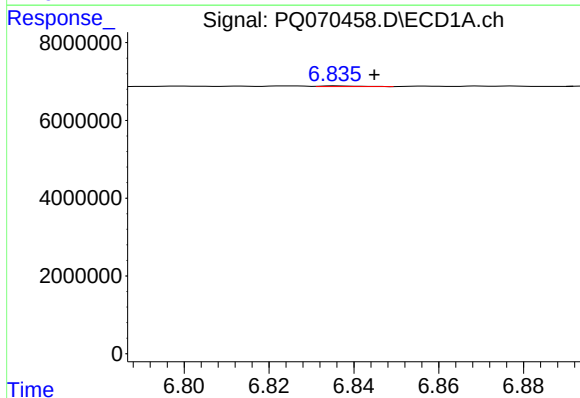


#34 AR-1260-4

R.T.: 6.835 min
Delta R.T.: -0.009 min
Response: 96013
Conc: 0.35 ng/ml

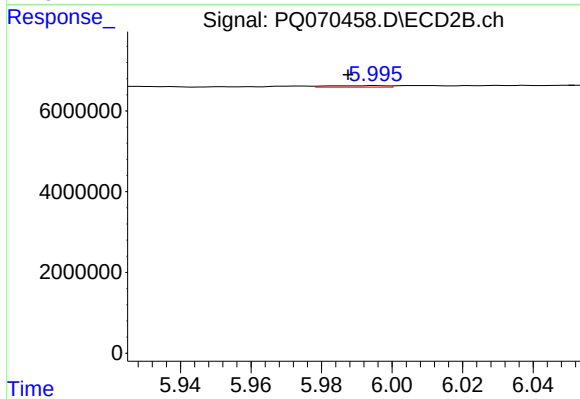

#34 AR-1260-4


R.T.: 5.995 min
Delta R.T.: 0.008 min
Response: 414554
Conc: 1.13 ng/ml

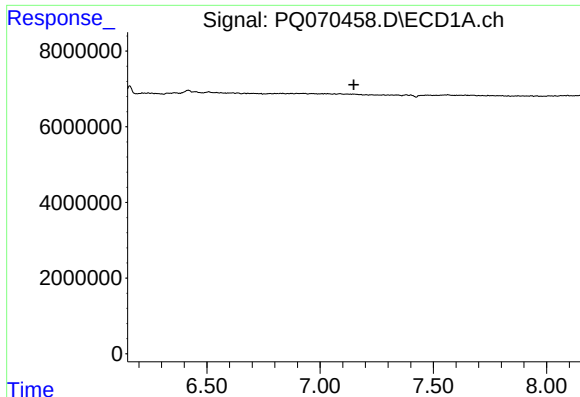

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 7.149 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

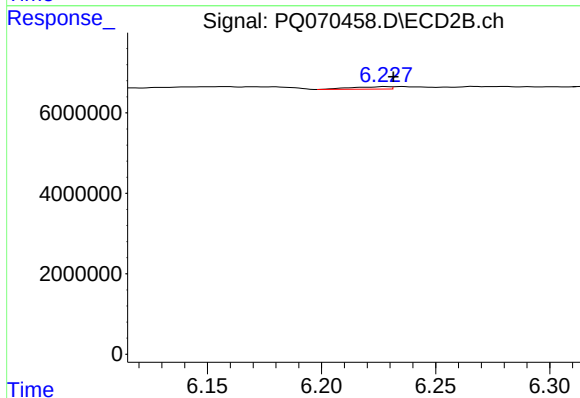


#35 AR-1260-5

R.T.: 6.228 min
Delta R.T.: -0.004 min
Response: 700051
Conc: 0.84 ng/ml

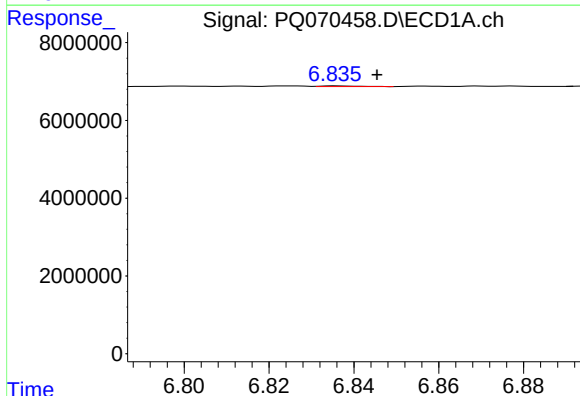


#36 AR-1262-1

R.T.: 6.835 min
Delta R.T.: -0.010 min
Response: 96013
Conc: 0.27 ng/ml

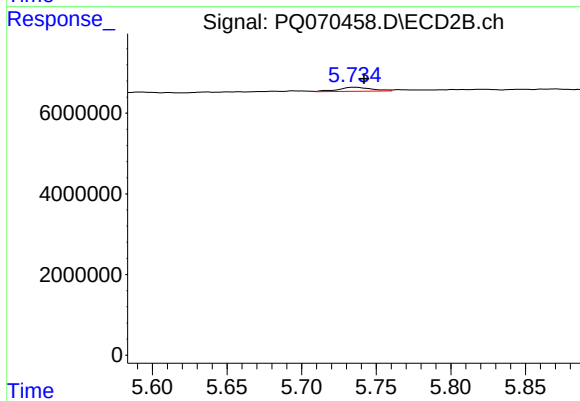

#36 AR-1262-1


R.T.: 5.735 min
Delta R.T.: -0.007 min
Response: 1564435
Conc: 2.86 ng/ml

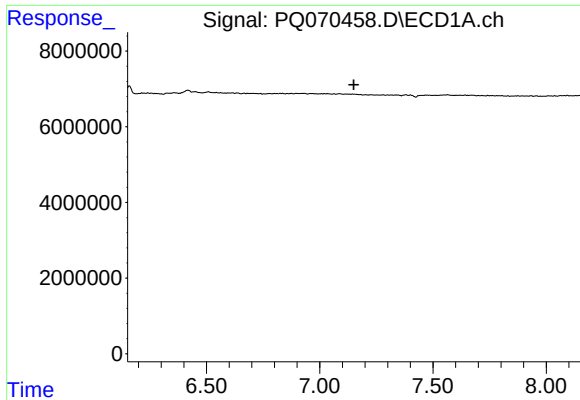

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 7.151 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

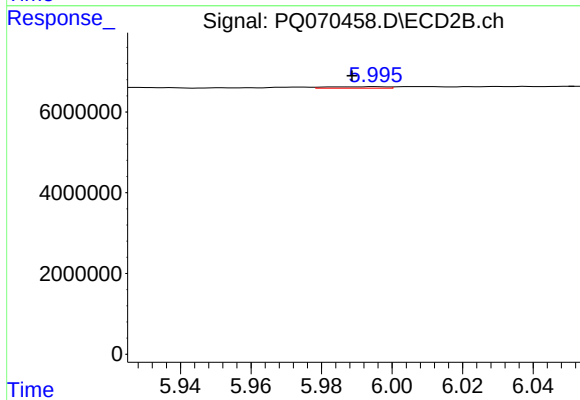


#37 AR-1262-2

R.T.: 5.995 min
Delta R.T.: 0.007 min
Response: 414554
Conc: 0.82 ng/ml

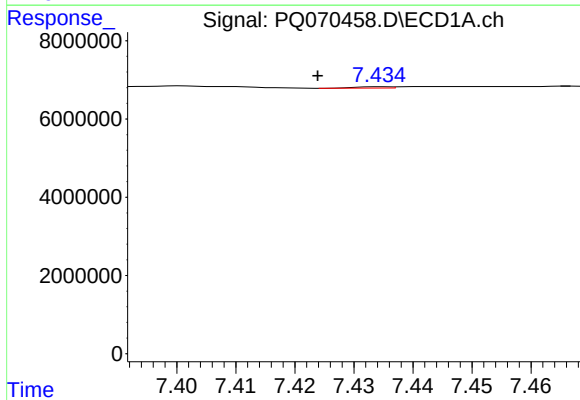


#38 AR-1262-3

R.T.: 7.435 min
Delta R.T.: 0.011 min
Response: 135996
Conc: 0.35 ng/ml

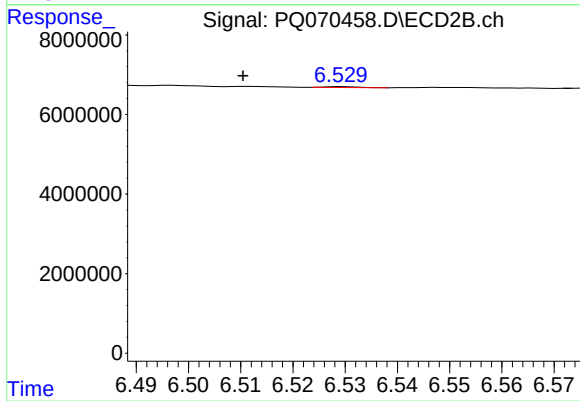

#38 AR-1262-3


R.T.: 6.529 min
Delta R.T.: 0.019 min
Response: 97121
Conc: 0.25 ng/ml

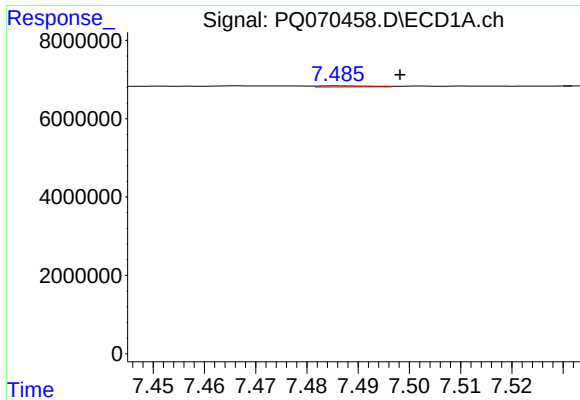

#39 AR-1262-4


R.T.: 7.486 min
Delta R.T.: -0.012 min
Response: 191502
Conc: 0.60 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

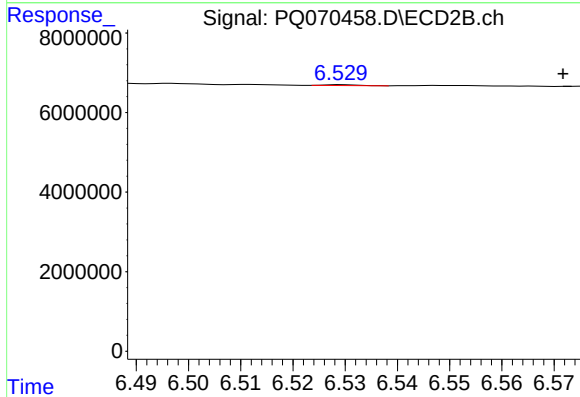


#39 AR-1262-4

R.T.: 6.529 min
Delta R.T.: -0.042 min
Response: 97121
Conc: 0.14 ng/ml

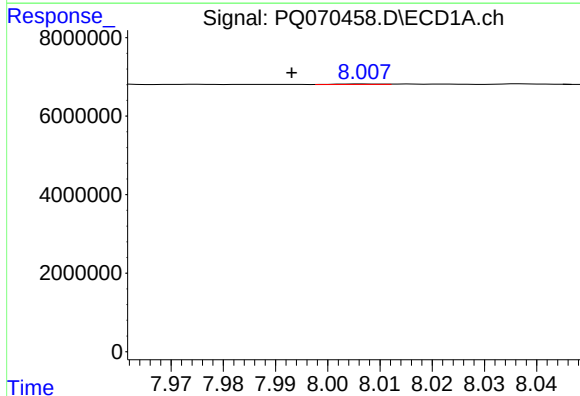


#40 AR-1262-5

R.T.: 8.007 min
Delta R.T.: 0.014 min
Response: 84193
Conc: 0.45 ng/ml

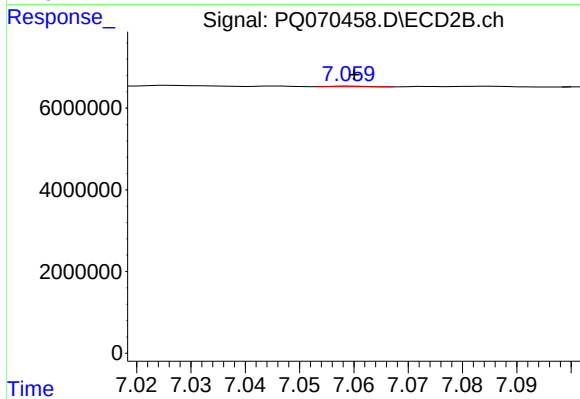

#40 AR-1262-5


R.T.: 7.059 min
Delta R.T.: 0.000 min
Response: 63654
Conc: 0.20 ng/ml

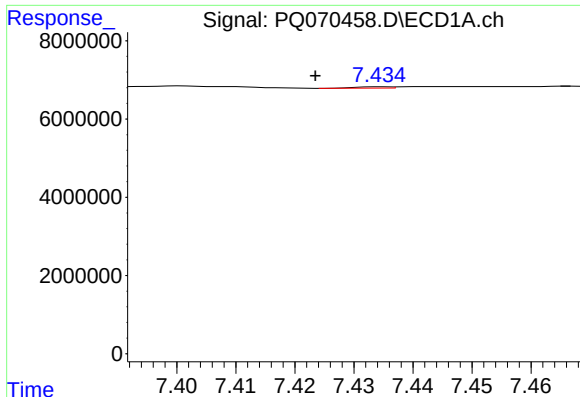

#41 AR-1268-1


R.T.: 7.435 min
Delta R.T.: 0.011 min
Response: 135996
Conc: 0.19 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

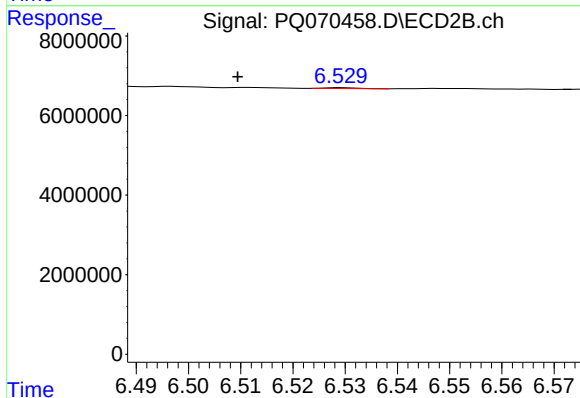


#41 AR-1268-1

R.T.: 6.529 min
Delta R.T.: 0.020 min
Response: 97121
Conc: 0.08 ng/ml

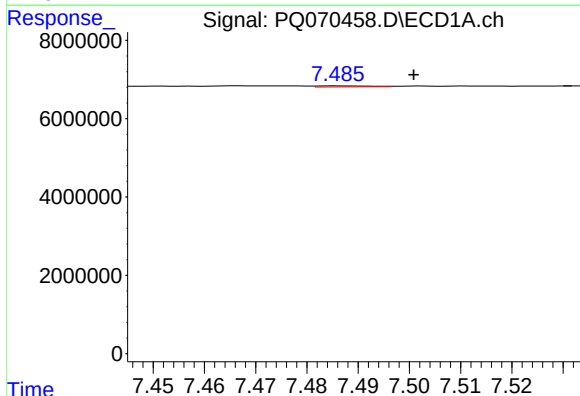


#42 AR-1268-2

R.T.: 7.486 min
Delta R.T.: -0.015 min
Response: 191502
Conc: 0.29 ng/ml

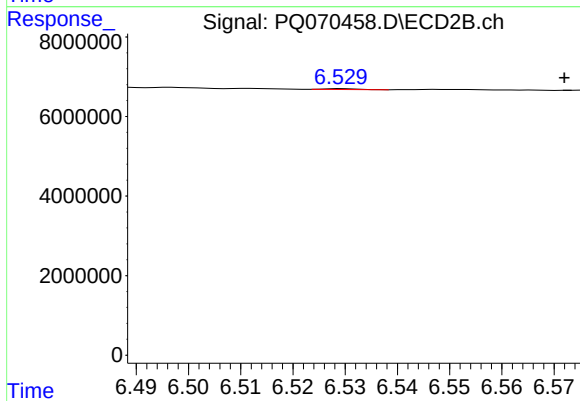

#42 AR-1268-2


R.T.: 6.529 min
Delta R.T.: -0.043 min
Response: 97121
Conc: 0.09 ng/ml

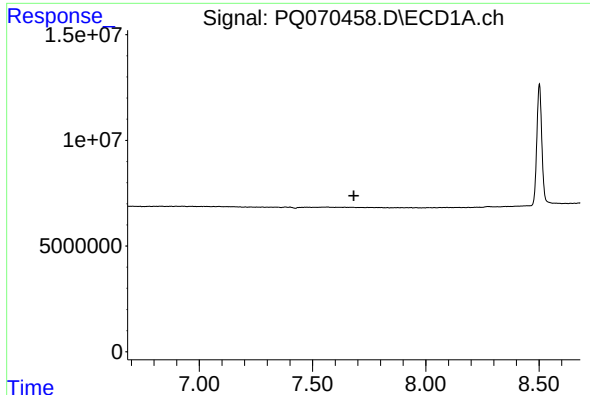

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 7.682 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

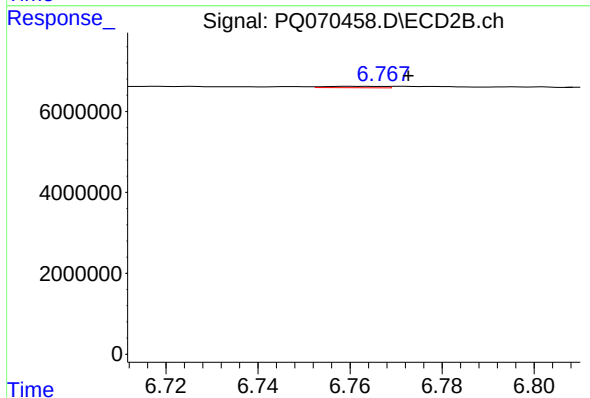


#43 AR-1268-3

R.T.: 6.760 min
Delta R.T.: -0.013 min
Response: 308093
Conc: 0.32 ng/ml

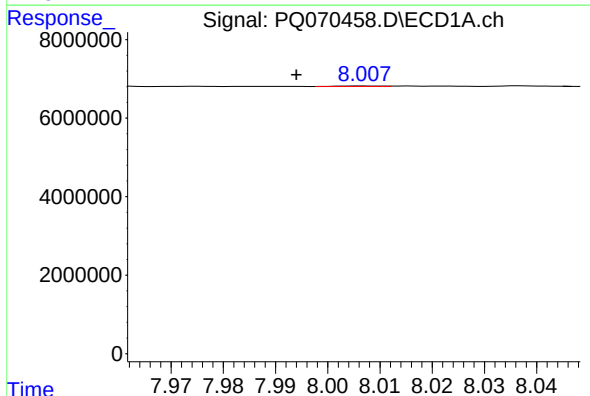


#44 AR-1268-4

R.T.: 8.007 min
Delta R.T.: 0.013 min
Response: 84193
Conc: 0.41 ng/ml

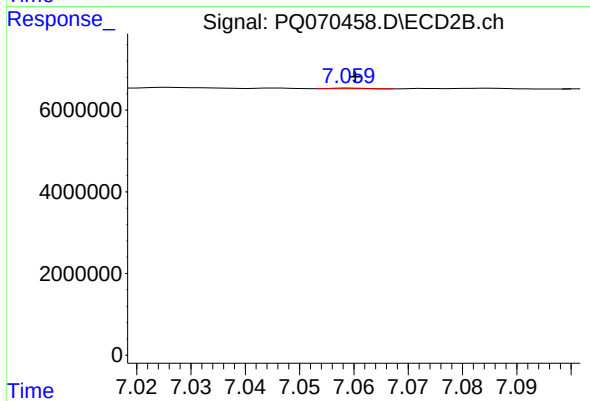

#44 AR-1268-4


R.T.: 7.059 min
Delta R.T.: -0.001 min
Response: 63654
Conc: 0.17 ng/ml

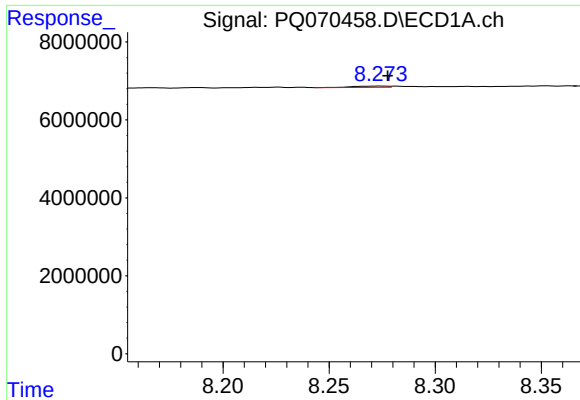

#45 AR-1268-5

R.T.: 8.274 min
Delta R.T.: -0.004 min
Response: 396898
Conc: 0.25 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

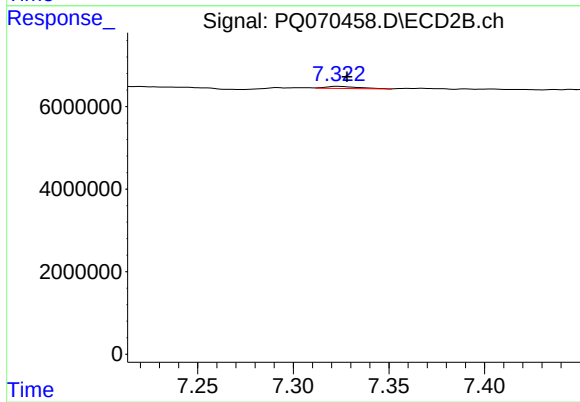

#45 AR-1268-5

R.T.: 7.323 min
Delta R.T.: -0.005 min
Response: 613549
Conc: 0.23 ng/ml