

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ062525\
 Data File : PQ070462.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jun 2025 11:51
 Operator : YP\AJ
 Sample : Q2126-09
 Misc : AR1262 MDL 25 PPB
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 MDL-WATER-03-QT2-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 04:57:18 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ062425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jun 26 02:49:53 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.404	2.782	111.3E6	126.7E6	18.180	18.761
2)	SA Decachlor...	8.502	7.542	88881082	155.4E6	21.591	21.430
Target Compounds							
3)	L1 AR-1016-1	4.479	3.786	383109	627817	2.041	3.023 #
4)	L1 AR-1016-2	4.500	3.802	188193	194367	0.608	0.575
5)	L1 AR-1016-3	4.578	3.965	199372	429940	0.991	2.291 #
6)	L1 AR-1016-4	4.644	4.008	173305	486696	1.095	2.774 #
7)	L1 AR-1016-5	4.936	4.207	170903	99807	1.051	0.494 #
8)	L2 AR-1221-1	3.574	2.992	90523	182726	1.056	1.787 #
9)	L2 AR-1221-2	3.676	3.050	1704659	2183800	26.375	27.685
10)	L2 AR-1221-3	3.740	3.124	176479	483185	0.910	2.132 #
11)	L3 AR-1232-1	3.740	3.124	176479	483185	1.247	2.899 #
12)	L3 AR-1232-2	4.230	3.802	349022	194367	4.307	1.218 #
13)	L3 AR-1232-3	4.500	3.965	188193	429940	1.319	4.892 #
14)	L3 AR-1232-4	4.644	4.047	173305	112216	2.410	1.455 #
15)	L3 AR-1232-5	4.788	4.207	251399	99807	4.207	1.192 #
16)	L4 AR-1242-1	4.479	3.786	383109	627817	2.476	3.579 #
17)	L4 AR-1242-2	4.500	3.802	188193	194367	0.716	0.698
18)	L4 AR-1242-3	4.578	3.965	199372	429940	1.174	2.736 #
19)	L4 AR-1242-4	4.644	4.047	173305	112216	1.284	0.737 #
20)	L4 AR-1242-5	5.383f	4.538	528729	2618812	3.931	14.352 #
21)	L5 AR-1248-1	4.479	3.786	383109	627817	3.093	4.467 #
22)	L5 AR-1248-2	4.749	4.008	299634	486696	1.624	2.085 #
23)	L5 AR-1248-3	4.936	4.047	170903	112216	0.774	0.498 #
24)	L5 AR-1248-4	5.328	4.207	1933905	99807	8.714	0.366 #
25)	L5 AR-1248-5	5.383f	4.577	528729	521806	2.288	2.084
26)	L6 AR-1254-1	5.297	4.538	1721599	2618812	6.959	6.464
27)	L6 AR-1254-2	5.510	4.685	1623859	2977742	4.323	8.246 #
28)	L6 AR-1254-3	5.861	5.083	634145	10439474	1.633	18.459 #
29)	L6 AR-1254-4	6.131	5.291	389213	432737	1.564	1.419
30)	L6 AR-1254-5	6.545	5.695	6076326	6205187	20.455	12.057 #
31)	L7 AR-1260-1	6.024	5.195	6388561	7640743	22.109	20.002
32)	L7 AR-1260-2	6.280	5.384	6689649	8799727	20.985	20.086
33)	L7 AR-1260-3	6.631	5.527	8464291	8689575	32.595	20.140 #
34)	L7 AR-1260-4	6.845	5.986	7924988	13021993	29.086	35.485
35)	L7 AR-1260-5	7.150	6.231	14331245	22521505	28.766	27.096
36)	L8 AR-1262-1	6.845	5.739	7924988	15277404	22.506	27.920
37)	L8 AR-1262-2	7.150	5.986	14331245	13021993	25.300	25.606
38)	L8 AR-1262-3	7.423	6.508	8086064	9654095	20.757	24.590
39)	L8 AR-1262-4	7.494	6.568	6749188	17882885	21.093	25.527
40)	L8 AR-1262-5	7.992	7.058	4221664	7601563	22.535	23.971
41)	L9 AR-1268-1	7.423	6.508	8086064	9654095	11.221	8.330 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ062525\
 Data File : PQ070462.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jun 2025 11:51
 Operator : YP\AJ
 Sample : Q2126-09
 Misc : AR1262 MDL 25 PPB
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 MDL-WATER-03-QT2-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 04:57:18 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ062425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jun 26 02:49:53 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	7.494	6.568	6749188	17882885	10.161	16.678 #
43) L9	AR-1268-3	7.678	6.770	690872	2099031	1.218	2.199 #
44) L9	AR-1268-4	7.992	7.058	4221664	7601563	20.464	20.210
45) L9	AR-1268-5	8.276	7.325	2190816	3107480	1.368	1.182



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ062525\
Data File : PQ070462.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jun 2025 11:51
Operator : YP\AJ
Sample : Q2126-09
Misc : AR1262 MDL 25 PPB
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 04:57:18 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ062425.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 26 02:49:53 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

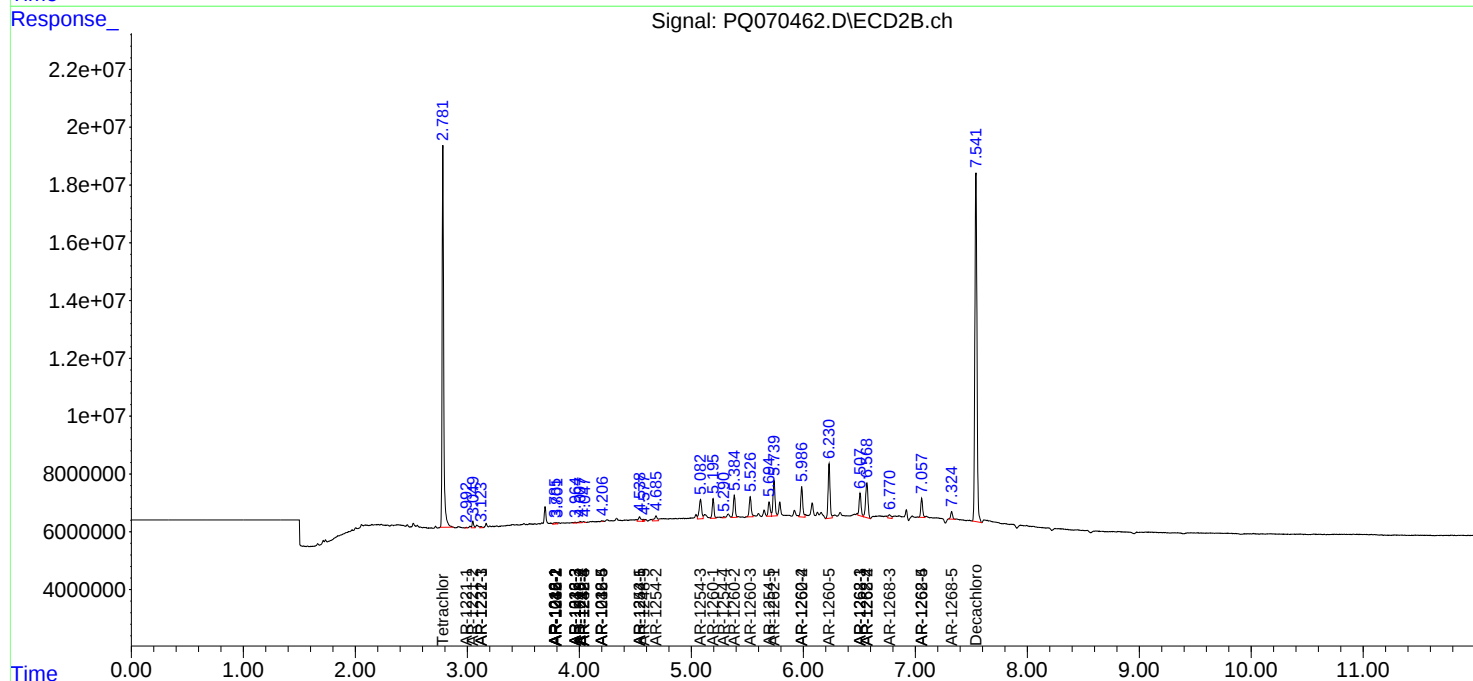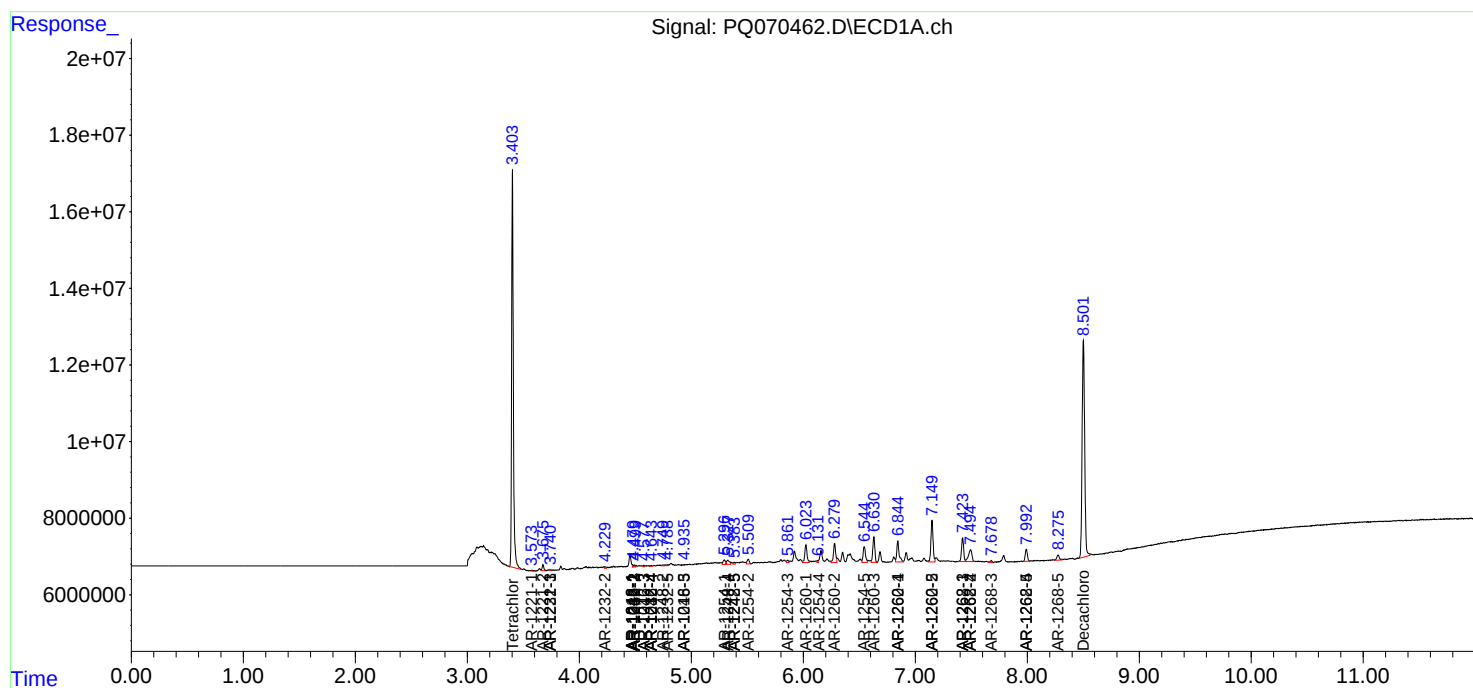


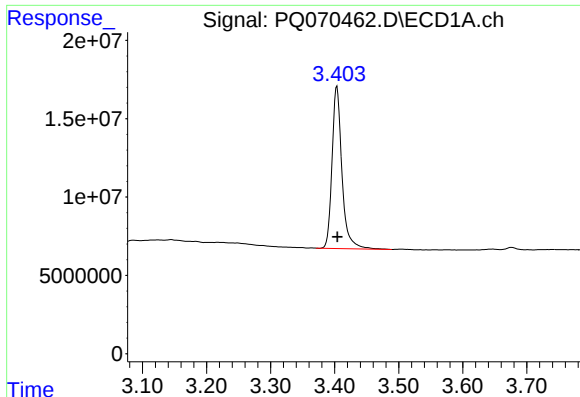

#1 Tetrachloro-m-xylene


R.T.: 3.404 min
Delta R.T.: 0.000 min
Response: 111293231
Conc: 18.18 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

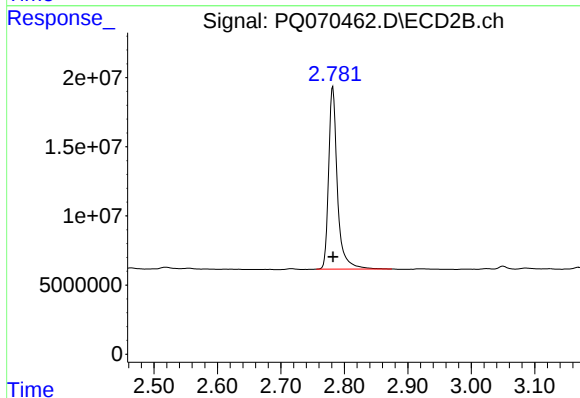


#1 Tetrachloro-m-xylene

R.T.: 2.782 min
Delta R.T.: 0.000 min
Response: 126696335
Conc: 18.76 ng/ml

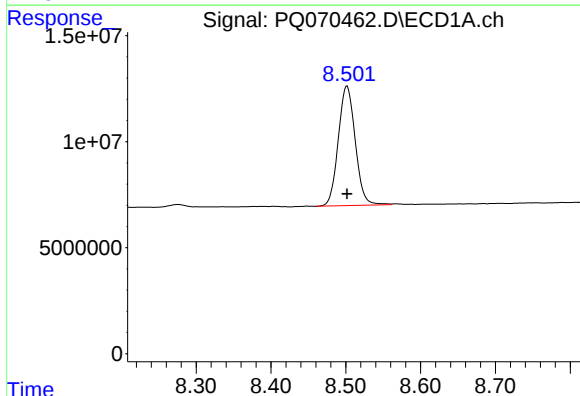


#2 Decachlorobiphenyl

R.T.: 8.502 min
Delta R.T.: 0.000 min
Response: 88881082
Conc: 21.59 ng/ml

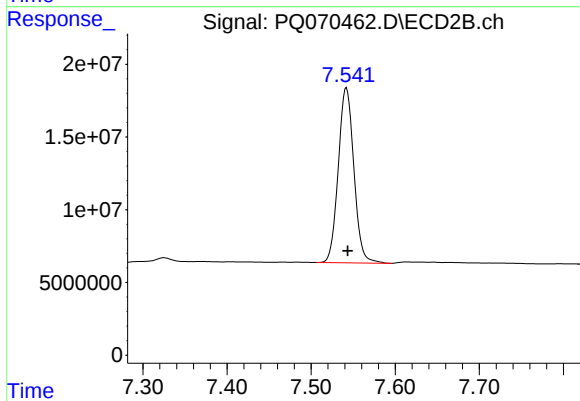

#2 Decachlorobiphenyl


R.T.: 7.542 min
Delta R.T.: -0.002 min
Response: 155354922
Conc: 21.43 ng/ml

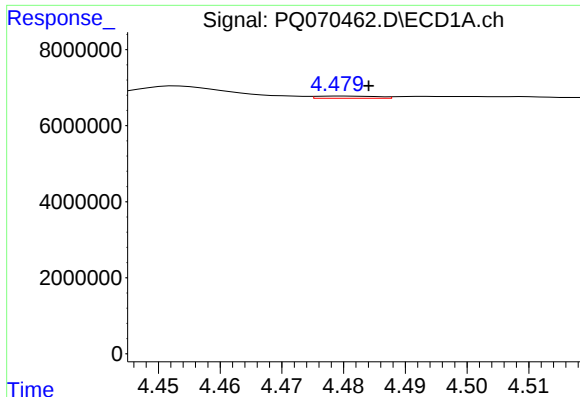

#3 AR-1016-1


R.T.: 4.479 min
Delta R.T.: -0.005 min
Response: 383109
Conc: 2.04 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

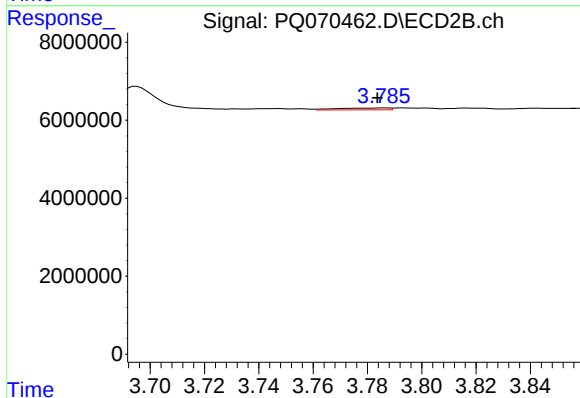


#3 AR-1016-1

R.T.: 3.786 min
Delta R.T.: 0.002 min
Response: 627817
Conc: 3.02 ng/ml

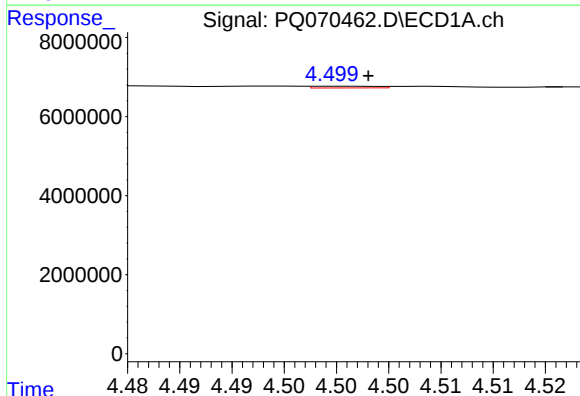


#4 AR-1016-2

R.T.: 4.500 min
Delta R.T.: -0.003 min
Response: 188193
Conc: 0.61 ng/ml

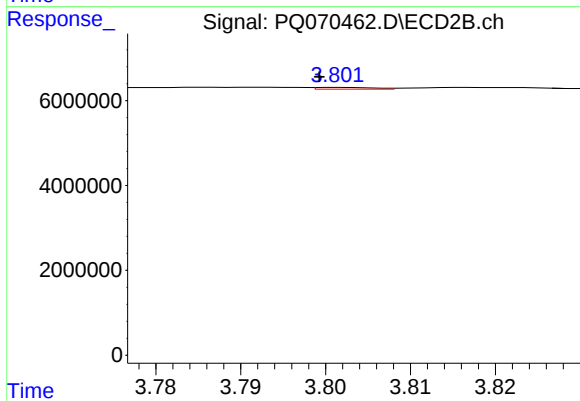

#4 AR-1016-2


R.T.: 3.802 min
Delta R.T.: 0.002 min
Response: 194367
Conc: 0.57 ng/ml

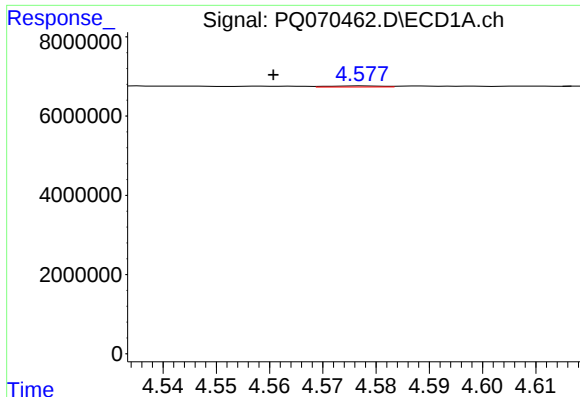

#5 AR-1016-3


R.T.: 4.578 min
Delta R.T.: 0.017 min
Response: 199372
Conc: 0.99 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

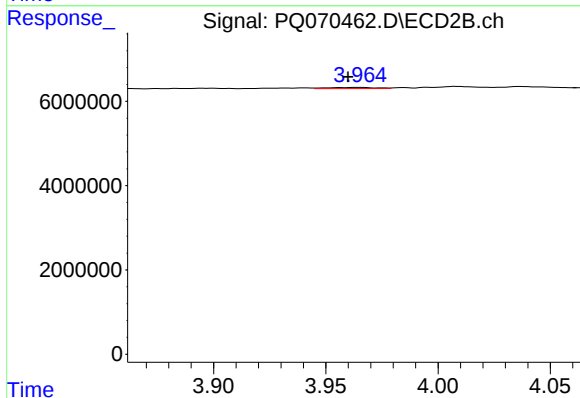


#5 AR-1016-3

R.T.: 3.965 min
Delta R.T.: 0.005 min
Response: 429940
Conc: 2.29 ng/ml

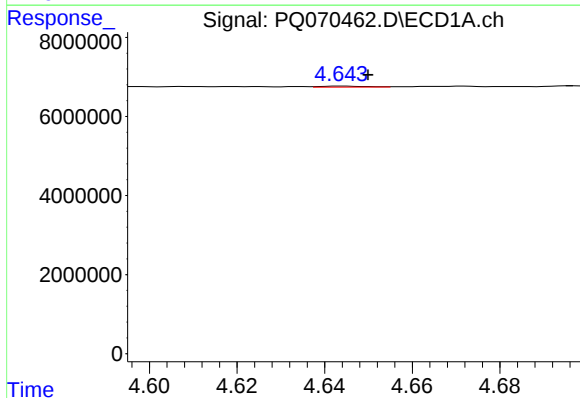


#6 AR-1016-4

R.T.: 4.644 min
Delta R.T.: -0.006 min
Response: 173305
Conc: 1.09 ng/ml

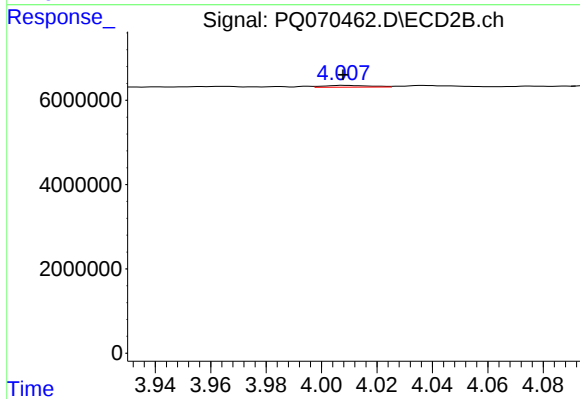

#6 AR-1016-4


R.T.: 4.008 min
Delta R.T.: 0.000 min
Response: 486696
Conc: 2.77 ng/ml

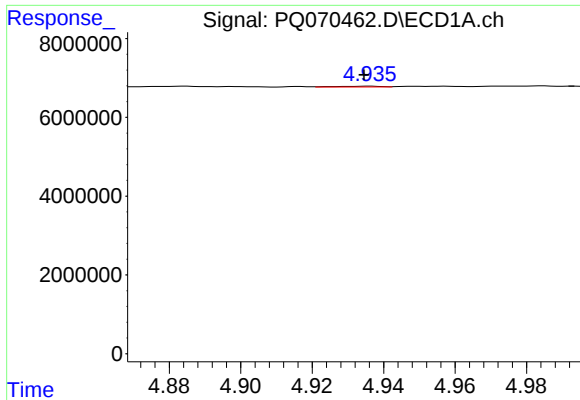

#7 AR-1016-5


R.T.: 4.936 min
Delta R.T.: 0.002 min
Response: 170903
Conc: 1.05 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

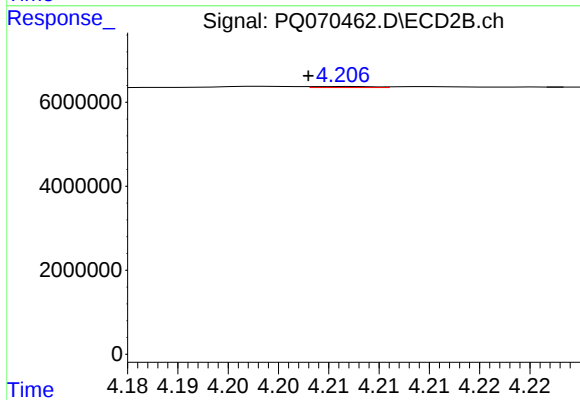


#7 AR-1016-5

R.T.: 4.207 min
Delta R.T.: 0.004 min
Response: 99807
Conc: 0.49 ng/ml

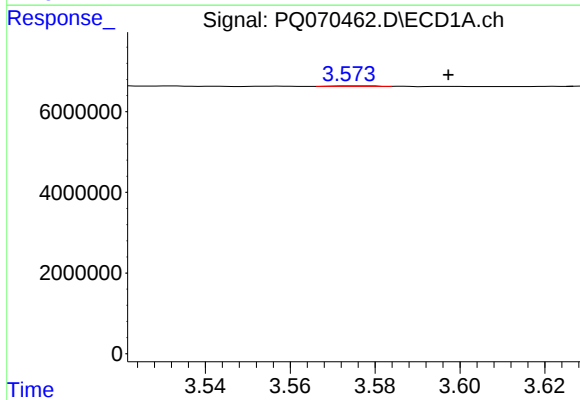


#8 AR-1221-1

R.T.: 3.574 min
Delta R.T.: -0.023 min
Response: 90523
Conc: 1.06 ng/ml

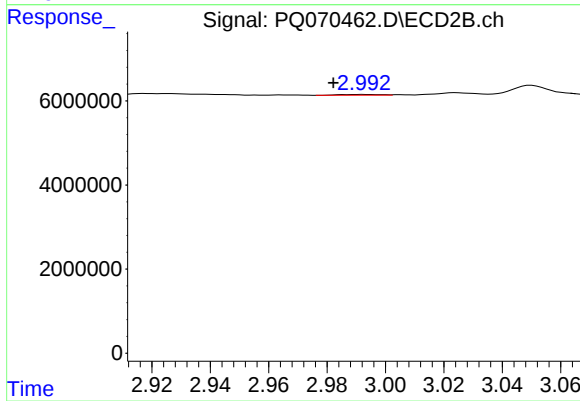

#8 AR-1221-1


R.T.: 2.992 min
Delta R.T.: 0.010 min
Response: 182726
Conc: 1.79 ng/ml

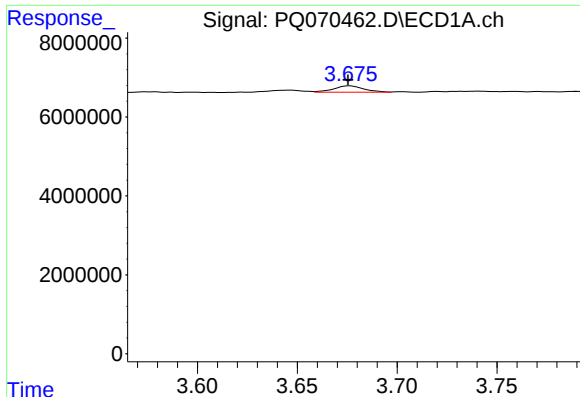

#9 AR-1221-2


R.T.: 3.676 min
Delta R.T.: 0.000 min
Response: 1704659
Conc: 26.38 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

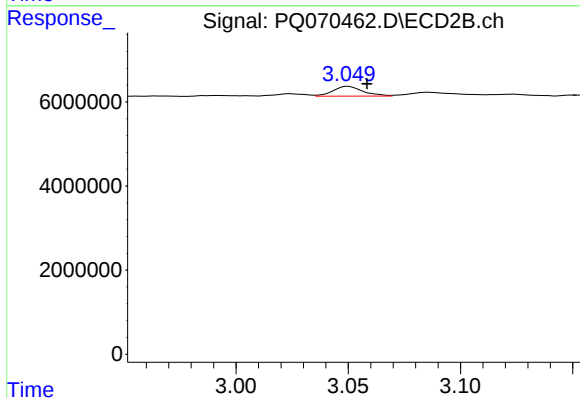


#9 AR-1221-2

R.T.: 3.050 min
Delta R.T.: -0.009 min
Response: 2183800
Conc: 27.68 ng/ml

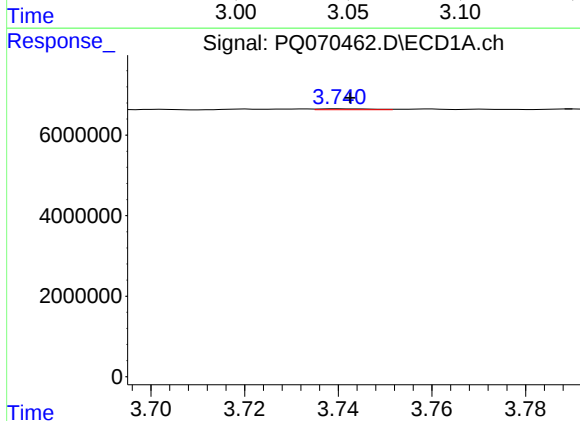


#10 AR-1221-3

R.T.: 3.740 min
Delta R.T.: -0.002 min
Response: 176479
Conc: 0.91 ng/ml

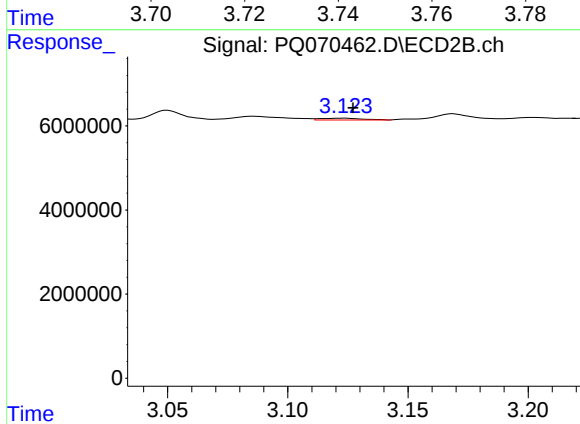

#10 AR-1221-3


R.T.: 3.124 min
Delta R.T.: -0.004 min
Response: 483185
Conc: 2.13 ng/ml

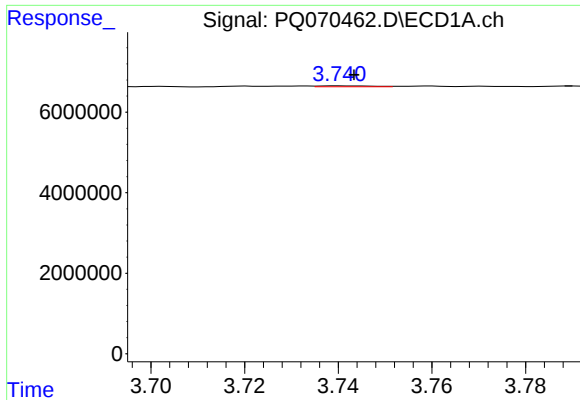

#11 AR-1232-1


R.T.: 3.740 min
Delta R.T.: -0.003 min
Response: 176479
Conc: 1.25 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

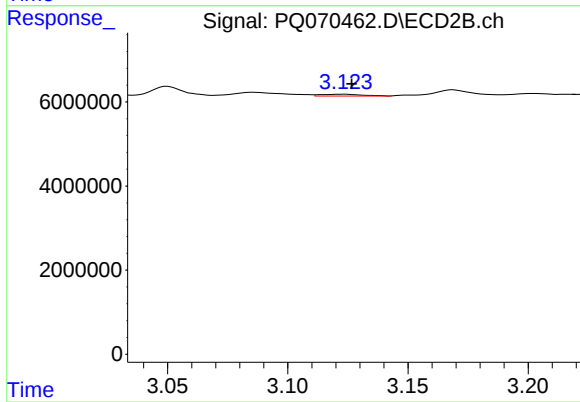


#11 AR-1232-1

R.T.: 3.124 min
Delta R.T.: -0.003 min
Response: 483185
Conc: 2.90 ng/ml

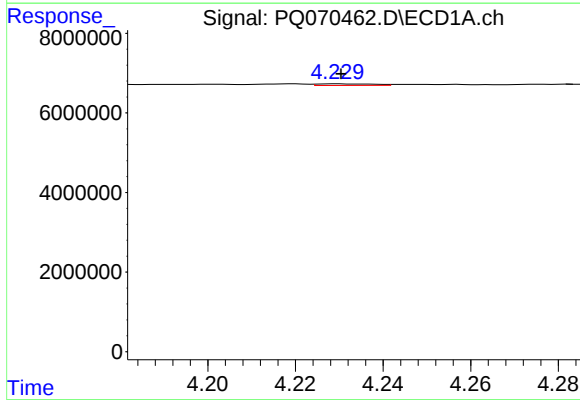


#12 AR-1232-2

R.T.: 4.230 min
Delta R.T.: 0.000 min
Response: 349022
Conc: 4.31 ng/ml

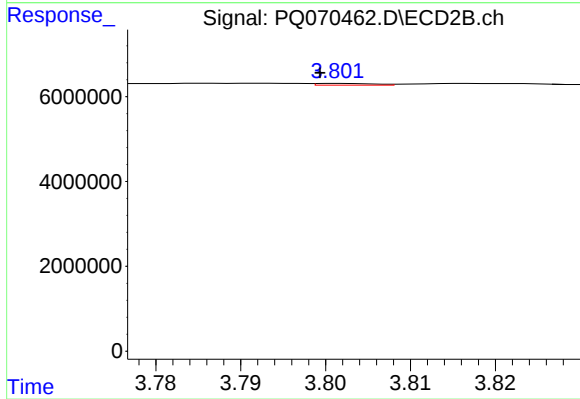

#12 AR-1232-2


R.T.: 3.802 min
Delta R.T.: 0.002 min
Response: 194367
Conc: 1.22 ng/ml

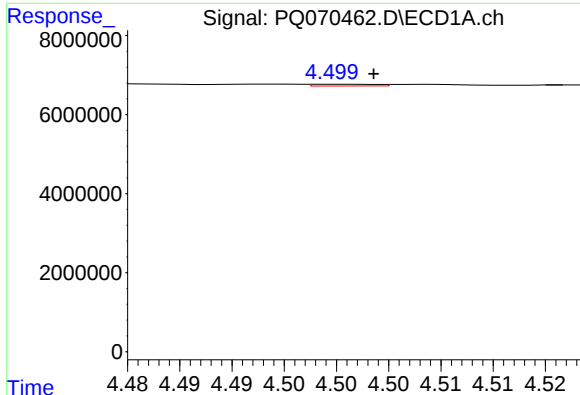

#13 AR-1232-3


R.T.: 4.500 min
Delta R.T.: -0.004 min
Response: 188193
Conc: 1.32 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

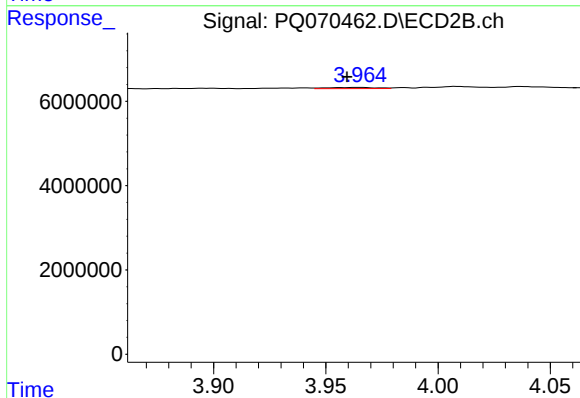


#13 AR-1232-3

R.T.: 3.965 min
Delta R.T.: 0.006 min
Response: 429940
Conc: 4.89 ng/ml

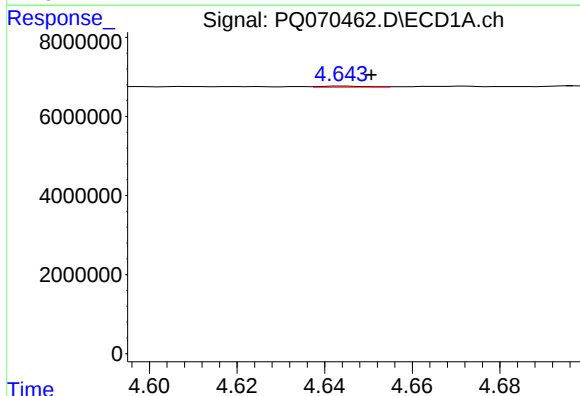


#14 AR-1232-4

R.T.: 4.644 min
Delta R.T.: -0.007 min
Response: 173305
Conc: 2.41 ng/ml

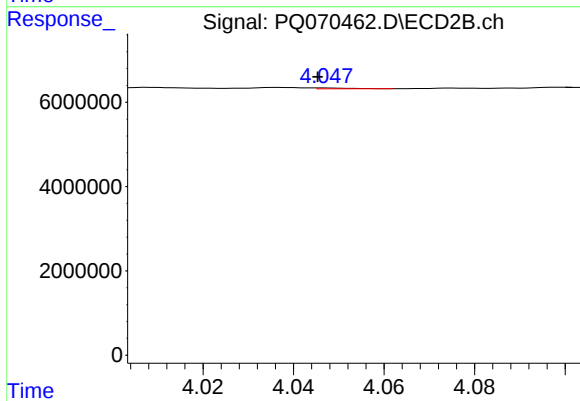

#14 AR-1232-4


R.T.: 4.047 min
Delta R.T.: 0.002 min
Response: 112216
Conc: 1.45 ng/ml

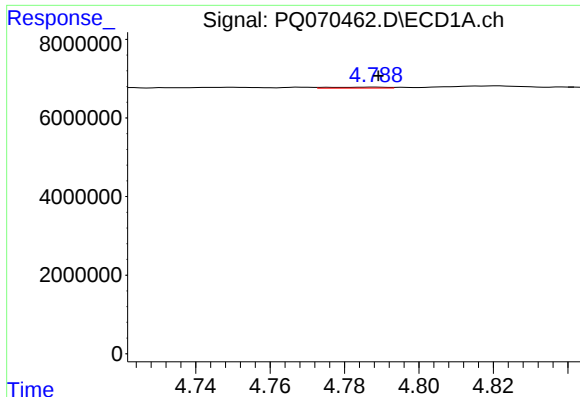

#15 AR-1232-5


R.T.: 4.788 min
Delta R.T.: 0.000 min
Response: 251399
Conc: 4.21 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

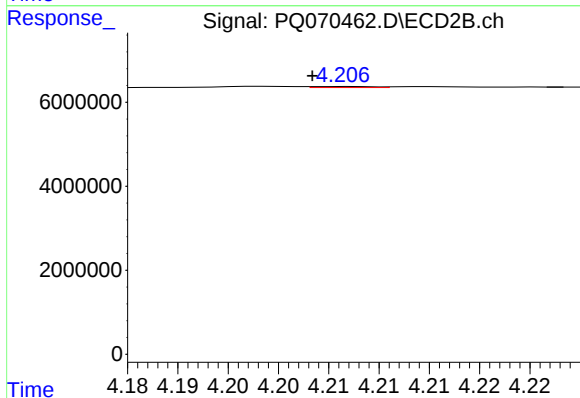


#15 AR-1232-5

R.T.: 4.207 min
Delta R.T.: 0.003 min
Response: 99807
Conc: 1.19 ng/ml

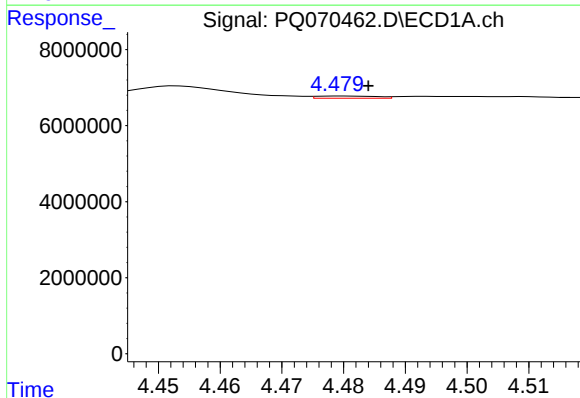


#16 AR-1242-1

R.T.: 4.479 min
Delta R.T.: -0.005 min
Response: 383109
Conc: 2.48 ng/ml

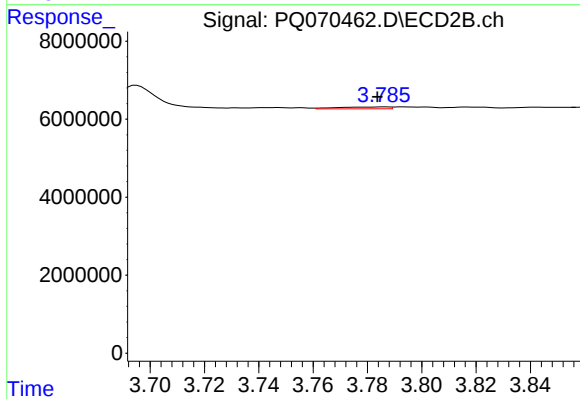

#16 AR-1242-1


R.T.: 3.786 min
Delta R.T.: 0.002 min
Response: 627817
Conc: 3.58 ng/ml

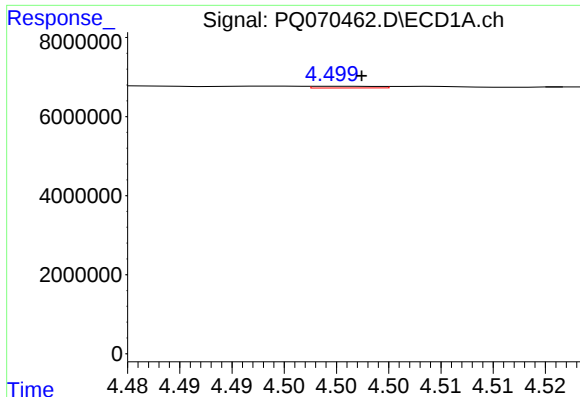

#17 AR-1242-2


R.T.: 4.500 min
Delta R.T.: -0.003 min
Response: 188193
Conc: 0.72 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

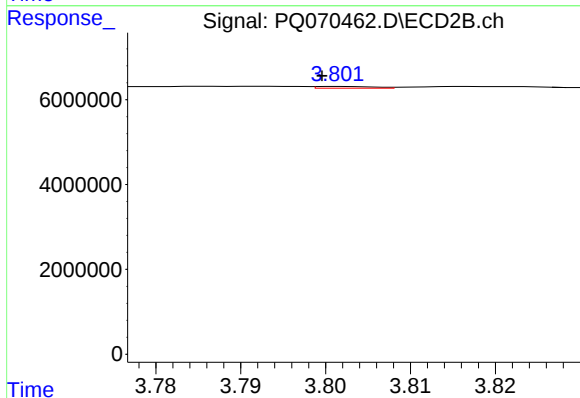


#17 AR-1242-2

R.T.: 3.802 min
Delta R.T.: 0.002 min
Response: 194367
Conc: 0.70 ng/ml

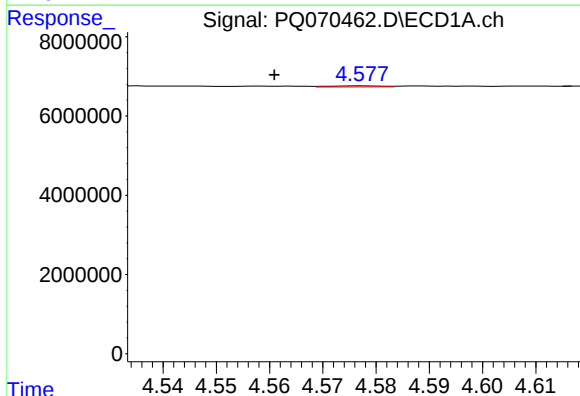


#18 AR-1242-3

R.T.: 4.578 min
Delta R.T.: 0.017 min
Response: 199372
Conc: 1.17 ng/ml

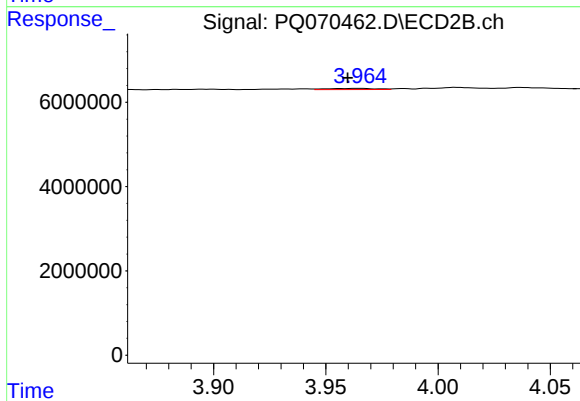

#18 AR-1242-3


R.T.: 3.965 min
Delta R.T.: 0.005 min
Response: 429940
Conc: 2.74 ng/ml

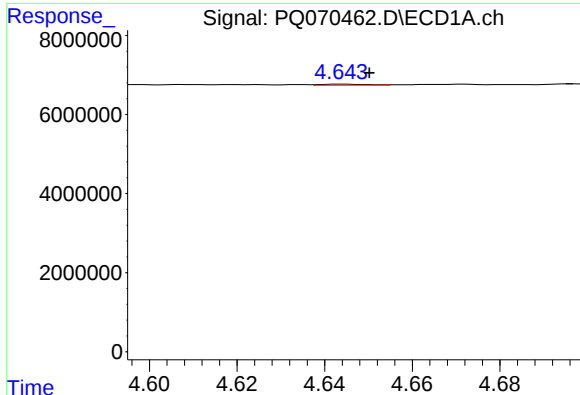

#19 AR-1242-4


R.T.: 4.644 min
Delta R.T.: -0.006 min
Response: 173305
Conc: 1.28 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

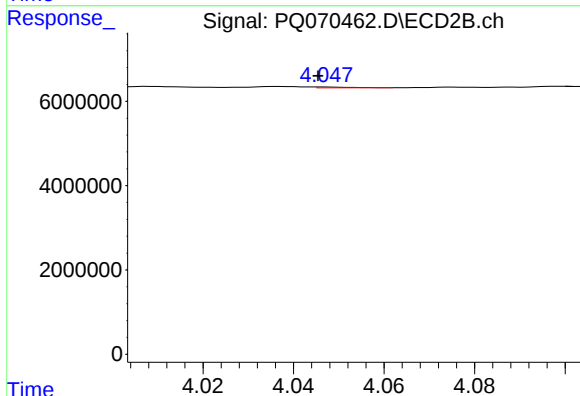


#19 AR-1242-4

R.T.: 4.047 min
Delta R.T.: 0.002 min
Response: 112216
Conc: 0.74 ng/ml

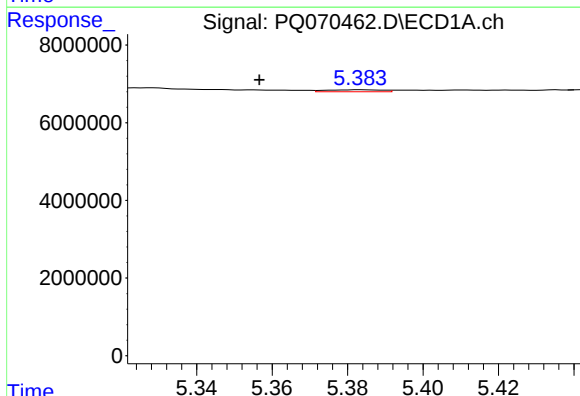


#20 AR-1242-5

R.T.: 5.383 min
Delta R.T.: 0.027 min
Response: 528729
Conc: 3.93 ng/ml

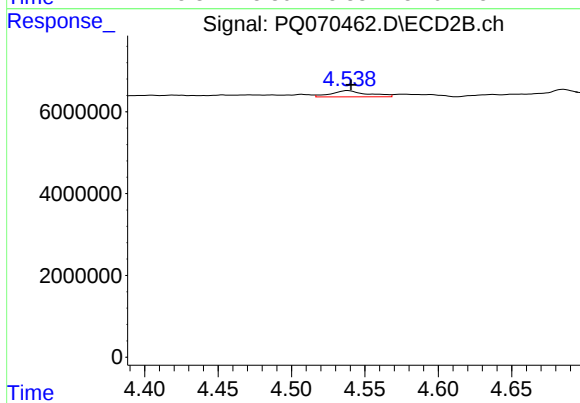

#20 AR-1242-5


R.T.: 4.538 min
Delta R.T.: -0.002 min
Response: 2618812
Conc: 14.35 ng/ml

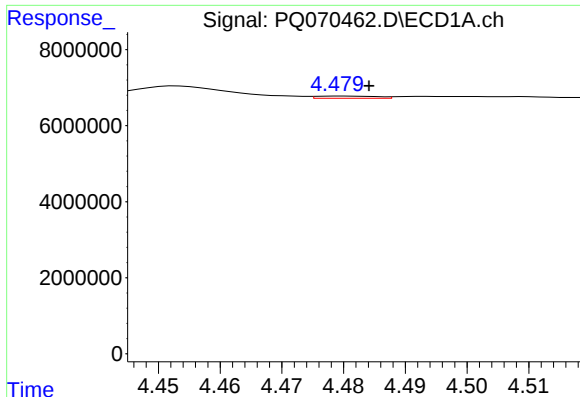

#21 AR-1248-1


R.T.: 4.479 min
Delta R.T.: -0.005 min
Response: 383109
Conc: 3.09 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

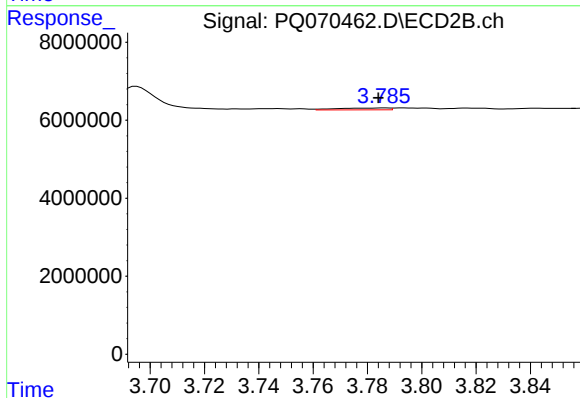


#21 AR-1248-1

R.T.: 3.786 min
Delta R.T.: 0.002 min
Response: 627817
Conc: 4.47 ng/ml

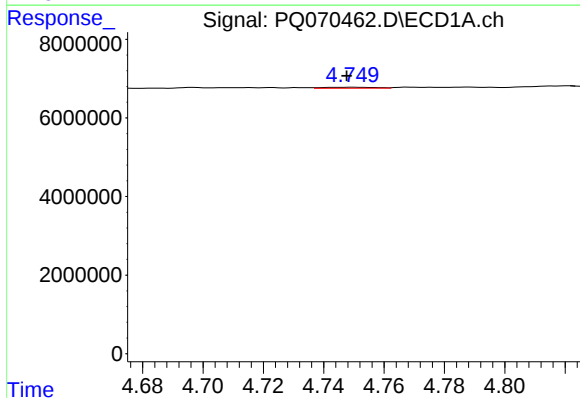


#22 AR-1248-2

R.T.: 4.749 min
Delta R.T.: 0.002 min
Response: 299634
Conc: 1.62 ng/ml

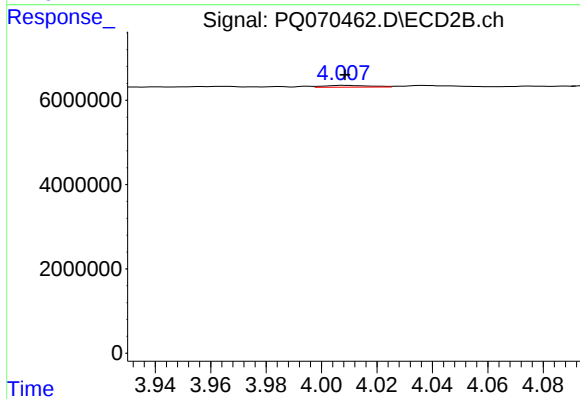

#22 AR-1248-2


R.T.: 4.008 min
Delta R.T.: 0.000 min
Response: 486696
Conc: 2.08 ng/ml

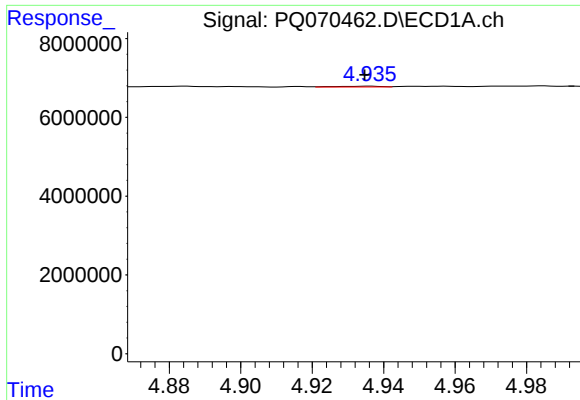

#23 AR-1248-3


R.T.: 4.936 min
Delta R.T.: 0.001 min
Response: 170903
Conc: 0.77 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

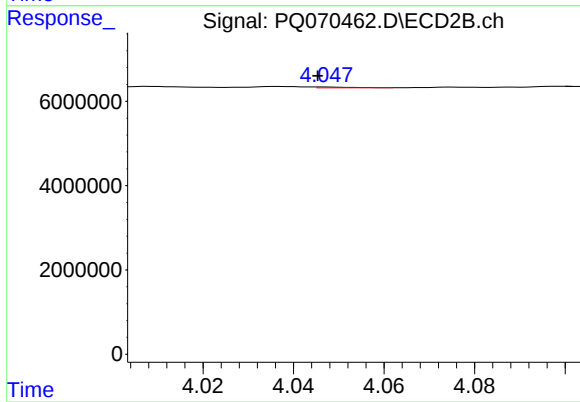


#23 AR-1248-3

R.T.: 4.047 min
Delta R.T.: 0.002 min
Response: 112216
Conc: 0.50 ng/ml

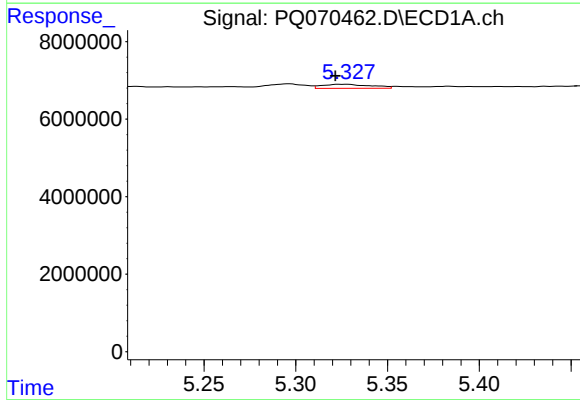


#24 AR-1248-4

R.T.: 5.328 min
Delta R.T.: 0.006 min
Response: 1933905
Conc: 8.71 ng/ml

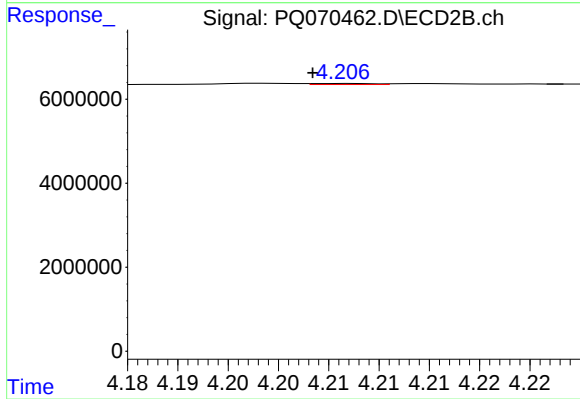

#24 AR-1248-4


R.T.: 4.207 min
Delta R.T.: 0.003 min
Response: 99807
Conc: 0.37 ng/ml

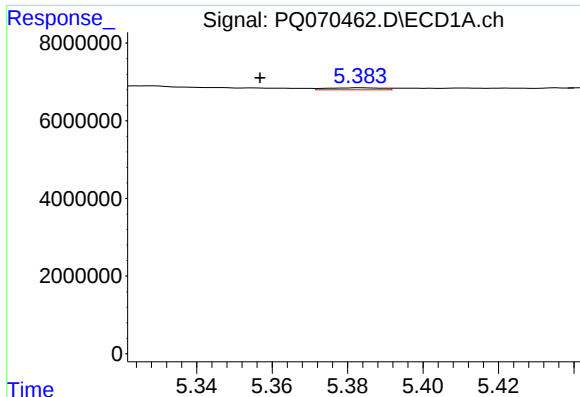

#25 AR-1248-5


R.T.: 5.383 min
Delta R.T.: 0.027 min
Response: 528729
Conc: 2.29 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

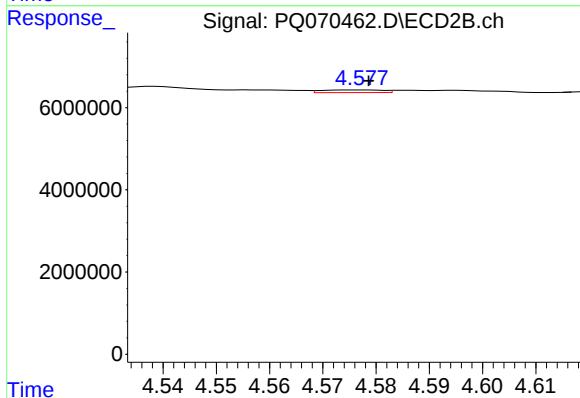


#25 AR-1248-5

R.T.: 4.577 min
Delta R.T.: -0.001 min
Response: 521806
Conc: 2.08 ng/ml

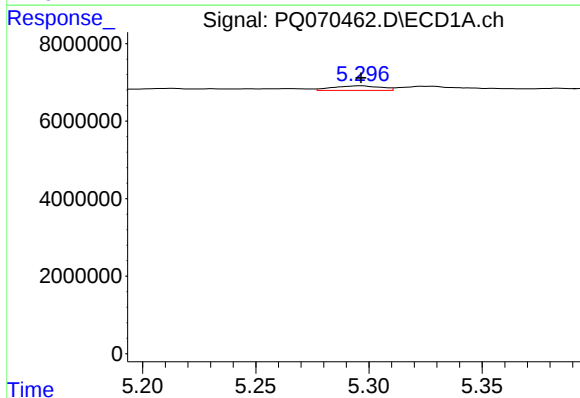


#26 AR-1254-1

R.T.: 5.297 min
Delta R.T.: 0.000 min
Response: 1721599
Conc: 6.96 ng/ml

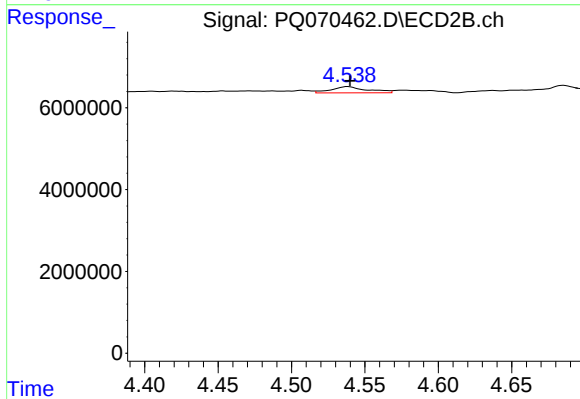

#26 AR-1254-1


R.T.: 4.538 min
Delta R.T.: -0.002 min
Response: 2618812
Conc: 6.46 ng/ml

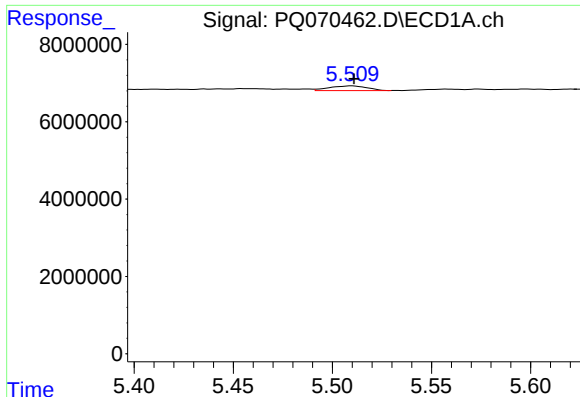

#27 AR-1254-2


R.T.: 5.510 min
Delta R.T.: -0.001 min
Response: 1623859
Conc: 4.32 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

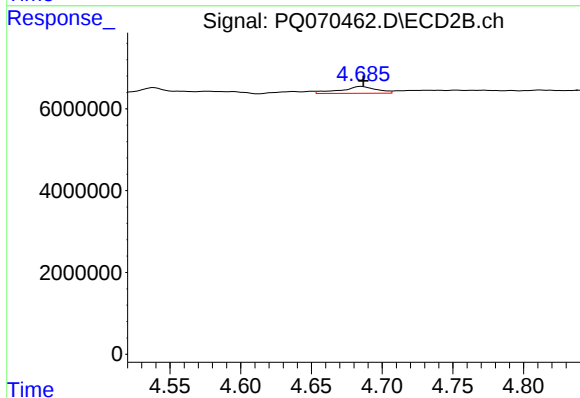


#27 AR-1254-2

R.T.: 4.685 min
Delta R.T.: -0.001 min
Response: 2977742
Conc: 8.25 ng/ml

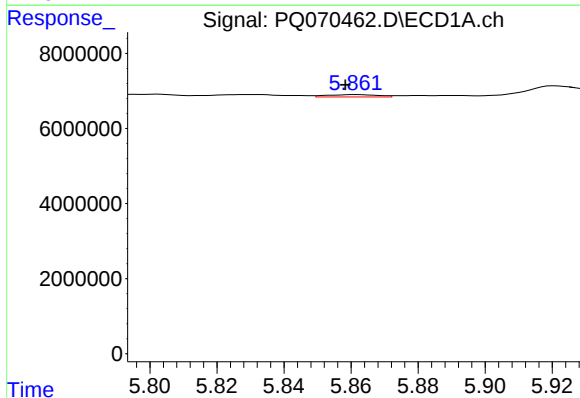


#28 AR-1254-3

R.T.: 5.861 min
Delta R.T.: 0.003 min
Response: 634145
Conc: 1.63 ng/ml

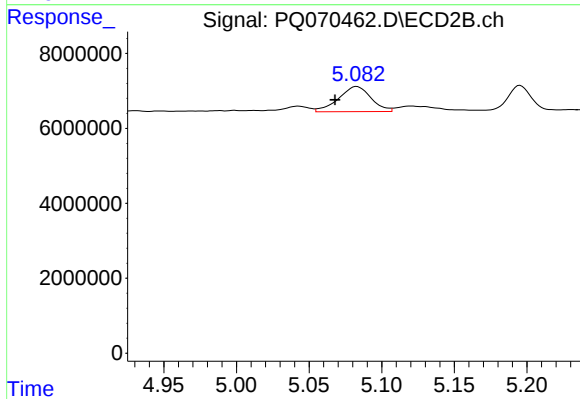

#28 AR-1254-3


R.T.: 5.083 min
Delta R.T.: 0.015 min
Response: 10439474
Conc: 18.46 ng/ml

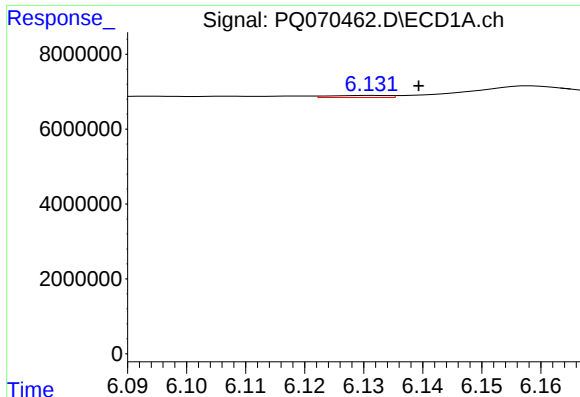

#29 AR-1254-4


R.T.: 6.131 min
Delta R.T.: -0.008 min
Response: 389213
Conc: 1.56 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

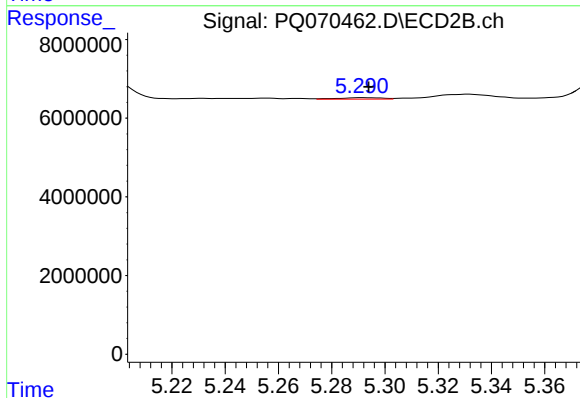


#29 AR-1254-4

R.T.: 5.291 min
Delta R.T.: -0.003 min
Response: 432737
Conc: 1.42 ng/ml

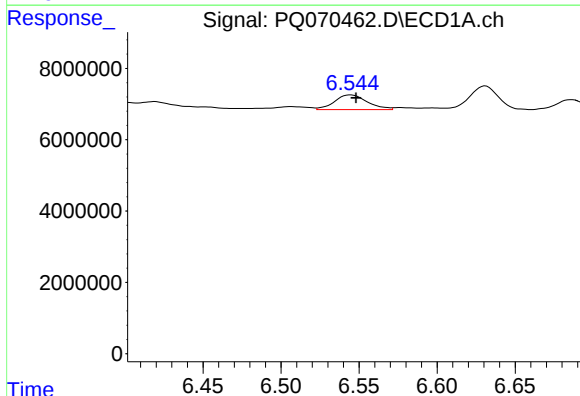


#30 AR-1254-5

R.T.: 6.545 min
Delta R.T.: -0.003 min
Response: 6076326
Conc: 20.46 ng/ml

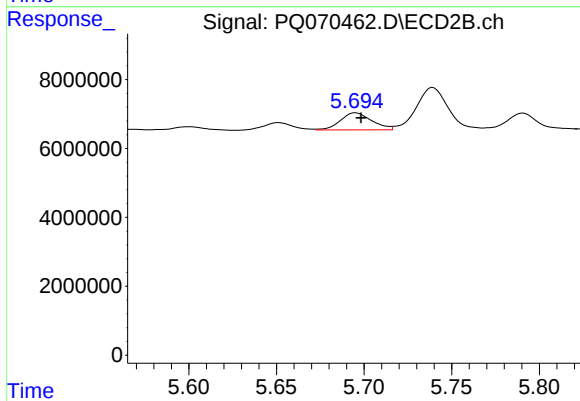

#30 AR-1254-5


R.T.: 5.695 min
Delta R.T.: -0.003 min
Response: 6205187
Conc: 12.06 ng/ml

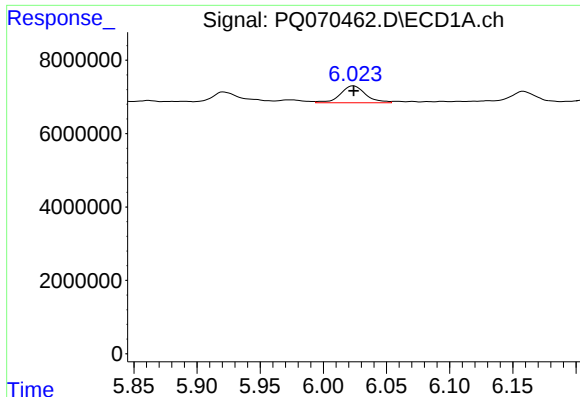

#31 AR-1260-1


R.T.: 6.024 min
Delta R.T.: 0.000 min
Response: 6388561
Conc: 22.11 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

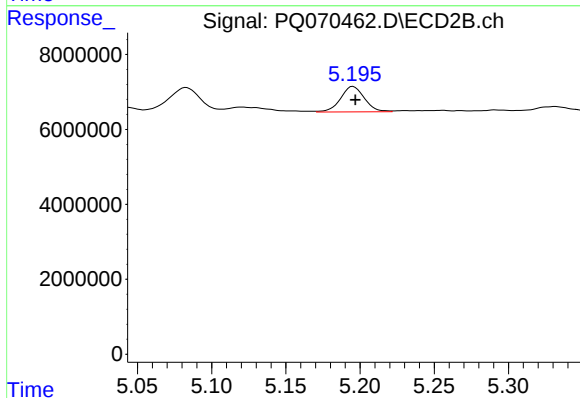


#31 AR-1260-1

R.T.: 5.195 min
Delta R.T.: -0.002 min
Response: 7640743
Conc: 20.00 ng/ml

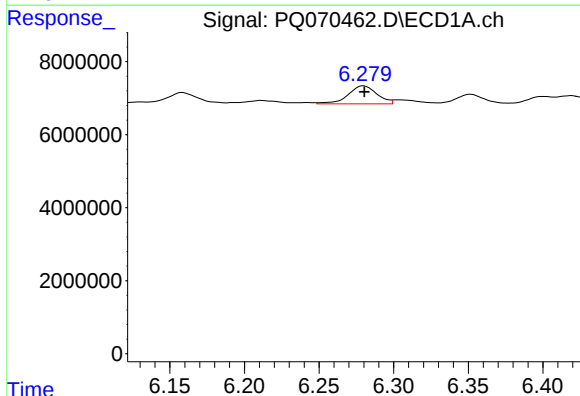


#32 AR-1260-2

R.T.: 6.280 min
Delta R.T.: 0.000 min
Response: 6689649
Conc: 20.98 ng/ml

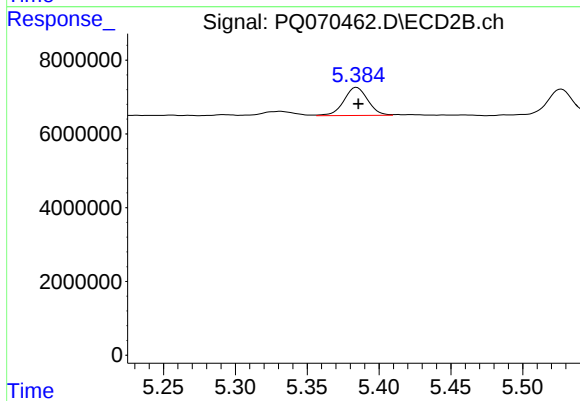

#32 AR-1260-2


R.T.: 5.384 min
Delta R.T.: -0.001 min
Response: 8799727
Conc: 20.09 ng/ml

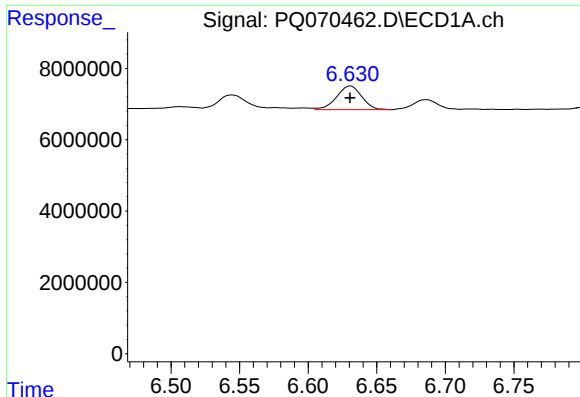

#33 AR-1260-3


R.T.: 6.631 min
Delta R.T.: 0.000 min
Response: 8464291
Conc: 32.60 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

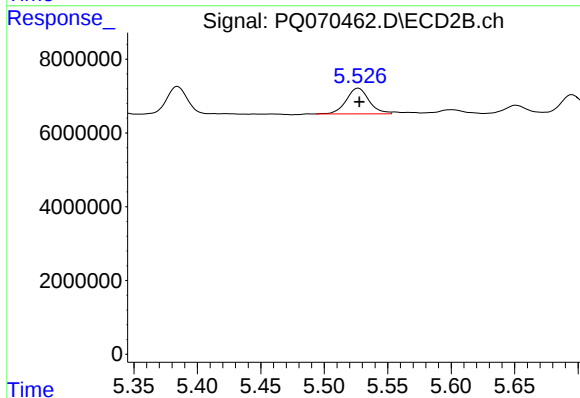


#33 AR-1260-3

R.T.: 5.527 min
Delta R.T.: 0.000 min
Response: 8689575
Conc: 20.14 ng/ml

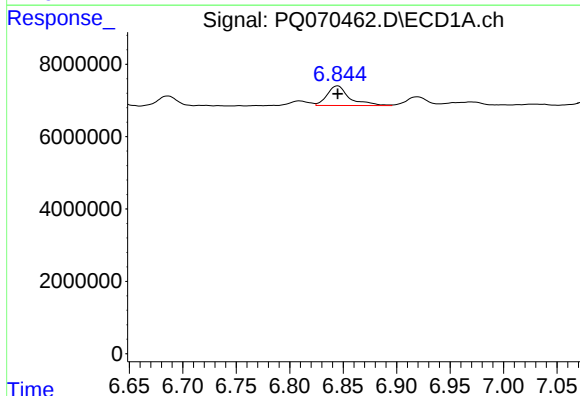


#34 AR-1260-4

R.T.: 6.845 min
Delta R.T.: 0.000 min
Response: 7924988
Conc: 29.09 ng/ml

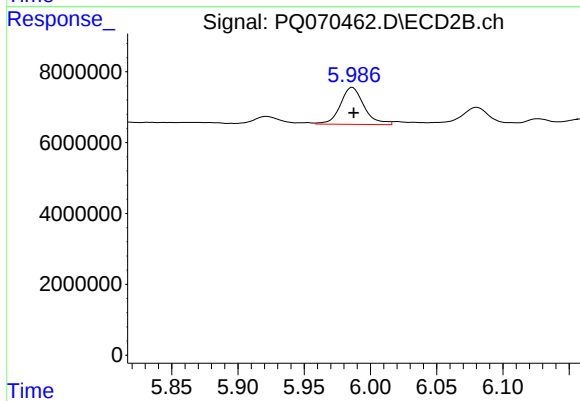

#34 AR-1260-4


R.T.: 5.986 min
Delta R.T.: -0.001 min
Response: 13021993
Conc: 35.49 ng/ml

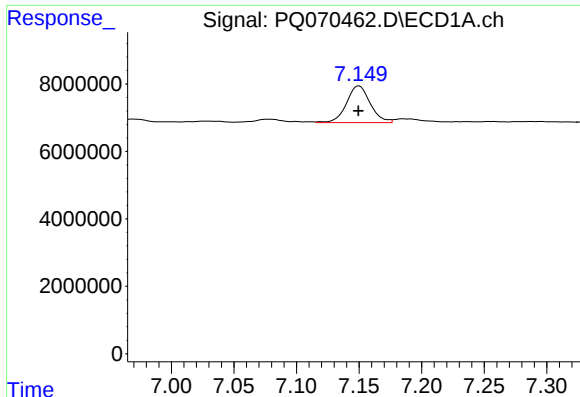

#35 AR-1260-5


R.T.: 7.150 min
Delta R.T.: 0.000 min
Response: 14331245
Conc: 28.77 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

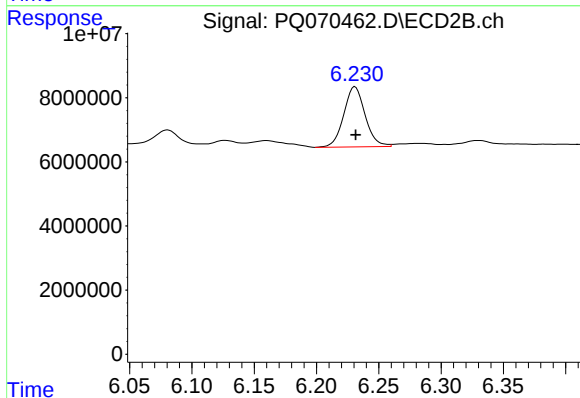


#35 AR-1260-5

R.T.: 6.231 min
Delta R.T.: 0.000 min
Response: 22521505
Conc: 27.10 ng/ml

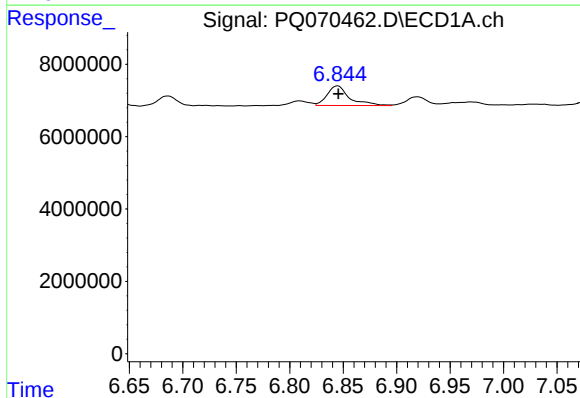


#36 AR-1262-1

R.T.: 6.845 min
Delta R.T.: 0.000 min
Response: 7924988
Conc: 22.51 ng/ml

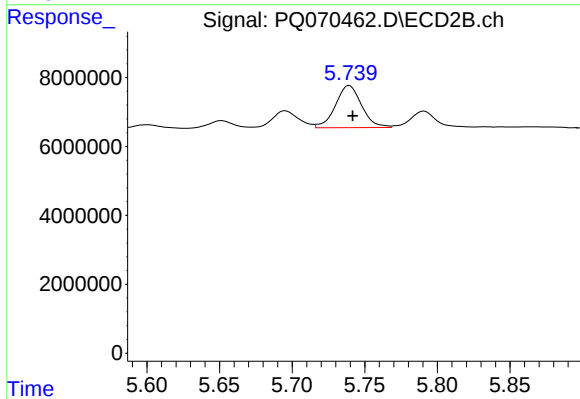

#36 AR-1262-1


R.T.: 5.739 min
Delta R.T.: -0.002 min
Response: 15277404
Conc: 27.92 ng/ml

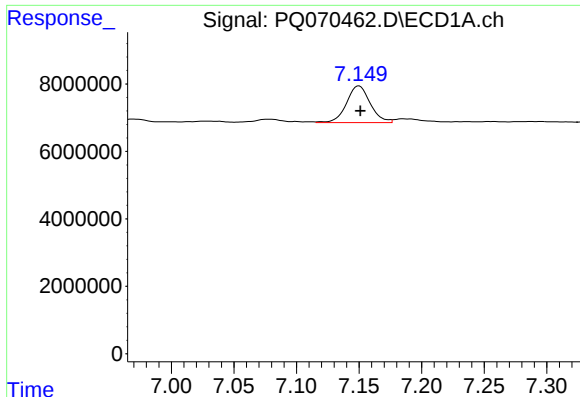

#37 AR-1262-2


R.T.: 7.150 min
Delta R.T.: -0.001 min
Response: 14331245
Conc: 25.30 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

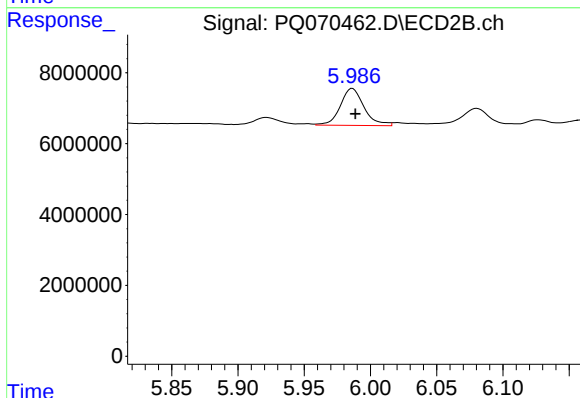


#37 AR-1262-2

R.T.: 5.986 min
Delta R.T.: -0.002 min
Response: 13021993
Conc: 25.61 ng/ml

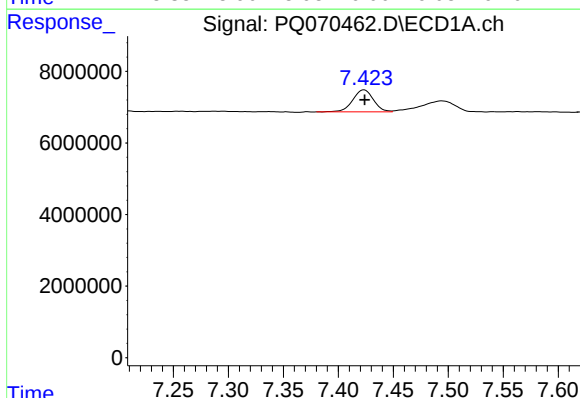


#38 AR-1262-3

R.T.: 7.423 min
Delta R.T.: 0.000 min
Response: 8086064
Conc: 20.76 ng/ml

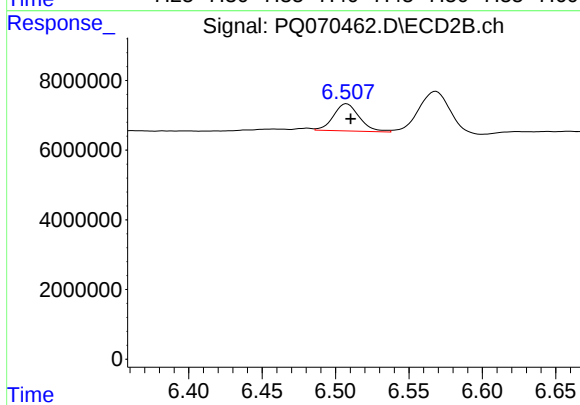

#38 AR-1262-3


R.T.: 6.508 min
Delta R.T.: -0.003 min
Response: 9654095
Conc: 24.59 ng/ml

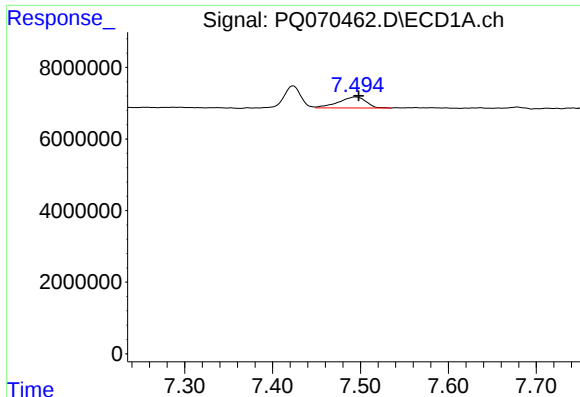

#39 AR-1262-4


R.T.: 7.494 min
Delta R.T.: -0.004 min
Response: 6749188
Conc: 21.09 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

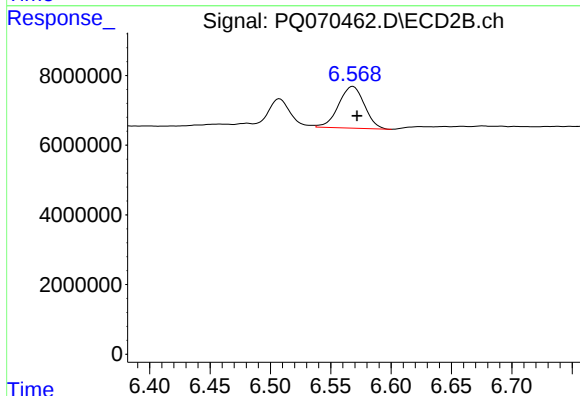


#39 AR-1262-4

R.T.: 6.568 min
Delta R.T.: -0.003 min
Response: 17882885
Conc: 25.53 ng/ml

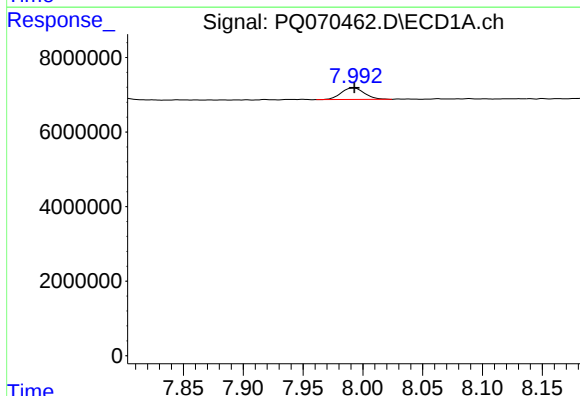


#40 AR-1262-5

R.T.: 7.992 min
Delta R.T.: 0.000 min
Response: 4221664
Conc: 22.54 ng/ml

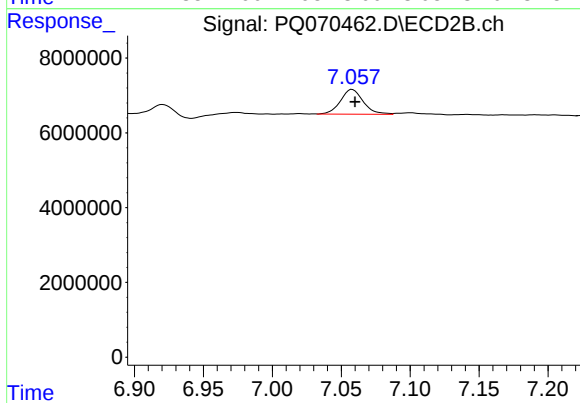

#40 AR-1262-5


R.T.: 7.058 min
Delta R.T.: -0.002 min
Response: 7601563
Conc: 23.97 ng/ml

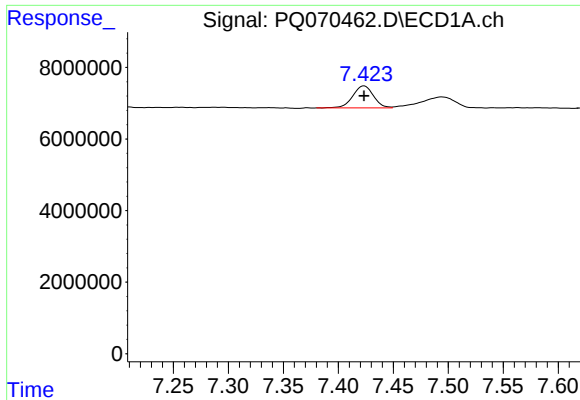

#41 AR-1268-1


R.T.: 7.423 min
Delta R.T.: 0.000 min
Response: 8086064
Conc: 11.22 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

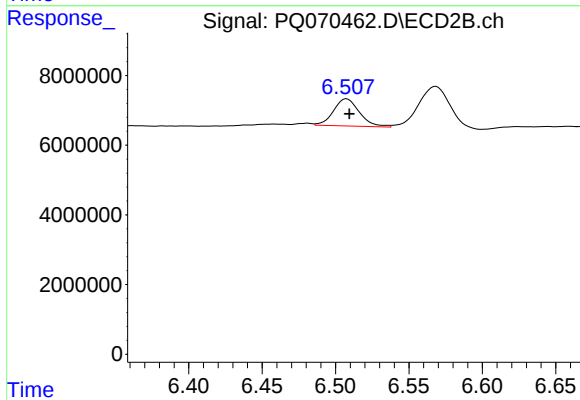


#41 AR-1268-1

R.T.: 6.508 min
Delta R.T.: -0.002 min
Response: 9654095
Conc: 8.33 ng/ml

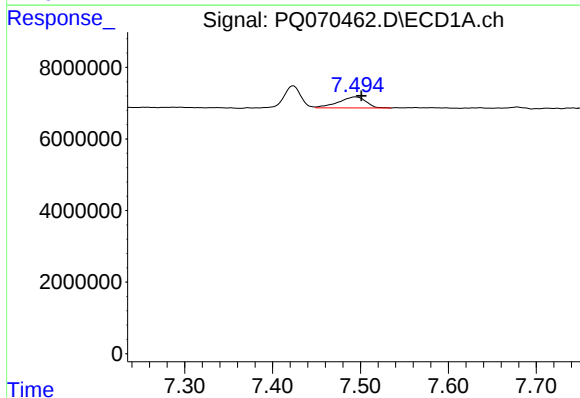


#42 AR-1268-2

R.T.: 7.494 min
Delta R.T.: -0.006 min
Response: 6749188
Conc: 10.16 ng/ml

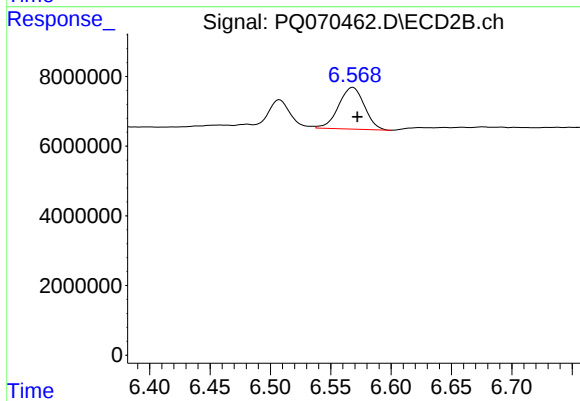

#42 AR-1268-2


R.T.: 6.568 min
Delta R.T.: -0.004 min
Response: 17882885
Conc: 16.68 ng/ml

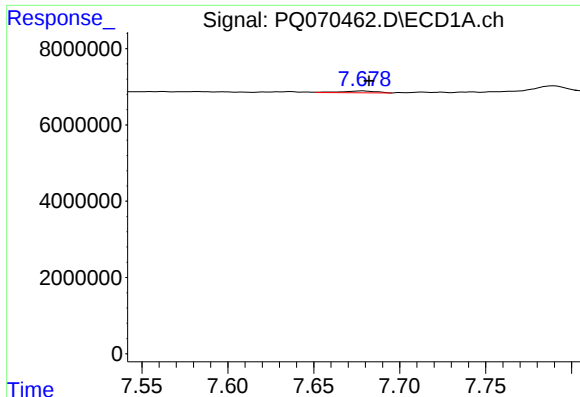

#43 AR-1268-3


R.T.: 7.678 min
Delta R.T.: -0.004 min
Response: 690872
Conc: 1.22 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

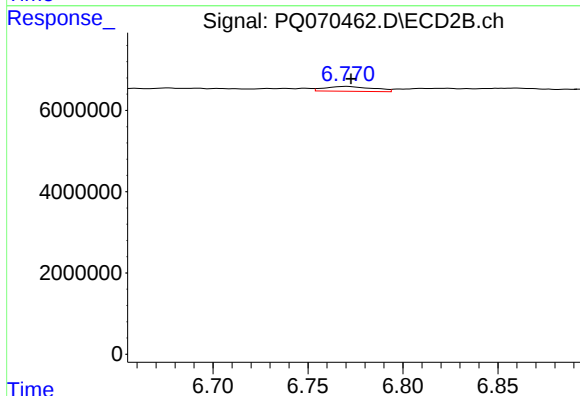


#43 AR-1268-3

R.T.: 6.770 min
Delta R.T.: -0.003 min
Response: 2099031
Conc: 2.20 ng/ml

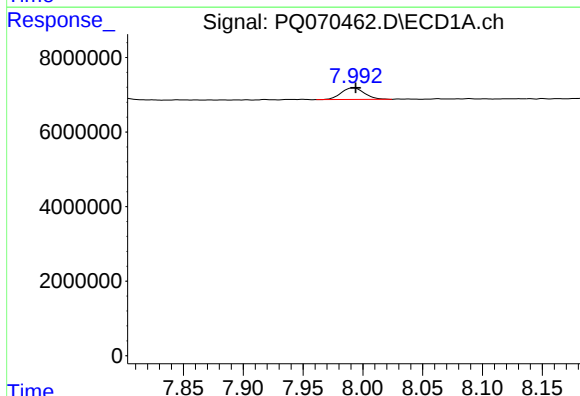


#44 AR-1268-4

R.T.: 7.992 min
Delta R.T.: -0.002 min
Response: 4221664
Conc: 20.46 ng/ml

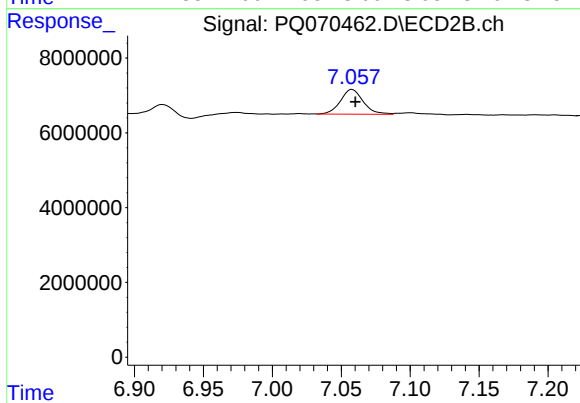

#44 AR-1268-4


R.T.: 7.058 min
Delta R.T.: -0.002 min
Response: 7601563
Conc: 20.21 ng/ml

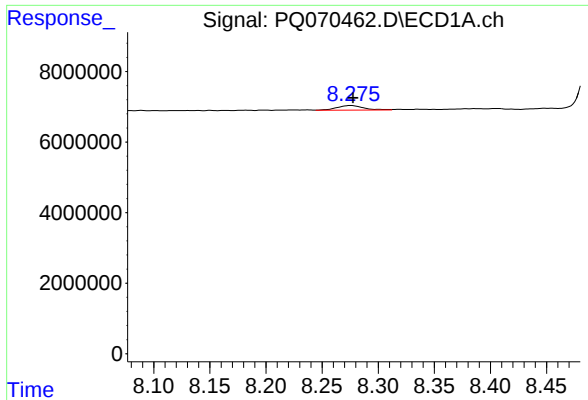

#45 AR-1268-5

R.T.: 8.276 min
Delta R.T.: -0.002 min
Response: 2190816
Conc: 1.37 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT2-2025

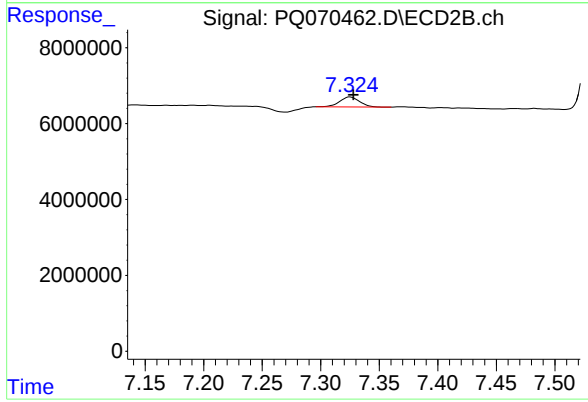

#45 AR-1268-5

R.T.: 7.325 min
Delta R.T.: -0.003 min
Response: 3107480
Conc: 1.18 ng/ml