

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ062623\
 Data File : PQ061698.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jun 2023 16:30
 Operator : YP\AJ
 Sample : 03393-03
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 SF-10

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/27/2023
 Supervised By :Ankita Jodhani 06/27/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 21:52:46 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ060923.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 09 18:19:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.404	2.759	86061982	53757176	19.146	20.131
2) SA Decachlor...	8.580	7.530	65639091	63697049	19.485m	18.977

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ062623\
Data File : PQ061698.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jun 2023 16:30
Operator : YP\AJ
Sample : 03393-03
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
SF-10


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/27/2023
Supervised By :Ankita Jodhani 06/27/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 21:52:46 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ060923.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 09 18:19:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

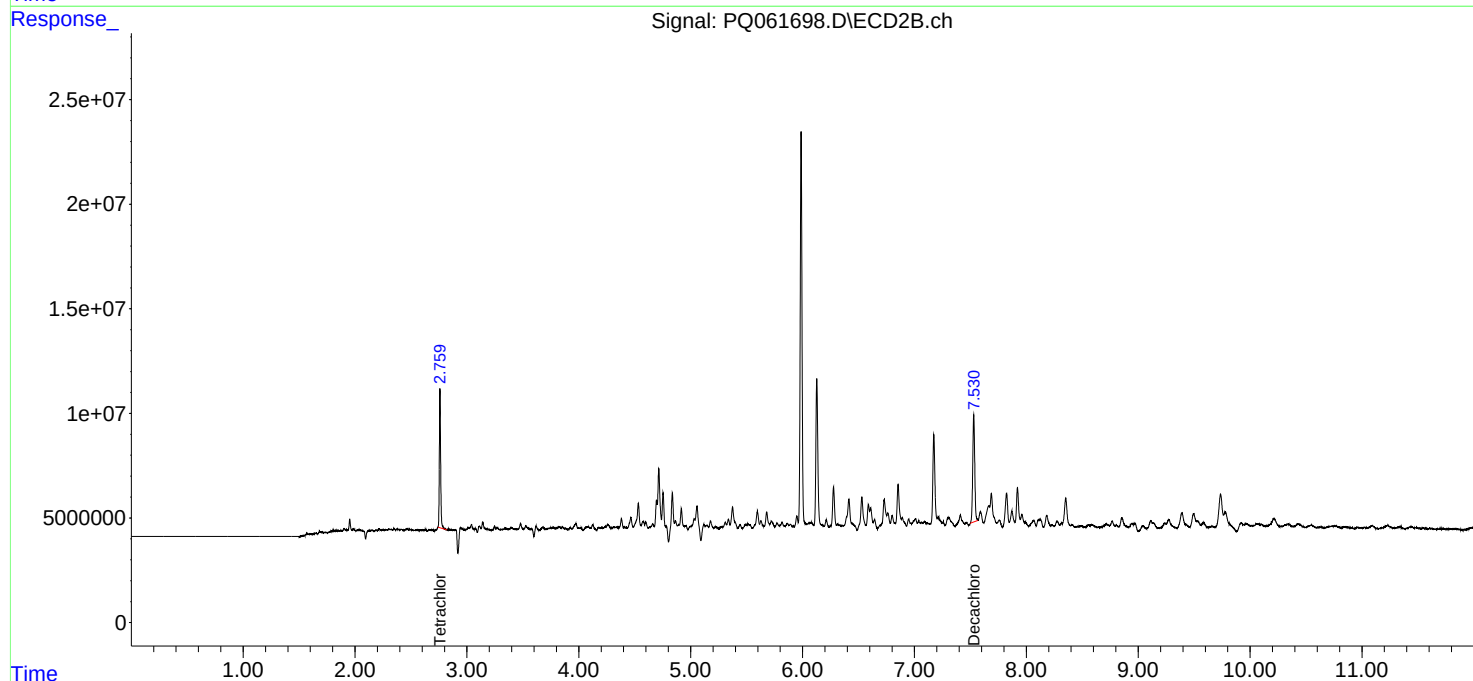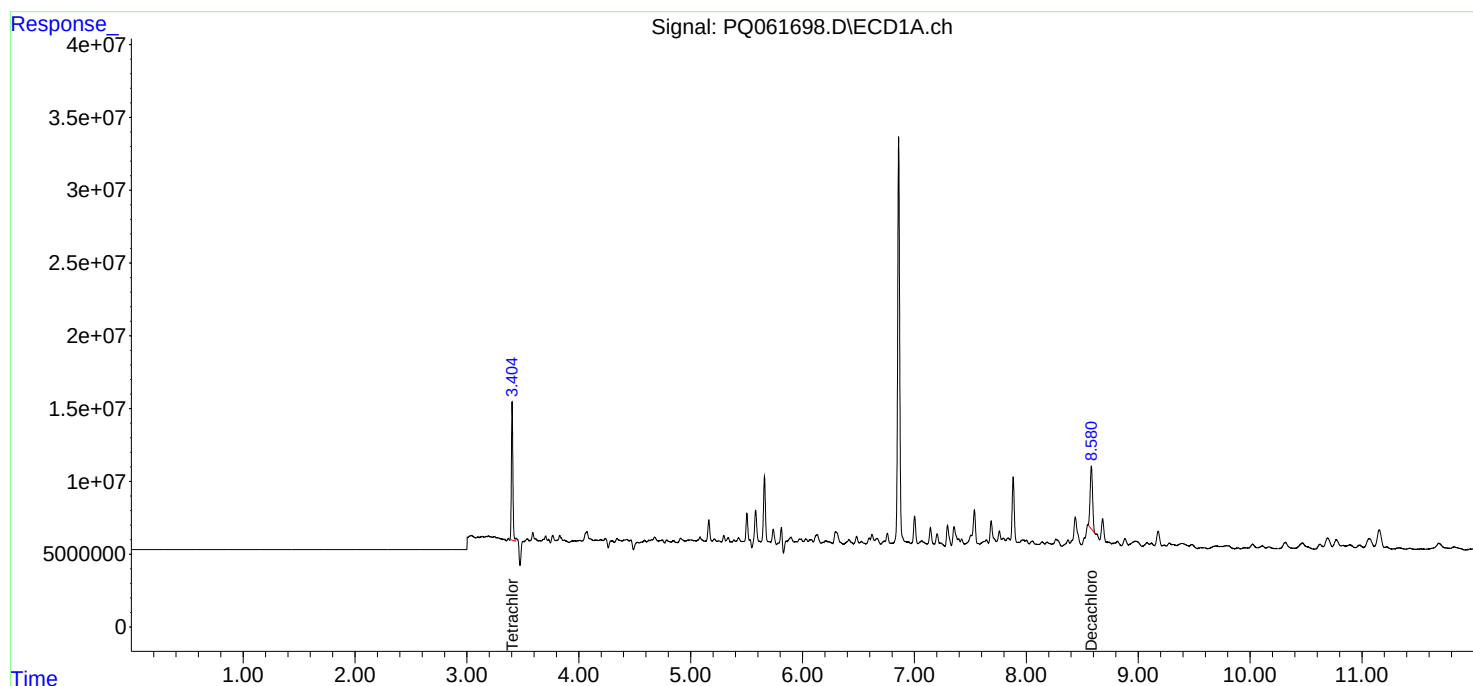

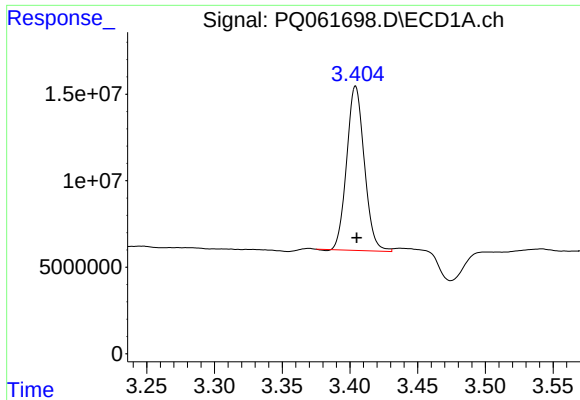


#1 Tetrachloro-m-xylene

R.T.: 3.404 min
Delta R.T.: 0.000 min
Response: 86061982
Conc: 19.15 ng/ml

Instrument :
ECD_Q
ClientSampleId :
SF-10


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/27/2023
Supervised By :Ankita Jodhani 06/27/2023

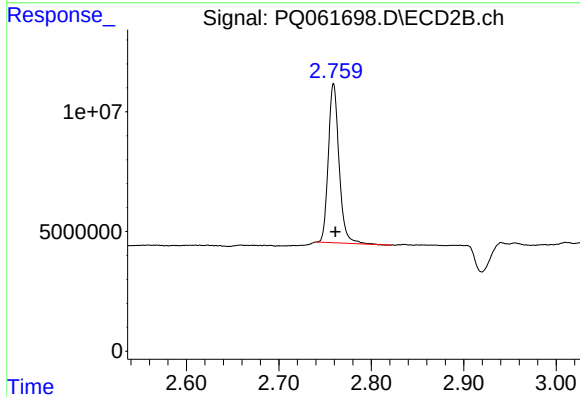


#1 Tetrachloro-m-xylene

R.T.: 2.759 min
Delta R.T.: -0.002 min
Response: 53757176
Conc: 20.13 ng/ml

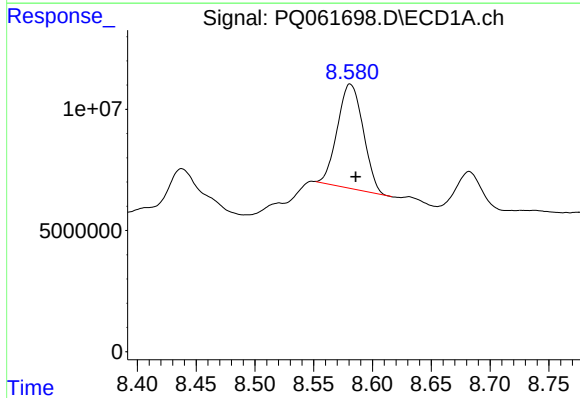

#2 Decachlorobiphenyl

R.T.: 8.580 min
Delta R.T.: -0.005 min
Response: 65639091
Conc: 19.49 ng/ml m

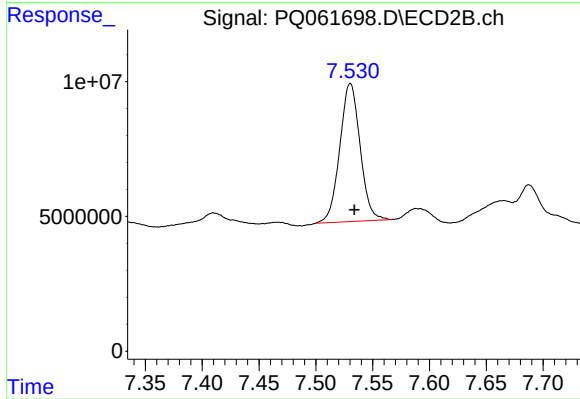

#2 Decachlorobiphenyl

R.T.: 7.530 min
Delta R.T.: -0.004 min
Response: 63697049
Conc: 18.98 ng/ml