

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ062823\
 Data File : PQ061717.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jun 2023 15:11
 Operator : YP\AJ
 Sample : 03429-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 SB-COMP-0627

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/29/2023
 Supervised By :Ankita Jodhani 06/29/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 17:58:55 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ060923.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 09 18:19:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.405	2.759	83773252	52335025	18.637	19.599
2) SA Decachlor...	8.584	7.530	45577648	45106675	13.530m	13.439m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ062823\
Data File : PQ061717.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jun 2023 15:11
Operator : YP\AJ
Sample : 03429-01
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
SB-COMP-0627


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/29/2023
Supervised By :Ankita Jodhani 06/29/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 17:58:55 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ060923.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 09 18:19:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

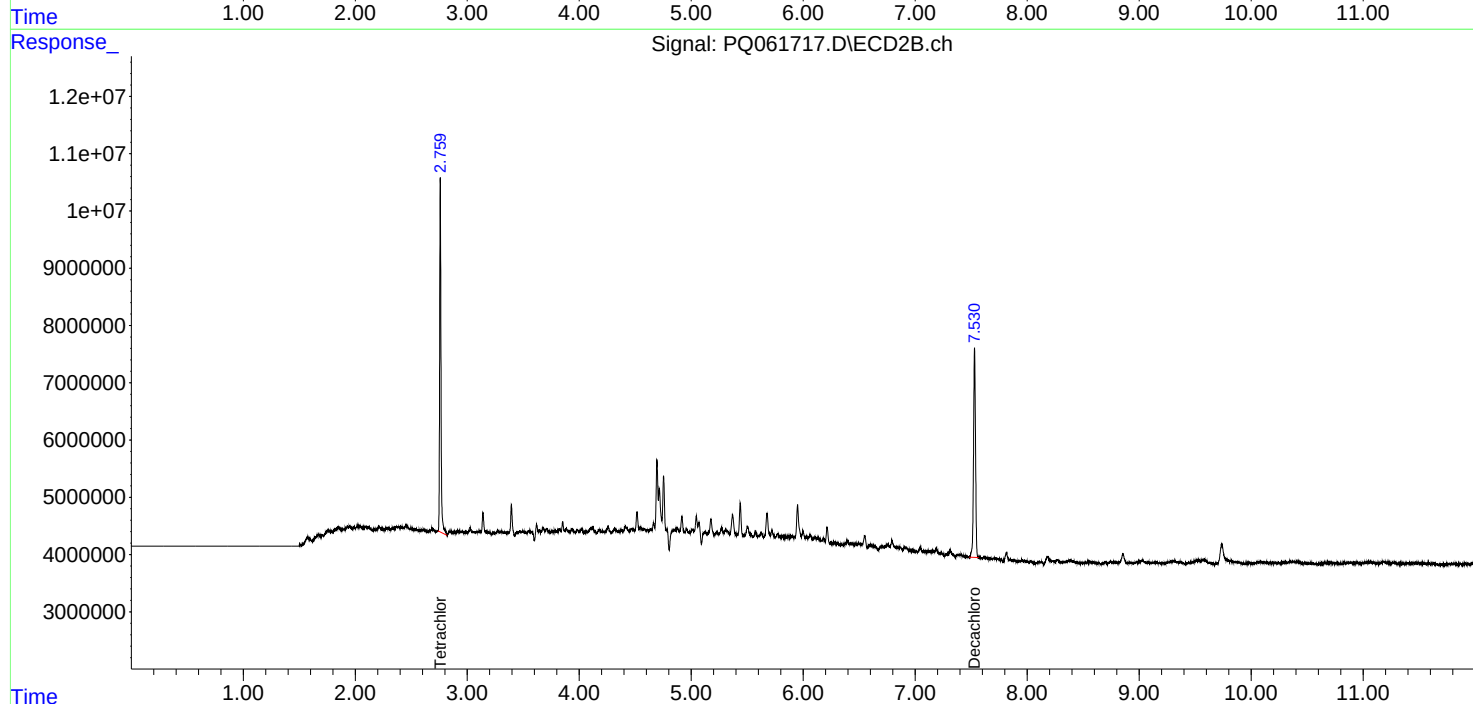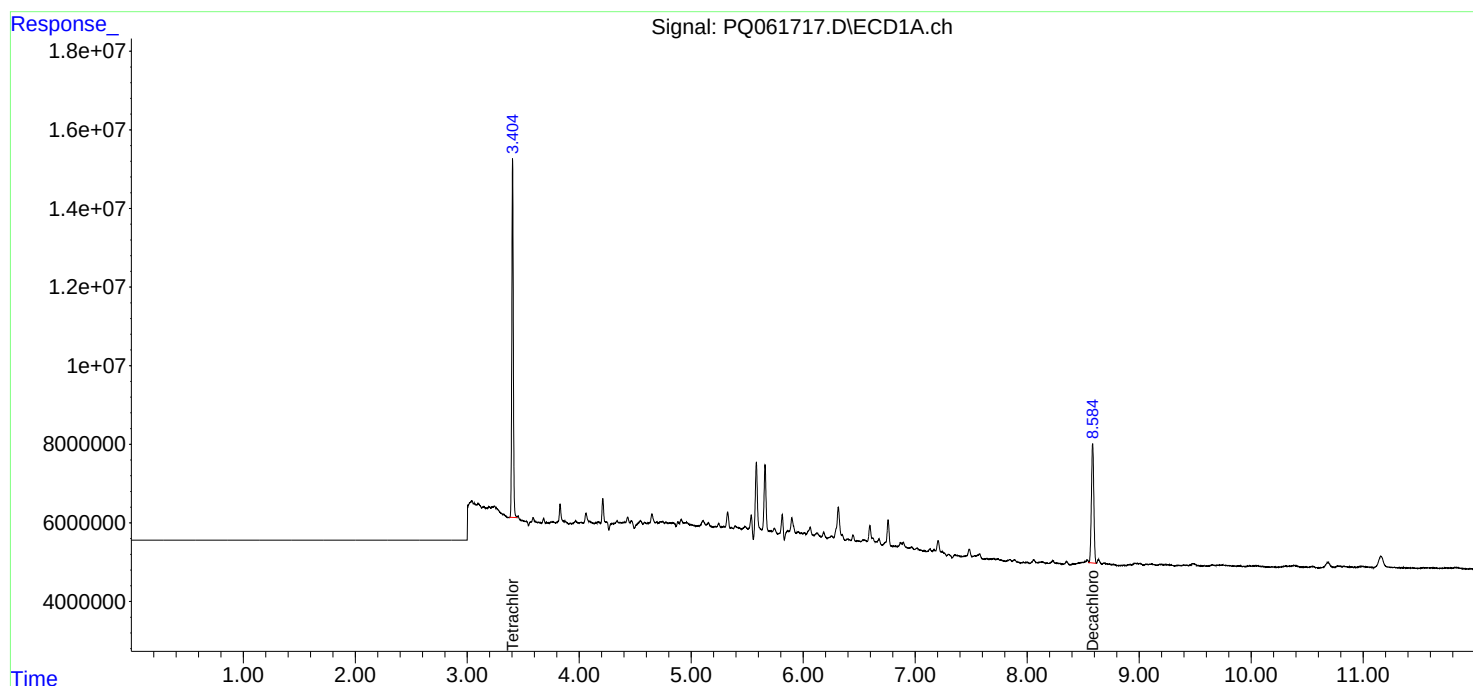

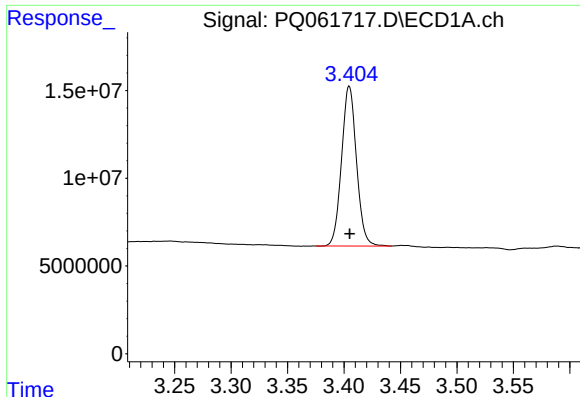


#1 Tetrachloro-m-xylene

R.T.: 3.405 min
Delta R.T.: 0.000 min
Response: 83773252
Conc: 18.64 ng/ml

Instrument :
ECD_Q
ClientSampleId :
SB-COMP-0627


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/29/2023
Supervised By :Ankita Jodhani 06/29/2023

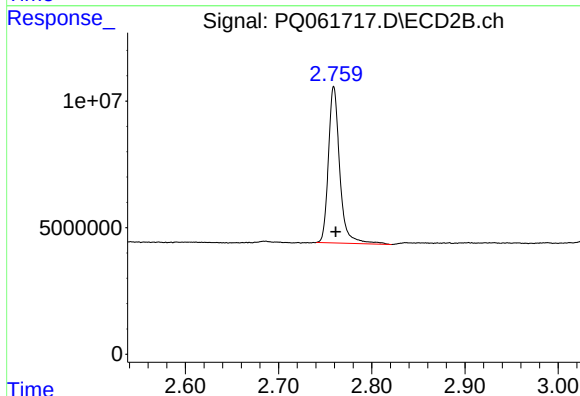


#1 Tetrachloro-m-xylene

R.T.: 2.759 min
Delta R.T.: -0.002 min
Response: 52335025
Conc: 19.60 ng/ml

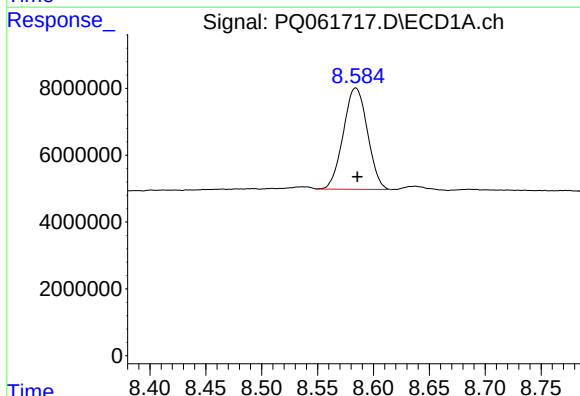

#2 Decachlorobiphenyl

R.T.: 8.584 min
Delta R.T.: -0.002 min
Response: 45577648
Conc: 13.53 ng/ml m

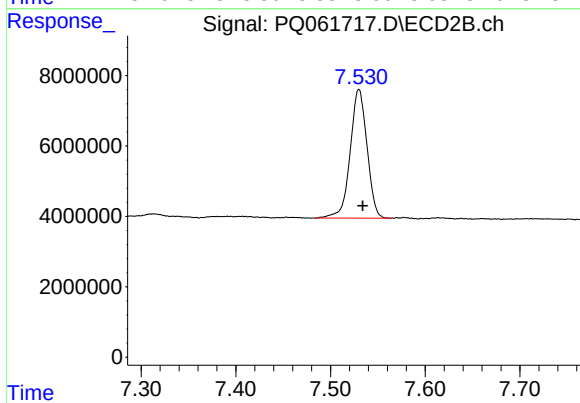

#2 Decachlorobiphenyl

R.T.: 7.530 min
Delta R.T.: -0.004 min
Response: 45106675
Conc: 13.44 ng/ml m