

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ062923\
 Data File : PQ061771.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jun 2023 23:08
 Operator : YP\AJ
 Sample : 03465-03 10X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 3110

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/30/2023
 Supervised By :Ankita Jodhani 06/30/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 30 05:07:48 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ060923.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 09 18:19:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.404	2.758	3932126	2091425	0.875	0.783m
2) SA Decachlor...	8.579	7.529	2512998	1610466	0.746m	0.480 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ062923\
Data File : PQ061771.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jun 2023 23:08
Operator : YP\AJ
Sample : 03465-03 10X
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
3110


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/30/2023
Supervised By :Ankita Jodhani 06/30/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 30 05:07:48 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ060923.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 09 18:19:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

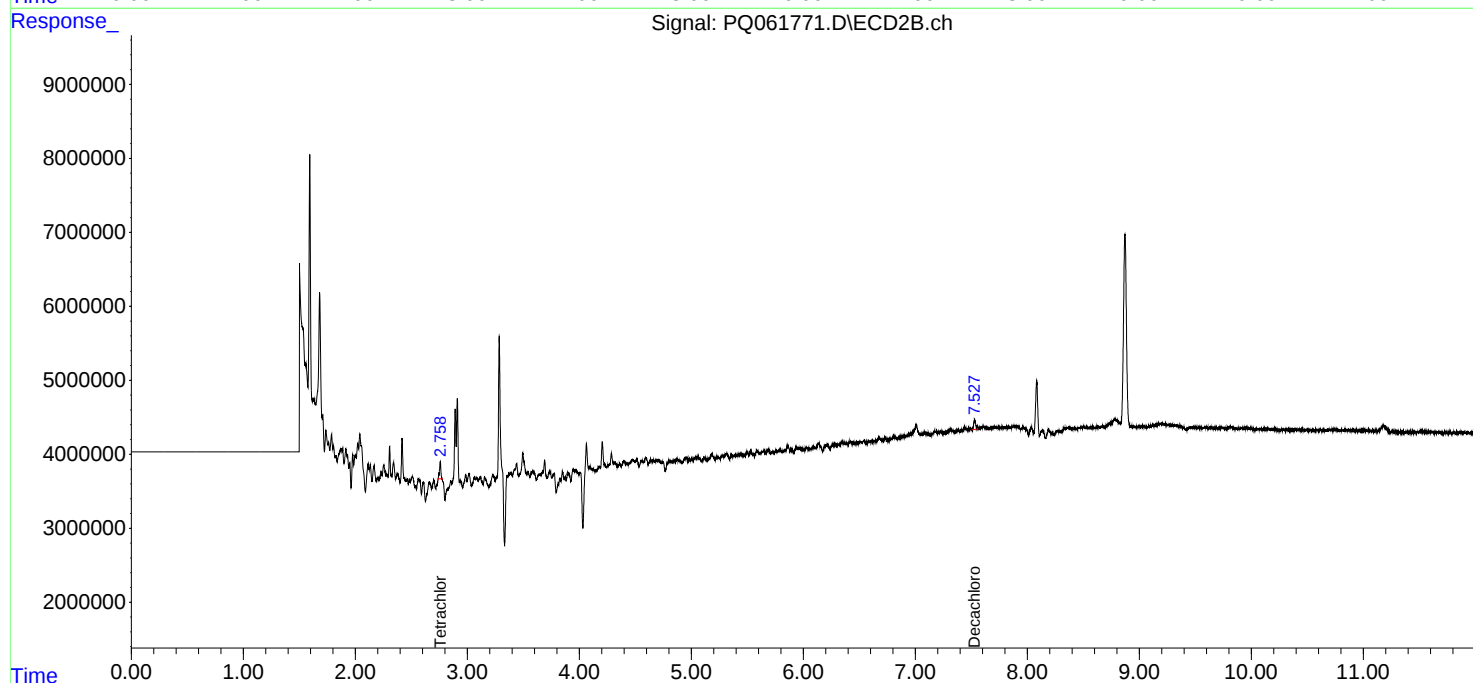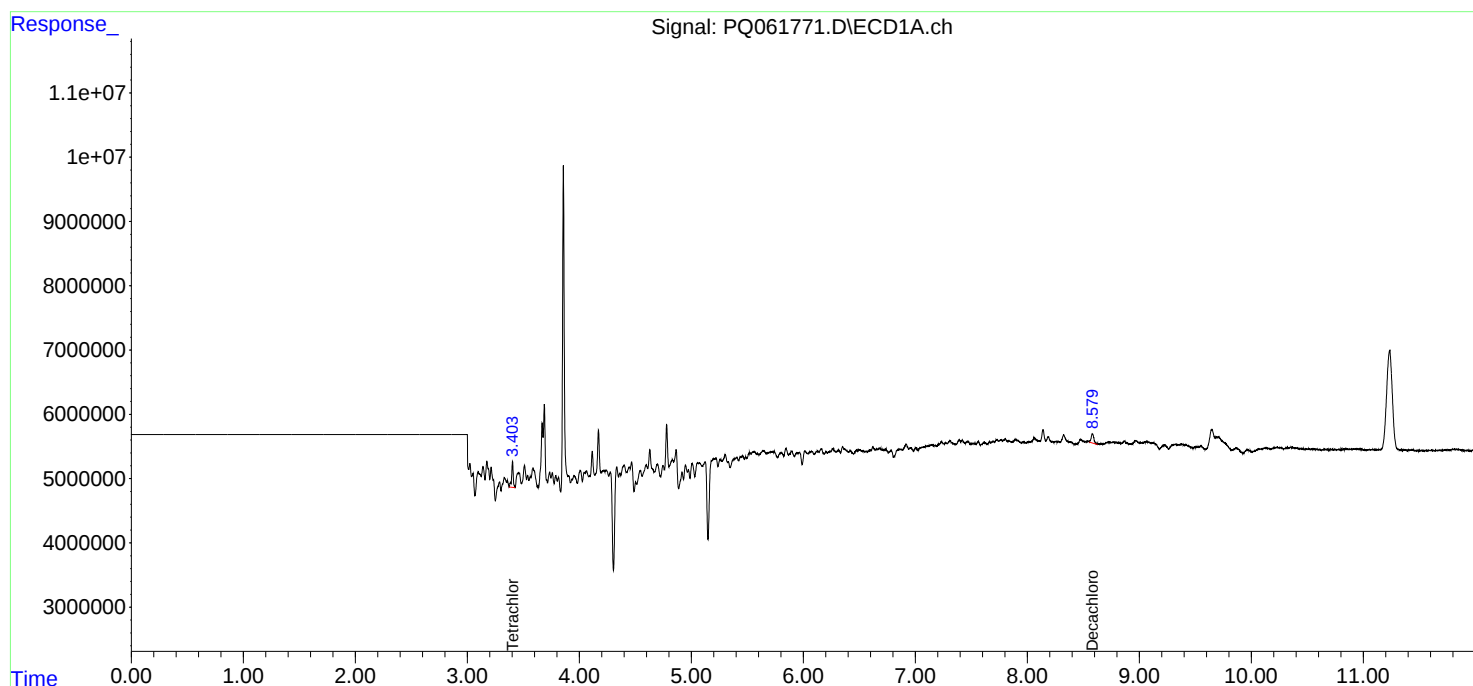

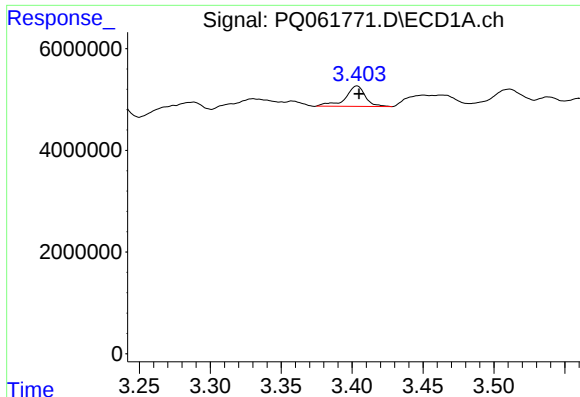


#1 Tetrachloro-m-xylene

R.T.: 3.404 min
Delta R.T.: -0.001 min
Response: 3932126
Conc: 0.87 ng/ml

Instrument :
ECD_Q
ClientSampleId :
3110


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/30/2023
Supervised By :Ankita Jodhani 06/30/2023

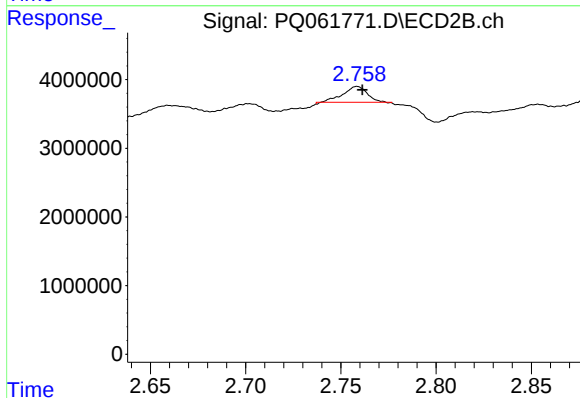


#1 Tetrachloro-m-xylene

R.T.: 2.758 min
Delta R.T.: -0.003 min
Response: 2091425
Conc: 0.78 ng/ml m

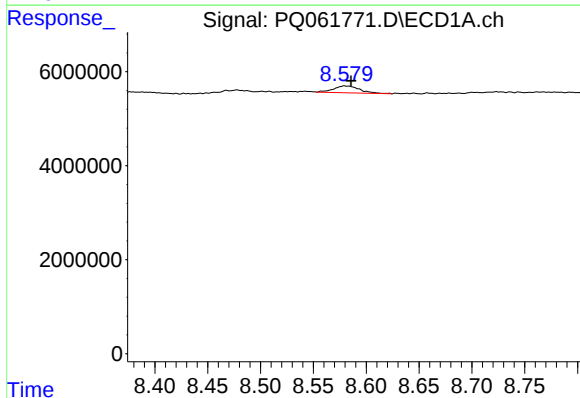

#2 Decachlorobiphenyl

R.T.: 8.579 min
Delta R.T.: -0.007 min
Response: 2512998
Conc: 0.75 ng/ml m

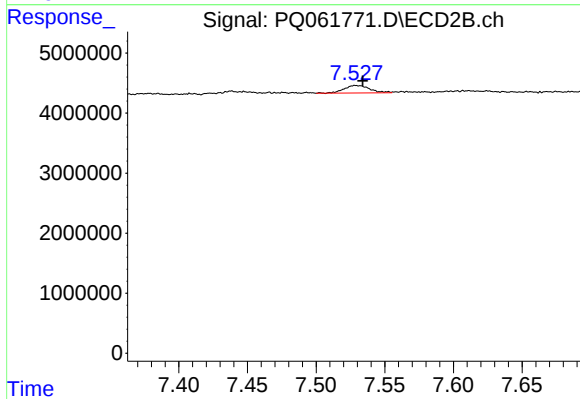

#2 Decachlorobiphenyl

R.T.: 7.529 min
Delta R.T.: -0.005 min
Response: 1610466
Conc: 0.48 ng/ml