

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ070125\
 Data File : PQ070502.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jul 2025 11:34
 Operator : YP\AJ
 Sample : Q2445-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 CONCRETE-PAD-6-27-25

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 02 01:46:41 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ062425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jun 26 02:49:53 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.403	2.782	59398795	64564540	9.703	9.561
2) SA Decachlor...	8.500	7.541	81887600	136.7E6	19.892	18.862

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ070125\
Data File : PQ070502.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jul 2025 11:34
Operator : YP\AJ
Sample : Q2445-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
CONCRETE-PAD-6-27-25

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 02 01:46:41 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ062425.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 26 02:49:53 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

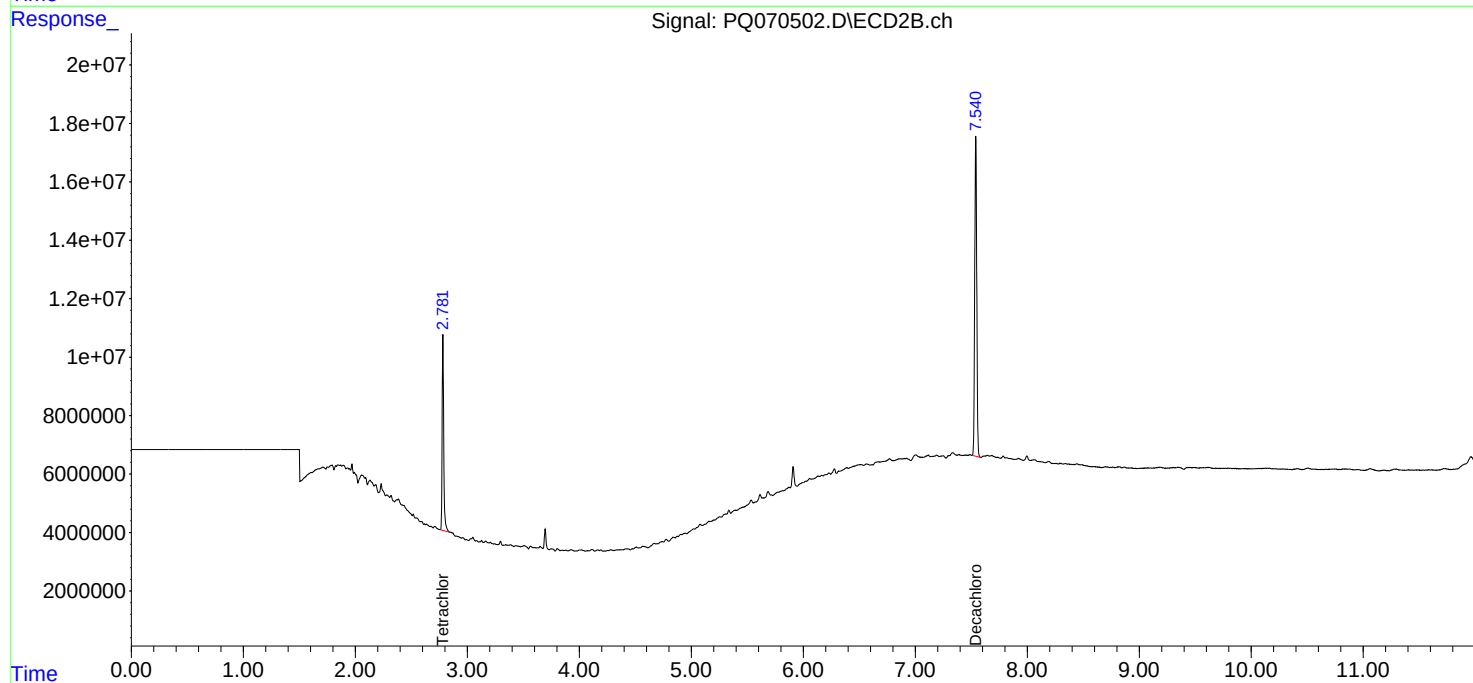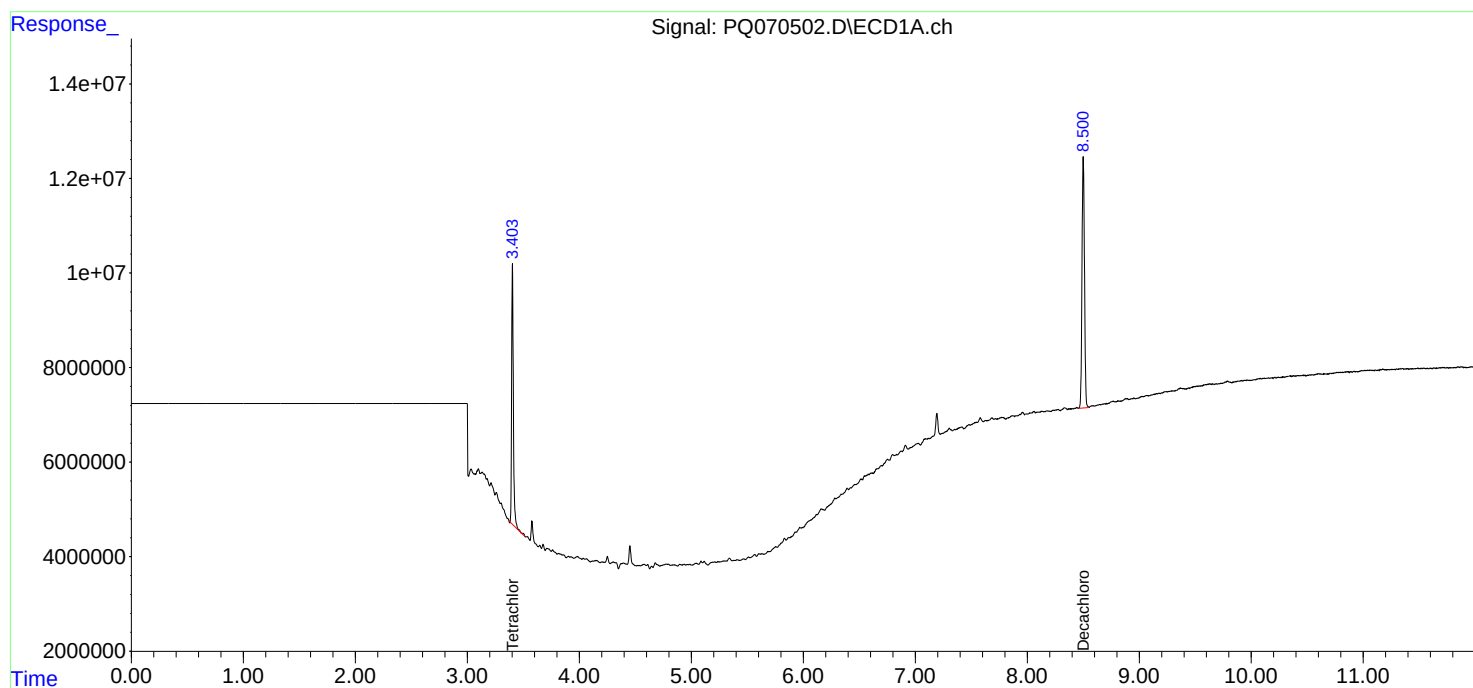


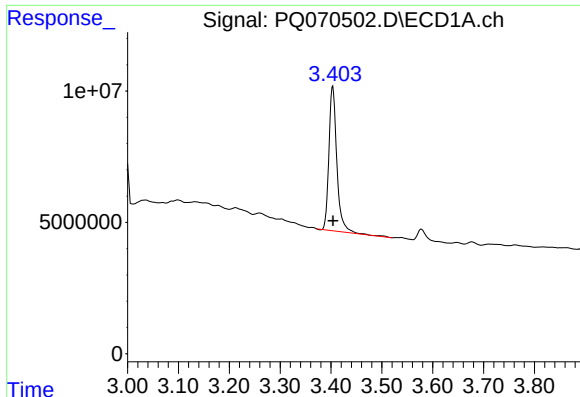

#1 Tetrachloro-m-xylene


R.T.: 3.403 min
Delta R.T.: 0.000 min
Response: 59398795
Conc: 9.70 ng/ml

Instrument :
ECD_Q
ClientSampleId :
CONCRETE-PAD-6-27-25

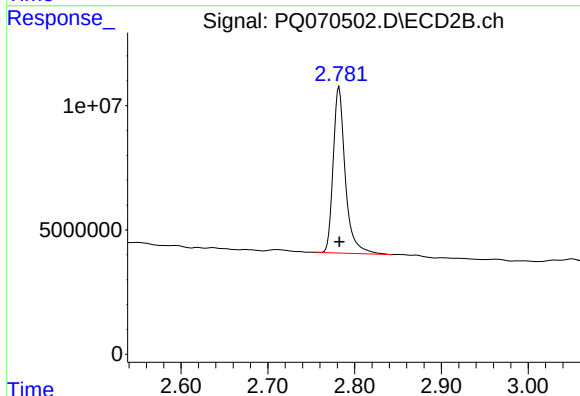


#1 Tetrachloro-m-xylene

R.T.: 2.782 min
Delta R.T.: 0.000 min
Response: 64564540
Conc: 9.56 ng/ml

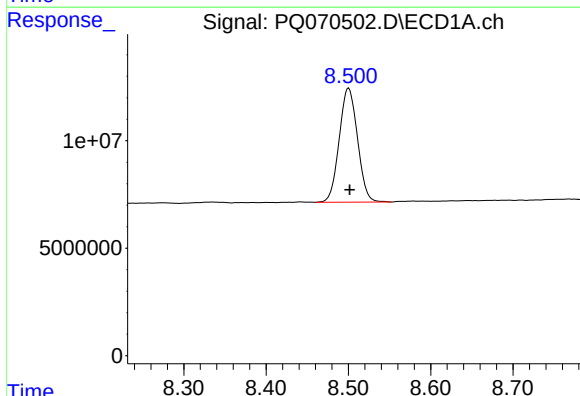

#2 Decachlorobiphenyl

R.T.: 8.500 min
Delta R.T.: -0.001 min
Response: 81887600
Conc: 19.89 ng/ml

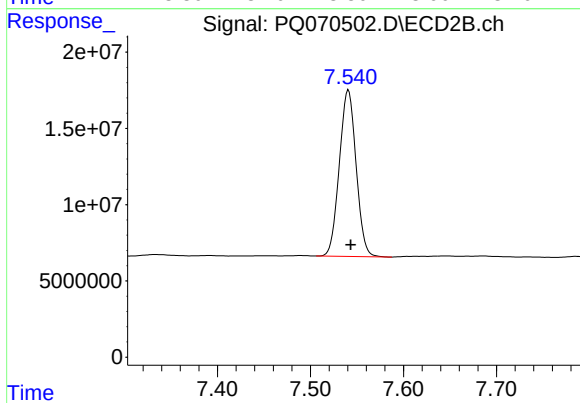

#2 Decachlorobiphenyl

R.T.: 7.541 min
Delta R.T.: -0.003 min
Response: 136739923
Conc: 18.86 ng/ml