

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ070125\
 Data File : PQ070510.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jul 2025 13:31
 Operator : YP\AJ
 Sample : Q2447-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 COMP-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/02/2025
 Supervised By :mohammad ahmed 07/02/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 02 01:49:23 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ062425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jun 26 02:49:53 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.411	2.793	52767851	56056095	8.620	8.301
2) SA Decachlor...	8.502	7.542	56606230	72148536	13.751m	9.952m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ070125\
Data File : PQ070510.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jul 2025 13:31
Operator : YP\AJ
Sample : Q2447-04
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
COMP-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/02/2025
Supervised By :mohammad ahmed 07/02/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 02 01:49:23 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ062425.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 26 02:49:53 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

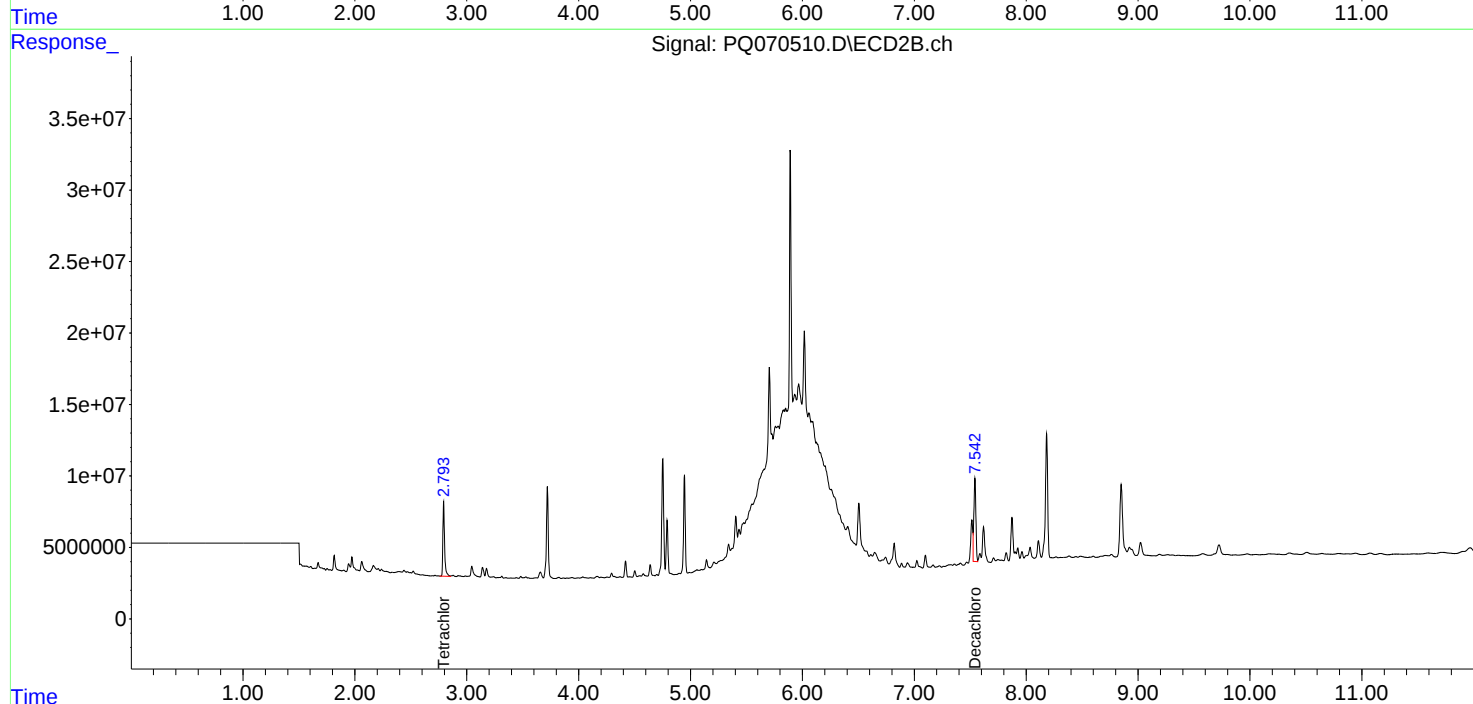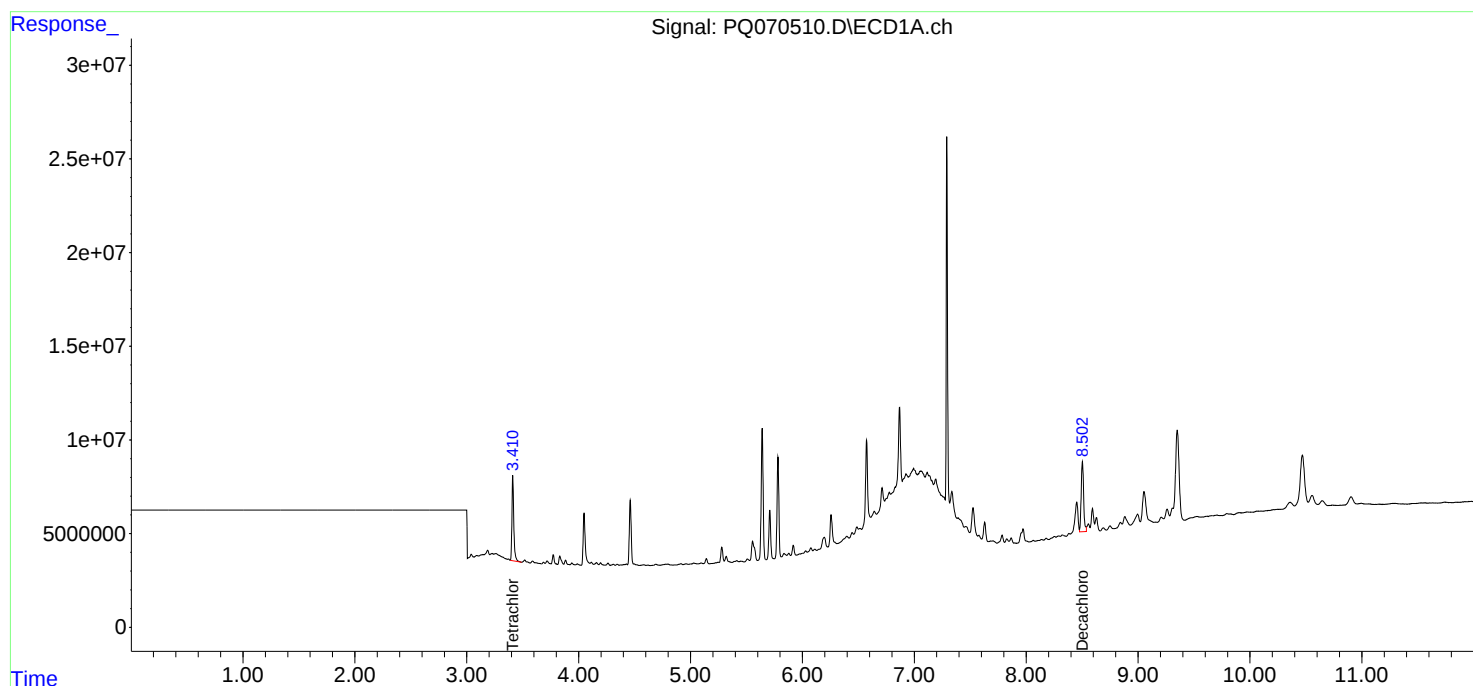

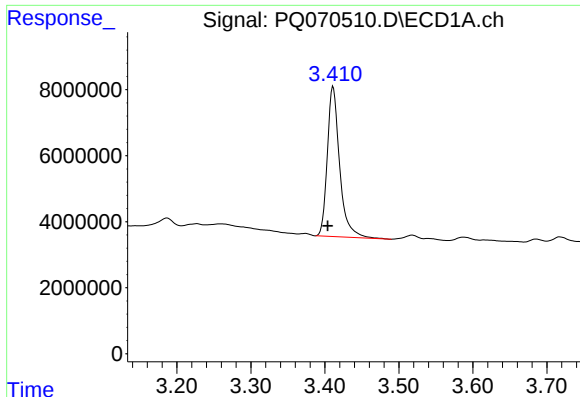


#1 Tetrachloro-m-xylene

R.T.: 3.411 min
Delta R.T.: 0.007 min
Response: 52767851
Conc: 8.62 ng/ml

Instrument :
ECD_Q
ClientSampleId :
COMP-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/02/2025
Supervised By :mohammad ahmed 07/02/2025

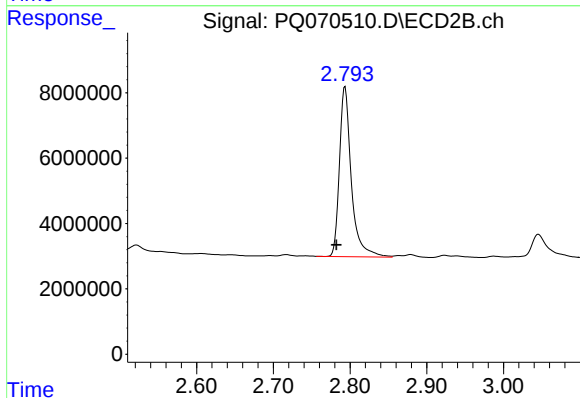


#1 Tetrachloro-m-xylene

R.T.: 2.793 min
Delta R.T.: 0.011 min
Response: 56056095
Conc: 8.30 ng/ml

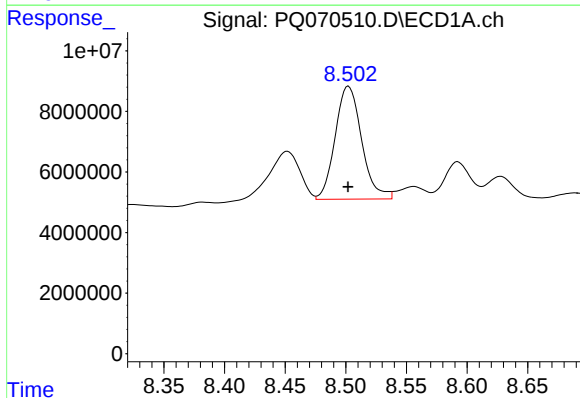

#2 Decachlorobiphenyl

R.T.: 8.502 min
Delta R.T.: 0.000 min
Response: 56606230
Conc: 13.75 ng/ml m

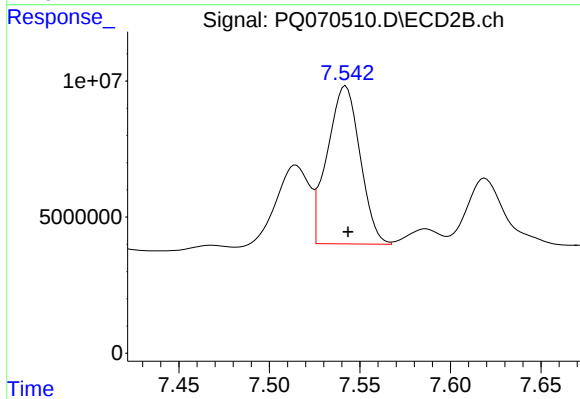

#2 Decachlorobiphenyl

R.T.: 7.542 min
Delta R.T.: -0.002 min
Response: 72148536
Conc: 9.95 ng/ml m