

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ070720\
 Data File : PQ048636.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2020 13:18
 Operator : DD\AJ
 Sample : L3217-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 E3-41-BOILER-ROOM

Manual Integrations
 APPROVED

Ankita
 7/8/2020 10:20:56 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 07 15:07:23 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ061720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 17 15:37:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.284	4.293	111.5E6	60878116	15.131	17.243
2) SA Decachlor...	11.539	9.651	222.5E6	114.8E6	22.996m	23.866m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ070720\
Data File : PQ048636.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jul 2020 13:18
Operator : DD\AJ
Sample : L3217-05
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
E3-41-BOILER-ROOM


Manual Integrations
APPROVED

Ankita
7/8/2020 10:20:56 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 07 15:07:23 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ061720.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 17 15:37:20 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

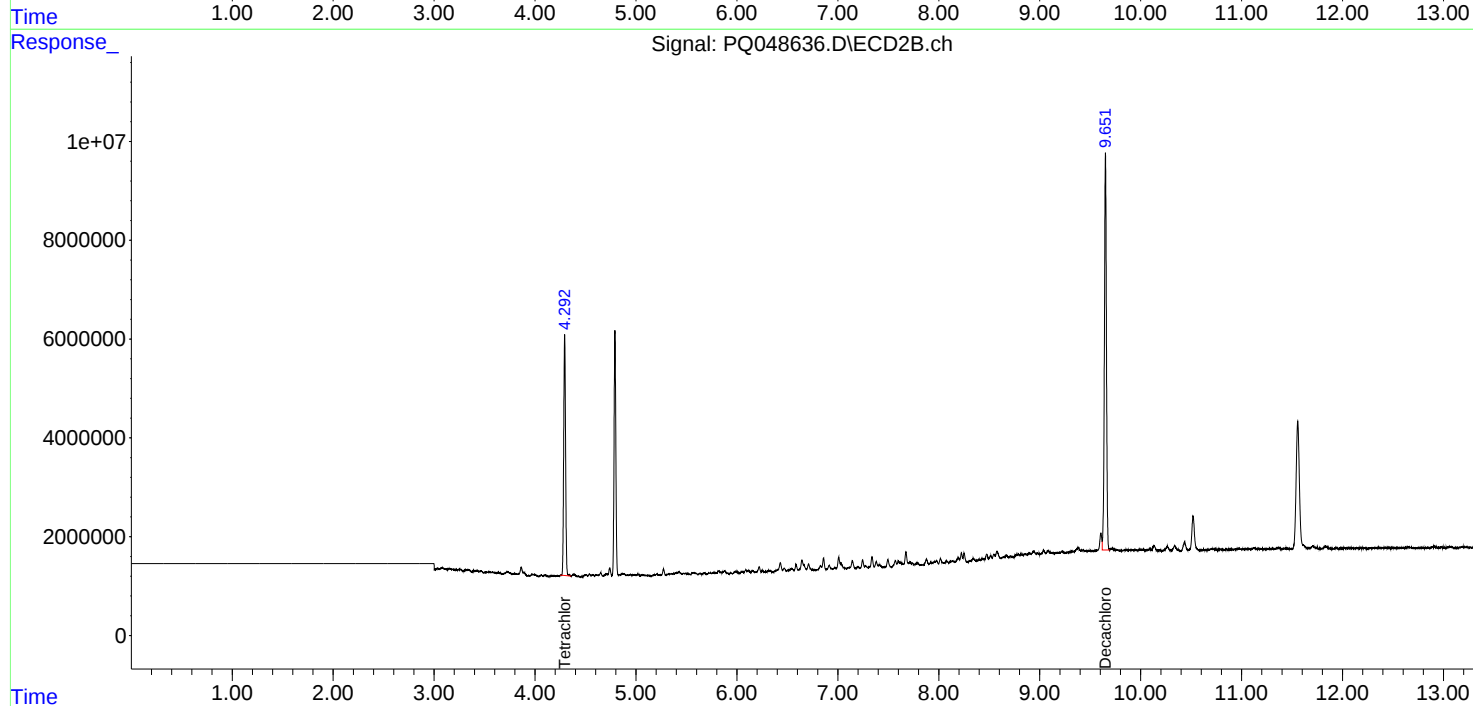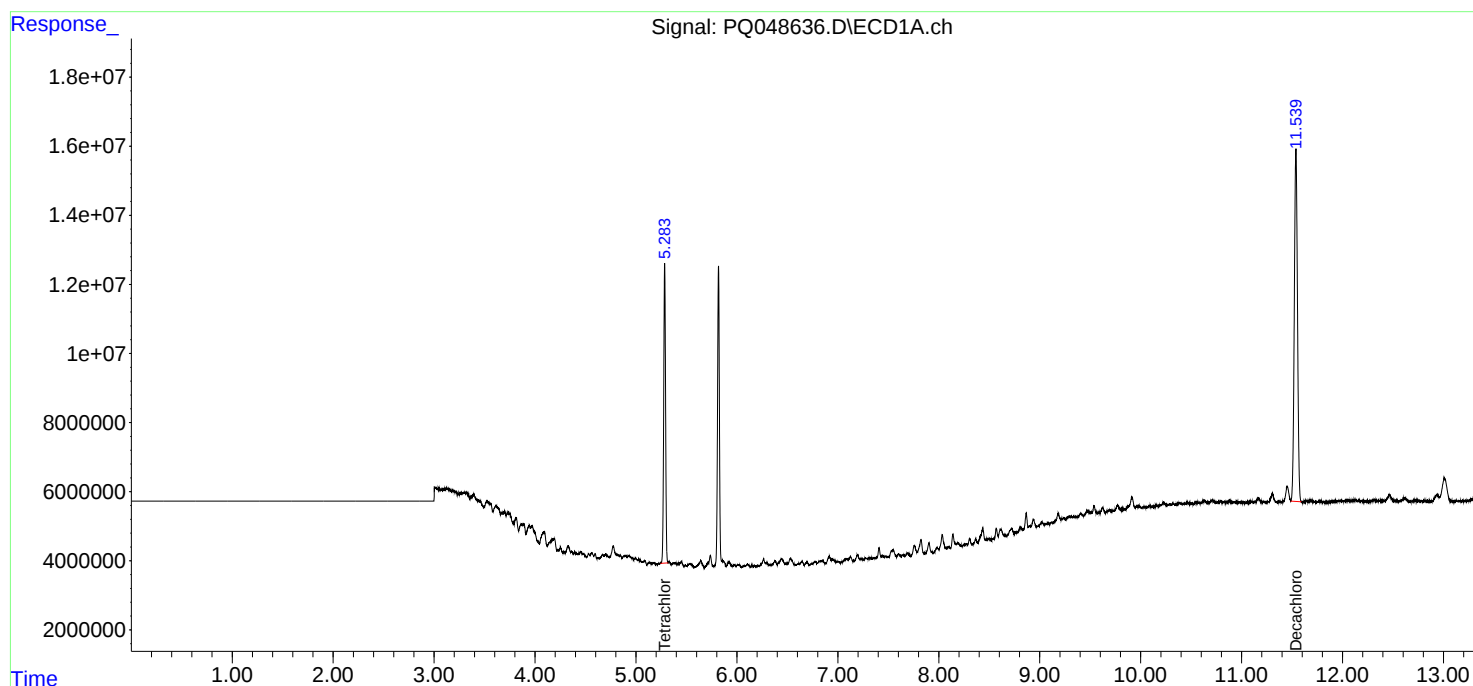

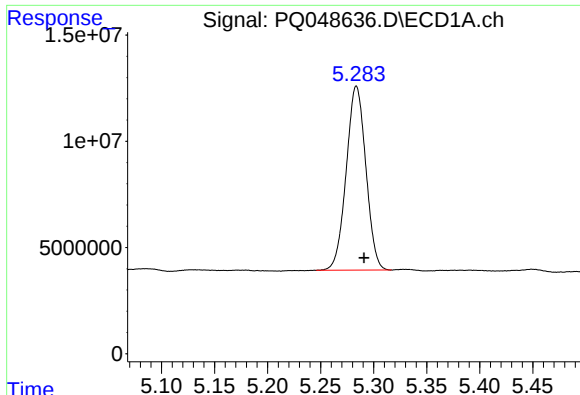


#1 Tetrachloro-m-xylene

R.T.: 5.284 min
Delta R.T.: -0.007 min
Response: 111537875
Conc: 15.13 ng/ml

Instrument :
ECD_Q
ClientSampleId :
E3-41-BOILER-ROOM


Manual Integrations
APPROVED

Ankita
7/8/2020 10:20:56 AM

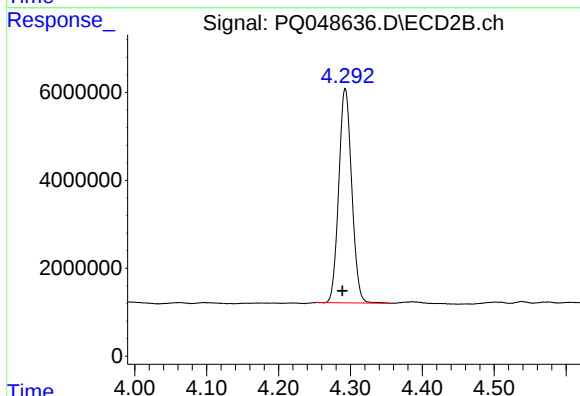


#1 Tetrachloro-m-xylene

R.T.: 4.293 min
Delta R.T.: 0.004 min
Response: 60878116
Conc: 17.24 ng/ml

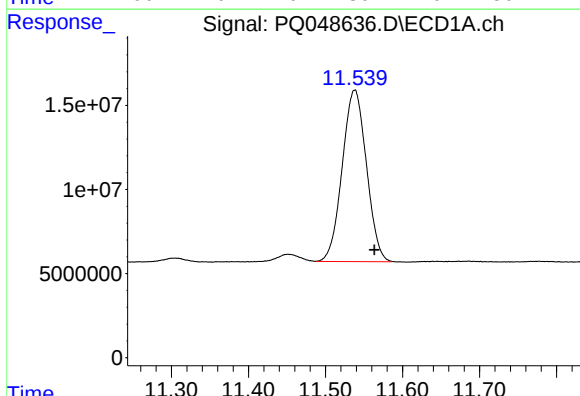

#2 Decachlorobiphenyl

R.T.: 11.539 min
Delta R.T.: -0.025 min
Response: 222509322
Conc: 23.00 ng/ml m

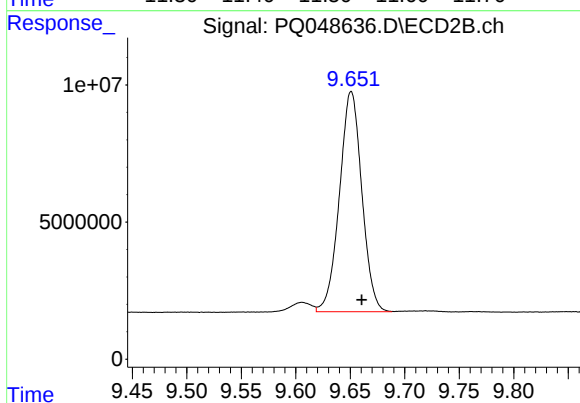

#2 Decachlorobiphenyl

R.T.: 9.651 min
Delta R.T.: -0.010 min
Response: 114849264
Conc: 23.87 ng/ml m