

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ071123\
 Data File : PQ062100.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jul 2023 13:47
 Operator : YP\AJ
 Sample : 03565-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 PAT-DIS-01-7-10-2023

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/12/2023
 Supervised By :Ankita Jodhani 07/12/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 11 21:36:23 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ070123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 04 05:32:27 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.403	2.757	80958978	56415772	16.596m	22.484 #
2) SA Decachlor...	8.585	7.528	60546240	43493435	16.667	13.053

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ071123\
Data File : PQ062100.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jul 2023 13:47
Operator : YP\AJ
Sample : 03565-01
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
PAT-DIS-01-7-10-2023


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/12/2023
Supervised By :Ankita Jodhani 07/12/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 11 21:36:23 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ070123.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 04 05:32:27 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

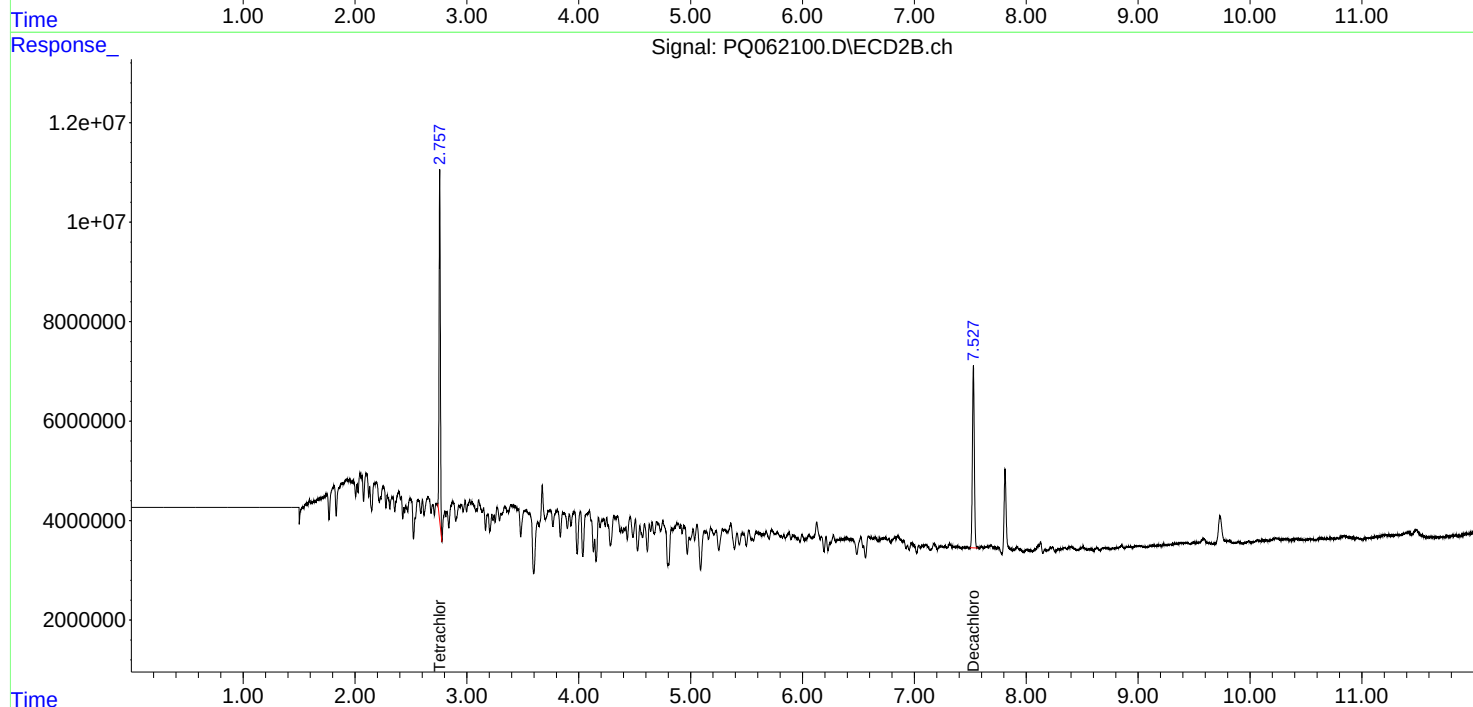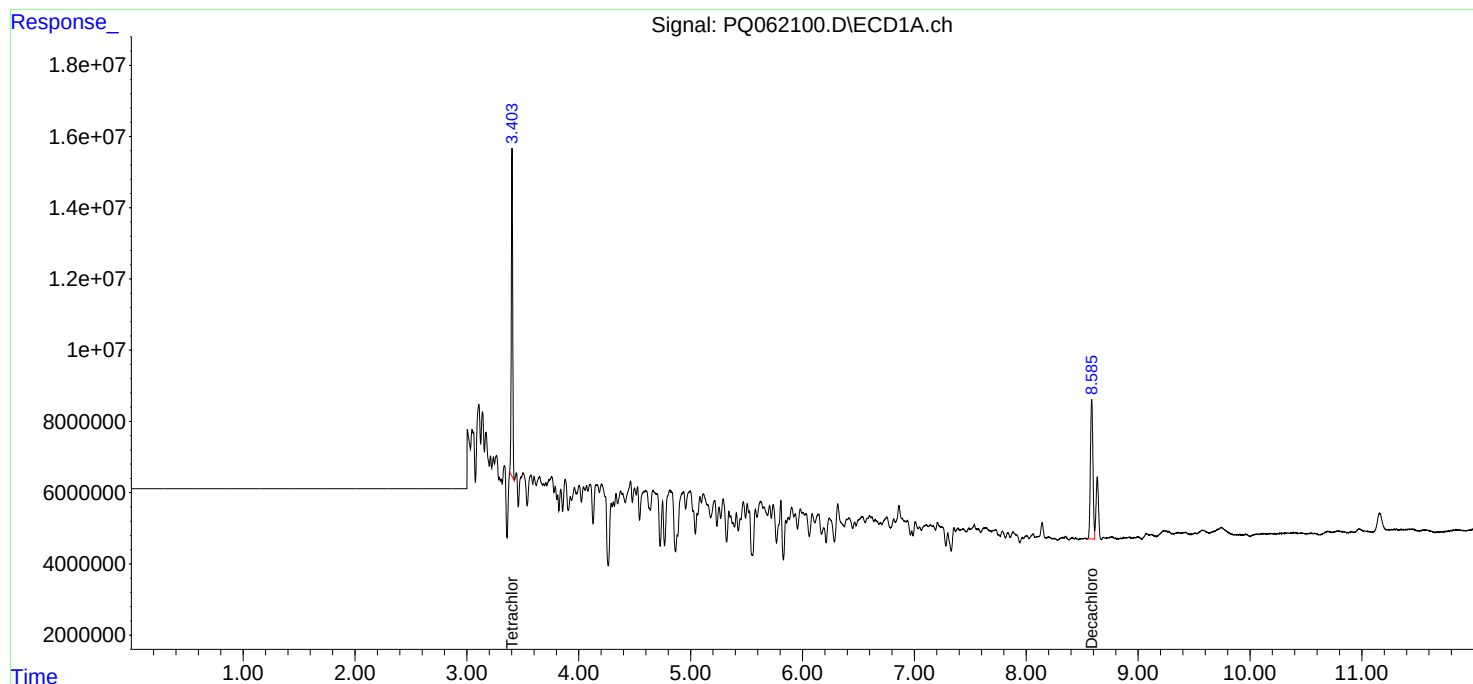

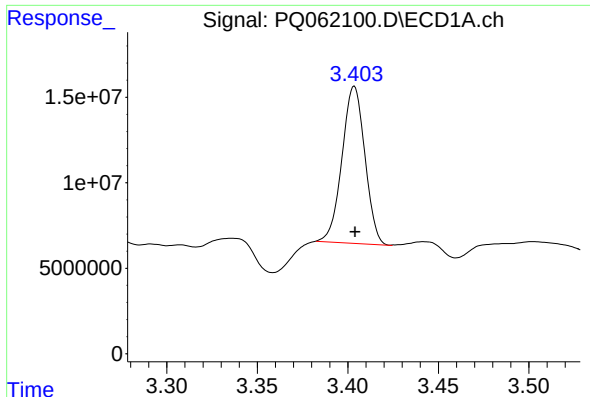

#1 Tetrachloro-m-xylene

R.T.: 3.403 min
Delta R.T.: 0.000 min
Response: 80958978
Conc: 16.60 ng/ml

Instrument :

ECD_Q


ClientSampleId :

PAT-DIS-01-7-10-2023

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 07/12/2023
Supervised By :Ankita Jodhani 07/12/2023

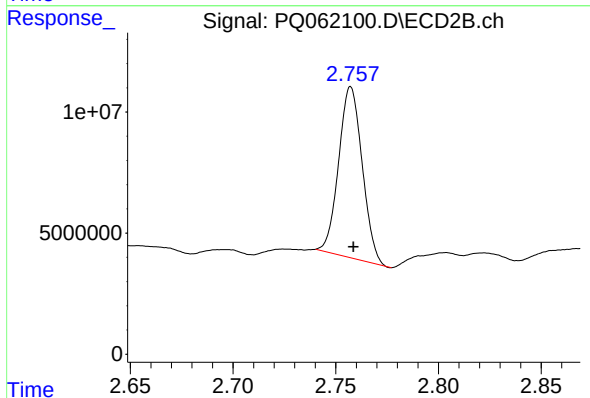


#1 Tetrachloro-m-xylene

R.T.: 2.757 min
Delta R.T.: -0.001 min
Response: 56415772
Conc: 22.48 ng/ml

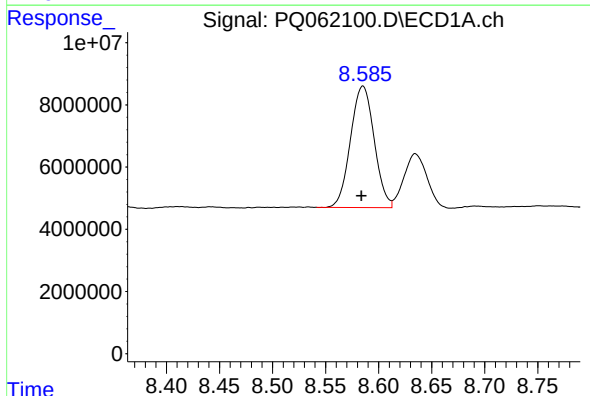

#2 Decachlorobiphenyl

R.T.: 8.585 min
Delta R.T.: 0.001 min
Response: 60546240
Conc: 16.67 ng/ml

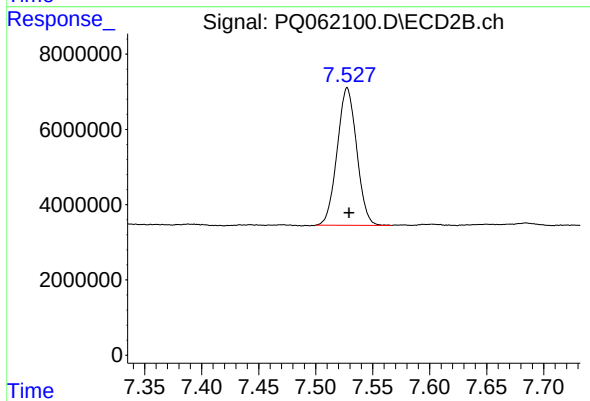

#2 Decachlorobiphenyl

R.T.: 7.528 min
Delta R.T.: -0.002 min
Response: 43493435
Conc: 13.05 ng/ml