

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ071123\
 Data File : PQ062104.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jul 2023 14:46
 Operator : YP\AJ
 Sample : 03570-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 EO-01-071023

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/12/2023
 Supervised By :Ankita Jodhani 07/12/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 11 21:41:34 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ070123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 04 05:32:27 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.403	2.758	75516211	46216662	15.480m	18.420
2) SA Decachlor...	8.585	7.528	48290499	35305921	13.293	10.595

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ071123\
Data File : PQ062104.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jul 2023 14:46
Operator : YP\AJ
Sample : 03570-03
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
EO-01-071023


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/12/2023
Supervised By :Ankita Jodhani 07/12/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 11 21:41:34 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ070123.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 04 05:32:27 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

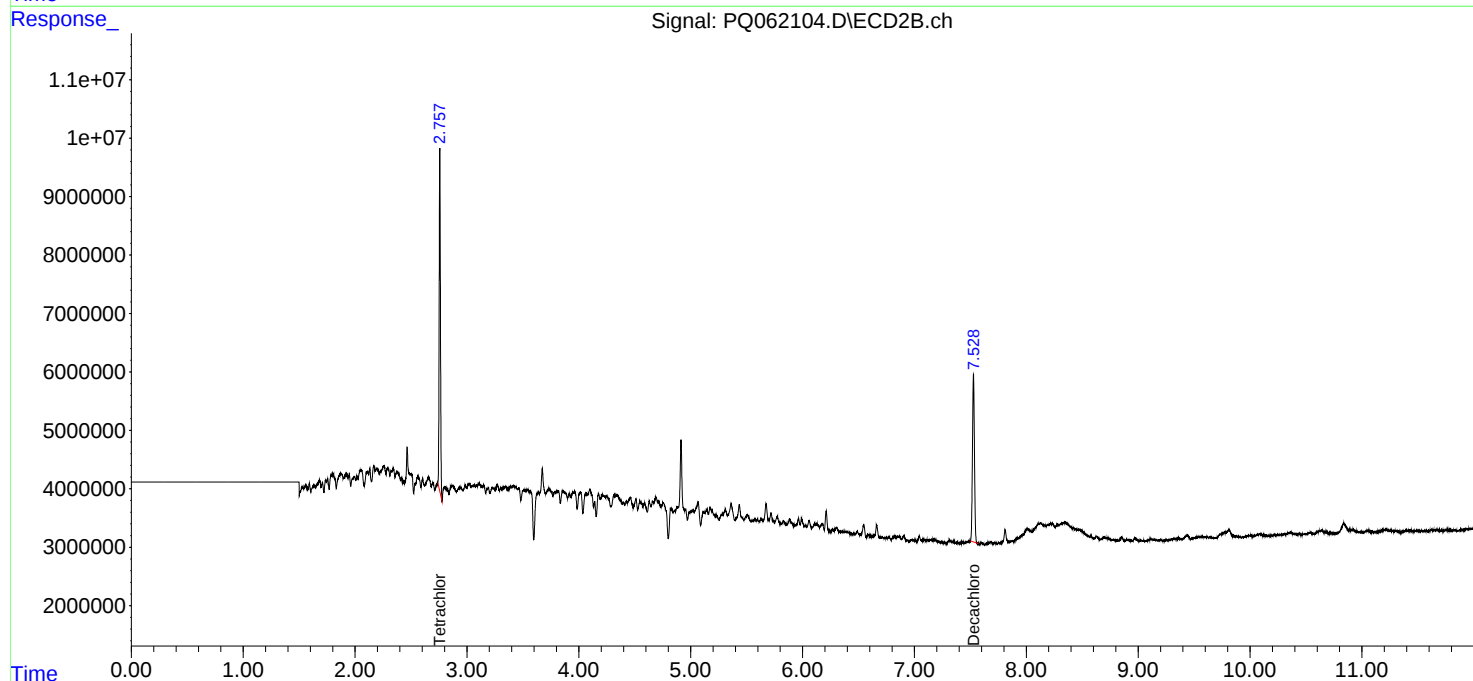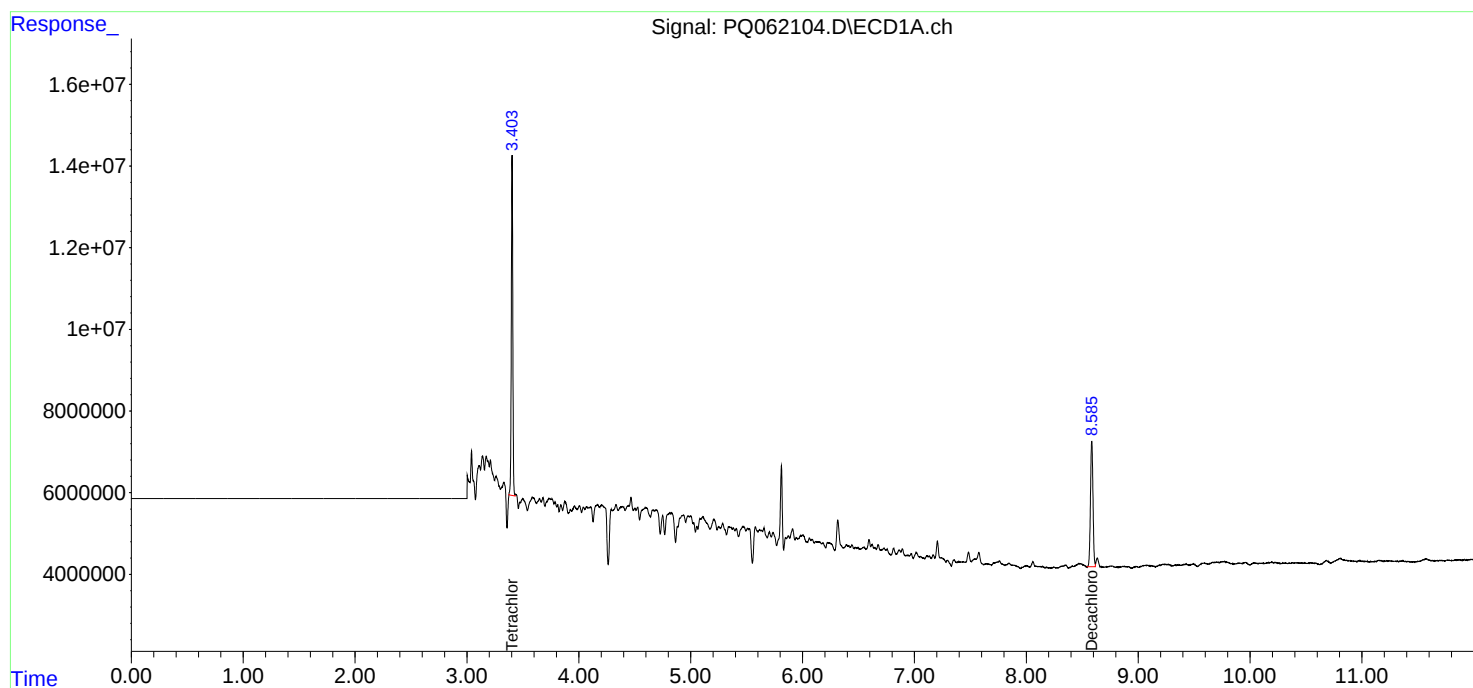

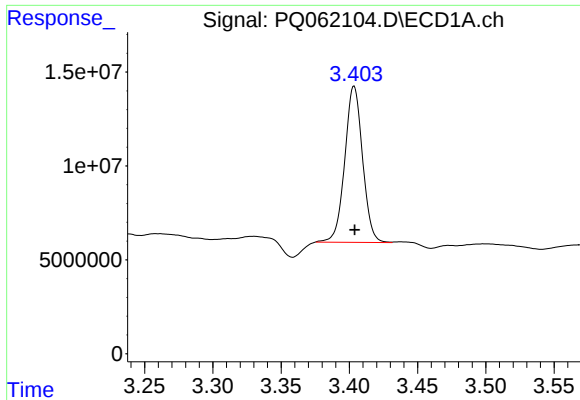


#1 Tetrachloro-m-xylene

R.T.: 3.403 min
Delta R.T.: 0.000 min
Response: 75516211
Conc: 15.48 ng/ml

Instrument :
ECD_Q
ClientSampleId :
EO-01-071023


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/12/2023
Supervised By :Ankita Jodhani 07/12/2023

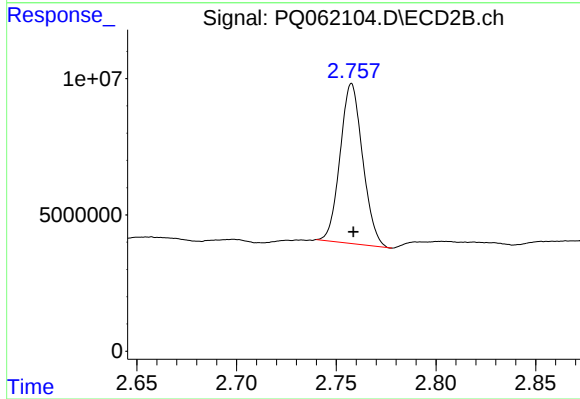


#1 Tetrachloro-m-xylene

R.T.: 2.758 min
Delta R.T.: 0.000 min
Response: 46216662
Conc: 18.42 ng/ml

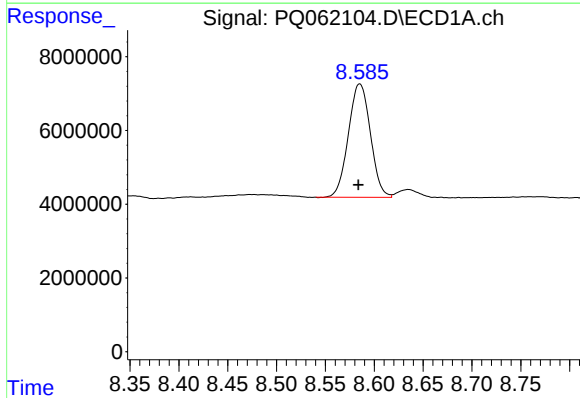

#2 Decachlorobiphenyl

R.T.: 8.585 min
Delta R.T.: 0.001 min
Response: 48290499
Conc: 13.29 ng/ml

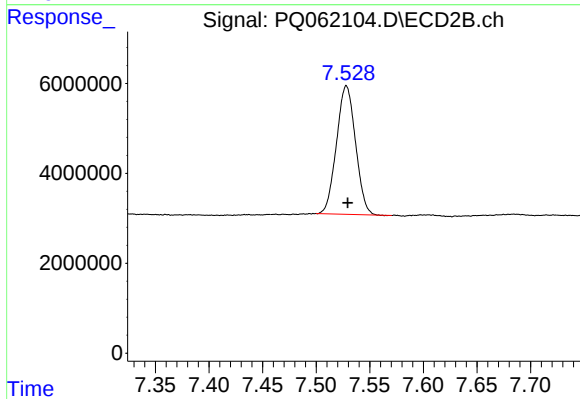

#2 Decachlorobiphenyl

R.T.: 7.528 min
Delta R.T.: -0.001 min
Response: 35305921
Conc: 10.60 ng/ml