

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ071224\
 Data File : PQ067302.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jul 2024 16:17
 Operator : YP\AJ
 Sample : P3223-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 PILE-CAP

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/15/2024
 Supervised By :Ankita Jodhani 07/15/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 13 00:06:56 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ062124.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 21 17:20:22 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.451	2.822	105.6E6	106.4E6	17.048m	17.601
2) SA Decachlor...	8.718	7.606	68353354	95856729	18.139m	15.858

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ071224\
Data File : PQ067302.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jul 2024 16:17
Operator : YP\AJ
Sample : P3223-01
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
PILE-CAP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/15/2024
Supervised By :Ankita Jodhani 07/15/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 13 00:06:56 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ062124.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 21 17:20:22 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

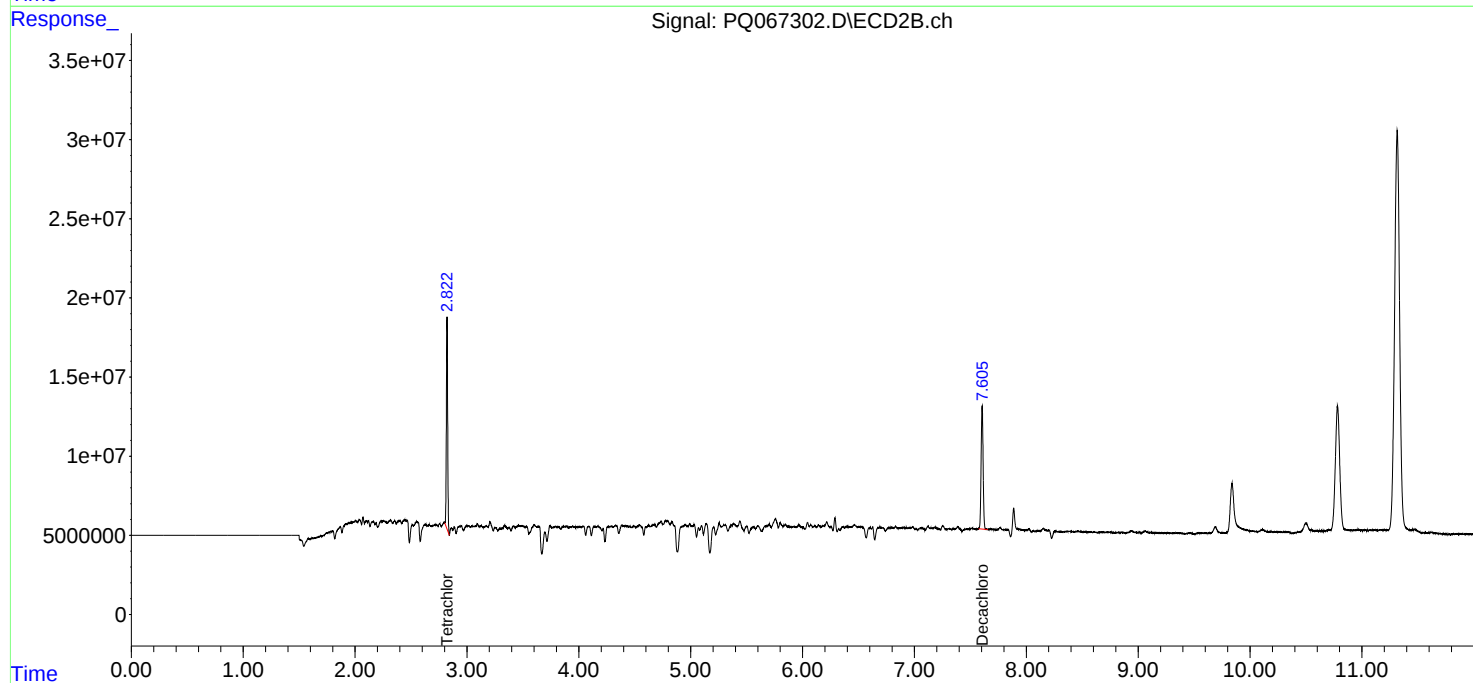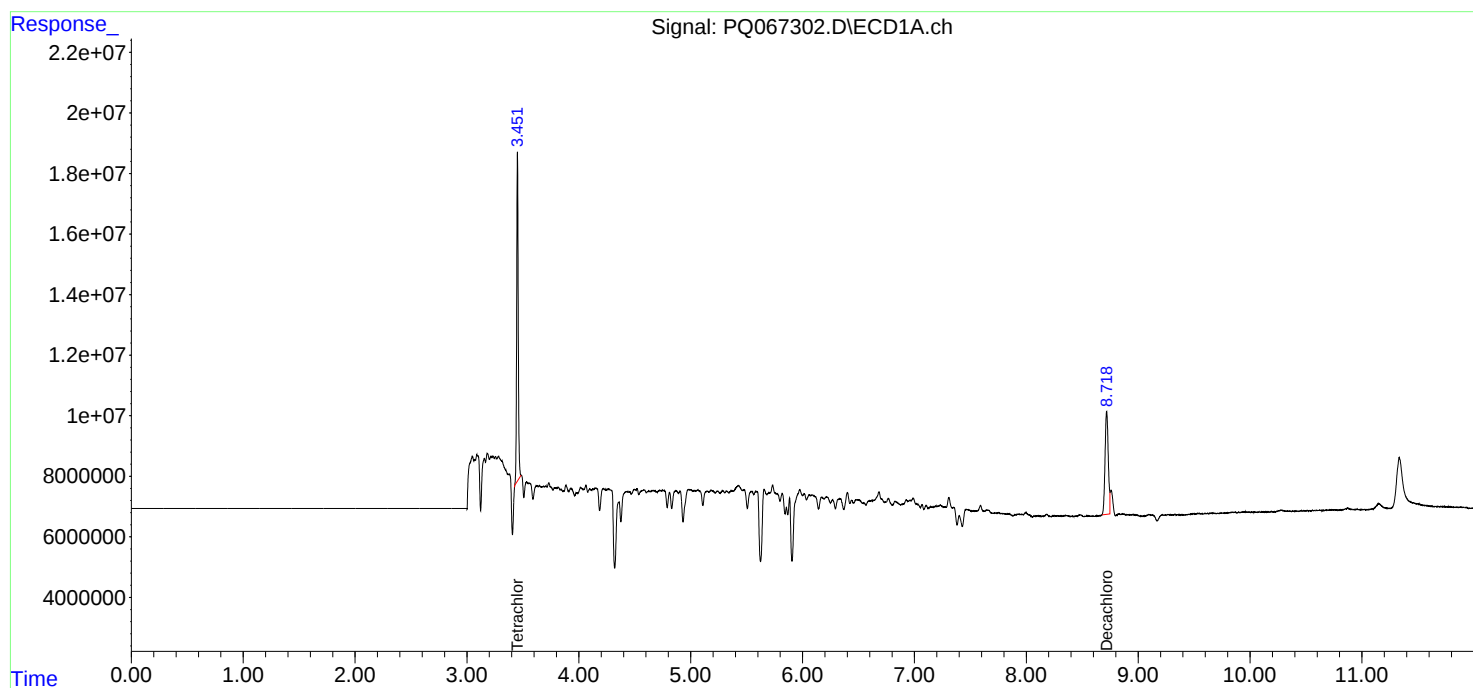

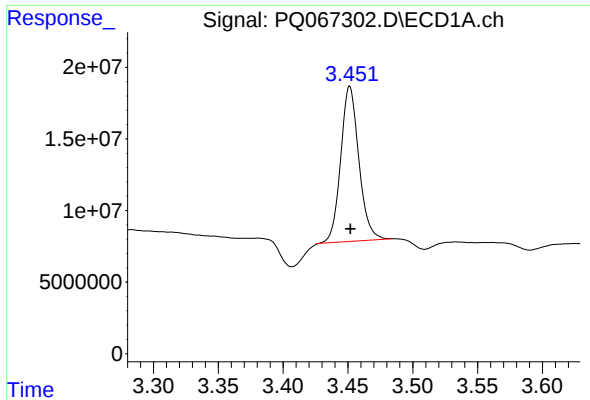


#1 Tetrachloro-m-xylene

R.T.: 3.451 min
Delta R.T.: -0.001 min
Response: 105617639
Conc: 17.05 ng/ml

Instrument :
ECD_Q
ClientSampleId :
PILE-CAP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/15/2024
Supervised By :Ankita Jodhani 07/15/2024

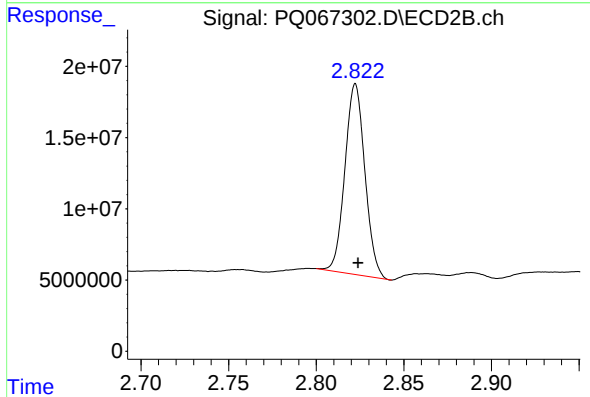


#1 Tetrachloro-m-xylene

R.T.: 2.822 min
Delta R.T.: -0.001 min
Response: 106410493
Conc: 17.60 ng/ml

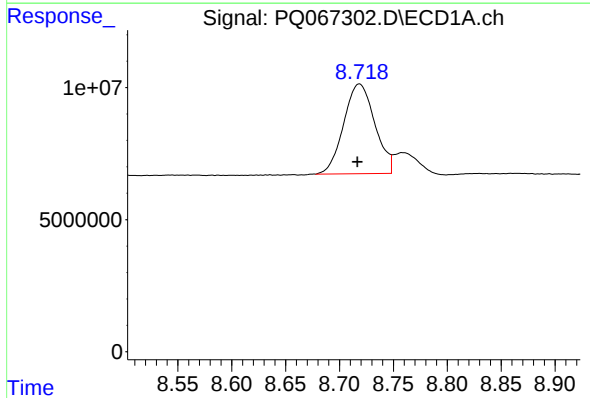

#2 Decachlorobiphenyl

R.T.: 8.718 min
Delta R.T.: 0.002 min
Response: 68353354
Conc: 18.14 ng/ml m

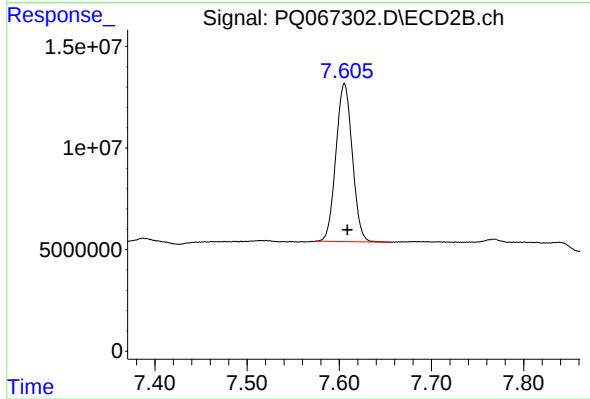

#2 Decachlorobiphenyl

R.T.: 7.606 min
Delta R.T.: -0.003 min
Response: 95856729
Conc: 15.86 ng/ml