

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ071224\
 Data File : PQ067319.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jul 2024 21:09
 Operator : YP\AJ
 Sample : P3227-01
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 EO-03-07112024

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/15/2024
 Supervised By :Ankita Jodhani 07/15/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 13 00:22:12 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ062124.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 21 17:20:22 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.452	2.822	80539650	76305274	13.000	12.622
2) SA Decachlor...	8.716	7.606	58036349	62742963	15.402m	10.380 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ071224\
Data File : PQ067319.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jul 2024 21:09
Operator : YP\AJ
Sample : P3227-01
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
EO-03-07112024


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/15/2024
Supervised By :Ankita Jodhani 07/15/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 13 00:22:12 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ062124.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 21 17:20:22 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

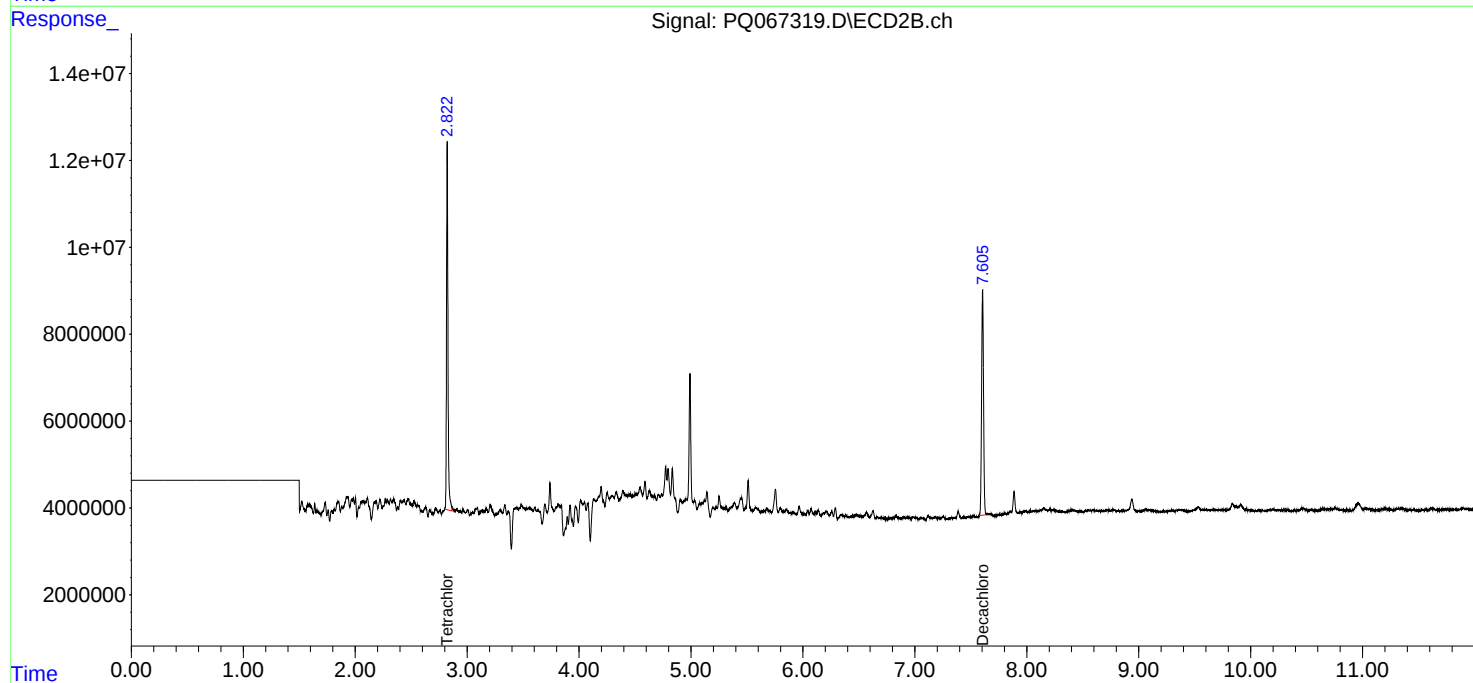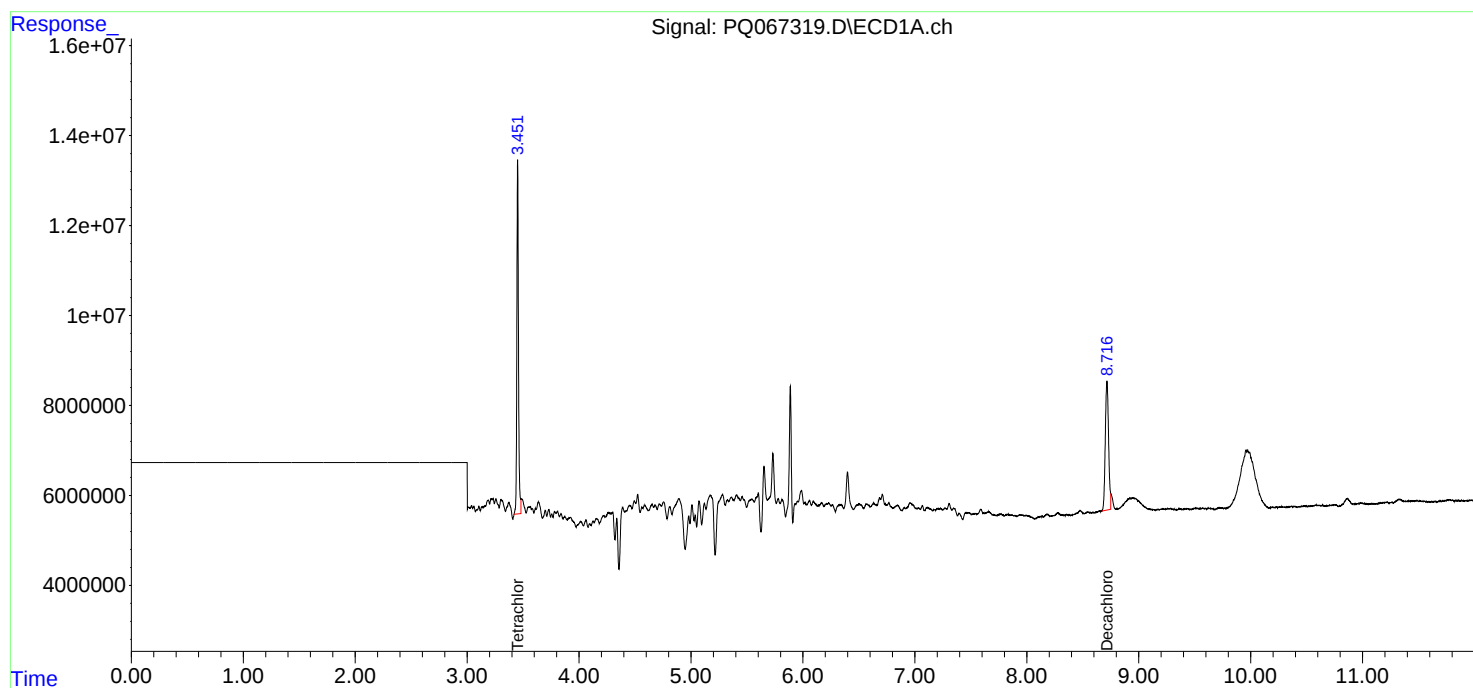

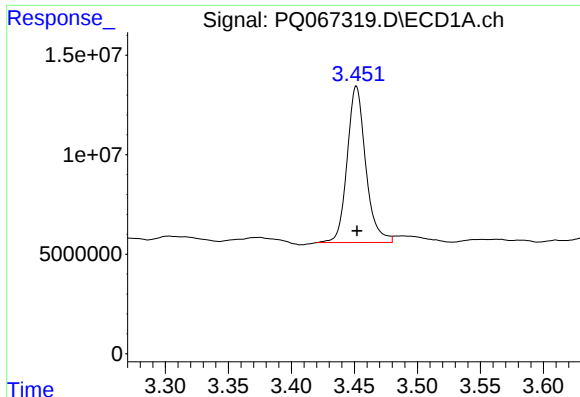


#1 Tetrachloro-m-xylene

R.T.: 3.452 min
Delta R.T.: 0.000 min
Response: 80539650
Conc: 13.00 ng/ml

Instrument :
ECD_Q
ClientSampleId :
EO-03-07112024


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/15/2024
Supervised By :Ankita Jodhani 07/15/2024

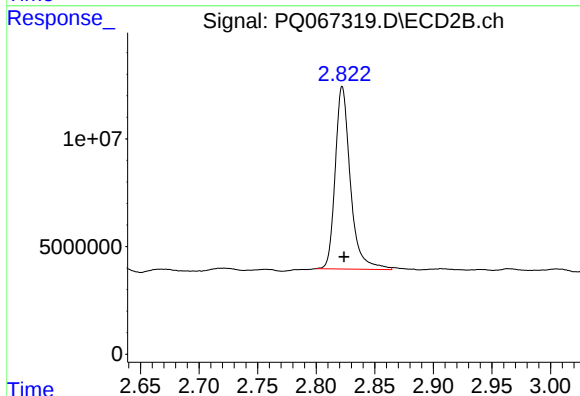


#1 Tetrachloro-m-xylene

R.T.: 2.822 min
Delta R.T.: -0.002 min
Response: 76305274
Conc: 12.62 ng/ml

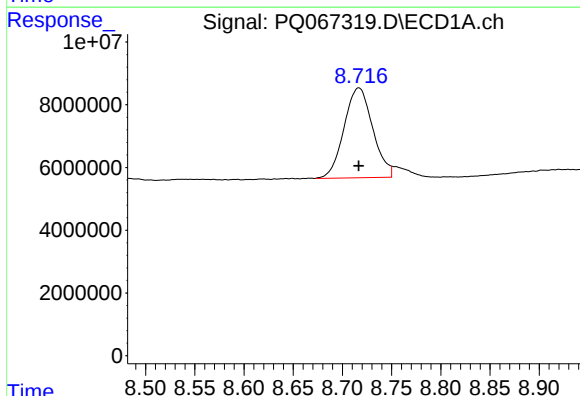

#2 Decachlorobiphenyl

R.T.: 8.716 min
Delta R.T.: 0.000 min
Response: 58036349
Conc: 15.40 ng/ml m

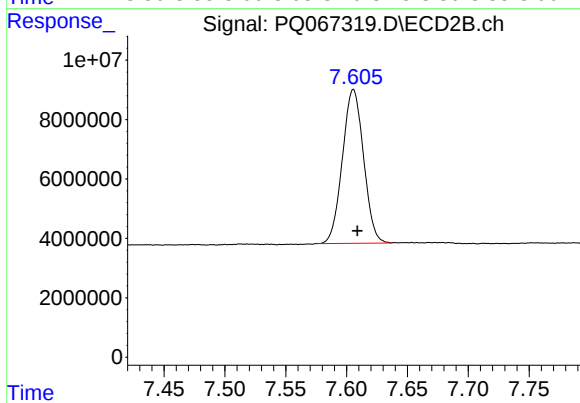

#2 Decachlorobiphenyl

R.T.: 7.606 min
Delta R.T.: -0.003 min
Response: 62742963
Conc: 10.38 ng/ml