

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ071618\
 Data File : PQ030724.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2018 04:30
 Operator : SM\SJ
 Sample : LOD-LOQ BL WATER
 Misc : 100PPB LOQ ECD-Q WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 LOD-LOQ BL WATER

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 07:47:37 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ071618.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 17 07:30:03 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.424	3.691	647.8E6	172.9E6	17.139	15.150
2) SA Decachlor...	10.094	8.650	659.7E6	359.4E6	18.143	16.967

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ071618\
Data File : PQ030724.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2018 04:30
Operator : SM\SJ
Sample : LOD-LOQ BL WATER
Misc : 100PPB LOQ ECD-Q WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
LOD-LOQ BL WATER

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 07:47:37 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ071618.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 17 07:30:03 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

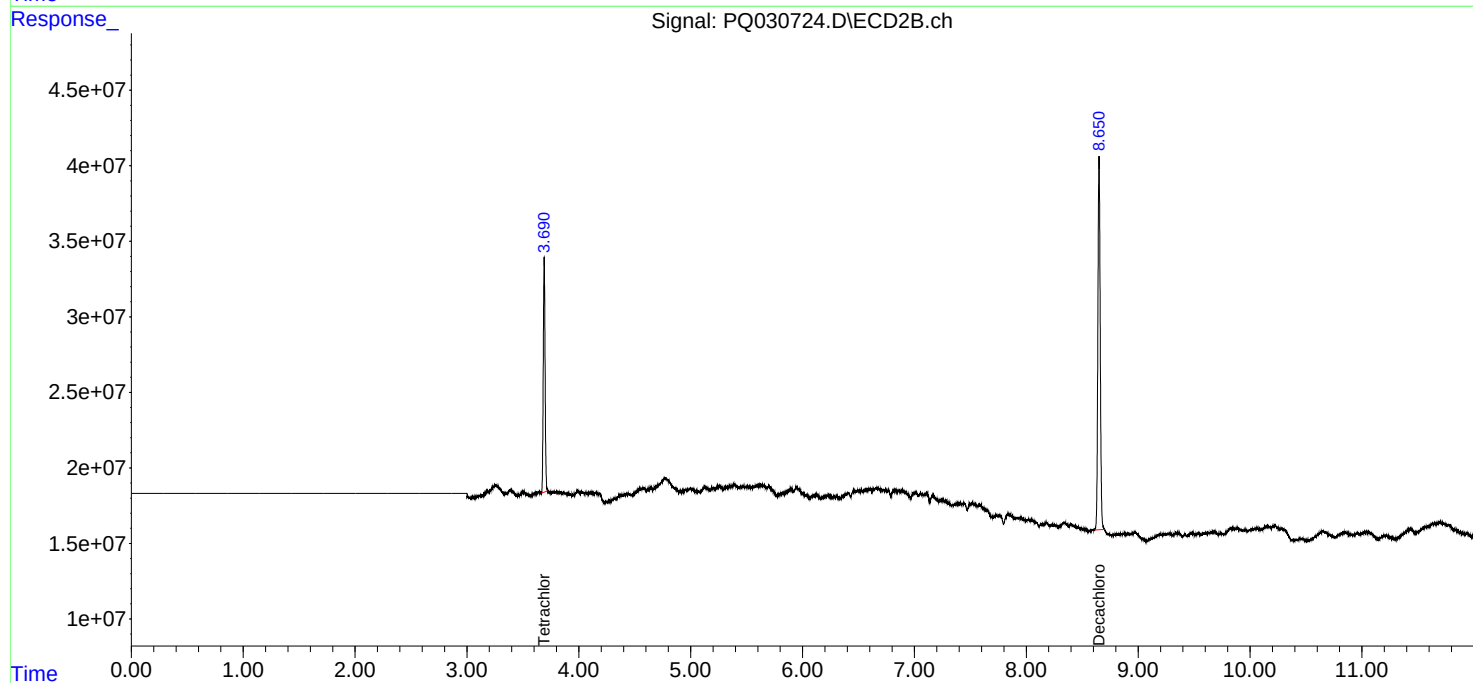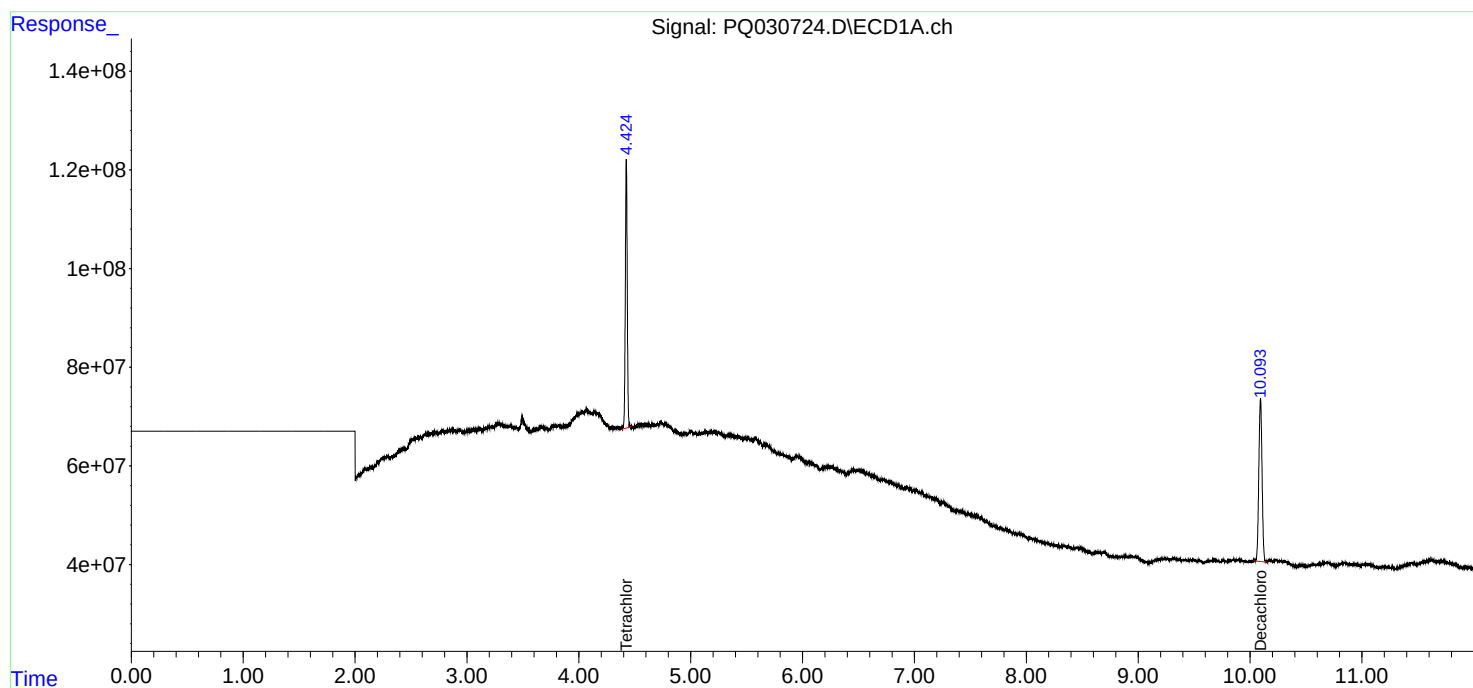


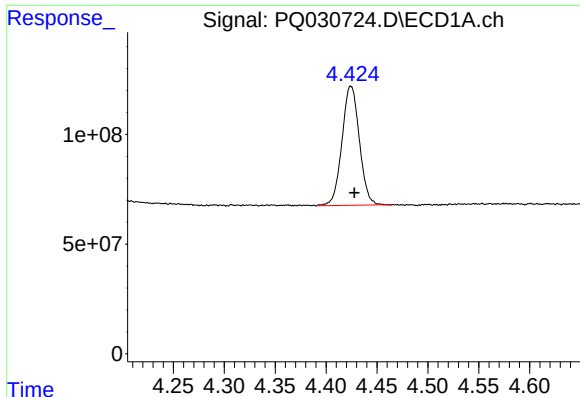

#1 Tetrachloro-m-xylene


R.T.: 4.424 min
Delta R.T.: -0.004 min
Response: 647769457
Conc: 17.14 ng/ml

Instrument :
ECD_Q
ClientSampleId :
LOD-LOQ BL WATER

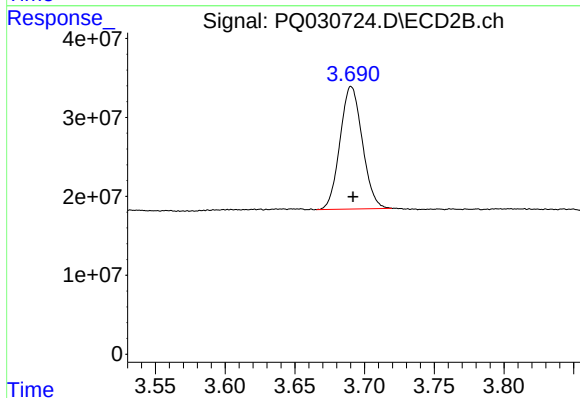


#1 Tetrachloro-m-xylene

R.T.: 3.691 min
Delta R.T.: -0.001 min
Response: 172933532
Conc: 15.15 ng/ml

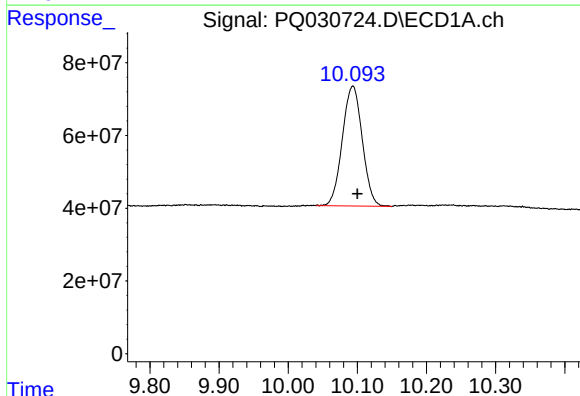

#2 Decachlorobiphenyl

R.T.: 10.094 min
Delta R.T.: -0.007 min
Response: 659715419
Conc: 18.14 ng/ml

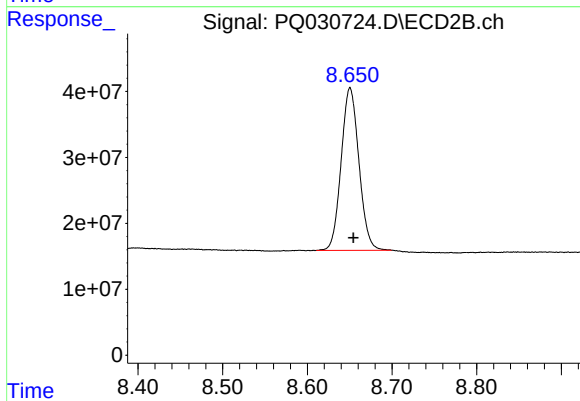

#2 Decachlorobiphenyl

R.T.: 8.650 min
Delta R.T.: -0.004 min
Response: 359411818
Conc: 16.97 ng/ml