

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ071624\
 Data File : PQ067381.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jul 2024 16:23
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/17/2024
 Supervised By :Ankita Jodhani 07/17/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 02:46:29 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ062124.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 21 17:20:22 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.452	2.822	140.7E6	126.1E6	22.718	20.862m
2) SA Decachlor...	8.721	7.608	89287086	124.6E6	23.695	20.609

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ071624\
Data File : PQ067381.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jul 2024 16:23
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/17/2024
Supervised By :Ankita Jodhani 07/17/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 02:46:29 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ062124.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 21 17:20:22 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

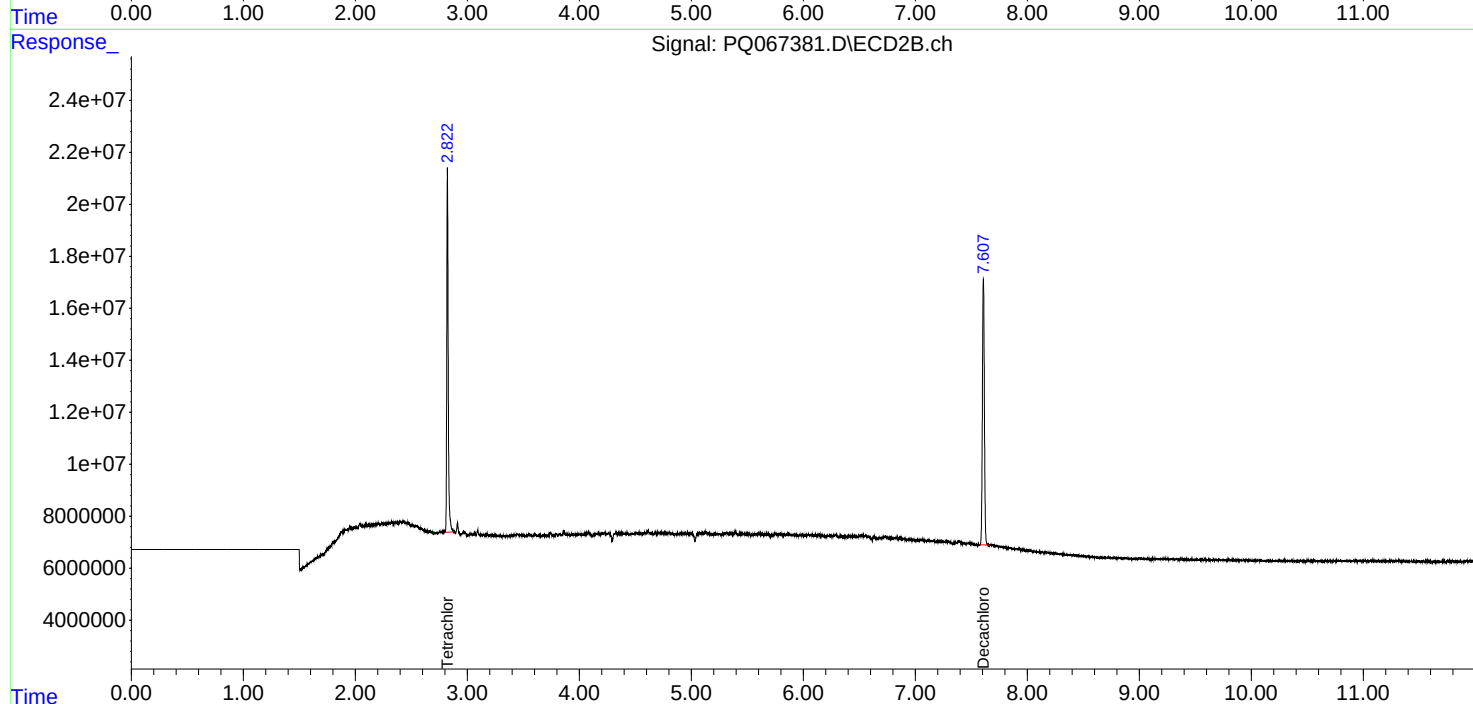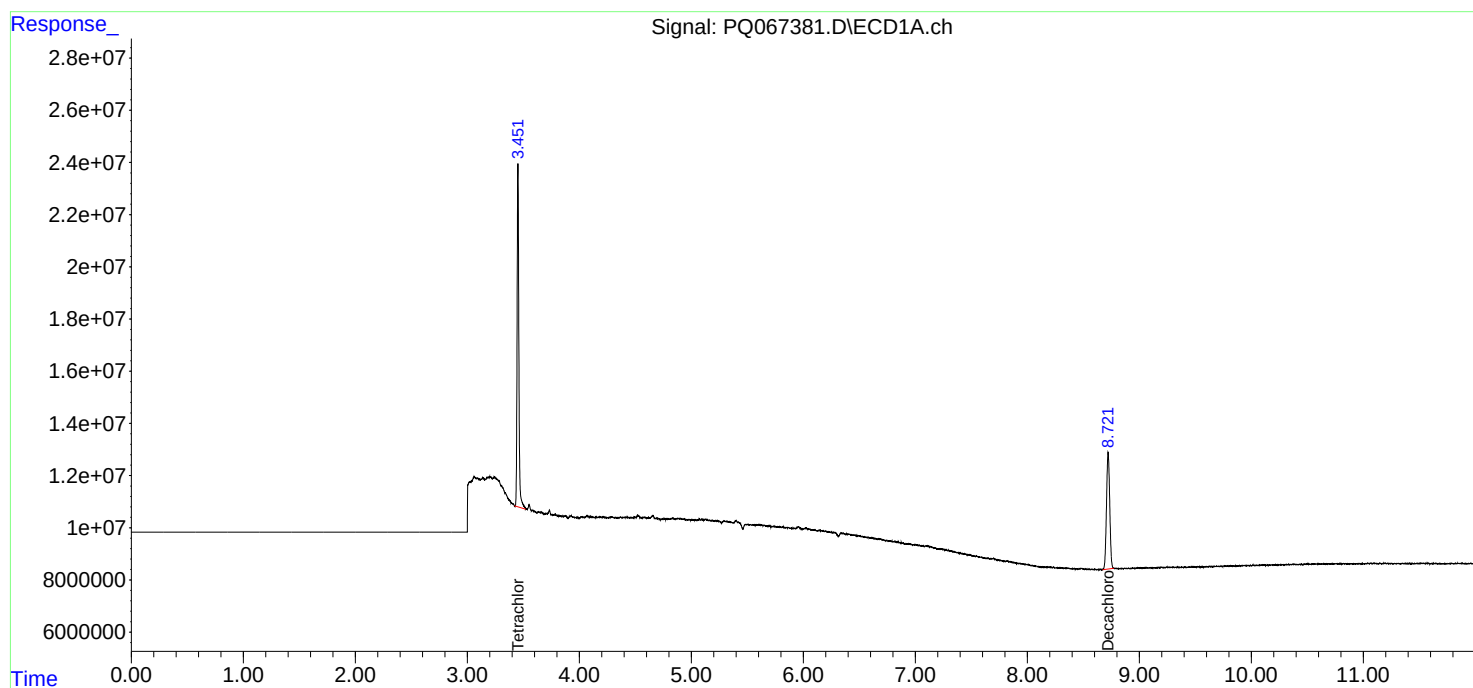

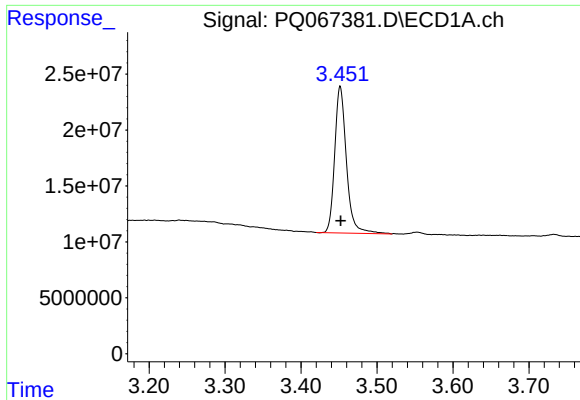


#1 Tetrachloro-m-xylene

R.T.: 3.452 min
Delta R.T.: 0.000 min
Response: 140743526
Conc: 22.72 ng/ml

Instrument :
ECD_Q
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/17/2024
Supervised By :Ankita Jodhani 07/17/2024

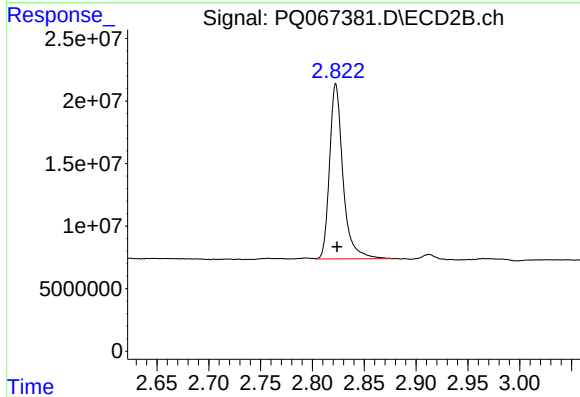


#1 Tetrachloro-m-xylene

R.T.: 2.822 min
Delta R.T.: -0.002 min
Response: 126126799
Conc: 20.86 ng/ml m

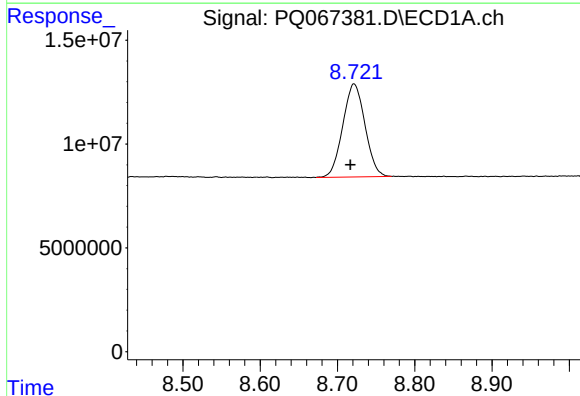

#2 Decachlorobiphenyl

R.T.: 8.721 min
Delta R.T.: 0.005 min
Response: 89287086
Conc: 23.69 ng/ml

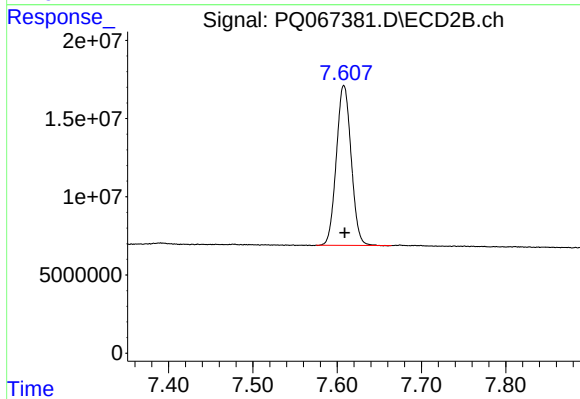

#2 Decachlorobiphenyl

R.T.: 7.608 min
Delta R.T.: 0.000 min
Response: 124572598
Conc: 20.61 ng/ml