

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ071723\
 Data File : PQ062281.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2023 15:00
 Operator : YP\AJ
 Sample : 03633-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 SS-01-COMP

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/18/2023
 Supervised By :Ankita Jodhani 07/18/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 02:18:12 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ070123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 04 05:32:27 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.404	2.758	53065526	38996389	10.878	15.542m#
2) SA Decachlor...	8.589	7.529	36484609	34867731	10.043m	10.464m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ071723\
Data File : PQ062281.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2023 15:00
Operator : YP\AJ
Sample : 03633-02
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
SS-01-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/18/2023
Supervised By :Ankita Jodhani 07/18/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 02:18:12 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ070123.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 04 05:32:27 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

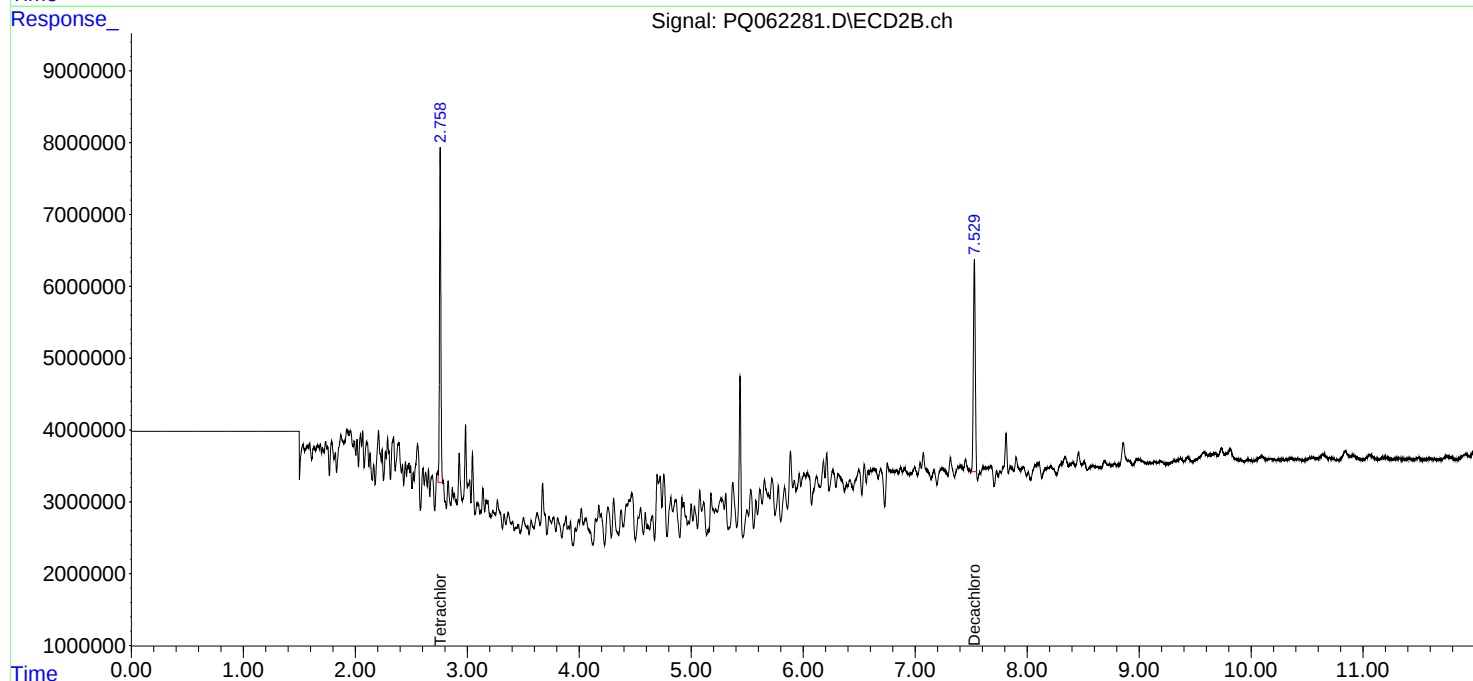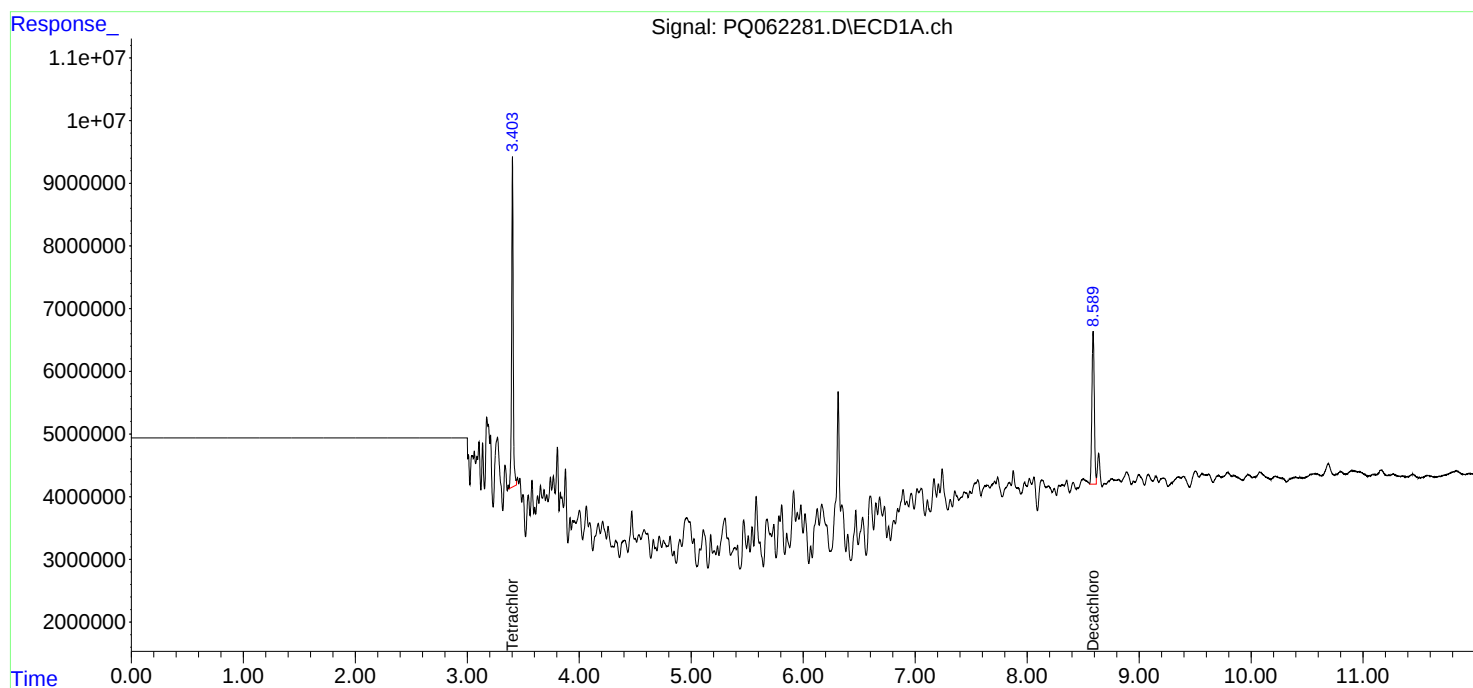

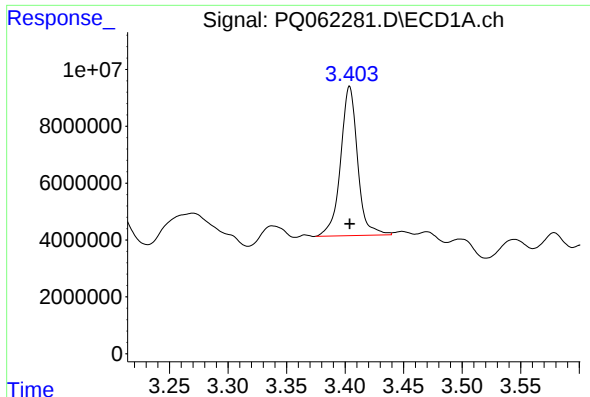


#1 Tetrachloro-m-xylene

R.T.: 3.404 min
Delta R.T.: 0.000 min
Response: 53065526
Conc: 10.88 ng/ml

Instrument :
ECD_Q
ClientSampleId :
SS-01-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/18/2023
Supervised By :Ankita Jodhani 07/18/2023

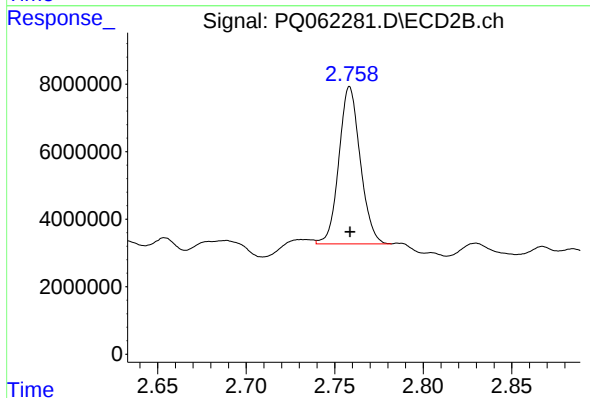


#1 Tetrachloro-m-xylene

R.T.: 2.758 min
Delta R.T.: 0.000 min
Response: 38996389
Conc: 15.54 ng/ml m

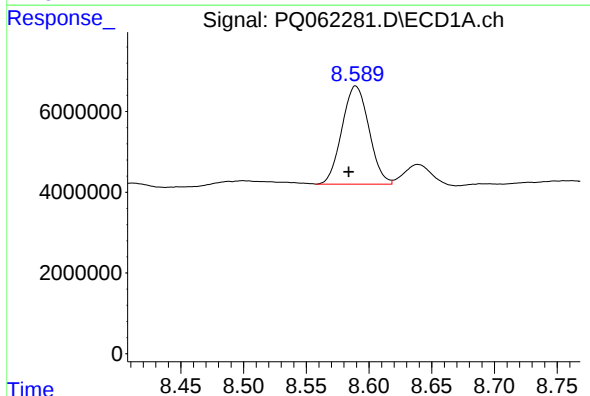

#2 Decachlorobiphenyl

R.T.: 8.589 min
Delta R.T.: 0.005 min
Response: 36484609
Conc: 10.04 ng/ml m

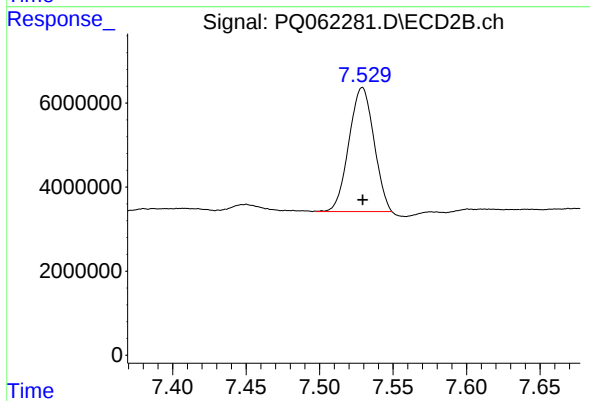

#2 Decachlorobiphenyl

R.T.: 7.529 min
Delta R.T.: 0.000 min
Response: 34867731
Conc: 10.46 ng/ml m