

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ071818\
 Data File : PQ030731.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jul 2018 17:16
 Operator : SM\SJ
 Sample : J4006-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 RR-BASELINE-WATER

Manual Integrations
 APPROVED

Sohil
 7/19/2018 11:15:39 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 01:39:32 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ071618.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 17 07:30:03 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.433	3.690	238.5E6	80031415	6.310m	7.011
2) SA Decachlor...	10.113	8.659	166.1E6	78156713	4.569	3.690

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ071818\
Data File : PQ030731.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jul 2018 17:16
Operator : SM\SJ
Sample : J4006-01
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
RR-BASELINE-WATER


Manual Integrations
APPROVED

Sohil
7/19/2018 11:15:39 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 01:39:32 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ071618.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 17 07:30:03 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

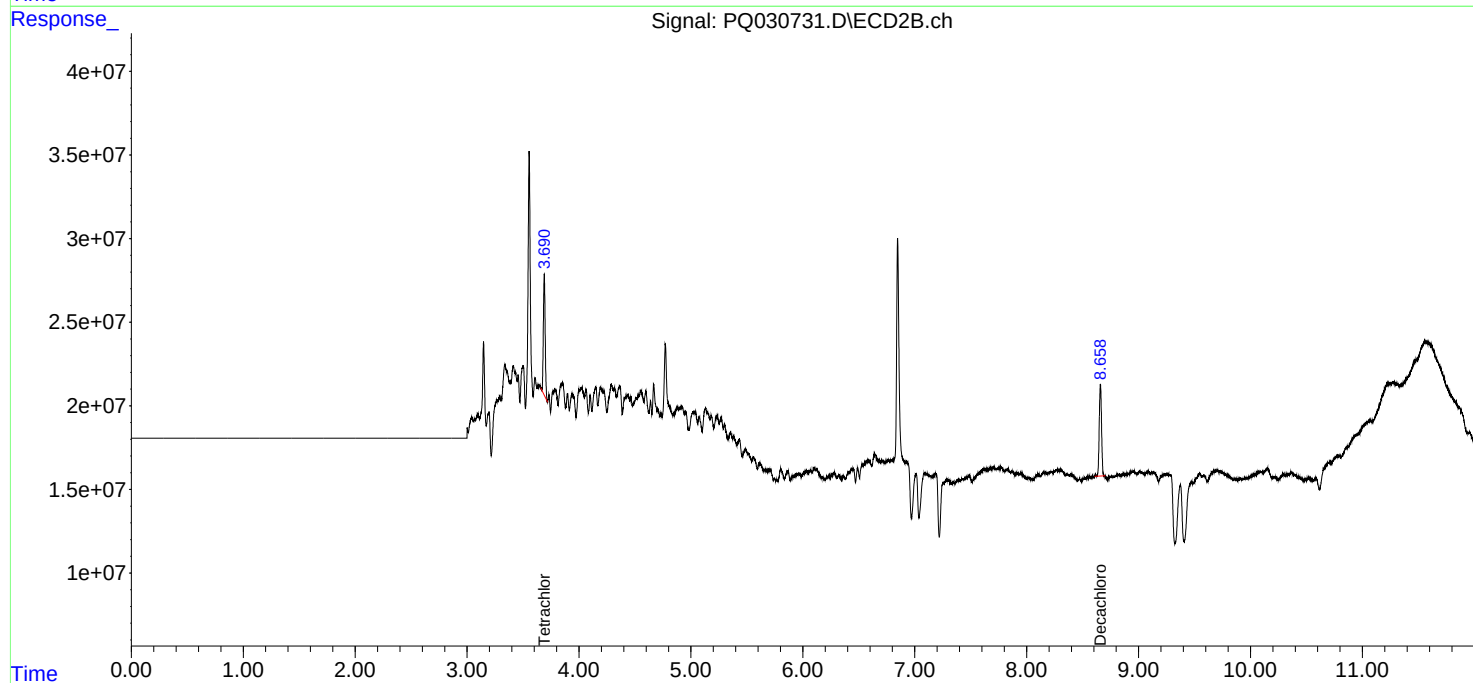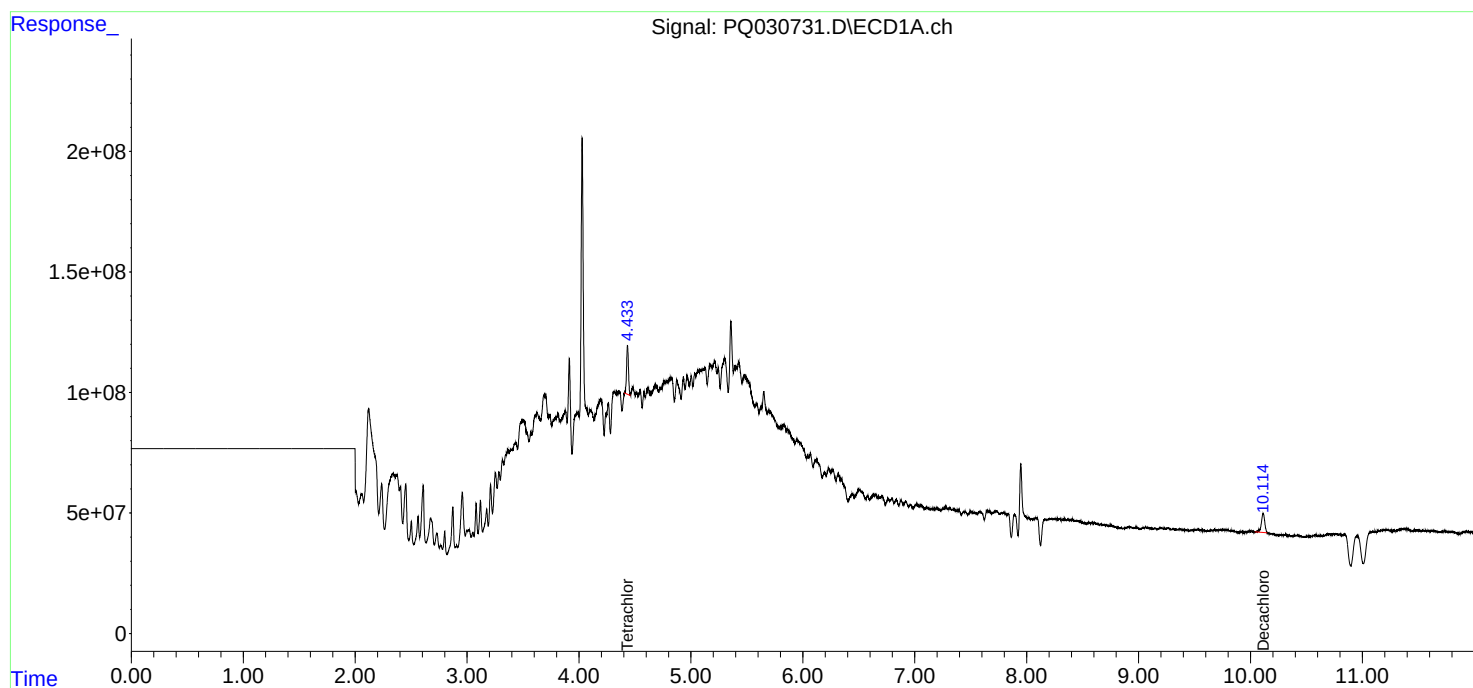

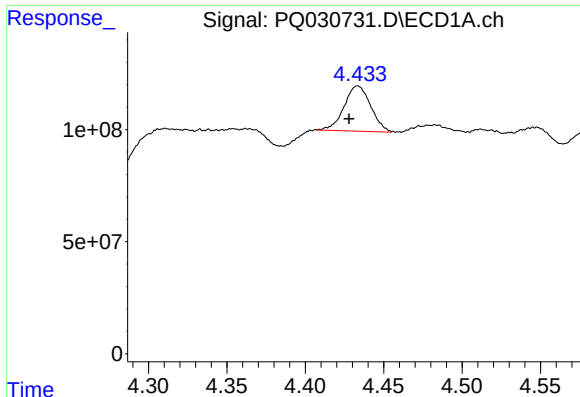


#1 Tetrachloro-m-xylene

R.T.: 4.433 min
Delta R.T.: 0.005 min
Response: 238471116
Conc: 6.31 ng/ml m

Instrument :
ECD_Q
ClientSampleId :
RR-BASELINE-WATER


Manual Integrations
APPROVED

Sohil
7/19/2018 11:15:39 AM

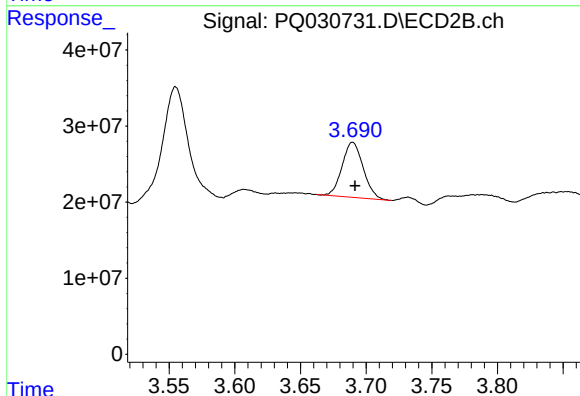


#1 Tetrachloro-m-xylene

R.T.: 3.690 min
Delta R.T.: -0.002 min
Response: 80031415
Conc: 7.01 ng/ml

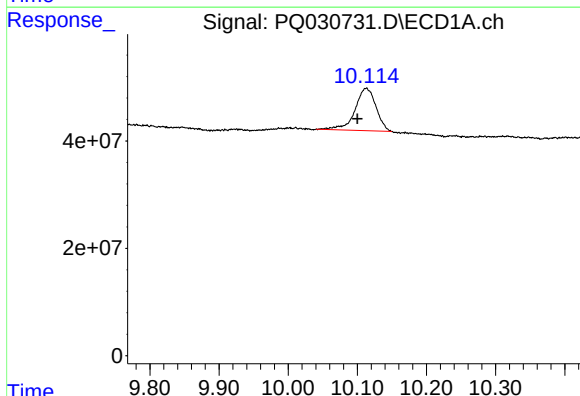

#2 Decachlorobiphenyl

R.T.: 10.113 min
Delta R.T.: 0.012 min
Response: 166143613
Conc: 4.57 ng/ml

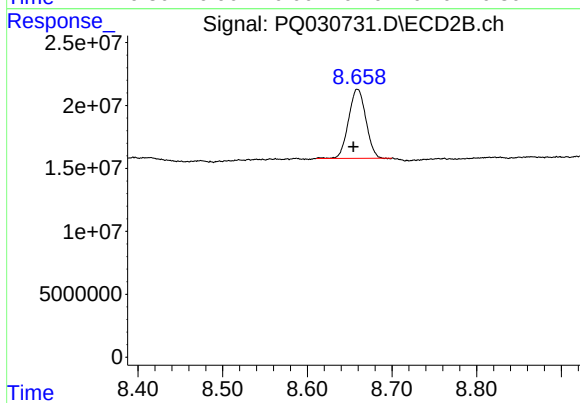

#2 Decachlorobiphenyl

R.T.: 8.659 min
Delta R.T.: 0.005 min
Response: 78156713
Conc: 3.69 ng/ml