

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ071819\
 Data File : PQ041292.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jul 2019 11:25
 Operator : SM\AJ
 Sample : K3627-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 TR-04-071519

Manual Integrations
 APPROVED

Ankita
 7/19/2019 11:06:35 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 12:38:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ071719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 18 01:40:31 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.709	4.765	115.8E6	87834486	27.683m	26.866m
2)	SA Decachlor...	12.126	10.538	175.1E6	60415904	20.763	18.335

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ071819\
Data File : PQ041292.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jul 2019 11:25
Operator : SM\AJ
Sample : K3627-03
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampled :
TR-04-071519


Manual Integrations
APPROVED

Ankita
7/19/2019 11:06:35 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 12:38:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ071719.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 18 01:40:31 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

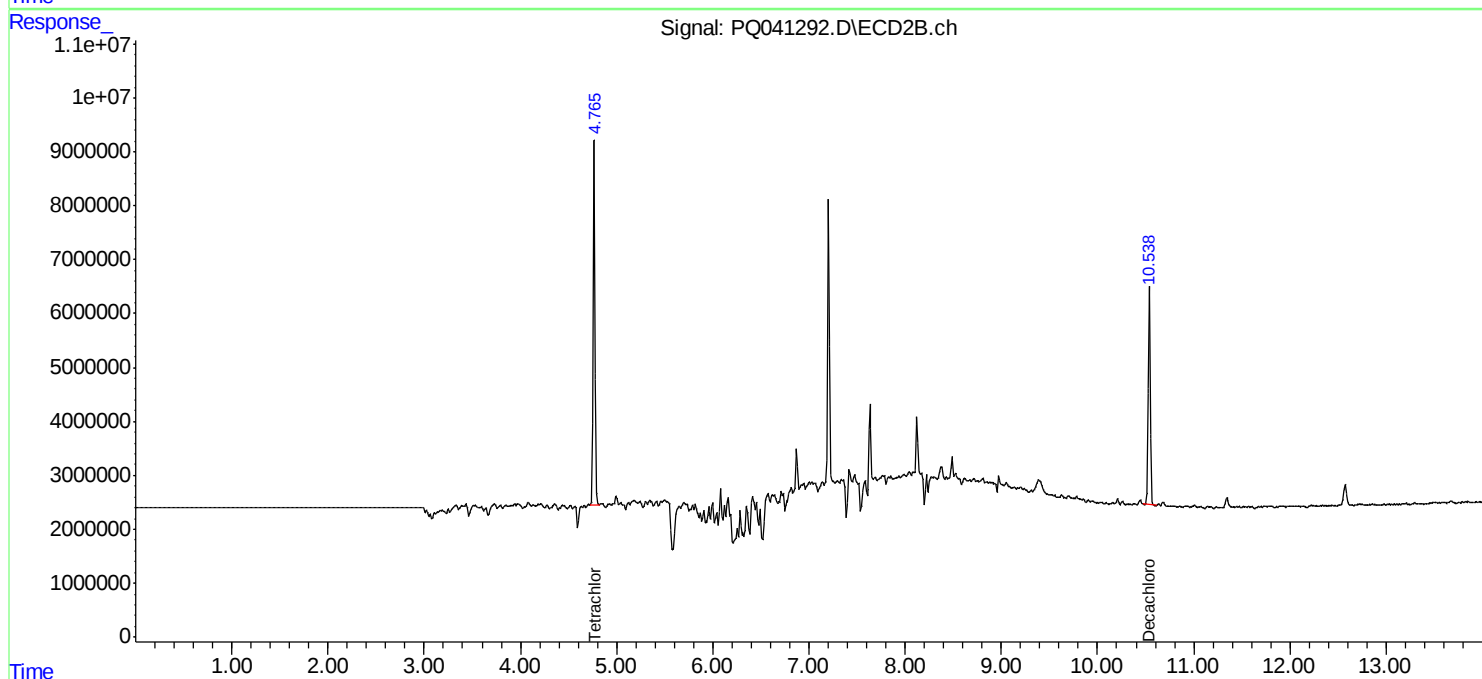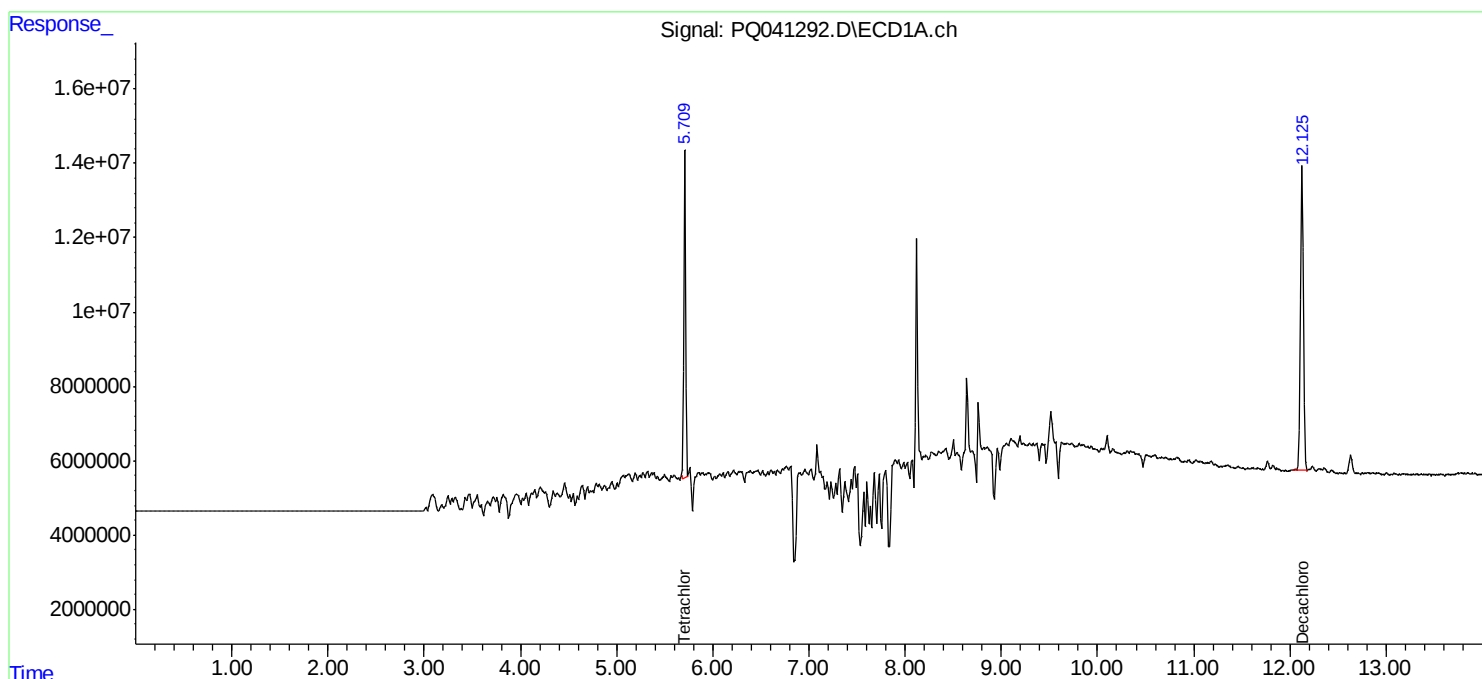

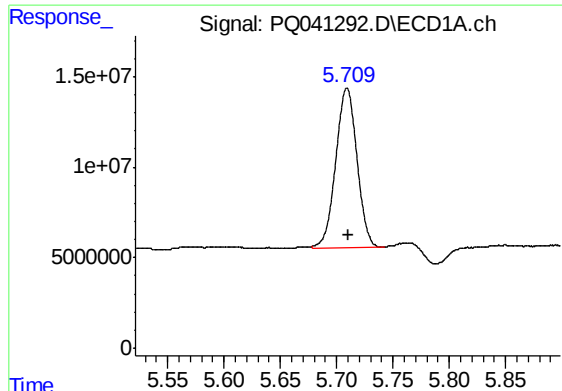


#1 Tetrachloro-m-xylene

R.T.: 5.709 min
Delta R.T.: -0.002 min
Response: 115792443
Conc: 27.68 ng/ml m

Instrument :
ECD_Q
ClientSampleId :
TR-04-071519


Manual Integrations
APPROVED

Ankita
7/19/2019 11:06:35 AM

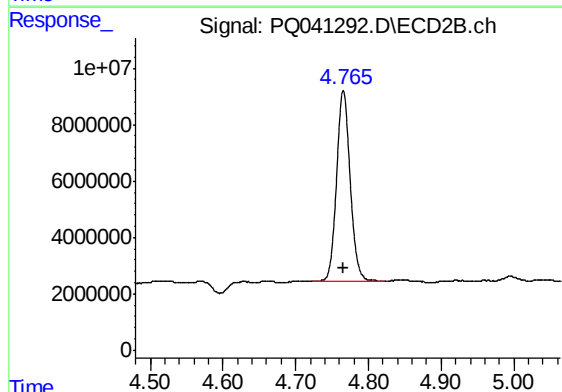


#1 Tetrachloro-m-xylene

R.T.: 4.765 min
Delta R.T.: 0.000 min
Response: 87834486
Conc: 26.87 ng/ml m

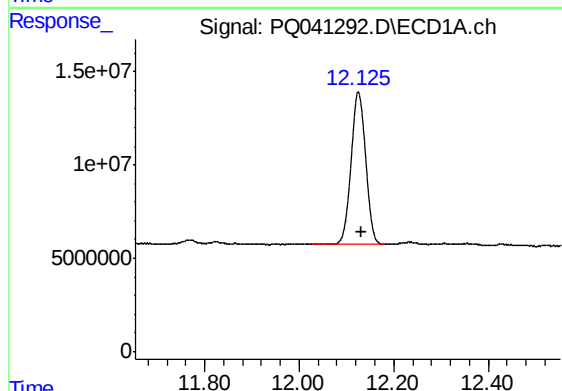

#2 Decachlorobiphenyl

R.T.: 12.126 min
Delta R.T.: -0.007 min
Response: 175063106
Conc: 20.76 ng/ml

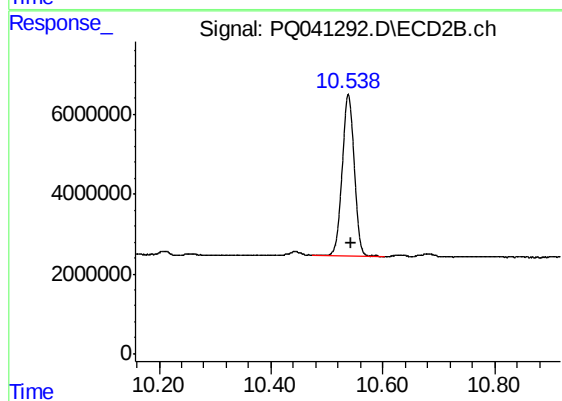

#2 Decachlorobiphenyl

R.T.: 10.538 min
Delta R.T.: -0.005 min
Response: 60415904
Conc: 18.34 ng/ml