

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ071823\
 Data File : PQ062356.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jul 2023 18:42
 Operator : YP\AJ
 Sample : 03645-06
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 SB-10-(0.5-2.0)

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/19/2023
 Supervised By :Ankita Jodhani 07/19/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 02:52:59 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ070123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 04 05:32:27 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.401	2.755	107.3E6	51986201	21.998m	20.719
2) SA Decachlor...	8.583	7.524	74581083	69331280	20.530m	20.807m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ071823\
Data File : PQ062356.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jul 2023 18:42
Operator : YP\AJ
Sample : 03645-06
Misc :
ALS Vial : 25 Sample Multiplier: 1


Instrument :
ECD_Q
ClientSampleId :
SB-10-(0.5-2.0)


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/19/2023
Supervised By :Ankita Jodhani 07/19/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 02:52:59 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ070123.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 04 05:32:27 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

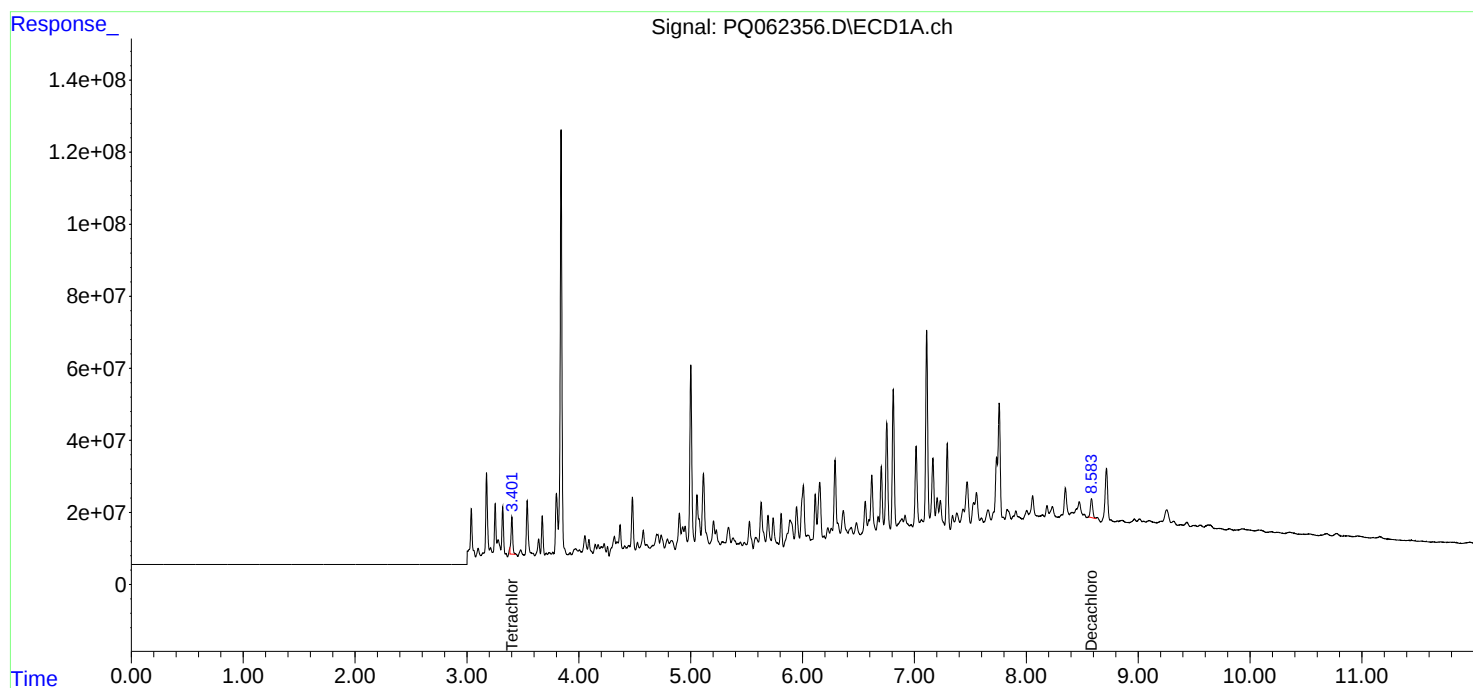

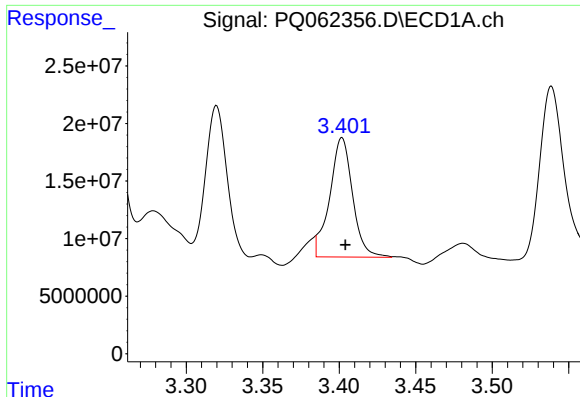

#1 Tetrachloro-m-xylene

R.T.: 3.401 min
Delta R.T.: -0.003 min
Response: 107308706
Conc: 22.00 ng/ml


Instrument :

ECD_Q

ClientSampleId :
SB-10-(0.5-2.0)


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/19/2023
Supervised By :Ankita Jodhani 07/19/2023

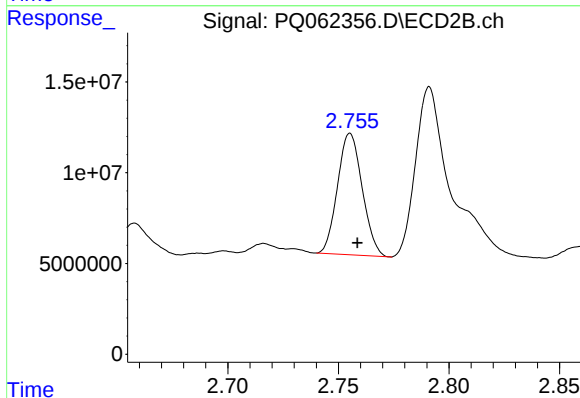


#1 Tetrachloro-m-xylene

R.T.: 2.755 min
Delta R.T.: -0.003 min
Response: 51986201
Conc: 20.72 ng/ml

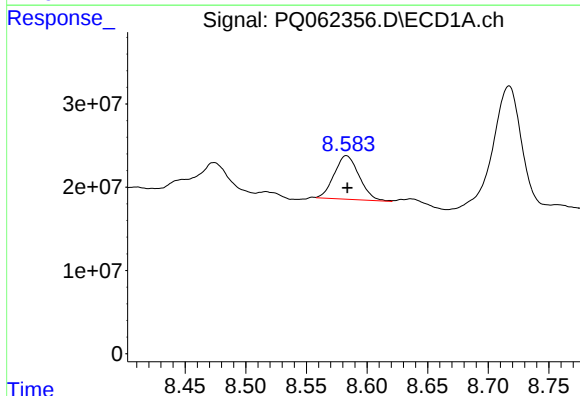

#2 Decachlorobiphenyl

R.T.: 8.583 min
Delta R.T.: -0.001 min
Response: 74581083
Conc: 20.53 ng/ml m

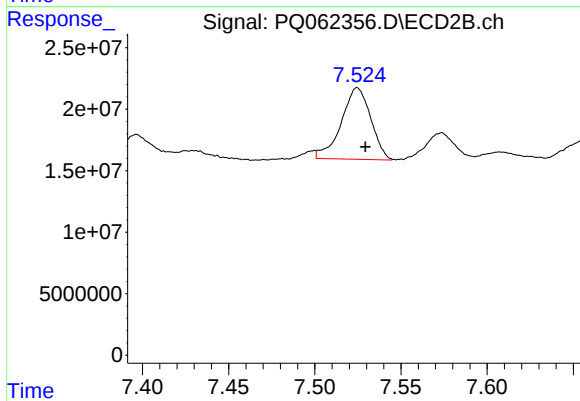

#2 Decachlorobiphenyl

R.T.: 7.524 min
Delta R.T.: -0.005 min
Response: 69331280
Conc: 20.81 ng/ml m