

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ071823\
 Data File : PQ062369.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jul 2023 22:37
 Operator : YP\AJ
 Sample : 03651-01 10X
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 NWB-1925

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/19/2023
 Supervised By :Ankita Jodhani 07/19/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 02:59:24 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ070123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 04 05:32:27 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.401	2.756	5237153	4494046	1.074m	1.791m#
2) SA Decachlor...	8.582	7.529	3622962	13023339	0.997m	3.908 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ071823\
Data File : PQ062369.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jul 2023 22:37
Operator : YP\AJ
Sample : 03651-01 10X
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
NWB-1925


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/19/2023
Supervised By :Ankita Jodhani 07/19/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 02:59:24 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ070123.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 04 05:32:27 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

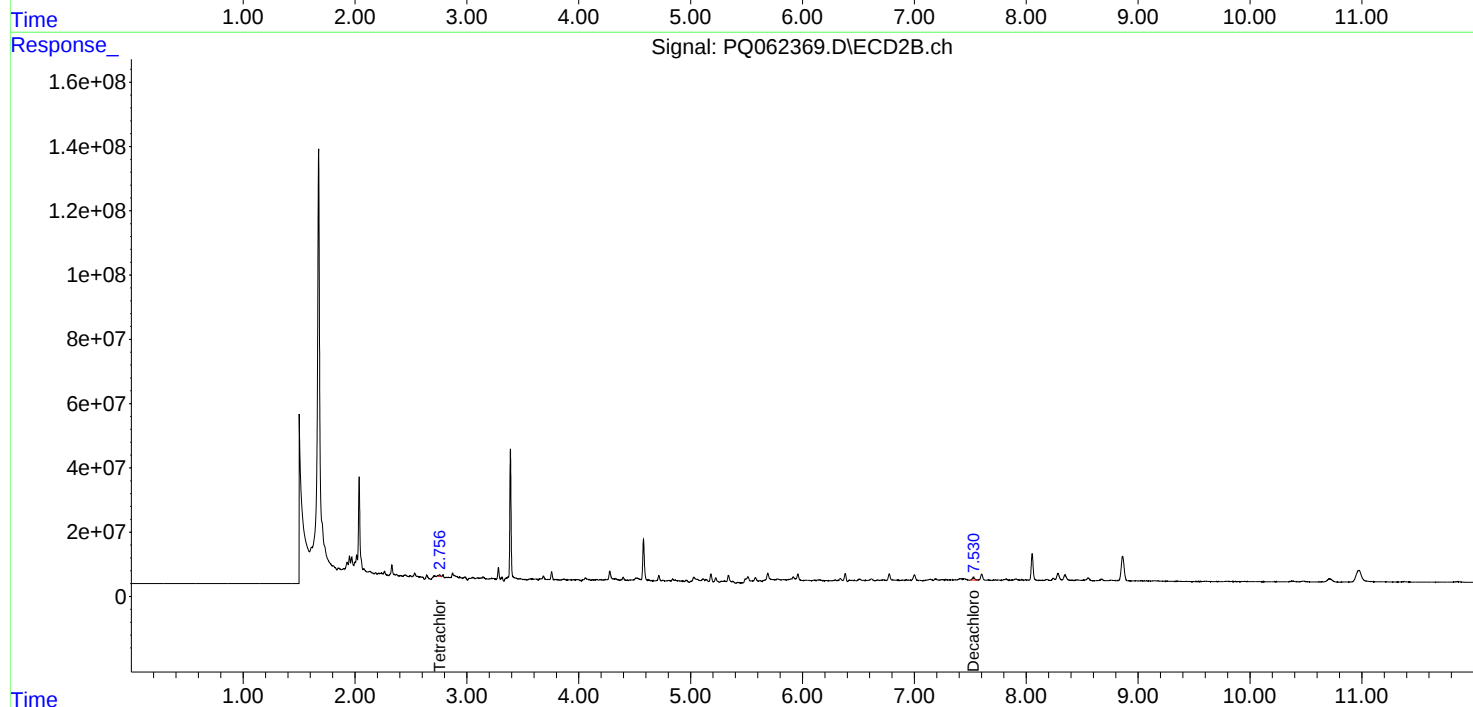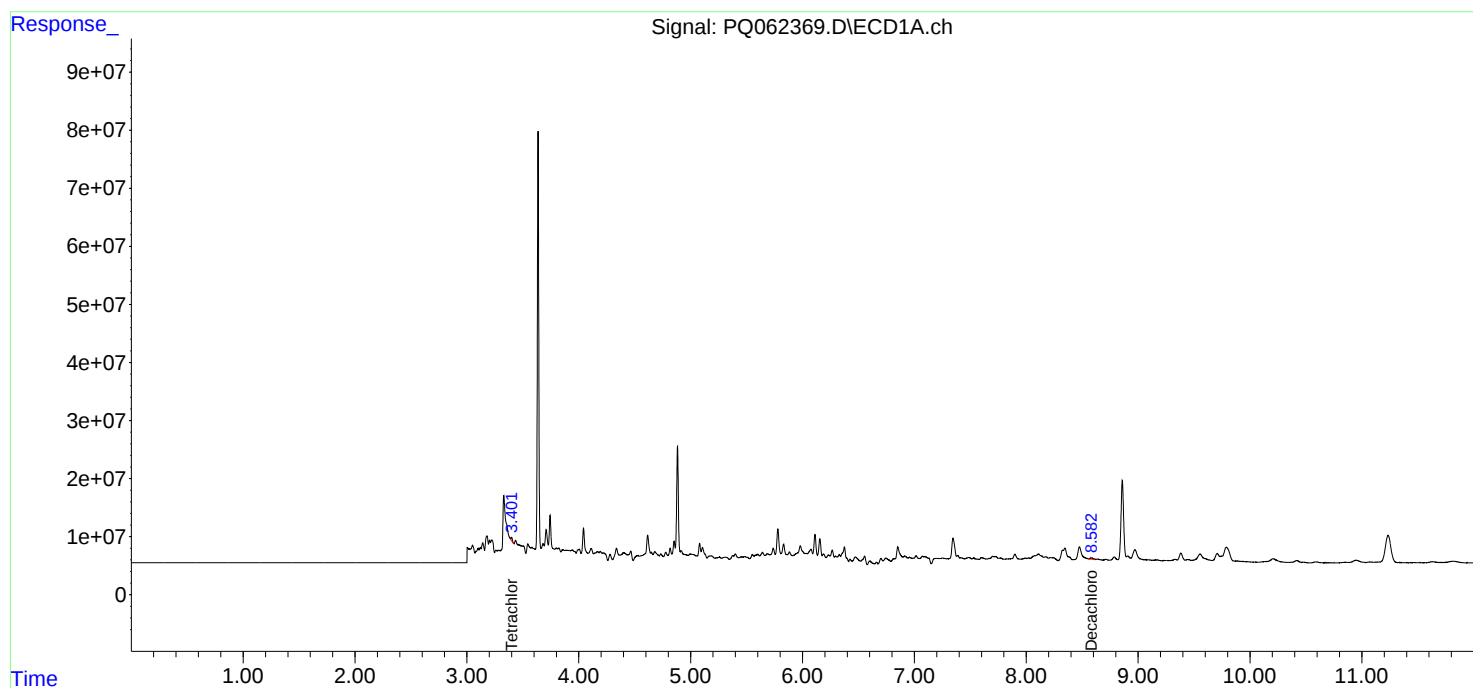

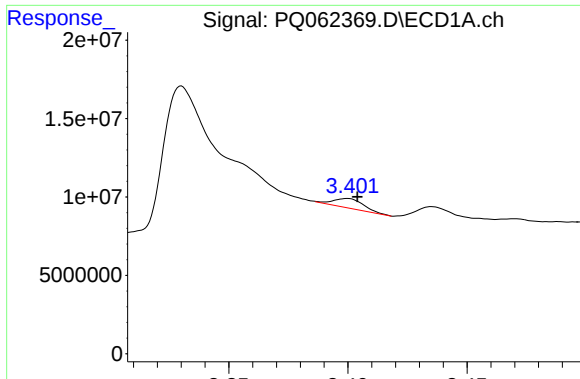


#1 Tetrachloro-m-xylene

R.T.: 3.401 min
Delta R.T.: -0.003 min
Response: 5237153
Conc: 1.07 ng/ml

Instrument : ECD_Q
ClientSampleId : NWB-1925


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/19/2023
Supervised By :Ankita Jodhani 07/19/2023

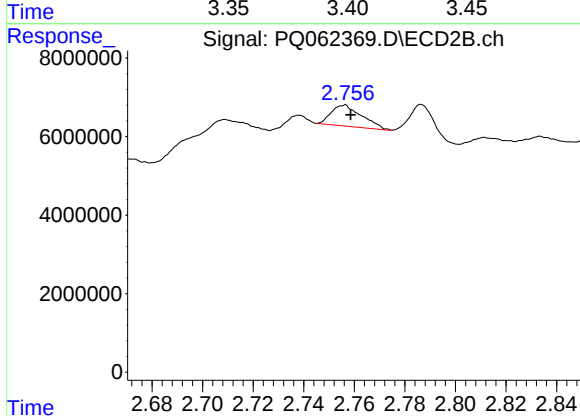


#1 Tetrachloro-m-xylene

R.T.: 2.756 min
Delta R.T.: -0.002 min
Response: 4494046
Conc: 1.79 ng/ml m

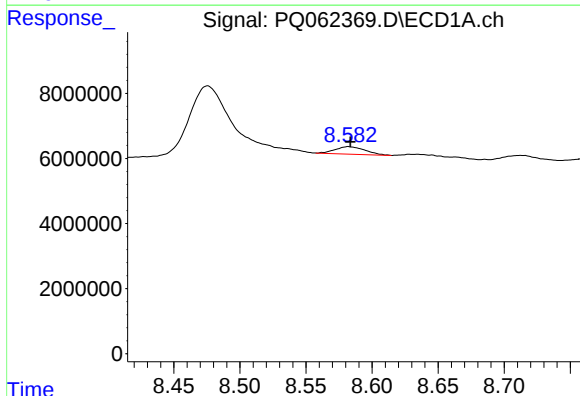

#2 Decachlorobiphenyl

R.T.: 8.582 min
Delta R.T.: -0.002 min
Response: 3622962
Conc: 1.00 ng/ml m

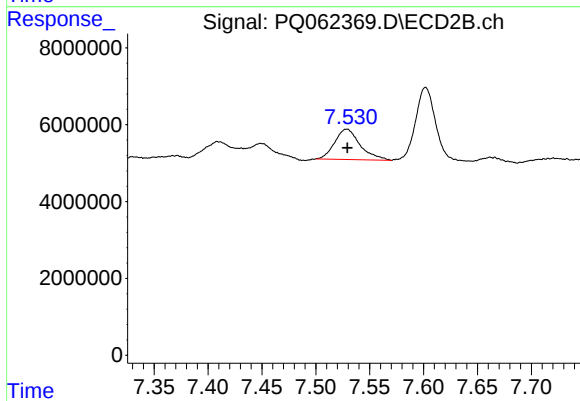

#2 Decachlorobiphenyl

R.T.: 7.529 min
Delta R.T.: 0.000 min
Response: 13023339
Conc: 3.91 ng/ml