

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ072023\
 Data File : PQ062462.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jul 2023 21:41
 Operator : YP\AJ
 Sample : 03664-06 10X
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 AUD-1022

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/21/2023
 Supervised By :Ankita Jodhani 07/21/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 21 06:03:18 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ070123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 04 05:32:27 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.396	2.758	2875140	4450549	0.589m	1.774m#
2) SA Decachlor...	8.576	7.524	2894787	8065882	0.797m	2.421m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ072023\
Data File : PQ062462.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2023 21:41
Operator : YP\AJ
Sample : 03664-06 10X
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
AUD-1022


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/21/2023
Supervised By :Ankita Jodhani 07/21/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 21 06:03:18 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ070123.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 04 05:32:27 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

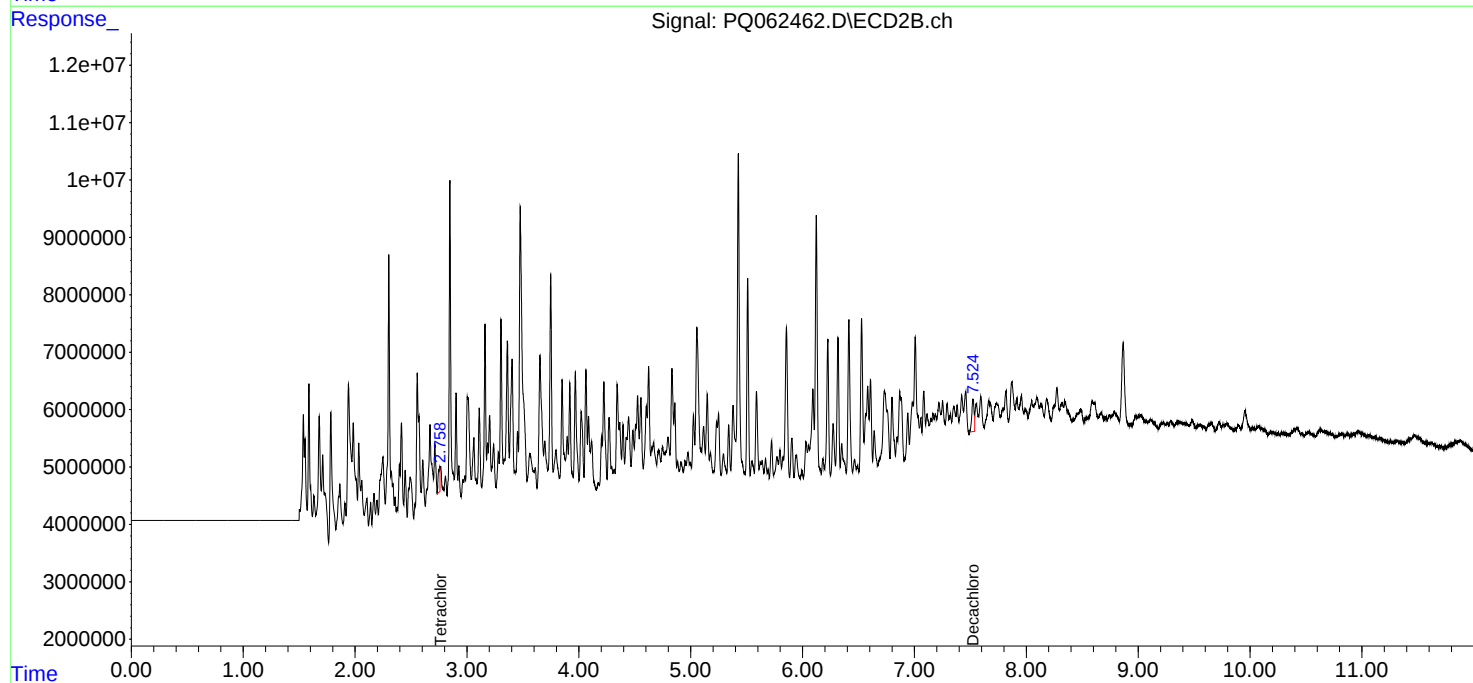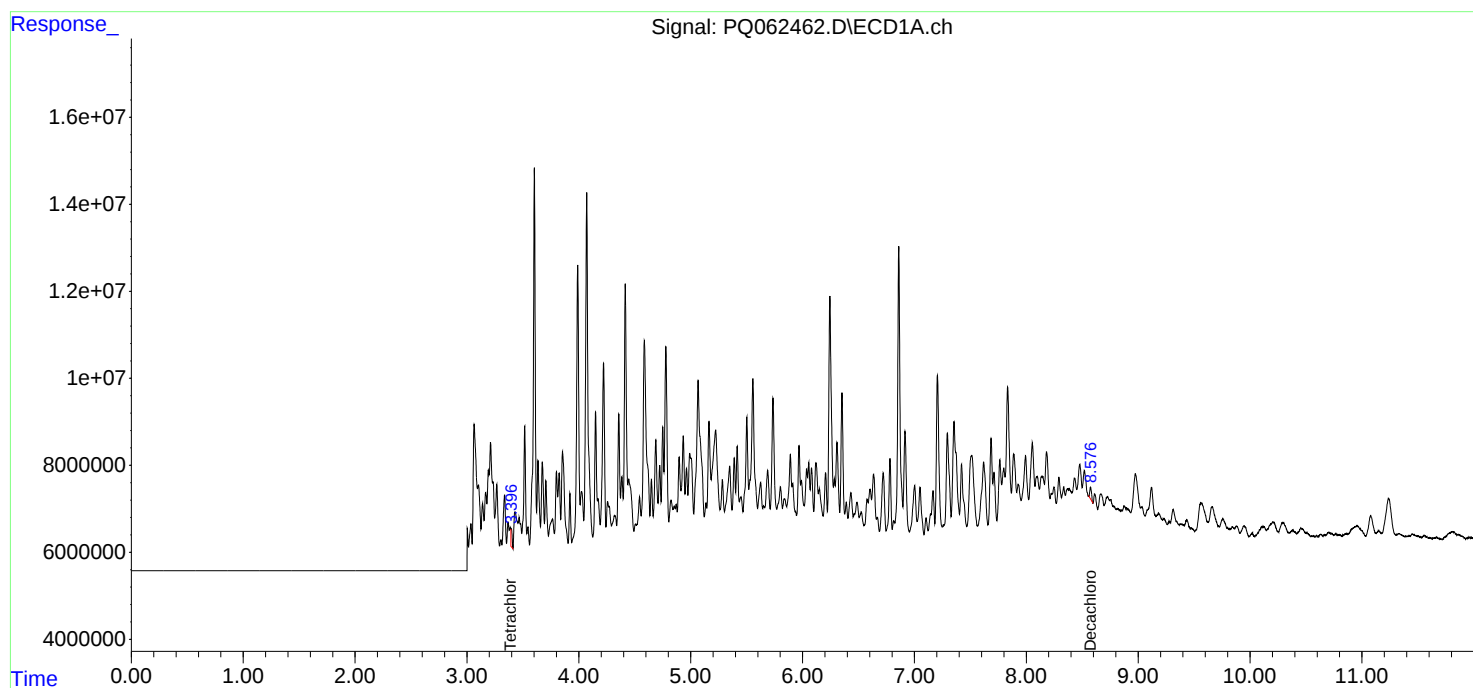

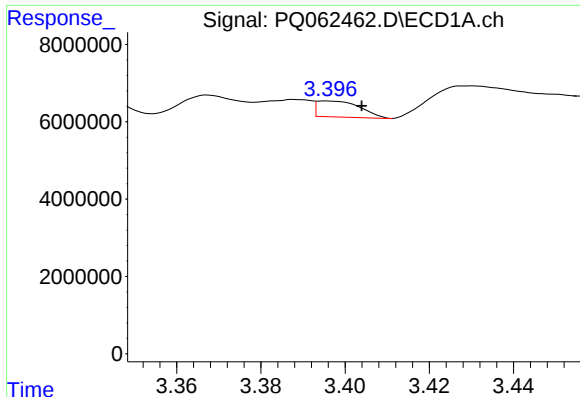


#1 Tetrachloro-m-xylene

R.T.: 3.396 min
Delta R.T.: -0.008 min
Response: 2875140
Conc: 0.59 ng/ml

Instrument :
ECD_Q
ClientSampleId :
AUD-1022


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/21/2023
Supervised By :Ankita Jodhani 07/21/2023

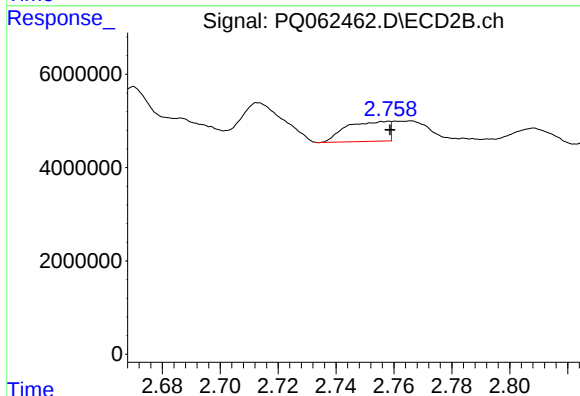


#1 Tetrachloro-m-xylene

R.T.: 2.758 min
Delta R.T.: 0.000 min
Response: 4450549
Conc: 1.77 ng/ml m

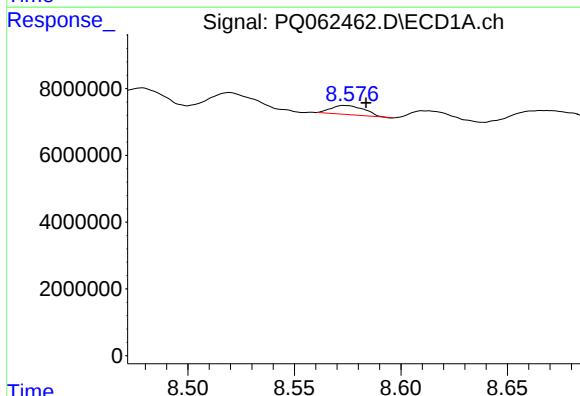

#2 Decachlorobiphenyl

R.T.: 8.576 min
Delta R.T.: -0.008 min
Response: 2894787
Conc: 0.80 ng/ml m

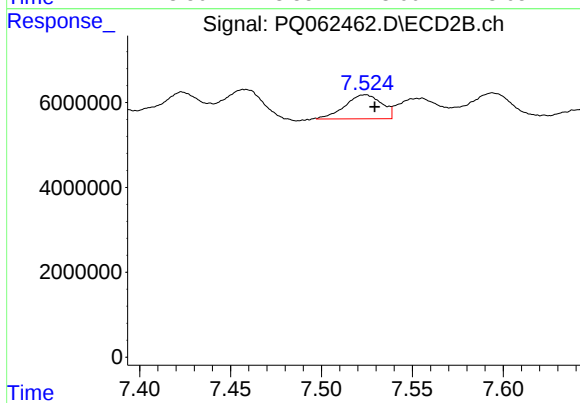

#2 Decachlorobiphenyl

R.T.: 7.524 min
Delta R.T.: -0.006 min
Response: 8065882
Conc: 2.42 ng/ml m