

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ072123\
 Data File : PQ062474.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2023 10:08
 Operator : YP\AJ
 Sample : PB154320BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 PB154320BL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/24/2023
 Supervised By :Ankita Jodhani 07/24/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 21 12:42:27 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ070123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 04 05:32:27 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.401	2.754	102.3E6	58835601	20.962	23.449m
2) SA Decachlor...	8.585	7.524	85613653	78896438	23.567	23.677m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ072123\
Data File : PQ062474.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jul 2023 10:08
Operator : YP\AJ
Sample : PB154320BL
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
PB154320BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/24/2023
Supervised By :Ankita Jodhani 07/24/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 21 12:42:27 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ070123.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 04 05:32:27 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

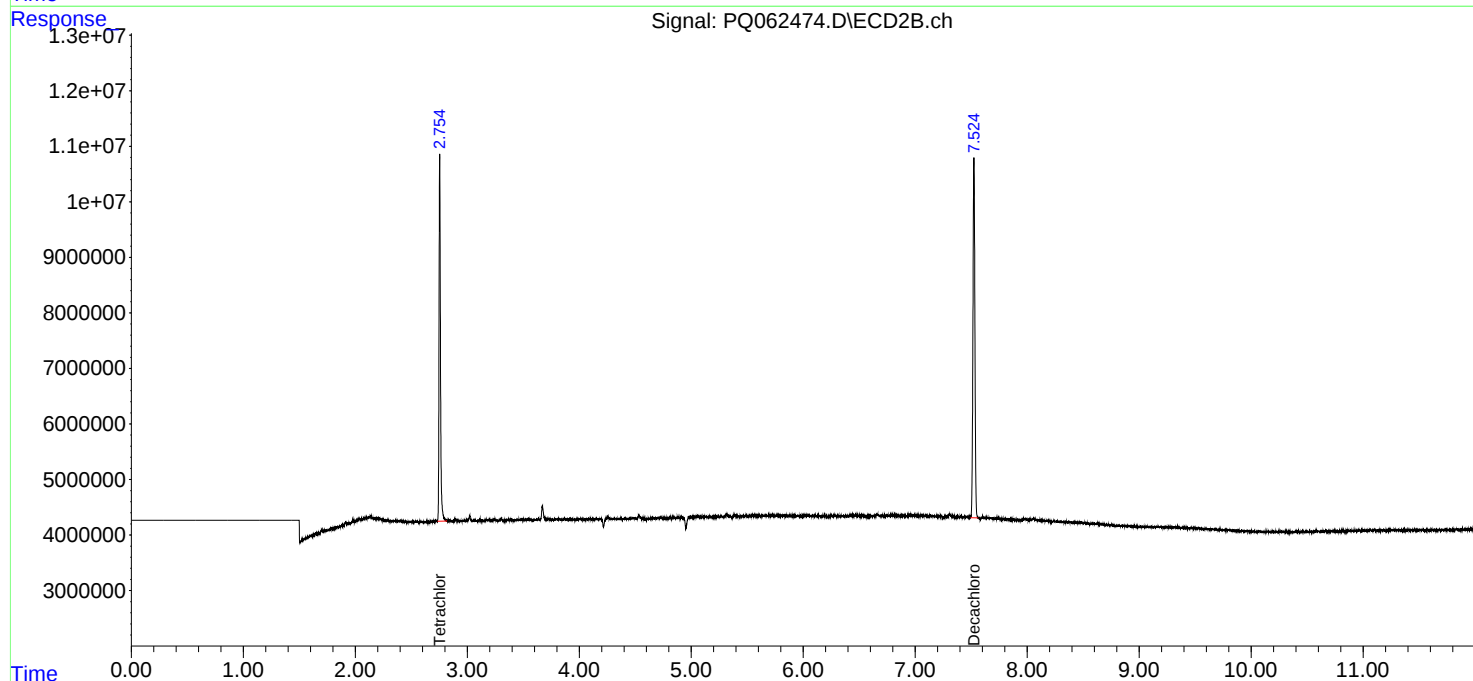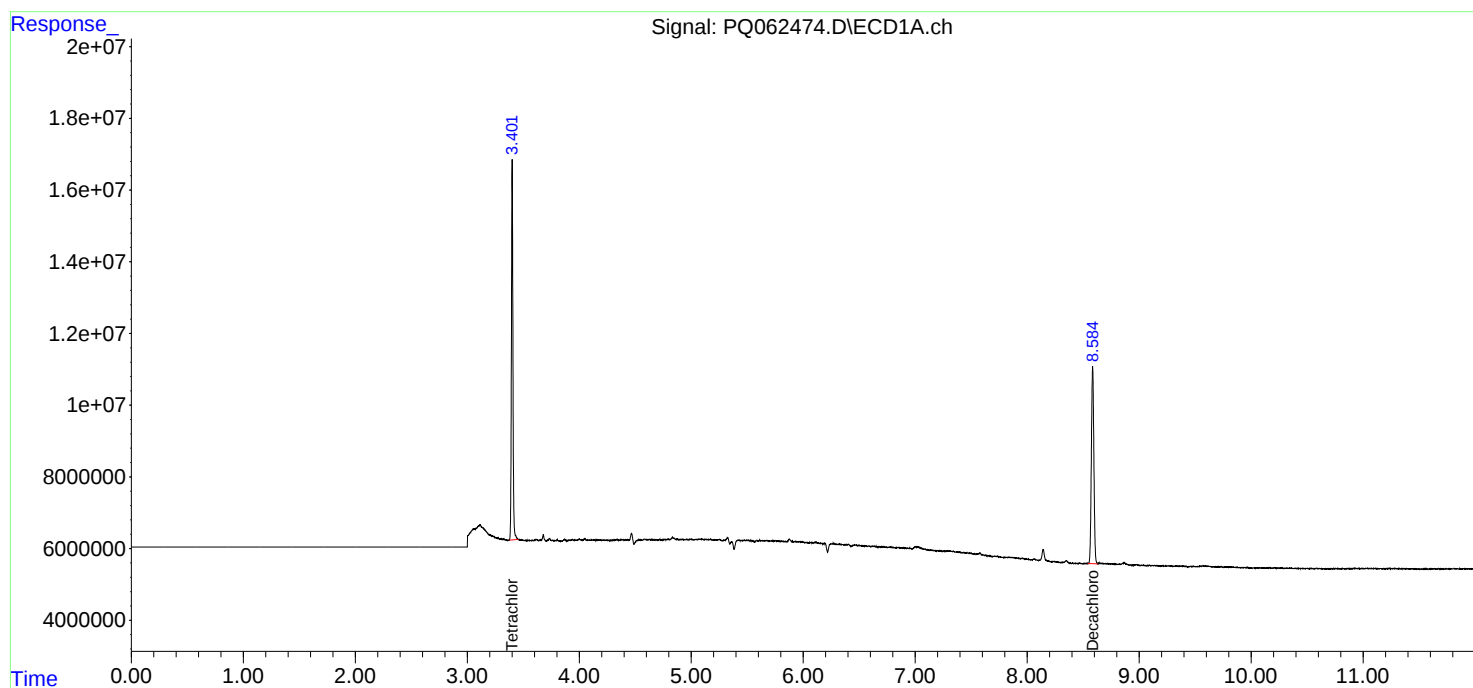

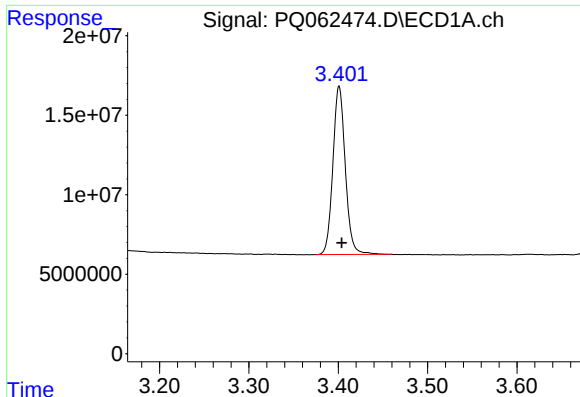

#1 Tetrachloro-m-xylene

R.T.: 3.401 min
Delta R.T.: -0.003 min
Response: 102254694
Conc: 20.96 ng/ml

Instrument :

ECD_Q


ClientSampleId :

PB154320BL

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 07/24/2023
Supervised By :Ankita Jodhani 07/24/2023

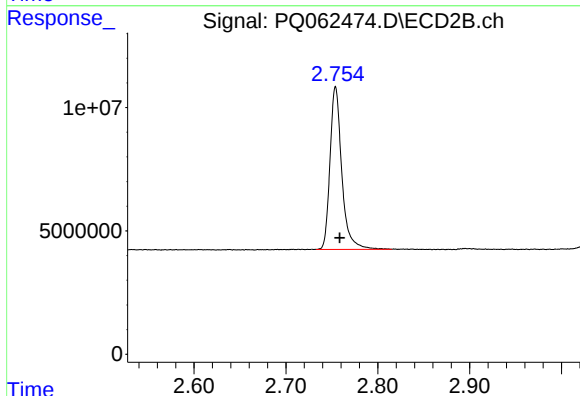


#1 Tetrachloro-m-xylene

R.T.: 2.754 min
Delta R.T.: -0.005 min
Response: 58835601
Conc: 23.45 ng/ml m

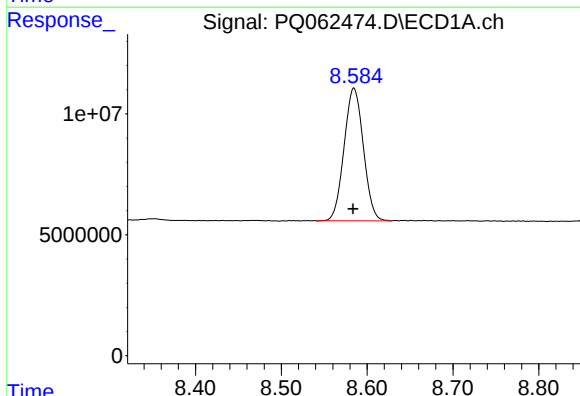

#2 Decachlorobiphenyl

R.T.: 8.585 min
Delta R.T.: 0.000 min
Response: 85613653
Conc: 23.57 ng/ml

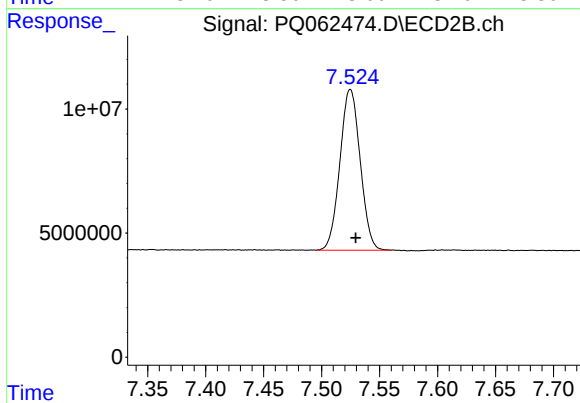

#2 Decachlorobiphenyl

R.T.: 7.524 min
Delta R.T.: -0.005 min
Response: 78896438
Conc: 23.68 ng/ml m