

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ072123\
 Data File : PQ062526.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jul 2023 02:01
 Operator : YP\AJ
 Sample : 03681-13
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 RPTP-5-CS-5

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/24/2023
 Supervised By :Ankita Jodhani 07/24/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 15:01:13 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ070123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 04 05:32:27 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.402	2.755	81035628	47655489	16.612	18.993
2) SA Decachlor...	8.582	7.523	64358040	57744484	17.716	17.329m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ072123\
Data File : PQ062526.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jul 2023 02:01
Operator : YP\AJ
Sample : 03681-13
Misc :
ALS Vial : 44 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
RPTP-5-CS-5


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/24/2023
Supervised By :Ankita Jodhani 07/24/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 22 15:01:13 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ070123.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 04 05:32:27 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

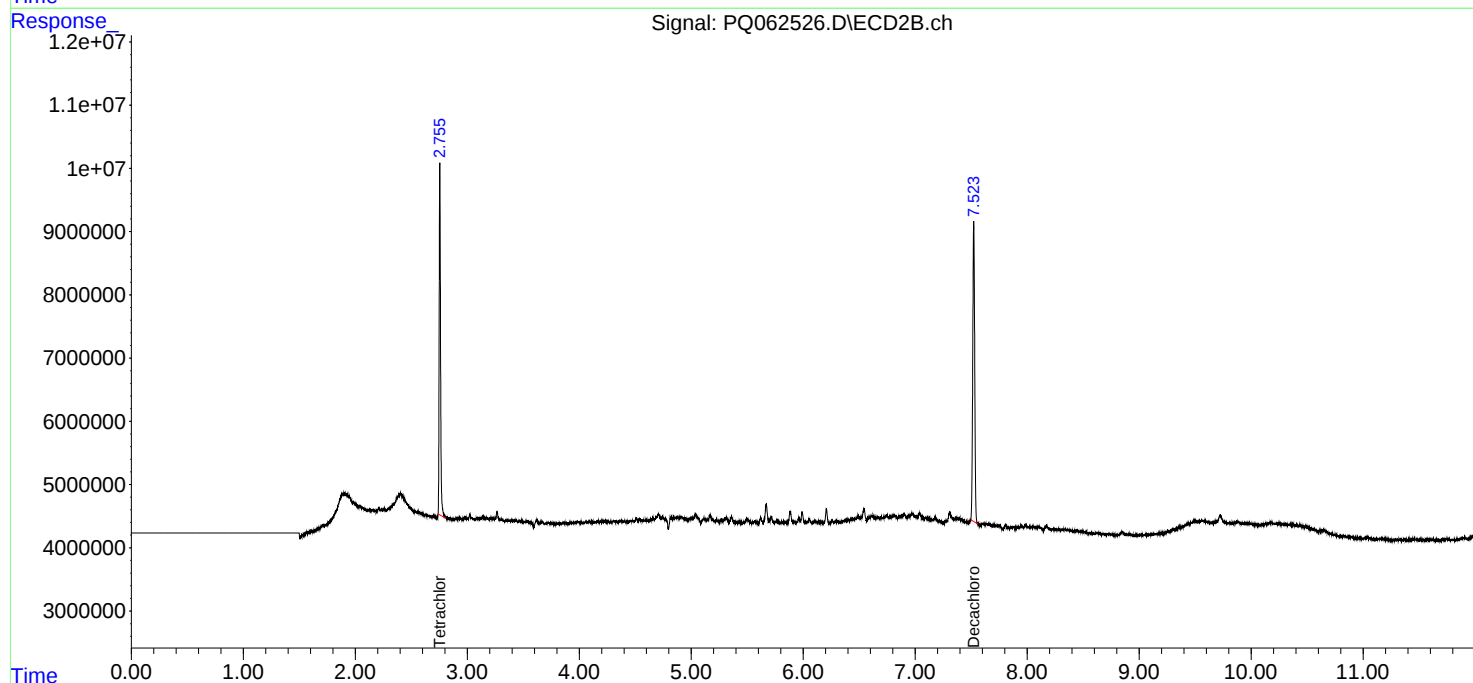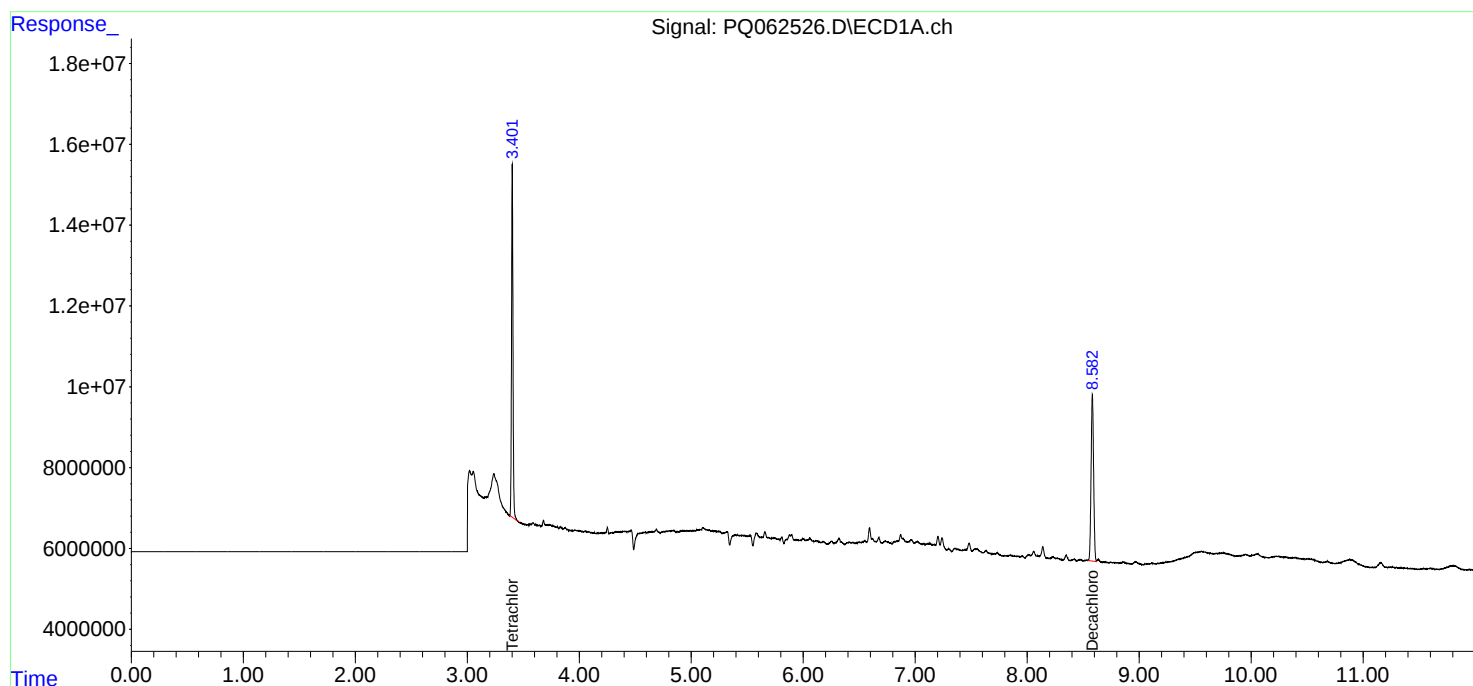

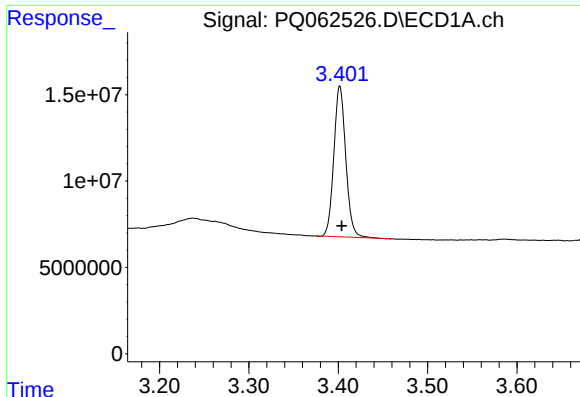


#1 Tetrachloro-m-xylene

R.T.: 3.402 min
Delta R.T.: -0.002 min
Response: 81035628
Conc: 16.61 ng/ml

Instrument :
ECD_Q
ClientSampleId :
RPTP-5-CS-5


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/24/2023
Supervised By :Ankita Jodhani 07/24/2023

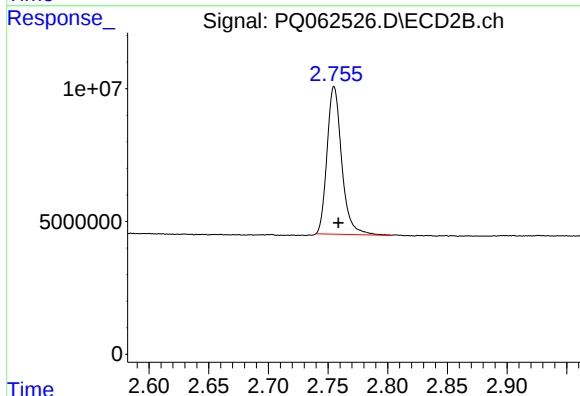


#1 Tetrachloro-m-xylene

R.T.: 2.755 min
Delta R.T.: -0.003 min
Response: 47655489
Conc: 18.99 ng/ml

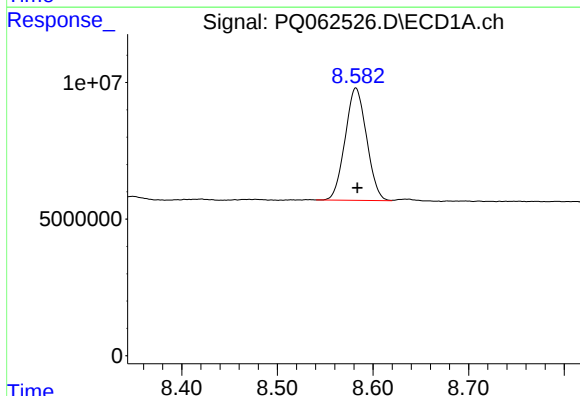

#2 Decachlorobiphenyl

R.T.: 8.582 min
Delta R.T.: -0.002 min
Response: 64358040
Conc: 17.72 ng/ml

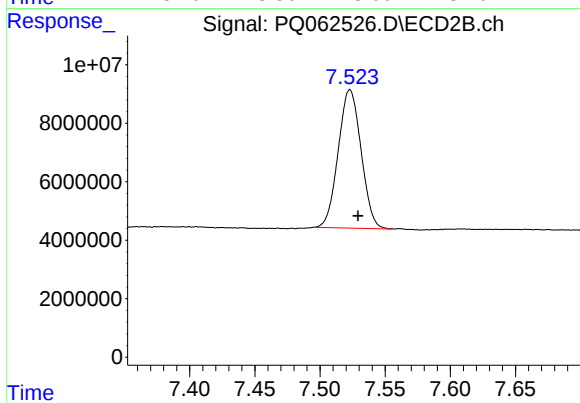

#2 Decachlorobiphenyl

R.T.: 7.523 min
Delta R.T.: -0.007 min
Response: 57744484
Conc: 17.33 ng/ml m