

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ072423\
 Data File : PQ062564.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jul 2023 13:10
 Operator : YP\AJ
 Sample : PB154343BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 PB154343BL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/25/2023
 Supervised By :Ankita Jodhani 07/25/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 15:52:16 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ070123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 04 05:32:27 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.401	2.753	75316763	54563612	15.439	21.746m#
2) SA Decachlor...	8.584	7.523	61446708	59550091	16.915m	17.871m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ072423\
Data File : PQ062564.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jul 2023 13:10
Operator : YP\AJ
Sample : PB154343BL
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
PB154343BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/25/2023
Supervised By :Ankita Jodhani 07/25/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 15:52:16 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ070123.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 04 05:32:27 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

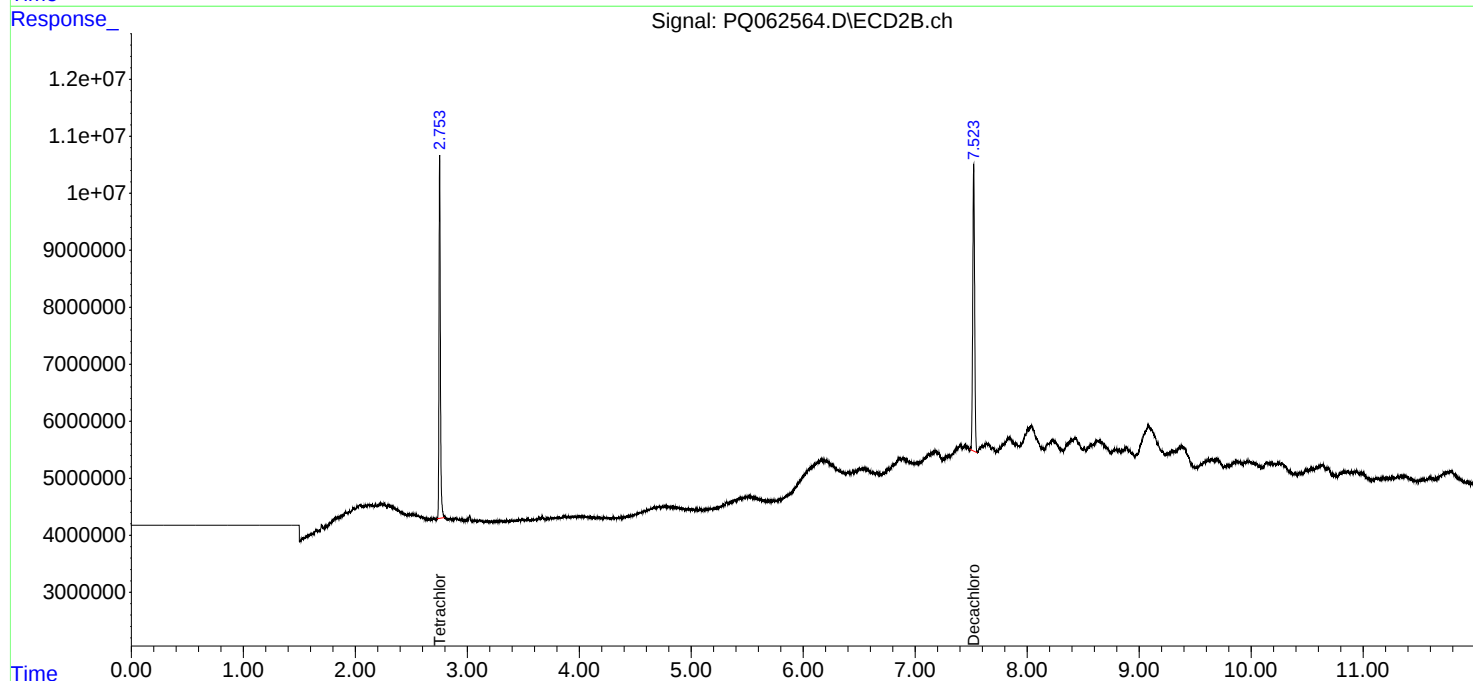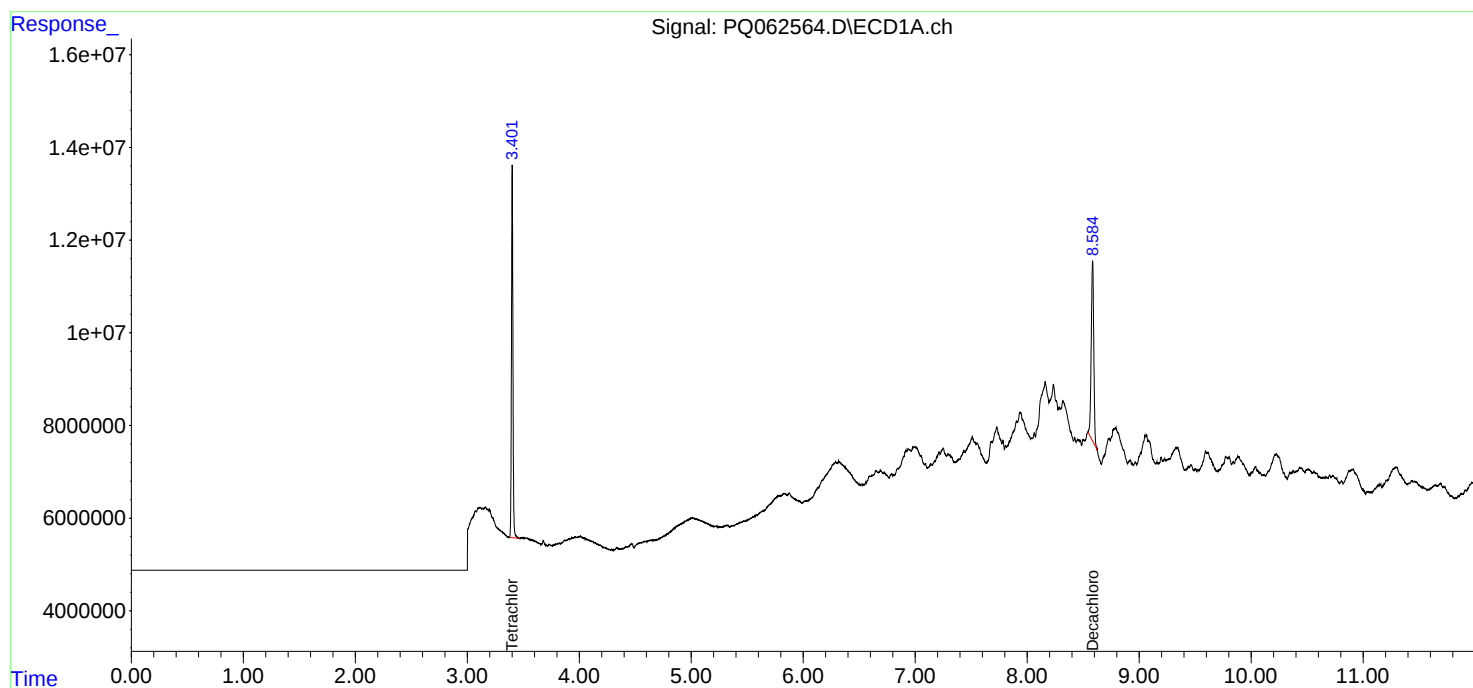

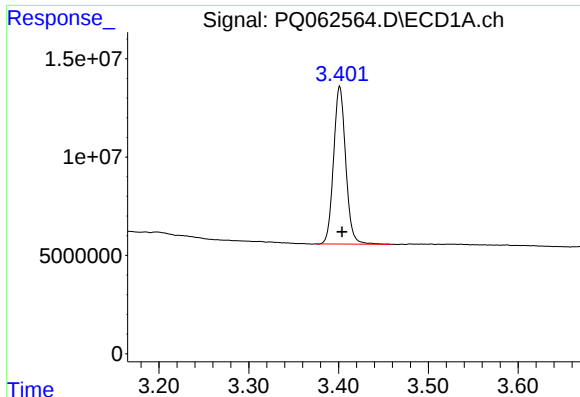

#1 Tetrachloro-m-xylene

R.T.: 3.401 min
Delta R.T.: -0.003 min
Response: 75316763
Conc: 15.44 ng/ml

Instrument :

ECD_Q


ClientSampleId :

PB154343BL

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 07/25/2023
Supervised By :Ankita Jodhani 07/25/2023

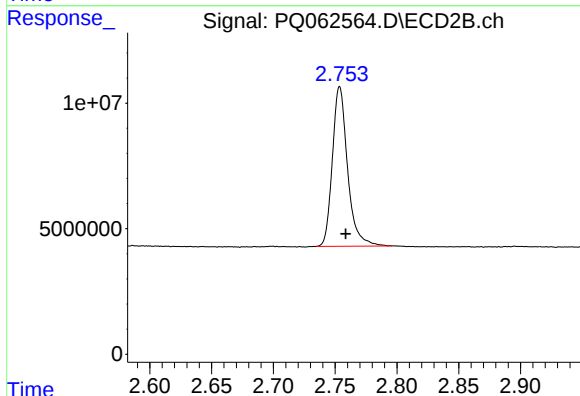


#1 Tetrachloro-m-xylene

R.T.: 2.753 min
Delta R.T.: -0.005 min
Response: 54563612
Conc: 21.75 ng/ml m

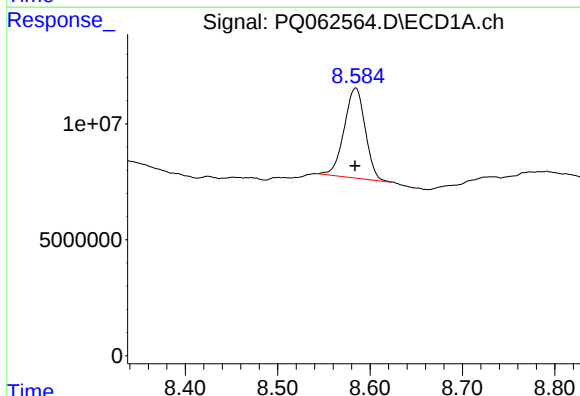

#2 Decachlorobiphenyl

R.T.: 8.584 min
Delta R.T.: 0.000 min
Response: 61446708
Conc: 16.91 ng/ml m

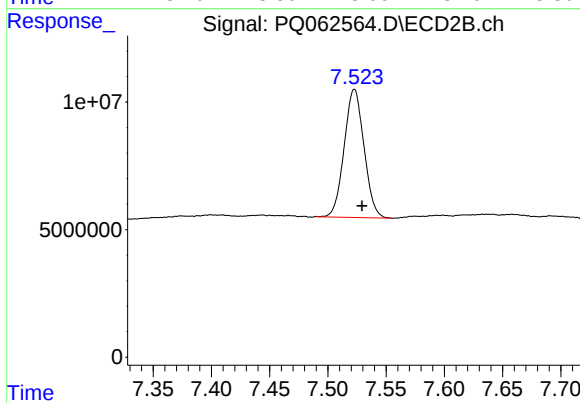

#2 Decachlorobiphenyl

R.T.: 7.523 min
Delta R.T.: -0.007 min
Response: 59550091
Conc: 17.87 ng/ml m