

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ072423\
 Data File : PQ062568.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jul 2023 14:09
 Operator : YP\AJ
 Sample : 03682-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 ELZ-23-00066-00070

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/25/2023
 Supervised By :Ankita Jodhani 07/25/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 15:54:11 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ070123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 04 05:32:27 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.405	2.761	42381057	24991326	8.688m	9.960
2) SA Decachlor...	8.593	7.534	44539530	78160834	12.261m	23.456m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ072423\
Data File : PQ062568.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jul 2023 14:09
Operator : YP\AJ
Sample : 03682-01
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
ELZ-23-00066-00070


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/25/2023
Supervised By :Ankita Jodhani 07/25/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 15:54:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ070123.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 04 05:32:27 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

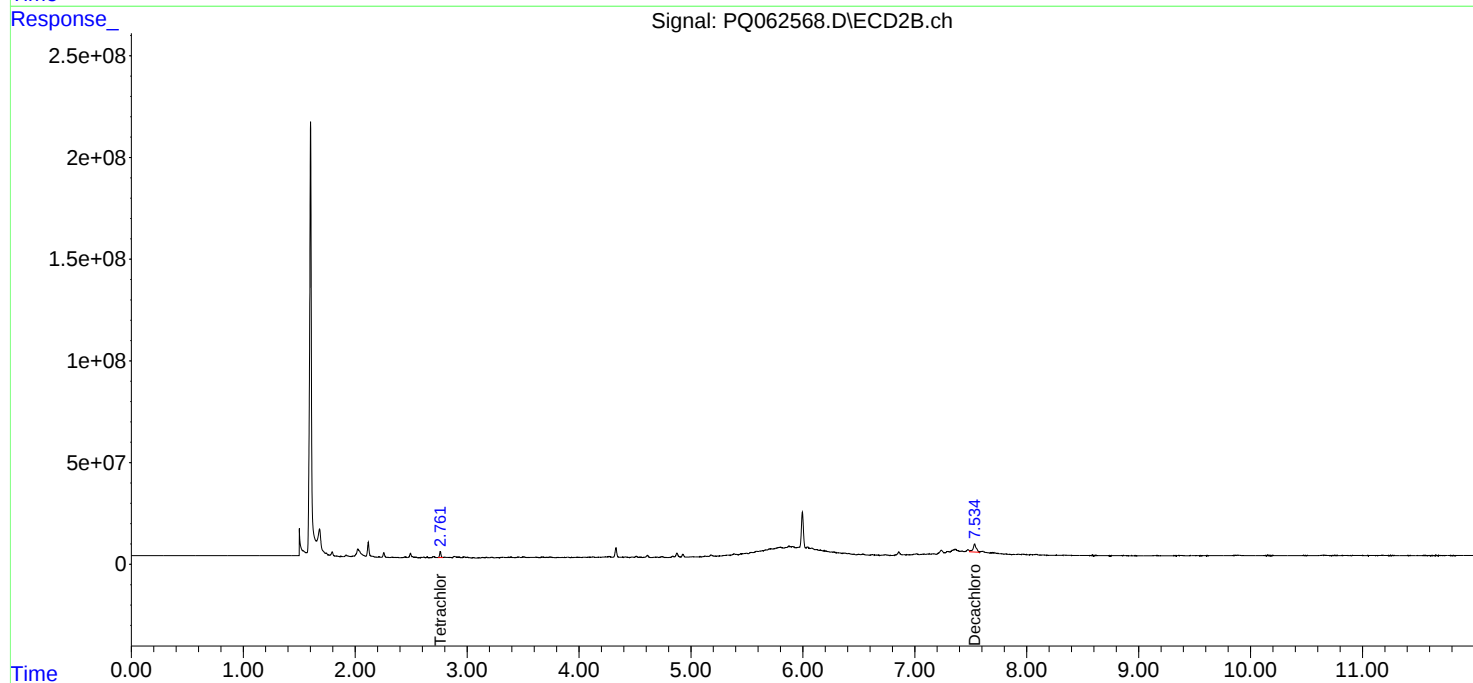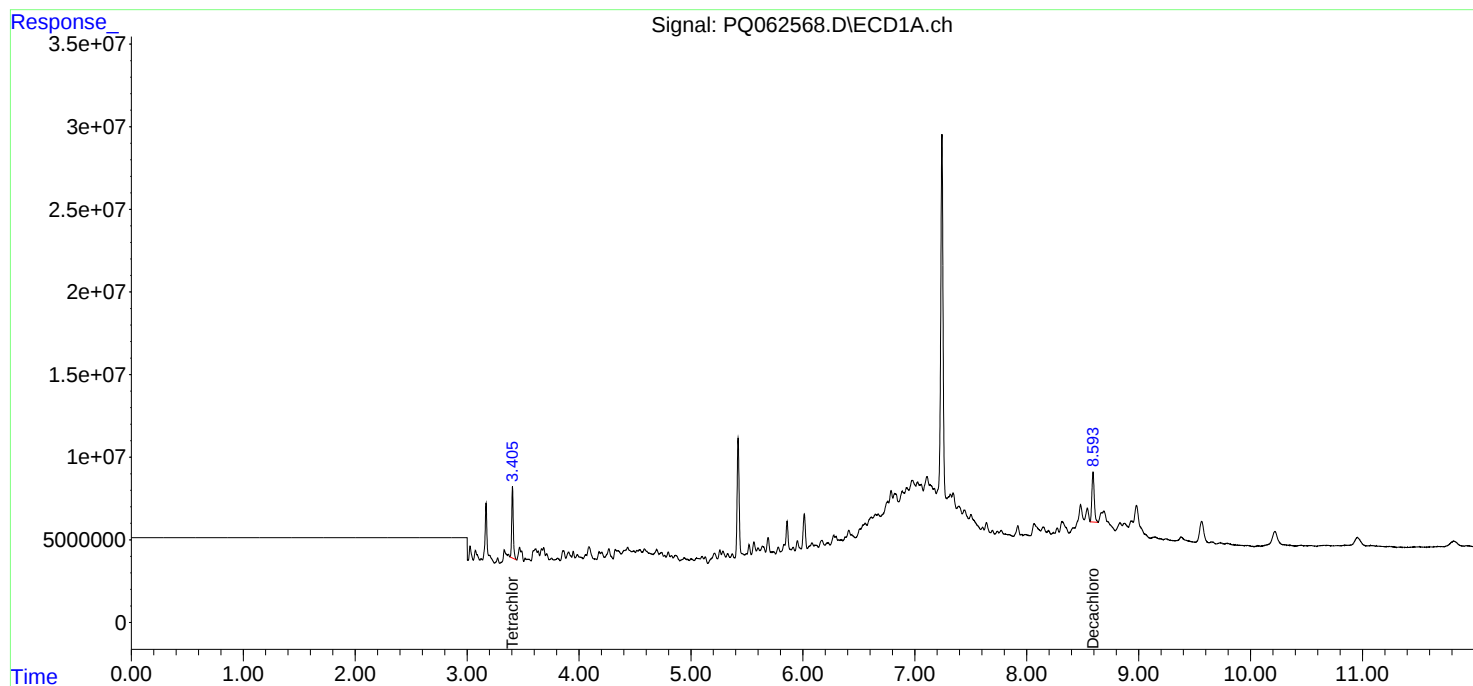

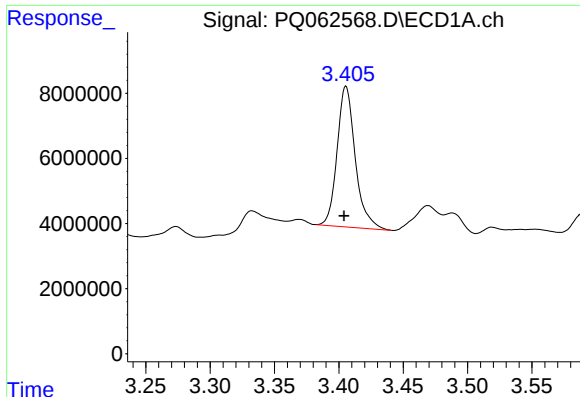


#1 Tetrachloro-m-xylene

R.T.: 3.405 min
Delta R.T.: 0.001 min
Response: 42381057
Conc: 8.69 ng/ml

Instrument :
ECD_Q
ClientSampleId :
ELZ-23-00066-00070


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/25/2023
Supervised By :Ankita Jodhani 07/25/2023

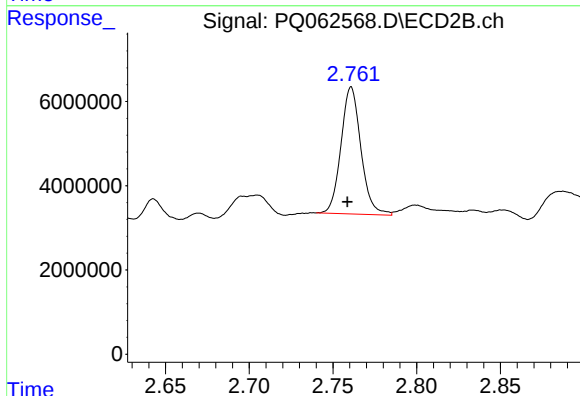


#1 Tetrachloro-m-xylene

R.T.: 2.761 min
Delta R.T.: 0.002 min
Response: 24991326
Conc: 9.96 ng/ml

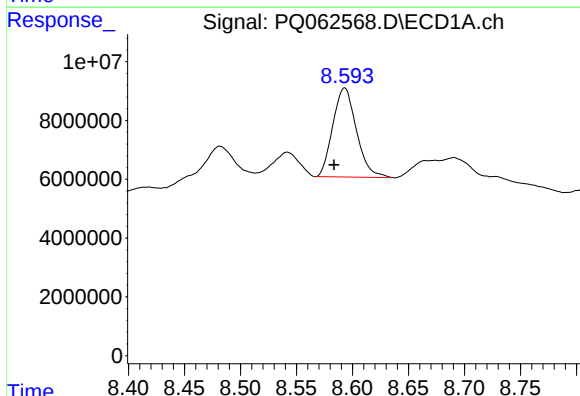

#2 Decachlorobiphenyl

R.T.: 8.593 min
Delta R.T.: 0.009 min
Response: 44539530
Conc: 12.26 ng/ml m

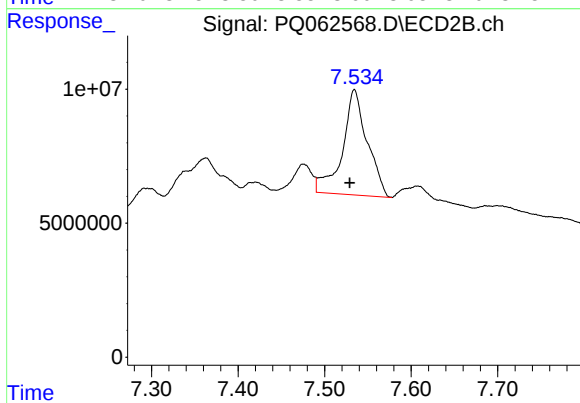

#2 Decachlorobiphenyl

R.T.: 7.534 min
Delta R.T.: 0.005 min
Response: 78160834
Conc: 23.46 ng/ml m