

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ072423\
 Data File : PQ062583.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jul 2023 18:32
 Operator : YP\AJ
 Sample : 03708-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 PL-02-072023

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/25/2023
 Supervised By :Ankita Jodhani 07/25/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 21:55:38 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ070123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 04 05:32:27 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.402	2.754	82497408	53105919	16.911	21.165m#
2) SA Decachlor...	8.583	7.524	54891910	47841725	15.110m	14.357m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ072423\
Data File : PQ062583.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jul 2023 18:32
Operator : YP\AJ
Sample : 03708-01
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
PL-02-072023


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/25/2023
Supervised By :Ankita Jodhani 07/25/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 21:55:38 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ070123.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 04 05:32:27 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

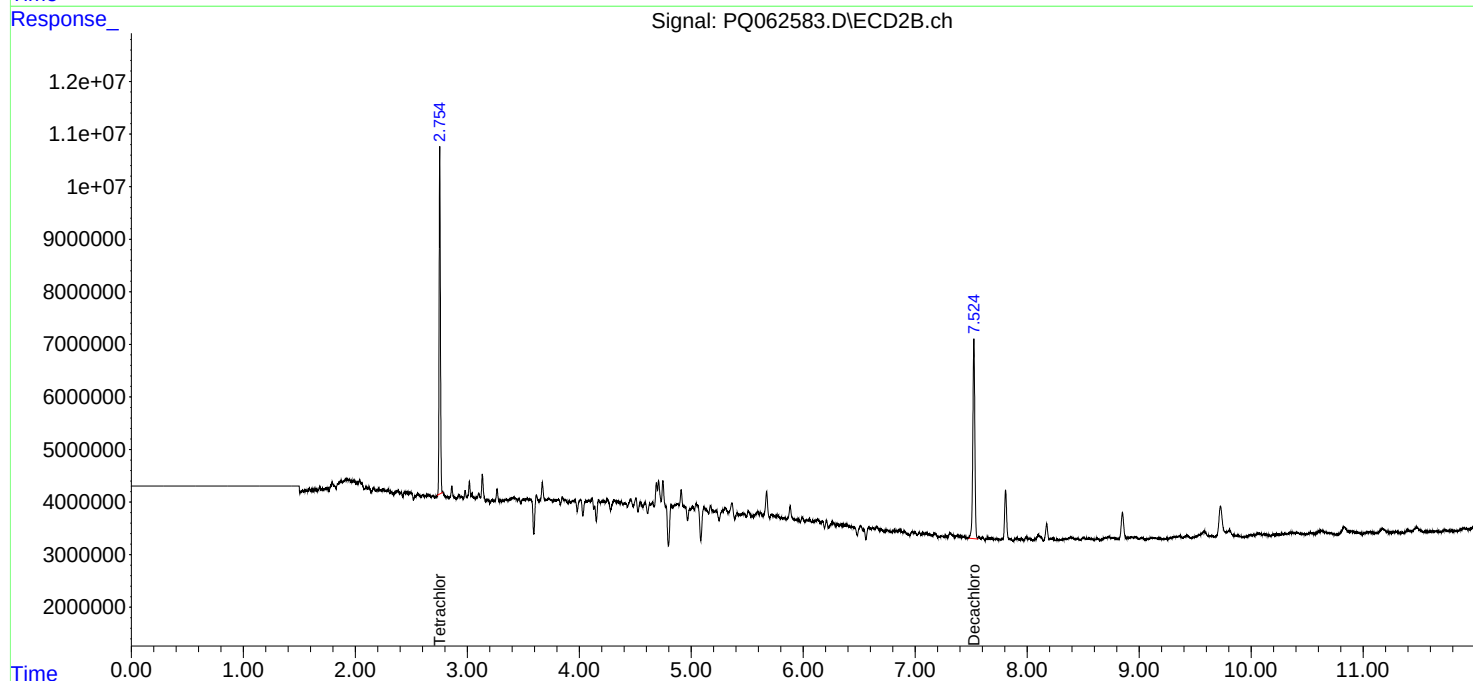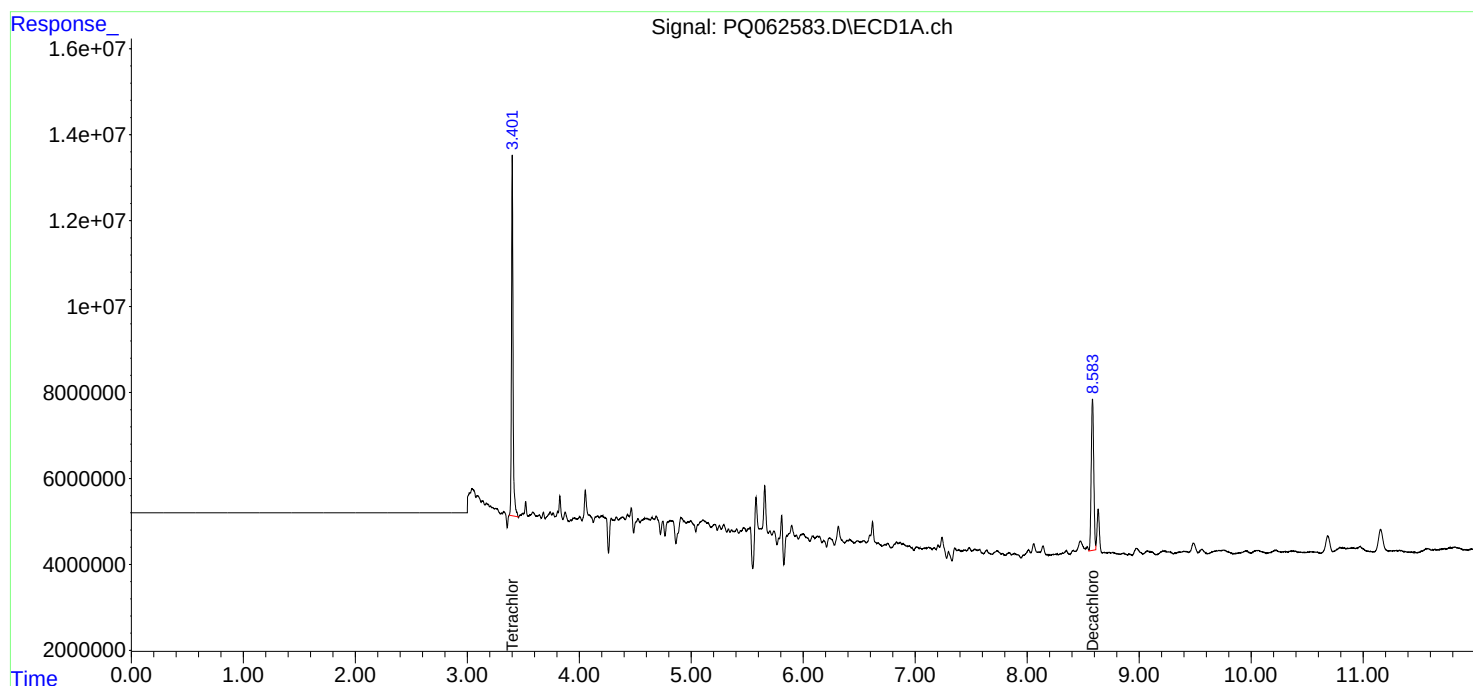

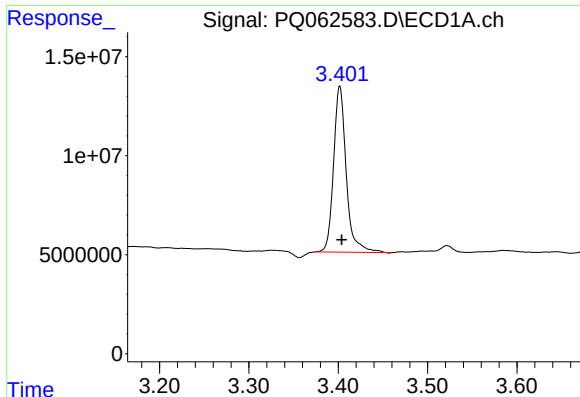

#1 Tetrachloro-m-xylene

R.T.: 3.402 min
Delta R.T.: -0.002 min
Response: 82497408
Conc: 16.91 ng/ml

Instrument :


ECD_Q

ClientSampleId :

PL-02-072023


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/25/2023
Supervised By :Ankita Jodhani 07/25/2023

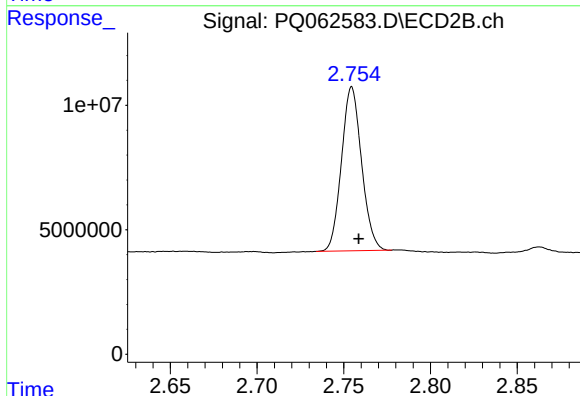


#1 Tetrachloro-m-xylene

R.T.: 2.754 min
Delta R.T.: -0.004 min
Response: 53105919
Conc: 21.17 ng/ml m

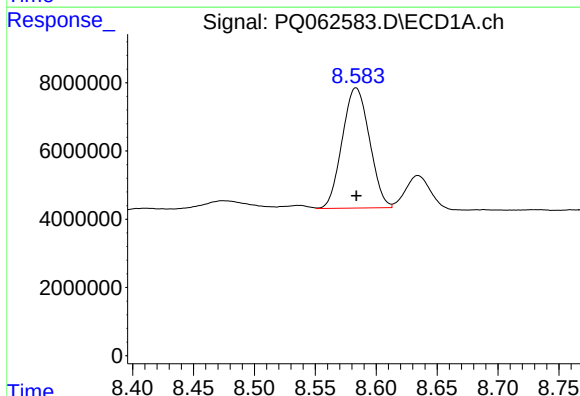

#2 Decachlorobiphenyl

R.T.: 8.583 min
Delta R.T.: 0.000 min
Response: 54891910
Conc: 15.11 ng/ml m

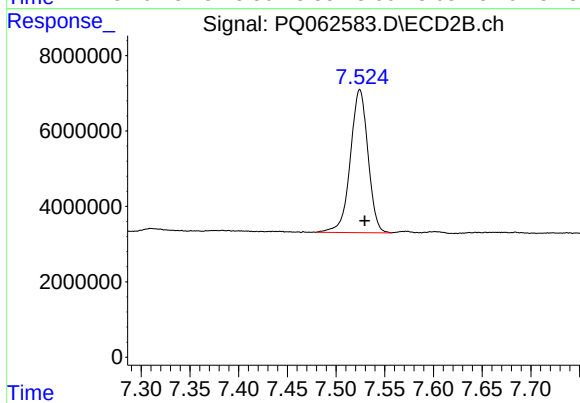

#2 Decachlorobiphenyl

R.T.: 7.524 min
Delta R.T.: -0.005 min
Response: 47841725
Conc: 14.36 ng/ml m