

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ072425\
 Data File : PQ070652.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jul 2025 14:26
 Operator : YP\AJ
 Sample : DDT ANALOG
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 DDT ANALOG

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 23:35:12 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ072225.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 09:47:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
30) L6 AR-1254-5	6.569	5.696	2882.2E6	3577.1E6	8200.814	5882.123 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ072425\
Data File : PQ070652.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jul 2025 14:26
Operator : YP\AJ
Sample : DDT ANALOG
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
DDT ANALOG

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 23:35:12 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ072225.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 23 09:47:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

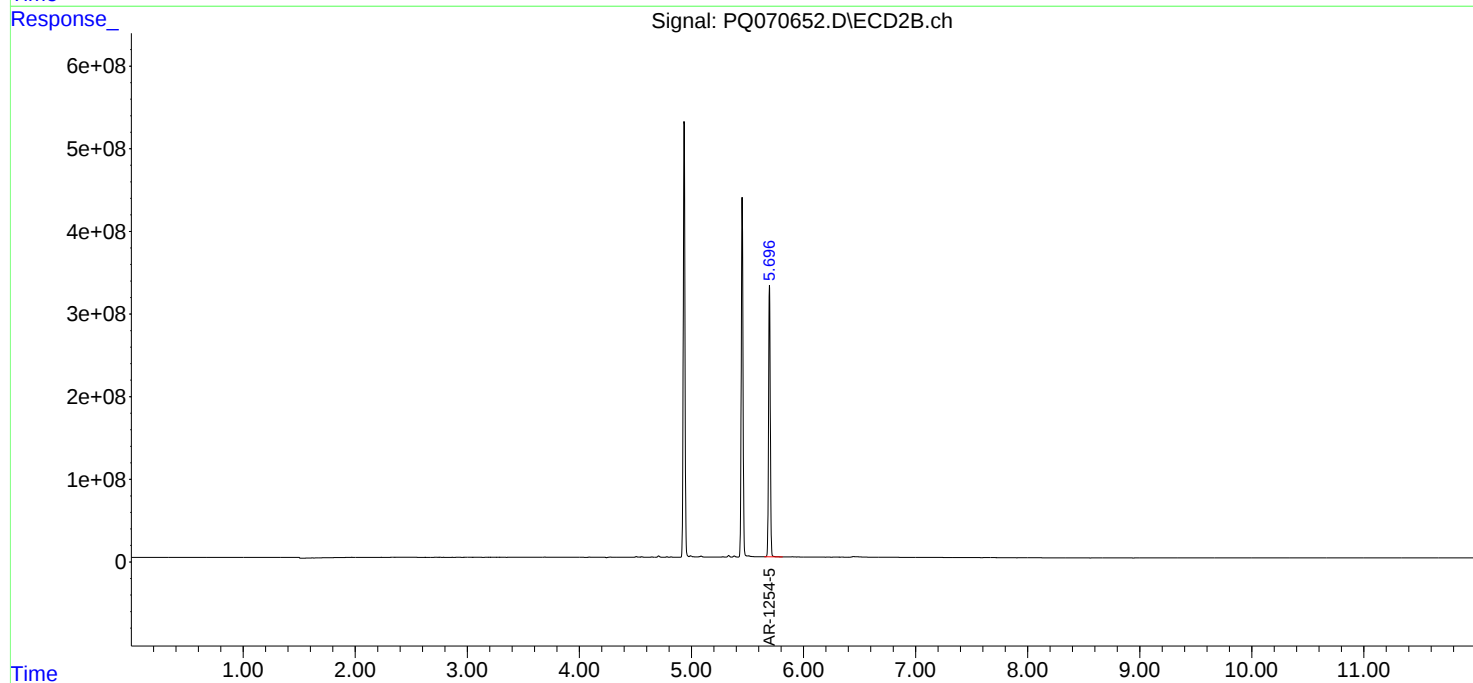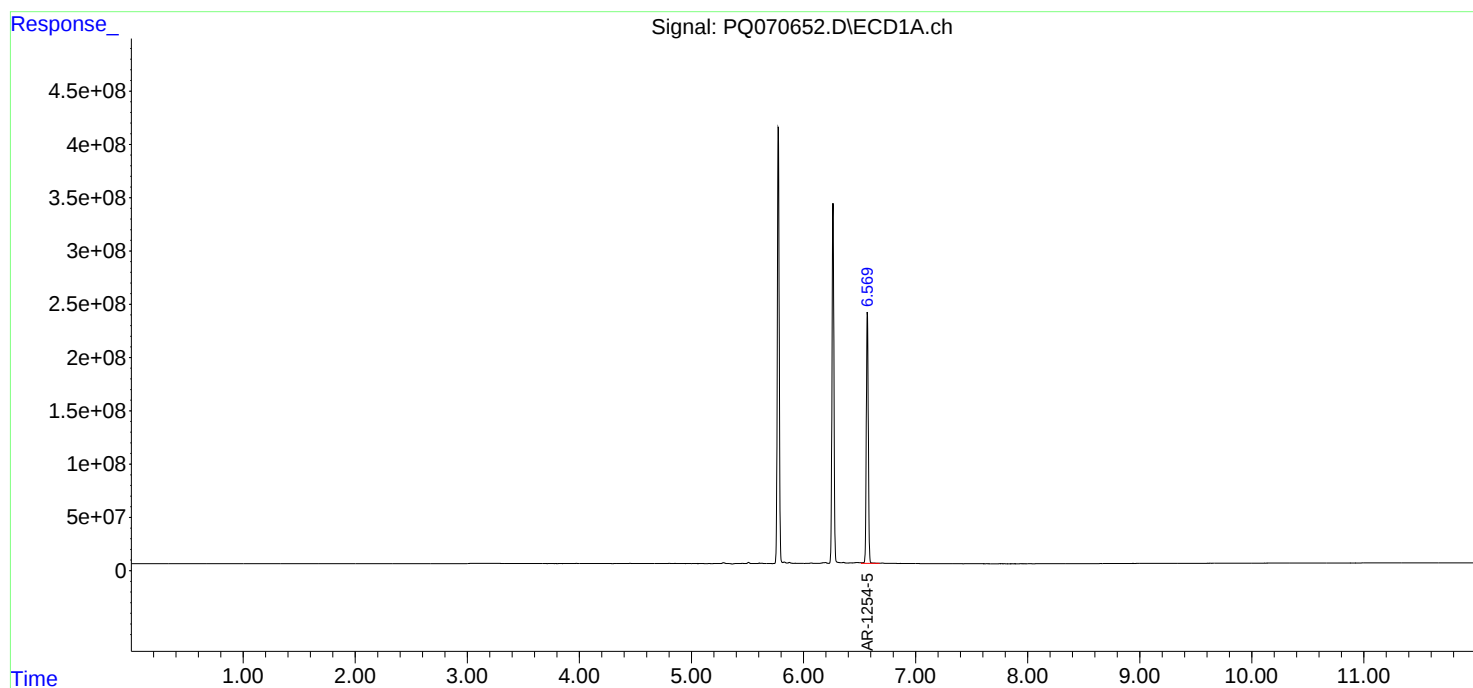


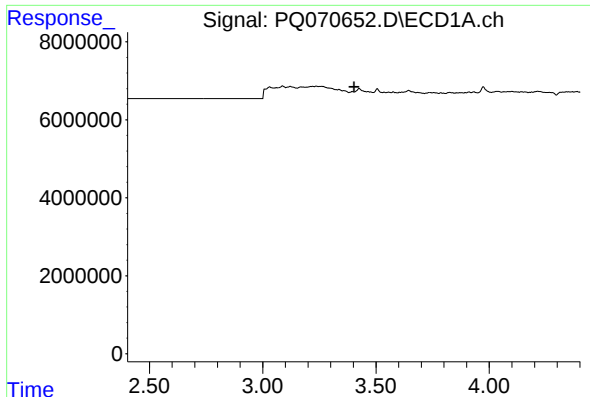

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.403 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
DDT ANALOG

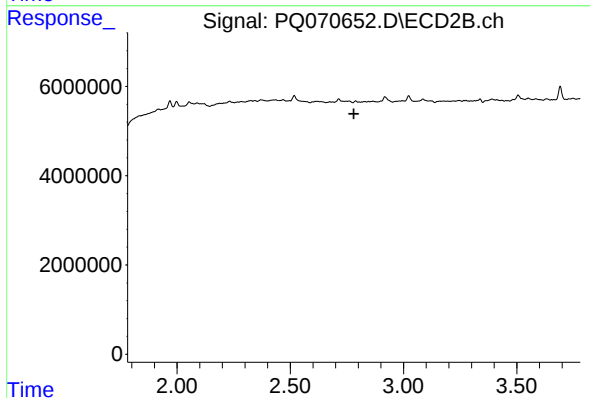


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 2.780 min
Response: 0
Conc: N.D.

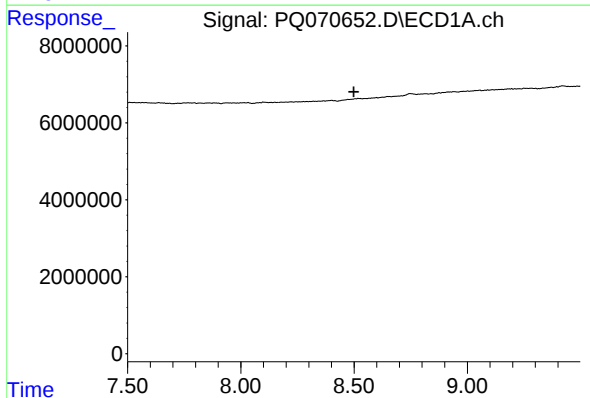


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.499 min
Response: 0
Conc: N.D.

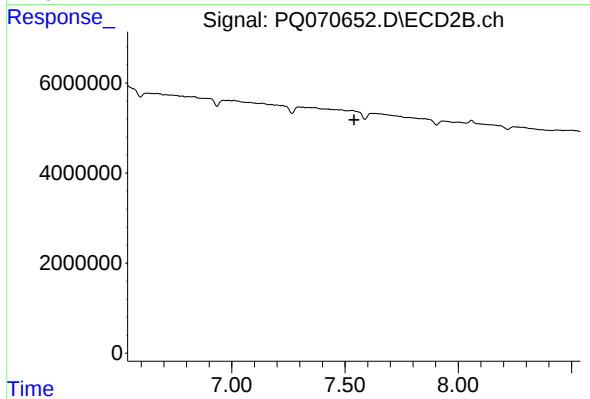

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T. : 7.540 min
Response: 0
Conc: N.D.

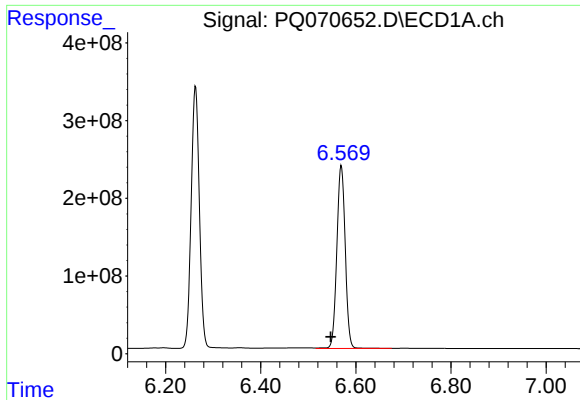

#30 AR-1254-5

R.T.: 6.569 min
Delta R.T.: 0.022 min
Response: 2882228675
Conc: 8200.81 ng/m

Instrument :
ECD_Q
ClientSampleId :
DDT ANALOG

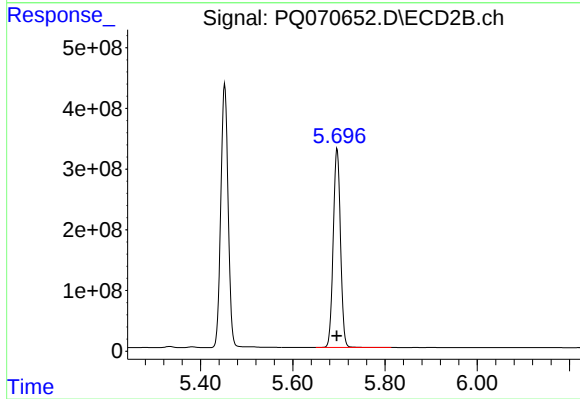

#30 AR-1254-5

R.T.: 5.696 min
Delta R.T.: 0.000 min
Response: 3577051079
Conc: 5882.12 ng/ml