

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ072921\
 Data File : PQ054149.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jul 2021 20:31
 Operator : AJ\MA
 Sample : M2940-07
 Misc : AR1268 LOD 25 PPB
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 04:17:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ072921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jul 30 02:37:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.204	4.208	394.8E6	224.5E6	16.906	15.879
2)	SA Decachlor...	11.376	9.545	342.5E6	277.6E6	20.358	22.010
Target Compounds							
3)	L1 AR-1016-1	0.000	5.496f	0	2870496	N.D.	6.341 #
4)	L1 AR-1016-2	0.000	5.496	0	2870496	N.D.	3.873 #
5)	L1 AR-1016-3	6.599f	5.681	2066973	432804	2.996	1.201 #
6)	L1 AR-1016-4	0.000	5.720	0	537709	N.D.	1.884 #
7)	L1 AR-1016-5	0.000	5.939f	0	1791932	N.D.	4.918 #
8)	L2 AR-1221-1	5.426f	0.000	1803756	0	7.455	N.D. #
9)	L2 AR-1221-2	5.562	4.565	8627703	2902304	47.629	27.512 #
10)	L2 AR-1221-3	0.000	4.639f	0	1510862	N.D.	4.305 #
11)	L3 AR-1232-1	0.000	4.639f	0	1510862	N.D.	6.473 #
12)	L3 AR-1232-2	0.000	5.496	0	2870496	N.D.	9.911 #
13)	L3 AR-1232-3	0.000	5.681	0	432804	N.D.	3.262 #
14)	L3 AR-1232-4	0.000	5.755f	0	2837290	N.D.	24.865 #
15)	L3 AR-1232-5	0.000	5.939f	0	1791932	N.D.	13.944 #
16)	L4 AR-1242-1	0.000	5.496f	0	2870496	N.D.	10.557 #
17)	L4 AR-1242-2	0.000	5.496	0	2870496	N.D.	6.099 #
18)	L4 AR-1242-3	6.599f	5.681	2066973	432804	4.748	1.962 #
19)	L4 AR-1242-4	0.000	5.755f	0	2837290	N.D.	13.115 #
20)	L4 AR-1242-5	0.000	6.344	0	1118258	N.D.	3.770 #
21)	L5 AR-1248-1	0.000	5.496f	0	2870496	N.D.	12.723 #
22)	L5 AR-1248-2	0.000	5.720f	0	537709	N.D.	1.638 #
23)	L5 AR-1248-3	0.000	5.755f	0	2837290	N.D.	8.580 #
24)	L5 AR-1248-4	0.000	5.939f	0	1791932	N.D.	4.515 #
25)	L5 AR-1248-5	0.000	6.385	0	1269291	N.D.	3.185 #
26)	L6 AR-1254-1	0.000	6.344	0	1118258	N.D.	1.672 #
27)	L6 AR-1254-2	0.000	6.501	0	777367	N.D.	1.264 #
28)	L6 AR-1254-3	0.000	6.949f	0	2822268	N.D.	2.923 #
29)	L6 AR-1254-4	0.000	7.179f	0	4681896	N.D.	7.025 #
30)	L6 AR-1254-5	0.000	7.594	0	1399439	N.D.	1.435 #
31)	L7 AR-1260-1	8.243f	7.061	2155557	5835353	2.195	7.785 #
32)	L7 AR-1260-2	8.491	7.236f	3631942	3649103	3.199	3.493
33)	L7 AR-1260-3	8.844	7.403	10067652	6289840	14.232	7.227 #
34)	L7 AR-1260-4	9.102	7.892	12919448	14974796	14.604	24.051 #
35)	L7 AR-1260-5	9.429	8.141	5855464	5857323	3.478	3.419
36)	L8 AR-1262-1	8.844	7.594	10067652	1399439	10.178	3.097 #
37)	L8 AR-1262-2	9.429	8.141	5855464	5857323	3.244	3.110
38)	L8 AR-1262-3	9.760	8.428	56174993	55527564	45.847	72.330 #
39)	L8 AR-1262-4	9.863	8.493	52686064	48131129	58.197	38.500 #
40)	L8 AR-1262-5	10.572	8.993	22303279	17443114	33.649	30.224
41)	L9 AR-1268-1	9.760	8.428	56174993	55527564	26.634	24.618

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ072921\
 Data File : PQ054149.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jul 2021 20:31
 Operator : AJ\MA
 Sample : M2940-07
 Misc : AR1268 LOD 25 PPB
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 04:17:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ072921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jul 30 02:37:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	9.863	8.493	52686064	48131129	27.315	25.768
43) L9	AR-1268-3	10.103	8.700	42695509	43088600	26.520	25.776
44) L9	AR-1268-4	10.572	8.993	22303279	17443114	30.492	26.748
45) L9	AR-1268-5	11.015	9.288	144.1E6	123.2E6	26.423	26.143



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ072921\
Data File : PQ054149.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jul 2021 20:31
Operator : AJ\MA
Sample : M2940-07
Misc : AR1268 LOD 25 PPB
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 30 04:17:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ072921.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 30 02:37:02 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

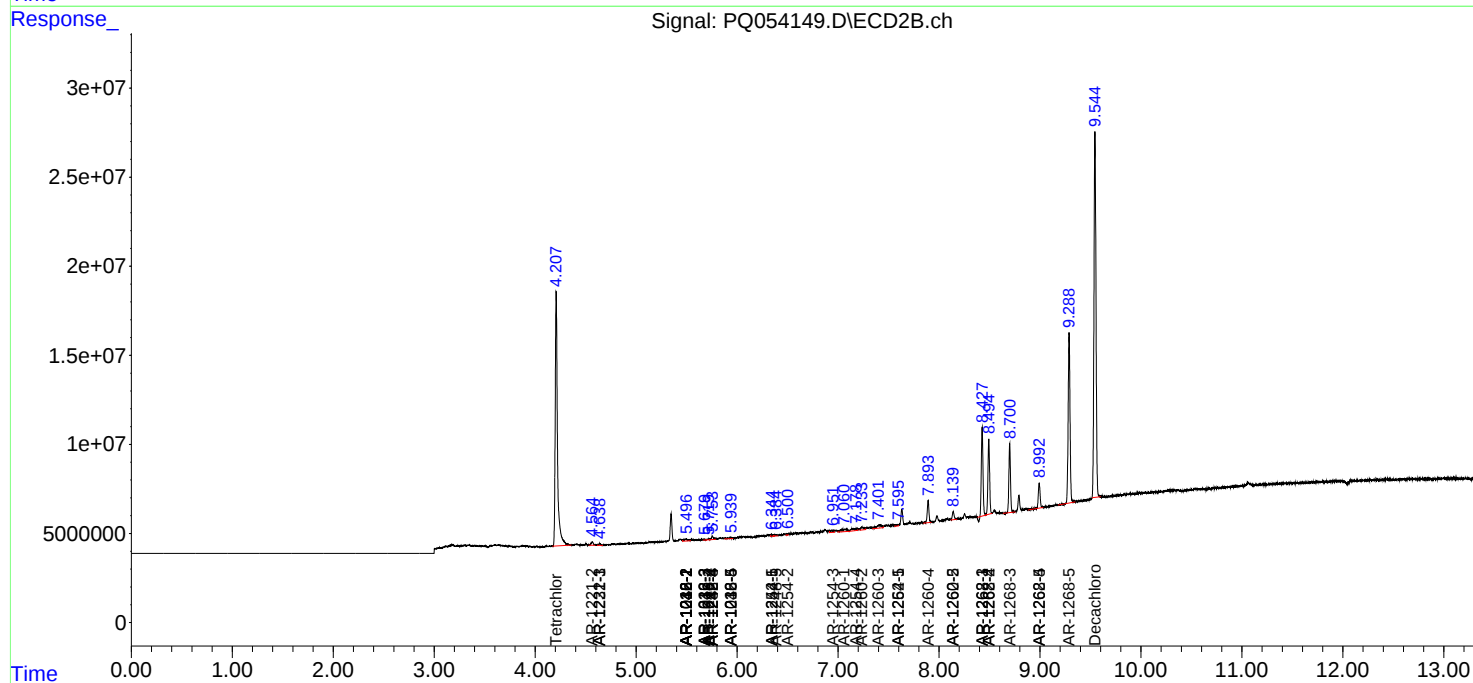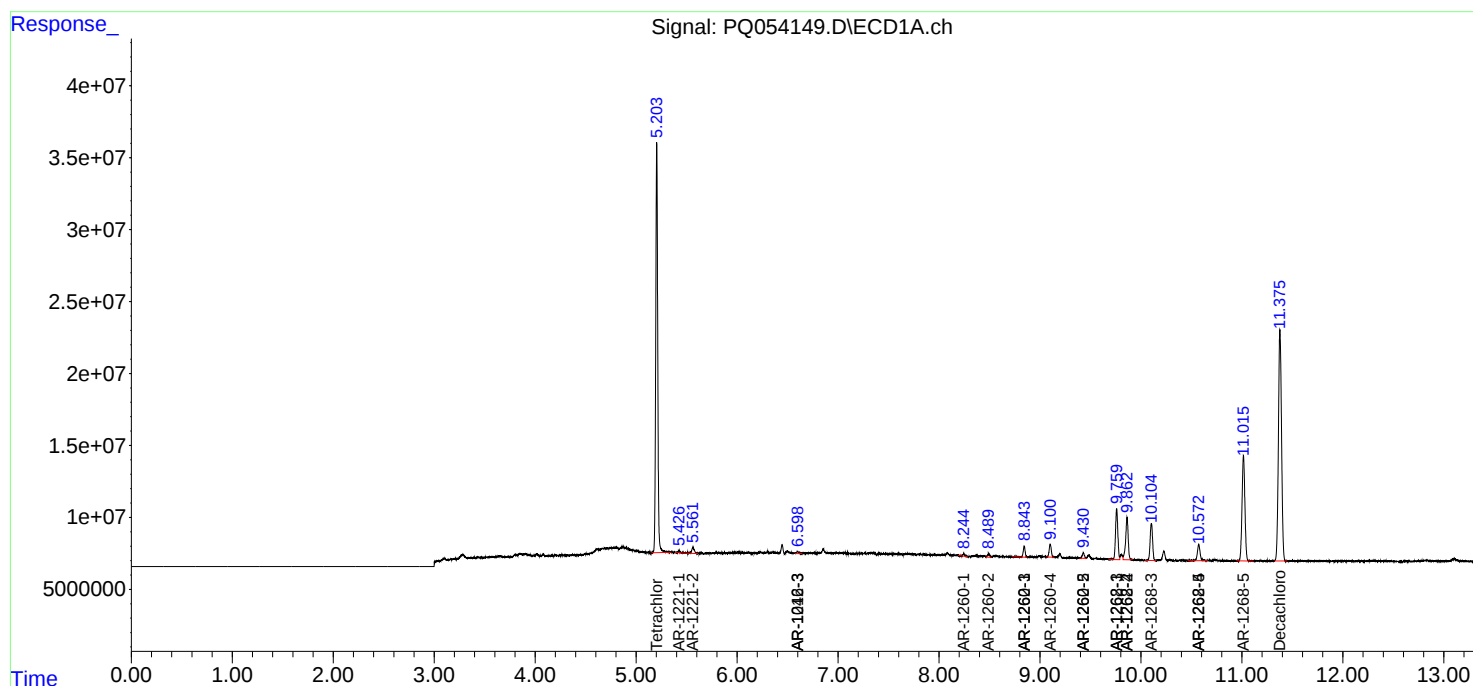


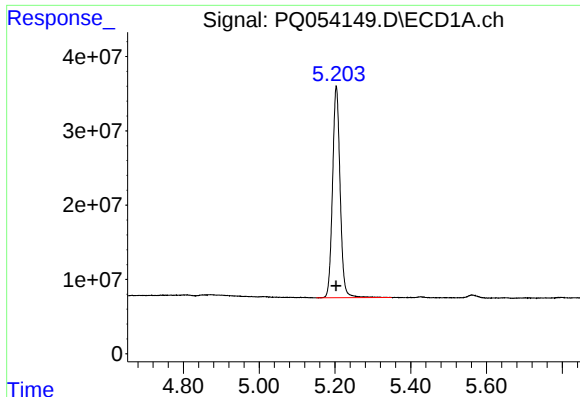

#1 Tetrachloro-m-xylene


R.T.: 5.204 min
Delta R.T.: 0.000 min
Response: 394798879
Conc: 16.91 ng/ml

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

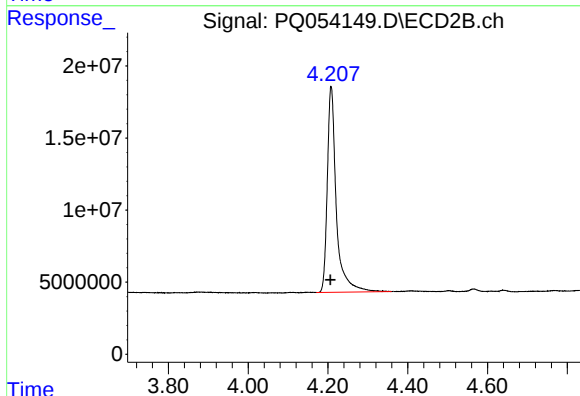


#1 Tetrachloro-m-xylene

R.T.: 4.208 min
Delta R.T.: 0.002 min
Response: 224484989
Conc: 15.88 ng/ml

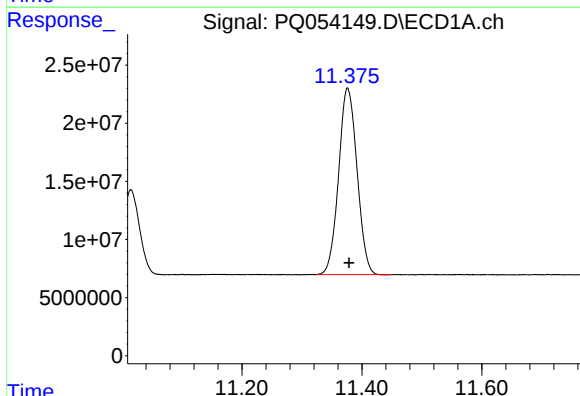


#2 Decachlorobiphenyl

R.T.: 11.376 min
Delta R.T.: -0.003 min
Response: 342537278
Conc: 20.36 ng/ml

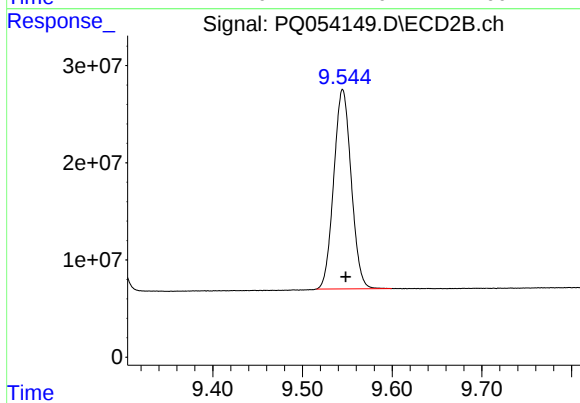

#2 Decachlorobiphenyl


R.T.: 9.545 min
Delta R.T.: -0.003 min
Response: 277638791
Conc: 22.01 ng/ml

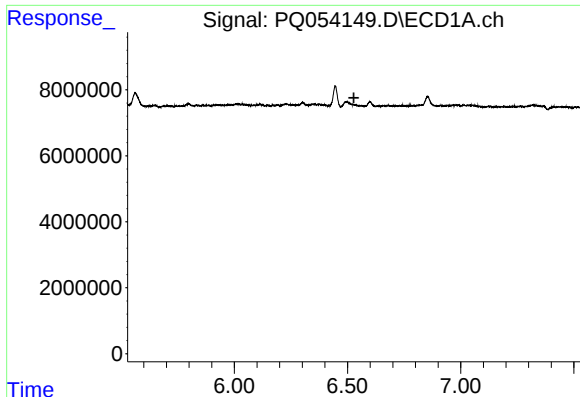

#3 AR-1016-1


R.T.: 0.000 min
Exp R.T.: 6.528 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

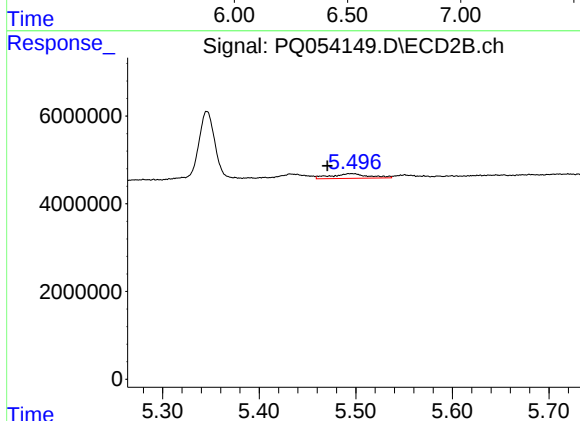


#3 AR-1016-1

R.T.: 5.496 min
Delta R.T.: 0.026 min
Response: 2870496
Conc: 6.34 ng/ml

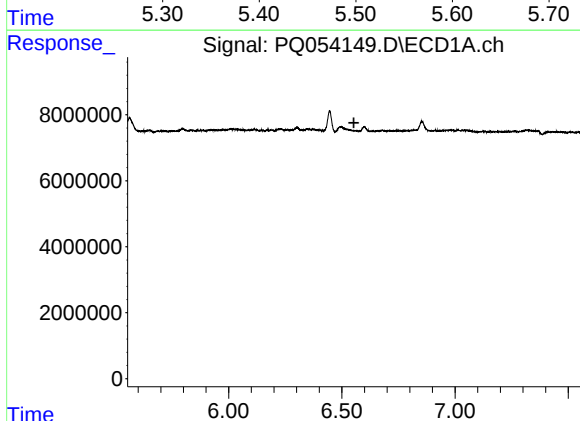


#4 AR-1016-2

R.T.: 0.000 min
Exp R.T.: 6.553 min
Response: 0
Conc: N.D.

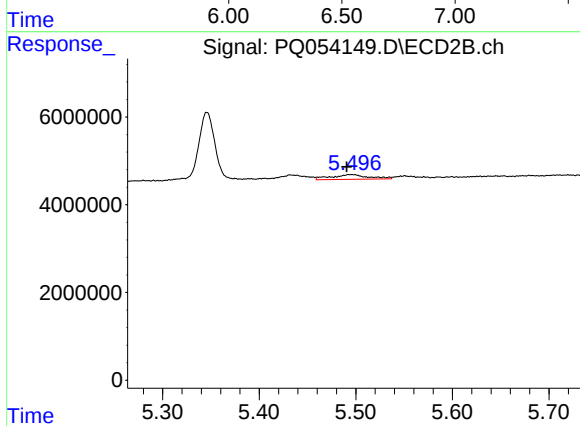

#4 AR-1016-2


R.T.: 5.496 min
Delta R.T.: 0.006 min
Response: 2870496
Conc: 3.87 ng/ml

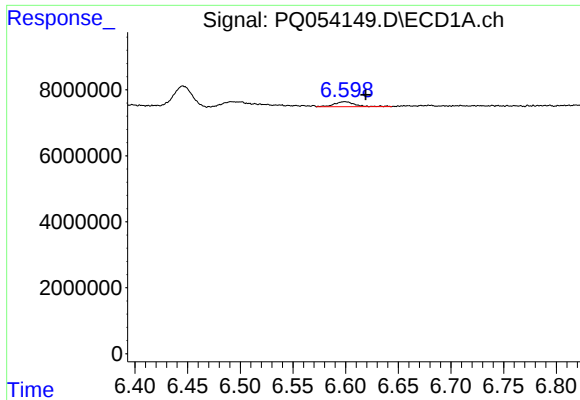

#5 AR-1016-3


R.T.: 6.599 min
Delta R.T.: -0.020 min
Response: 2066973
Conc: 3.00 ng/ml

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

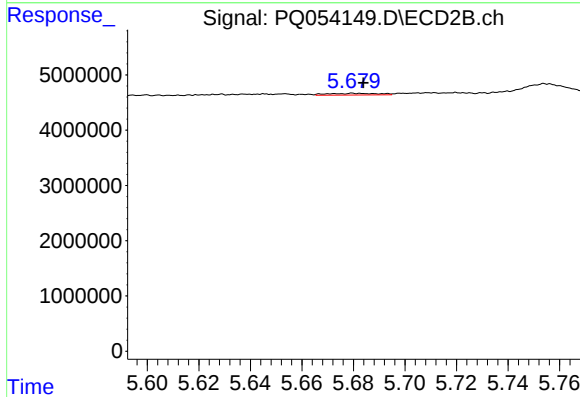


#5 AR-1016-3

R.T.: 5.681 min
Delta R.T.: -0.003 min
Response: 432804
Conc: 1.20 ng/ml

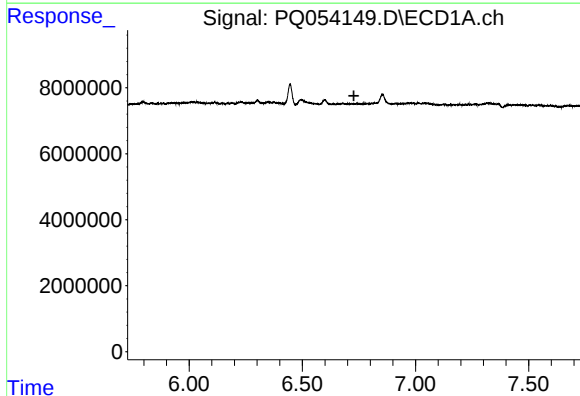


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T. : 6.728 min
Response: 0
Conc: N.D.

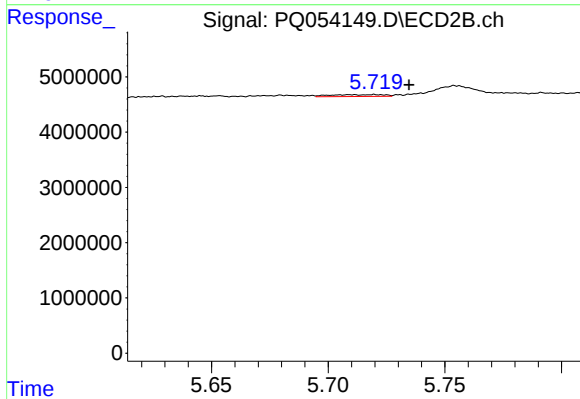

#6 AR-1016-4


R.T.: 5.720 min
Delta R.T.: -0.015 min
Response: 537709
Conc: 1.88 ng/ml

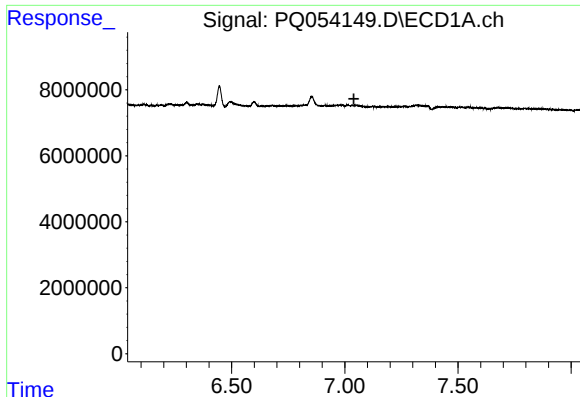

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 7.040 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

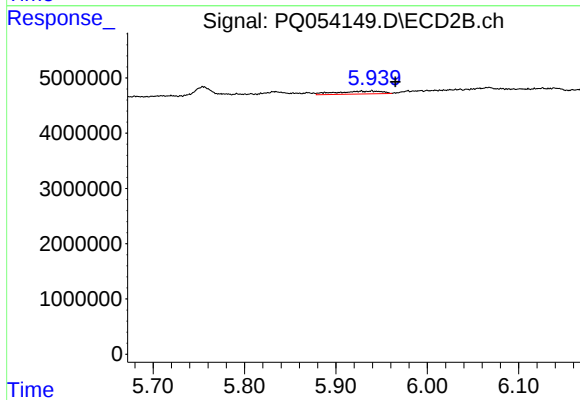


#7 AR-1016-5

R.T.: 5.939 min
Delta R.T.: -0.026 min
Response: 1791932
Conc: 4.92 ng/ml

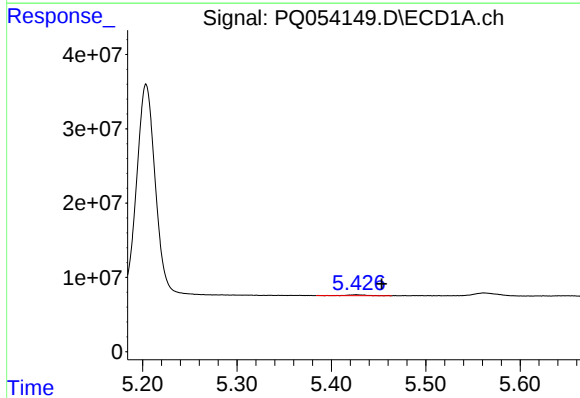


#8 AR-1221-1

R.T.: 5.426 min
Delta R.T.: -0.027 min
Response: 1803756
Conc: 7.46 ng/ml

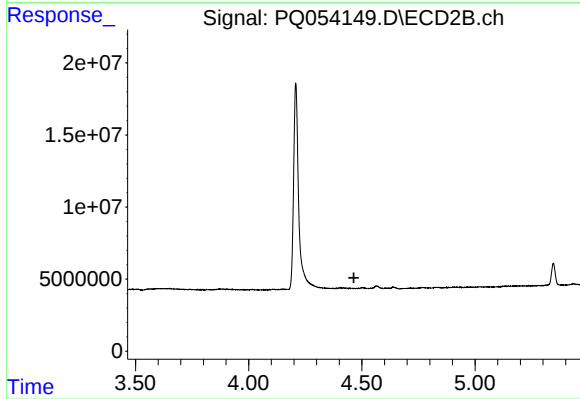

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T.: 4.465 min
Response: 0
Conc: N.D.

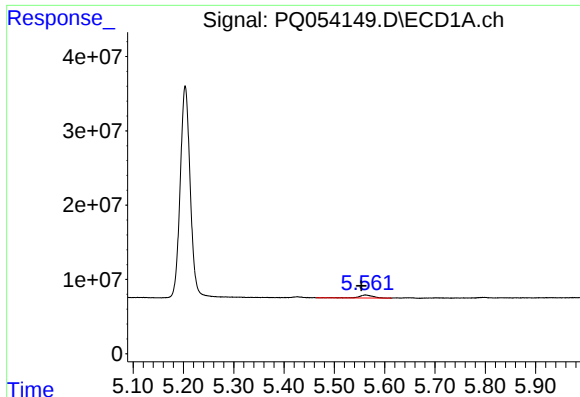

#9 AR-1221-2


R.T.: 5.562 min
Delta R.T.: 0.008 min
Response: 8627703
Conc: 47.63 ng/ml

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

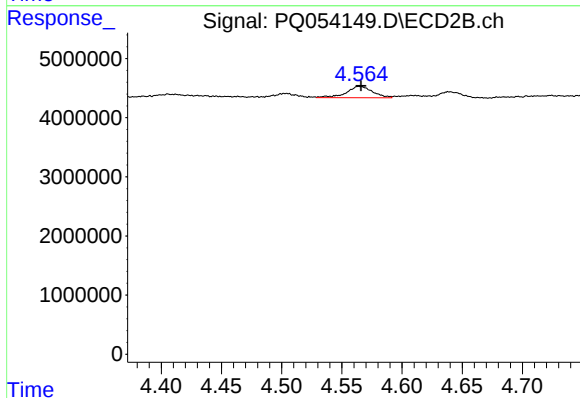


#9 AR-1221-2

R.T.: 4.565 min
Delta R.T.: -0.001 min
Response: 2902304
Conc: 27.51 ng/ml

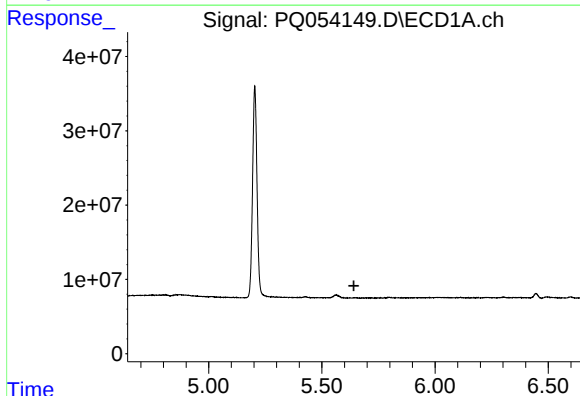


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 5.641 min
Response: 0
Conc: N.D.

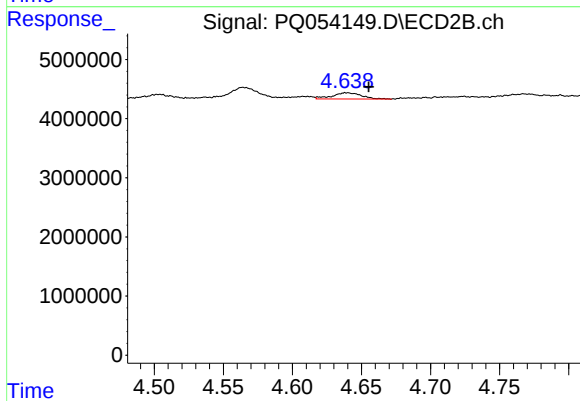

#10 AR-1221-3


R.T.: 4.639 min
Delta R.T.: -0.016 min
Response: 1510862
Conc: 4.31 ng/ml

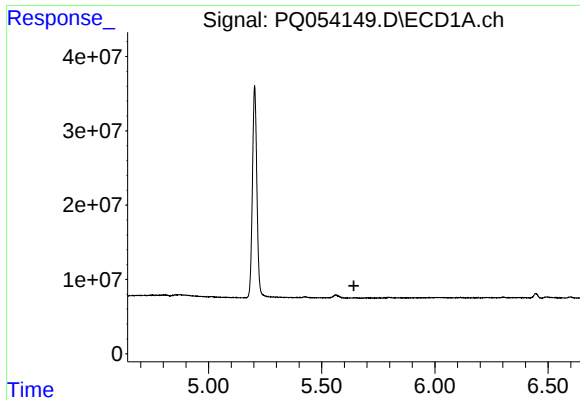

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T.: 5.642 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

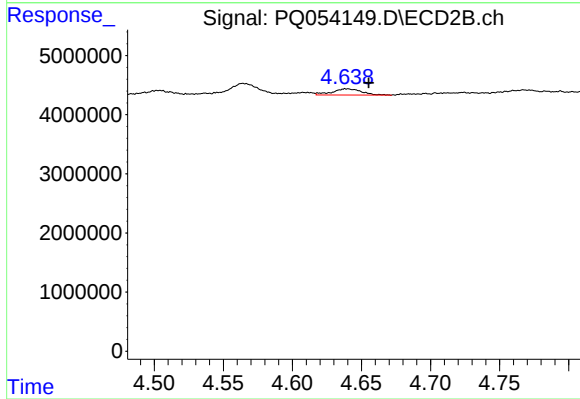


#11 AR-1232-1

R.T.: 4.639 min
Delta R.T.: -0.016 min
Response: 1510862
Conc: 6.47 ng/ml

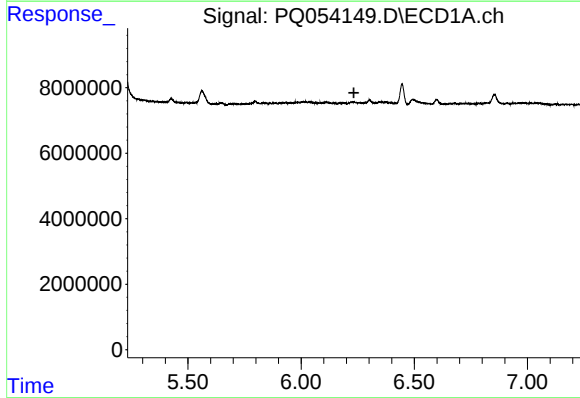


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T.: 6.233 min
Response: 0
Conc: N.D.

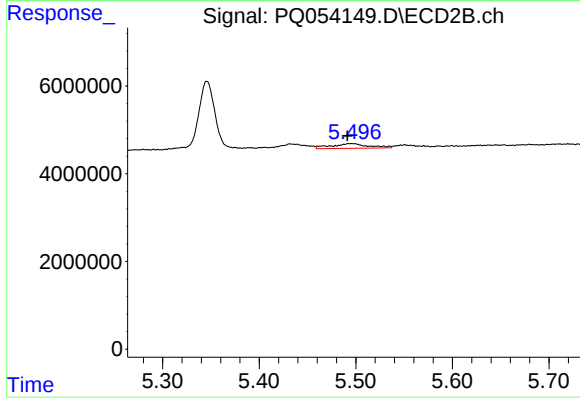

#12 AR-1232-2


R.T.: 5.496 min
Delta R.T.: 0.005 min
Response: 2870496
Conc: 9.91 ng/ml

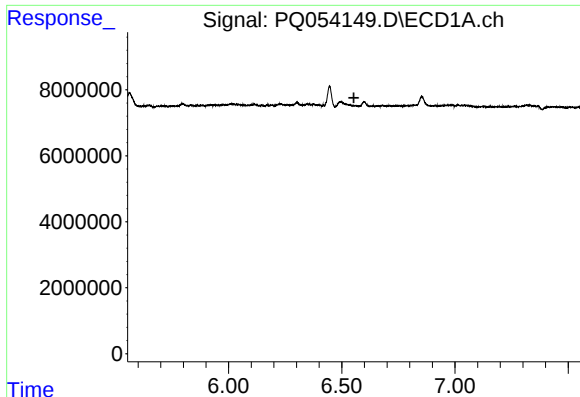

#13 AR-1232-3


R.T.: 0.000 min
Exp R.T.: 6.554 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

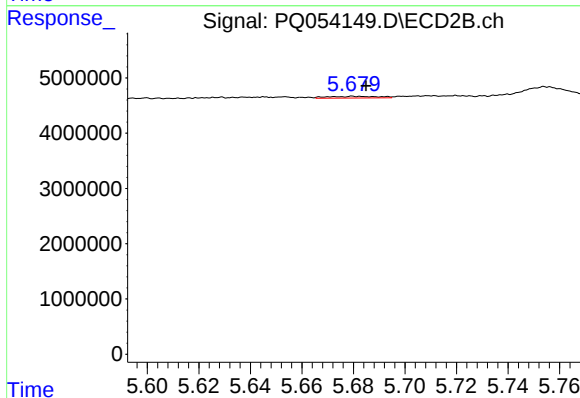


#13 AR-1232-3

R.T.: 5.681 min
Delta R.T.: -0.004 min
Response: 432804
Conc: 3.26 ng/ml

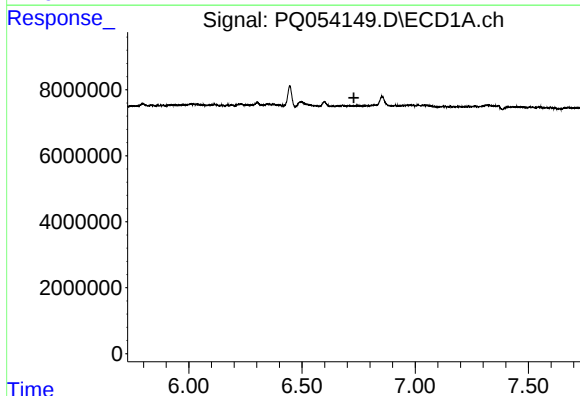


#14 AR-1232-4

R.T.: 0.000 min
Exp R.T.: 6.729 min
Response: 0
Conc: N.D.

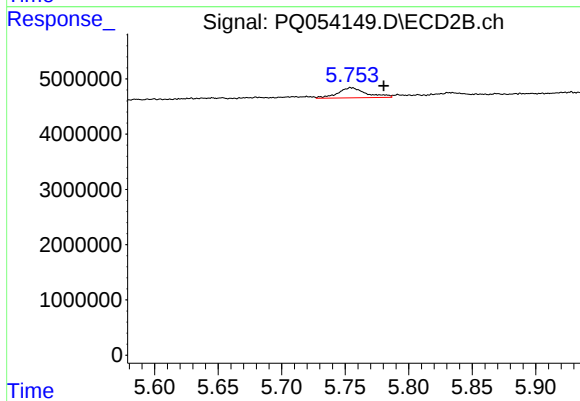

#14 AR-1232-4


R.T.: 5.755 min
Delta R.T.: -0.025 min
Response: 2837290
Conc: 24.86 ng/ml

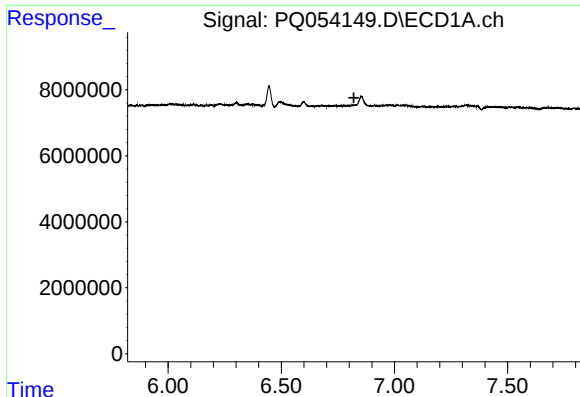

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T.: 6.821 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

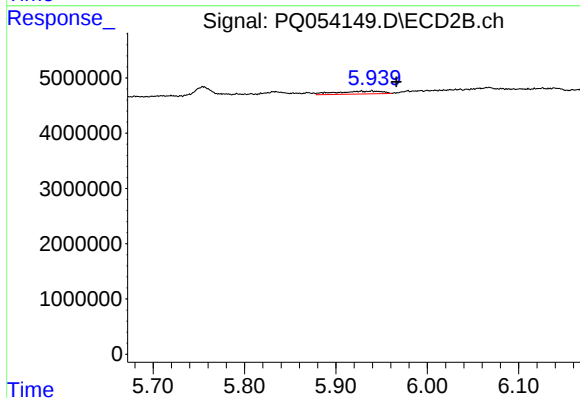


#15 AR-1232-5

R.T.: 5.939 min
Delta R.T.: -0.027 min
Response: 1791932
Conc: 13.94 ng/ml

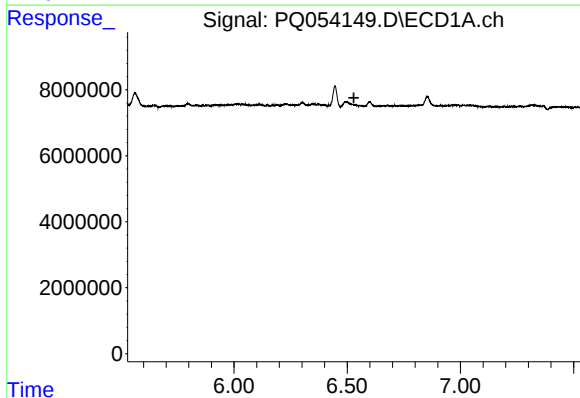


#16 AR-1242-1

R.T.: 0.000 min
Exp R.T.: 6.530 min
Response: 0
Conc: N.D.

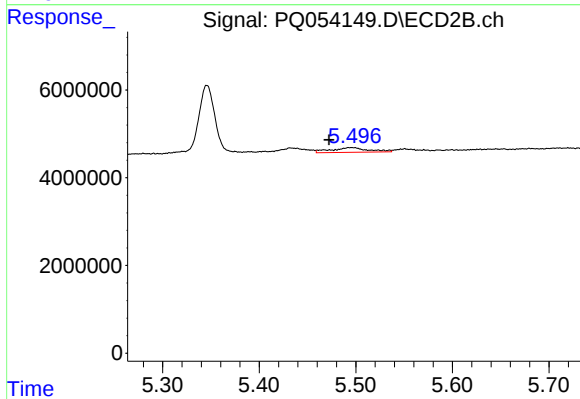

#16 AR-1242-1


R.T.: 5.496 min
Delta R.T.: 0.024 min
Response: 2870496
Conc: 10.56 ng/ml

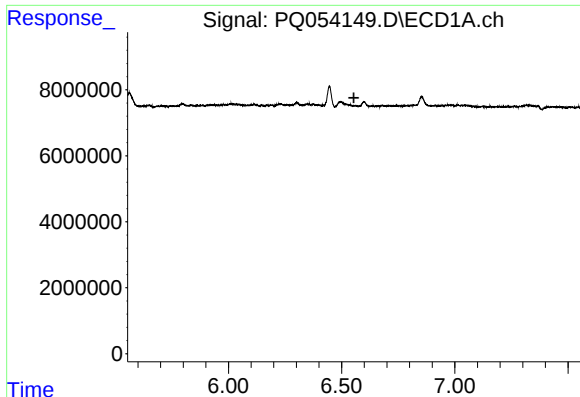

#17 AR-1242-2


R.T.: 0.000 min
Exp R.T.: 6.554 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

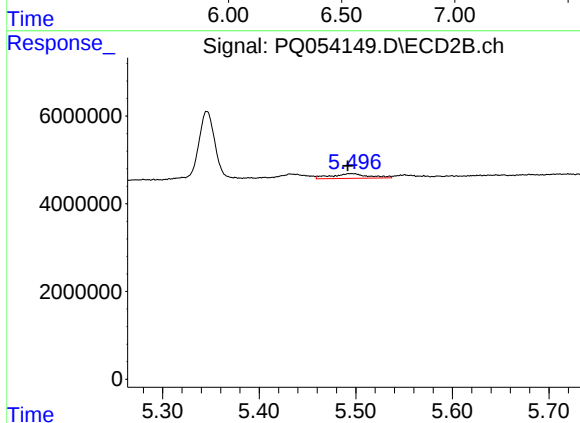


#17 AR-1242-2

R.T.: 5.496 min
Delta R.T.: 0.005 min
Response: 2870496
Conc: 6.10 ng/ml

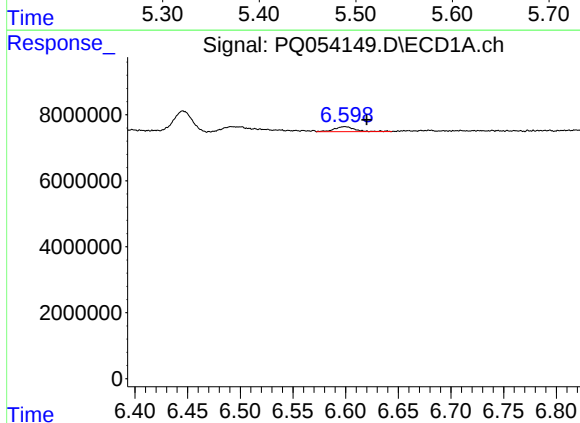


#18 AR-1242-3

R.T.: 6.599 min
Delta R.T.: -0.021 min
Response: 2066973
Conc: 4.75 ng/ml

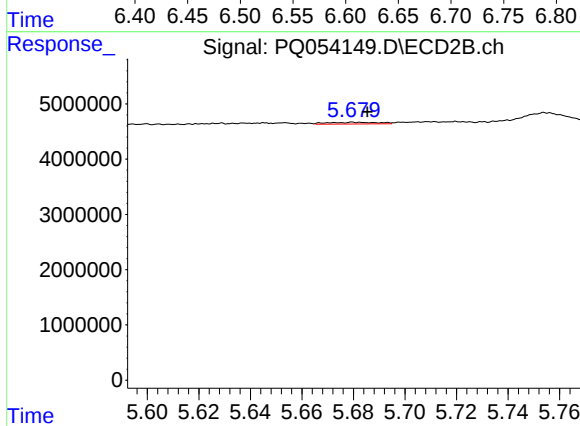

#18 AR-1242-3


R.T.: 5.681 min
Delta R.T.: -0.005 min
Response: 432804
Conc: 1.96 ng/ml

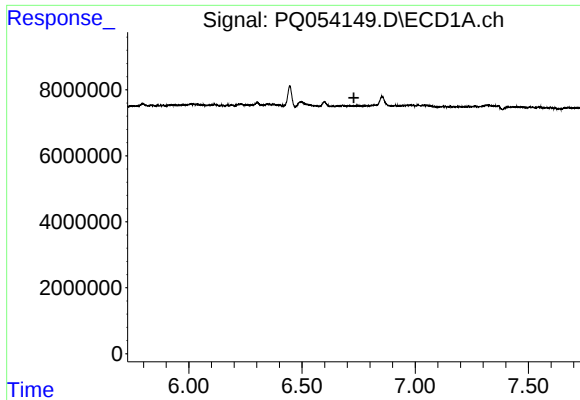

#19 AR-1242-4


R.T.: 0.000 min
Exp R.T.: 6.729 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

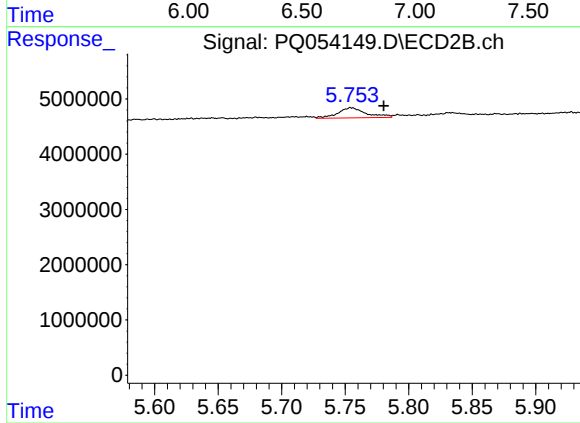


#19 AR-1242-4

R.T.: 5.755 min
Delta R.T.: -0.026 min
Response: 2837290
Conc: 13.11 ng/ml

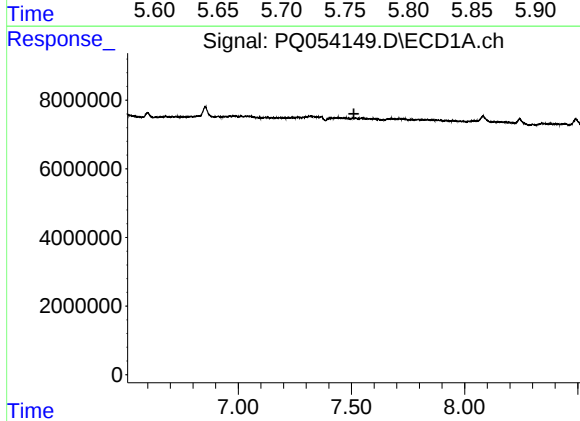


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T.: 7.511 min
Response: 0
Conc: N.D.

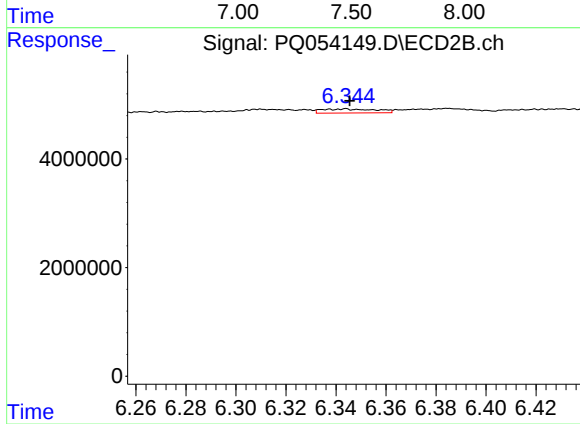

#20 AR-1242-5


R.T.: 6.344 min
Delta R.T.: -0.002 min
Response: 1118258
Conc: 3.77 ng/ml

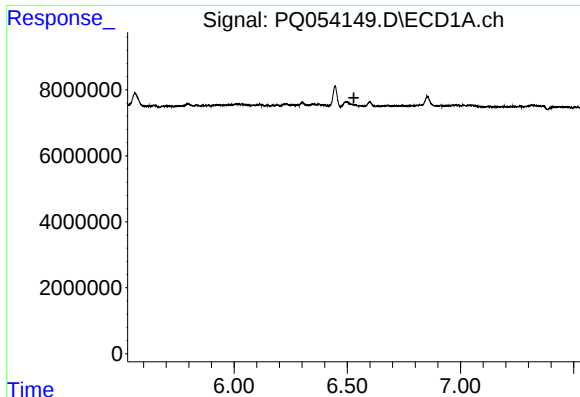

#21 AR-1248-1


R.T.: 0.000 min
Exp R.T.: 6.529 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

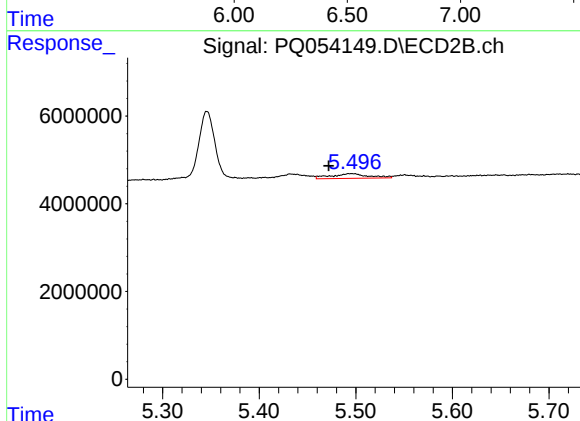


#21 AR-1248-1

R.T.: 5.496 min
Delta R.T.: 0.024 min
Response: 2870496
Conc: 12.72 ng/ml

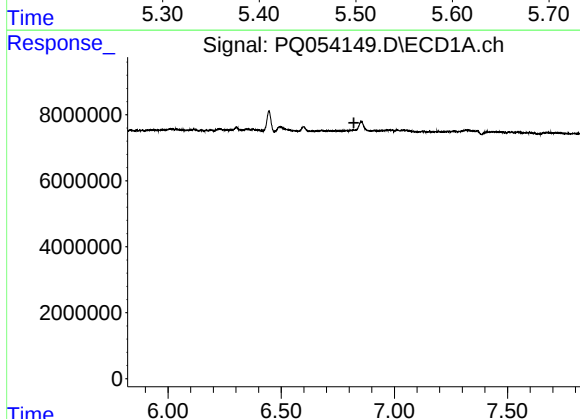


#22 AR-1248-2

R.T.: 0.000 min
Exp R.T.: 6.821 min
Response: 0
Conc: N.D.

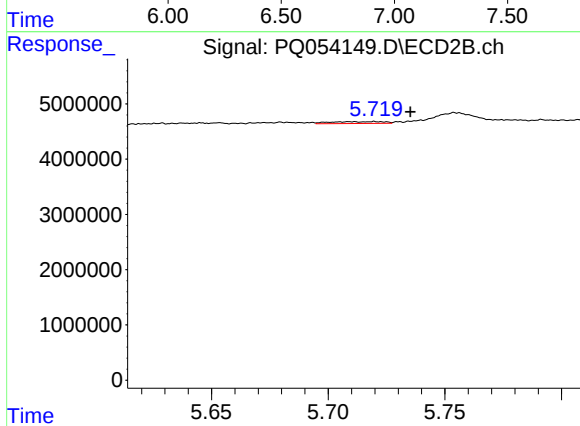

#22 AR-1248-2


R.T.: 5.720 min
Delta R.T.: -0.015 min
Response: 537709
Conc: 1.64 ng/ml

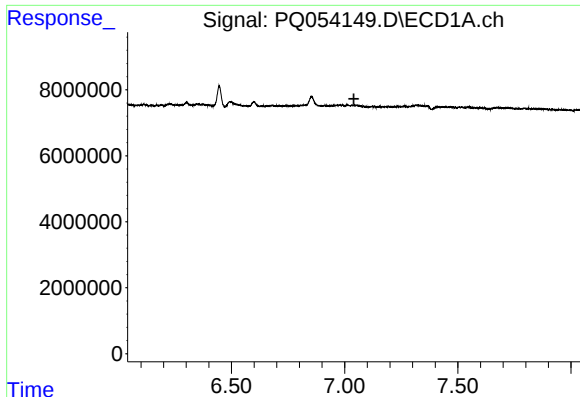

#23 AR-1248-3


R.T.: 0.000 min
Exp R.T.: 7.041 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

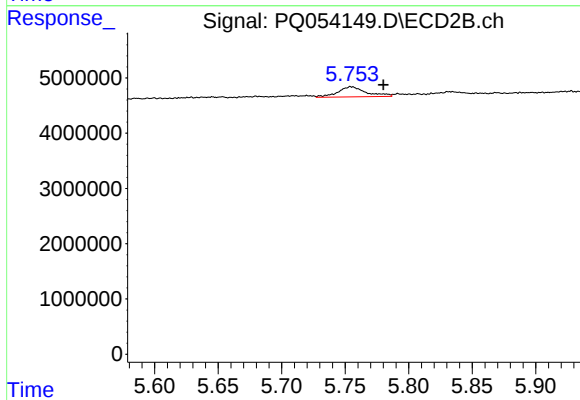


#23 AR-1248-3

R.T.: 5.755 min
Delta R.T.: -0.025 min
Response: 2837290
Conc: 8.58 ng/ml

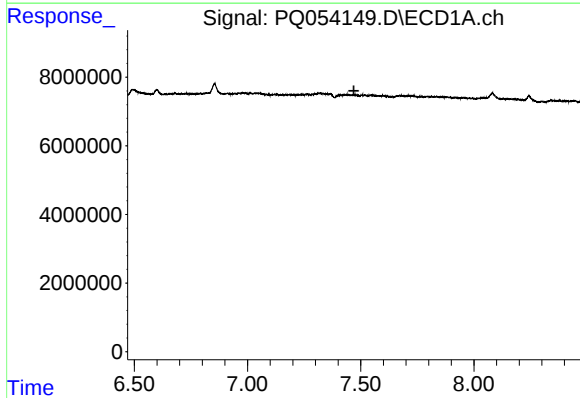


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T.: 7.470 min
Response: 0
Conc: N.D.

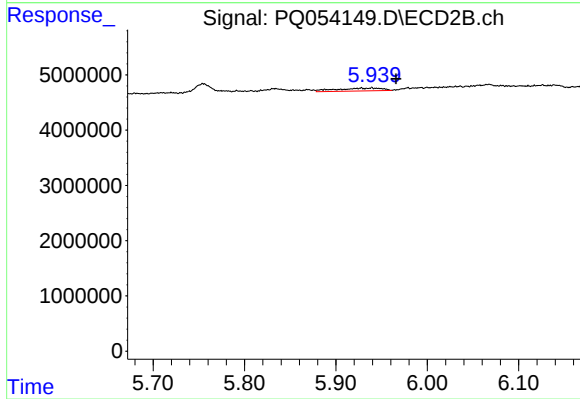

#24 AR-1248-4


R.T.: 5.939 min
Delta R.T.: -0.027 min
Response: 1791932
Conc: 4.52 ng/ml

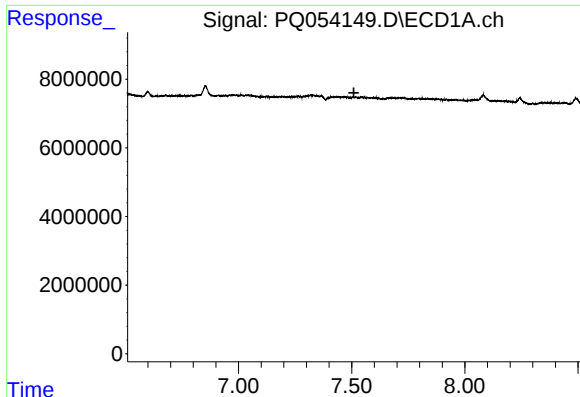

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 7.510 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

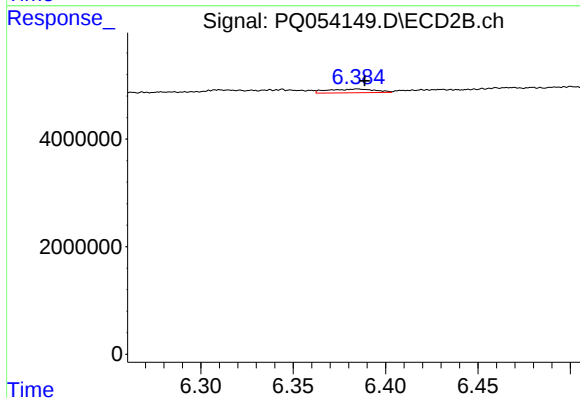


#25 AR-1248-5

R.T.: 6.385 min
Delta R.T.: -0.004 min
Response: 1269291
Conc: 3.18 ng/ml

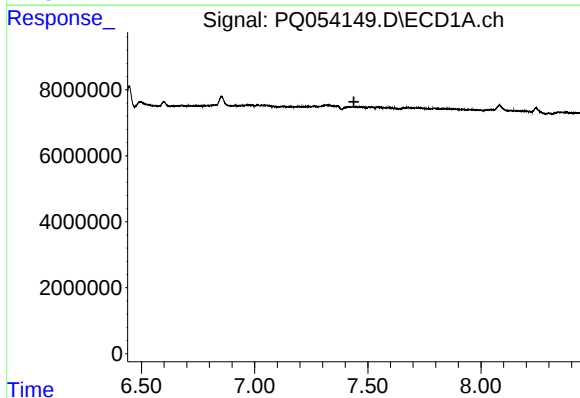


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T.: 7.439 min
Response: 0
Conc: N.D.

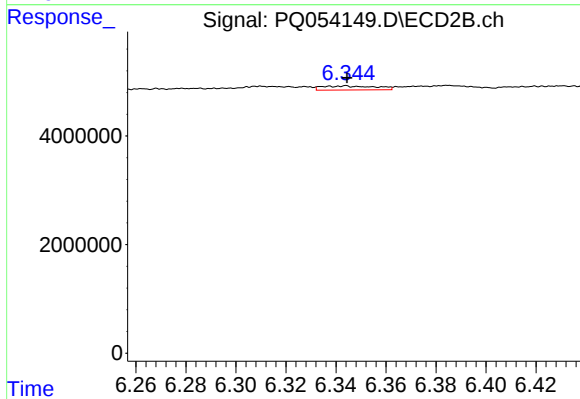

#26 AR-1254-1


R.T.: 6.344 min
Delta R.T.: 0.000 min
Response: 1118258
Conc: 1.67 ng/ml

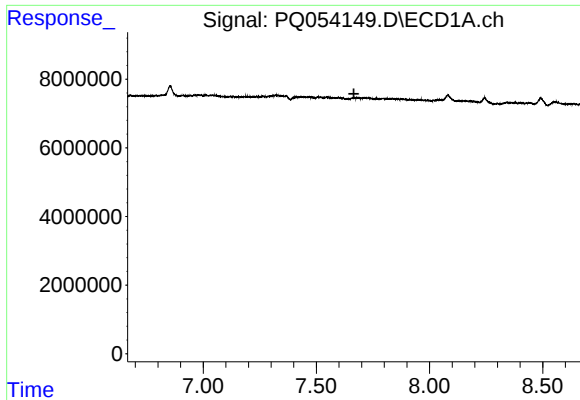

#27 AR-1254-2


R.T.: 0.000 min
Exp R.T.: 7.666 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

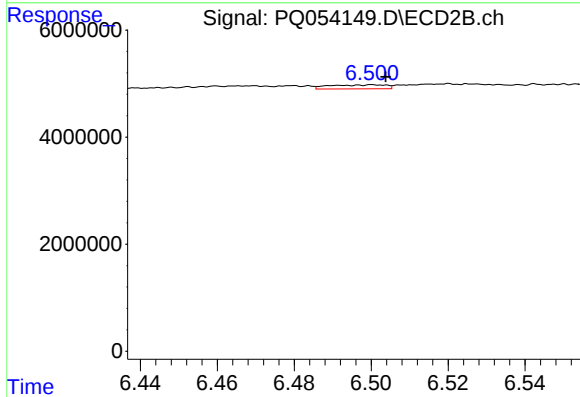


#27 AR-1254-2

R.T.: 6.501 min
Delta R.T.: -0.003 min
Response: 777367
Conc: 1.26 ng/ml

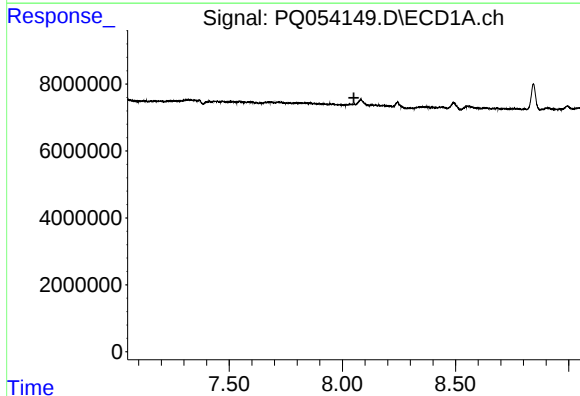


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T.: 8.051 min
Response: 0
Conc: N.D.

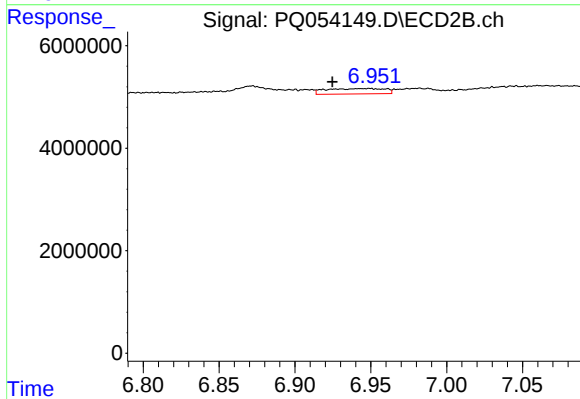

#28 AR-1254-3


R.T.: 6.949 min
Delta R.T.: 0.024 min
Response: 2822268
Conc: 2.92 ng/ml

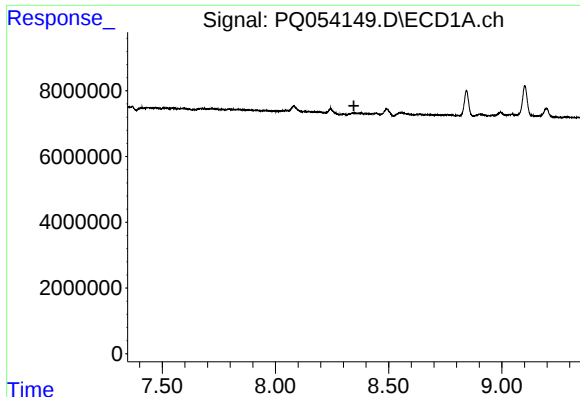

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T.: 8.346 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

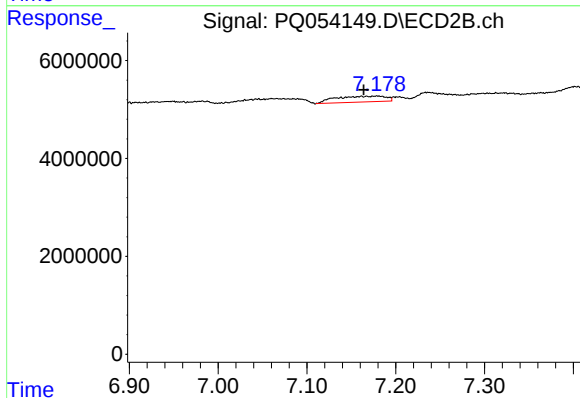


#29 AR-1254-4

R.T.: 7.179 min
Delta R.T.: 0.015 min
Response: 4681896
Conc: 7.03 ng/ml

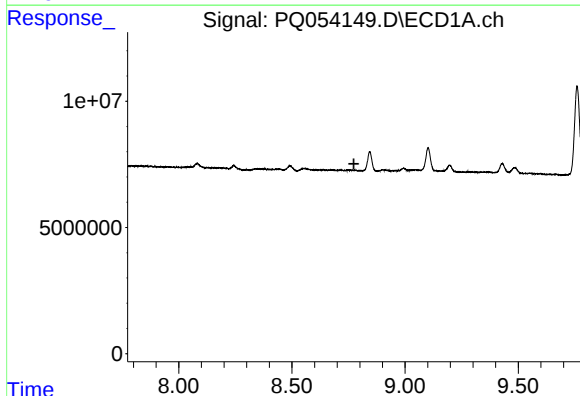


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T.: 8.774 min
Response: 0
Conc: N.D.

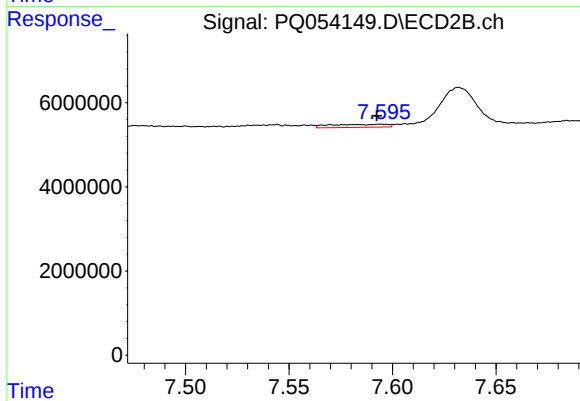

#30 AR-1254-5


R.T.: 7.594 min
Delta R.T.: 0.002 min
Response: 1399439
Conc: 1.43 ng/ml

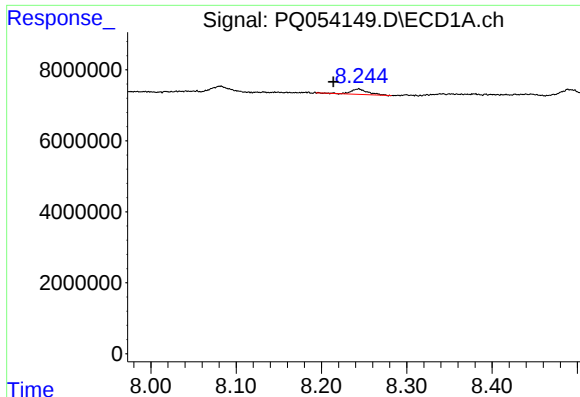

#31 AR-1260-1


R.T.: 8.243 min
Delta R.T.: 0.029 min
Response: 2155557
Conc: 2.20 ng/ml

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

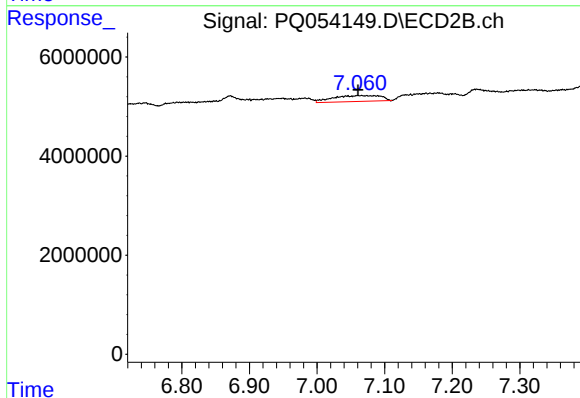


#31 AR-1260-1

R.T.: 7.061 min
Delta R.T.: 0.000 min
Response: 5835353
Conc: 7.78 ng/ml

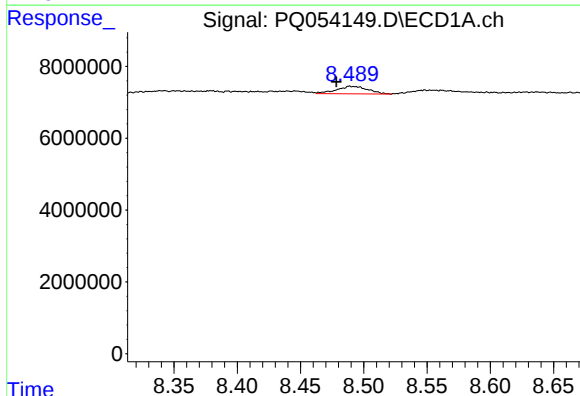


#32 AR-1260-2

R.T.: 8.491 min
Delta R.T.: 0.013 min
Response: 3631942
Conc: 3.20 ng/ml

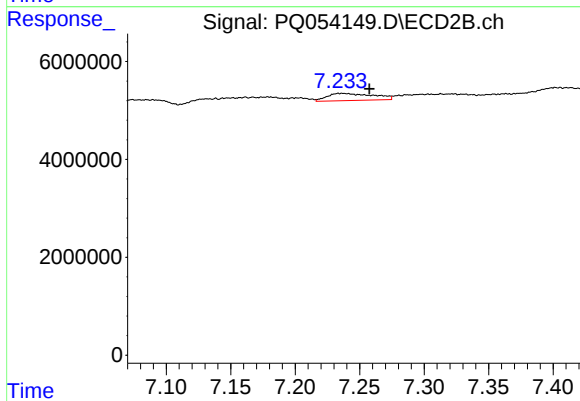

#32 AR-1260-2


R.T.: 7.236 min
Delta R.T.: -0.021 min
Response: 3649103
Conc: 3.49 ng/ml

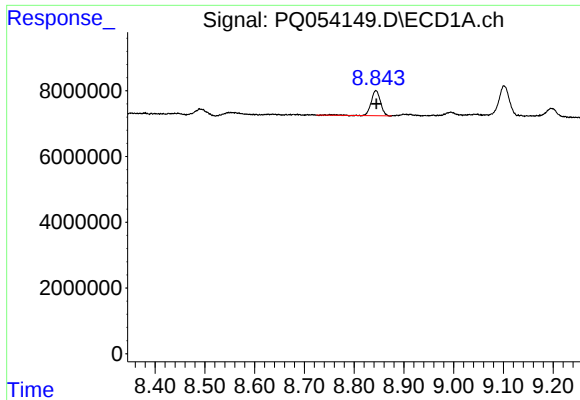

#33 AR-1260-3


R.T.: 8.844 min
Delta R.T.: 0.000 min
Response: 10067652
Conc: 14.23 ng/ml

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

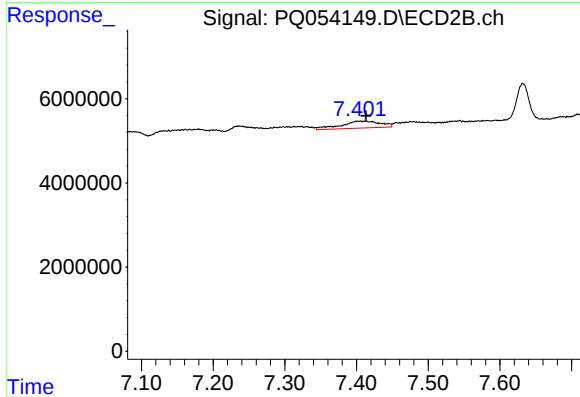


#33 AR-1260-3

R.T.: 7.403 min
Delta R.T.: -0.011 min
Response: 6289840
Conc: 7.23 ng/ml

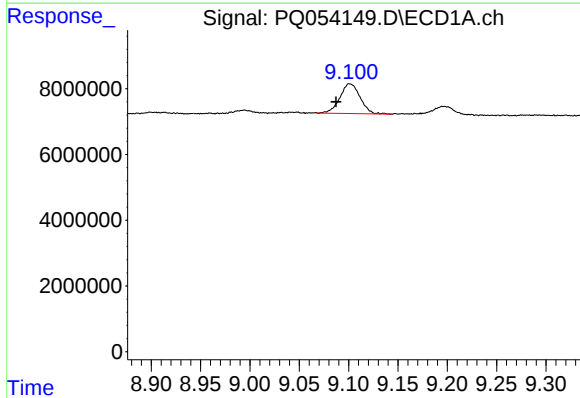


#34 AR-1260-4

R.T.: 9.102 min
Delta R.T.: 0.014 min
Response: 12919448
Conc: 14.60 ng/ml

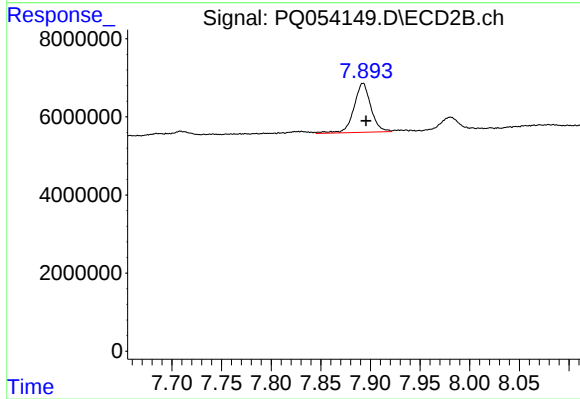

#34 AR-1260-4


R.T.: 7.892 min
Delta R.T.: -0.003 min
Response: 14974796
Conc: 24.05 ng/ml

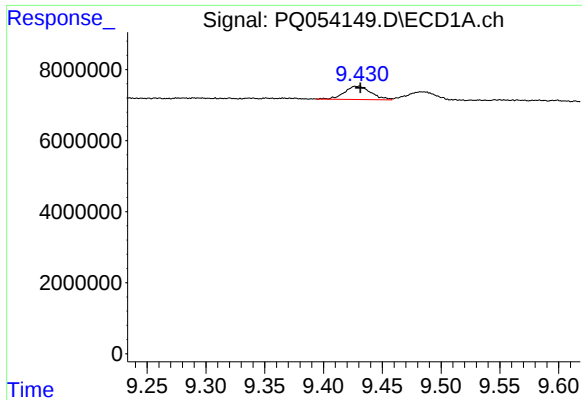

#35 AR-1260-5


R.T.: 9.429 min
Delta R.T.: -0.002 min
Response: 5855464
Conc: 3.48 ng/ml

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

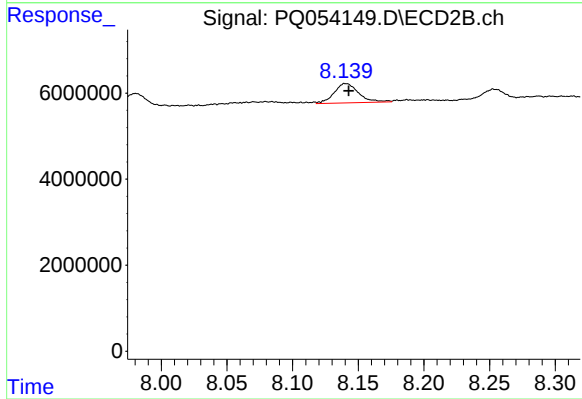


#35 AR-1260-5

R.T.: 8.141 min
Delta R.T.: -0.002 min
Response: 5857323
Conc: 3.42 ng/ml

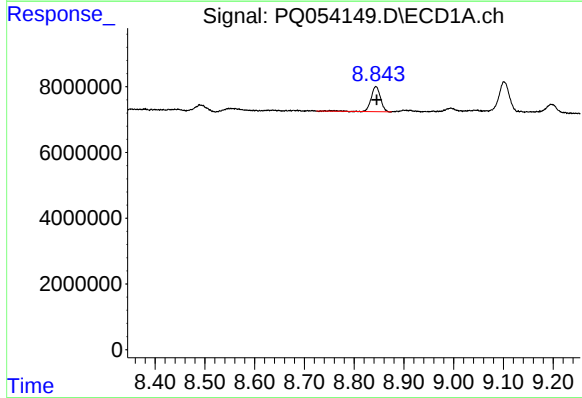


#36 AR-1262-1

R.T.: 8.844 min
Delta R.T.: -0.001 min
Response: 10067652
Conc: 10.18 ng/ml

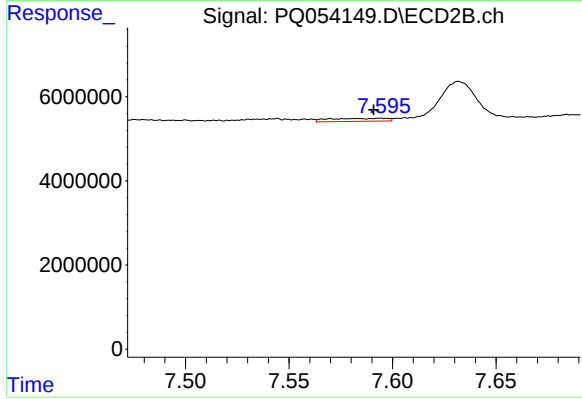

#36 AR-1262-1


R.T.: 7.594 min
Delta R.T.: 0.004 min
Response: 1399439
Conc: 3.10 ng/ml

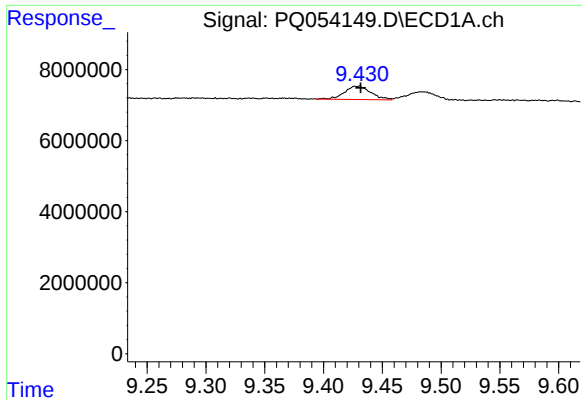

#37 AR-1262-2


R.T.: 9.429 min
Delta R.T.: -0.003 min
Response: 5855464
Conc: 3.24 ng/ml

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

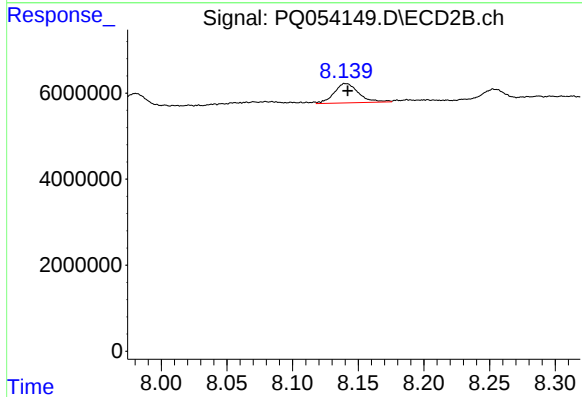


#37 AR-1262-2

R.T.: 8.141 min
Delta R.T.: -0.001 min
Response: 5857323
Conc: 3.11 ng/ml

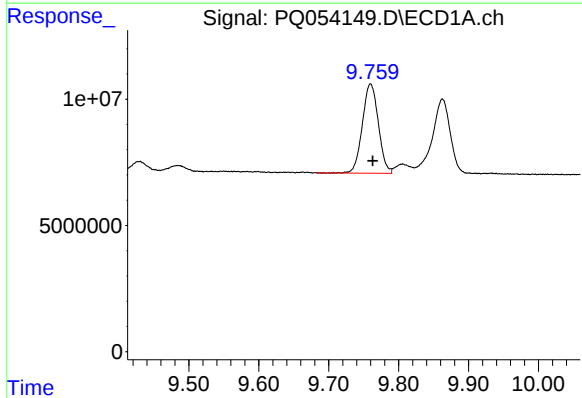


#38 AR-1262-3

R.T.: 9.760 min
Delta R.T.: -0.003 min
Response: 56174993
Conc: 45.85 ng/ml

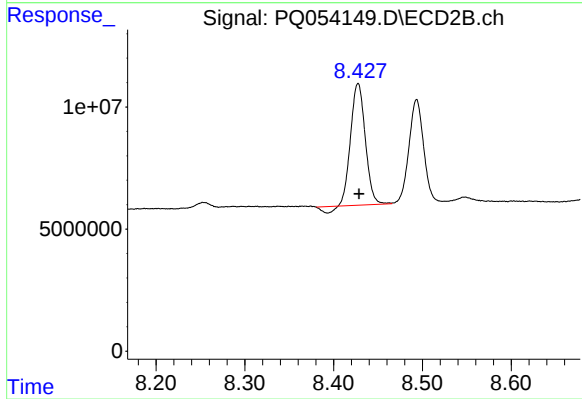

#38 AR-1262-3


R.T.: 8.428 min
Delta R.T.: -0.001 min
Response: 55527564
Conc: 72.33 ng/ml

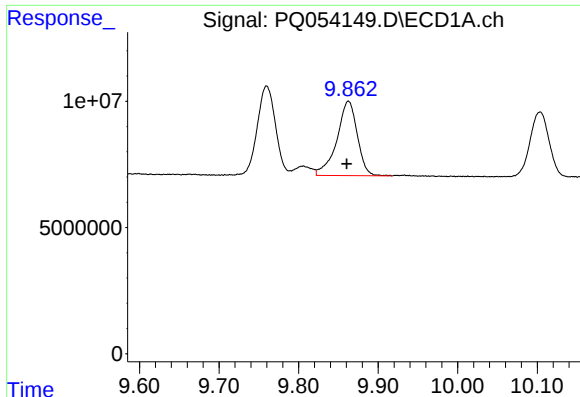

#39 AR-1262-4


R.T.: 9.863 min
Delta R.T.: 0.002 min
Response: 52686064
Conc: 58.20 ng/ml

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

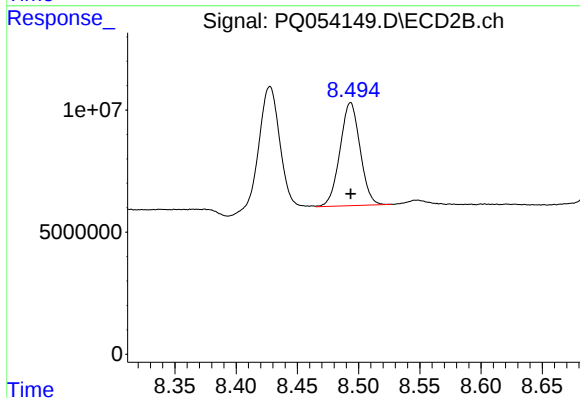


#39 AR-1262-4

R.T.: 8.493 min
Delta R.T.: 0.000 min
Response: 48131129
Conc: 38.50 ng/ml

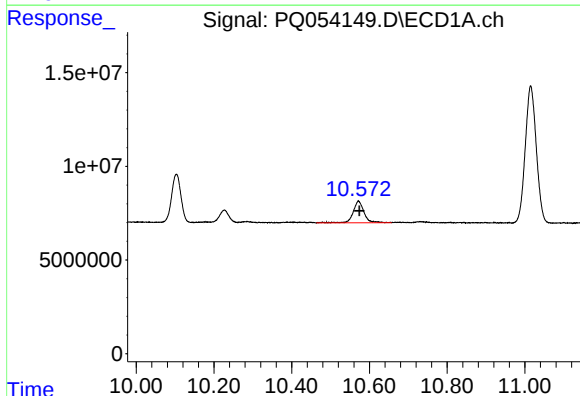


#40 AR-1262-5

R.T.: 10.572 min
Delta R.T.: -0.002 min
Response: 22303279
Conc: 33.65 ng/ml

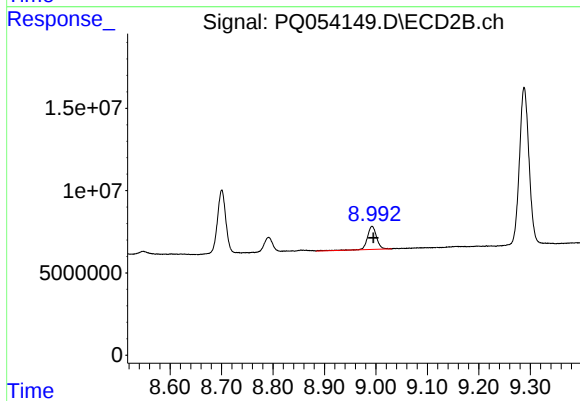

#40 AR-1262-5


R.T.: 8.993 min
Delta R.T.: -0.002 min
Response: 17443114
Conc: 30.22 ng/ml

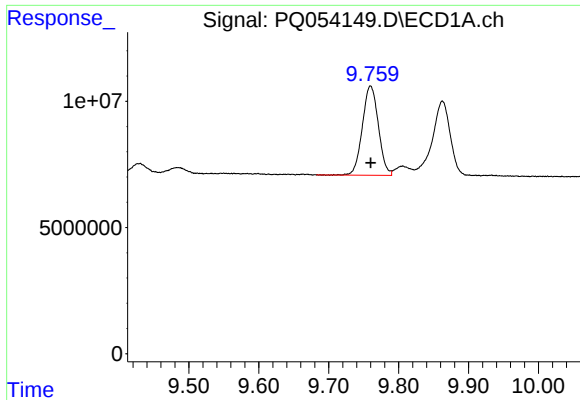

#41 AR-1268-1


R.T.: 9.760 min
Delta R.T.: 0.000 min
Response: 56174993
Conc: 26.63 ng/ml

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

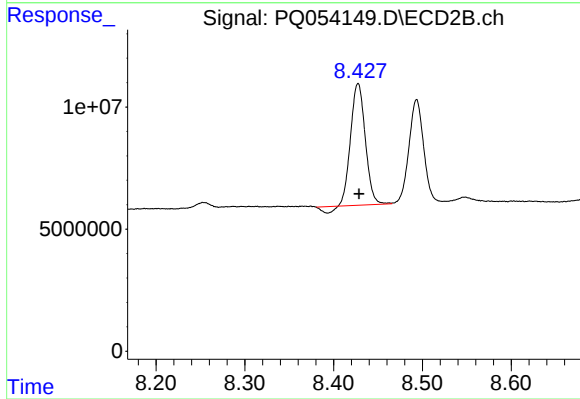


#41 AR-1268-1

R.T.: 8.428 min
Delta R.T.: 0.000 min
Response: 55527564
Conc: 24.62 ng/ml

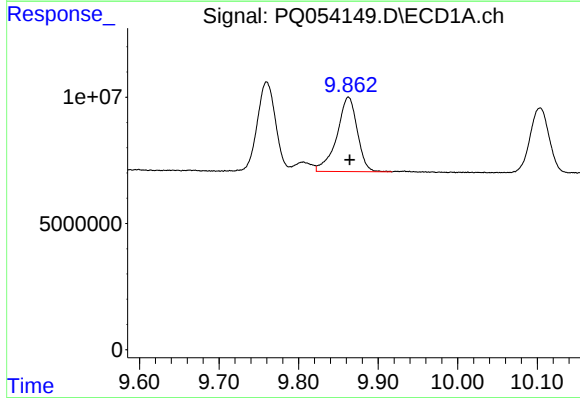


#42 AR-1268-2

R.T.: 9.863 min
Delta R.T.: -0.002 min
Response: 52686064
Conc: 27.31 ng/ml

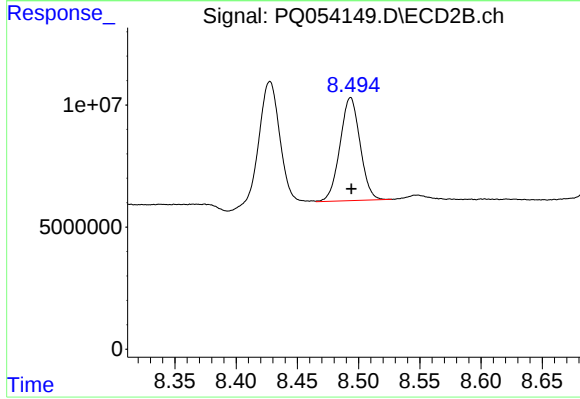

#42 AR-1268-2


R.T.: 8.493 min
Delta R.T.: 0.000 min
Response: 48131129
Conc: 25.77 ng/ml

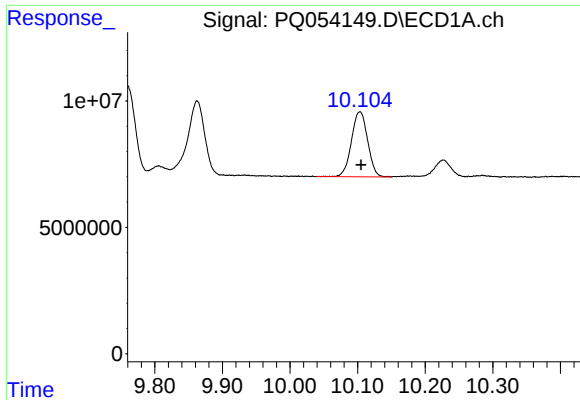

#43 AR-1268-3


R.T.: 10.103 min
Delta R.T.: -0.002 min
Response: 42695509
Conc: 26.52 ng/ml

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

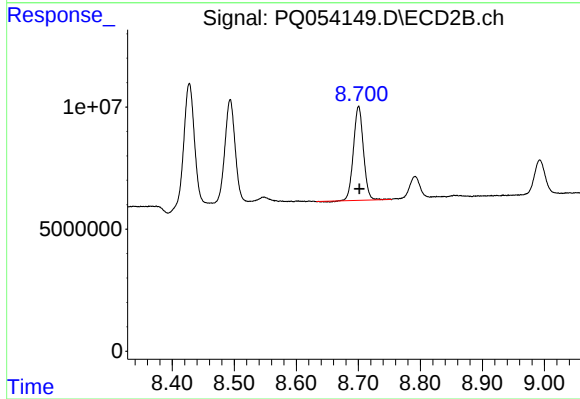


#43 AR-1268-3

R.T.: 8.700 min
Delta R.T.: -0.001 min
Response: 43088600
Conc: 25.78 ng/ml

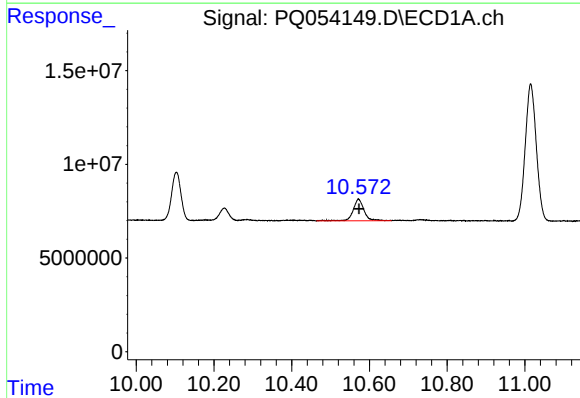


#44 AR-1268-4

R.T.: 10.572 min
Delta R.T.: -0.001 min
Response: 22303279
Conc: 30.49 ng/ml

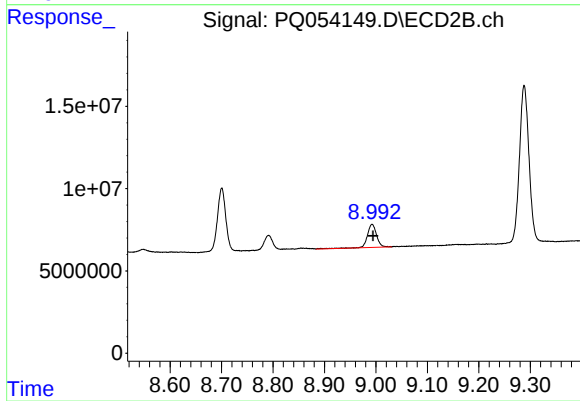

#44 AR-1268-4


R.T.: 8.993 min
Delta R.T.: -0.002 min
Response: 17443114
Conc: 26.75 ng/ml

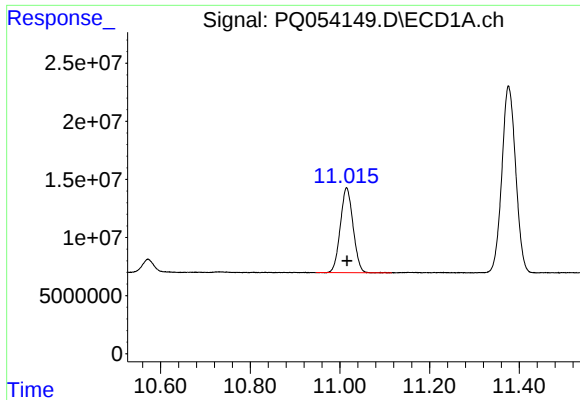

#45 AR-1268-5

R.T.: 11.015 min
Delta R.T.: -0.001 min
Response: 144088544
Conc: 26.42 ng/ml

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

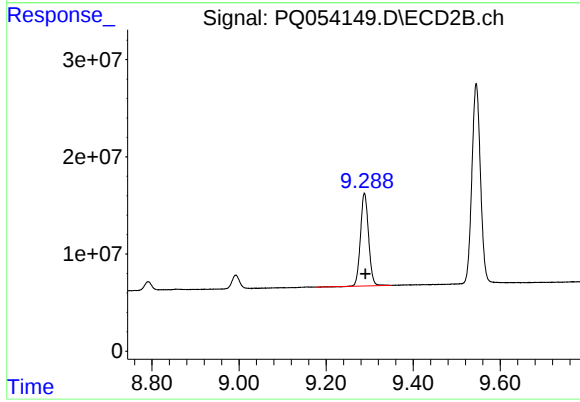

#45 AR-1268-5

R.T.: 9.288 min
Delta R.T.: -0.002 min
Response: 123185381
Conc: 26.14 ng/ml