

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ073021\
 Data File : PQ054215.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jul 2021 16:16
 Operator : AJ\MA
 Sample : M2940-07
 Misc : AR1262 MDL 25 PPB
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 02:18:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ072921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jul 30 02:37:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.204	4.208	395.7E6	222.8E6	16.945	15.757
2)	SA Decachlor...	11.379	9.547	334.0E6	271.6E6	19.849	21.530
Target Compounds							
3)	L1 AR-1016-1	6.500f	5.471	1687503	336729	2.302	0.744 #
4)	L1 AR-1016-2	0.000	5.493	0	2044294	N.D.	2.758 #
5)	L1 AR-1016-3	0.000	5.689	0	515468	N.D.	1.430 #
6)	L1 AR-1016-4	0.000	5.755f	0	2140912	N.D.	7.501 #
7)	L1 AR-1016-5	0.000	5.956	0	948193	N.D.	2.602 #
8)	L2 AR-1221-1	5.425f	0.000	1857783	0	7.679	N.D. #
9)	L2 AR-1221-2	5.564	4.565	7123409	3244461	39.324	30.756
10)	L2 AR-1221-3	0.000	4.641	0	1720118	N.D.	4.902 #
11)	L3 AR-1232-1	0.000	4.641	0	1720118	N.D.	7.369 #
12)	L3 AR-1232-2	0.000	5.493	0	2044294	N.D.	7.058 #
13)	L3 AR-1232-3	0.000	5.689	0	515468	N.D.	3.885 #
14)	L3 AR-1232-4	0.000	5.787	0	1164250	N.D.	10.203 #
15)	L3 AR-1232-5	0.000	5.956	0	948193	N.D.	7.378 #
16)	L4 AR-1242-1	6.500f	5.471	1687503	336729	3.675	1.238 #
17)	L4 AR-1242-2	0.000	5.493	0	2044294	N.D.	4.343 #
18)	L4 AR-1242-3	0.000	5.689	0	515468	N.D.	2.336 #
19)	L4 AR-1242-4	0.000	5.787	0	1164250	N.D.	5.382 #
20)	L4 AR-1242-5	0.000	6.344	0	3371150	N.D.	11.364 #
21)	L5 AR-1248-1	6.500f	5.471	1687503	336729	4.549	1.492 #
22)	L5 AR-1248-2	0.000	5.755f	0	2140912	N.D.	6.523 #
23)	L5 AR-1248-3	0.000	5.787	0	1164250	N.D.	3.521 #
24)	L5 AR-1248-4	0.000	5.956	0	948193	N.D.	2.389 #
25)	L5 AR-1248-5	0.000	6.383	0	1962358	N.D.	4.924 #
26)	L6 AR-1254-1	7.439	6.344	4329722	3371150	6.126	5.041
27)	L6 AR-1254-2	7.665	6.503	3542579	7111319	3.235	11.566 #
28)	L6 AR-1254-3	8.051	6.942f	2289218	11436342	1.946	11.844 #
29)	L6 AR-1254-4	8.346	7.164	2803829	1611821	3.181	2.419
30)	L6 AR-1254-5	8.772	7.590	18745318	16989570	19.210	17.419
31)	L7 AR-1260-1	8.214	7.060	21322613	18750642	21.717	25.015
32)	L7 AR-1260-2	8.479	7.257	22109112	20146224	19.473	19.287
33)	L7 AR-1260-3	8.845	7.414	26573853	27731917	37.567	31.865
34)	L7 AR-1260-4	9.088	7.895	28339508	24987239	32.035	40.131 #
35)	L7 AR-1260-5	9.432	8.142	49490359	47357055	29.397	27.640
36)	L8 AR-1262-1	8.845	7.590	26573853	16989570	26.866	37.593 #
37)	L8 AR-1262-2	9.432	8.142	49490359	47357055	27.417	25.148
38)	L8 AR-1262-3	9.761	8.429	21686912	15480682	17.700	20.165
39)	L8 AR-1262-4	9.862	8.493	14223284	33473176	15.711	26.775 #
40)	L8 AR-1262-5	10.573	8.994	20549261	17924914	31.003	31.059
41)	L9 AR-1268-1	9.761	8.429	21686912	15480682	10.282	6.863 #
42)	L9 AR-1268-2	9.862	8.493	14223284	33473176	7.374	17.921 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ073021\
 Data File : PQ054215.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jul 2021 16:16
 Operator : AJ\MA
 Sample : M2940-07
 Misc : AR1262 MDL 25 PPB
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 02:18:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ072921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jul 30 02:37:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
43) L9	AR-1268-3	0.000	8.700	0	3698484	N.D.	2.212 #
44) L9	AR-1268-4	10.573	8.994	20549261	17924914	28.094	27.486
45) L9	AR-1268-5	11.017	9.290	8563584	7779849	1.570	1.651



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ073021\
Data File : PQ054215.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jul 2021 16:16
Operator : AJ\MA
Sample : M2940-07
Misc : AR1262 MDL 25 PPB
ALS Vial : 72 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 02:18:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ072921.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 30 02:37:02 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

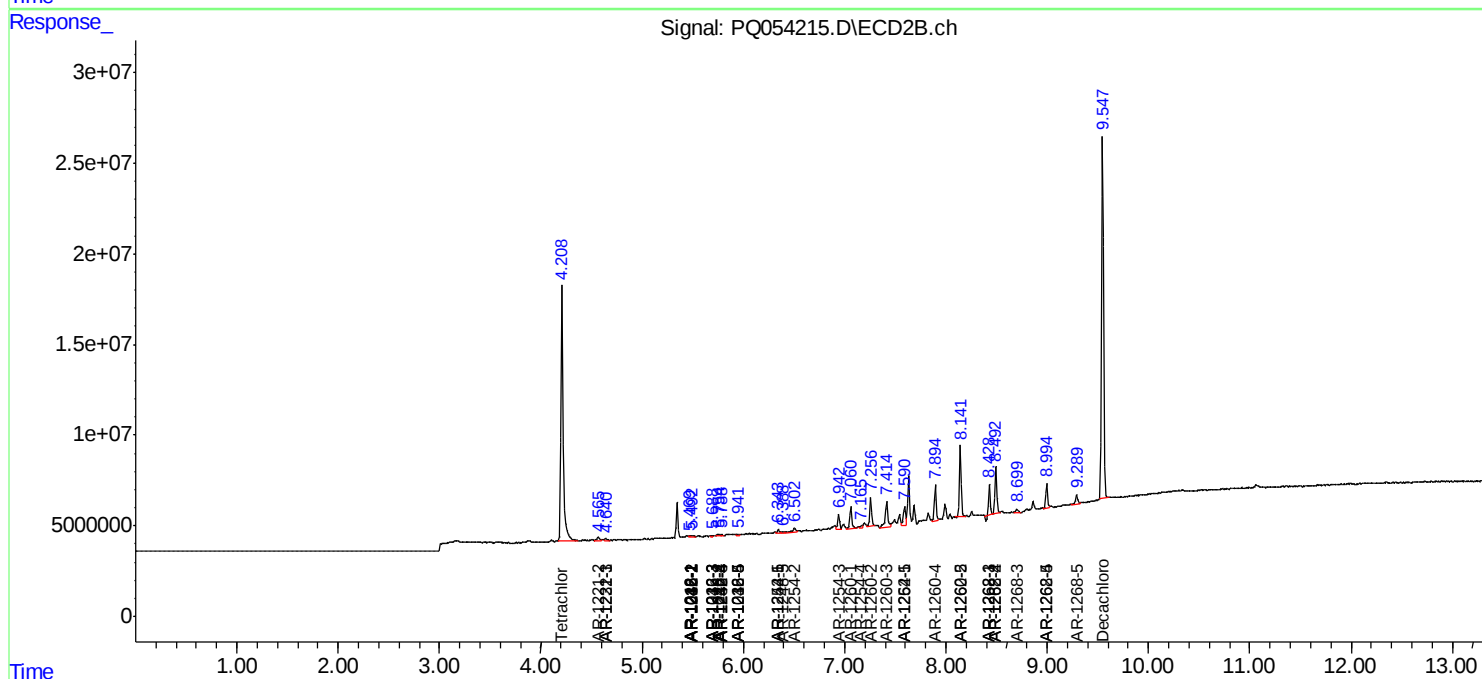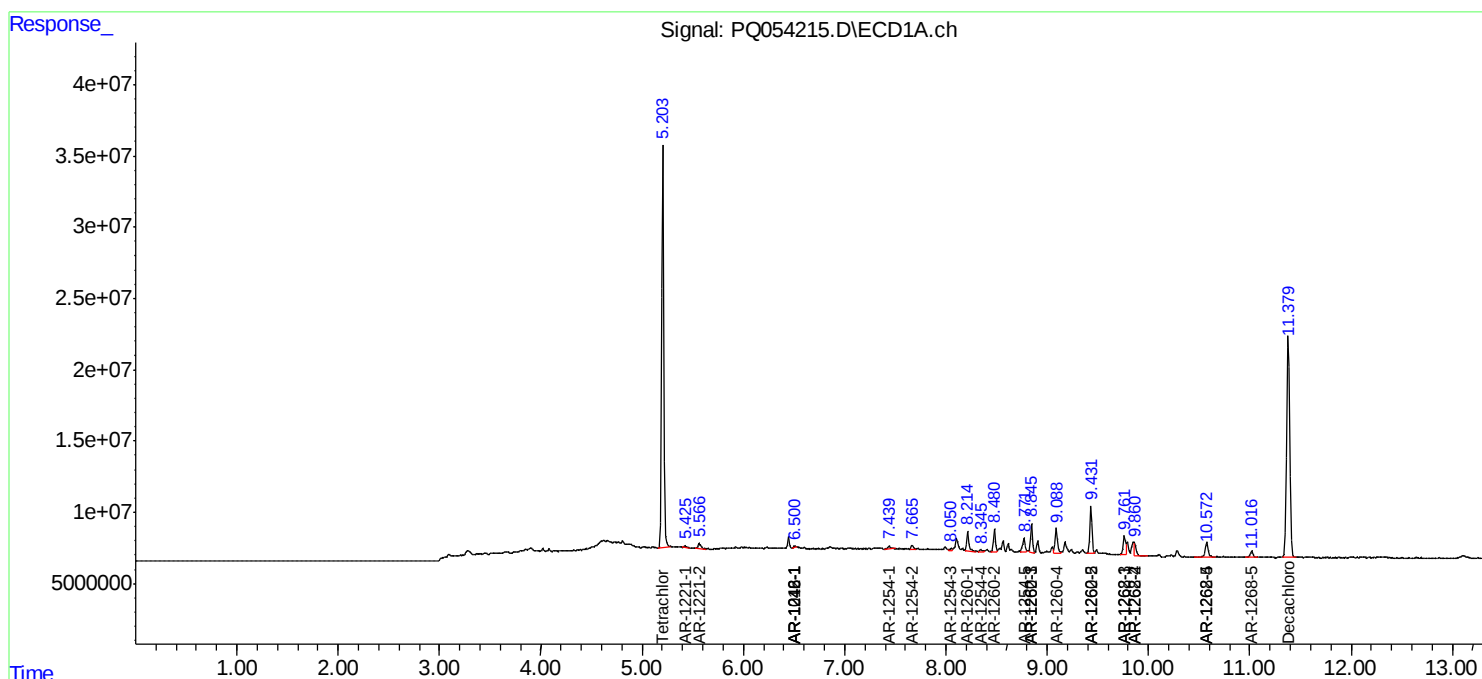




#1 Tetrachloro-m-xylene


R.T.: 5.204 min
Delta R.T.: 0.000 min
Response: 395713182
Conc: 16.95 ng/ml

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021




#1 Tetrachloro-m-xylene

R.T.: 4.208 min
Delta R.T.: 0.002 min
Response: 222756867
Conc: 15.76 ng/ml




#2 Decachlorobiphenyl

R.T.: 11.379 min
Delta R.T.: 0.000 min
Response: 333986380
Conc: 19.85 ng/ml

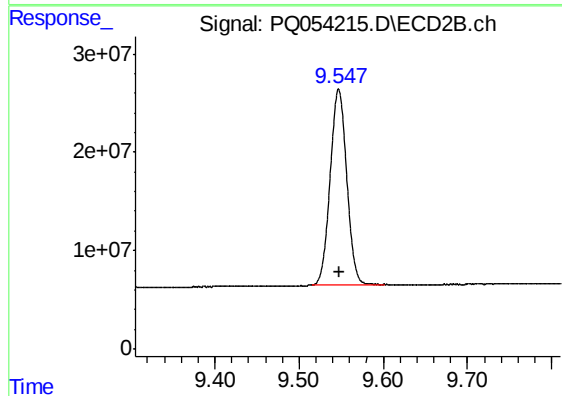

#2 Decachlorobiphenyl


R.T.: 9.547 min
Delta R.T.: -0.001 min
Response: 271585627
Conc: 21.53 ng/ml

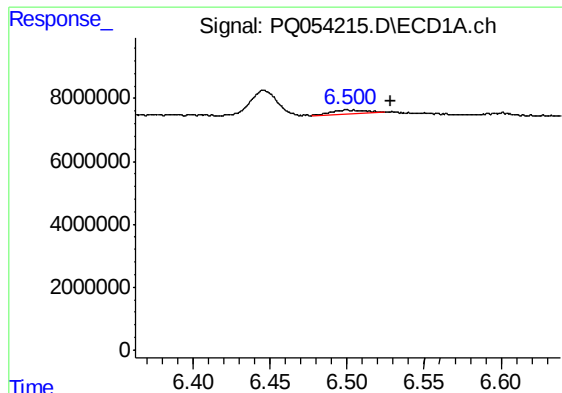

#3 AR-1016-1


R.T.: 6.500 min
Delta R.T.: -0.028 min
Response: 1687503
Conc: 2.30 ng/ml

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

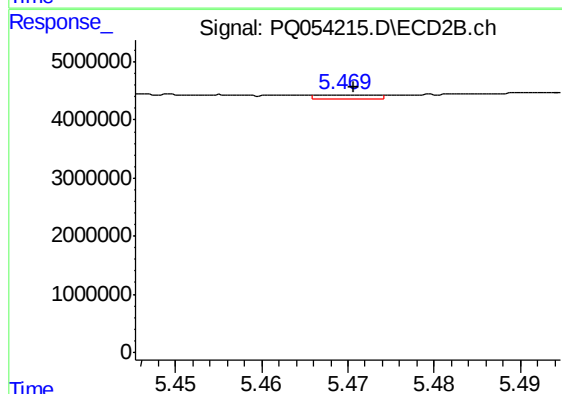


#3 AR-1016-1

R.T.: 5.471 min
Delta R.T.: 0.000 min
Response: 336729
Conc: 0.74 ng/ml

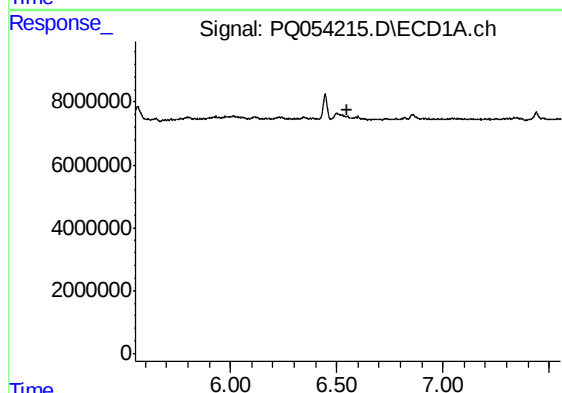


#4 AR-1016-2

R.T.: 0.000 min
Exp R.T. : 6.553 min
Response: 0
Conc: N.D.

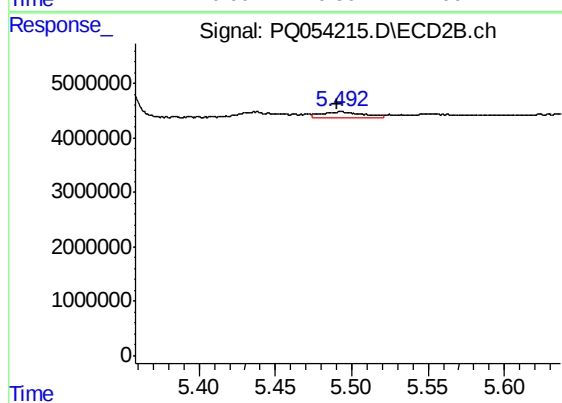

#4 AR-1016-2


R.T.: 5.493 min
Delta R.T.: 0.002 min
Response: 2044294
Conc: 2.76 ng/ml

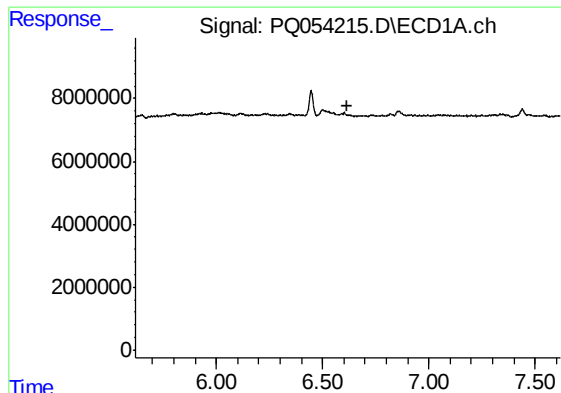

#5 AR-1016-3


R.T.: 0.000 min
Exp R.T. : 6.619 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

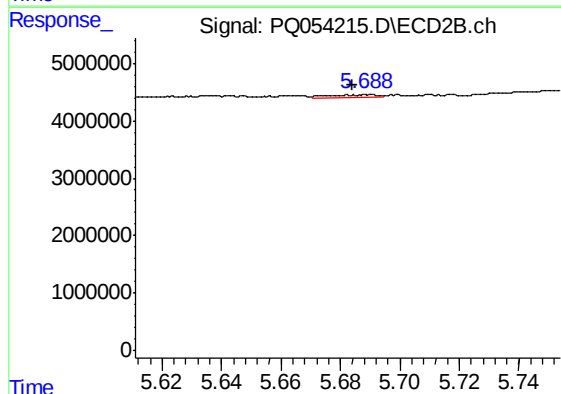


#5 AR-1016-3

R.T.: 5.689 min
Delta R.T.: 0.006 min
Response: 515468
Conc: 1.43 ng/ml

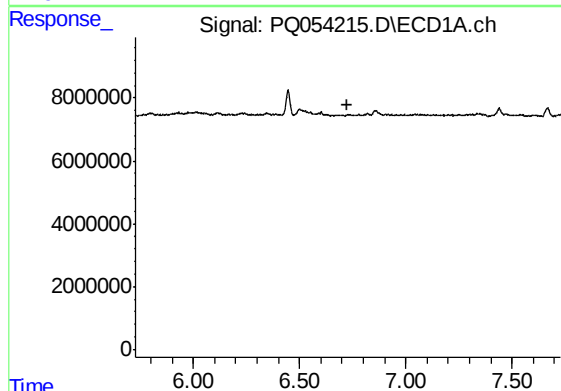


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T. : 6.728 min
Response: 0
Conc: N.D.

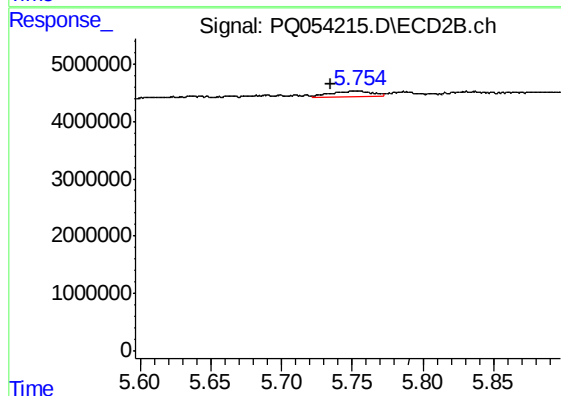

#6 AR-1016-4


R.T.: 5.755 min
Delta R.T.: 0.020 min
Response: 2140912
Conc: 7.50 ng/ml

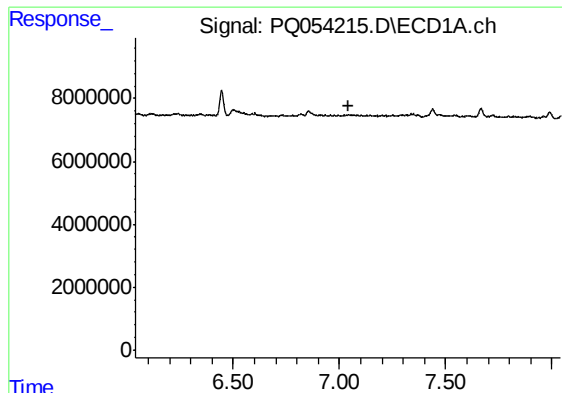

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T. : 7.040 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

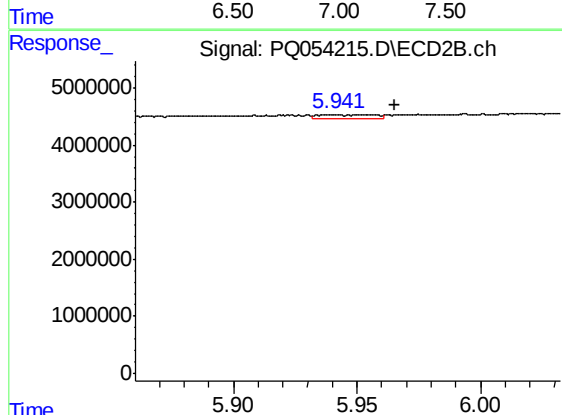


#7 AR-1016-5

R.T.: 5.956 min
Delta R.T.: -0.009 min
Response: 948193
Conc: 2.60 ng/ml

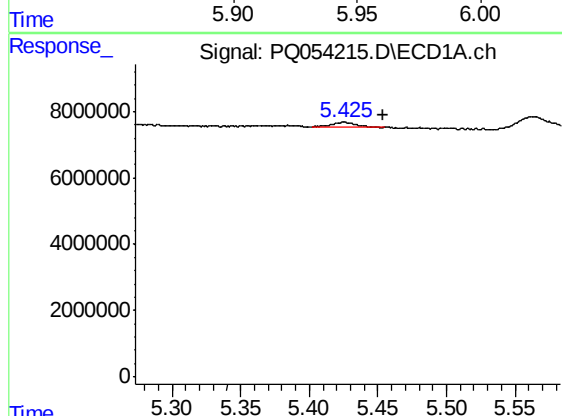


#8 AR-1221-1

R.T.: 5.425 min
Delta R.T.: -0.028 min
Response: 1857783
Conc: 7.68 ng/ml

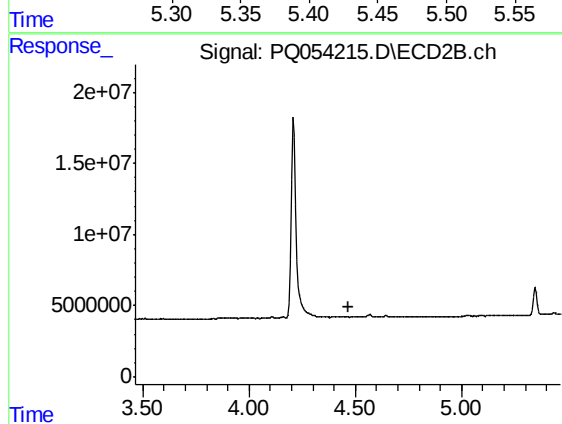

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T. : 4.465 min
Response: 0
Conc: N.D.

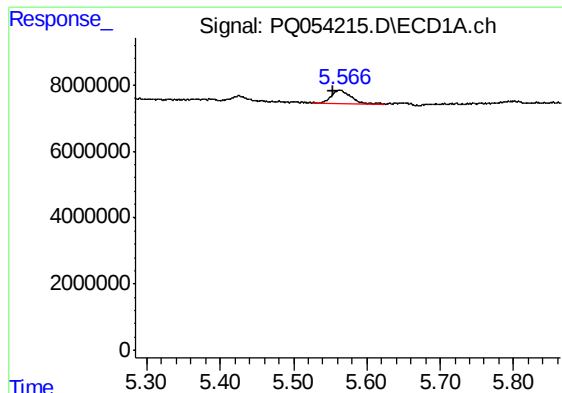

#9 AR-1221-2


R.T.: 5.564 min
Delta R.T.: 0.010 min
Response: 7123409
Conc: 39.32 ng/ml

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

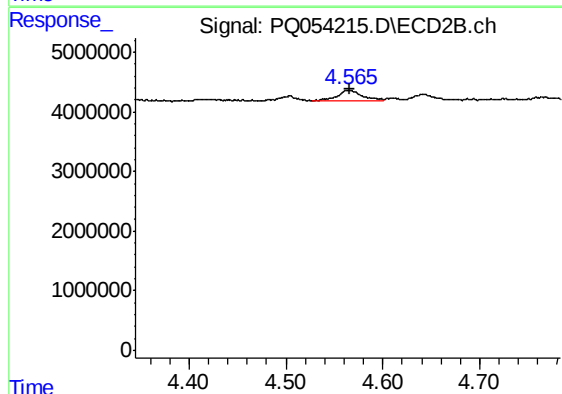


#9 AR-1221-2

R.T.: 4.565 min
Delta R.T.: 0.000 min
Response: 3244461
Conc: 30.76 ng/ml




#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 5.641 min
Response: 0
Conc: N.D.

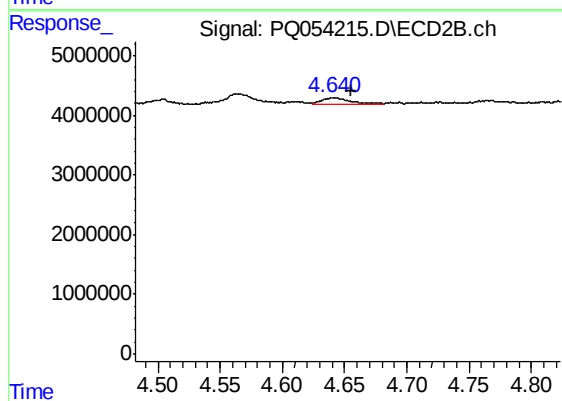

#10 AR-1221-3


R.T.: 4.641 min
Delta R.T.: -0.015 min
Response: 1720118
Conc: 4.90 ng/ml



#11 AR-1232-1


R.T.: 0.000 min
Exp R.T. : 5.642 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021




#11 AR-1232-1

R.T.: 4.641 min
Delta R.T.: -0.015 min
Response: 1720118
Conc: 7.37 ng/ml

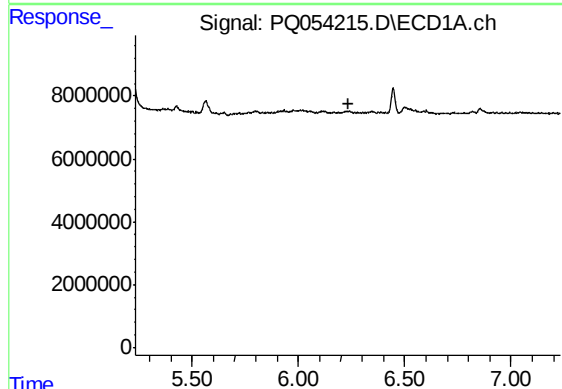


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T. : 6.233 min
Response: 0
Conc: N.D.

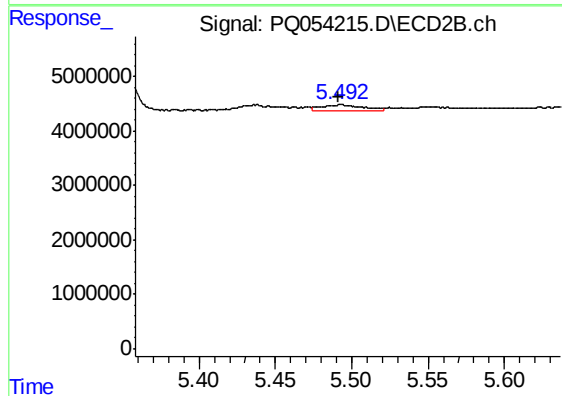

#12 AR-1232-2


R.T.: 5.493 min
Delta R.T.: 0.002 min
Response: 2044294
Conc: 7.06 ng/ml

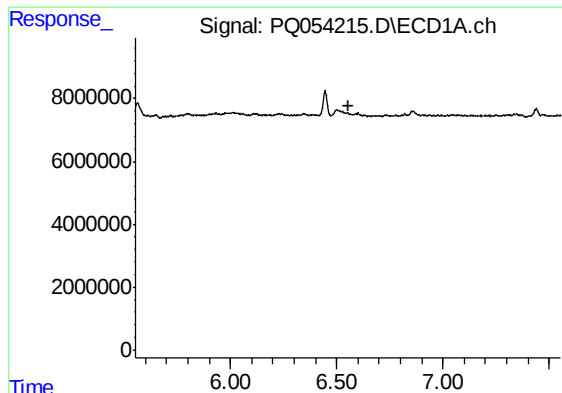

#13 AR-1232-3


R.T.: 0.000 min
Exp R.T. : 6.554 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

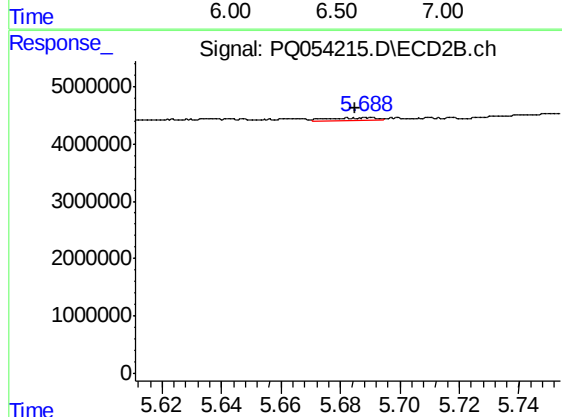


#13 AR-1232-3

R.T.: 5.689 min
Delta R.T.: 0.005 min
Response: 515468
Conc: 3.89 ng/ml

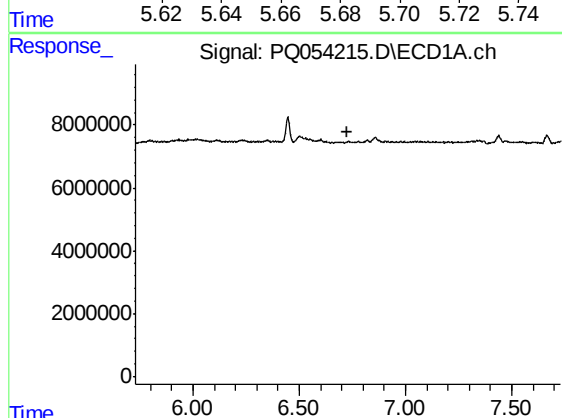


#14 AR-1232-4

R.T.: 0.000 min
Exp R.T. : 6.729 min
Response: 0
Conc: N.D.

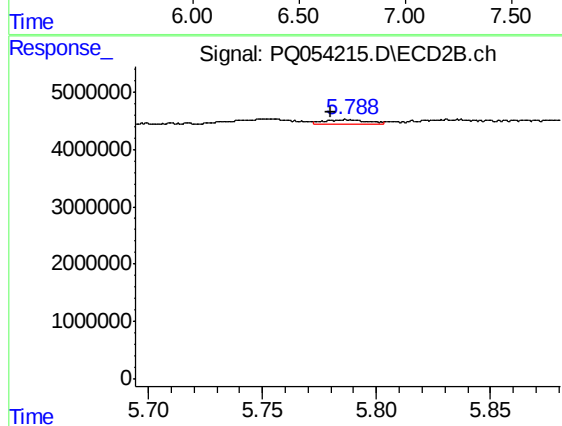

#14 AR-1232-4


R.T.: 5.787 min
Delta R.T.: 0.007 min
Response: 1164250
Conc: 10.20 ng/ml



#15 AR-1232-5


R.T.: 0.000 min
Exp R.T.: 6.821 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021




#15 AR-1232-5

R.T.: 5.956 min
Delta R.T.: -0.010 min
Response: 948193
Conc: 7.38 ng/ml




#16 AR-1242-1

R.T.: 6.500 min
Delta R.T.: -0.030 min
Response: 1687503
Conc: 3.67 ng/ml

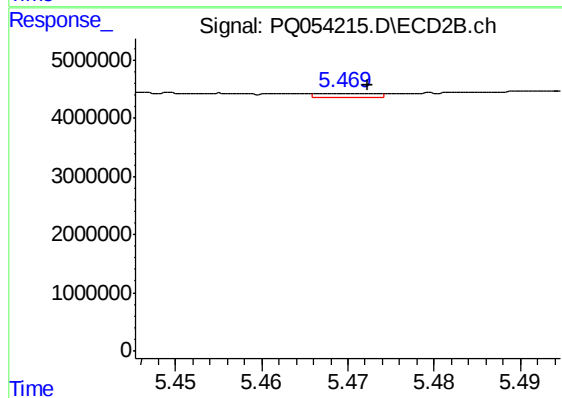

#16 AR-1242-1


R.T.: 5.471 min
Delta R.T.: -0.001 min
Response: 336729
Conc: 1.24 ng/ml

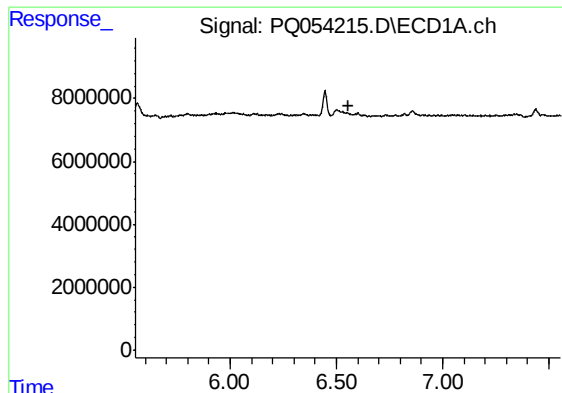

#17 AR-1242-2


R.T.: 0.000 min
Exp R.T. : 6.554 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

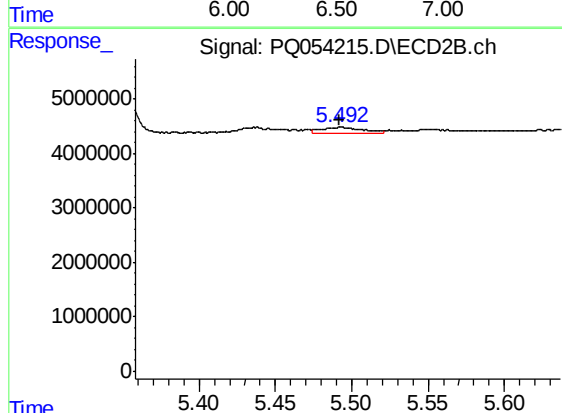


#17 AR-1242-2

R.T.: 5.493 min
Delta R.T.: 0.002 min
Response: 2044294
Conc: 4.34 ng/ml

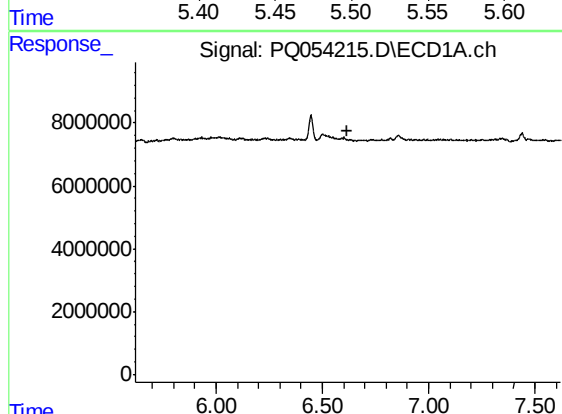


#18 AR-1242-3

R.T.: 0.000 min
Exp R.T. : 6.620 min
Response: 0
Conc: N.D.

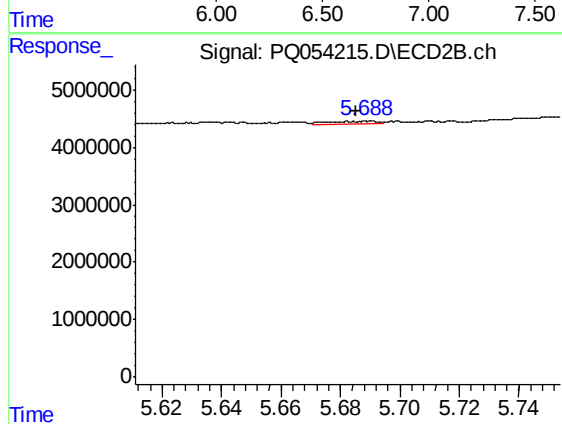

#18 AR-1242-3


R.T.: 5.689 min
Delta R.T.: 0.004 min
Response: 515468
Conc: 2.34 ng/ml



#19 AR-1242-4


R.T.: 0.000 min
Exp R.T. : 6.729 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

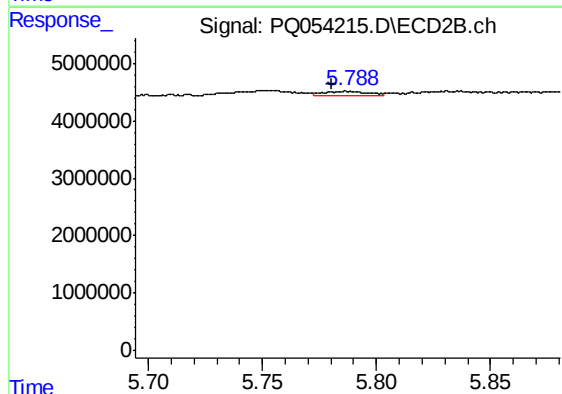


#19 AR-1242-4

R.T.: 5.787 min
Delta R.T.: 0.007 min
Response: 1164250
Conc: 5.38 ng/ml




#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 7.511 min
Response: 0
Conc: N.D.

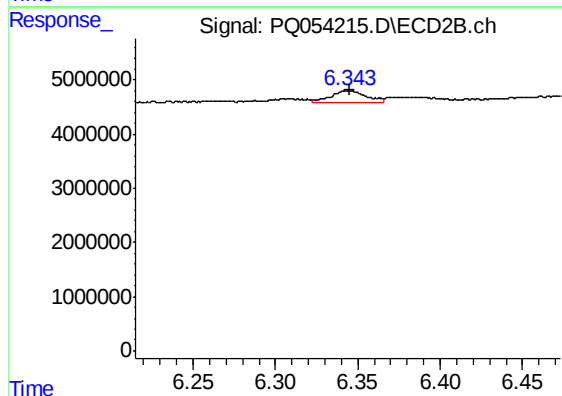

#20 AR-1242-5


R.T.: 6.344 min
Delta R.T.: -0.001 min
Response: 3371150
Conc: 11.36 ng/ml

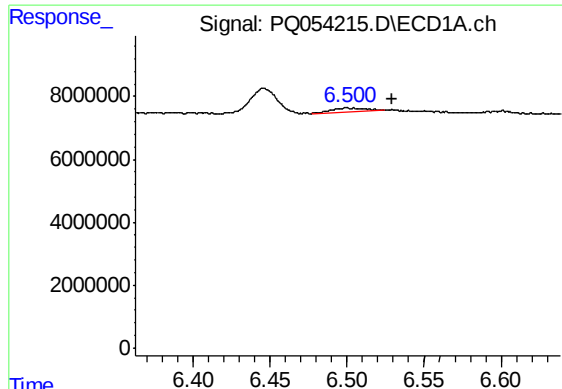

#21 AR-1248-1


R.T.: 6.500 min
Delta R.T.: -0.029 min
Response: 1687503
Conc: 4.55 ng/ml

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021




#21 AR-1248-1

R.T.: 5.471 min
Delta R.T.: 0.000 min
Response: 336729
Conc: 1.49 ng/ml




#22 AR-1248-2

R.T.: 0.000 min
Exp R.T. : 6.821 min
Response: 0
Conc: N.D.

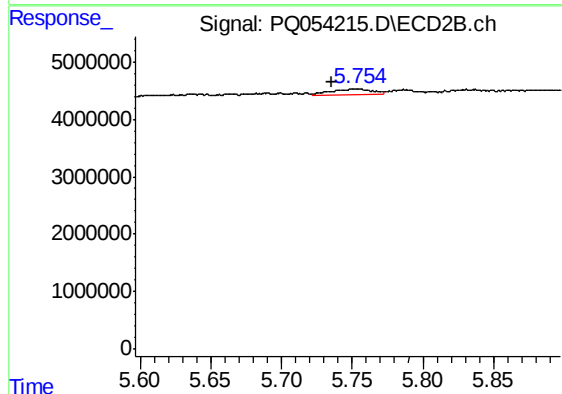

#22 AR-1248-2


R.T.: 5.755 min
Delta R.T.: 0.020 min
Response: 2140912
Conc: 6.52 ng/ml



#23 AR-1248-3


R.T.: 0.000 min
Exp R.T. : 7.041 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

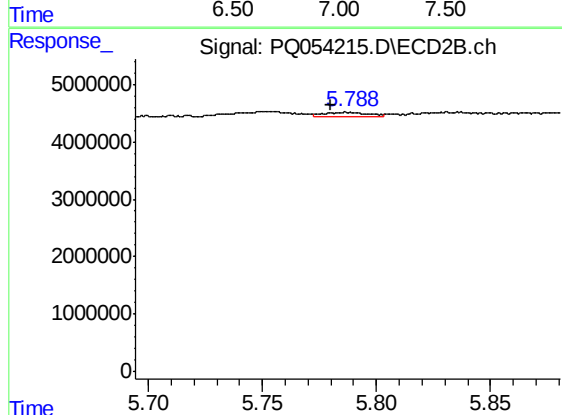


#23 AR-1248-3

R.T.: 5.787 min
Delta R.T.: 0.007 min
Response: 1164250
Conc: 3.52 ng/ml

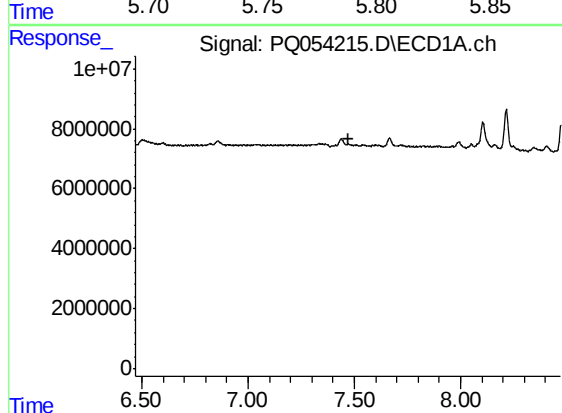


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 7.470 min
Response: 0
Conc: N.D.

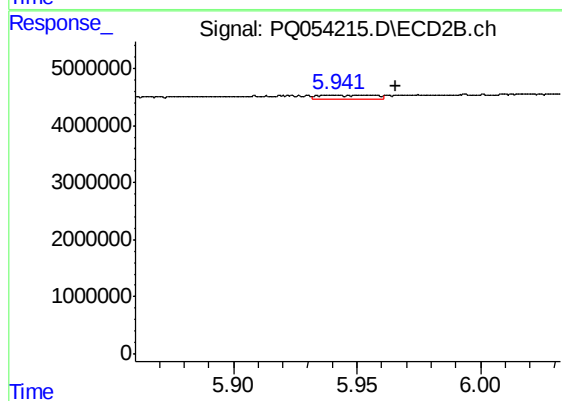

#24 AR-1248-4


R.T.: 5.956 min
Delta R.T.: -0.010 min
Response: 948193
Conc: 2.39 ng/ml

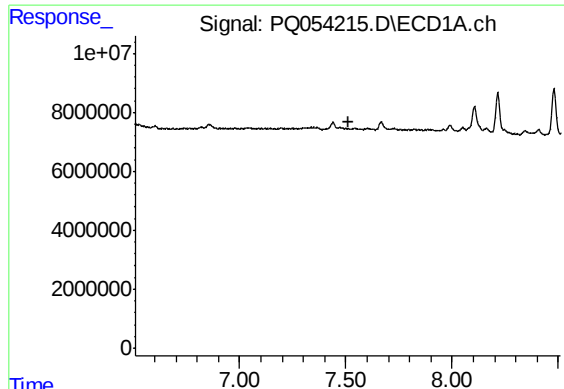

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 7.510 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

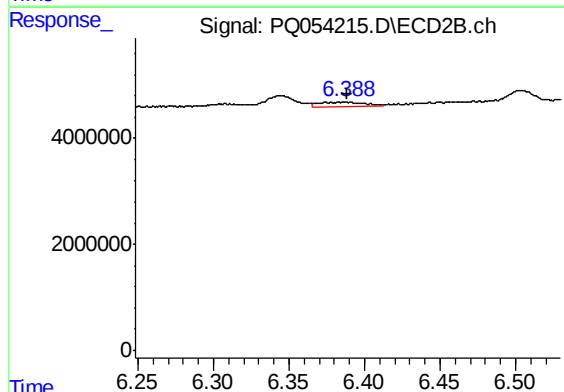


#25 AR-1248-5

R.T.: 6.383 min
Delta R.T.: -0.006 min
Response: 1962358
Conc: 4.92 ng/ml

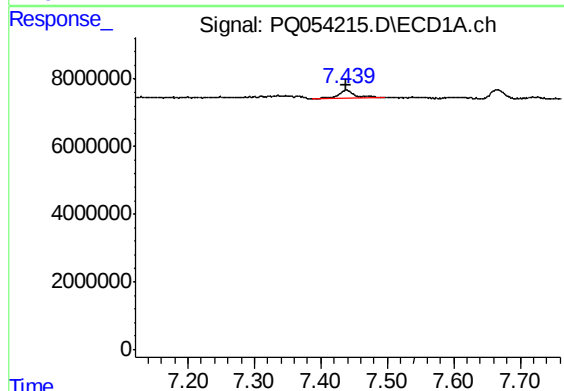


#26 AR-1254-1

R.T.: 7.439 min
Delta R.T.: 0.000 min
Response: 4329722
Conc: 6.13 ng/ml

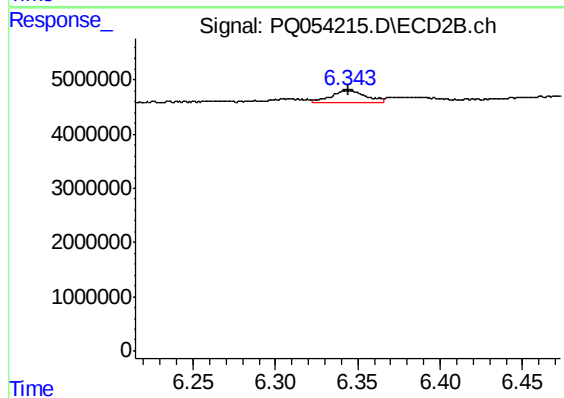

#26 AR-1254-1


R.T.: 6.344 min
Delta R.T.: 0.000 min
Response: 3371150
Conc: 5.04 ng/ml



#27 AR-1254-2


R.T.: 7.665 min
Delta R.T.: 0.000 min
Response: 3542579
Conc: 3.24 ng/ml

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

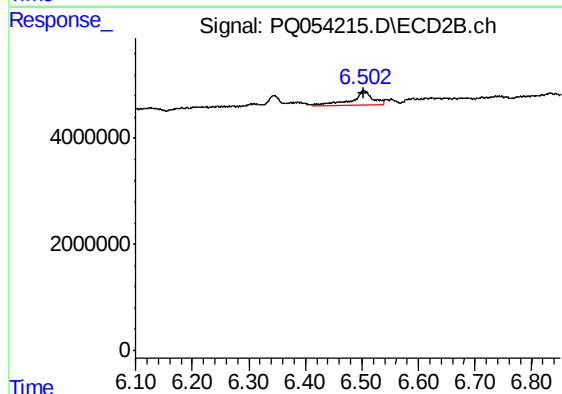


#27 AR-1254-2

R.T.: 6.503 min
Delta R.T.: 0.000 min
Response: 7111319
Conc: 11.57 ng/ml




#28 AR-1254-3

R.T.: 8.051 min
Delta R.T.: 0.000 min
Response: 2289218
Conc: 1.95 ng/ml

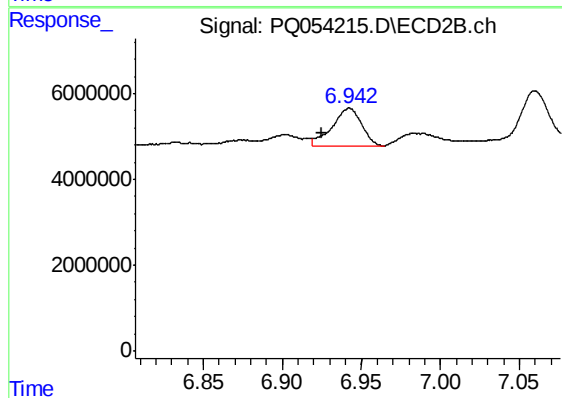

#28 AR-1254-3


R.T.: 6.942 min
Delta R.T.: 0.018 min
Response: 11436342
Conc: 11.84 ng/ml

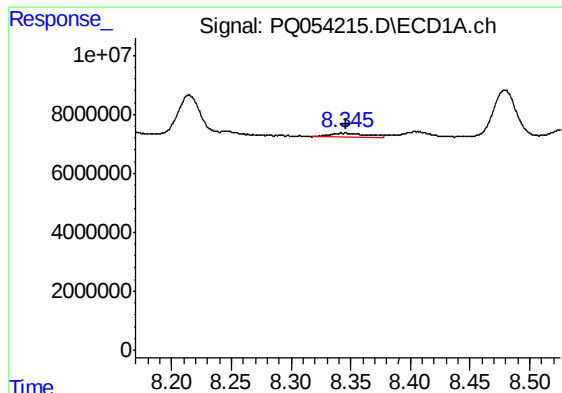

#29 AR-1254-4


R.T.: 8.346 min
Delta R.T.: 0.000 min
Response: 2803829
Conc: 3.18 ng/ml

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

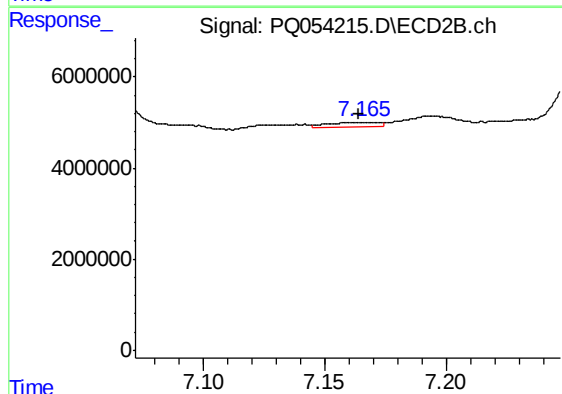


#29 AR-1254-4

R.T.: 7.164 min
Delta R.T.: 0.000 min
Response: 1611821
Conc: 2.42 ng/ml




#30 AR-1254-5

R.T.: 8.772 min
Delta R.T.: -0.002 min
Response: 18745318
Conc: 19.21 ng/ml

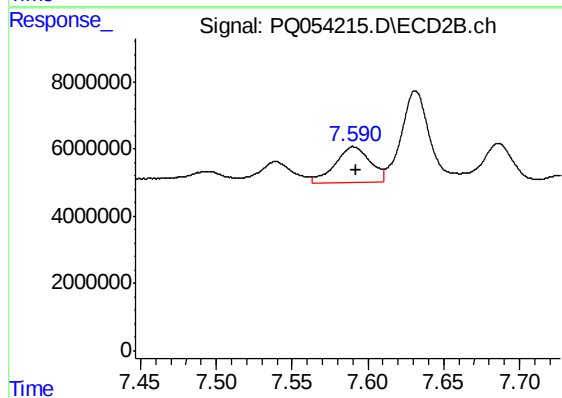

#30 AR-1254-5


R.T.: 7.590 min
Delta R.T.: -0.002 min
Response: 16989570
Conc: 17.42 ng/ml



#31 AR-1260-1


R.T.: 8.214 min
Delta R.T.: 0.000 min
Response: 21322613
Conc: 21.72 ng/ml

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021




#31 AR-1260-1

R.T.: 7.060 min
Delta R.T.: 0.000 min
Response: 18750642
Conc: 25.02 ng/ml




#32 AR-1260-2

R.T.: 8.479 min
Delta R.T.: 0.000 min
Response: 22109112
Conc: 19.47 ng/ml

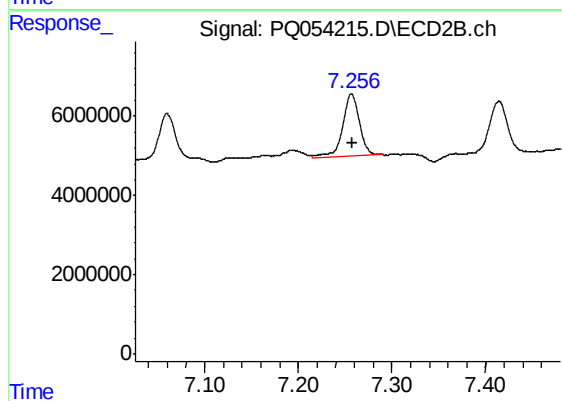

#32 AR-1260-2


R.T.: 7.257 min
Delta R.T.: 0.000 min
Response: 20146224
Conc: 19.29 ng/ml



#33 AR-1260-3


R.T.: 8.845 min
Delta R.T.: 0.000 min
Response: 26573853
Conc: 37.57 ng/ml

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021




#33 AR-1260-3

R.T.: 7.414 min
Delta R.T.: 0.001 min
Response: 27731917
Conc: 31.87 ng/ml




#34 AR-1260-4

R.T.: 9.088 min
Delta R.T.: 0.000 min
Response: 28339508
Conc: 32.04 ng/ml

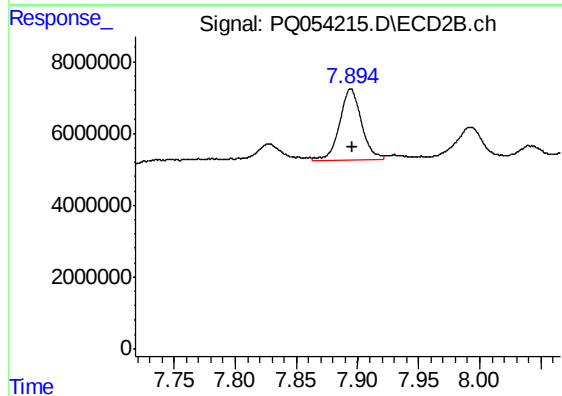

#34 AR-1260-4


R.T.: 7.895 min
Delta R.T.: -0.001 min
Response: 24987239
Conc: 40.13 ng/ml

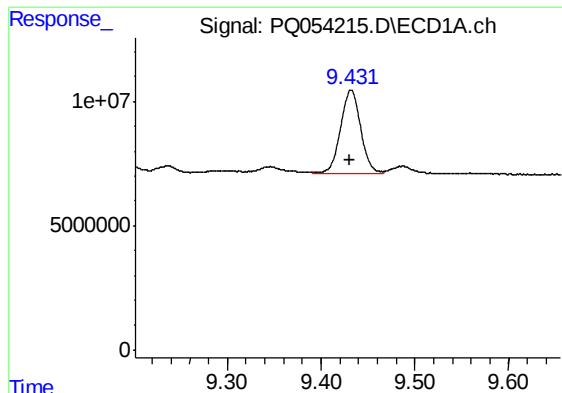

#35 AR-1260-5


R.T.: 9.432 min
Delta R.T.: 0.000 min
Response: 49490359
Conc: 29.40 ng/ml

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

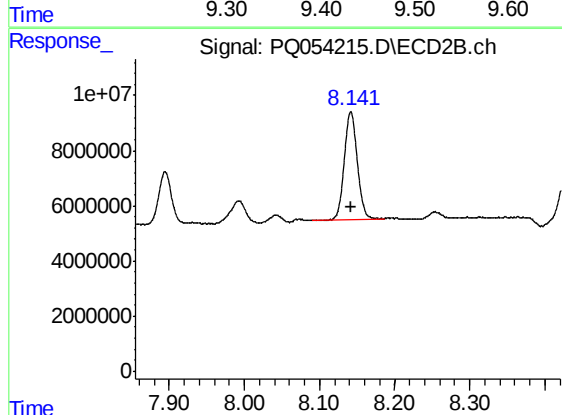


#35 AR-1260-5

R.T.: 8.142 min
Delta R.T.: 0.000 min
Response: 47357055
Conc: 27.64 ng/ml

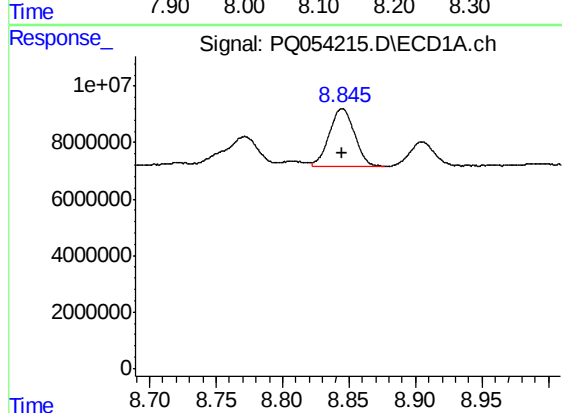


#36 AR-1262-1

R.T.: 8.845 min
Delta R.T.: 0.000 min
Response: 26573853
Conc: 26.87 ng/ml

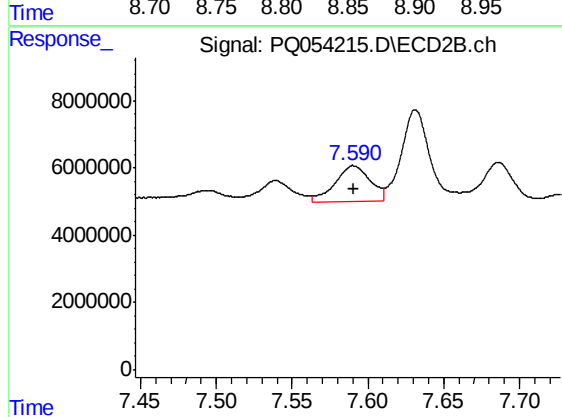

#36 AR-1262-1


R.T.: 7.590 min
Delta R.T.: 0.000 min
Response: 16989570
Conc: 37.59 ng/ml

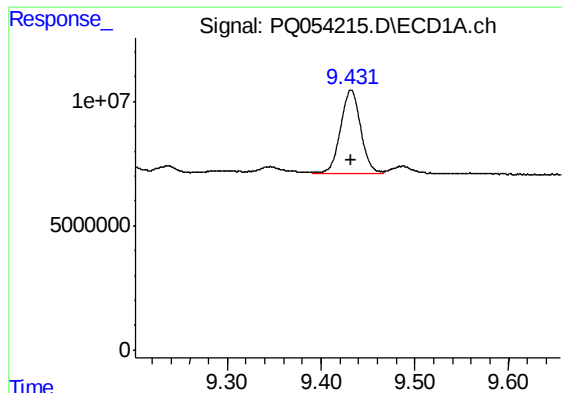

#37 AR-1262-2


R.T.: 9.432 min
Delta R.T.: 0.000 min
Response: 49490359
Conc: 27.42 ng/ml

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

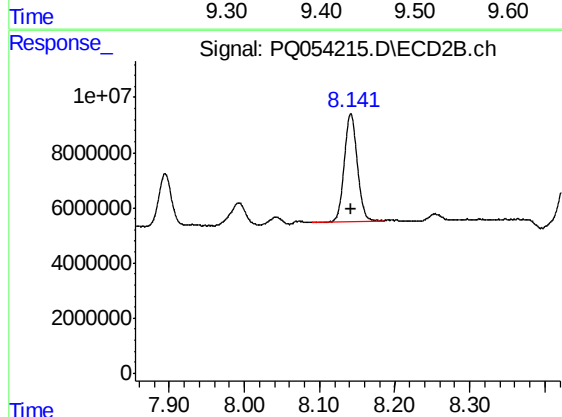


#37 AR-1262-2

R.T.: 8.142 min
Delta R.T.: 0.000 min
Response: 47357055
Conc: 25.15 ng/ml

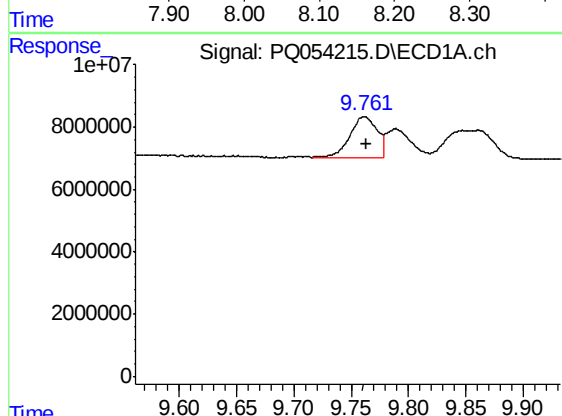


#38 AR-1262-3

R.T.: 9.761 min
Delta R.T.: -0.002 min
Response: 21686912
Conc: 17.70 ng/ml

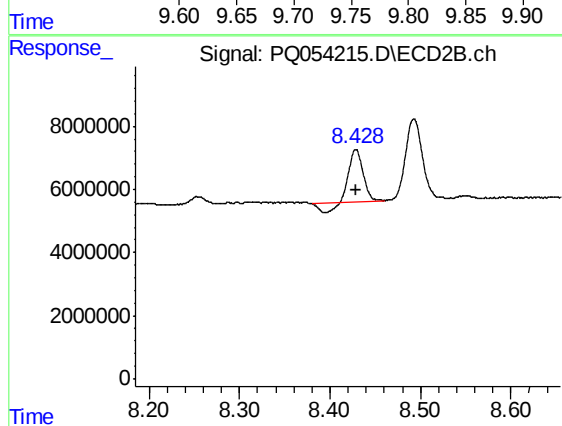

#38 AR-1262-3


R.T.: 8.429 min
Delta R.T.: 0.000 min
Response: 15480682
Conc: 20.17 ng/ml



#39 AR-1262-4


R.T.: 9.862 min
Delta R.T.: 0.001 min
Response: 14223284
Conc: 15.71 ng/ml

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021




#39 AR-1262-4

R.T.: 8.493 min
Delta R.T.: 0.000 min
Response: 33473176
Conc: 26.78 ng/ml




#40 AR-1262-5

R.T.: 10.573 min
Delta R.T.: 0.000 min
Response: 20549261
Conc: 31.00 ng/ml

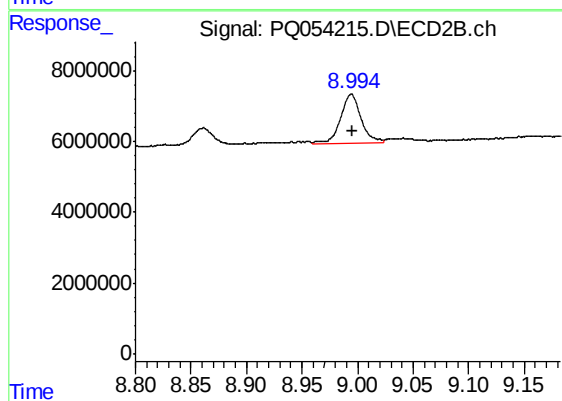

#40 AR-1262-5


R.T.: 8.994 min
Delta R.T.: 0.000 min
Response: 17924914
Conc: 31.06 ng/ml

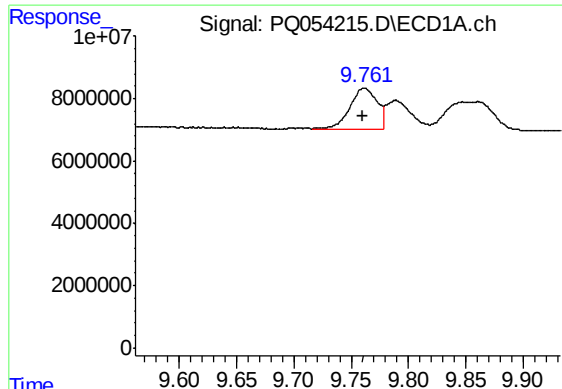

#41 AR-1268-1


R.T.: 9.761 min
Delta R.T.: 0.000 min
Response: 21686912
Conc: 10.28 ng/ml

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

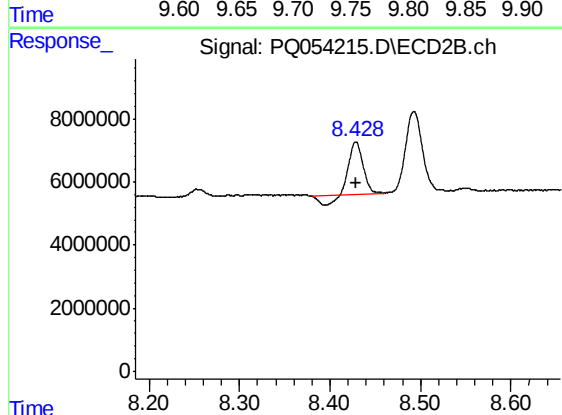


#41 AR-1268-1

R.T.: 8.429 min
Delta R.T.: 0.000 min
Response: 15480682
Conc: 6.86 ng/ml

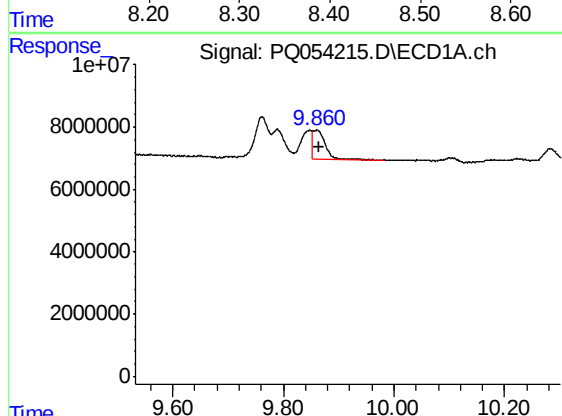


#42 AR-1268-2

R.T.: 9.862 min
Delta R.T.: -0.003 min
Response: 14223284
Conc: 7.37 ng/ml

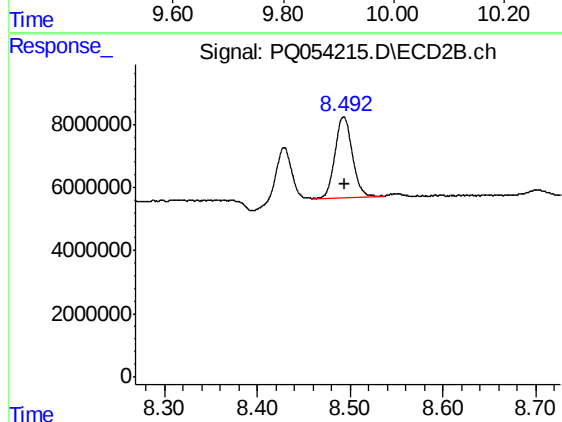

#42 AR-1268-2


R.T.: 8.493 min
Delta R.T.: -0.002 min
Response: 33473176
Conc: 17.92 ng/ml



#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 10.105 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021




#43 AR-1268-3

R.T.: 8.700 min
Delta R.T.: -0.002 min
Response: 3698484
Conc: 2.21 ng/ml




#44 AR-1268-4

R.T.: 10.573 min
Delta R.T.: 0.000 min
Response: 20549261
Conc: 28.09 ng/ml

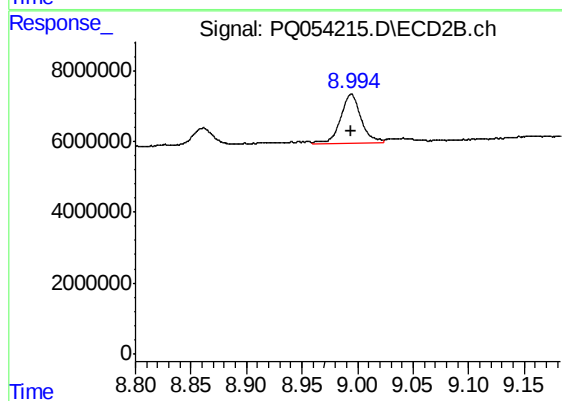

#44 AR-1268-4


R.T.: 8.994 min
Delta R.T.: 0.000 min
Response: 17924914
Conc: 27.49 ng/ml

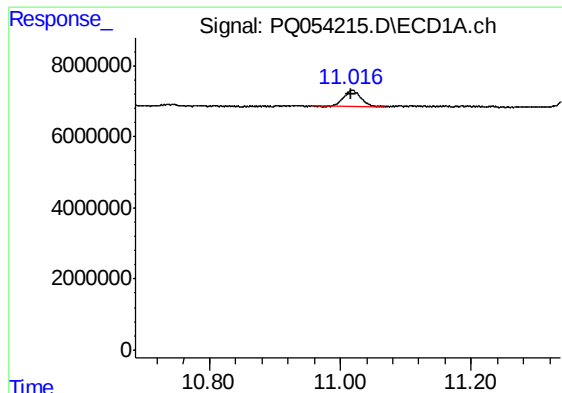

#45 AR-1268-5

R.T.: 11.017 min
Delta R.T.: 0.001 min
Response: 8563584
Conc: 1.57 ng/ml

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

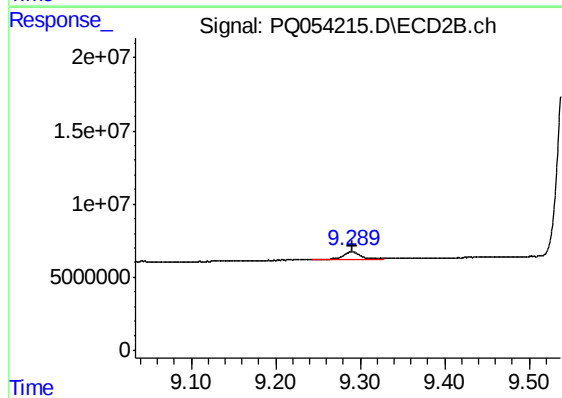

#45 AR-1268-5

R.T.: 9.290 min
Delta R.T.: 0.000 min
Response: 7779849
Conc: 1.65 ng/ml