

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ073119\
 Data File : PQ041902.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2019 02:53
 Operator : SM\AJ
 Sample : K4029-09
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 BENYO

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 04:42:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ072719CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jul 29 04:03:40 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.695	4.754	40689392	34815114	17.742	18.065
2)	SA Decachlor...	12.090	10.507	220.8E6	142.8E6	26.193	29.528
Target Compounds							
34)	L7 AR-1260-4	0.000	8.781	0	1467197	N.D.	7.253 #
35)	L7 AR-1260-5	0.000	9.030	0	2548493	N.D.	4.318 #
37)	L8 AR-1262-2	0.000	9.030	0	2548493	N.D.	3.439 #
38)	L8 AR-1262-3	0.000	9.365	0	1284306	N.D.	4.059 #
39)	L8 AR-1262-4	0.000	9.365	0	1284306	N.D.	2.284 #
41)	L9 AR-1268-1	0.000	9.365	0	1284306	N.D.	1.123 #
42)	L9 AR-1268-2	0.000	9.365	0	1284306	N.D.	1.251 #
43)	L9 AR-1268-3	0.000	9.602	0	1149086	N.D.	1.322 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ073119\
Data File : PQ041902.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Aug 2019 02:53
Operator : SM\AJ
Sample : K4029-09
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
BENYO

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 04:42:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ072719CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 29 04:03:40 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

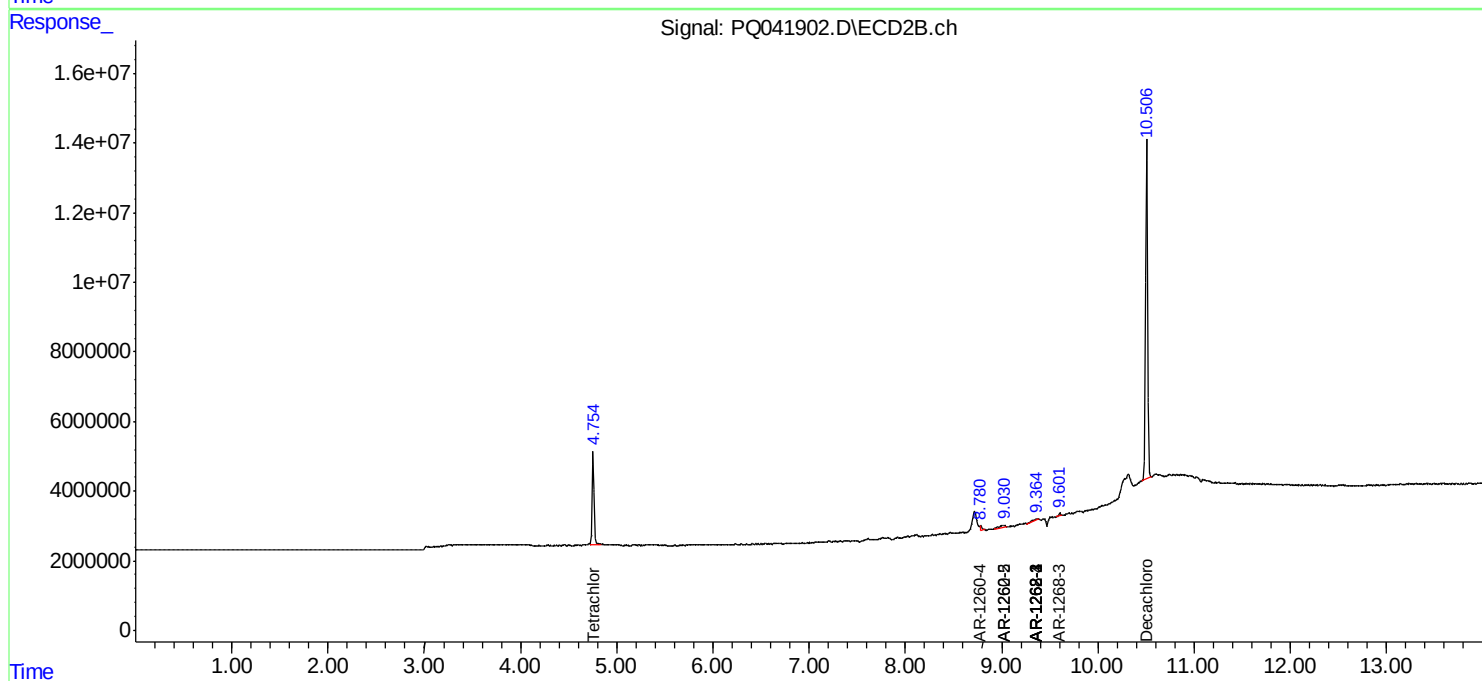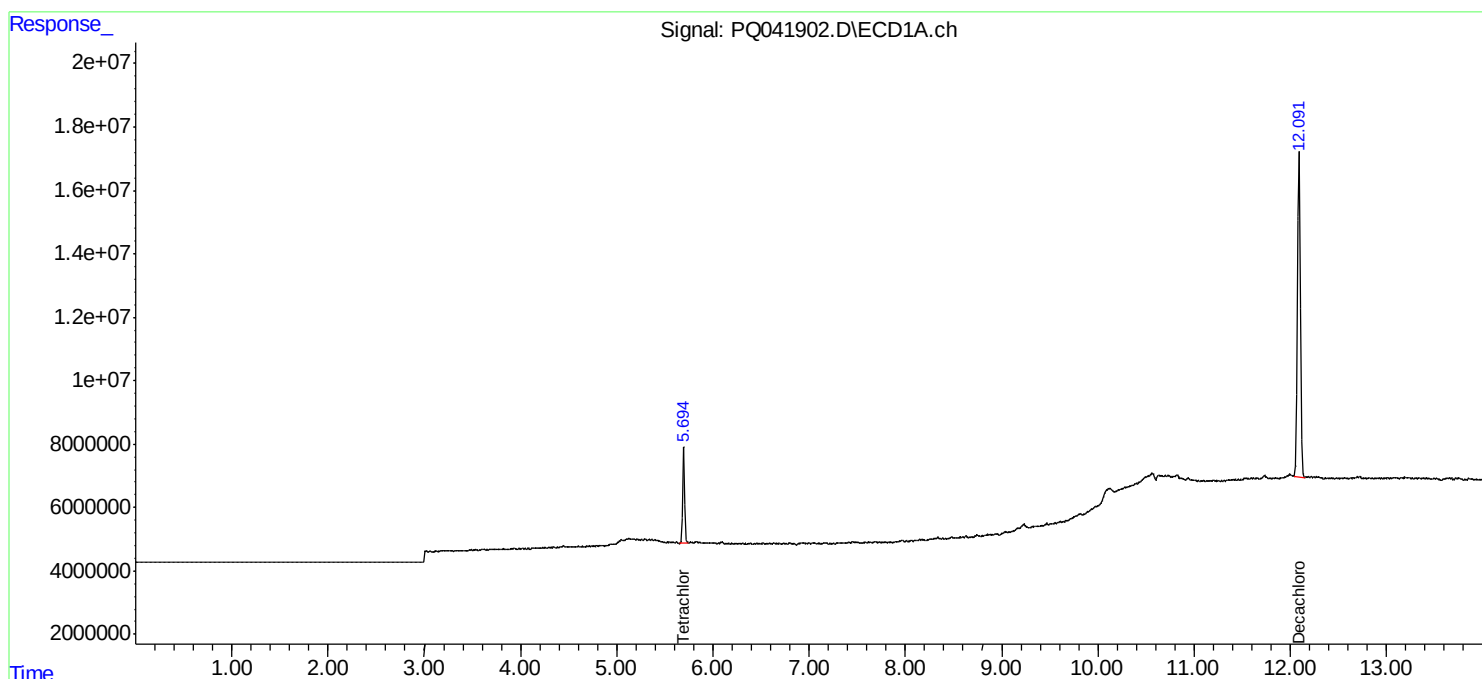


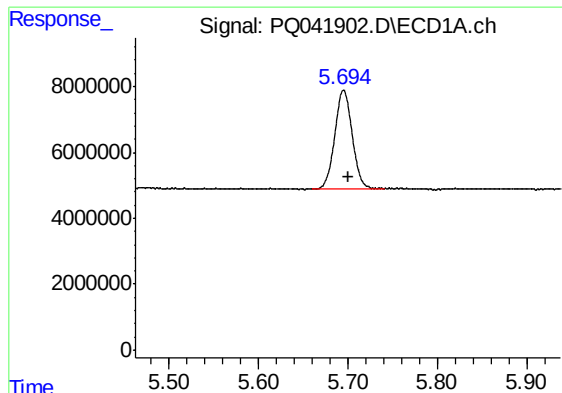

#1 Tetrachloro-m-xylene


R.T.: 5.695 min
Delta R.T.: -0.006 min
Response: 40689392
Conc: 17.74 ng/ml

Instrument :
ECD_Q
ClientSampleId :
BENY0

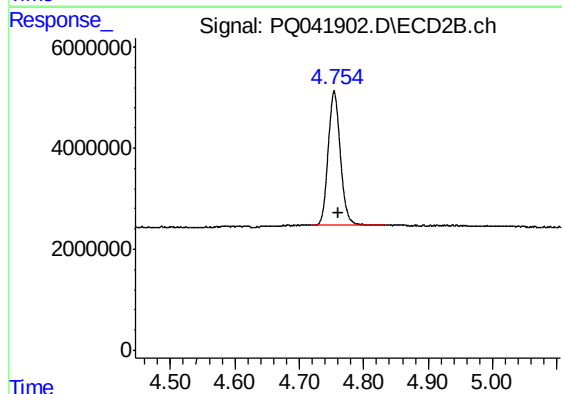


#1 Tetrachloro-m-xylene

R.T.: 4.754 min
Delta R.T.: -0.006 min
Response: 34815114
Conc: 18.06 ng/ml

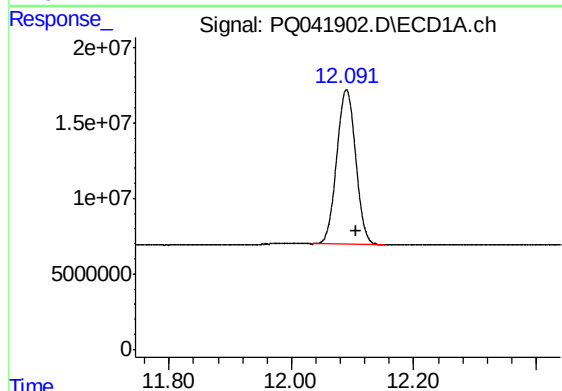


#2 Decachlorobiphenyl

R.T.: 12.090 min
Delta R.T.: -0.015 min
Response: 220843282
Conc: 26.19 ng/ml

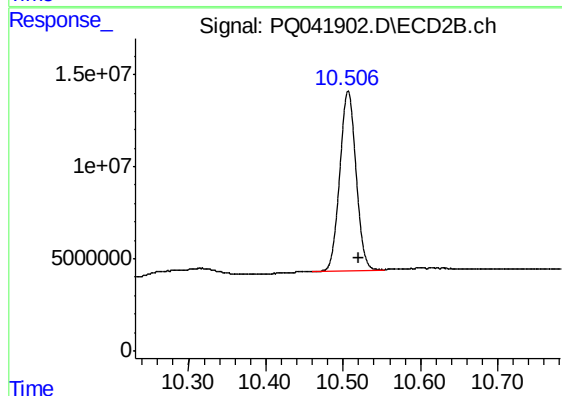

#2 Decachlorobiphenyl


R.T.: 10.507 min
Delta R.T.: -0.013 min
Response: 142838885
Conc: 29.53 ng/ml

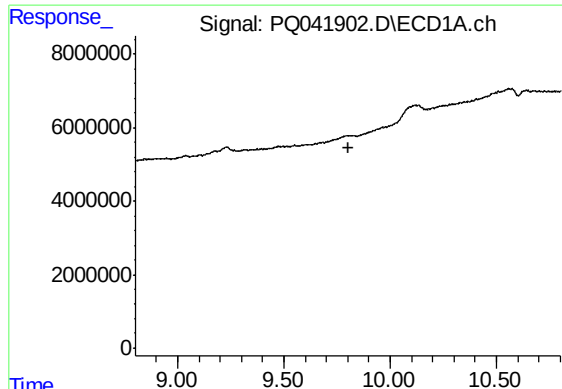

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 9.802 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
BENYO

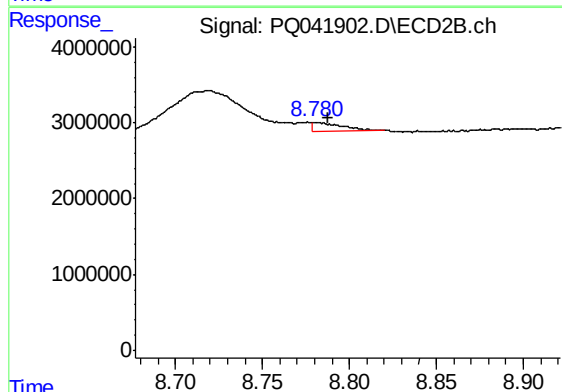


#34 AR-1260-4

R.T.: 8.781 min
Delta R.T.: -0.007 min
Response: 1467197
Conc: 7.25 ng/ml

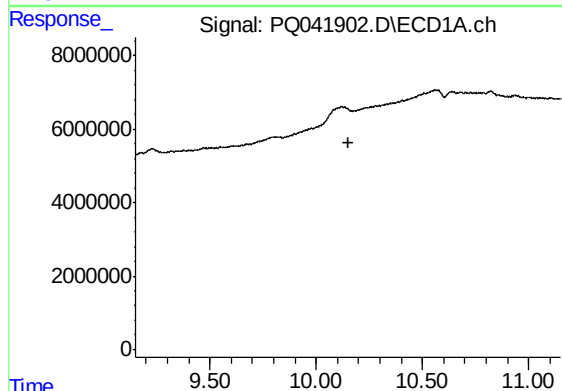


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 10.149 min
Response: 0
Conc: N.D.

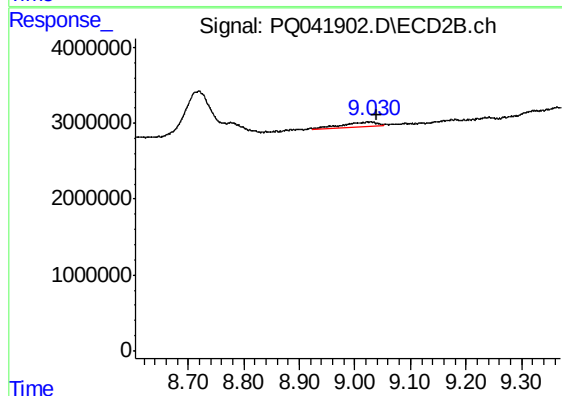

#35 AR-1260-5


R.T.: 9.030 min
Delta R.T.: -0.009 min
Response: 2548493
Conc: 4.32 ng/ml

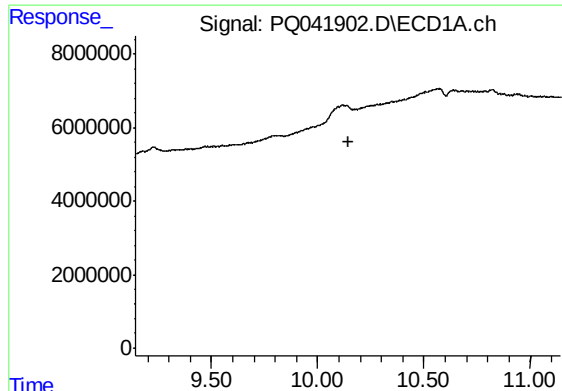

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T. : 10.142 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
BENYO

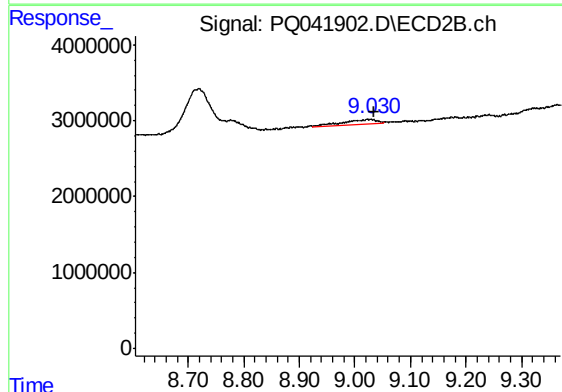


#37 AR-1262-2

R.T.: 9.030 min
Delta R.T.: -0.004 min
Response: 2548493
Conc: 3.44 ng/ml

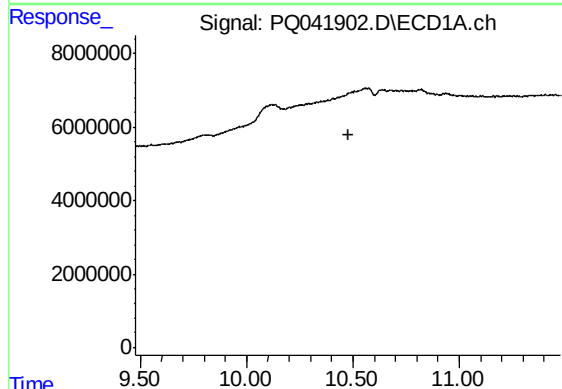


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 10.477 min
Response: 0
Conc: N.D.

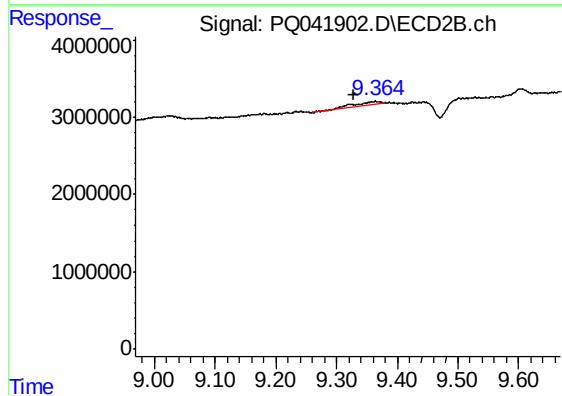

#38 AR-1262-3


R.T.: 9.365 min
Delta R.T.: 0.037 min
Response: 1284306
Conc: 4.06 ng/ml

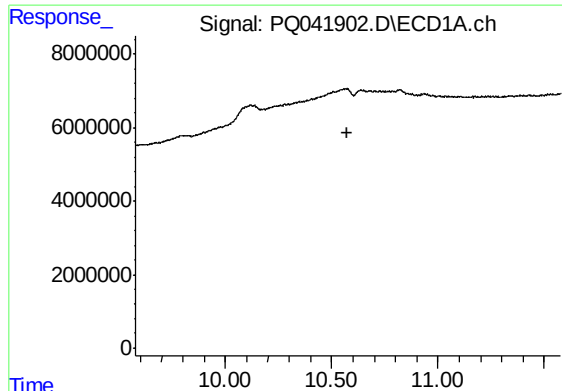

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T. : 10.576 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
BENYO

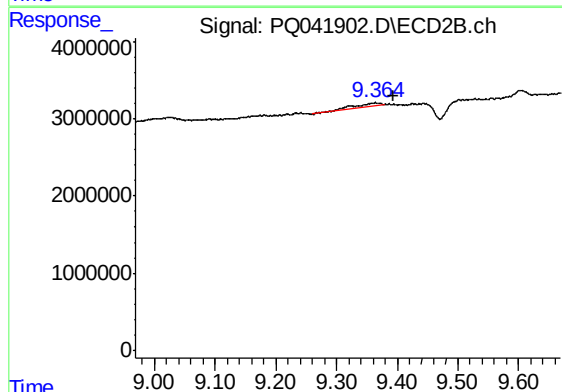


#39 AR-1262-4

R.T.: 9.365 min
Delta R.T.: -0.030 min
Response: 1284306
Conc: 2.28 ng/ml

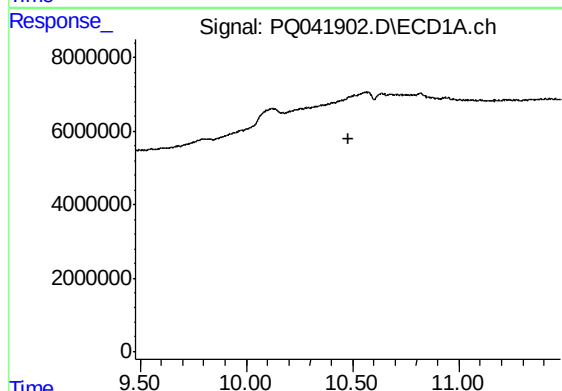


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 10.478 min
Response: 0
Conc: N.D.

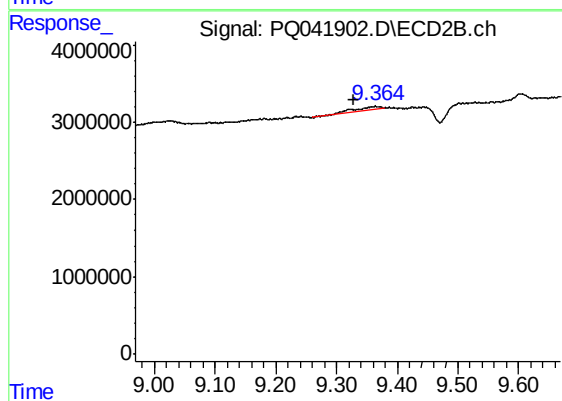

#41 AR-1268-1


R.T.: 9.365 min
Delta R.T.: 0.036 min
Response: 1284306
Conc: 1.12 ng/ml

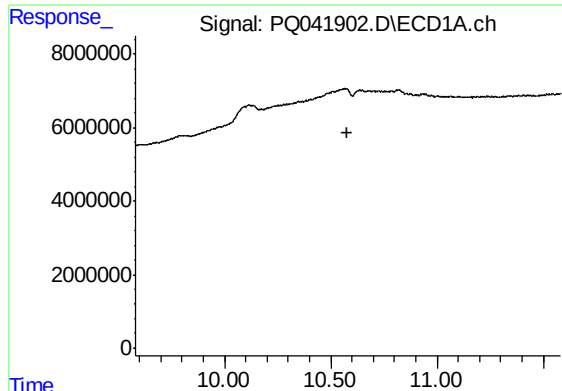

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T. : 10.581 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
BENYO

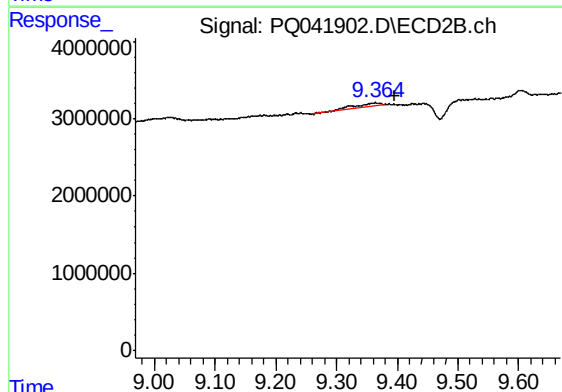


#42 AR-1268-2

R.T.: 9.365 min
Delta R.T.: -0.031 min
Response: 1284306
Conc: 1.25 ng/ml

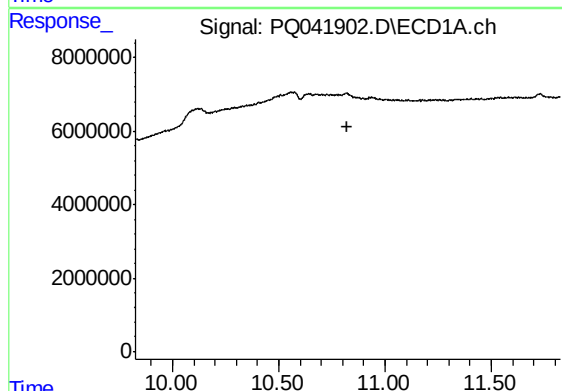

#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 10.825 min
Response: 0
Conc: N.D.

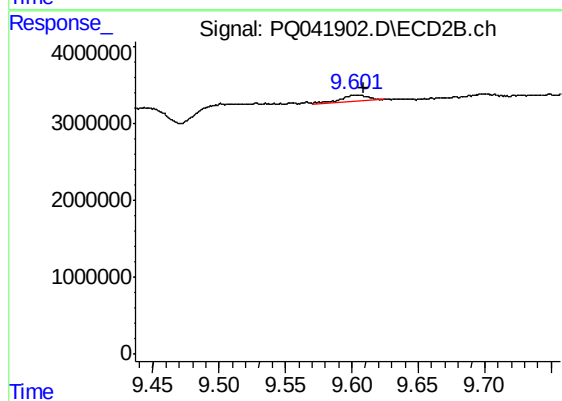

#43 AR-1268-3

R.T.: 9.602 min
Delta R.T.: -0.008 min
Response: 1149086
Conc: 1.32 ng/ml