

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ073124\
 Data File : PQ067564.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jul 2024 13:15
 Operator : YP\AJ
 Sample : P3392-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 31 13:48:44 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ072424.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 24 19:21:12 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	3.460	2.828	113.3E6	119.6E6	19.880	19.758
2) SA Decachlor...	8.739	7.613	49570871	70696860	12.948	12.298

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ073124\
Data File : PQ067564.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jul 2024 13:15
Operator : YP\AJ
Sample : P3392-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 31 13:48:44 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ072424.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 24 19:21:12 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

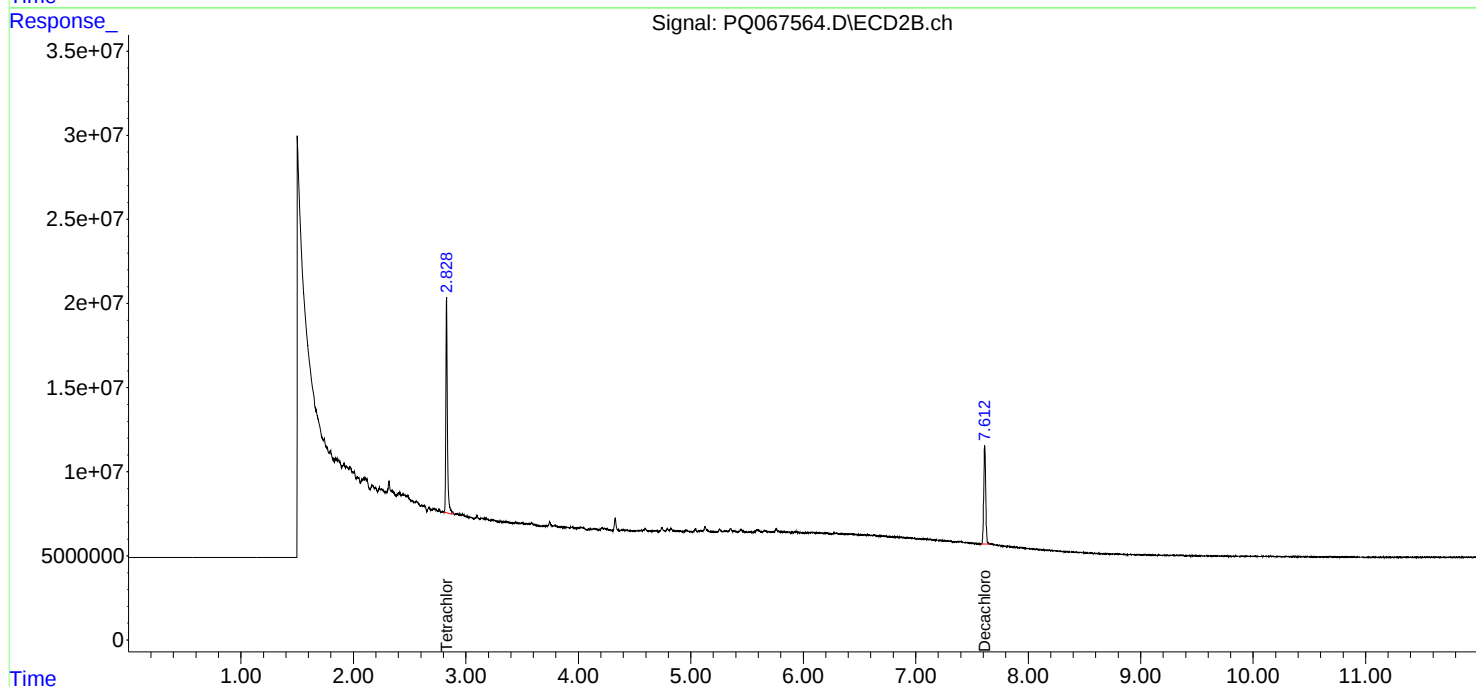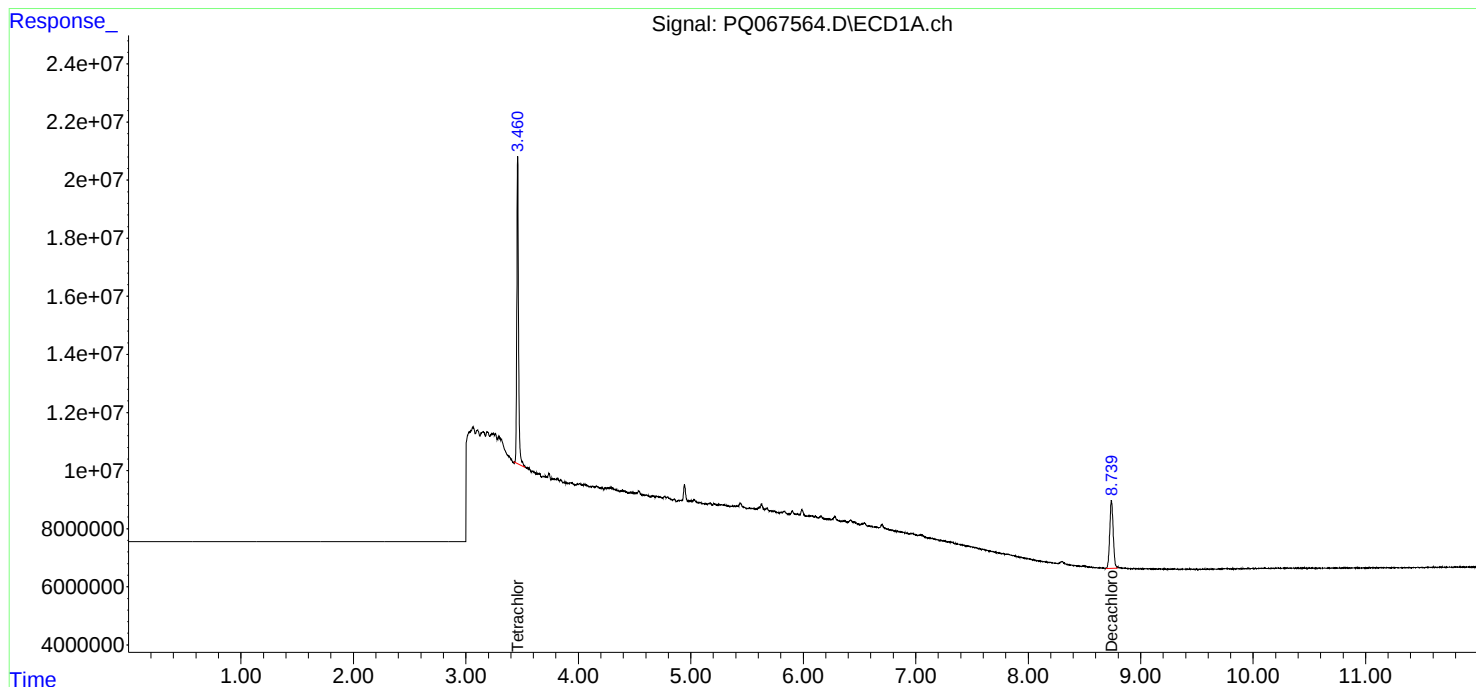


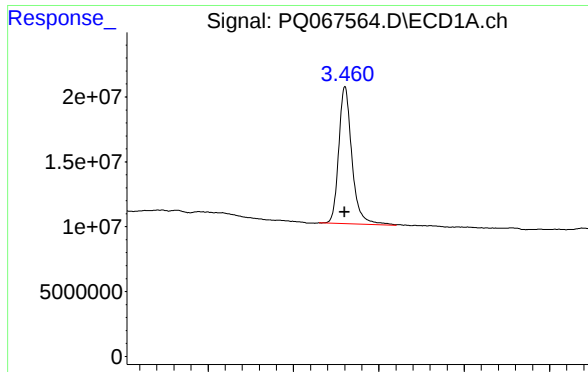

#1 Tetrachloro-m-xylene


R.T.: 3.460 min
Delta R.T.: 0.000 min
Response: 113260203
Conc: 19.88 ng/ml

Instrument :
ECD_Q
ClientSampleId :
COMP

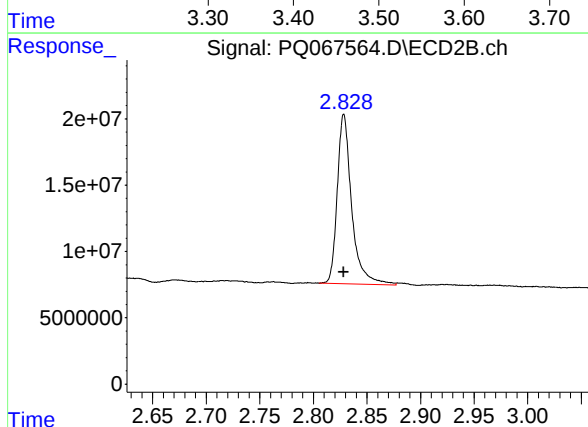


#1 Tetrachloro-m-xylene

R.T.: 2.828 min
Delta R.T.: 0.000 min
Response: 119639259
Conc: 19.76 ng/ml

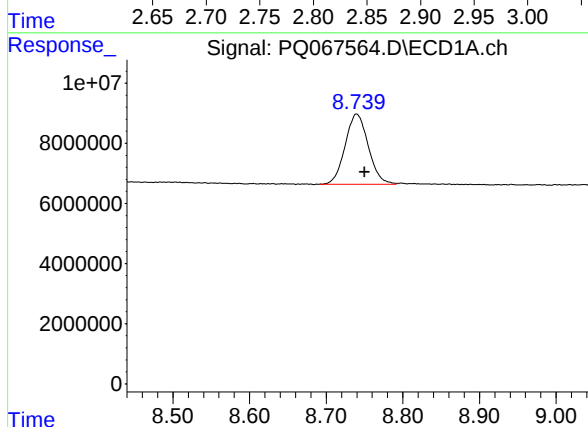

#2 Decachlorobiphenyl

R.T.: 8.739 min
Delta R.T.: -0.011 min
Response: 49570871
Conc: 12.95 ng/ml

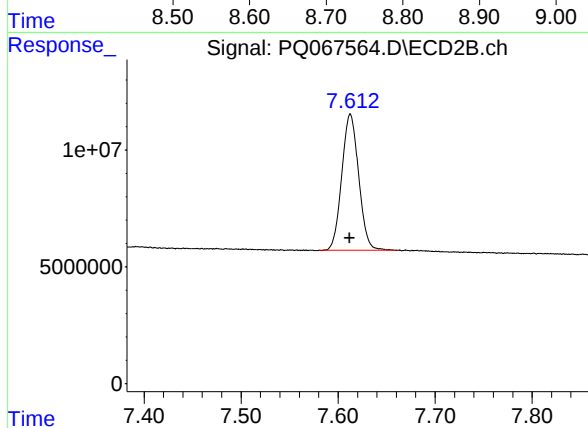

#2 Decachlorobiphenyl

R.T.: 7.613 min
Delta R.T.: 0.000 min
Response: 70696860
Conc: 12.30 ng/ml