

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ080723\
 Data File : PQ062838.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Aug 2023 19:38
 Operator : YP\AJ
 Sample : 03911-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 PSCR206(164716)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 08 02:25:37 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ072623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 27 01:22:50 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.401	2.754	81005606	76327635	17.969	25.082 #
2) SA Decachlor...	8.583	7.522	61575657	62850122	16.688	19.325

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ080723\
Data File : PQ062838.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Aug 2023 19:38
Operator : YP\AJ
Sample : 03911-01
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
PSCR206(164716)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 08 02:25:37 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ072623.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 27 01:22:50 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

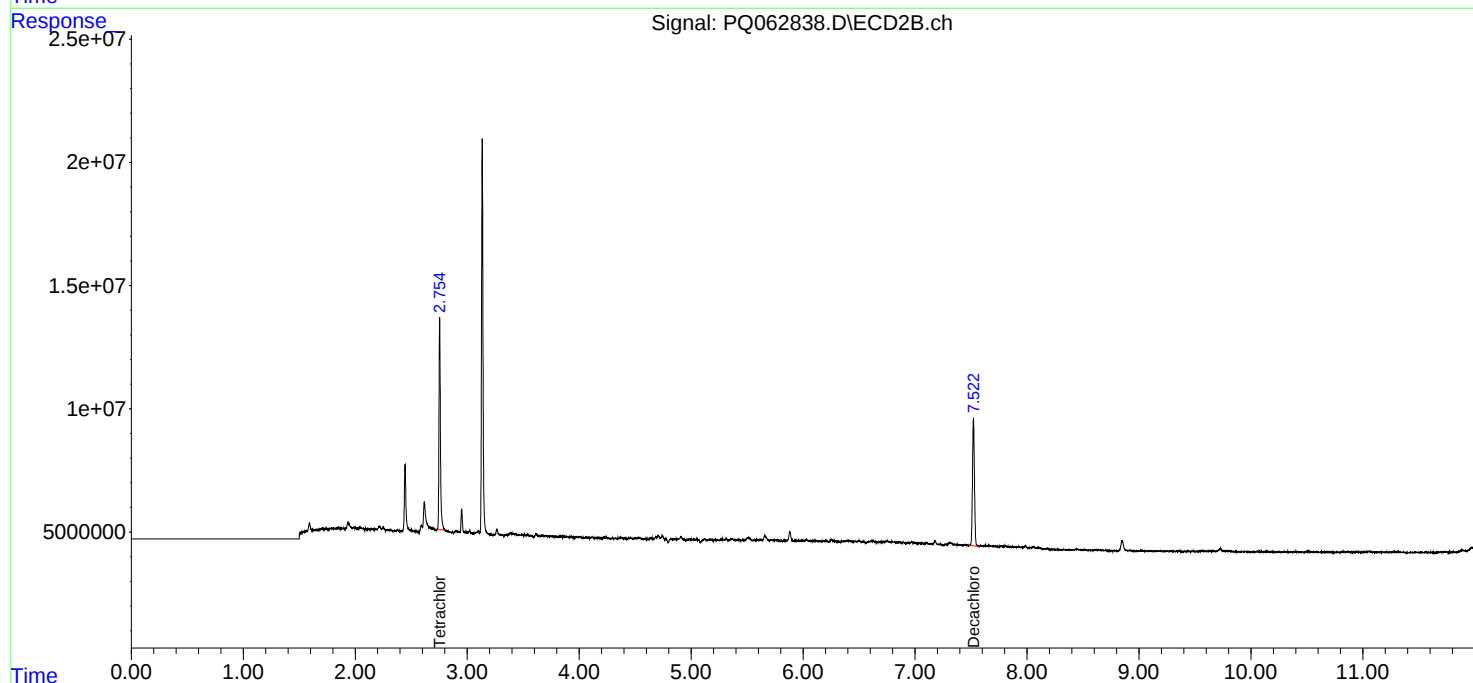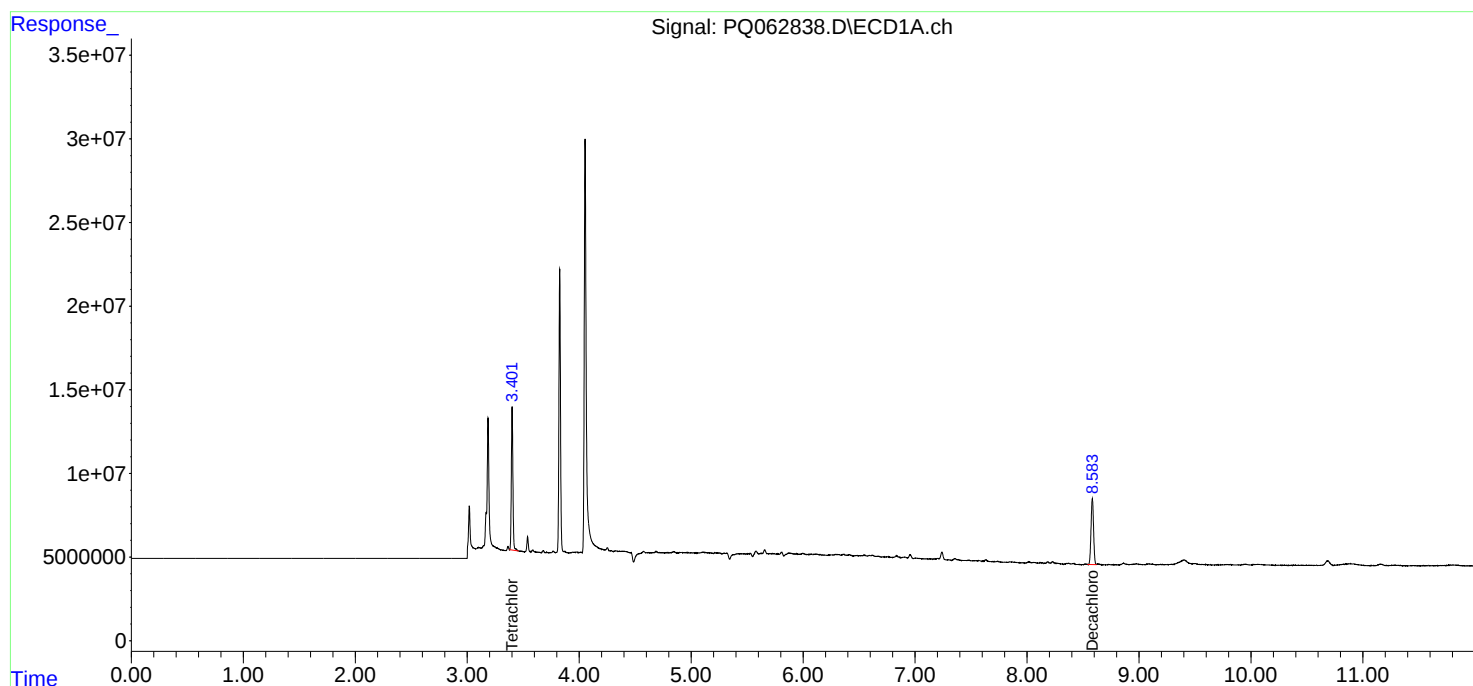


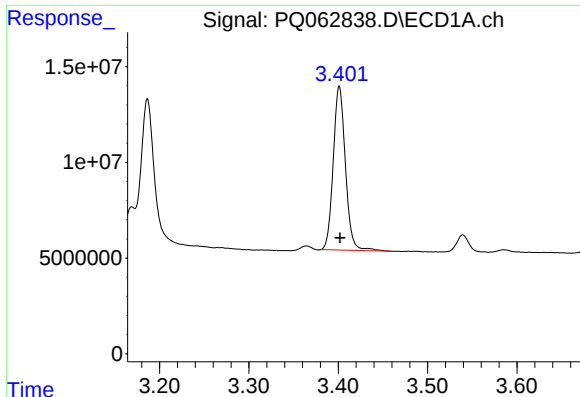

#1 Tetrachloro-m-xylene


R.T.: 3.401 min
Delta R.T.: 0.000 min
Response: 81005606
Conc: 17.97 ng/ml

Instrument :
ECD_Q
ClientSampleId :
PSCR206(164716)

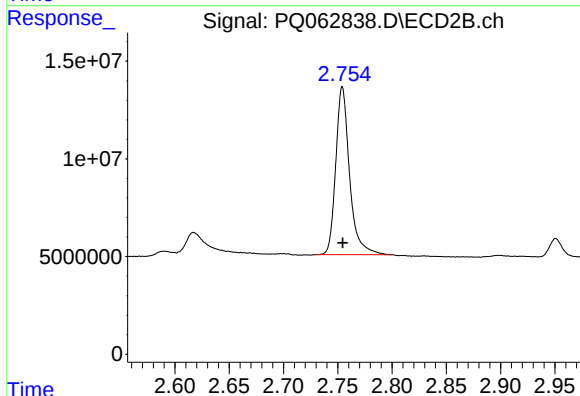


#1 Tetrachloro-m-xylene

R.T.: 2.754 min
Delta R.T.: 0.000 min
Response: 76327635
Conc: 25.08 ng/ml

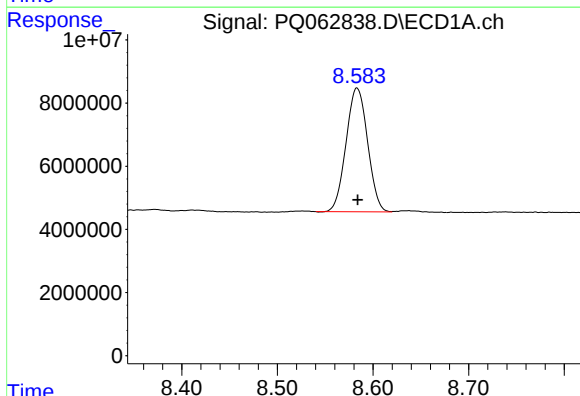

#2 Decachlorobiphenyl

R.T.: 8.583 min
Delta R.T.: 0.000 min
Response: 61575657
Conc: 16.69 ng/ml

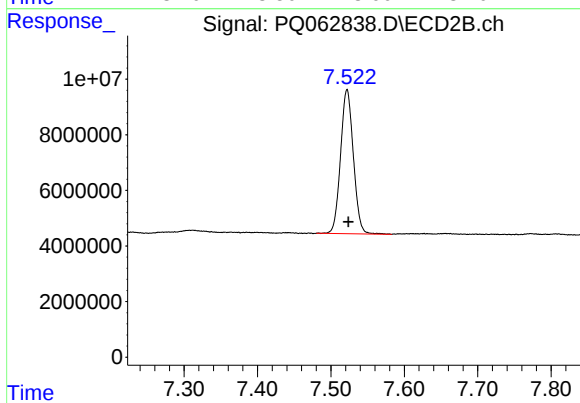

#2 Decachlorobiphenyl

R.T.: 7.522 min
Delta R.T.: -0.002 min
Response: 62850122
Conc: 19.33 ng/ml