

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ081023\
 Data File : PQ062995.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Aug 2023 03:47
 Operator : YP\AJ
 Sample : 03572-09
 Misc : AR1221 MDL 25 PPB
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 MDL-WATER-03-QT3-2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 11 05:51:04 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ080923.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Aug 10 11:15:56 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.453	2.782	98702023	74530076	18.369	18.071
2)	SA Decachlor...	8.687	7.591	83124357	86321703	21.469	19.957
Target Compounds							
8)	L2 AR-1221-1	3.656	2.986	1953411	1249111	28.707	22.764
9)	L2 AR-1221-2	3.734	3.053	2555210	1492191	53.556	39.561 #
10)	L2 AR-1221-3	3.805	3.132	4318561	3502866	27.983	29.112



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ081023\
Data File : PQ062995.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Aug 2023 03:47
Operator : YP\AJ
Sample : 03572-09
Misc : AR1221 MDL 25 PPB
ALS Vial : 57 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT3-2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 05:51:04 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ080923.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 10 11:15:56 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

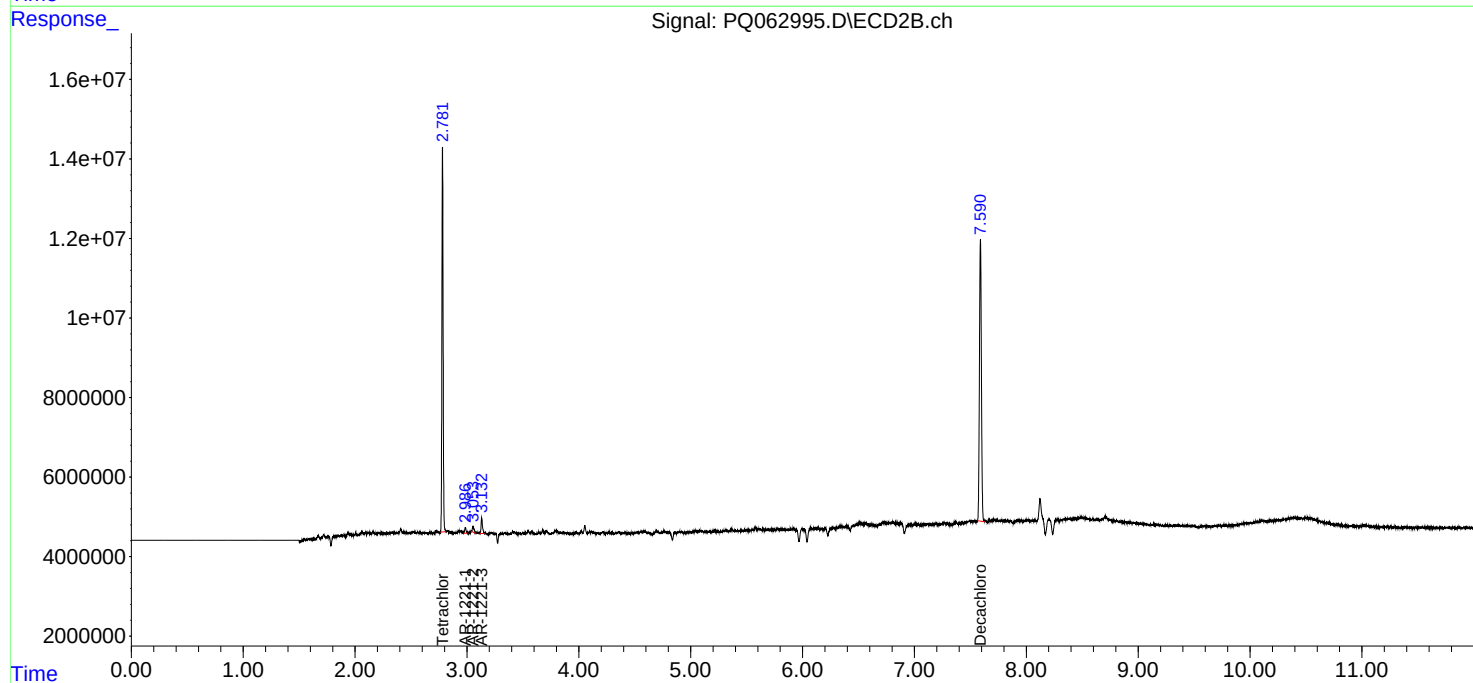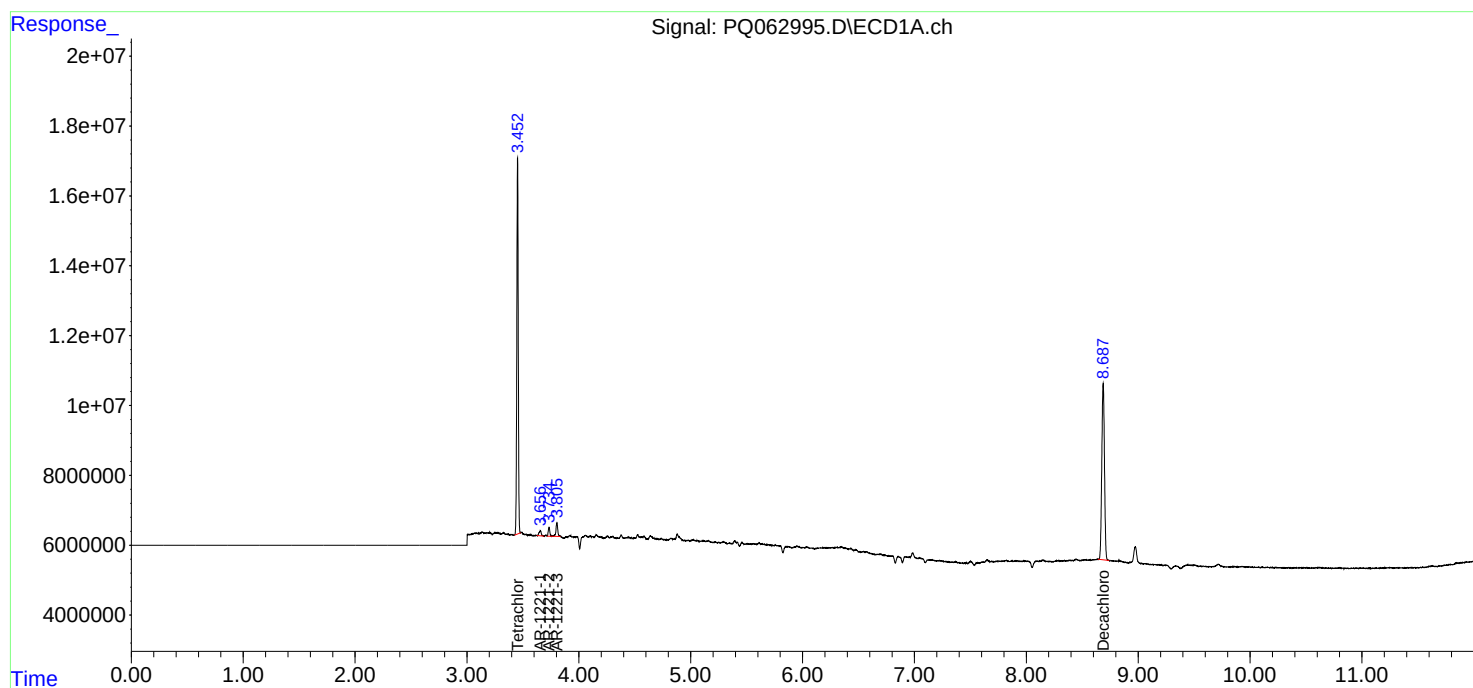


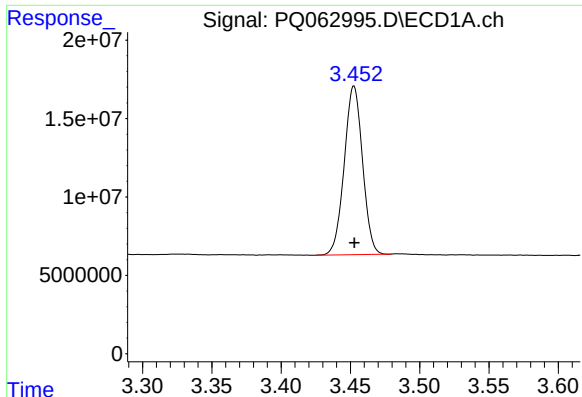

#1 Tetrachloro-m-xylene


R.T.: 3.453 min
Delta R.T.: 0.000 min
Response: 98702023
Conc: 18.37 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT3-2023

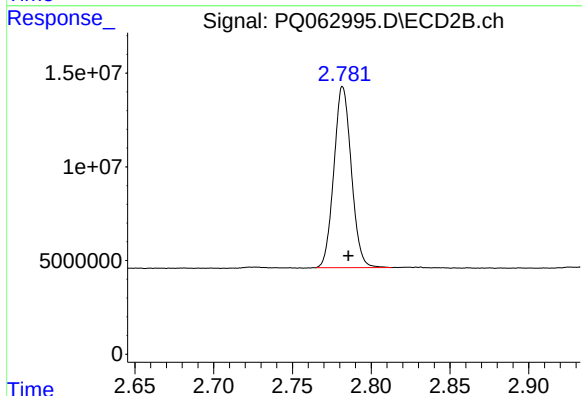


#1 Tetrachloro-m-xylene

R.T.: 2.782 min
Delta R.T.: -0.003 min
Response: 74530076
Conc: 18.07 ng/ml

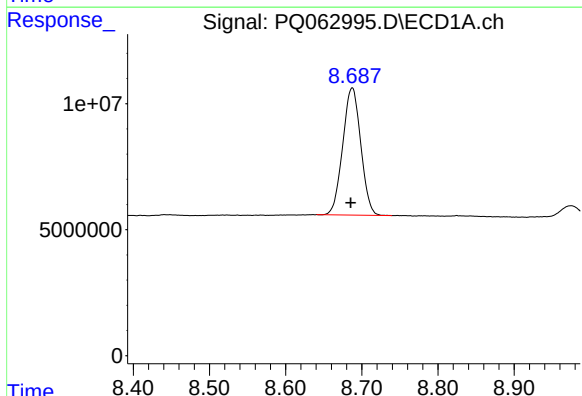


#2 Decachlorobiphenyl

R.T.: 8.687 min
Delta R.T.: 0.002 min
Response: 83124357
Conc: 21.47 ng/ml

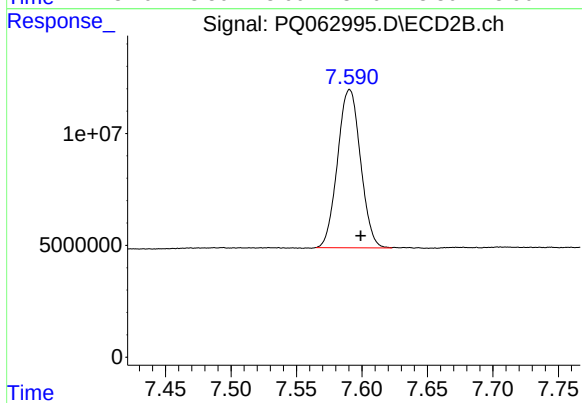

#2 Decachlorobiphenyl


R.T.: 7.591 min
Delta R.T.: -0.008 min
Response: 86321703
Conc: 19.96 ng/ml

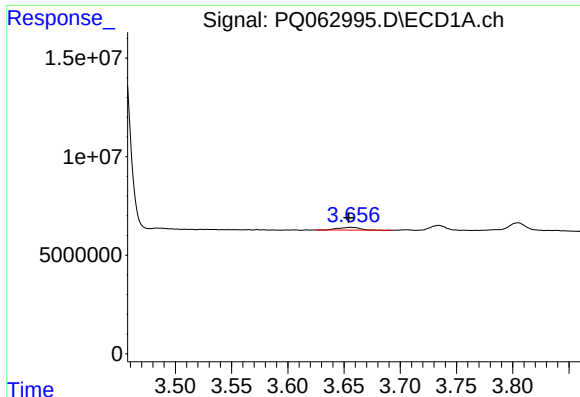

#8 AR-1221-1


R.T.: 3.656 min
Delta R.T.: 0.002 min
Response: 1953411
Conc: 28.71 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT3-2023

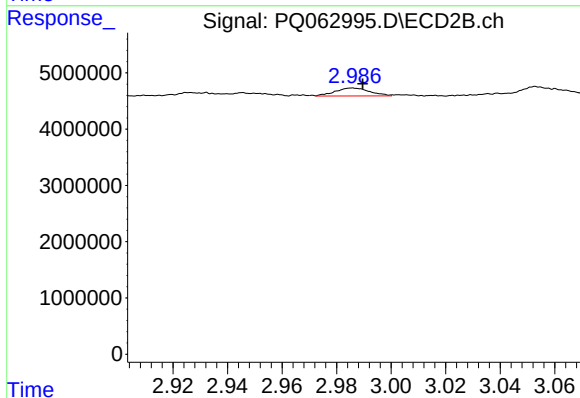


#8 AR-1221-1

R.T.: 2.986 min
Delta R.T.: -0.004 min
Response: 1249111
Conc: 22.76 ng/ml

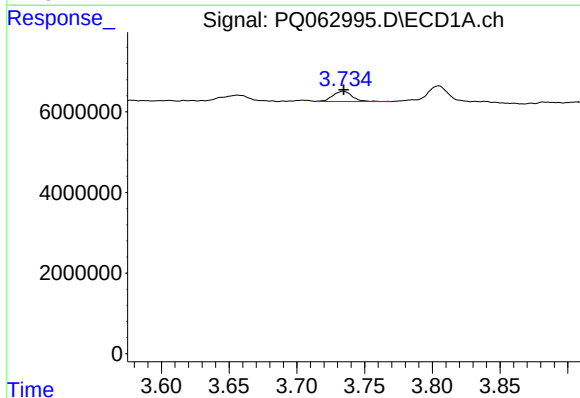


#9 AR-1221-2

R.T.: 3.734 min
Delta R.T.: 0.000 min
Response: 2555210
Conc: 53.56 ng/ml

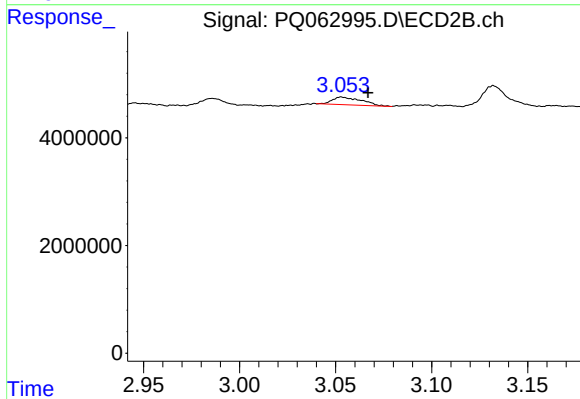

#9 AR-1221-2


R.T.: 3.053 min
Delta R.T.: -0.014 min
Response: 1492191
Conc: 39.56 ng/ml

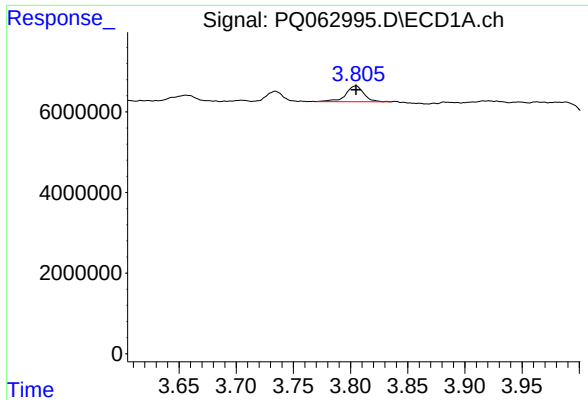

#10 AR-1221-3

R.T.: 3.805 min
Delta R.T.: 0.000 min
Response: 4318561
Conc: 27.98 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT3-2023

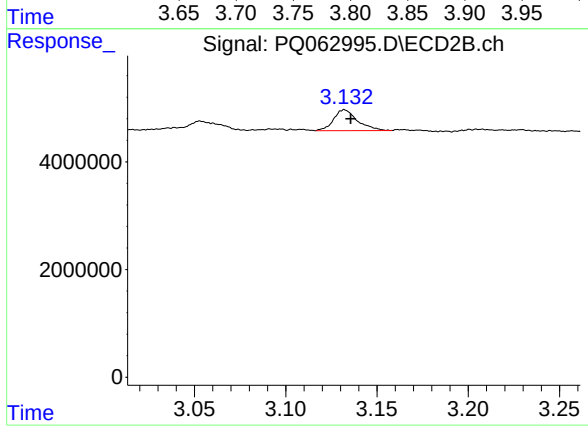

#10 AR-1221-3

R.T.: 3.132 min
Delta R.T.: -0.003 min
Response: 3502866
Conc: 29.11 ng/ml