

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ081124\
 Data File : PQ067854.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Aug 2024 06:31
 Operator : YP\AJ
 Sample : P3534-01
 Misc :
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 PIPE-BLAST-GRIT

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 12 09:03:00 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ080524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 09 02:37:44 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.459	2.826	145.2E6	153.7E6	24.469	24.236
2) SA Decachlor...	8.735	7.607	100.1E6	131.1E6	25.979	23.263

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ081124\
Data File : PQ067854.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Aug 2024 06:31
Operator : YP\AJ
Sample : P3534-01
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
PIPE-BLAST-GRIT

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 12 09:03:00 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ080524.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 09 02:37:44 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

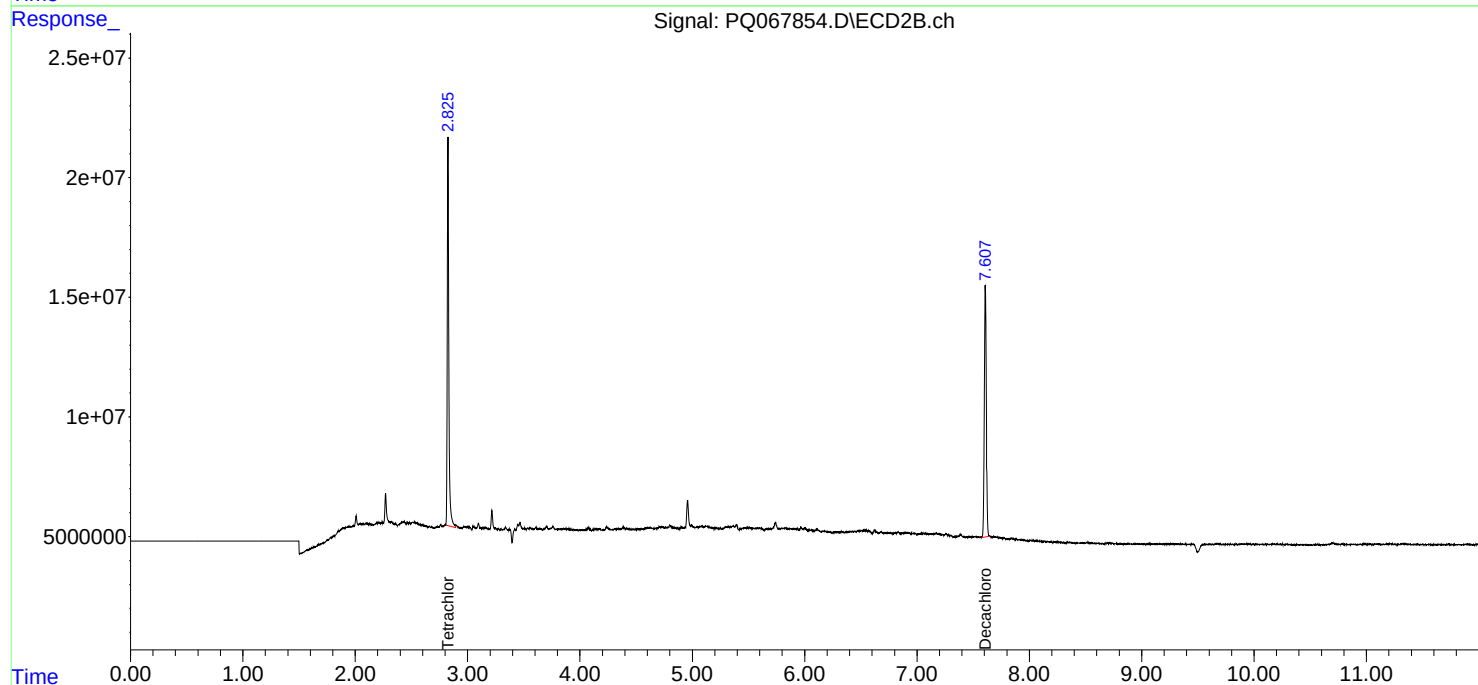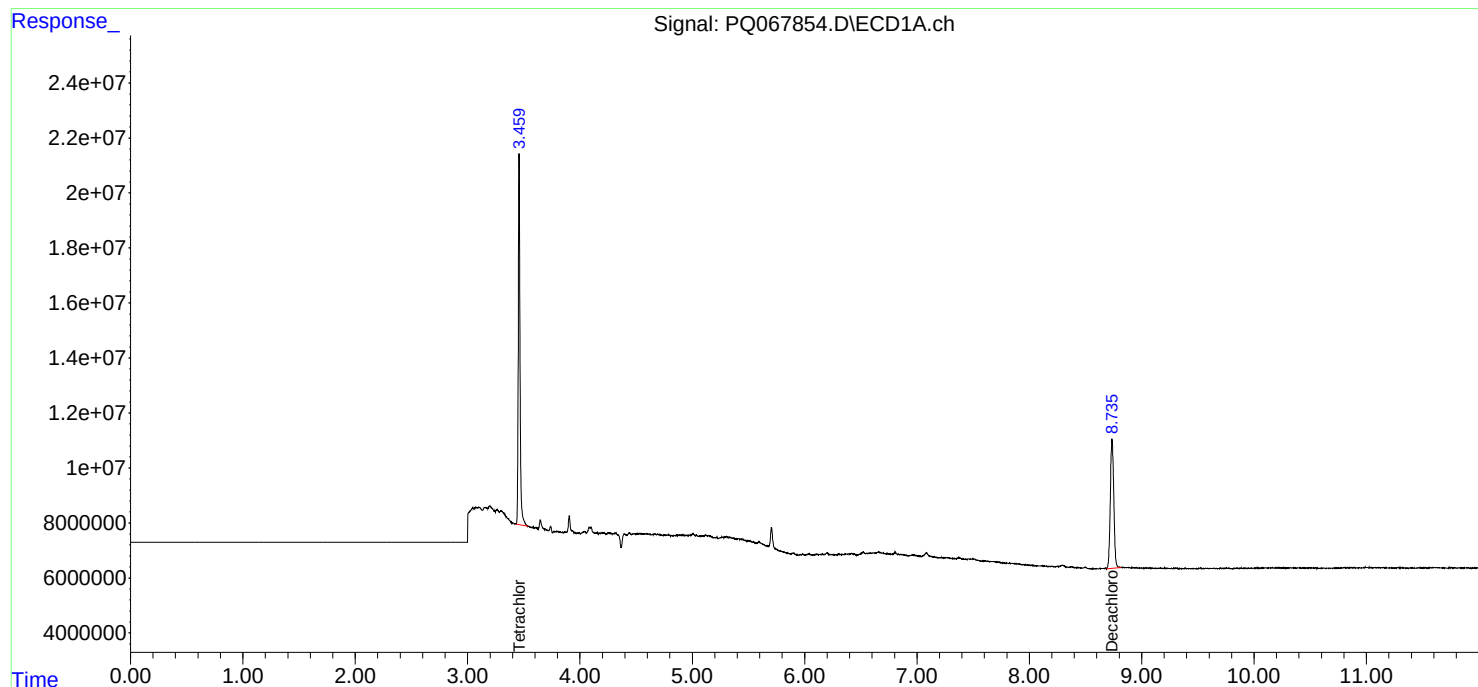


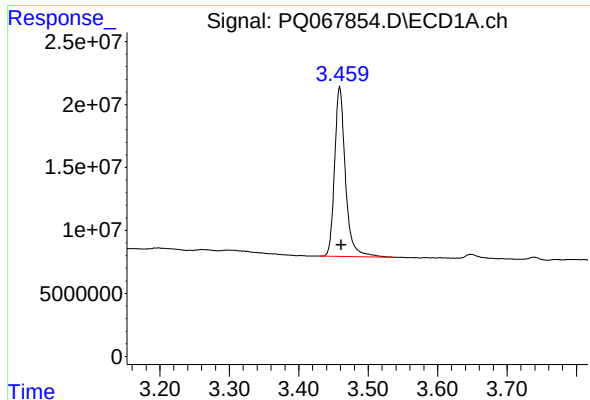

#1 Tetrachloro-m-xylene


R.T.: 3.459 min
Delta R.T.: -0.002 min
Response: 145176406
Conc: 24.47 ng/ml

Instrument :
ECD_Q
ClientSampleId :
PIPE-BLAST-GRIT

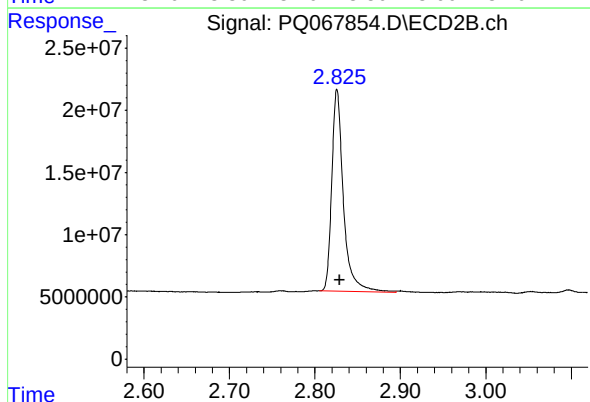


#1 Tetrachloro-m-xylene

R.T.: 2.826 min
Delta R.T.: -0.003 min
Response: 153710380
Conc: 24.24 ng/ml

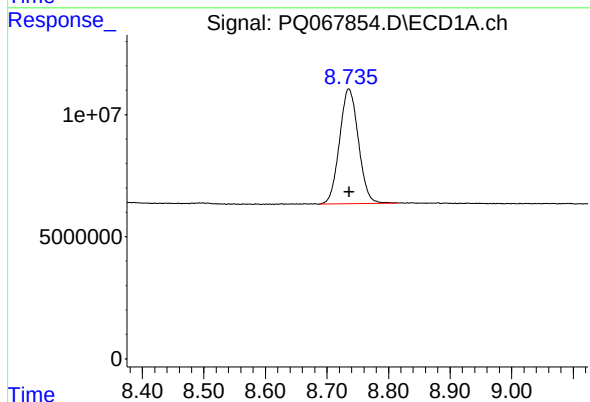

#2 Decachlorobiphenyl

R.T.: 8.735 min
Delta R.T.: 0.000 min
Response: 100099088
Conc: 25.98 ng/ml

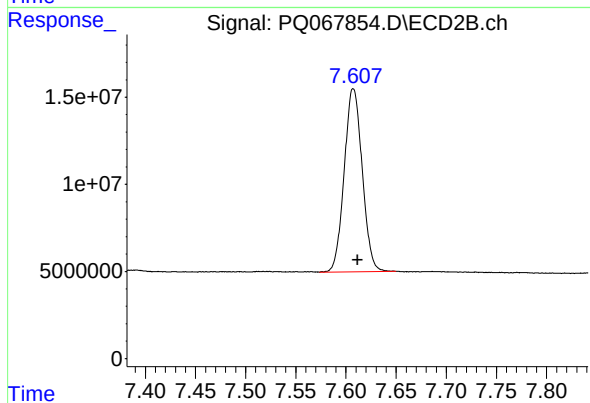

#2 Decachlorobiphenyl

R.T.: 7.607 min
Delta R.T.: -0.005 min
Response: 131109963
Conc: 23.26 ng/ml