

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ081324\
 Data File : PQ067932.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Aug 2024 05:43
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 10:20:03 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ080524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 09 02:37:44 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	3.459	2.826	131.7E6	145.3E6	22.201	22.910
2) SA Decachlor...	8.738	7.607	94831342	135.7E6	24.612	24.074

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ081324\
Data File : PQ067932.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2024 05:43
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 10:20:03 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ080524.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 09 02:37:44 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

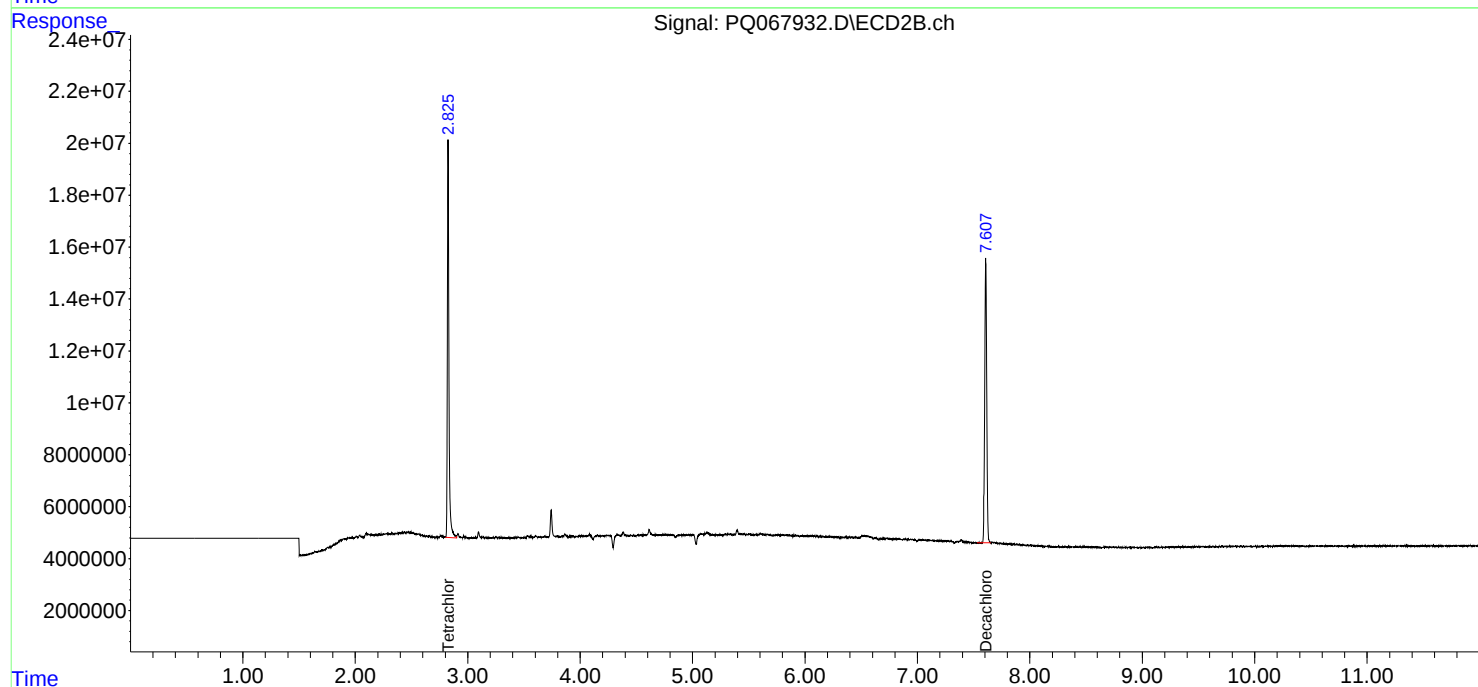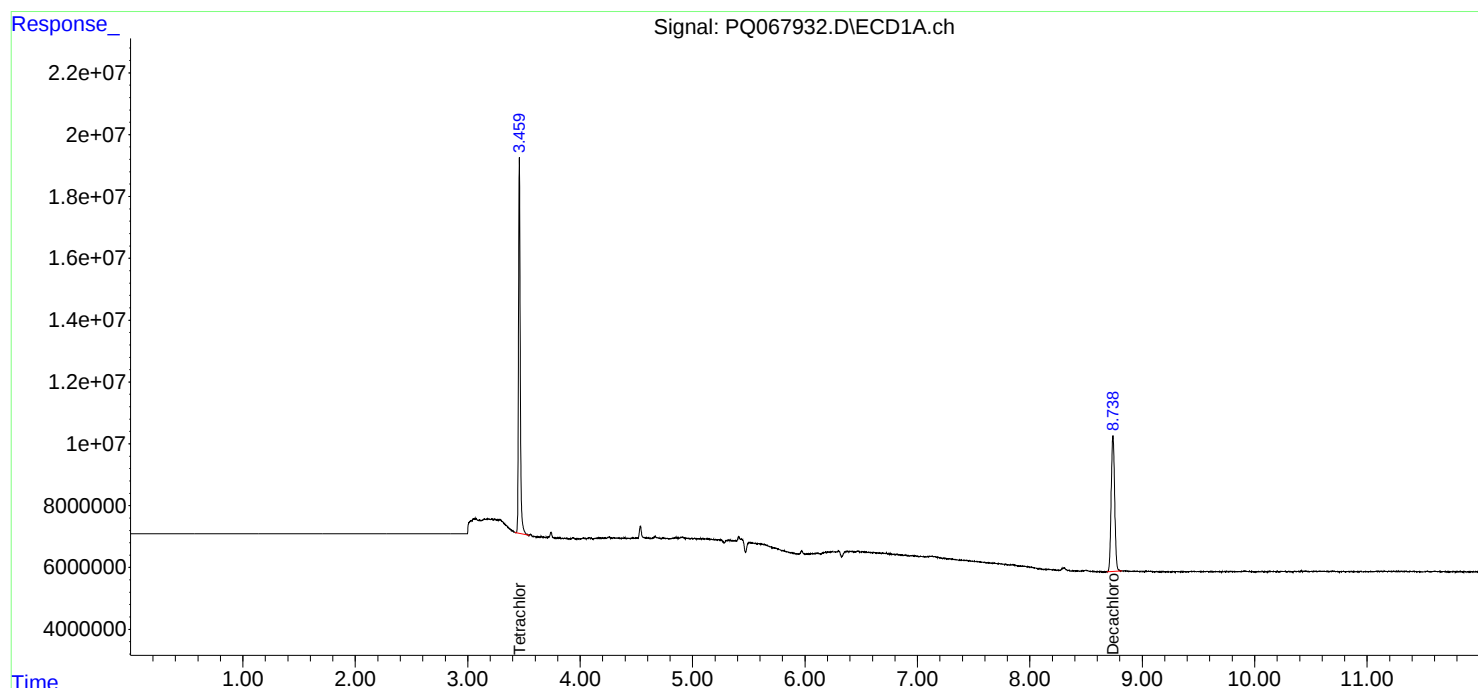


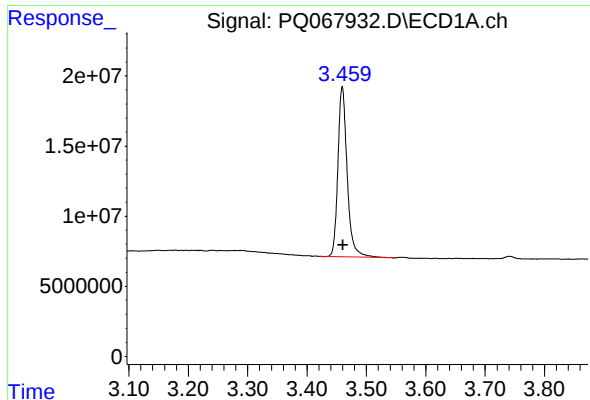

#1 Tetrachloro-m-xylene


R.T.: 3.459 min
Delta R.T.: -0.002 min
Response: 131722759
Conc: 22.20 ng/ml

Instrument :
ECD_Q
ClientSampleId :
I.BLK

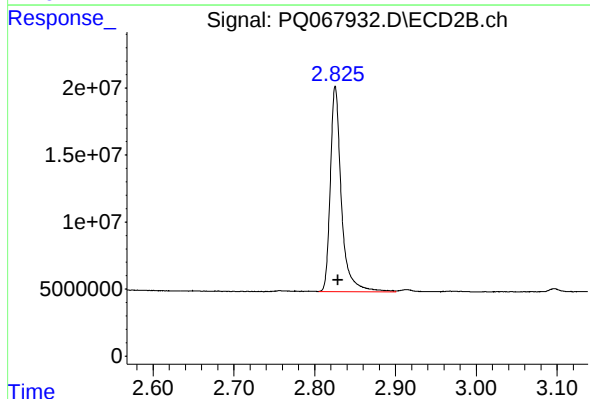


#1 Tetrachloro-m-xylene

R.T.: 2.826 min
Delta R.T.: -0.003 min
Response: 145299467
Conc: 22.91 ng/ml

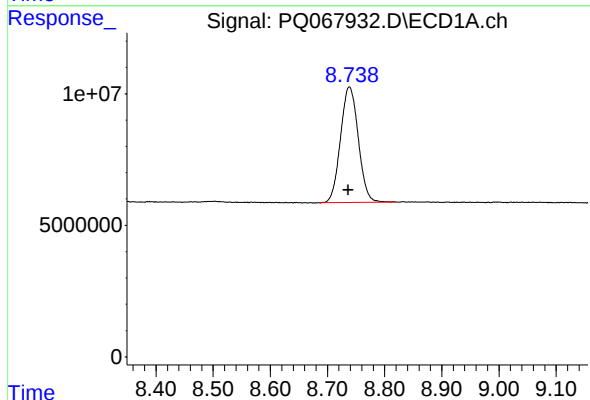

#2 Decachlorobiphenyl

R.T.: 8.738 min
Delta R.T.: 0.002 min
Response: 94831342
Conc: 24.61 ng/ml

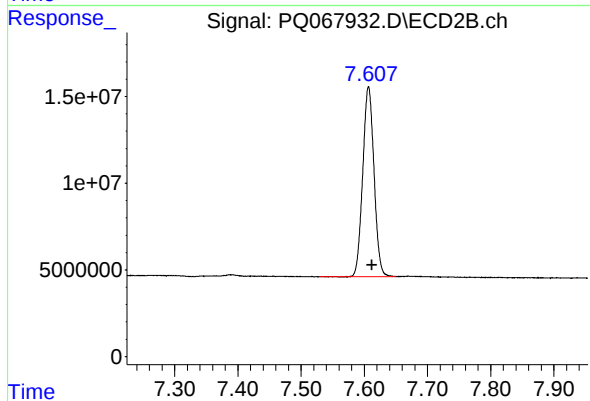

#2 Decachlorobiphenyl

R.T.: 7.607 min
Delta R.T.: -0.005 min
Response: 135683261
Conc: 24.07 ng/ml