

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ081424\
 Data File : PQ067963.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Aug 2024 18:29
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/14/2024
 Supervised By :Ankita Jodhani 08/14/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 02:21:09 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ080524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 09 02:37:44 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.459	2.826	135.9E6	149.2E6	22.903	23.528
2) SA Decachlor...	8.736	7.605	101.0E6	148.0E6	26.223	26.257m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ081424\
Data File : PQ067963.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2024 18:29
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/14/2024
Supervised By :Ankita Jodhani 08/14/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 02:21:09 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ080524.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 09 02:37:44 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

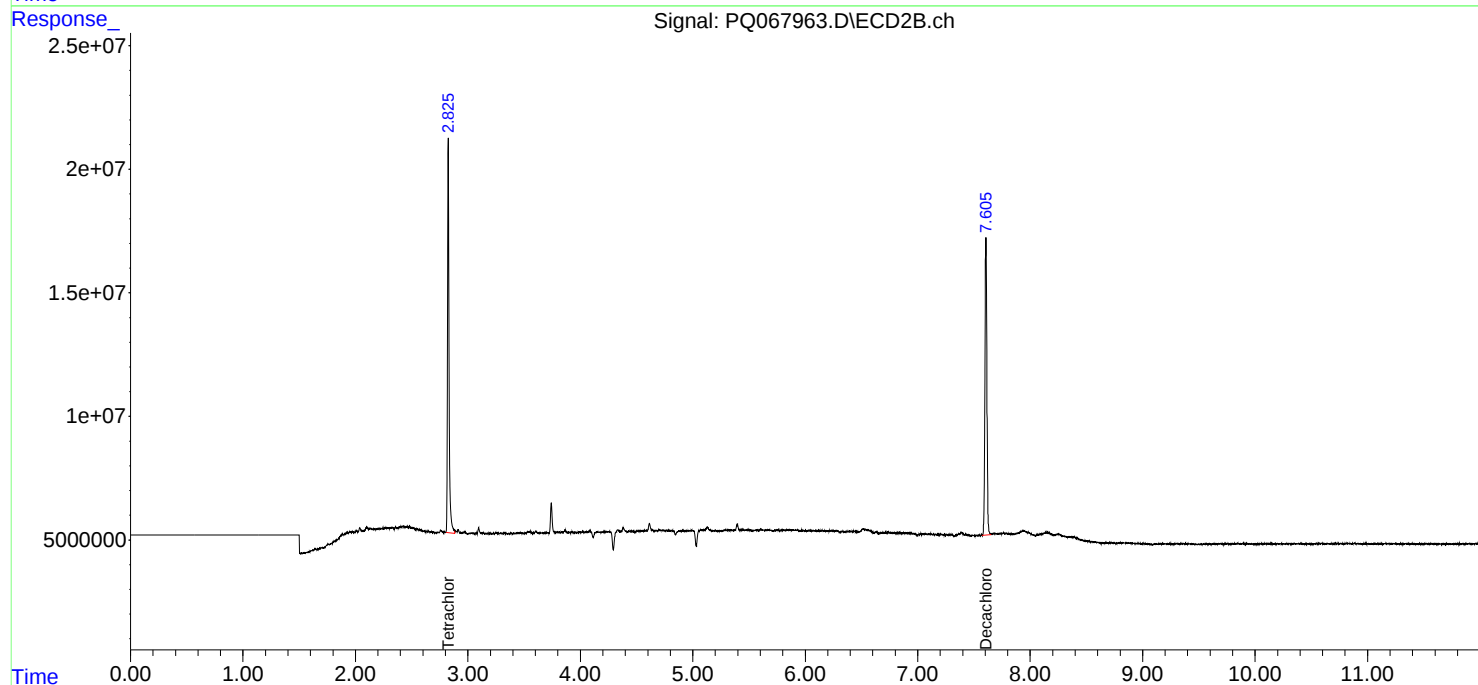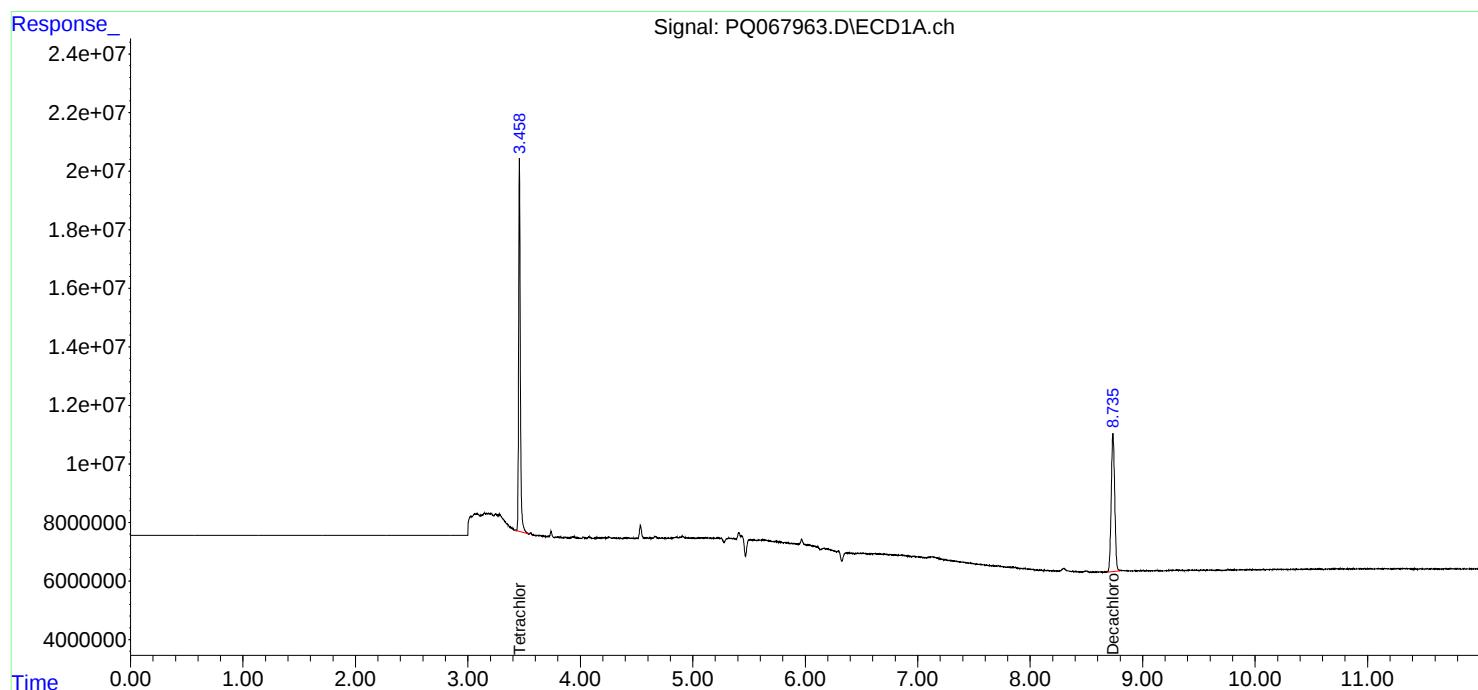

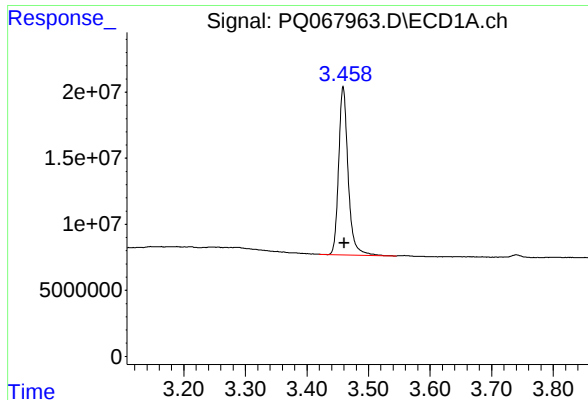


#1 Tetrachloro-m-xylene

R.T.: 3.459 min
Delta R.T.: -0.002 min
Response: 135885489
Conc: 22.90 ng/ml

Instrument :
ECD_Q
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/14/2024
Supervised By :Ankita Jodhani 08/14/2024

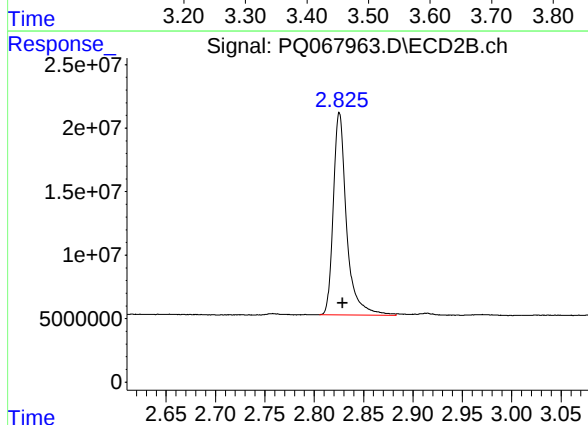


#1 Tetrachloro-m-xylene

R.T.: 2.826 min
Delta R.T.: -0.003 min
Response: 149218784
Conc: 23.53 ng/ml

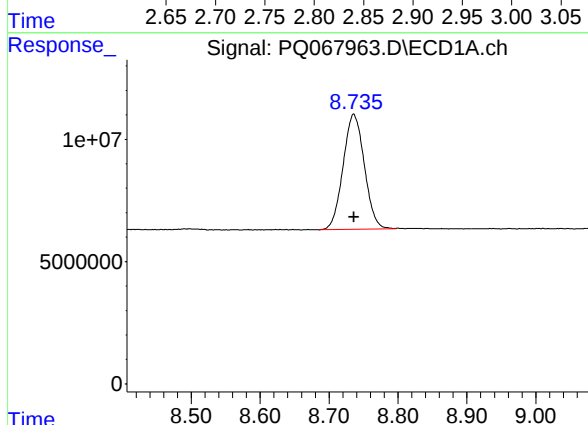

#2 Decachlorobiphenyl

R.T.: 8.736 min
Delta R.T.: 0.000 min
Response: 101037767
Conc: 26.22 ng/ml

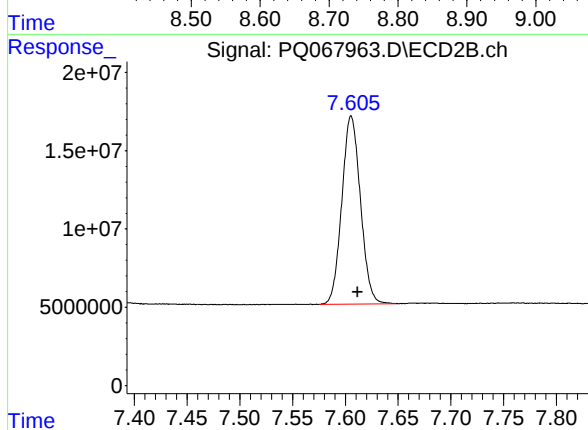

#2 Decachlorobiphenyl

R.T.: 7.605 min
Delta R.T.: -0.007 min
Response: 147987984
Conc: 26.26 ng/ml m