

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ081724\
 Data File : PQ068050.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Aug 2024 17:29
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 17 05:02:00 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ080524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 09 02:37:44 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	3.458	2.825	140.9E6	152.5E6	23.746	24.050
2) SA Decachlor...	8.739	7.606	105.2E6	150.9E6	27.296	26.782

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ081724\
Data File : PQ068050.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Aug 2024 17:29
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 17 05:02:00 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ080524.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 09 02:37:44 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

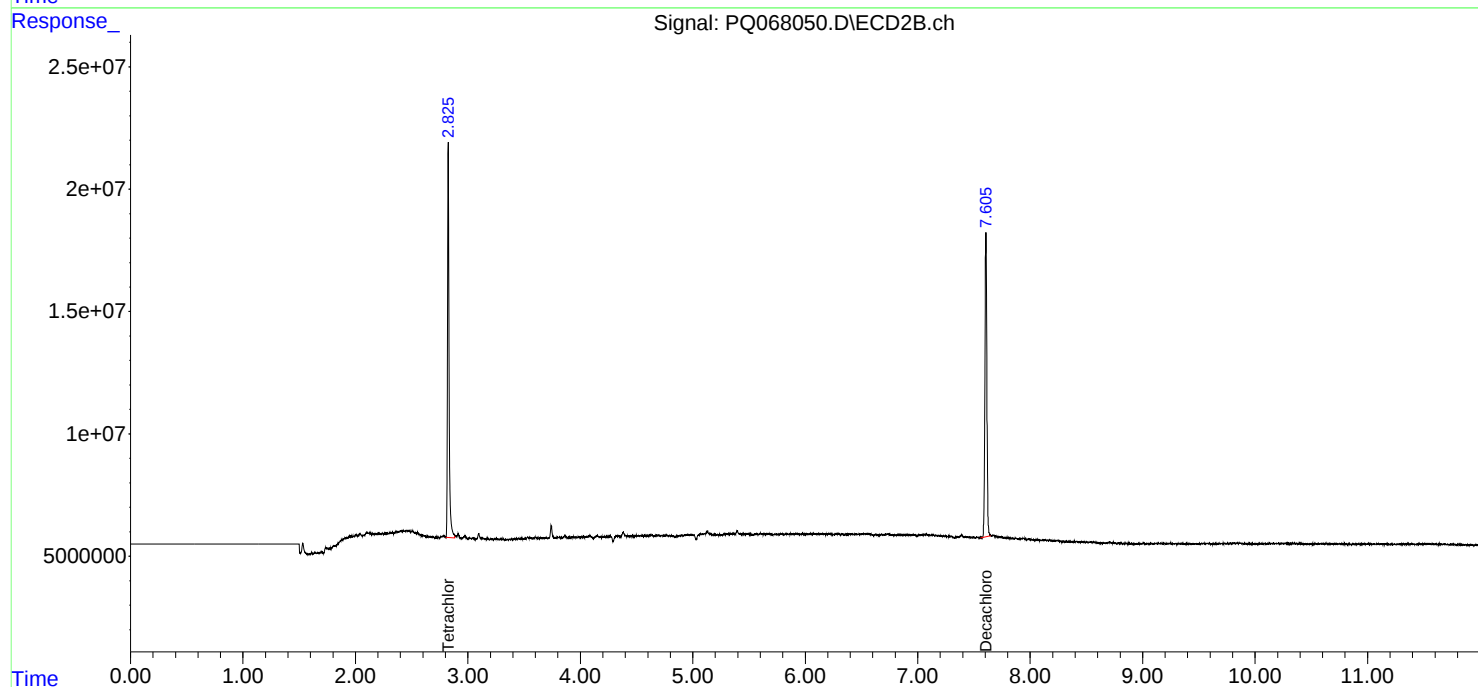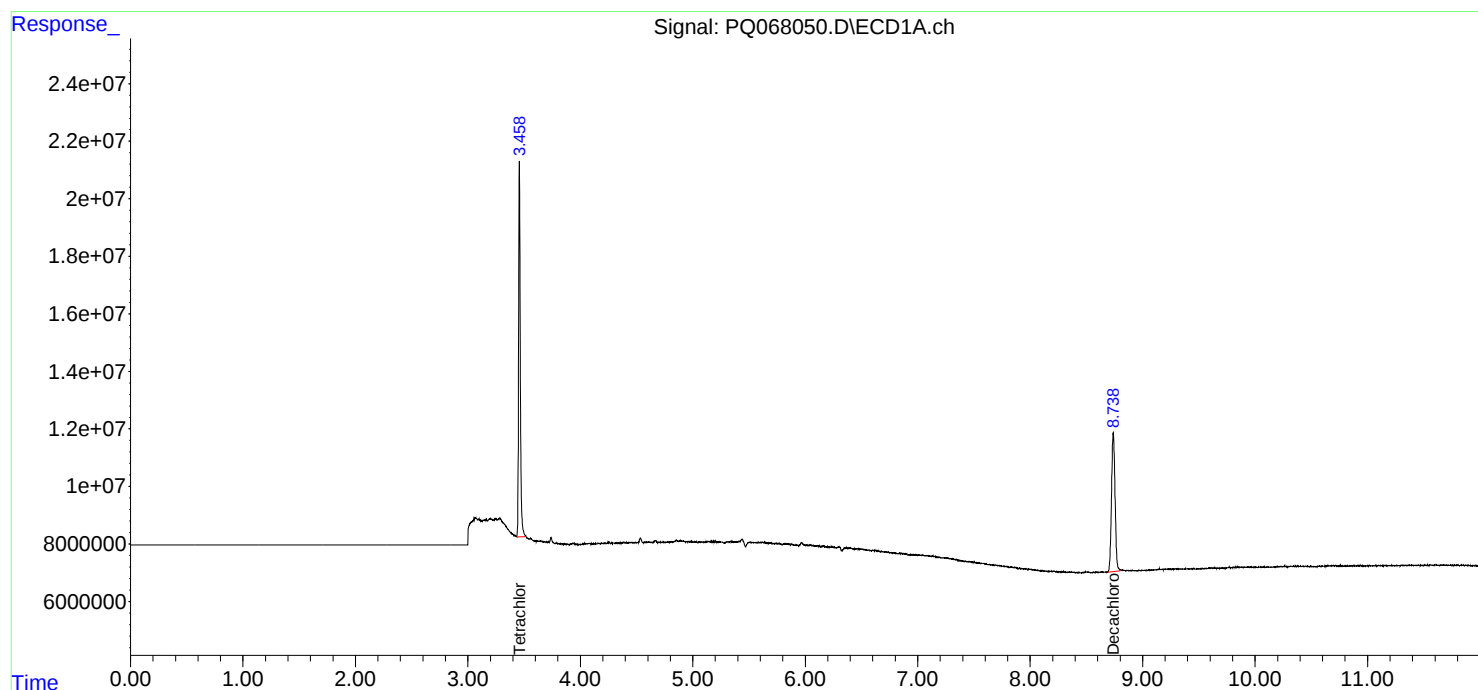


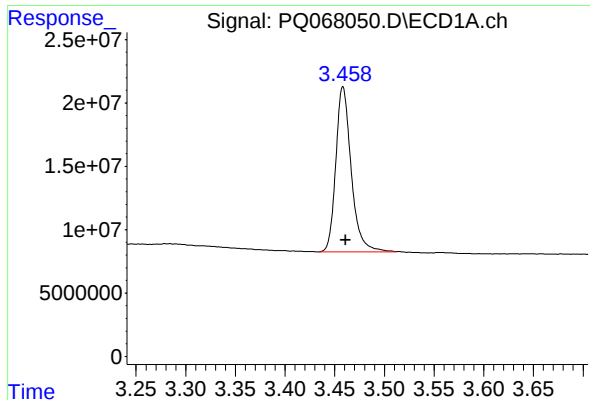

#1 Tetrachloro-m-xylene


R.T.: 3.458 min
Delta R.T.: -0.003 min
Response: 140887757
Conc: 23.75 ng/ml

Instrument :
ECD_Q
ClientSampleId :
I.BLK

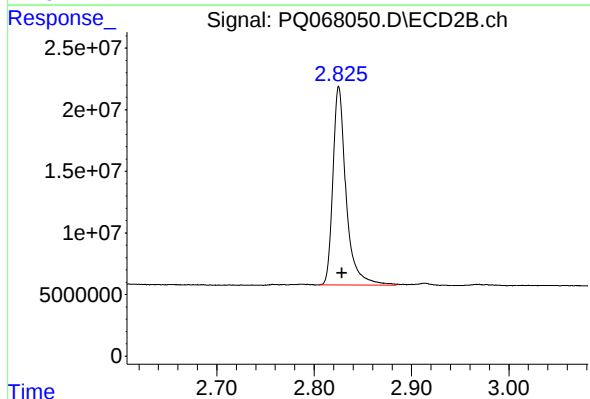


#1 Tetrachloro-m-xylene

R.T.: 2.825 min
Delta R.T.: -0.003 min
Response: 152530535
Conc: 24.05 ng/ml

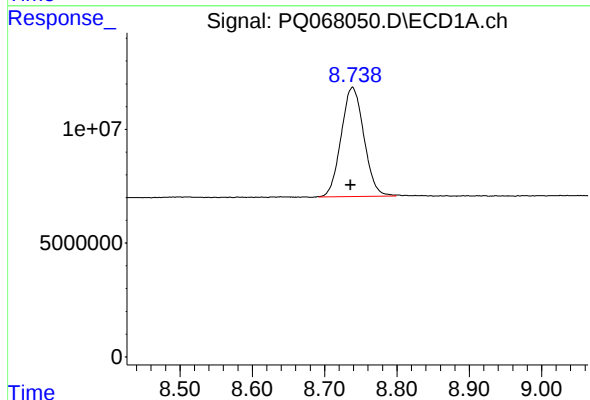

#2 Decachlorobiphenyl

R.T.: 8.739 min
Delta R.T.: 0.003 min
Response: 105173589
Conc: 27.30 ng/ml

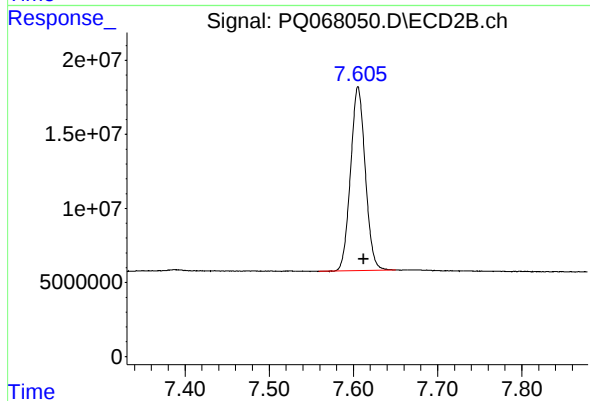

#2 Decachlorobiphenyl

R.T.: 7.606 min
Delta R.T.: -0.006 min
Response: 150943029
Conc: 26.78 ng/ml