

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ082820\
 Data File : PQ049593.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Aug 2020 00:27
 Operator : DD\AJ
 Sample : L3826-03
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 P-3-(0.0-0.5)

Manual Integrations
 APPROVED

Ankita
 8/31/2020 3:24:28 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 29 04:14:08 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ082820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 28 17:31:13 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.238	4.280	162.1E6	90622588	18.557	16.039
2) SA Decachlor...	11.456	9.635	97443841	57438727	10.005m	9.182m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ082820\
Data File : PQ049593.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Aug 2020 00:27
Operator : DD\AJ
Sample : L3826-03
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
P-3-(0.0-0.5)


Manual Integrations
APPROVED

Ankita
8/31/2020 3:24:28 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 29 04:14:08 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ082820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 28 17:31:13 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

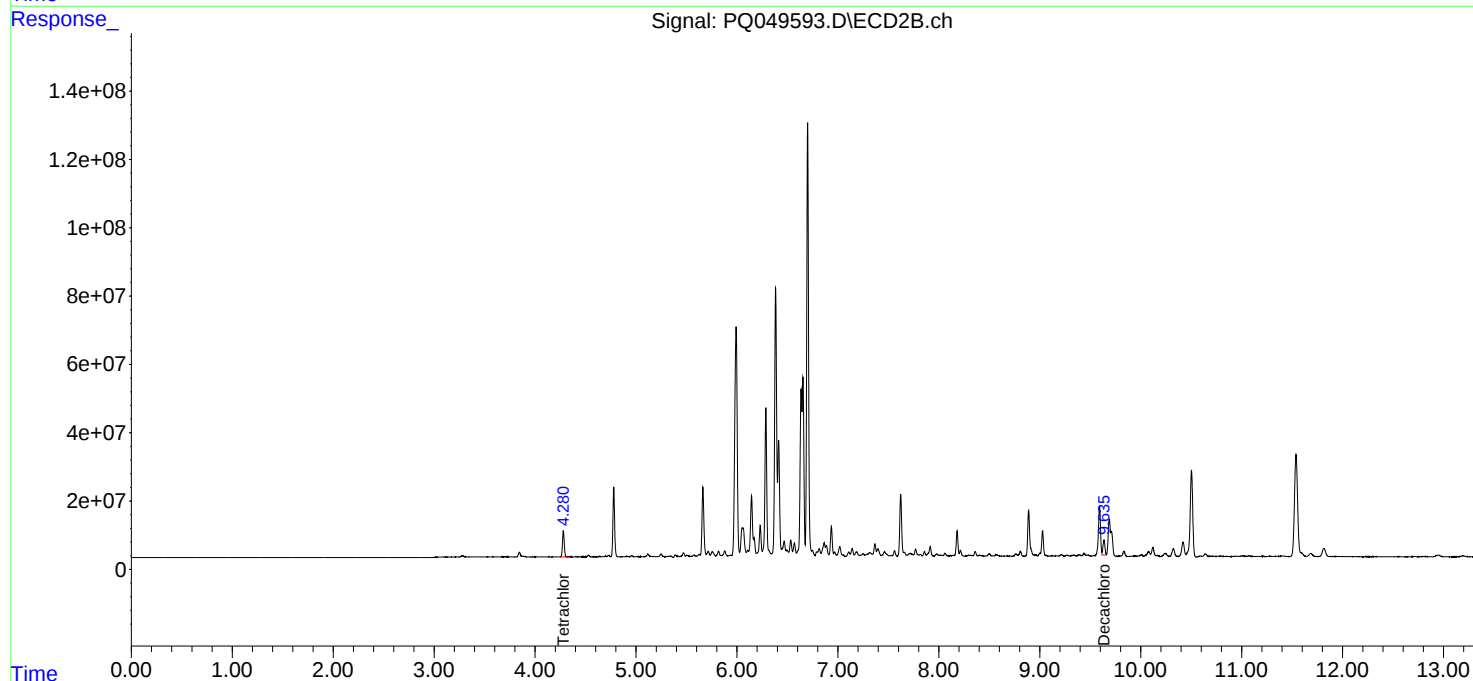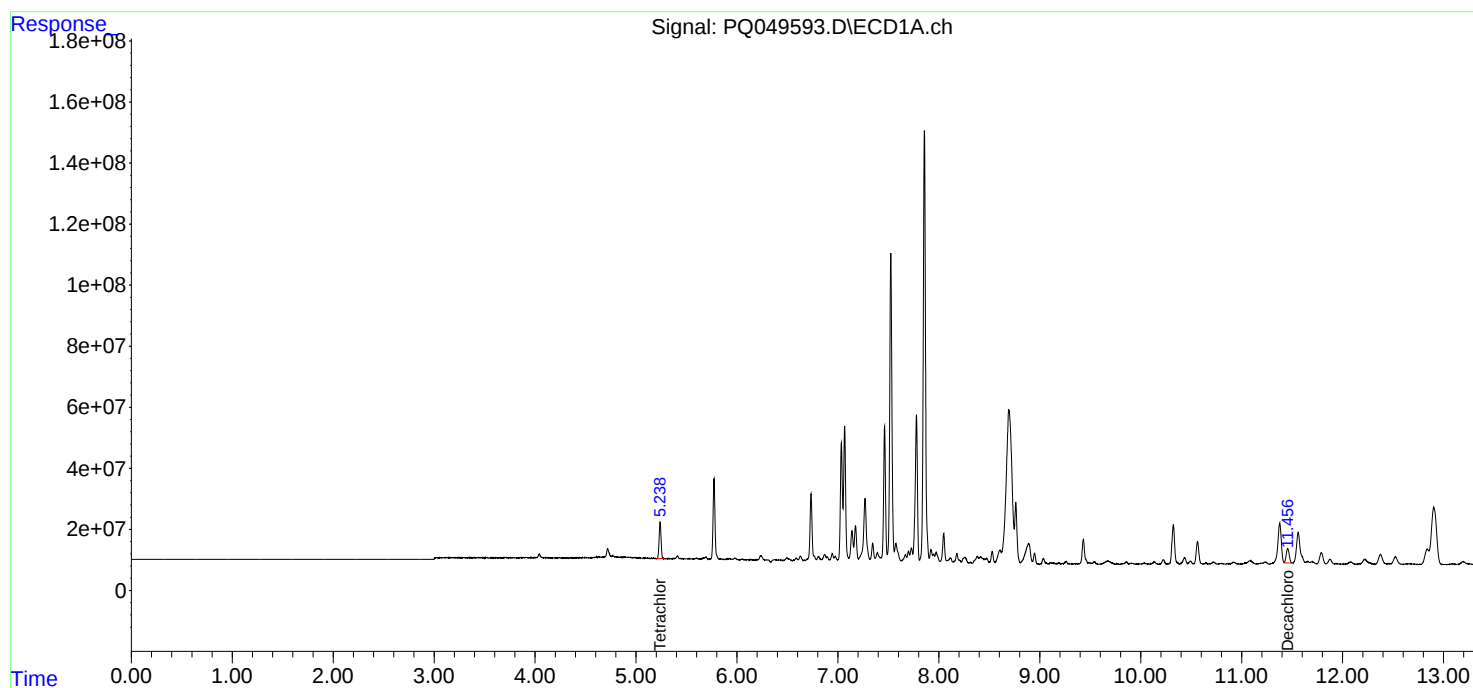

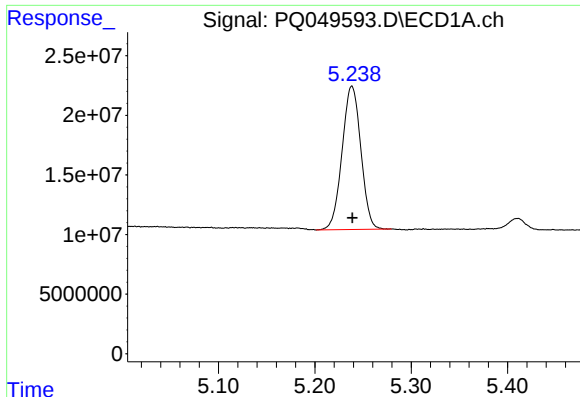


#1 Tetrachloro-m-xylene

R.T.: 5.238 min
Delta R.T.: 0.000 min
Response: 162051094
Conc: 18.56 ng/ml

Instrument :
ECD_Q
ClientSampleId :
P-3-(0.0-0.5)


Manual Integrations
APPROVED

Ankita
8/31/2020 3:24:28 PM

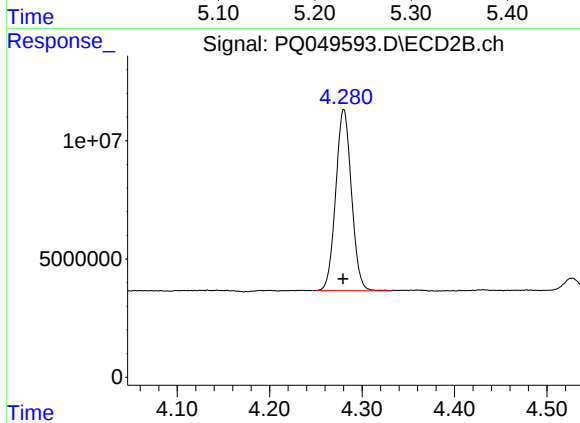


#1 Tetrachloro-m-xylene

R.T.: 4.280 min
Delta R.T.: 0.000 min
Response: 90622588
Conc: 16.04 ng/ml

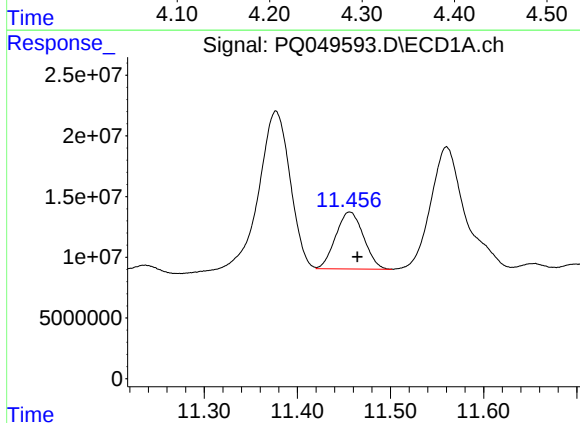

#2 Decachlorobiphenyl

R.T.: 11.456 min
Delta R.T.: -0.009 min
Response: 97443841
Conc: 10.00 ng/ml m

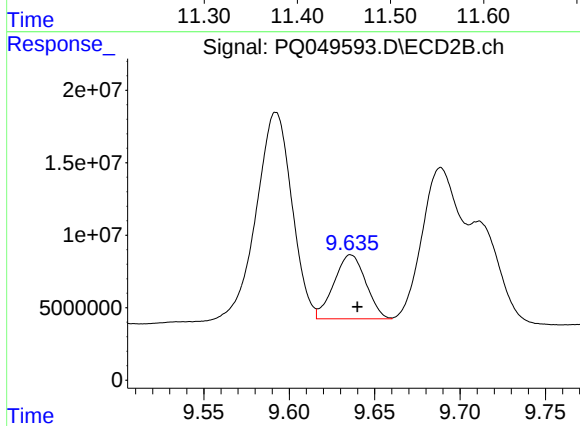

#2 Decachlorobiphenyl

R.T.: 9.635 min
Delta R.T.: -0.005 min
Response: 57438727
Conc: 9.18 ng/ml m