

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ090120\
 Data File : PQ049675.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Sep 2020 23:02
 Operator : DD\AJ
 Sample : L3848-23
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 LINDEN-BH-01-C

Manual Integrations
 APPROVED

Ankita
 9/2/2020 1:28:55 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 02 07:09:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ082820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 28 17:31:13 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.237	4.282	206.8E6	114.0E6	23.679	20.179
2) SA Decachlor...	11.452	9.634	172.9E6	90405298	17.750	14.452m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ090120\
Data File : PQ049675.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Sep 2020 23:02
Operator : DD\AJ
Sample : L3848-23
Misc :
ALS Vial : 37 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampled :
LINDEN-BH-01-C


Manual Integrations
APPROVED

Ankita
9/2/2020 1:28:55 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 02 07:09:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ082820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 28 17:31:13 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

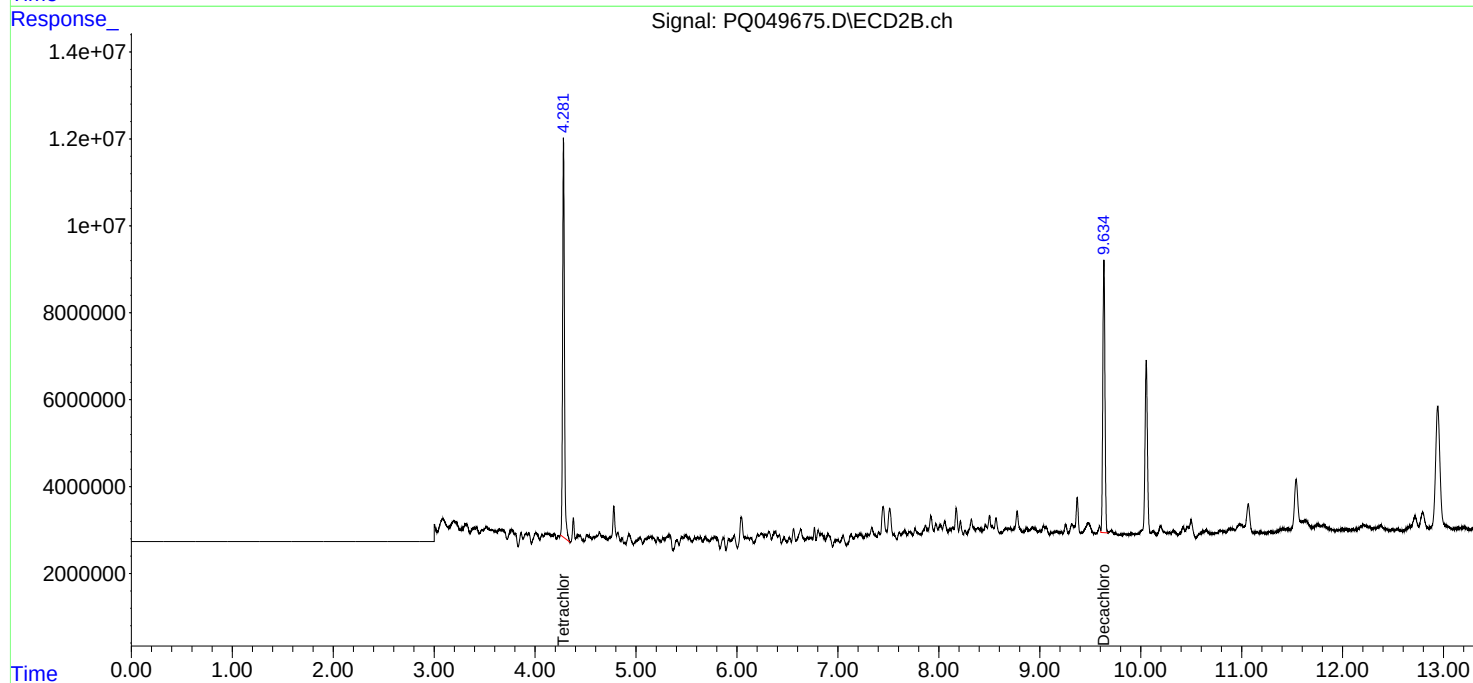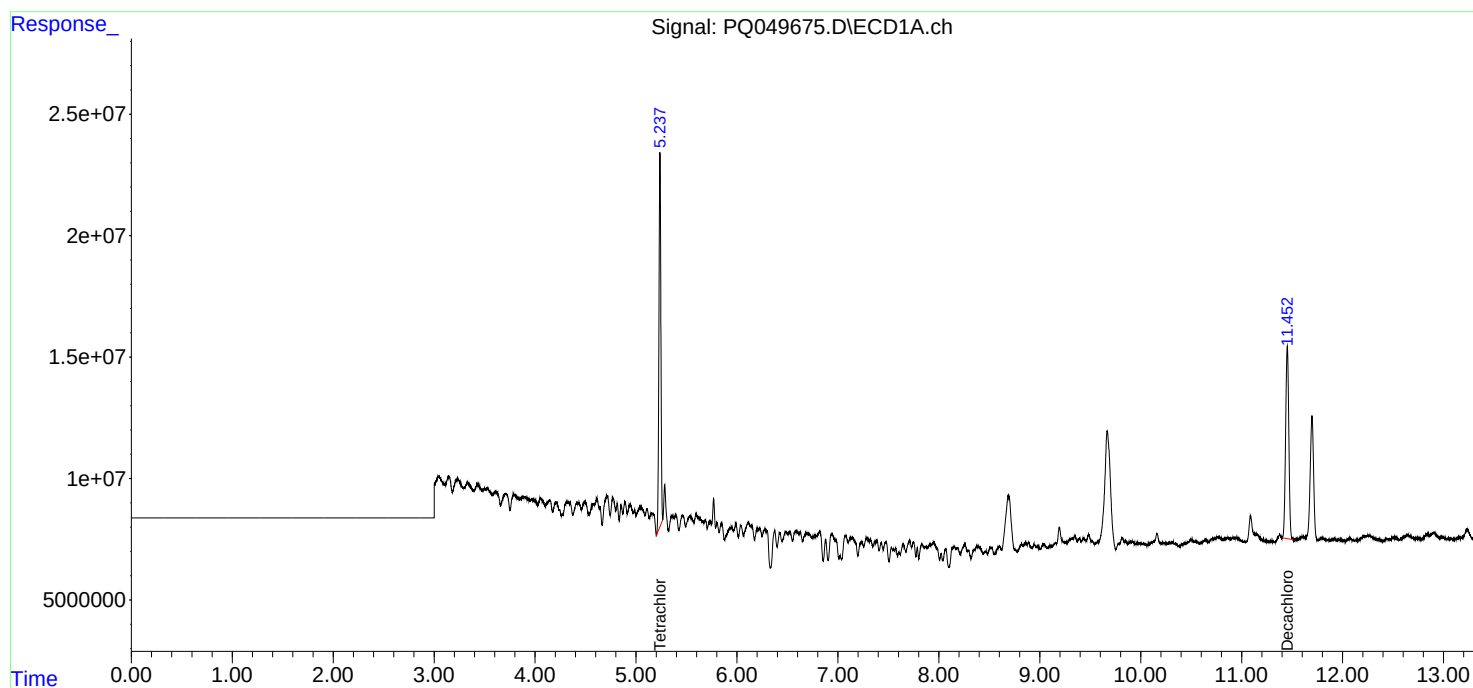

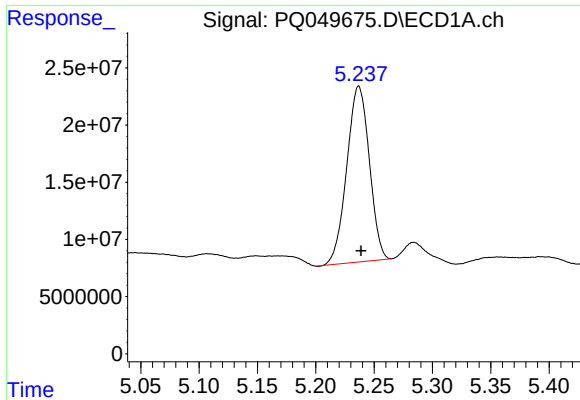


#1 Tetrachloro-m-xylene

R.T.: 5.237 min
Delta R.T.: -0.002 min
Response: 206779919
Conc: 23.68 ng/ml

Instrument :
ECD_Q
ClientSampleId :
LINDEN-BH-01-C


Manual Integrations
APPROVED

Ankita
9/2/2020 1:28:55 PM

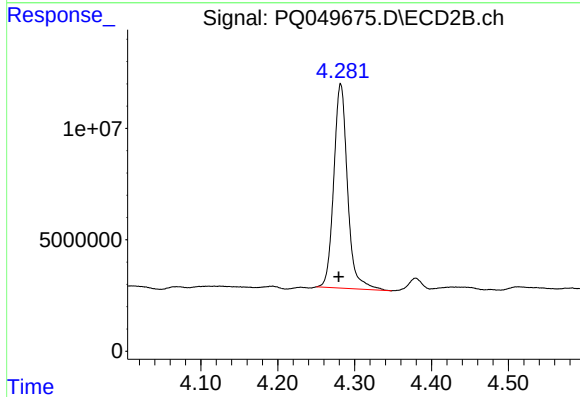


#1 Tetrachloro-m-xylene

R.T.: 4.282 min
Delta R.T.: 0.003 min
Response: 114012440
Conc: 20.18 ng/ml

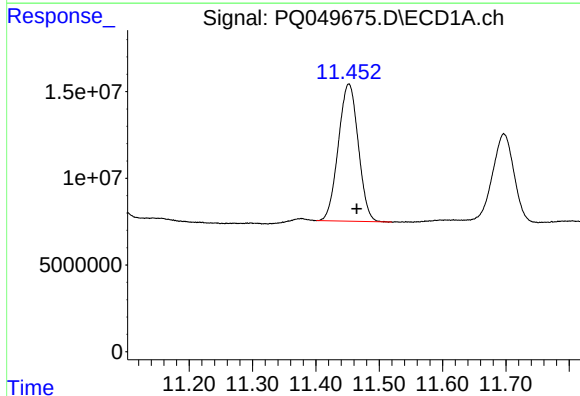

#2 Decachlorobiphenyl

R.T.: 11.452 min
Delta R.T.: -0.012 min
Response: 172883443
Conc: 17.75 ng/ml

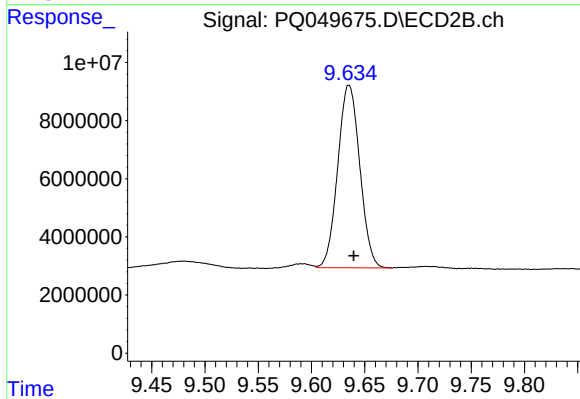

#2 Decachlorobiphenyl

R.T.: 9.634 min
Delta R.T.: -0.006 min
Response: 90405298
Conc: 14.45 ng/ml m