

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ090320\
 Data File : PQ049715.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Sep 2020 14:56
 Operator : DD\AJ
 Sample : L3895-09
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 SB-23A-(7-7.5)

Manual Integrations
 APPROVED

Ankita
 9/4/2020 2:42:27 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 04 01:48:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ082820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 28 17:31:13 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.234	4.280	198.4E6	96627981	22.715	17.102
2) SA Decachlor...	11.452	9.639	96475319	57925120	9.905m	9.260
Target Compounds						
31) L7 AR-1260-1	8.259	7.132	28681777	27633863	75.450	77.461
32) L7 AR-1260-2	8.525	7.329	33321823	33015891	68.918	65.676
33) L7 AR-1260-3	8.891	7.487	47456109	52865363	118.385	128.978
34) L7 AR-1260-4	9.137	7.969	39252764	72158886	87.625	197.932 #
35) L7 AR-1260-5	9.488	8.216	73272386	88390869	74.434m	89.004

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ090320\
Data File : PQ049715.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Sep 2020 14:56
Operator : DD\AJ
Sample : L3895-09
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
SB-23A-(7-7.5)


Manual Integrations
APPROVED

Ankita
9/4/2020 2:42:27 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 04 01:48:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ082820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 28 17:31:13 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

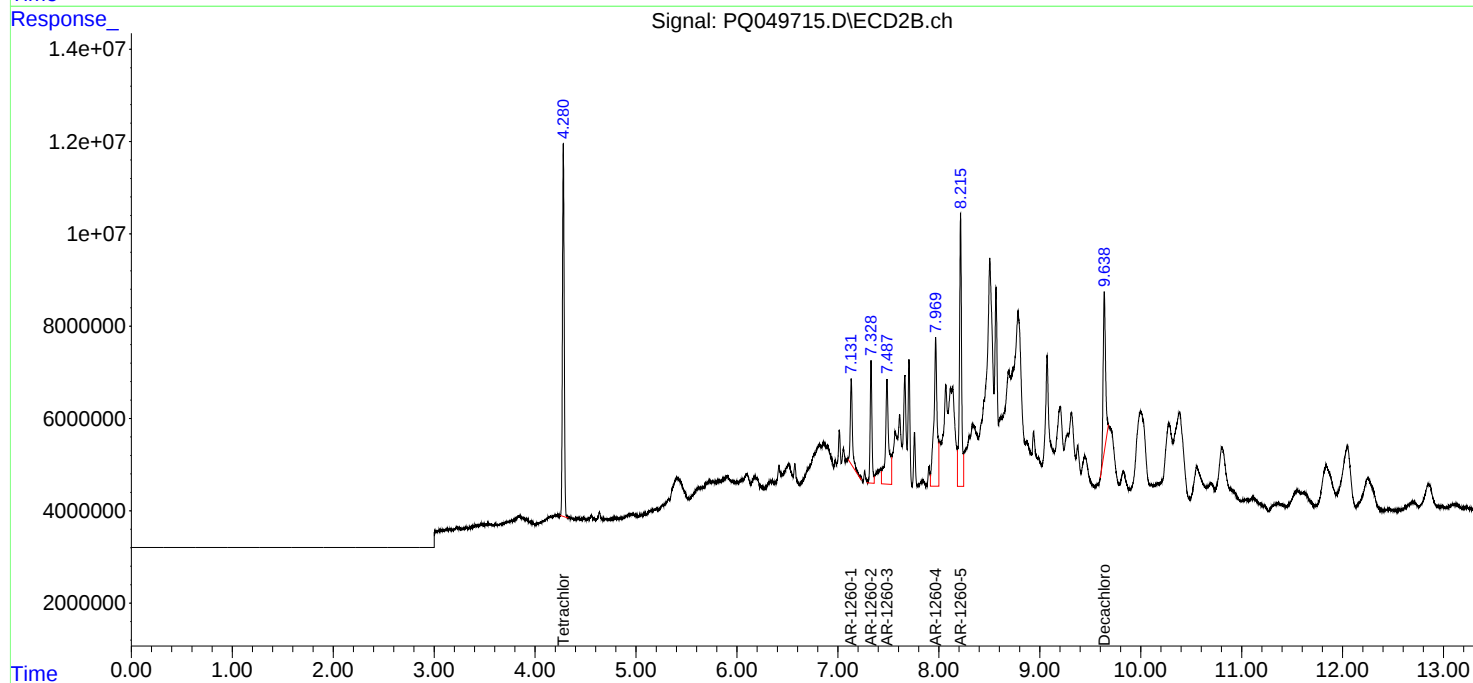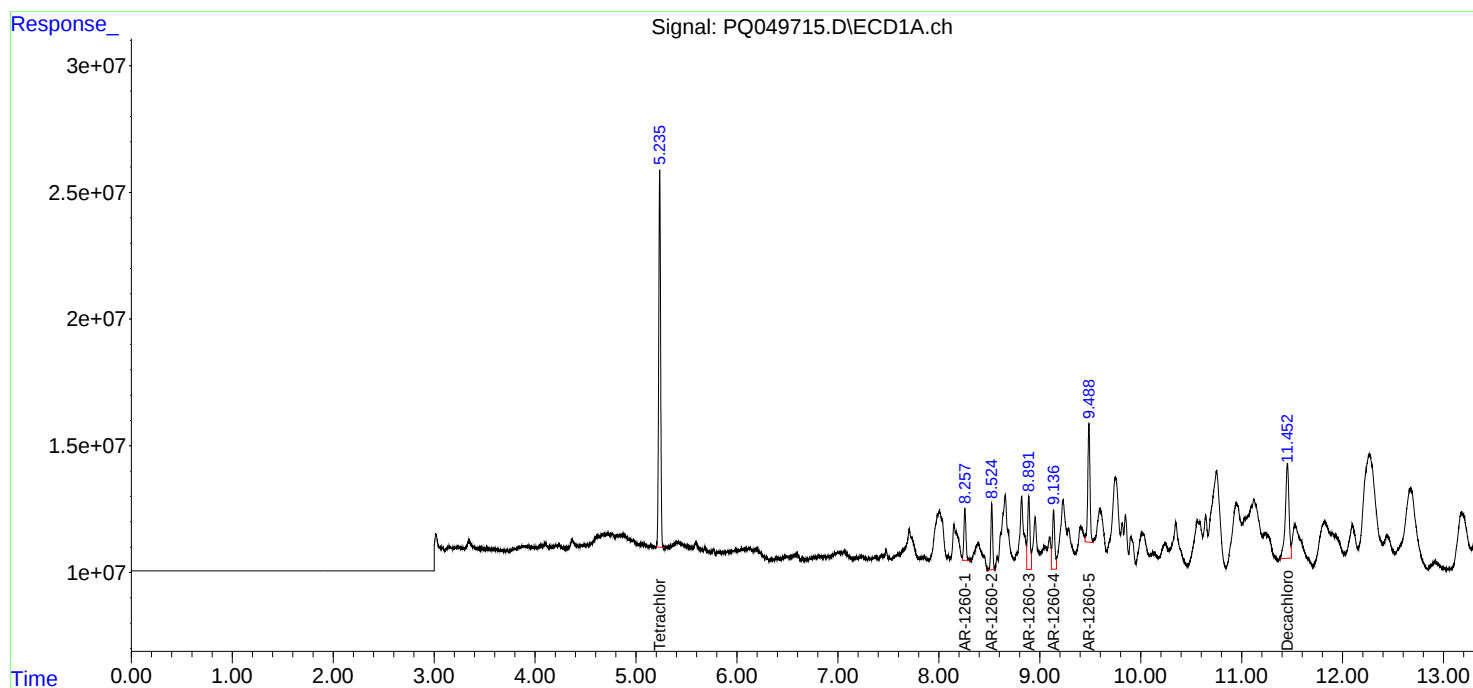

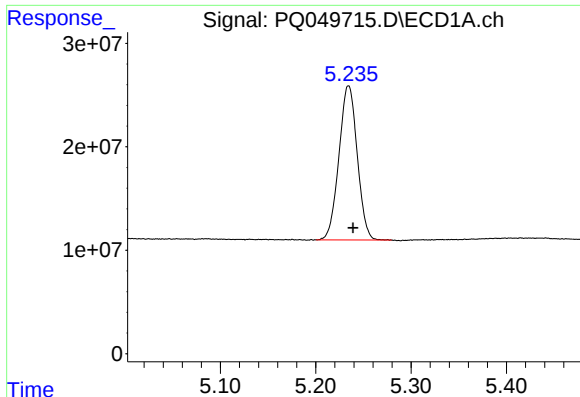


#1 Tetrachloro-m-xylene

R.T.: 5.234 min
Delta R.T.: -0.005 min
Response: 198354440
Conc: 22.71 ng/ml

Instrument :
ECD_Q
ClientSampleId :
SB-23A-(7-7.5)


Manual Integrations
APPROVED

Ankita
9/4/2020 2:42:27 PM

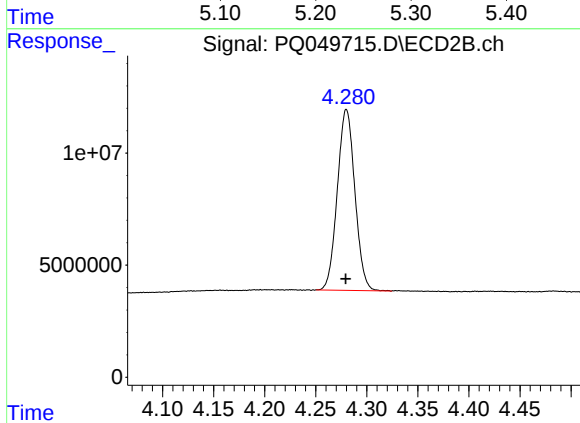


#1 Tetrachloro-m-xylene

R.T.: 4.280 min
Delta R.T.: 0.000 min
Response: 96627981
Conc: 17.10 ng/ml

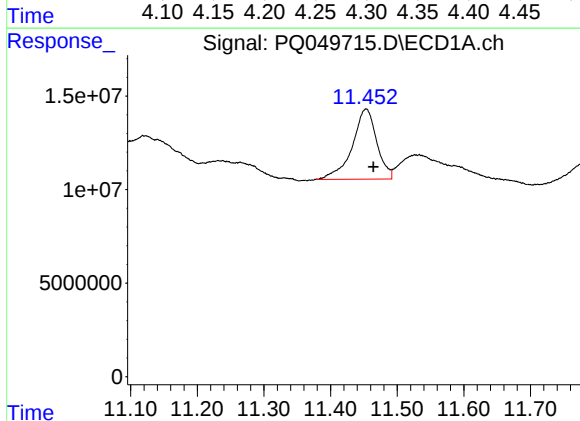


#2 Decachlorobiphenyl

R.T.: 11.452 min
Delta R.T.: -0.012 min
Response: 96475319
Conc: 9.91 ng/ml m

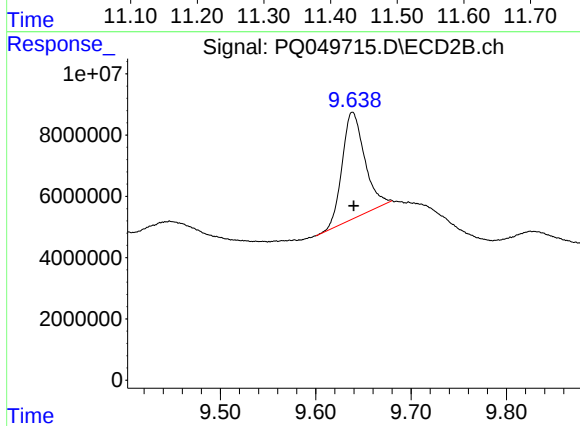

#2 Decachlorobiphenyl

R.T.: 9.639 min
Delta R.T.: -0.001 min
Response: 57925120
Conc: 9.26 ng/ml

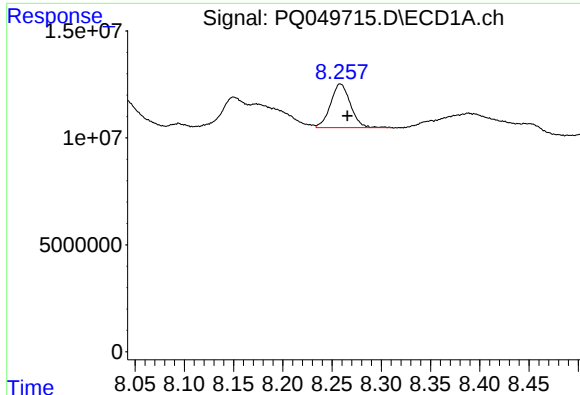


#31 AR-1260-1

R.T.: 8.259 min
Delta R.T.: -0.007 min
Response: 28681777
Conc: 75.45 ng/ml

Instrument :
ECD_Q
ClientSampleId :
SB-23A-(7-7.5)


Manual Integrations
APPROVED

Ankita
9/4/2020 2:42:27 PM

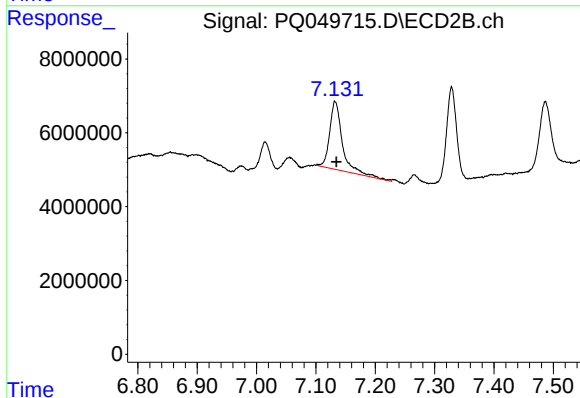


#31 AR-1260-1

R.T.: 7.132 min
Delta R.T.: -0.002 min
Response: 27633863
Conc: 77.46 ng/ml

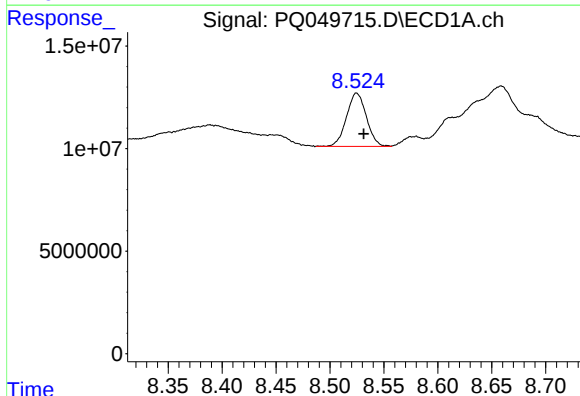


#32 AR-1260-2

R.T.: 8.525 min
Delta R.T.: -0.006 min
Response: 33321823
Conc: 68.92 ng/ml

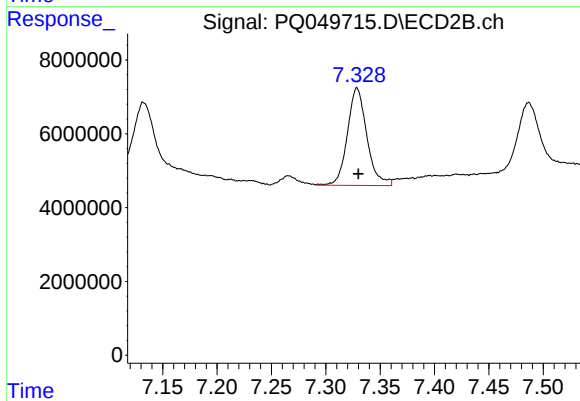

#32 AR-1260-2

R.T.: 7.329 min
Delta R.T.: -0.001 min
Response: 33015891
Conc: 65.68 ng/ml

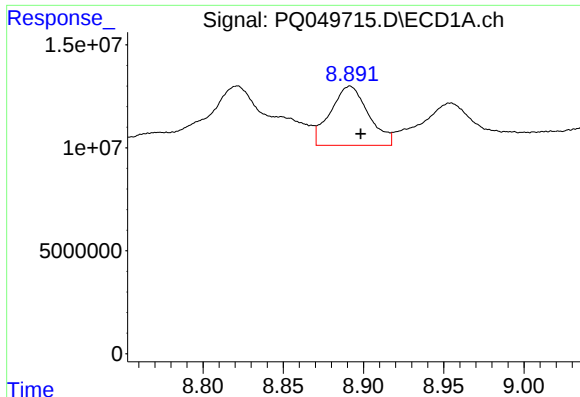


#33 AR-1260-3

R.T.: 8.891 min
Delta R.T.: -0.007 min
Response: 47456109
Conc: 118.39 ng/ml

Instrument :
ECD_Q
ClientSampleId :
SB-23A-(7-7.5)


Manual Integrations
APPROVED

Ankita
9/4/2020 2:42:27 PM

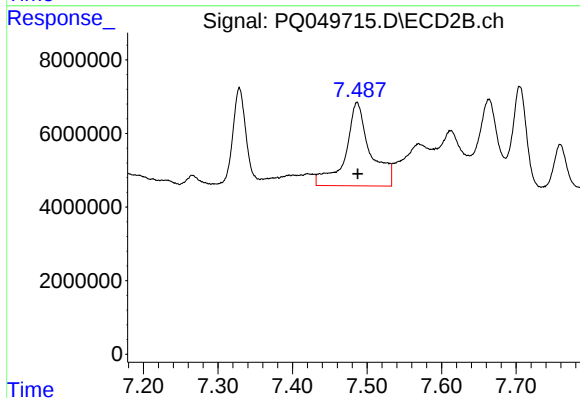


#33 AR-1260-3

R.T.: 7.487 min
Delta R.T.: 0.000 min
Response: 52865363
Conc: 128.98 ng/ml

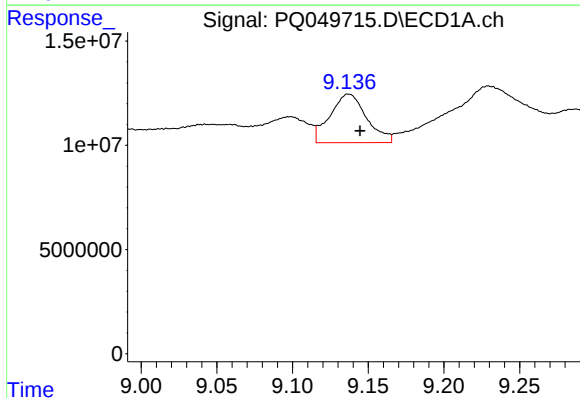


#34 AR-1260-4

R.T.: 9.137 min
Delta R.T.: -0.008 min
Response: 39252764
Conc: 87.63 ng/ml

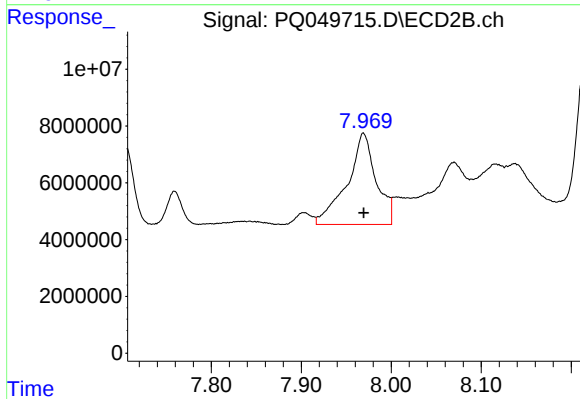

#34 AR-1260-4

R.T.: 7.969 min
Delta R.T.: 0.000 min
Response: 72158886
Conc: 197.93 ng/ml

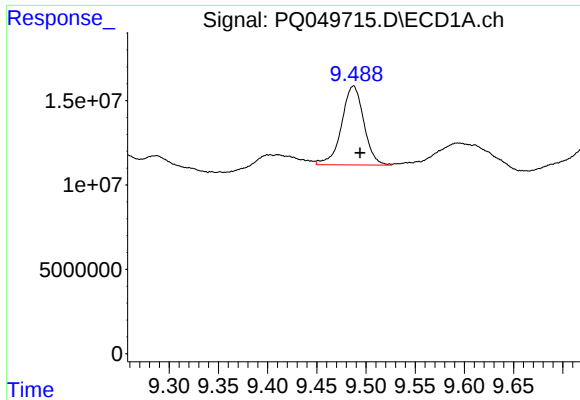


#35 AR-1260-5

R.T.: 9.488 min
Delta R.T.: -0.006 min
Response: 73272386
Conc: 74.43 ng/ml m

Instrument :
ECD_Q
ClientSampleId :
SB-23A-(7-7.5)

Manual Integrations
APPROVED

Ankita
9/4/2020 2:42:27 PM

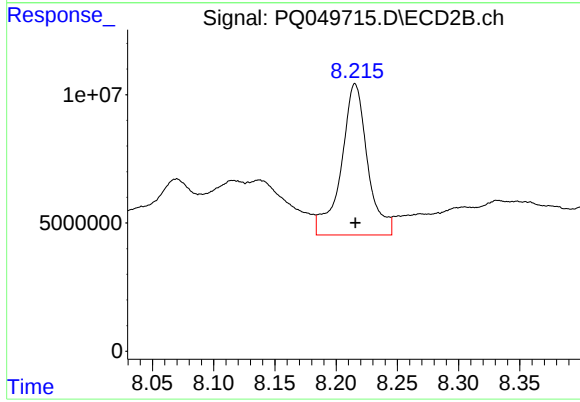

#35 AR-1260-5

R.T.: 8.216 min
Delta R.T.: 0.000 min
Response: 88390869
Conc: 89.00 ng/ml