

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ090924\
 Data File : PQ068480.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Sep 2024 04:55
 Operator : YP\AJ
 Sample : P3888-01
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 DN-B-36

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/10/2024
 Supervised By :Ankita Jodhani 09/10/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 07:13:16 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ090624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 07 07:27:42 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.438	2.821	151.0E6	137.7E6	21.146	19.330m
2) SA Decachlor...	8.610	7.598	76198256	139.5E6	17.484	21.122m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ090924\
Data File : PQ068480.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2024 04:55
Operator : YP\AJ
Sample : P3888-01
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
DN-B-36


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/10/2024
Supervised By :Ankita Jodhani 09/10/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 07:13:16 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ090624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 07 07:27:42 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

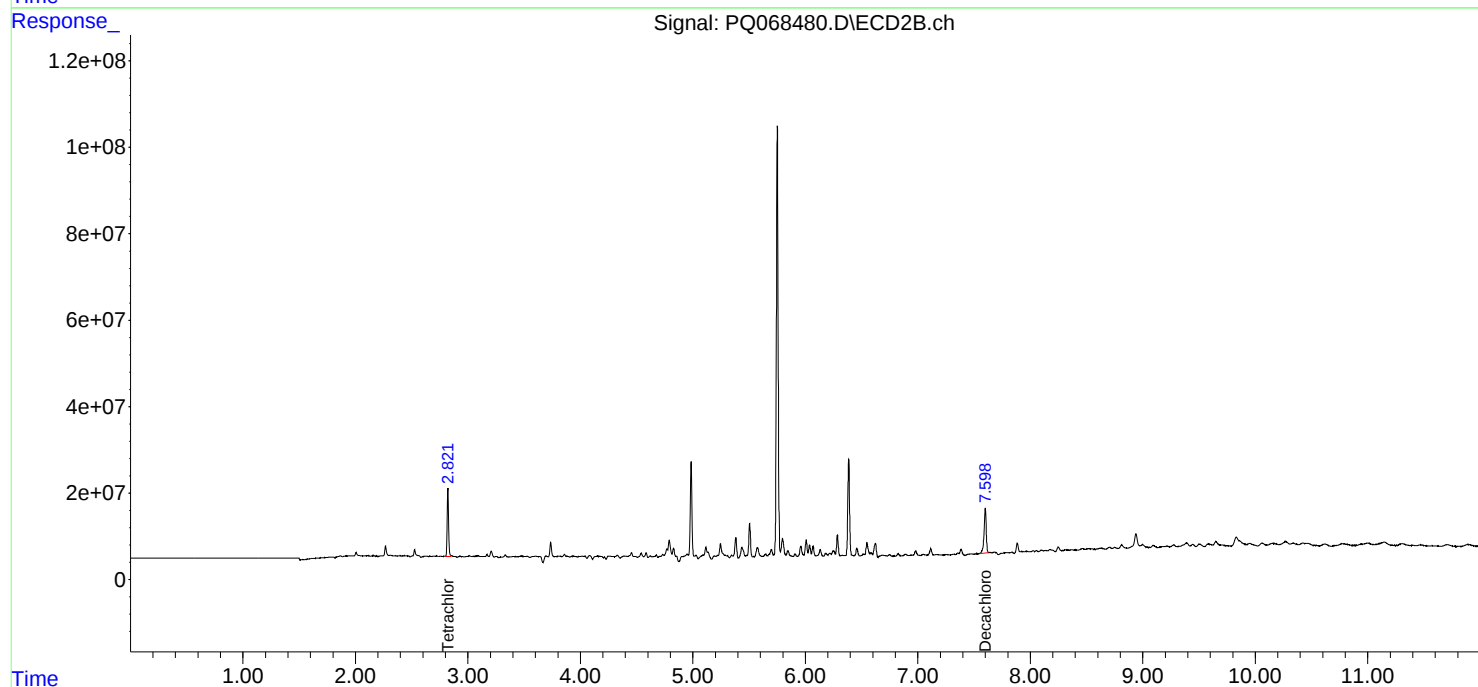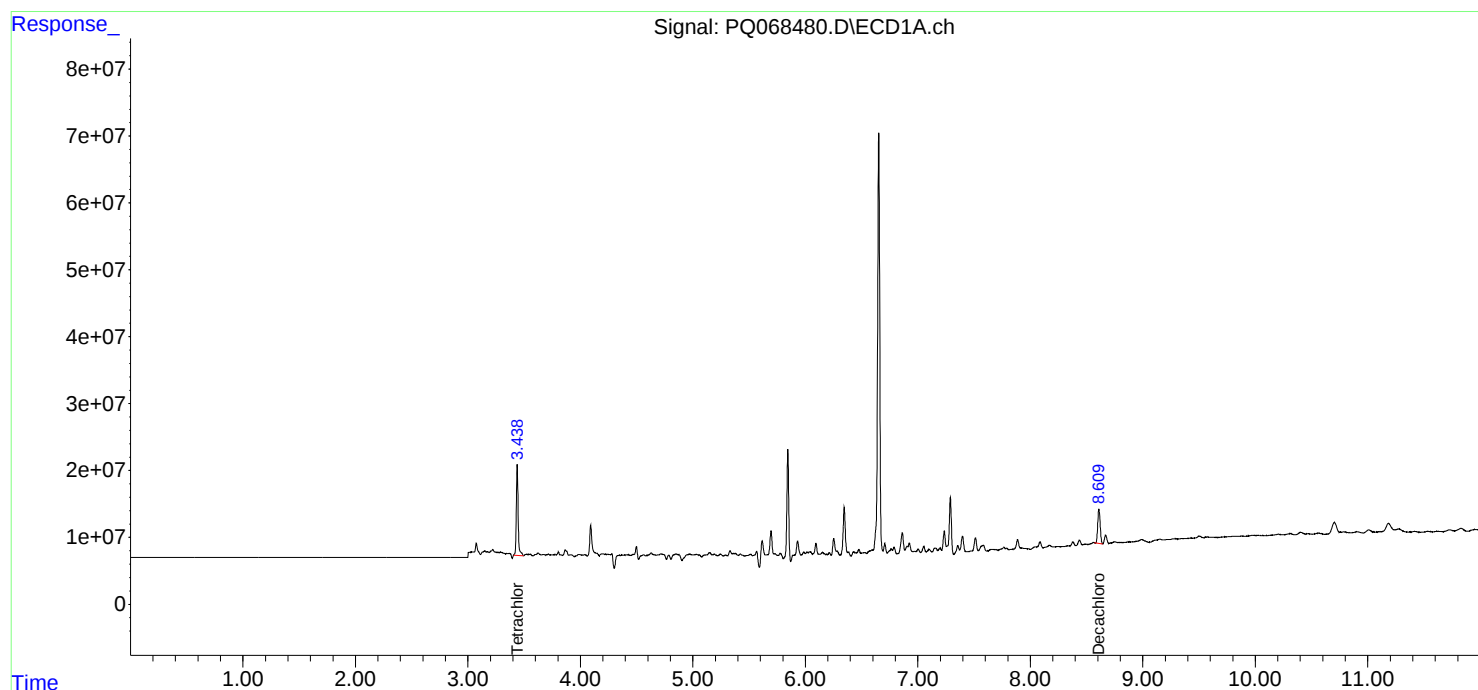

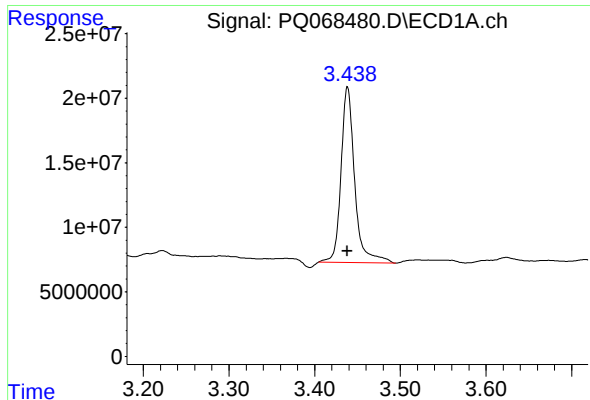


#1 Tetrachloro-m-xylene

R.T.: 3.438 min
Delta R.T.: 0.000 min
Response: 150996247
Conc: 21.15 ng/ml

Instrument :
ECD_Q
ClientSampleId :
DN-B-36


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/10/2024
Supervised By :Ankita Jodhani 09/10/2024

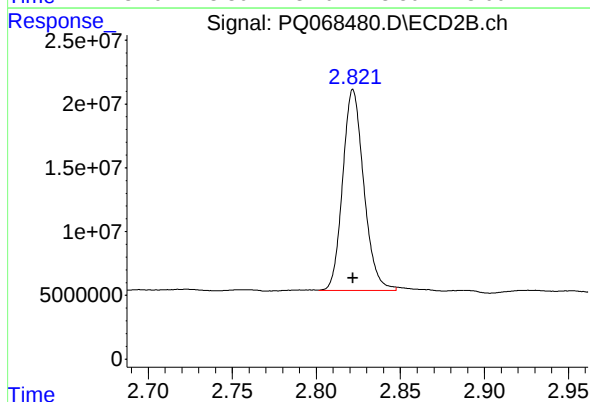


#1 Tetrachloro-m-xylene

R.T.: 2.821 min
Delta R.T.: 0.000 min
Response: 137672261
Conc: 19.33 ng/ml m

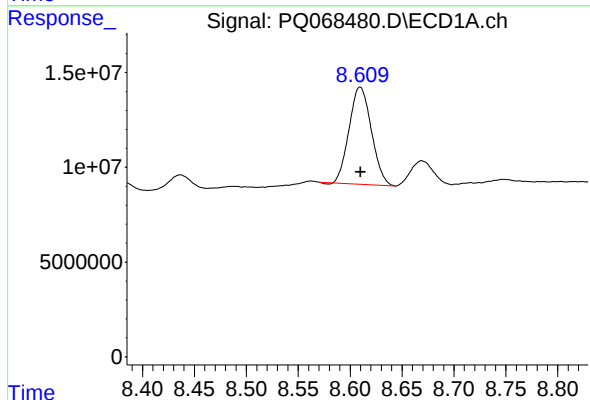

#2 Decachlorobiphenyl

R.T.: 8.610 min
Delta R.T.: 0.000 min
Response: 76198256
Conc: 17.48 ng/ml

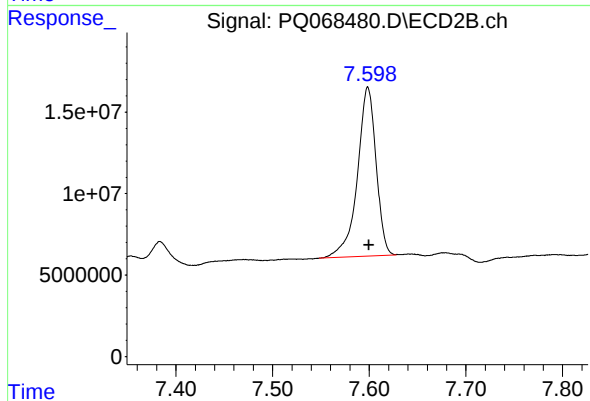

#2 Decachlorobiphenyl

R.T.: 7.598 min
Delta R.T.: -0.002 min
Response: 139487366
Conc: 21.12 ng/ml m