

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ091619\
 Data File : PQ043596.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Sep 2019 18:53
 Operator : SM\AJ
 Sample : K3591-09
 Misc : AR1221 MDL 25 PPB
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 MDL-MDL-WATER-03-QT3-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 04:49:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ091219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 13 03:48:31 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.702	4.787	20869663	8734317	8.239	8.489
2)	SA Decachlor...	12.095	10.560	105.3E6	41385263	12.717	11.004
Target Compounds							
3)	L1 AR-1016-1	7.146	0.000	230486	0	2.232	N.D. #
4)	L1 AR-1016-2	7.169	6.318	127291	232760	0.868	3.972 #
5)	L1 AR-1016-3	7.242	6.515	544137	654914	5.929	20.486 #
6)	L1 AR-1016-4	7.372	6.515	121100	654914	1.645	24.056 #
7)	L1 AR-1016-5	7.695	6.736	1038864	67223	13.439	1.904 #
8)	L2 AR-1221-1	5.953	5.097	1625996	89257	55.319	8.100 #
9)	L2 AR-1221-2	6.090	5.210	1165386	277853	53.249	32.106 #
10)	L2 AR-1221-3	6.183	5.316	1810723	1163313	26.007	40.513 #
11)	L3 AR-1232-1	6.183	5.316	1810723	1163313	18.454	28.533 #
12)	L3 AR-1232-2	6.811	6.318	1417842	232760	26.277	4.990 #
13)	L3 AR-1232-3	7.169	6.515	127291	654914	1.117	26.168 #
14)	L3 AR-1232-4	7.372	6.604	121100	989580	2.090	42.213 #
15)	L3 AR-1232-5	7.444	6.736	1436317	67223	35.482	2.620 #
16)	L4 AR-1242-1	7.146	0.000	230486	0	2.589	N.D. #
17)	L4 AR-1242-2	7.169	6.318	127291	232760	0.994	4.635 #
18)	L4 AR-1242-3	7.242	6.515	544137	654914	6.761	23.594 #
19)	L4 AR-1242-4	7.372	6.604	121100	989580	1.847	34.350 #
20)	L4 AR-1242-5	8.181	7.171	4387804	841754	48.353	20.034 #
21)	L5 AR-1248-1	7.146	0.000	230486	0	3.695	N.D. #
22)	L5 AR-1248-2	7.444	6.545	1436317	104401	15.763	2.871 #
23)	L5 AR-1248-3	7.695	6.560	1038864	151535	10.014	3.997 #
24)	L5 AR-1248-4	8.129	6.736	6184677	67223	45.523	1.454 #
25)	L5 AR-1248-5	8.181	7.246	4387804	1117551	33.096	21.644 #
26)	L6 AR-1254-1	8.129	7.171	6184677	841754	42.068	9.454 #
27)	L6 AR-1254-2	8.348	7.354	5358882	617529	21.892	7.595 #
28)	L6 AR-1254-3	8.738	7.809	4201489	1678652	14.570	11.887
29)	L6 AR-1254-4	9.092	8.016	8422238	1826590	36.076	18.732 #
30)	L6 AR-1254-5	9.453	8.523	431911	397752	1.624	2.867 #
31)	L7 AR-1260-1	8.930	7.902	4846764	517140	26.146	6.344 #
32)	L7 AR-1260-2	9.187	8.148	2306178	1060241	9.785	9.993
33)	L7 AR-1260-3	9.545	8.328	306704	2084676	1.608	21.761 #
34)	L7 AR-1260-4	9.840	8.841	2782840	681408	12.053	7.788 #
35)	L7 AR-1260-5	10.141	9.088	911498	600189	1.723	2.738 #
36)	L8 AR-1262-1	9.545	8.523	306704	397752	0.970	2.835 #
37)	L8 AR-1262-2	10.141	9.088	911498	600189	1.335	2.313 #
38)	L8 AR-1262-3	10.464	9.366	296927	513895	0.627	4.369 #
39)	L8 AR-1262-4	10.553	9.427	1454180	249433	4.035	1.051 #
40)	L8 AR-1262-5	0.000	9.991	0	758785	N.D.	5.191 #
41)	L9 AR-1268-1	10.464	9.366	296927	513895	0.370	1.584 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ091619\
 Data File : PQ043596.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Sep 2019 18:53
 Operator : SM\AJ
 Sample : K3591-09
 Misc : AR1221 MDL 25 PPB
 ALS Vial : 6 Sample Multiplier: 1


Instrument :
 ECD_Q
 ClientSampleId :
 MDL-MDL-WATER-03-QT3-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 04:49:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ091219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 13 03:48:31 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	10.587	9.427	757169	249433	0.982	0.797
43) L9	AR-1268-3	10.825	9.648	2760463	545818	4.187	1.931 #
44) L9	AR-1268-4	0.000	9.991	0	758785	N.D.	4.807 #
45) L9	AR-1268-5	11.732	10.276	732442	783310	0.275	0.643 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

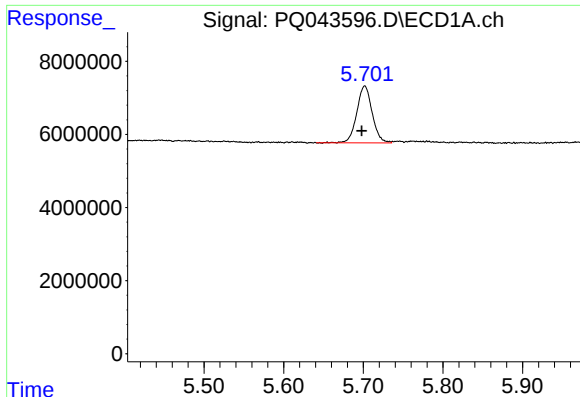

#1 Tetrachloro-m-xylene


R.T.: 5.702 min
Delta R.T.: 0.004 min
Response: 20869663
Conc: 8.24 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

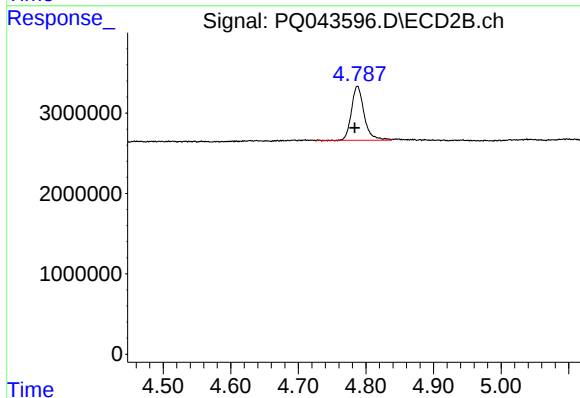


#1 Tetrachloro-m-xylene

R.T.: 4.787 min
Delta R.T.: 0.004 min
Response: 8734317
Conc: 8.49 ng/ml

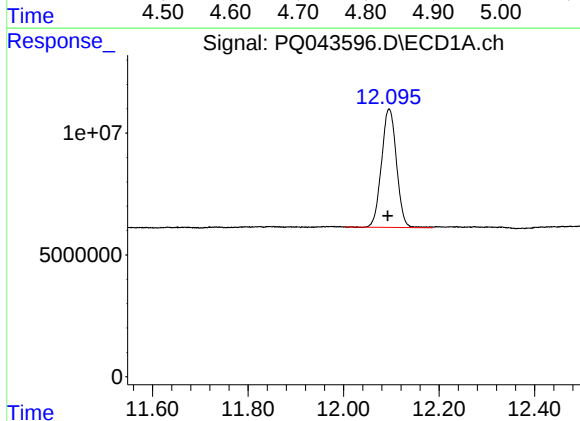


#2 Decachlorobiphenyl

R.T.: 12.095 min
Delta R.T.: 0.003 min
Response: 105290854
Conc: 12.72 ng/ml

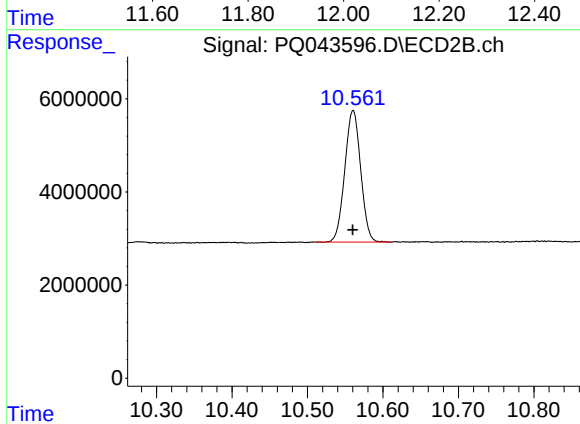

#2 Decachlorobiphenyl


R.T.: 10.560 min
Delta R.T.: 0.000 min
Response: 41385263
Conc: 11.00 ng/ml

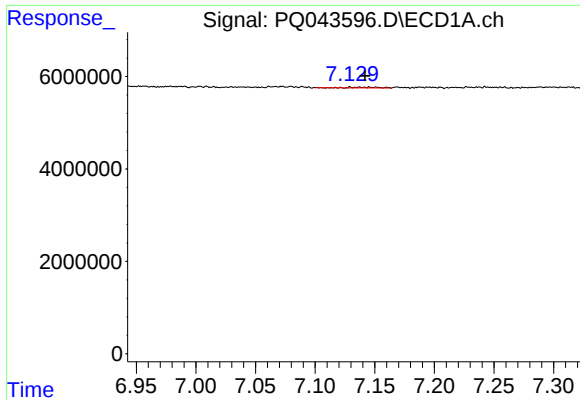

#3 AR-1016-1


R.T.: 7.146 min
Delta R.T.: 0.004 min
Response: 230486
Conc: 2.23 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

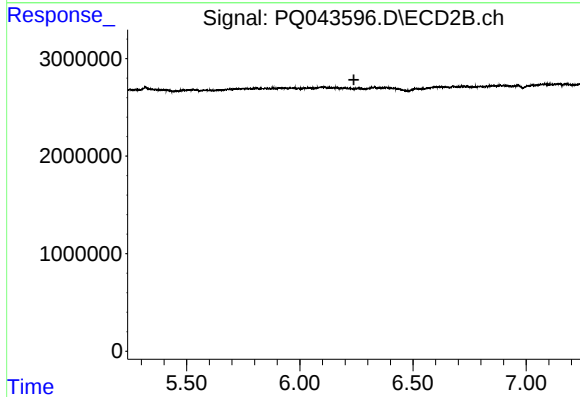


#3 AR-1016-1

R.T.: 0.000 min
Exp R.T. : 6.239 min
Response: 0
Conc: N.D.

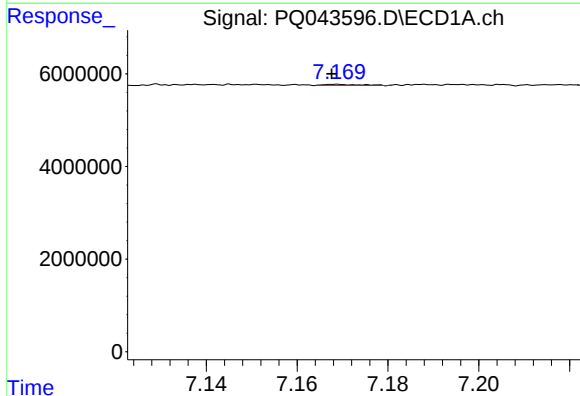


#4 AR-1016-2

R.T.: 7.169 min
Delta R.T.: 0.002 min
Response: 127291
Conc: 0.87 ng/ml

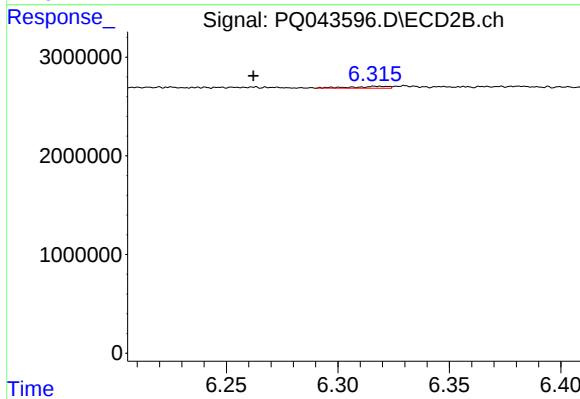

#4 AR-1016-2


R.T.: 6.318 min
Delta R.T.: 0.056 min
Response: 232760
Conc: 3.97 ng/ml

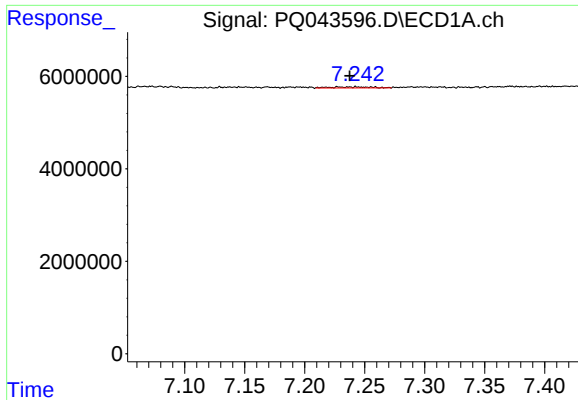

#5 AR-1016-3


R.T.: 7.242 min
Delta R.T.: 0.005 min
Response: 544137
Conc: 5.93 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

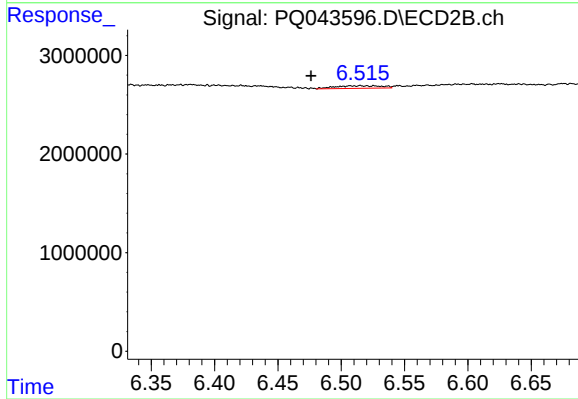


#5 AR-1016-3

R.T.: 6.515 min
Delta R.T.: 0.039 min
Response: 654914
Conc: 20.49 ng/ml

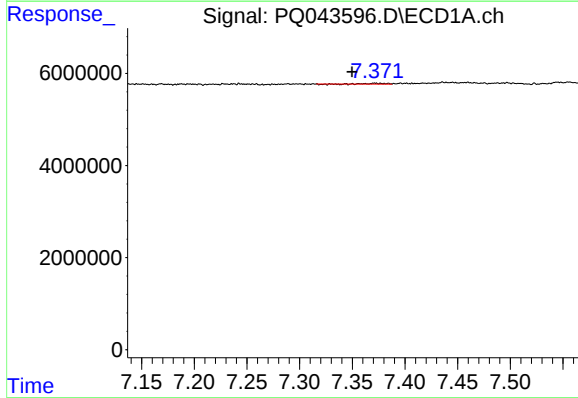


#6 AR-1016-4

R.T.: 7.372 min
Delta R.T.: 0.022 min
Response: 121100
Conc: 1.65 ng/ml

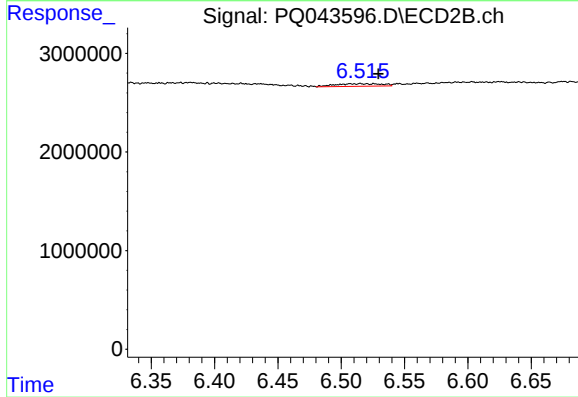

#6 AR-1016-4


R.T.: 6.515 min
Delta R.T.: -0.014 min
Response: 654914
Conc: 24.06 ng/ml

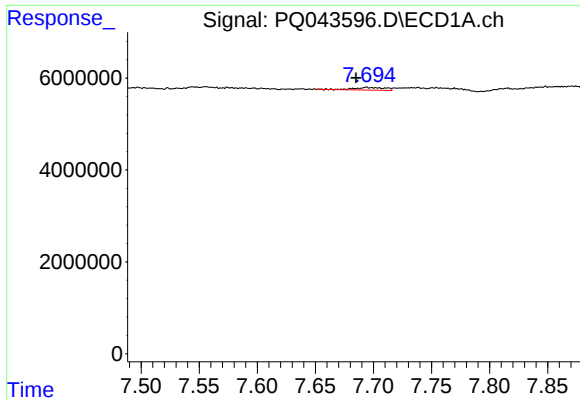

#7 AR-1016-5


R.T.: 7.695 min
Delta R.T.: 0.010 min
Response: 1038864
Conc: 13.44 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

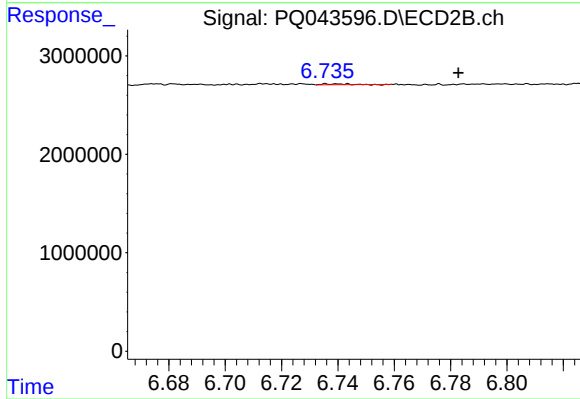


#7 AR-1016-5

R.T.: 6.736 min
Delta R.T.: -0.046 min
Response: 67223
Conc: 1.90 ng/ml

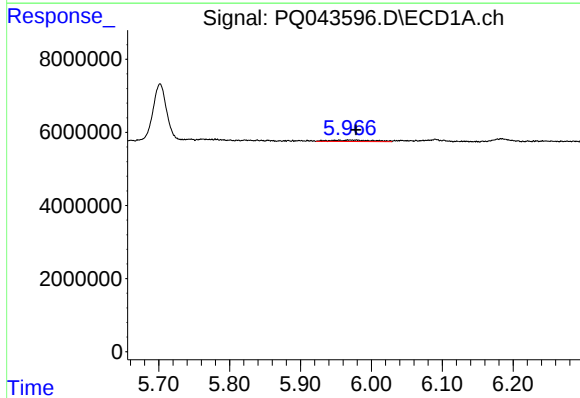


#8 AR-1221-1

R.T.: 5.953 min
Delta R.T.: -0.025 min
Response: 1625996
Conc: 55.32 ng/ml

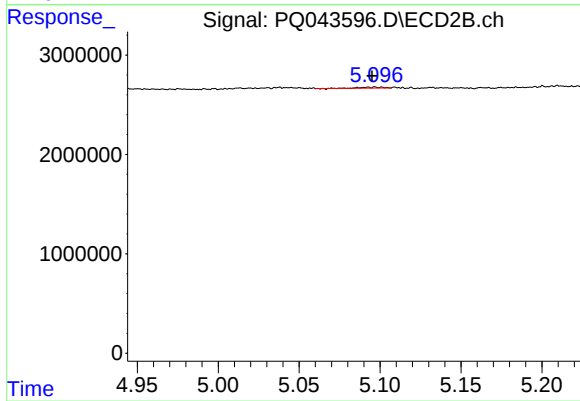

#8 AR-1221-1


R.T.: 5.097 min
Delta R.T.: 0.002 min
Response: 89257
Conc: 8.10 ng/ml

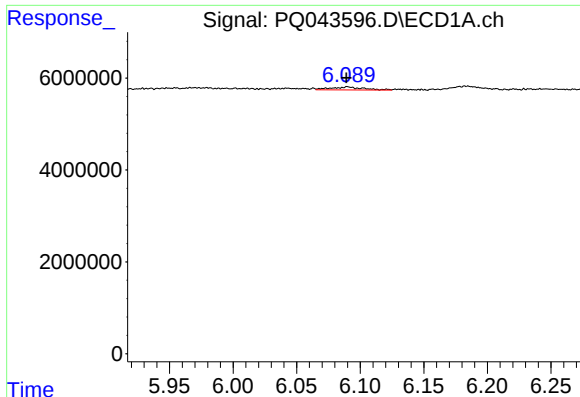

#9 AR-1221-2


R.T.: 6.090 min
Delta R.T.: 0.000 min
Response: 1165386
Conc: 53.25 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

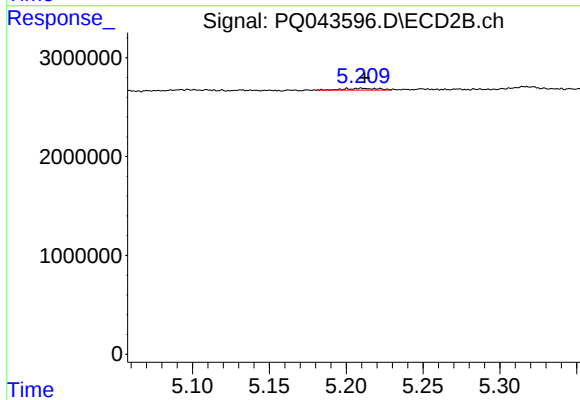


#9 AR-1221-2

R.T.: 5.210 min
Delta R.T.: -0.002 min
Response: 277853
Conc: 32.11 ng/ml

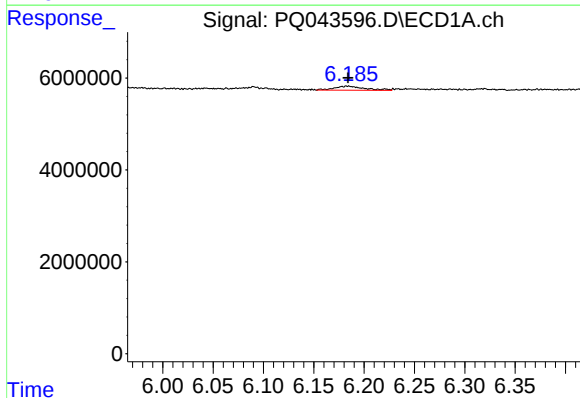


#10 AR-1221-3

R.T.: 6.183 min
Delta R.T.: -0.001 min
Response: 1810723
Conc: 26.01 ng/ml

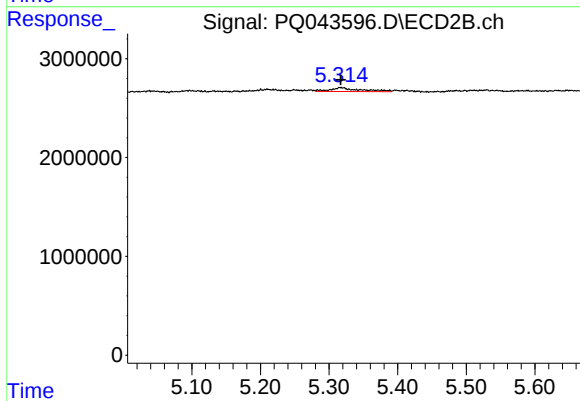

#10 AR-1221-3


R.T.: 5.316 min
Delta R.T.: 0.000 min
Response: 1163313
Conc: 40.51 ng/ml

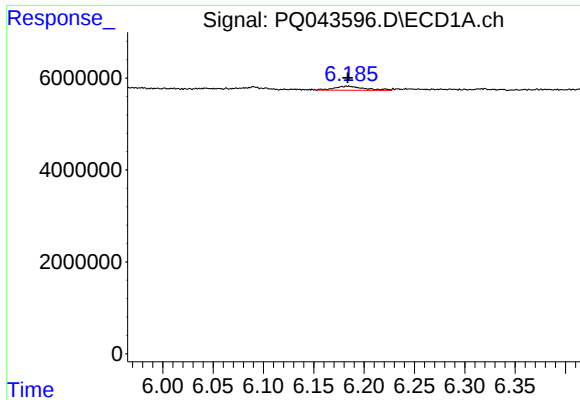

#11 AR-1232-1


R.T.: 6.183 min
Delta R.T.: 0.000 min
Response: 1810723
Conc: 18.45 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

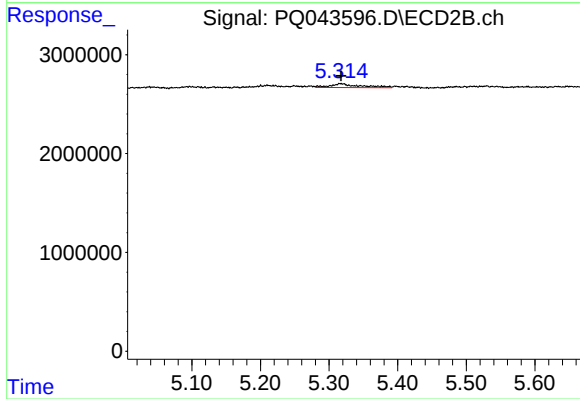


#11 AR-1232-1

R.T.: 5.316 min
Delta R.T.: -0.001 min
Response: 1163313
Conc: 28.53 ng/ml

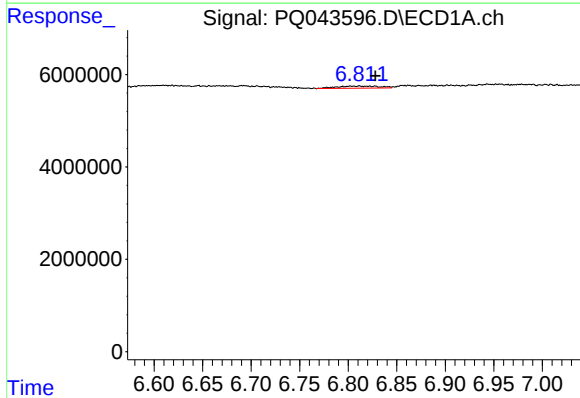


#12 AR-1232-2

R.T.: 6.811 min
Delta R.T.: -0.017 min
Response: 1417842
Conc: 26.28 ng/ml

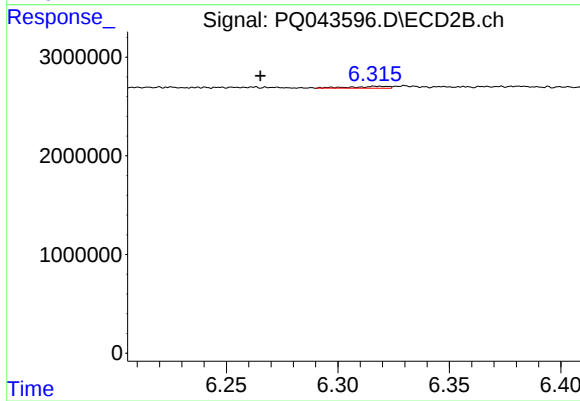

#12 AR-1232-2


R.T.: 6.318 min
Delta R.T.: 0.052 min
Response: 232760
Conc: 4.99 ng/ml

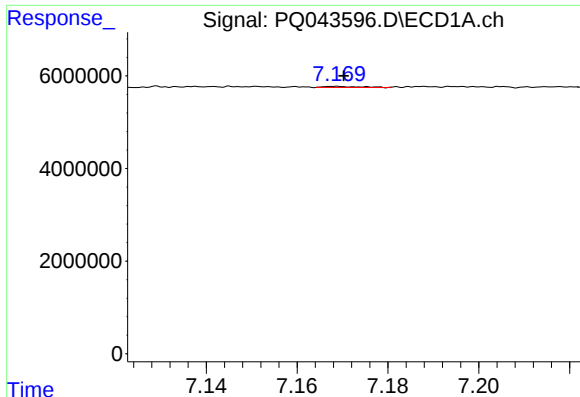

#13 AR-1232-3


R.T.: 7.169 min
Delta R.T.: 0.000 min
Response: 127291
Conc: 1.12 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

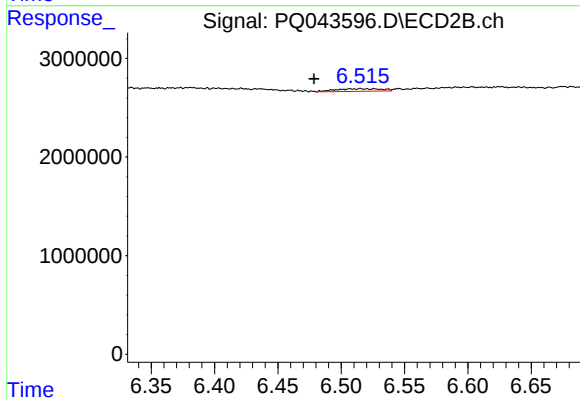


#13 AR-1232-3

R.T.: 6.515 min
Delta R.T.: 0.037 min
Response: 654914
Conc: 26.17 ng/ml

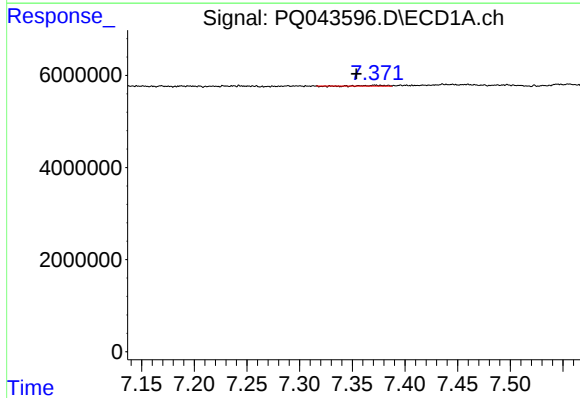


#14 AR-1232-4

R.T.: 7.372 min
Delta R.T.: 0.019 min
Response: 121100
Conc: 2.09 ng/ml

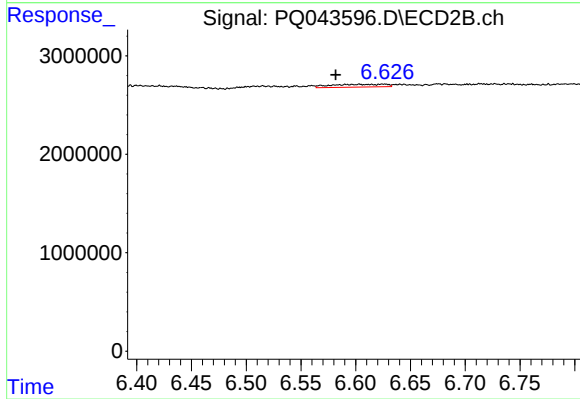

#14 AR-1232-4


R.T.: 6.604 min
Delta R.T.: 0.022 min
Response: 989580
Conc: 42.21 ng/ml

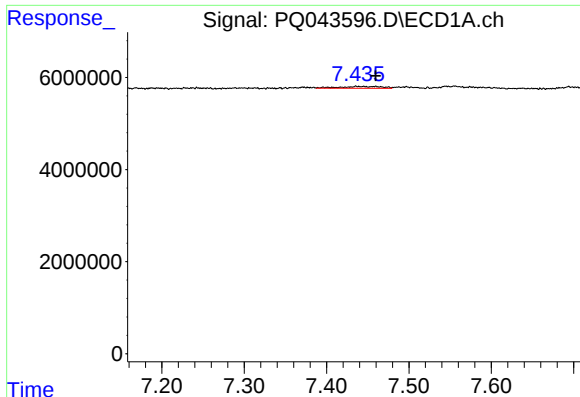

#15 AR-1232-5


R.T.: 7.444 min
Delta R.T.: -0.016 min
Response: 1436317
Conc: 35.48 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

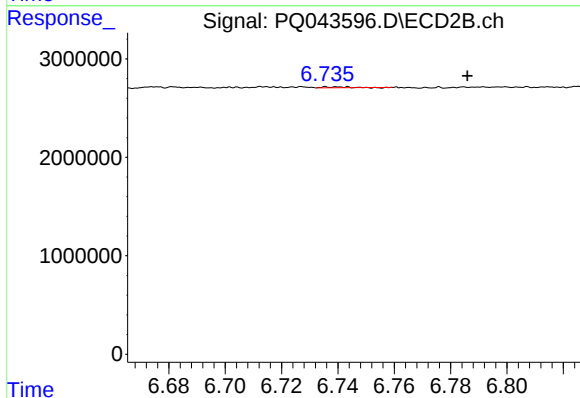


#15 AR-1232-5

R.T.: 6.736 min
Delta R.T.: -0.050 min
Response: 67223
Conc: 2.62 ng/ml

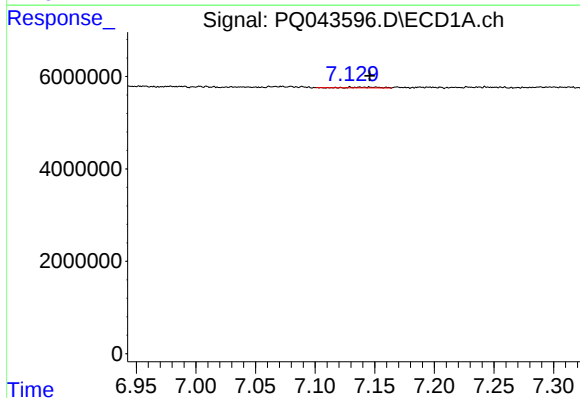


#16 AR-1242-1

R.T.: 7.146 min
Delta R.T.: 0.000 min
Response: 230486
Conc: 2.59 ng/ml

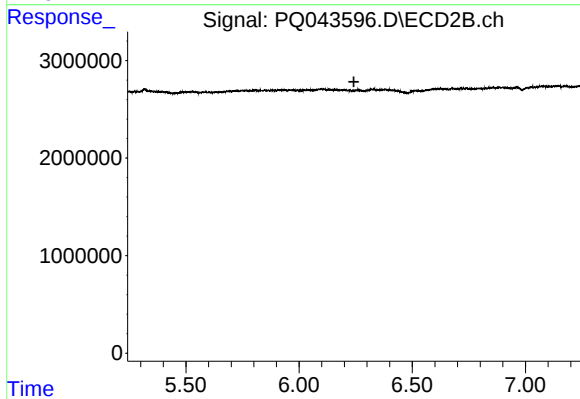

#16 AR-1242-1


R.T.: 0.000 min
Exp R.T.: 6.242 min
Response: 0
Conc: N.D.

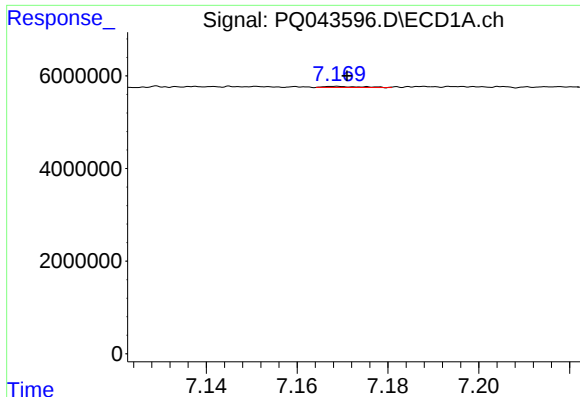

#17 AR-1242-2


R.T.: 7.169 min
Delta R.T.: -0.002 min
Response: 127291
Conc: 0.99 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

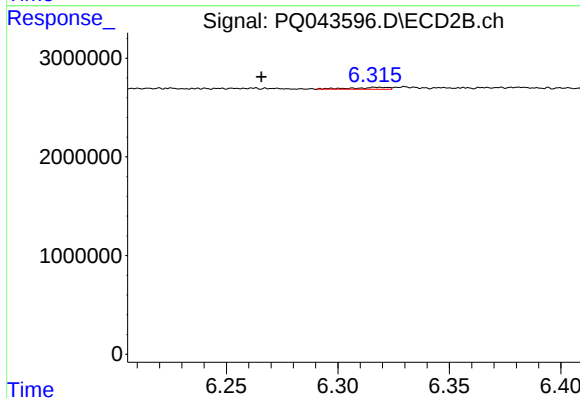


#17 AR-1242-2

R.T.: 6.318 min
Delta R.T.: 0.052 min
Response: 232760
Conc: 4.63 ng/ml

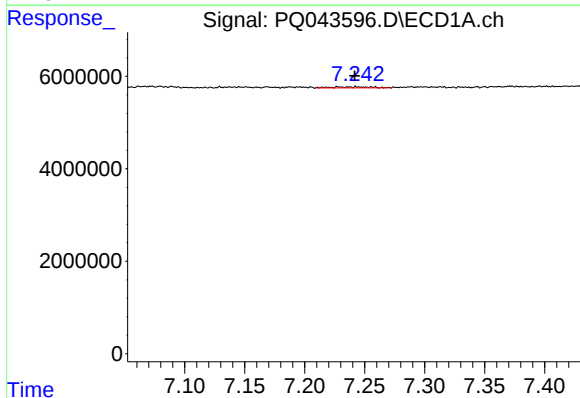


#18 AR-1242-3

R.T.: 7.242 min
Delta R.T.: 0.000 min
Response: 544137
Conc: 6.76 ng/ml

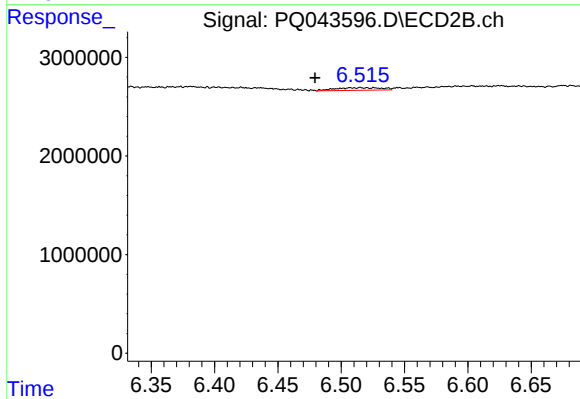

#18 AR-1242-3


R.T.: 6.515 min
Delta R.T.: 0.036 min
Response: 654914
Conc: 23.59 ng/ml

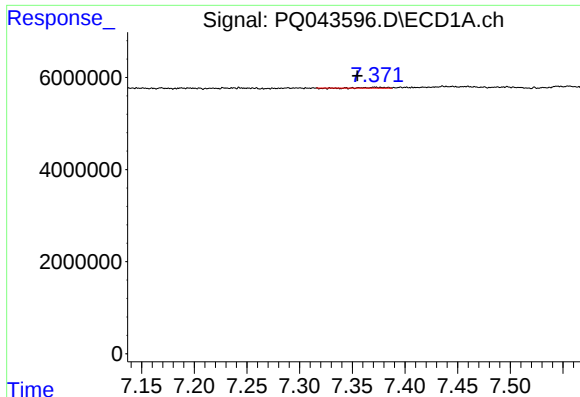

#19 AR-1242-4


R.T.: 7.372 min
Delta R.T.: 0.018 min
Response: 121100
Conc: 1.85 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

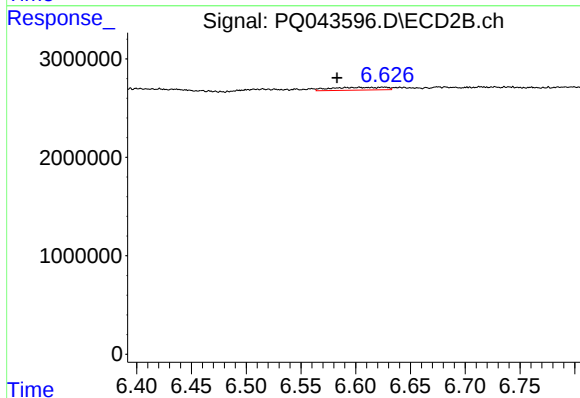


#19 AR-1242-4

R.T.: 6.604 min
Delta R.T.: 0.020 min
Response: 989580
Conc: 34.35 ng/ml

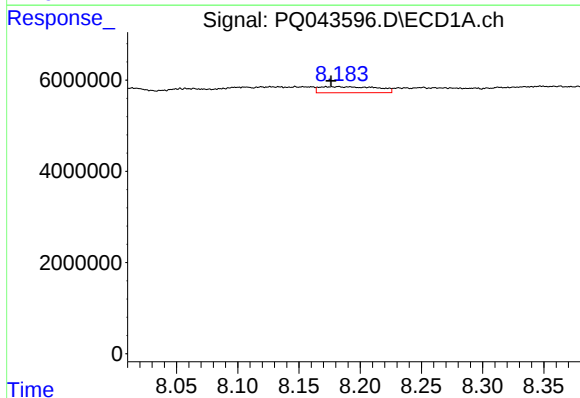


#20 AR-1242-5

R.T.: 8.181 min
Delta R.T.: 0.005 min
Response: 4387804
Conc: 48.35 ng/ml

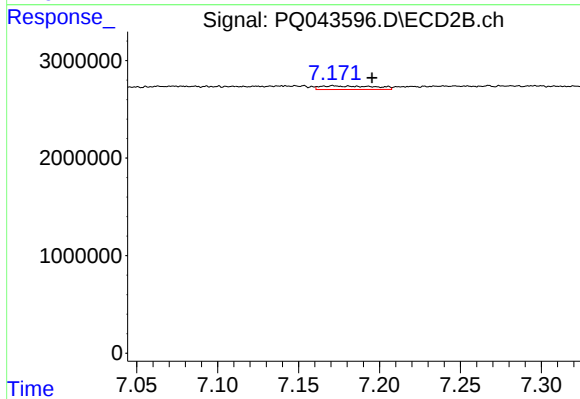

#20 AR-1242-5


R.T.: 7.171 min
Delta R.T.: -0.024 min
Response: 841754
Conc: 20.03 ng/ml

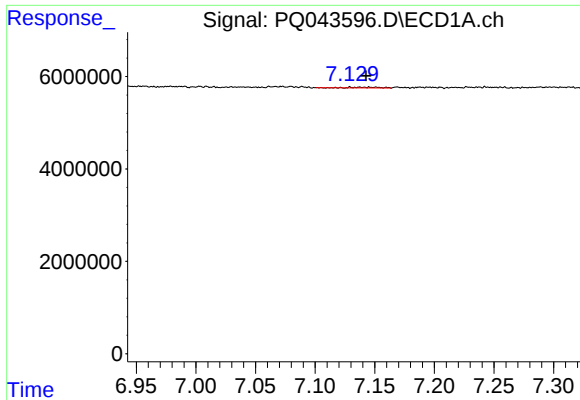

#21 AR-1248-1


R.T.: 7.146 min
Delta R.T.: 0.004 min
Response: 230486
Conc: 3.69 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

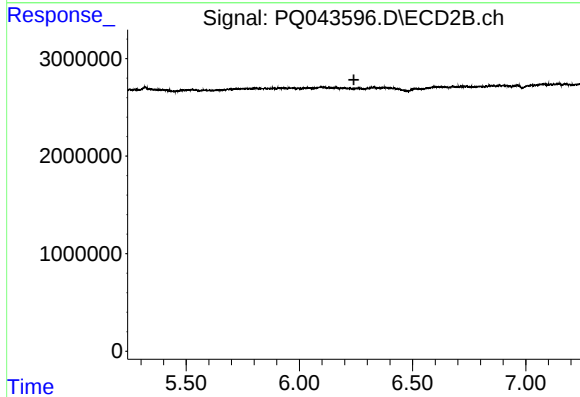


#21 AR-1248-1

R.T.: 0.000 min
Exp R.T. : 6.241 min
Response: 0
Conc: N.D.

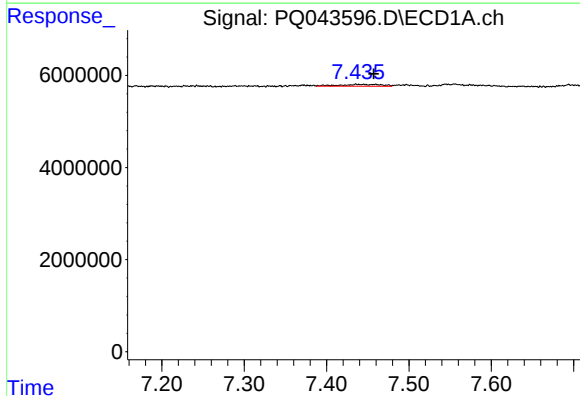


#22 AR-1248-2

R.T.: 7.444 min
Delta R.T.: -0.014 min
Response: 1436317
Conc: 15.76 ng/ml

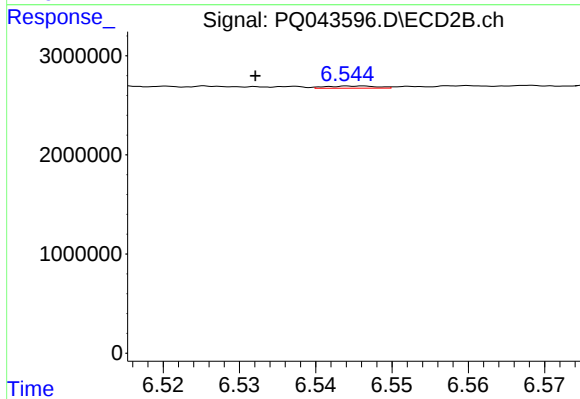

#22 AR-1248-2


R.T.: 6.545 min
Delta R.T.: 0.013 min
Response: 104401
Conc: 2.87 ng/ml

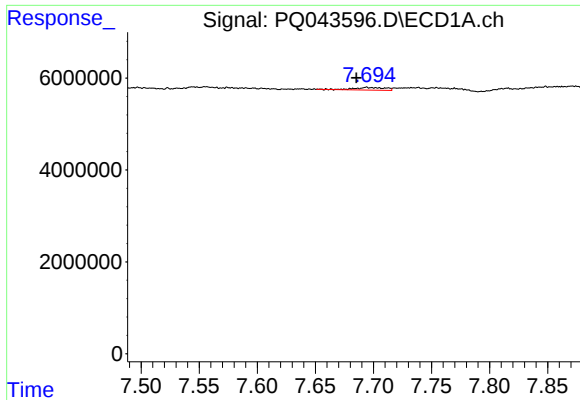

#23 AR-1248-3


R.T.: 7.695 min
Delta R.T.: 0.010 min
Response: 1038864
Conc: 10.01 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

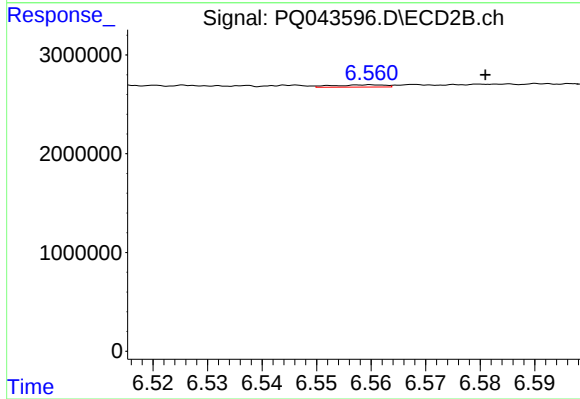


#23 AR-1248-3

R.T.: 6.560 min
Delta R.T.: -0.021 min
Response: 151535
Conc: 4.00 ng/ml

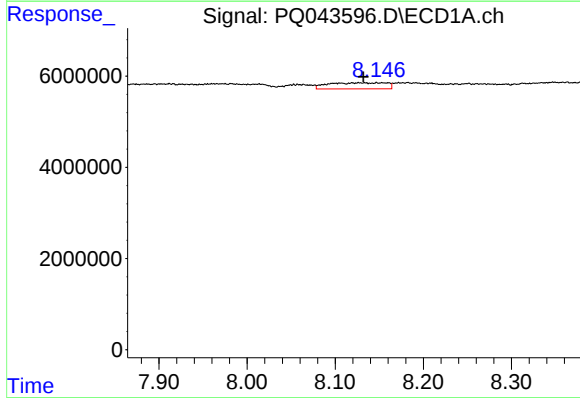


#24 AR-1248-4

R.T.: 8.129 min
Delta R.T.: -0.003 min
Response: 6184677
Conc: 45.52 ng/ml

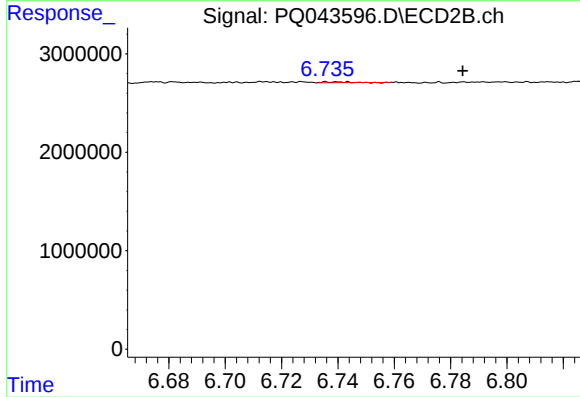

#24 AR-1248-4


R.T.: 6.736 min
Delta R.T.: -0.048 min
Response: 67223
Conc: 1.45 ng/ml

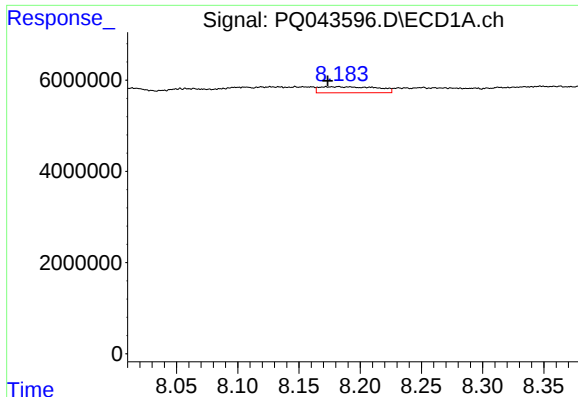

#25 AR-1248-5


R.T.: 8.181 min
Delta R.T.: 0.008 min
Response: 4387804
Conc: 33.10 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

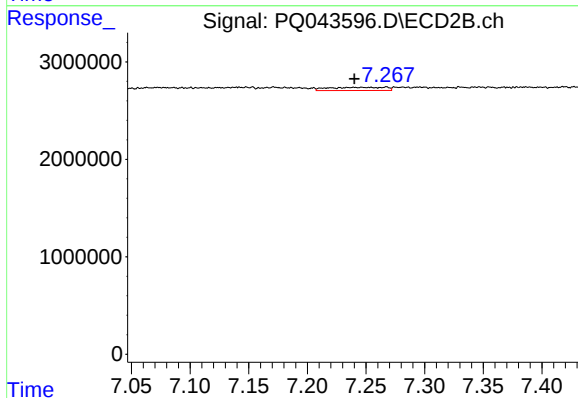


#25 AR-1248-5

R.T.: 7.246 min
Delta R.T.: 0.006 min
Response: 1117551
Conc: 21.64 ng/ml

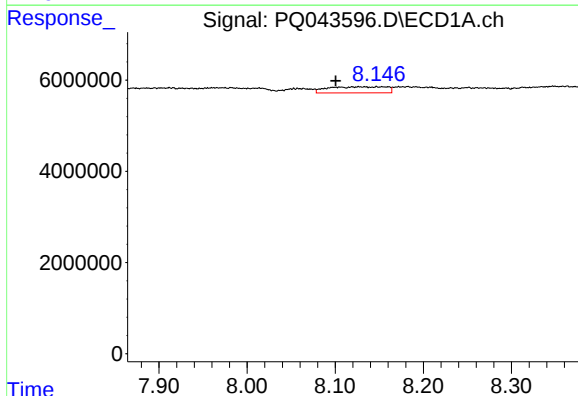


#26 AR-1254-1

R.T.: 8.129 min
Delta R.T.: 0.028 min
Response: 6184677
Conc: 42.07 ng/ml

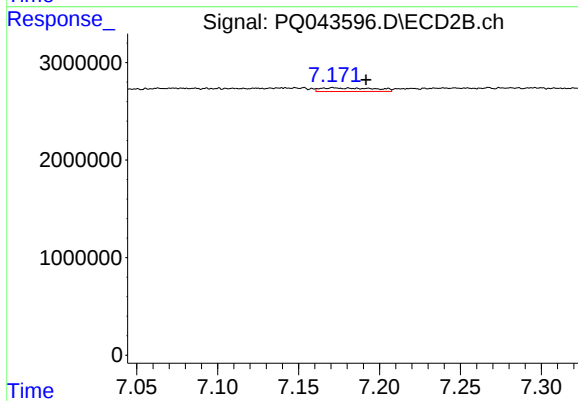

#26 AR-1254-1


R.T.: 7.171 min
Delta R.T.: -0.021 min
Response: 841754
Conc: 9.45 ng/ml

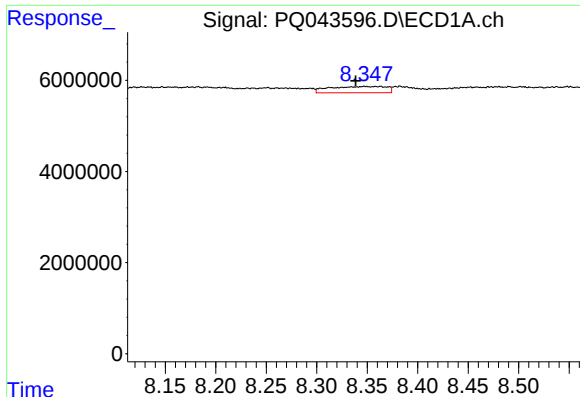

#27 AR-1254-2


R.T.: 8.348 min
Delta R.T.: 0.009 min
Response: 5358882
Conc: 21.89 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

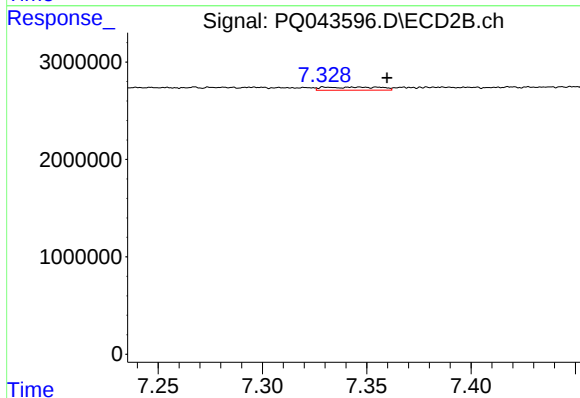


#27 AR-1254-2

R.T.: 7.354 min
Delta R.T.: -0.006 min
Response: 617529
Conc: 7.59 ng/ml

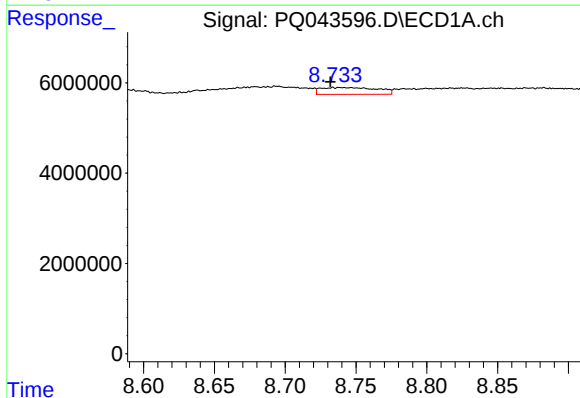


#28 AR-1254-3

R.T.: 8.738 min
Delta R.T.: 0.006 min
Response: 4201489
Conc: 14.57 ng/ml

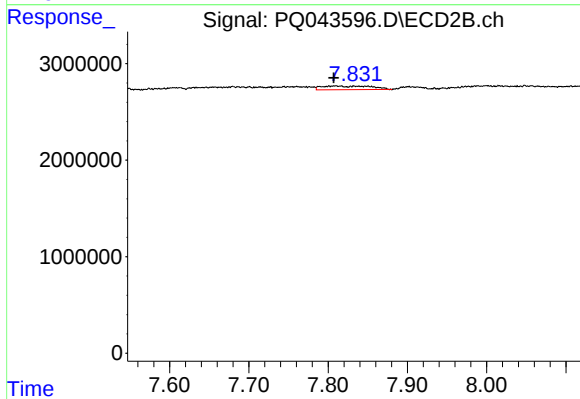

#28 AR-1254-3


R.T.: 7.809 min
Delta R.T.: 0.002 min
Response: 1678652
Conc: 11.89 ng/ml

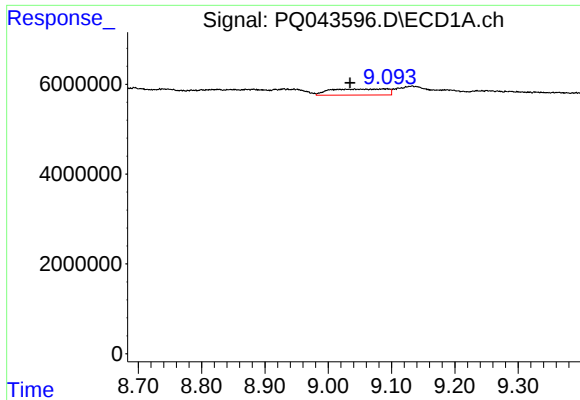

#29 AR-1254-4


R.T.: 9.092 min
Delta R.T.: 0.057 min
Response: 8422238
Conc: 36.08 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

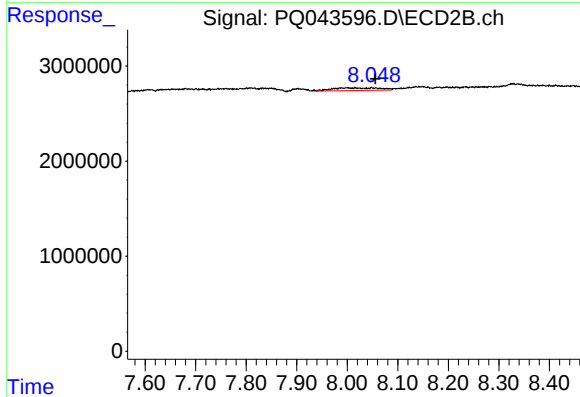


#29 AR-1254-4

R.T.: 8.016 min
Delta R.T.: -0.039 min
Response: 1826590
Conc: 18.73 ng/ml

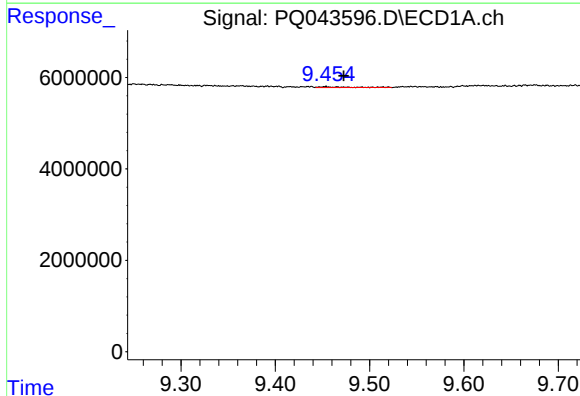


#30 AR-1254-5

R.T.: 9.453 min
Delta R.T.: -0.020 min
Response: 431911
Conc: 1.62 ng/ml

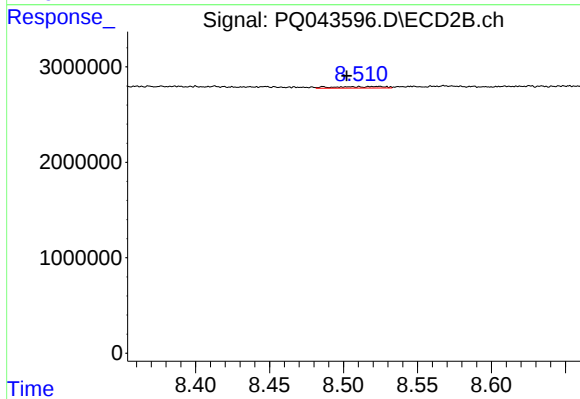

#30 AR-1254-5


R.T.: 8.523 min
Delta R.T.: 0.021 min
Response: 397752
Conc: 2.87 ng/ml

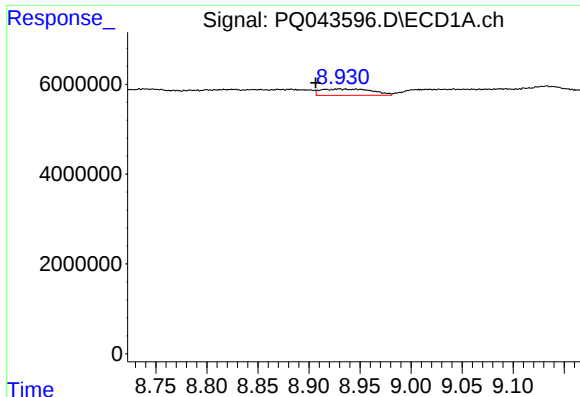

#31 AR-1260-1


R.T.: 8.930 min
Delta R.T.: 0.024 min
Response: 4846764
Conc: 26.15 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

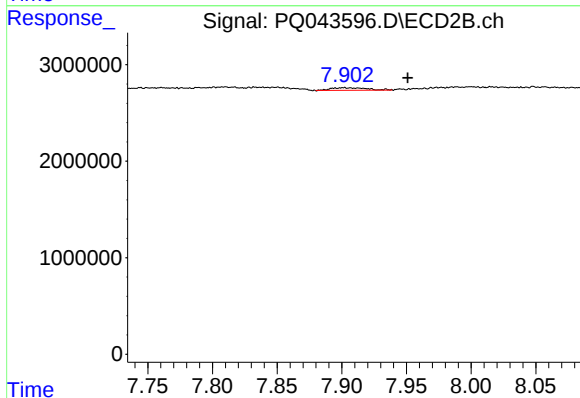


#31 AR-1260-1

R.T.: 7.902 min
Delta R.T.: -0.049 min
Response: 517140
Conc: 6.34 ng/ml

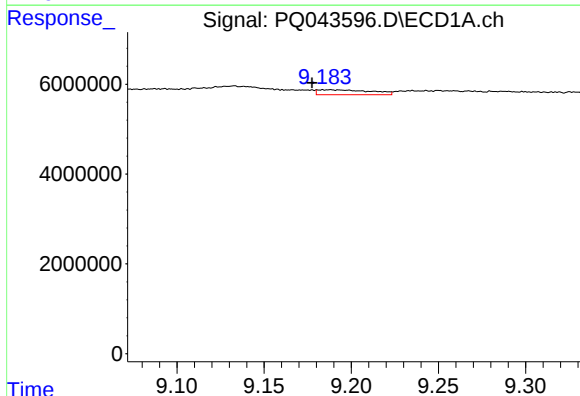


#32 AR-1260-2

R.T.: 9.187 min
Delta R.T.: 0.009 min
Response: 2306178
Conc: 9.79 ng/ml

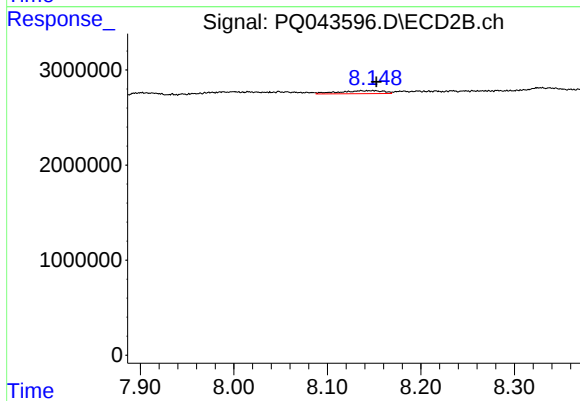

#32 AR-1260-2


R.T.: 8.148 min
Delta R.T.: -0.005 min
Response: 1060241
Conc: 9.99 ng/ml

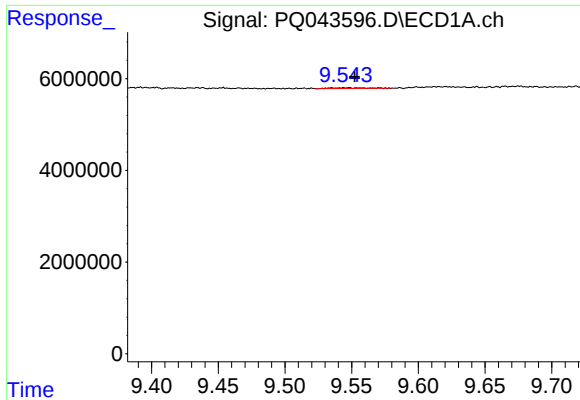

#33 AR-1260-3


R.T.: 9.545 min
Delta R.T.: -0.008 min
Response: 306704
Conc: 1.61 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

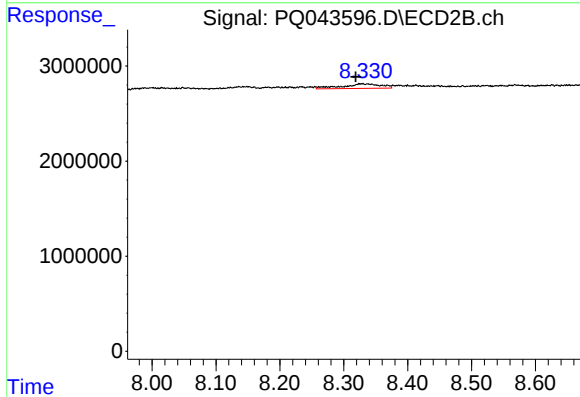


#33 AR-1260-3

R.T.: 8.328 min
Delta R.T.: 0.009 min
Response: 2084676
Conc: 21.76 ng/ml

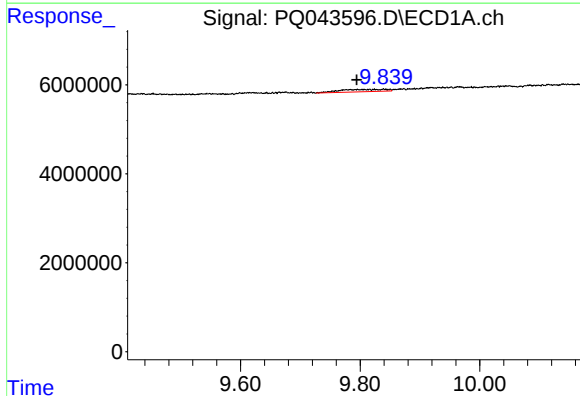


#34 AR-1260-4

R.T.: 9.840 min
Delta R.T.: 0.046 min
Response: 2782840
Conc: 12.05 ng/ml

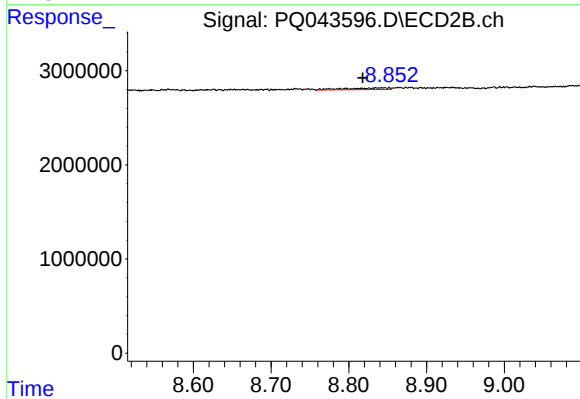

#34 AR-1260-4


R.T.: 8.841 min
Delta R.T.: 0.023 min
Response: 681408
Conc: 7.79 ng/ml

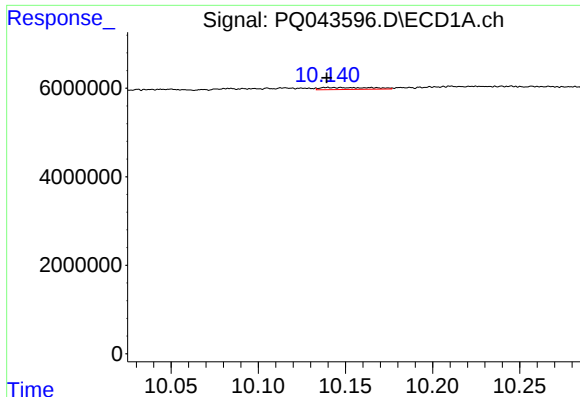

#35 AR-1260-5


R.T.: 10.141 min
Delta R.T.: 0.002 min
Response: 911498
Conc: 1.72 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

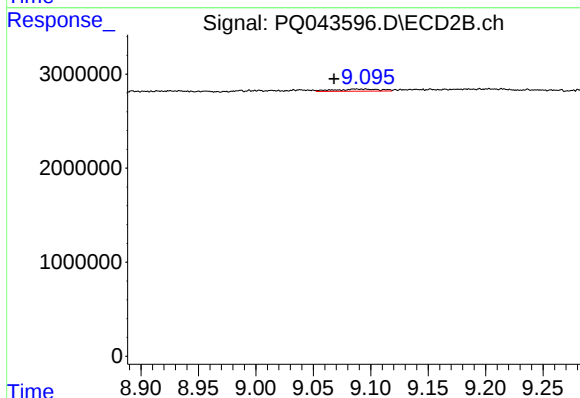


#35 AR-1260-5

R.T.: 9.088 min
Delta R.T.: 0.020 min
Response: 600189
Conc: 2.74 ng/ml

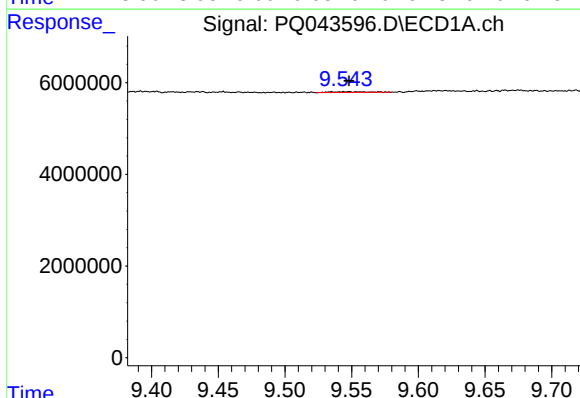


#36 AR-1262-1

R.T.: 9.545 min
Delta R.T.: -0.003 min
Response: 306704
Conc: 0.97 ng/ml

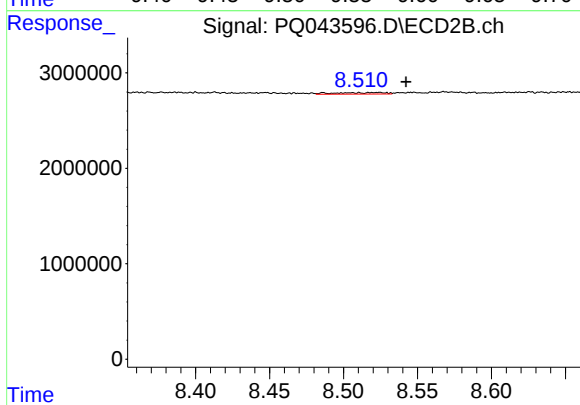

#36 AR-1262-1


R.T.: 8.523 min
Delta R.T.: -0.020 min
Response: 397752
Conc: 2.83 ng/ml

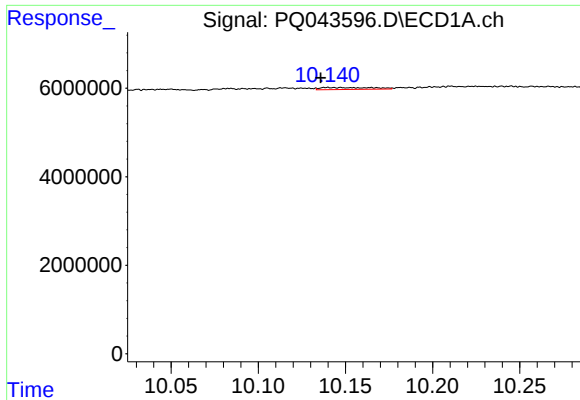

#37 AR-1262-2


R.T.: 10.141 min
Delta R.T.: 0.006 min
Response: 911498
Conc: 1.33 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

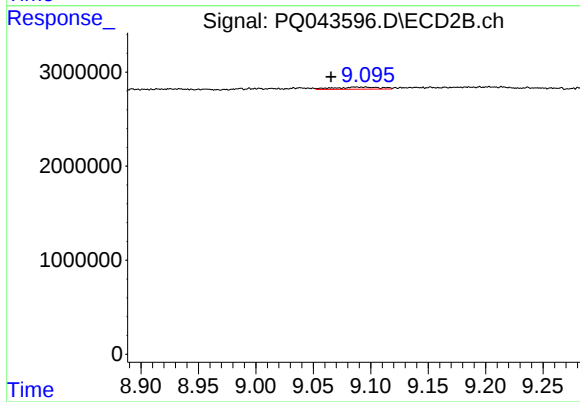


#37 AR-1262-2

R.T.: 9.088 min
Delta R.T.: 0.023 min
Response: 600189
Conc: 2.31 ng/ml

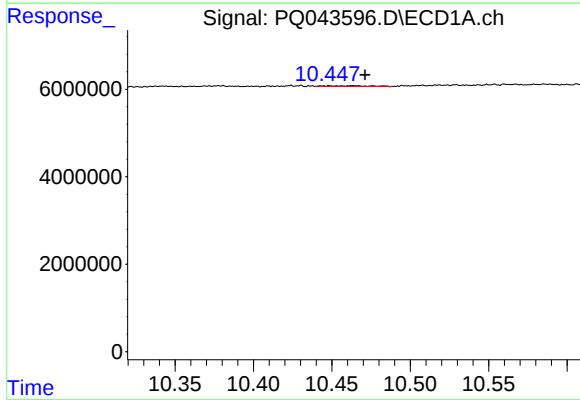


#38 AR-1262-3

R.T.: 10.464 min
Delta R.T.: -0.007 min
Response: 296927
Conc: 0.63 ng/ml

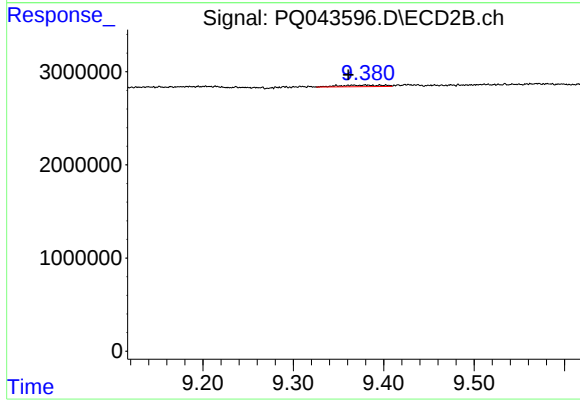

#38 AR-1262-3


R.T.: 9.366 min
Delta R.T.: 0.005 min
Response: 513895
Conc: 4.37 ng/ml

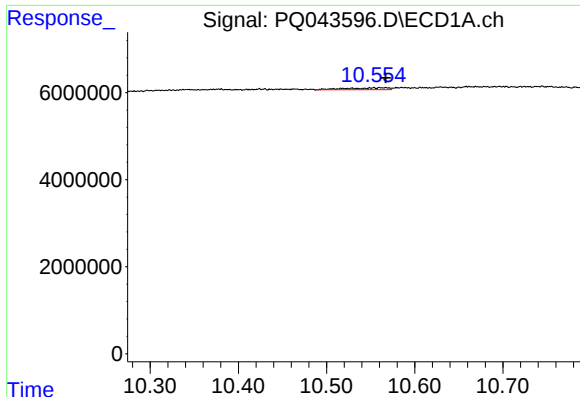

#39 AR-1262-4


R.T.: 10.553 min
Delta R.T.: -0.014 min
Response: 1454180
Conc: 4.04 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

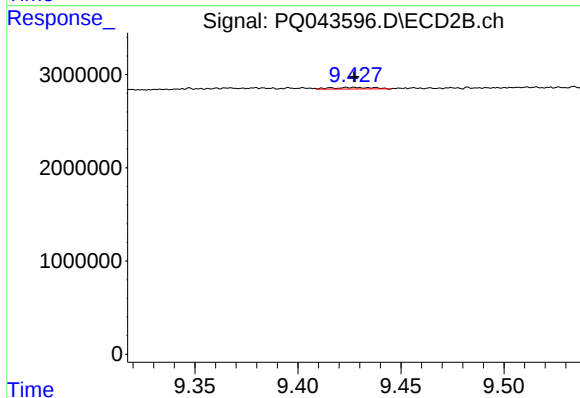


#39 AR-1262-4

R.T.: 9.427 min
Delta R.T.: 0.000 min
Response: 249433
Conc: 1.05 ng/ml

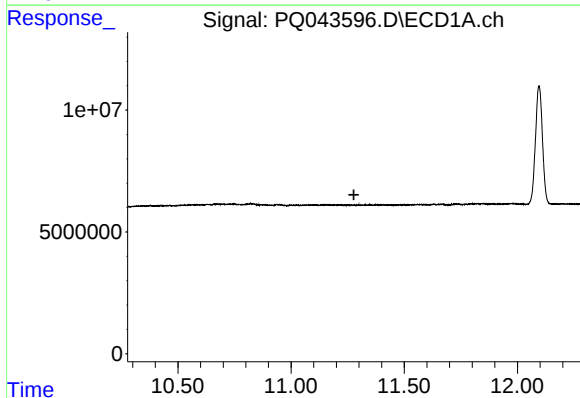


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T. : 11.277 min
Response: 0
Conc: N.D.

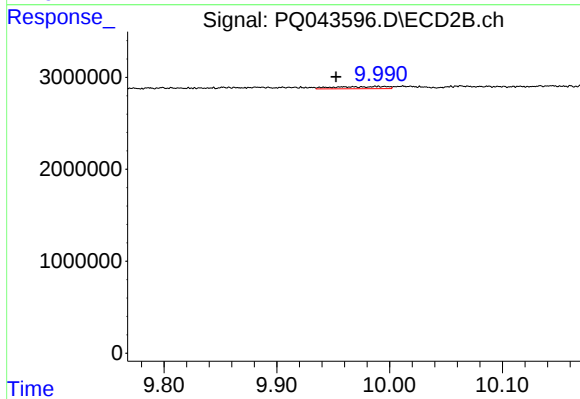

#40 AR-1262-5


R.T.: 9.991 min
Delta R.T.: 0.039 min
Response: 758785
Conc: 5.19 ng/ml

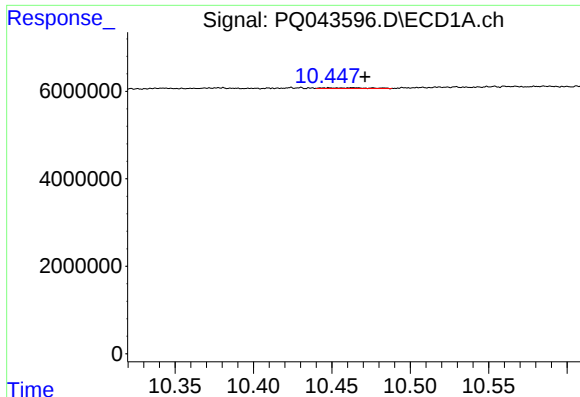

#41 AR-1268-1


R.T.: 10.464 min
Delta R.T.: -0.008 min
Response: 296927
Conc: 0.37 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

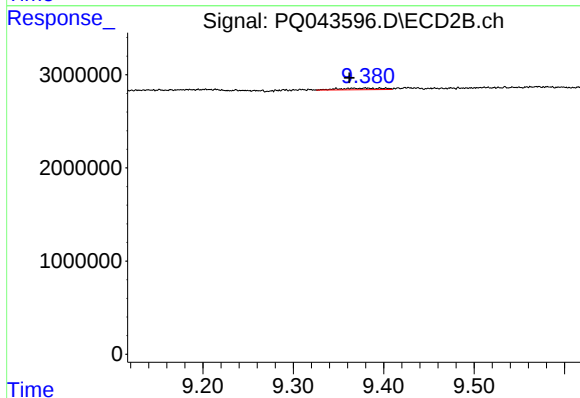


#41 AR-1268-1

R.T.: 9.366 min
Delta R.T.: 0.004 min
Response: 513895
Conc: 1.58 ng/ml

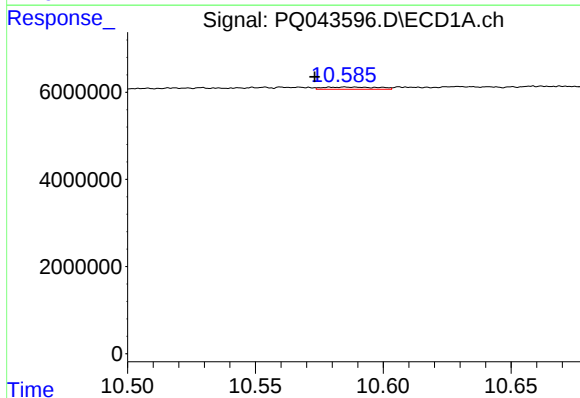


#42 AR-1268-2

R.T.: 10.587 min
Delta R.T.: 0.014 min
Response: 757169
Conc: 0.98 ng/ml

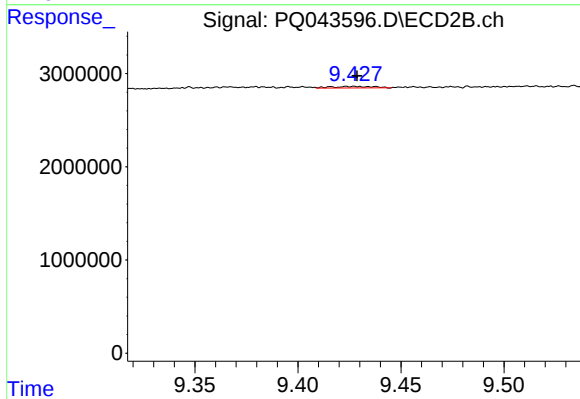

#42 AR-1268-2


R.T.: 9.427 min
Delta R.T.: -0.001 min
Response: 249433
Conc: 0.80 ng/ml

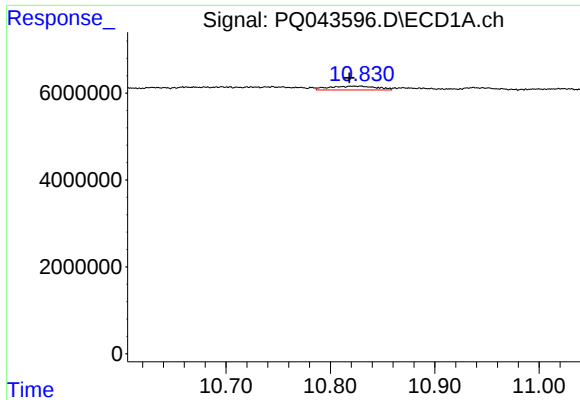

#43 AR-1268-3


R.T.: 10.825 min
Delta R.T.: 0.007 min
Response: 2760463
Conc: 4.19 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

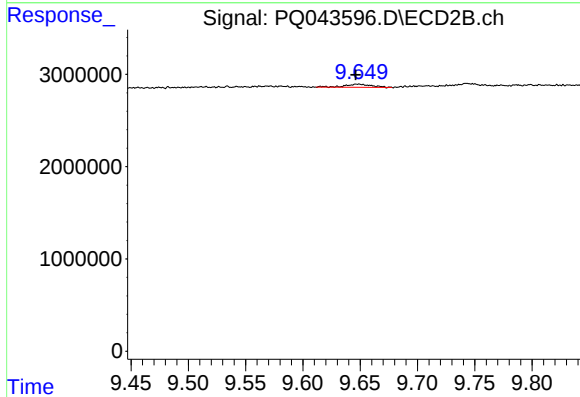


#43 AR-1268-3

R.T.: 9.648 min
Delta R.T.: 0.002 min
Response: 545818
Conc: 1.93 ng/ml

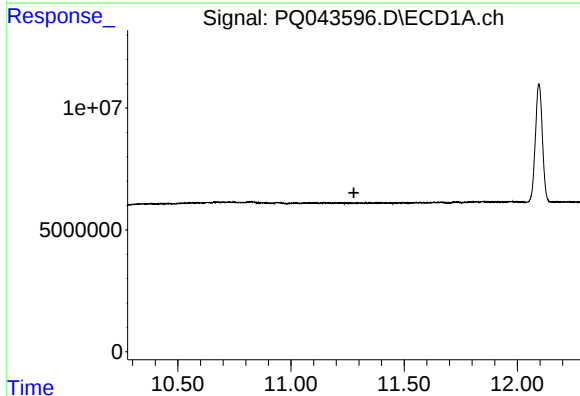


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 11.278 min
Response: 0
Conc: N.D.

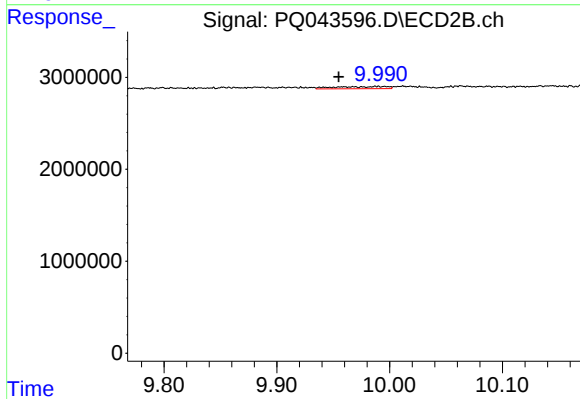

#44 AR-1268-4


R.T.: 9.991 min
Delta R.T.: 0.037 min
Response: 758785
Conc: 4.81 ng/ml

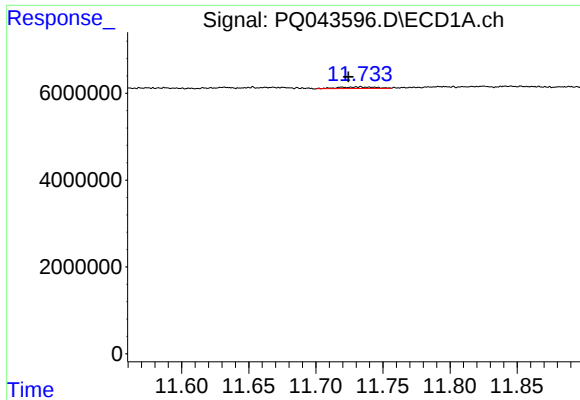

#45 AR-1268-5

R.T.: 11.732 min
Delta R.T.: 0.008 min
Response: 732442
Conc: 0.28 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

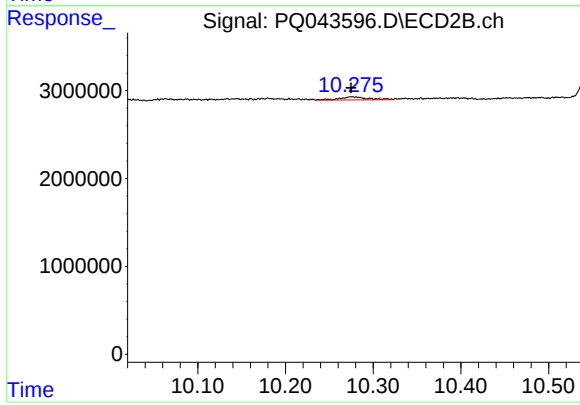

#45 AR-1268-5

R.T.: 10.276 min
Delta R.T.: 0.001 min
Response: 783310
Conc: 0.64 ng/ml