

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ091619\
 Data File : PQ043600.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Sep 2019 19:56
 Operator : SM\AJ
 Sample : K3591-09
 Misc : AR1254 MDL 25 PPB
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 MDL-MDL-WATER-03-QT3-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 04:51:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ091219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 13 03:48:31 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.701	4.787	22945644	10415624	9.059	10.123
2)	SA Decachlor...	12.093	10.559	108.8E6	42754730	13.146	11.368
Target Compounds							
3)	L1 AR-1016-1	7.161	0.000	329667	0	3.192	N.D. #
4)	L1 AR-1016-2	7.161	0.000	329667	0	2.248	N.D. #
5)	L1 AR-1016-3	7.248	6.528	281201	352910	3.064	11.039 #
6)	L1 AR-1016-4	7.398	6.528	-11245	352910	N.D.	12.963 #
7)	L1 AR-1016-5	7.689	6.787	1867476	204496	24.158	5.792 #
8)	L2 AR-1221-1	5.987	5.123	180373	57115	6.137	5.183
9)	L2 AR-1221-2	6.092	5.263	913015	138315	41.717	15.982 #
10)	L2 AR-1221-3	6.165	5.345	544322	44832	7.818	1.561 #
11)	L3 AR-1232-1	6.165	5.345	544322	44832	5.548	1.100 #
12)	L3 AR-1232-2	6.819	0.000	1703864	0	31.578	N.D. #
13)	L3 AR-1232-3	7.161	6.528	329667	352910	2.893	14.101 #
14)	L3 AR-1232-4	7.398	6.575	-11245	213630	N.D.	9.113 #
15)	L3 AR-1232-5	7.457	6.787	1445808	204496	35.716	7.969 #
16)	L4 AR-1242-1	7.161	0.000	329667	0	3.703	N.D. #
17)	L4 AR-1242-2	7.161	0.000	329667	0	2.573	N.D. #
18)	L4 AR-1242-3	7.248	6.528	281201	352910	3.494	12.714 #
19)	L4 AR-1242-4	7.398	6.575	-11245	213630	N.D.	7.415 #
20)	L4 AR-1242-5	8.178	7.193	5618785	1600962	61.919	38.104 #
21)	L5 AR-1248-1	7.161	0.000	329667	0	5.285	N.D. #
22)	L5 AR-1248-2	7.457	6.528	1445808	352910	15.867	9.703 #
23)	L5 AR-1248-3	7.689	6.575	1867476	213630	18.001	5.634 #
24)	L5 AR-1248-4	8.133	6.787	3021622	204496	22.241	4.424 #
25)	L5 AR-1248-5	8.178	7.240	5618785	520939	42.381	10.089 #
26)	L6 AR-1254-1	8.103	7.193	5018252	1600962	34.134	17.982 #
27)	L6 AR-1254-2	8.340	7.361	9287916	1542017	37.943	18.964 #
28)	L6 AR-1254-3	8.735	7.809	8836695	3289623	30.644	23.295
29)	L6 AR-1254-4	9.036	8.057	7106046	2793411	30.438	28.647
30)	L6 AR-1254-5	9.475	8.504	5253249	3028045	19.753	21.823
31)	L7 AR-1260-1	8.910	7.951	5296261	3055124	28.571	37.481 #
32)	L7 AR-1260-2	9.177	8.152	3580757	2335234	15.193	22.009 #
33)	L7 AR-1260-3	9.547	8.320	1236877	2833627	6.484	29.579 #
34)	L7 AR-1260-4	9.782	8.819	2589408	408267	11.215	4.666 #
35)	L7 AR-1260-5	10.140	9.047	1705959	1234977	3.225	5.634 #
36)	L8 AR-1262-1	9.547	8.578	1236877	799473	3.913	5.697 #
37)	L8 AR-1262-2	10.140	9.047	1705959	1234977	2.498	4.759 #
38)	L8 AR-1262-3	10.499	9.372	570411	702335	1.204	5.972 #
39)	L8 AR-1262-4	10.555	9.427	579421	653570	1.608	2.755 #
40)	L8 AR-1262-5	11.280	10.016	860156	1890624	2.896	12.934 #
41)	L9 AR-1268-1	10.499	9.372	570411	702335	0.710	2.165 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ091619\
 Data File : PQ043600.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Sep 2019 19:56
 Operator : SM\AJ
 Sample : K3591-09
 Misc : AR1254 MDL 25 PPB
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 MDL-MDL-WATER-03-QT3-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 04:51:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ091219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 13 03:48:31 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	10.555	9.427	579421	653570	0.752	2.087 #
43) L9	AR-1268-3	10.821	9.648	1707759	607710	2.590	2.150
44) L9	AR-1268-4	11.280	10.016	860156	1890624	2.679	11.978 #
45) L9	AR-1268-5	11.728	10.275	1338789	1779965	0.503	1.461 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ091619\
Data File : PQ043600.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Sep 2019 19:56
Operator : SM\AJ
Sample : K3591-09
Misc : AR1254 MDL 25 PPB
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 04:51:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ091219.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 13 03:48:31 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

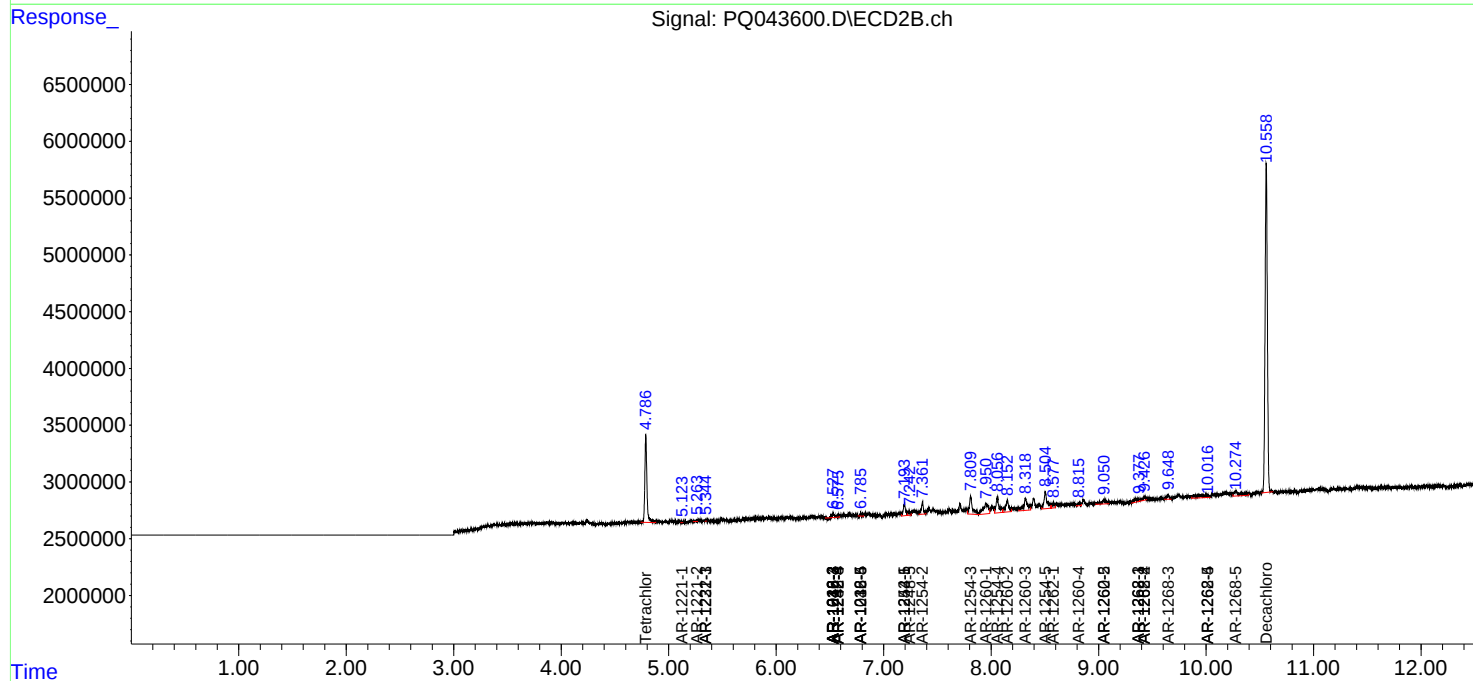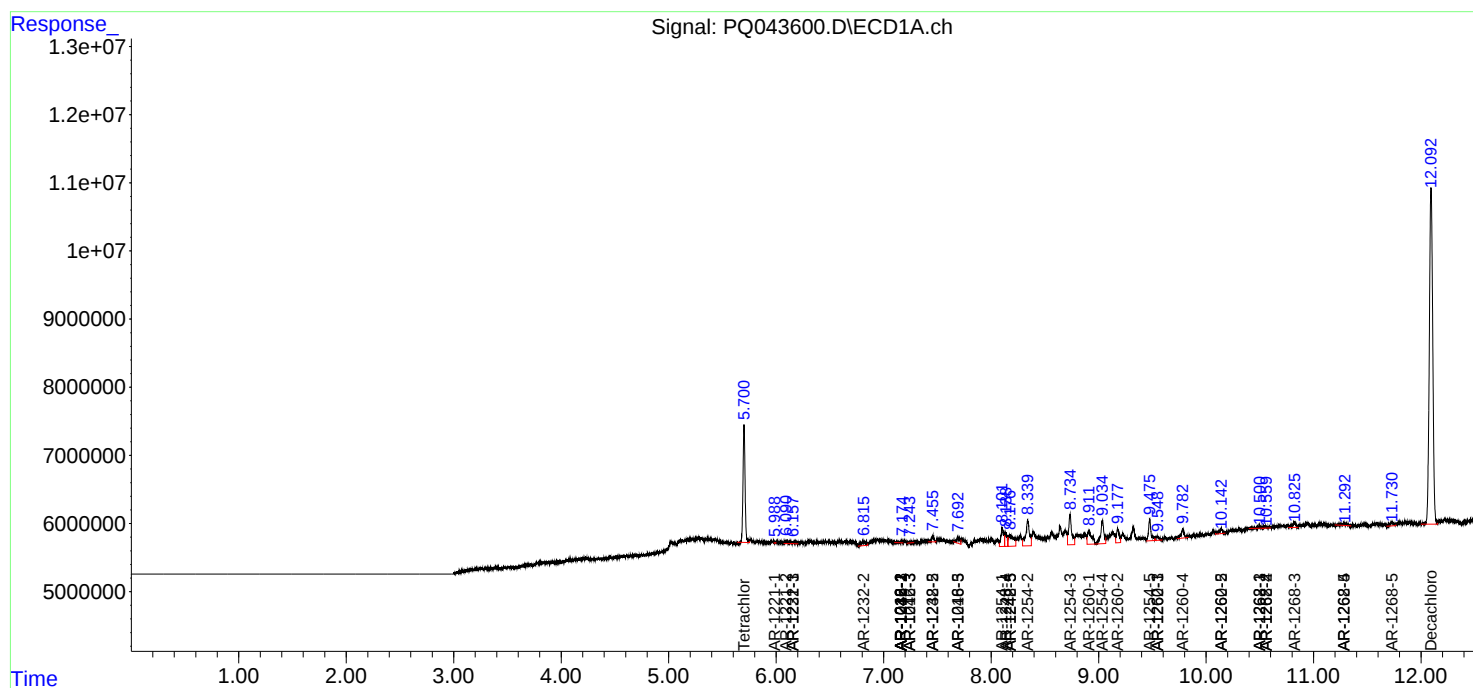


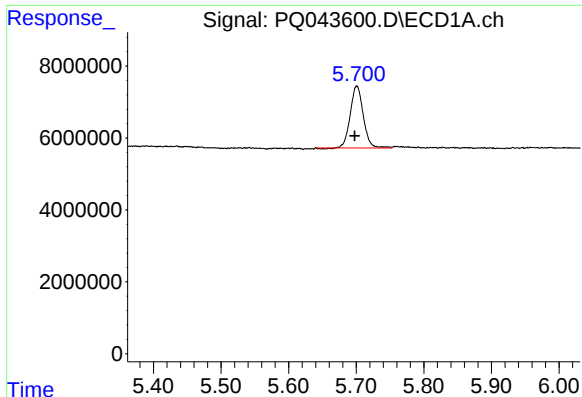

#1 Tetrachloro-m-xylene


R.T.: 5.701 min
Delta R.T.: 0.003 min
Response: 22945644
Conc: 9.06 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

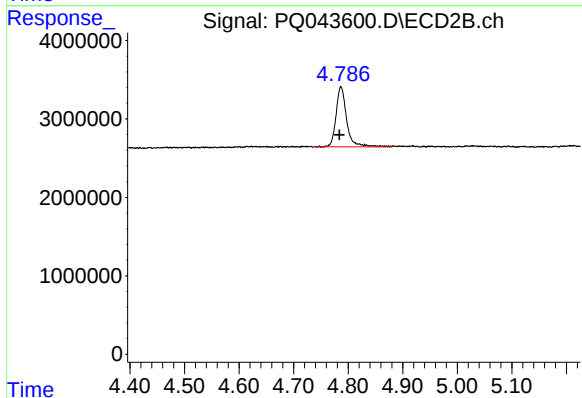


#1 Tetrachloro-m-xylene

R.T.: 4.787 min
Delta R.T.: 0.003 min
Response: 10415624
Conc: 10.12 ng/ml

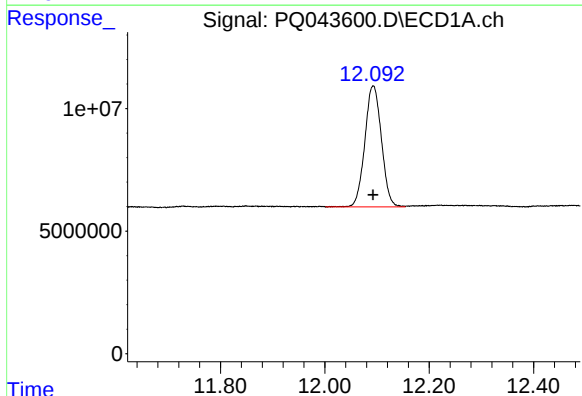


#2 Decachlorobiphenyl

R.T.: 12.093 min
Delta R.T.: 0.000 min
Response: 108848777
Conc: 13.15 ng/ml

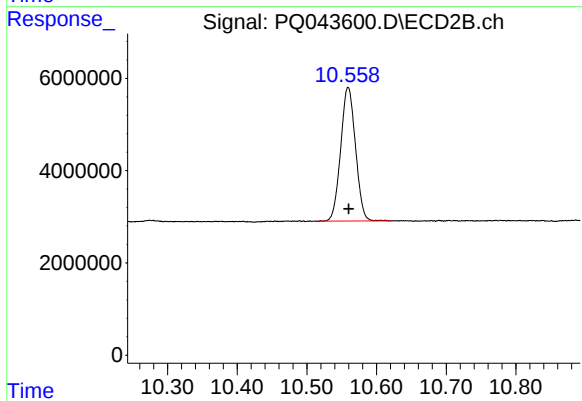

#2 Decachlorobiphenyl


R.T.: 10.559 min
Delta R.T.: 0.000 min
Response: 42754730
Conc: 11.37 ng/ml

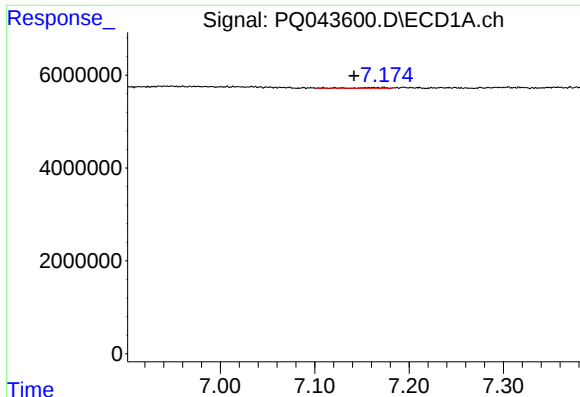

#3 AR-1016-1


R.T.: 7.161 min
Delta R.T.: 0.019 min
Response: 329667
Conc: 3.19 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

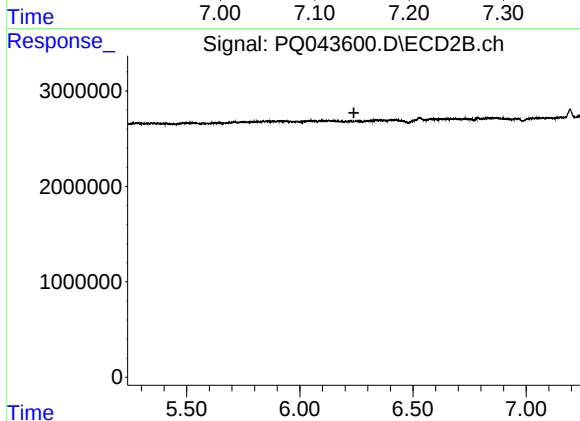


#3 AR-1016-1

R.T.: 0.000 min
Exp R.T. : 6.239 min
Response: 0
Conc: N.D.

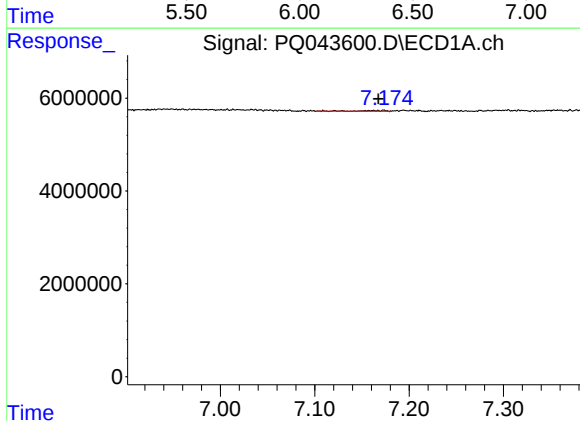


#4 AR-1016-2

R.T.: 7.161 min
Delta R.T.: -0.006 min
Response: 329667
Conc: 2.25 ng/ml

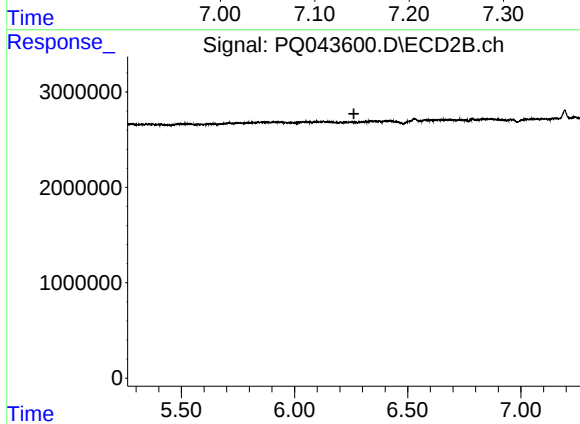

#4 AR-1016-2


R.T.: 0.000 min
Exp R.T. : 6.262 min
Response: 0
Conc: N.D.

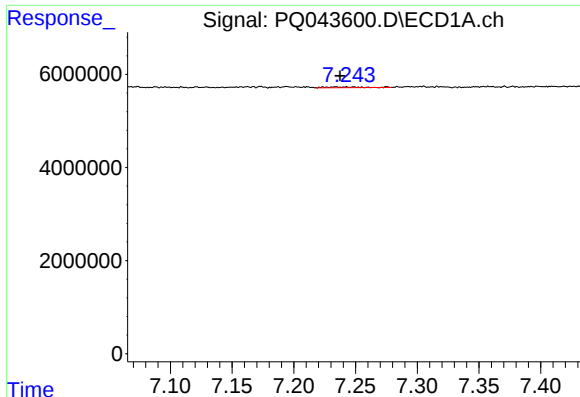

#5 AR-1016-3


R.T.: 7.248 min
Delta R.T.: 0.010 min
Response: 281201
Conc: 3.06 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

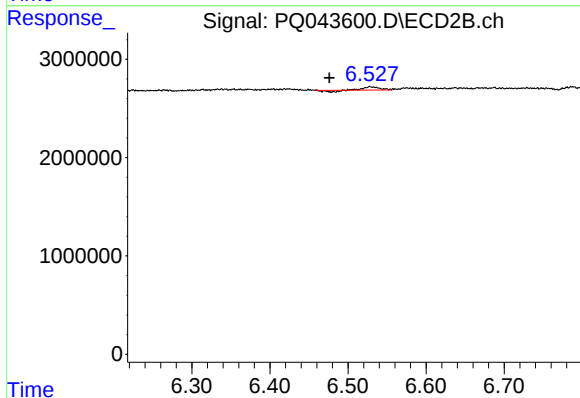


#5 AR-1016-3

R.T.: 6.528 min
Delta R.T.: 0.052 min
Response: 352910
Conc: 11.04 ng/ml

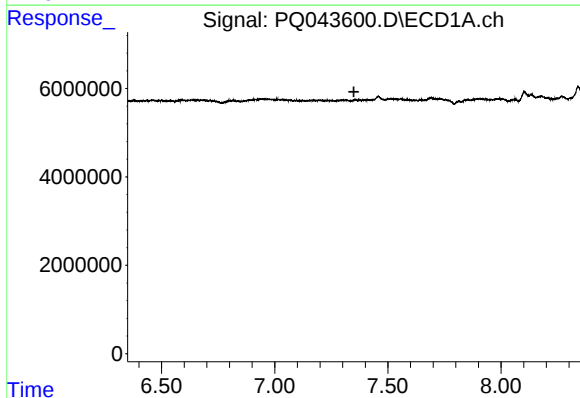


#6 AR-1016-4

R.T.: 7.398 min
Delta R.T.: 0.048 min
Response: -11245
Conc: N.D.

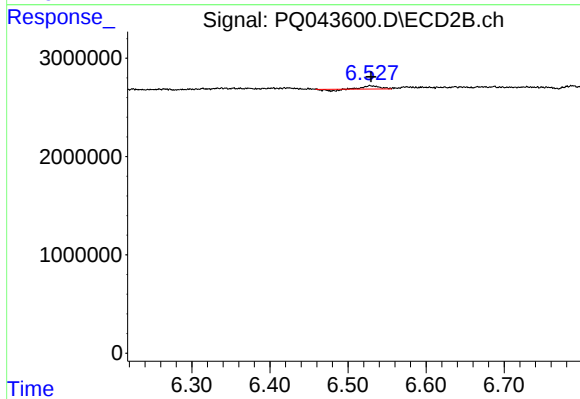

#6 AR-1016-4


R.T.: 6.528 min
Delta R.T.: -0.001 min
Response: 352910
Conc: 12.96 ng/ml

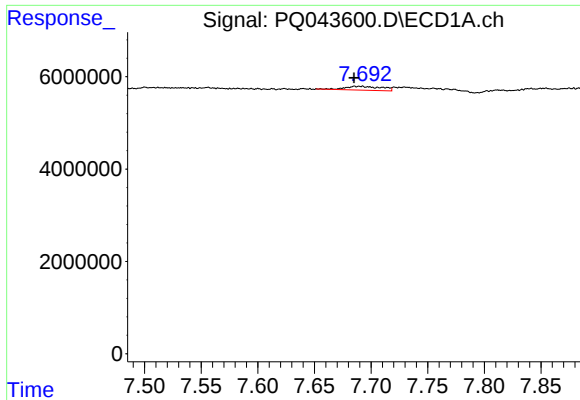

#7 AR-1016-5


R.T.: 7.689 min
Delta R.T.: 0.004 min
Response: 1867476
Conc: 24.16 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

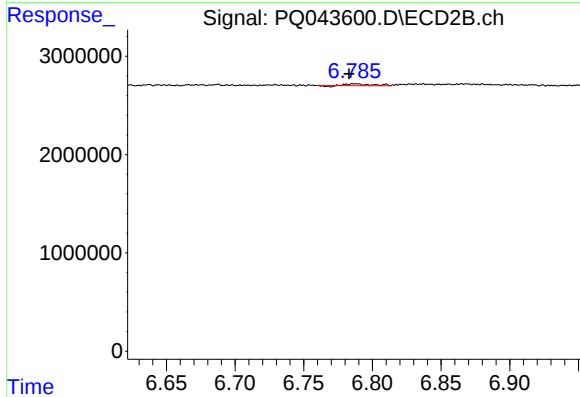


#7 AR-1016-5

R.T.: 6.787 min
Delta R.T.: 0.004 min
Response: 204496
Conc: 5.79 ng/ml

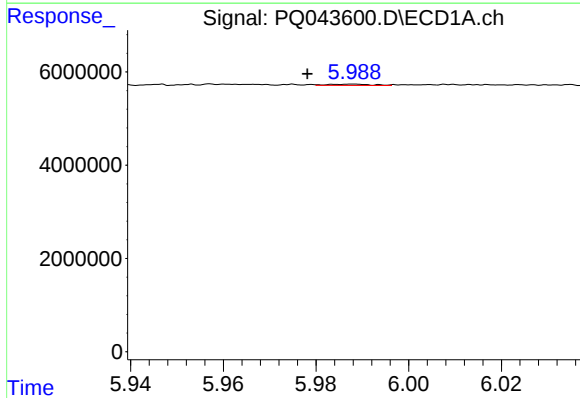


#8 AR-1221-1

R.T.: 5.987 min
Delta R.T.: 0.009 min
Response: 180373
Conc: 6.14 ng/ml

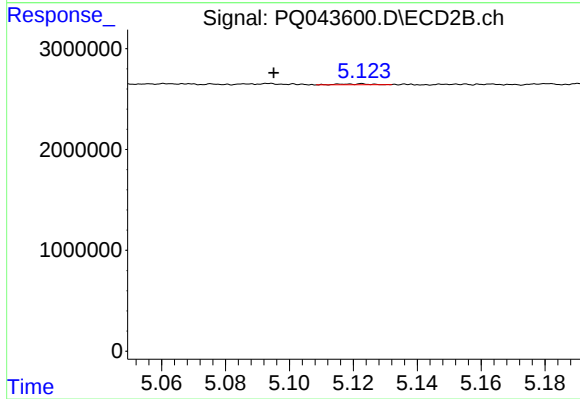

#8 AR-1221-1


R.T.: 5.123 min
Delta R.T.: 0.028 min
Response: 57115
Conc: 5.18 ng/ml

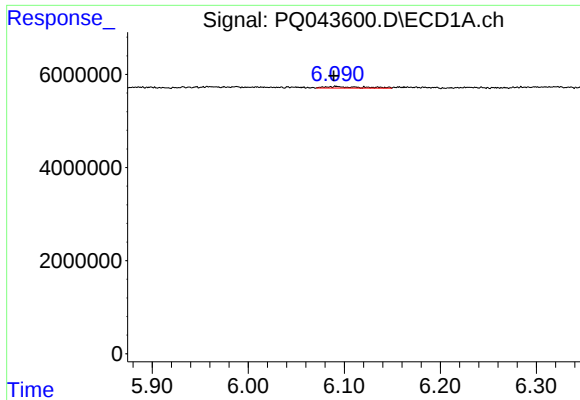

#9 AR-1221-2


R.T.: 6.092 min
Delta R.T.: 0.003 min
Response: 913015
Conc: 41.72 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

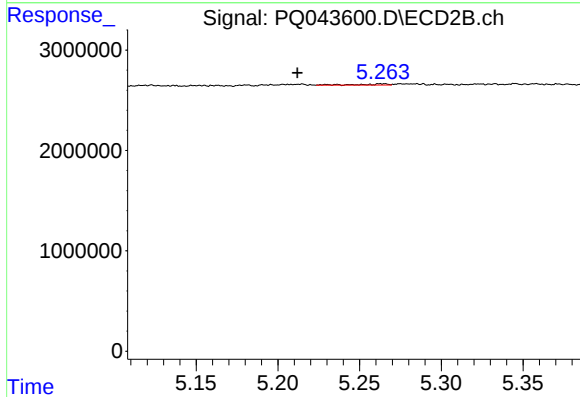


#9 AR-1221-2

R.T.: 5.263 min
Delta R.T.: 0.051 min
Response: 138315
Conc: 15.98 ng/ml

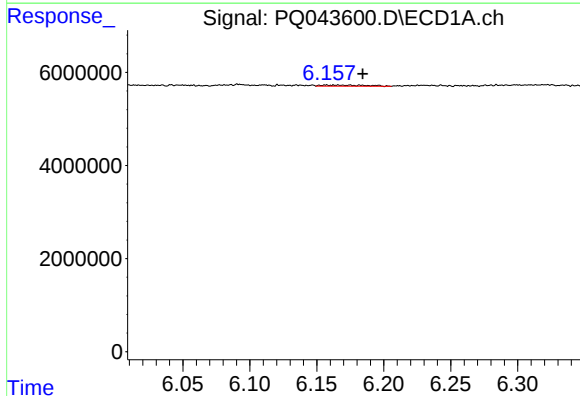


#10 AR-1221-3

R.T.: 6.165 min
Delta R.T.: -0.019 min
Response: 544322
Conc: 7.82 ng/ml

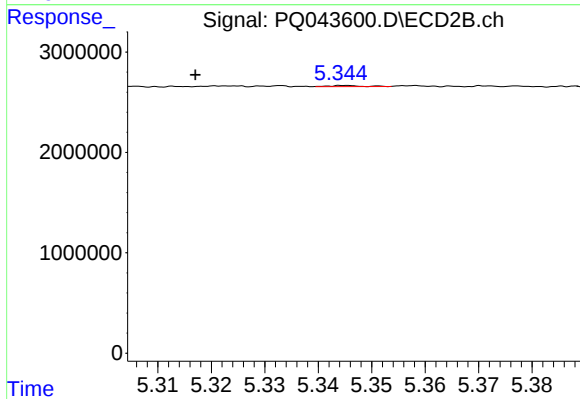

#10 AR-1221-3


R.T.: 5.345 min
Delta R.T.: 0.028 min
Response: 44832
Conc: 1.56 ng/ml

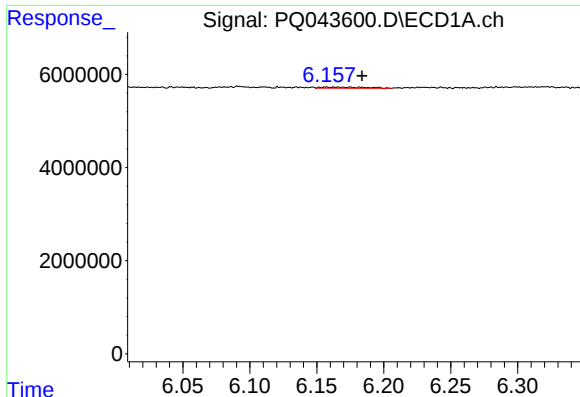

#11 AR-1232-1


R.T.: 6.165 min
Delta R.T.: -0.019 min
Response: 544322
Conc: 5.55 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

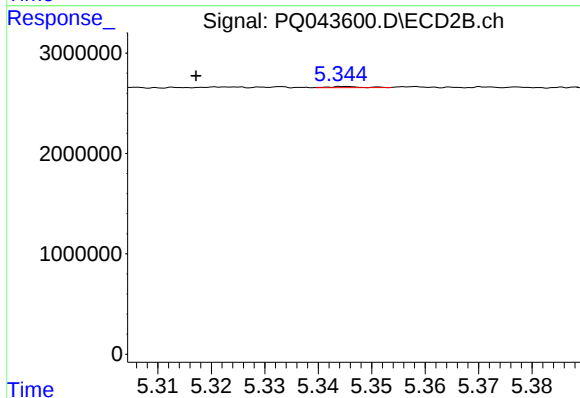


#11 AR-1232-1

R.T.: 5.345 min
Delta R.T.: 0.028 min
Response: 44832
Conc: 1.10 ng/ml

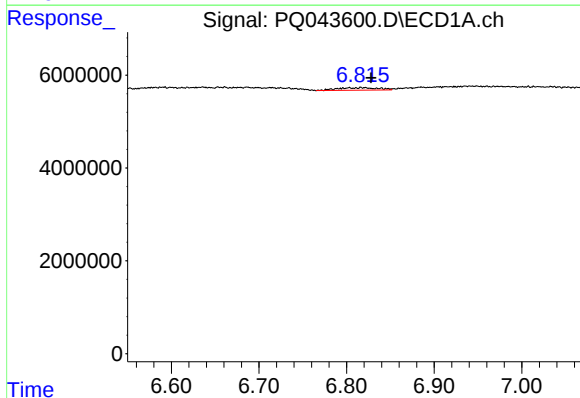


#12 AR-1232-2

R.T.: 6.819 min
Delta R.T.: -0.009 min
Response: 1703864
Conc: 31.58 ng/ml

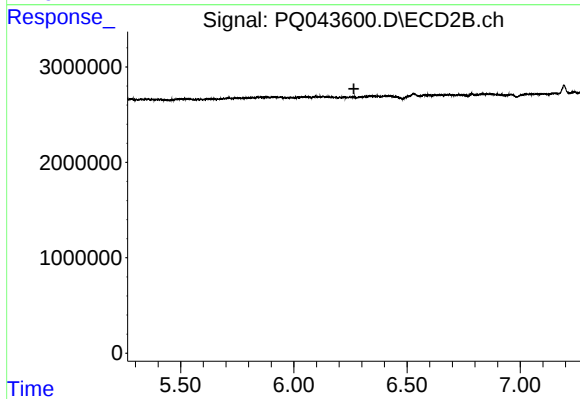

#12 AR-1232-2


R.T.: 0.000 min
Exp R.T.: 6.265 min
Response: 0
Conc: N.D.

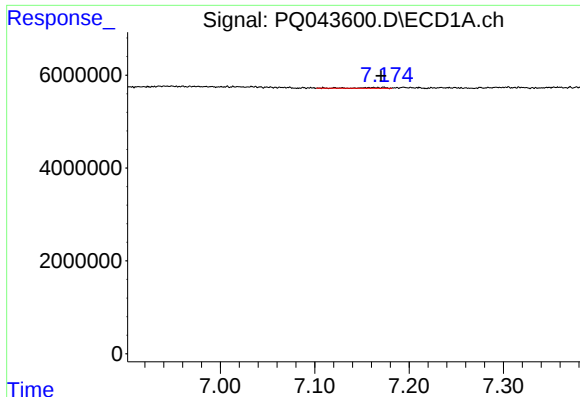

#13 AR-1232-3


R.T.: 7.161 min
Delta R.T.: -0.009 min
Response: 329667
Conc: 2.89 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

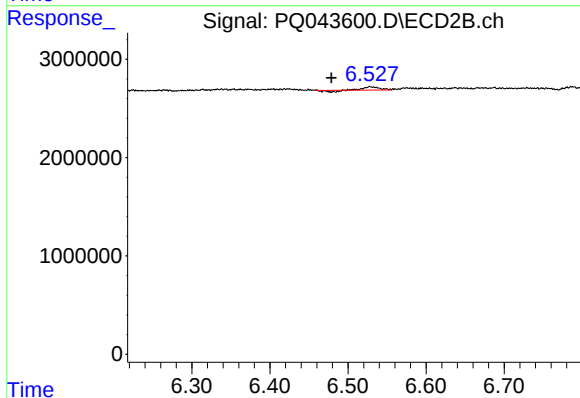


#13 AR-1232-3

R.T.: 6.528 min
Delta R.T.: 0.049 min
Response: 352910
Conc: 14.10 ng/ml

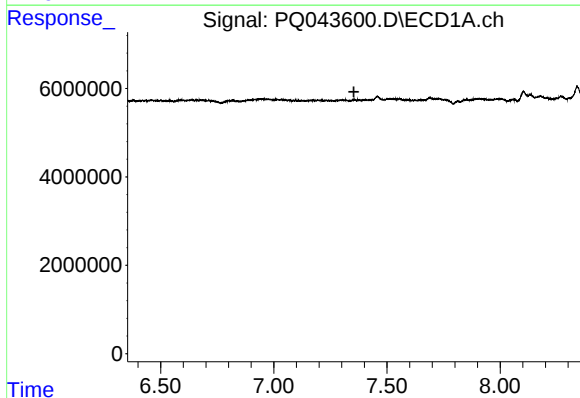


#14 AR-1232-4

R.T.: 7.398 min
Delta R.T.: 0.045 min
Response: -11245
Conc: N.D.

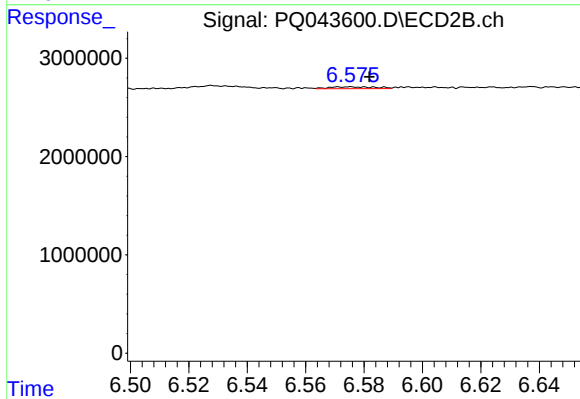

#14 AR-1232-4


R.T.: 6.575 min
Delta R.T.: -0.006 min
Response: 213630
Conc: 9.11 ng/ml

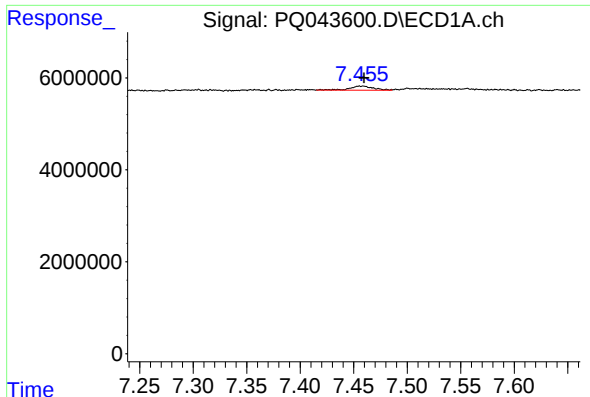

#15 AR-1232-5


R.T.: 7.457 min
Delta R.T.: -0.002 min
Response: 1445808
Conc: 35.72 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

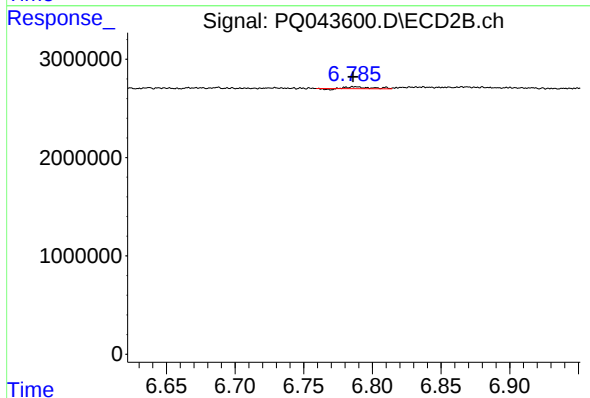


#15 AR-1232-5

R.T.: 6.787 min
Delta R.T.: 0.001 min
Response: 204496
Conc: 7.97 ng/ml

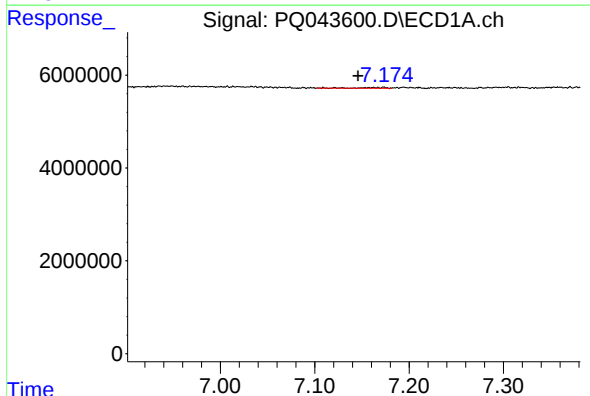


#16 AR-1242-1

R.T.: 7.161 min
Delta R.T.: 0.015 min
Response: 329667
Conc: 3.70 ng/ml

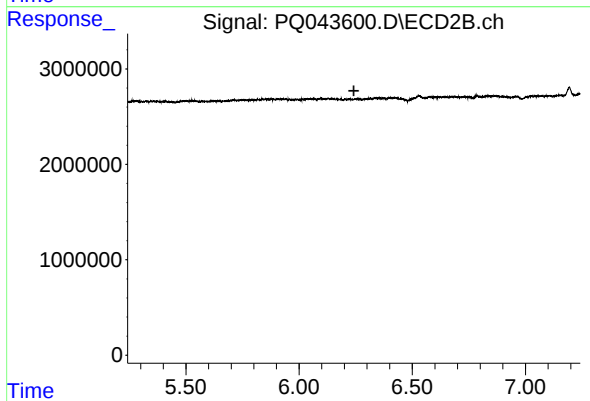

#16 AR-1242-1


R.T.: 0.000 min
Exp R.T.: 6.242 min
Response: 0
Conc: N.D.

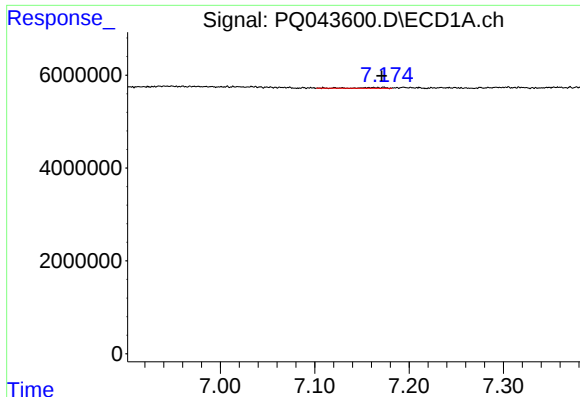

#17 AR-1242-2


R.T.: 7.161 min
Delta R.T.: -0.010 min
Response: 329667
Conc: 2.57 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

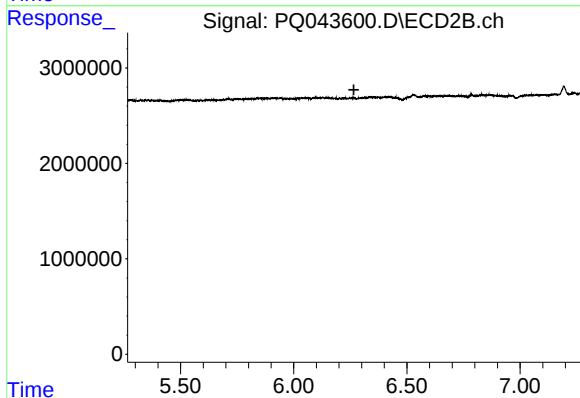


#17 AR-1242-2

R.T.: 0.000 min
Exp R.T. : 6.266 min
Response: 0
Conc: N.D.

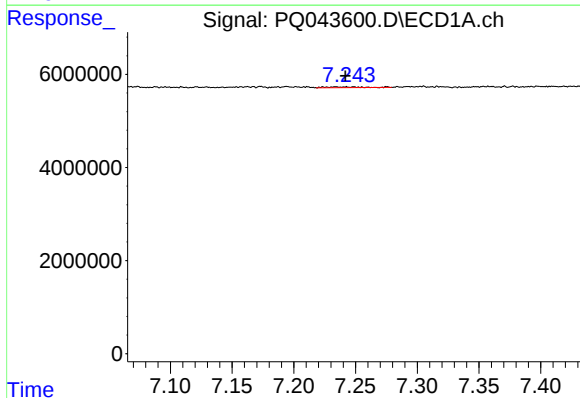


#18 AR-1242-3

R.T.: 7.248 min
Delta R.T.: 0.006 min
Response: 281201
Conc: 3.49 ng/ml

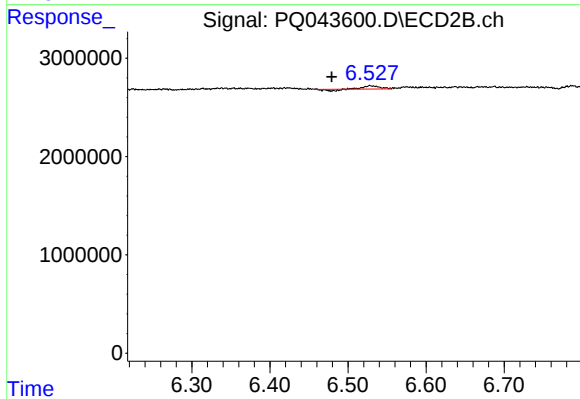

#18 AR-1242-3


R.T.: 6.528 min
Delta R.T.: 0.049 min
Response: 352910
Conc: 12.71 ng/ml

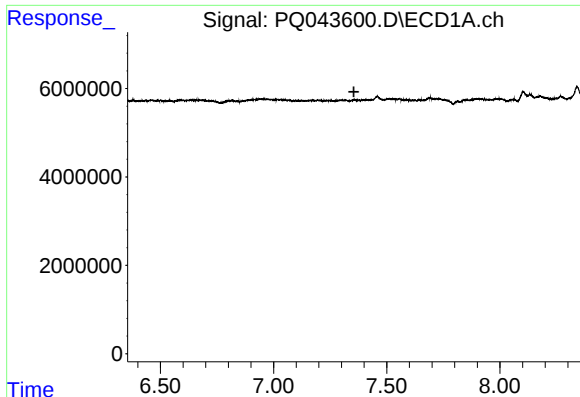

#19 AR-1242-4


R.T.: 7.398 min
Delta R.T.: 0.044 min
Response: -11245
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

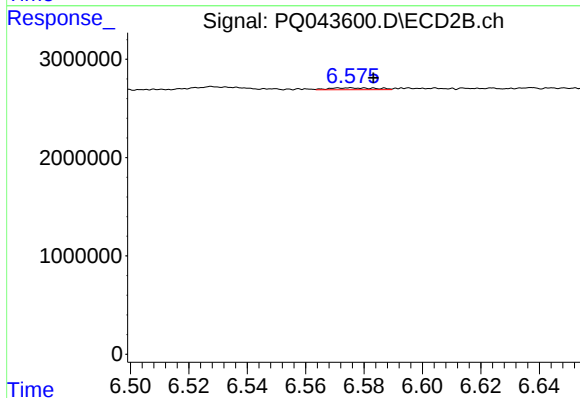


#19 AR-1242-4

R.T.: 6.575 min
Delta R.T.: -0.008 min
Response: 213630
Conc: 7.42 ng/ml

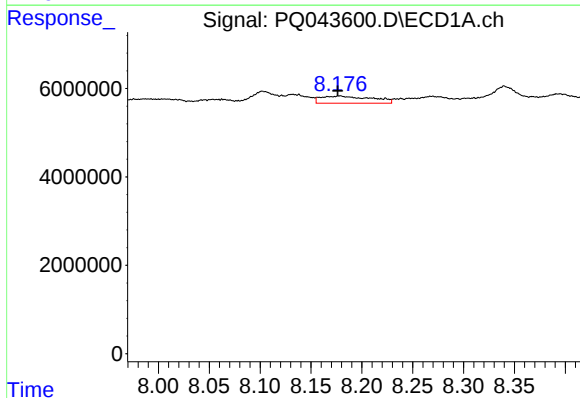


#20 AR-1242-5

R.T.: 8.178 min
Delta R.T.: 0.002 min
Response: 5618785
Conc: 61.92 ng/ml

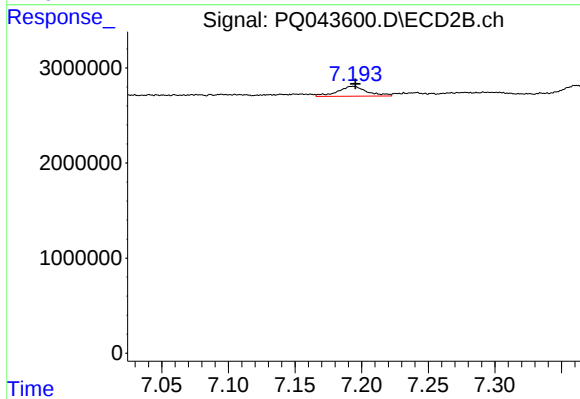

#20 AR-1242-5


R.T.: 7.193 min
Delta R.T.: -0.002 min
Response: 1600962
Conc: 38.10 ng/ml

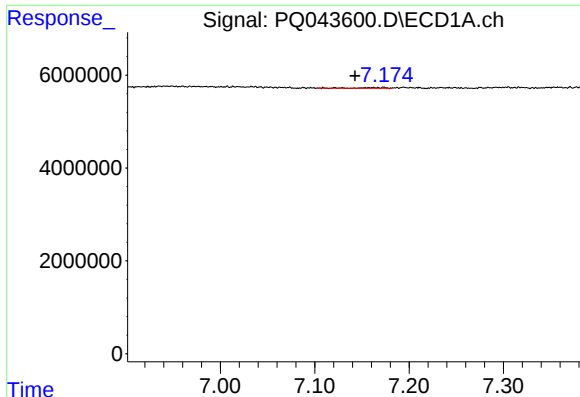

#21 AR-1248-1


R.T.: 7.161 min
Delta R.T.: 0.019 min
Response: 329667
Conc: 5.28 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

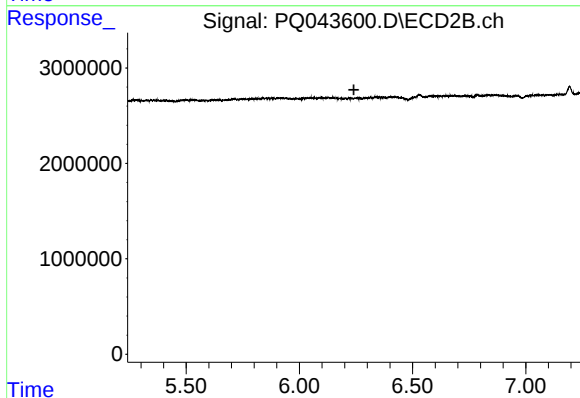


#21 AR-1248-1

R.T.: 0.000 min
Exp R.T. : 6.241 min
Response: 0
Conc: N.D.

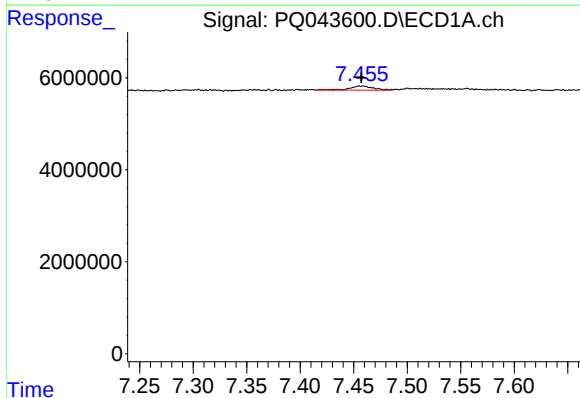


#22 AR-1248-2

R.T.: 7.457 min
Delta R.T.: 0.000 min
Response: 1445808
Conc: 15.87 ng/ml

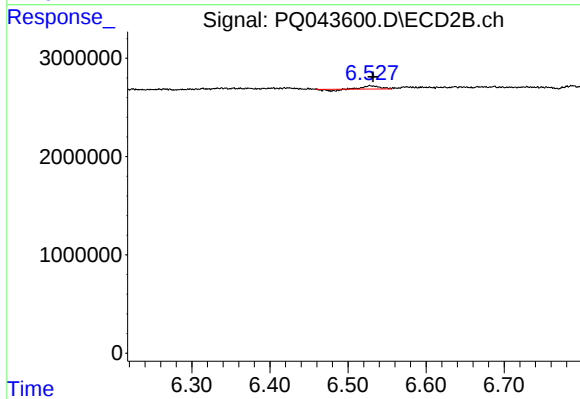

#22 AR-1248-2


R.T.: 6.528 min
Delta R.T.: -0.004 min
Response: 352910
Conc: 9.70 ng/ml

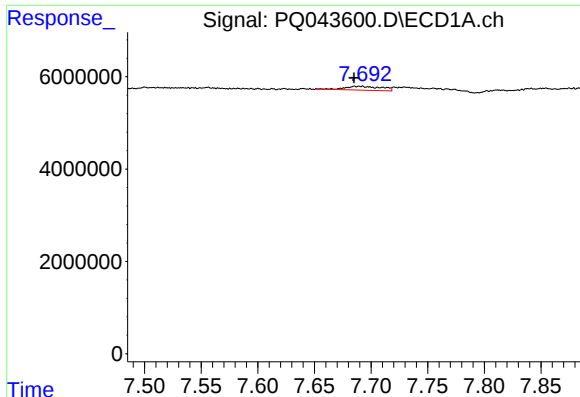

#23 AR-1248-3


R.T.: 7.689 min
Delta R.T.: 0.003 min
Response: 1867476
Conc: 18.00 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

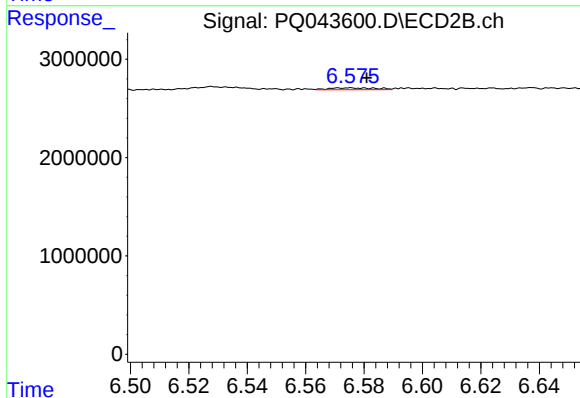


#23 AR-1248-3

R.T.: 6.575 min
Delta R.T.: -0.006 min
Response: 213630
Conc: 5.63 ng/ml

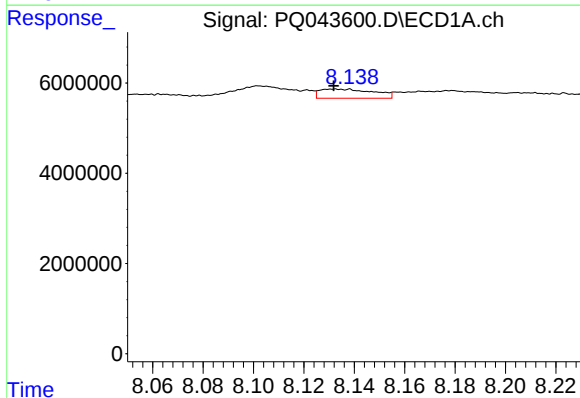


#24 AR-1248-4

R.T.: 8.133 min
Delta R.T.: 0.000 min
Response: 3021622
Conc: 22.24 ng/ml

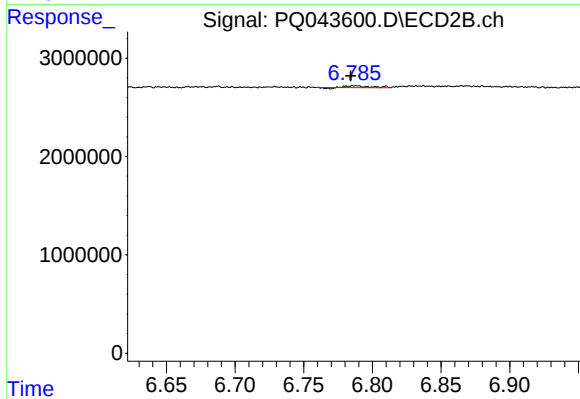

#24 AR-1248-4


R.T.: 6.787 min
Delta R.T.: 0.003 min
Response: 204496
Conc: 4.42 ng/ml

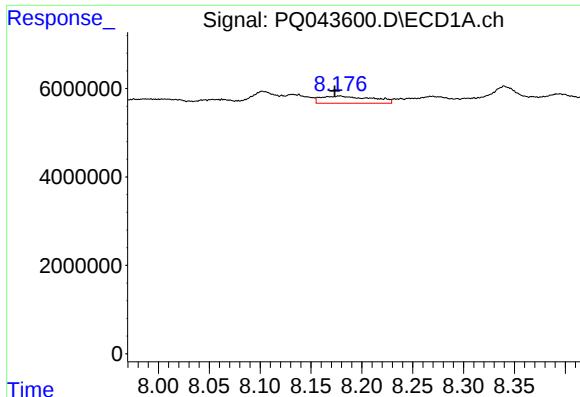

#25 AR-1248-5


R.T.: 8.178 min
Delta R.T.: 0.005 min
Response: 5618785
Conc: 42.38 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

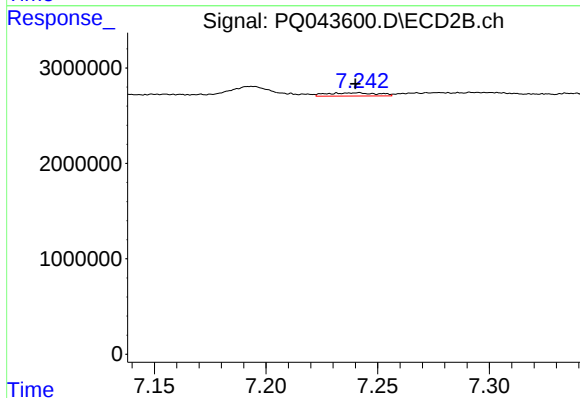


#25 AR-1248-5

R.T.: 7.240 min
Delta R.T.: 0.000 min
Response: 520939
Conc: 10.09 ng/ml

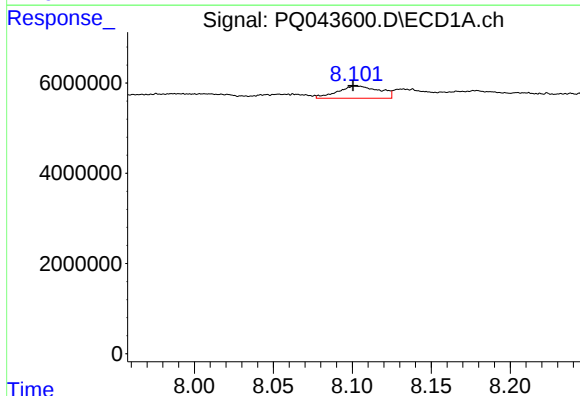


#26 AR-1254-1

R.T.: 8.103 min
Delta R.T.: 0.003 min
Response: 5018252
Conc: 34.13 ng/ml

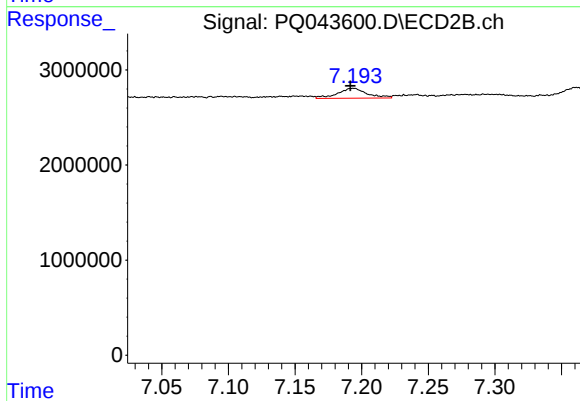

#26 AR-1254-1


R.T.: 7.193 min
Delta R.T.: 0.002 min
Response: 1600962
Conc: 17.98 ng/ml

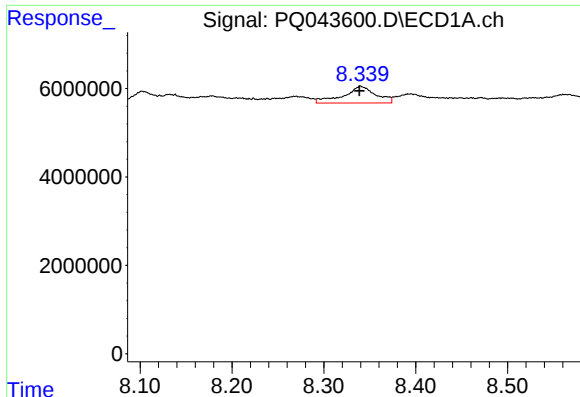

#27 AR-1254-2


R.T.: 8.340 min
Delta R.T.: 0.002 min
Response: 9287916
Conc: 37.94 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

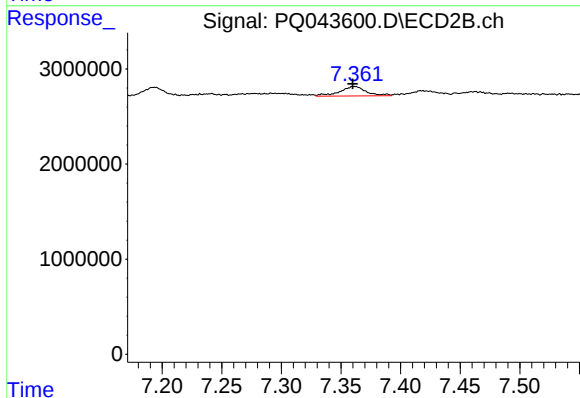


#27 AR-1254-2

R.T.: 7.361 min
Delta R.T.: 0.002 min
Response: 1542017
Conc: 18.96 ng/ml

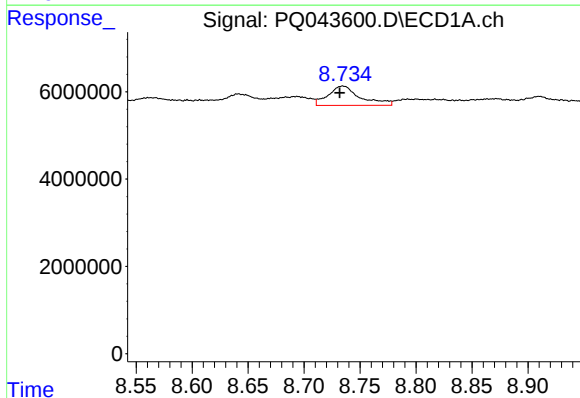


#28 AR-1254-3

R.T.: 8.735 min
Delta R.T.: 0.003 min
Response: 8836695
Conc: 30.64 ng/ml

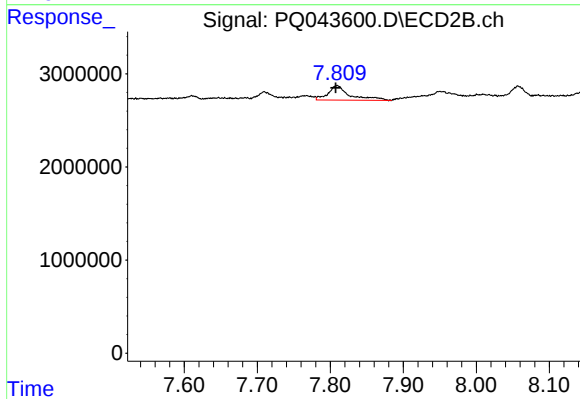

#28 AR-1254-3


R.T.: 7.809 min
Delta R.T.: 0.002 min
Response: 3289623
Conc: 23.30 ng/ml

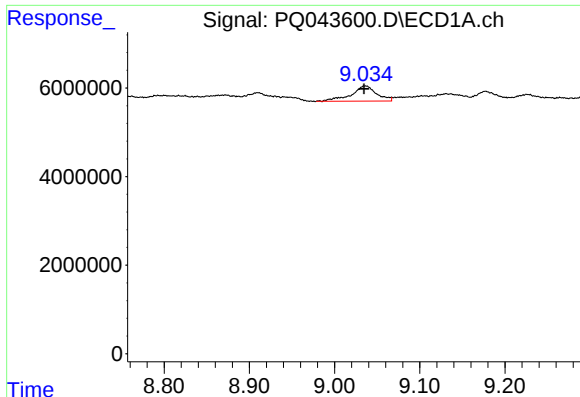

#29 AR-1254-4


R.T.: 9.036 min
Delta R.T.: 0.002 min
Response: 7106046
Conc: 30.44 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

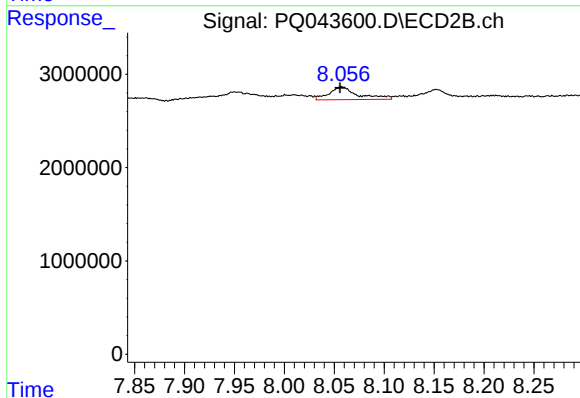


#29 AR-1254-4

R.T.: 8.057 min
Delta R.T.: 0.002 min
Response: 2793411
Conc: 28.65 ng/ml

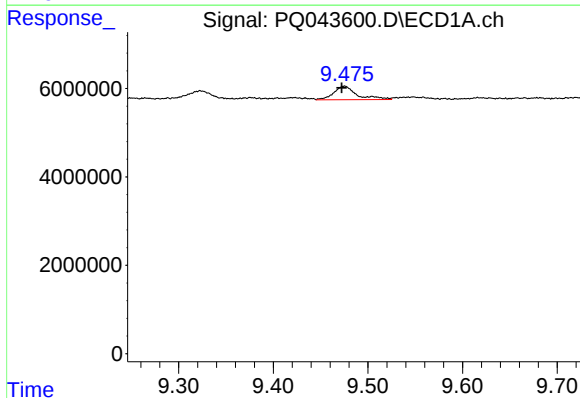


#30 AR-1254-5

R.T.: 9.475 min
Delta R.T.: 0.002 min
Response: 5253249
Conc: 19.75 ng/ml

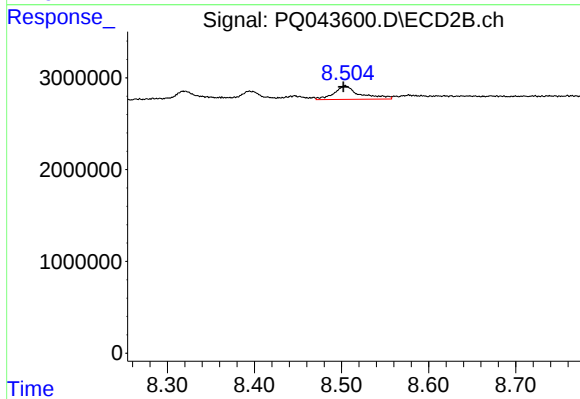

#30 AR-1254-5


R.T.: 8.504 min
Delta R.T.: 0.002 min
Response: 3028045
Conc: 21.82 ng/ml

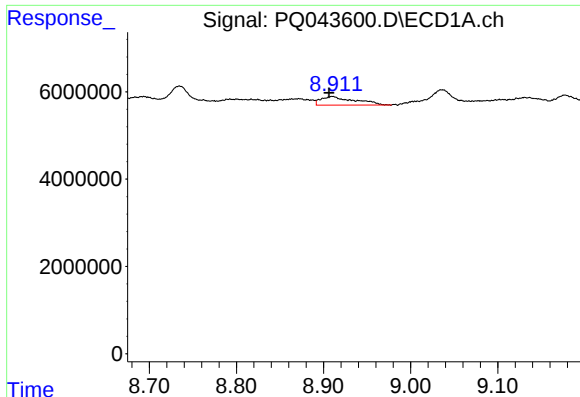

#31 AR-1260-1


R.T.: 8.910 min
Delta R.T.: 0.003 min
Response: 5296261
Conc: 28.57 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

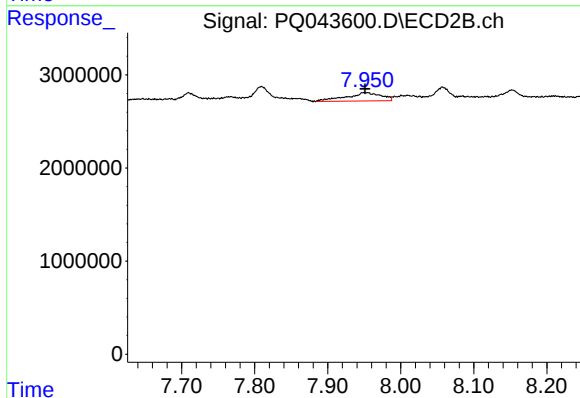


#31 AR-1260-1

R.T.: 7.951 min
Delta R.T.: 0.000 min
Response: 3055124
Conc: 37.48 ng/ml

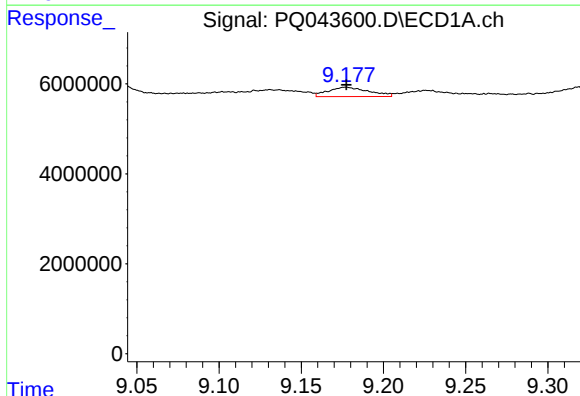


#32 AR-1260-2

R.T.: 9.177 min
Delta R.T.: 0.000 min
Response: 3580757
Conc: 15.19 ng/ml

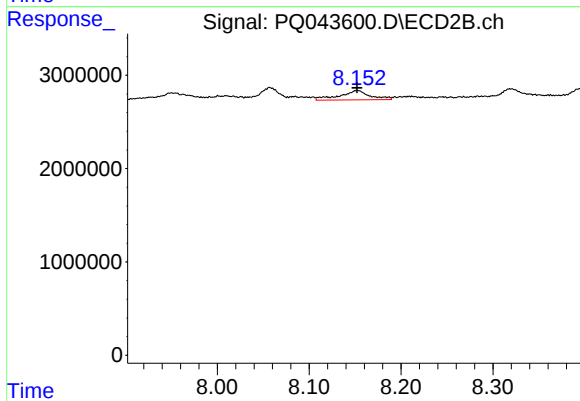

#32 AR-1260-2


R.T.: 8.152 min
Delta R.T.: 0.000 min
Response: 2335234
Conc: 22.01 ng/ml

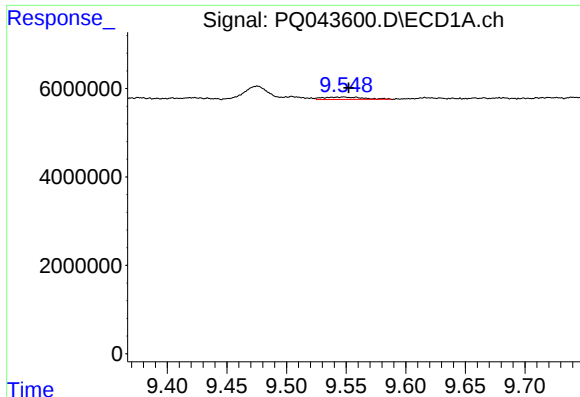

#33 AR-1260-3


R.T.: 9.547 min
Delta R.T.: -0.005 min
Response: 1236877
Conc: 6.48 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

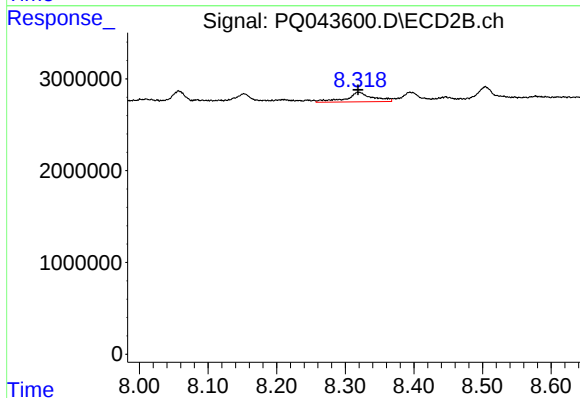


#33 AR-1260-3

R.T.: 8.320 min
Delta R.T.: 0.000 min
Response: 2833627
Conc: 29.58 ng/ml

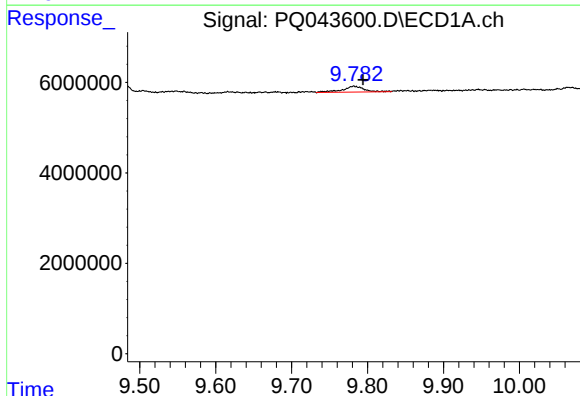


#34 AR-1260-4

R.T.: 9.782 min
Delta R.T.: -0.012 min
Response: 2589408
Conc: 11.22 ng/ml

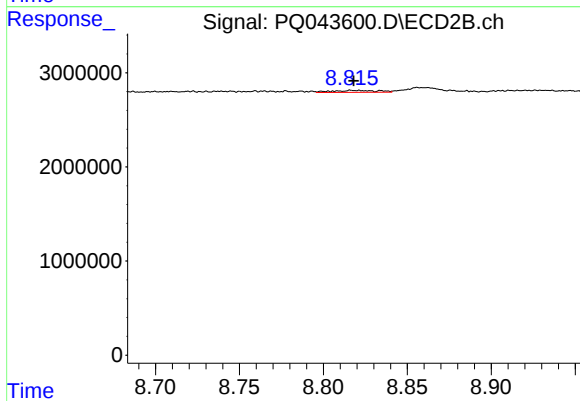

#34 AR-1260-4


R.T.: 8.819 min
Delta R.T.: 0.000 min
Response: 408267
Conc: 4.67 ng/ml

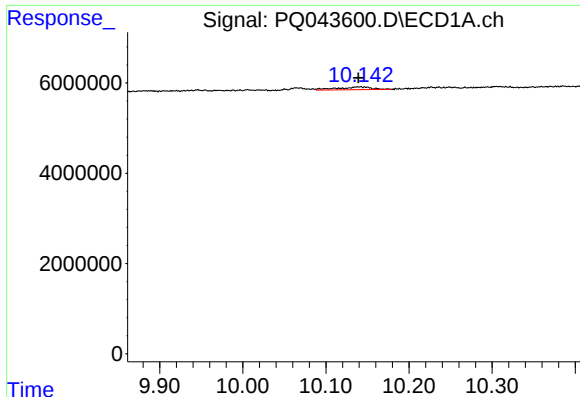

#35 AR-1260-5


R.T.: 10.140 min
Delta R.T.: 0.000 min
Response: 1705959
Conc: 3.23 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

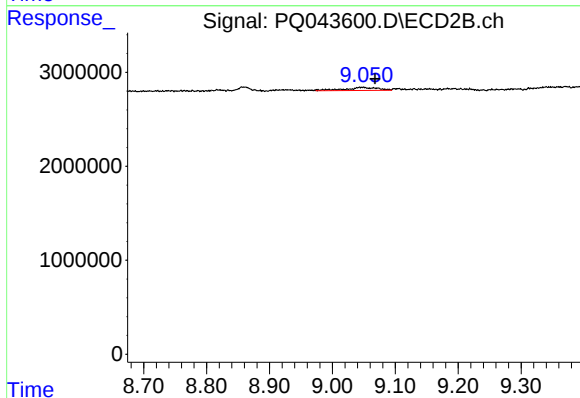


#35 AR-1260-5

R.T.: 9.047 min
Delta R.T.: -0.021 min
Response: 1234977
Conc: 5.63 ng/ml

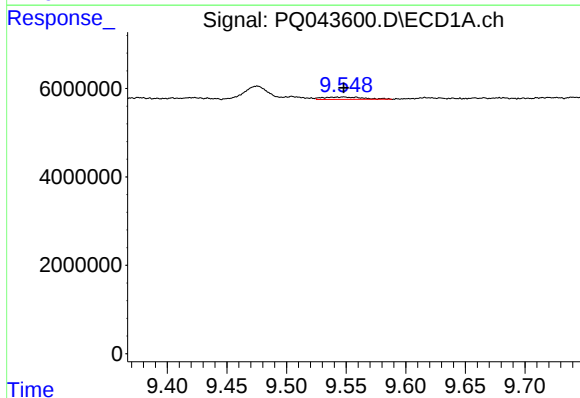


#36 AR-1262-1

R.T.: 9.547 min
Delta R.T.: 0.000 min
Response: 1236877
Conc: 3.91 ng/ml

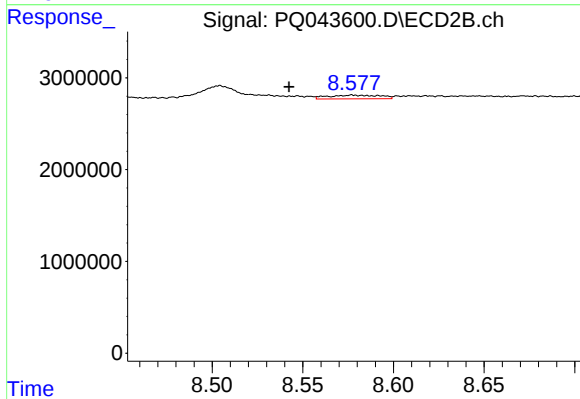

#36 AR-1262-1


R.T.: 8.578 min
Delta R.T.: 0.036 min
Response: 799473
Conc: 5.70 ng/ml

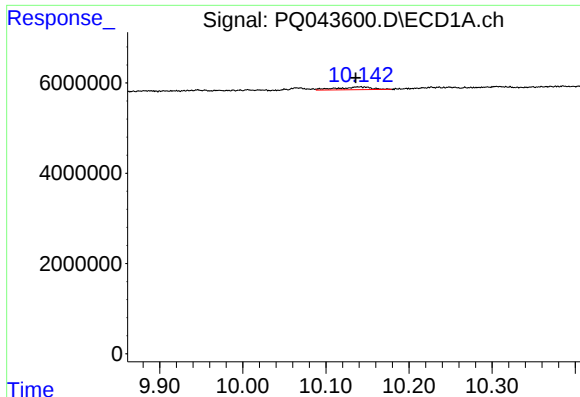

#37 AR-1262-2


R.T.: 10.140 min
Delta R.T.: 0.004 min
Response: 1705959
Conc: 2.50 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

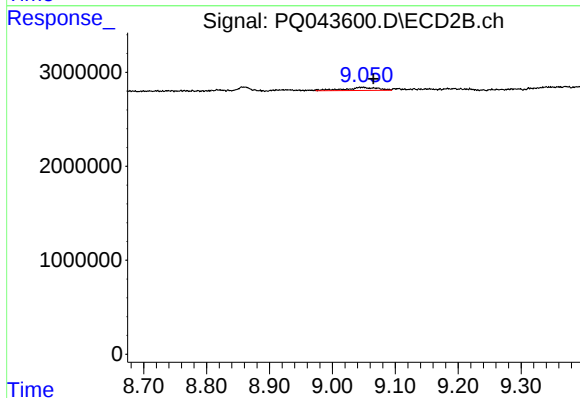


#37 AR-1262-2

R.T.: 9.047 min
Delta R.T.: -0.018 min
Response: 1234977
Conc: 4.76 ng/ml

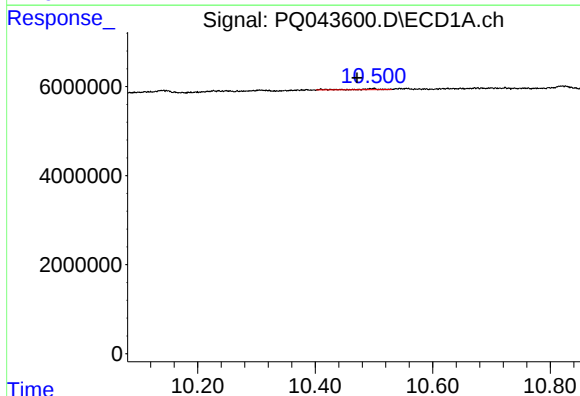


#38 AR-1262-3

R.T.: 10.499 min
Delta R.T.: 0.028 min
Response: 570411
Conc: 1.20 ng/ml

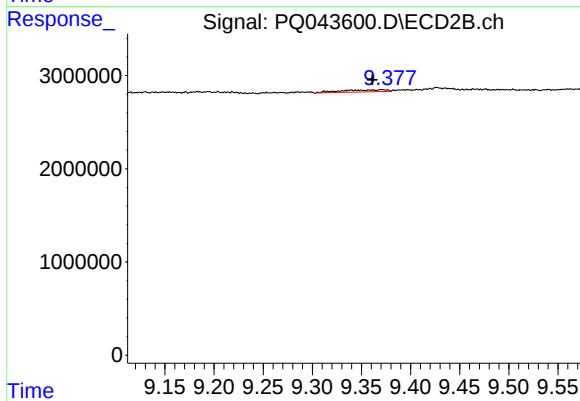

#38 AR-1262-3


R.T.: 9.372 min
Delta R.T.: 0.011 min
Response: 702335
Conc: 5.97 ng/ml

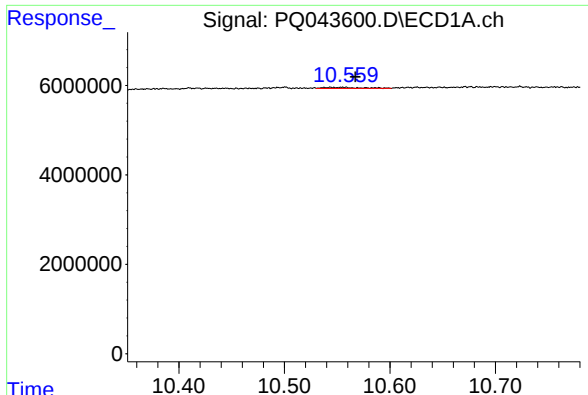

#39 AR-1262-4


R.T.: 10.555 min
Delta R.T.: -0.012 min
Response: 579421
Conc: 1.61 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

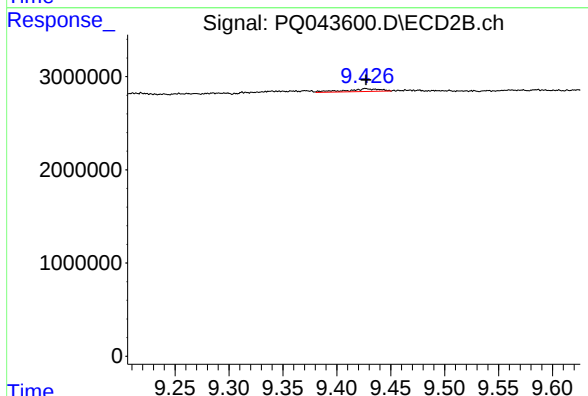


#39 AR-1262-4

R.T.: 9.427 min
Delta R.T.: 0.000 min
Response: 653570
Conc: 2.75 ng/ml

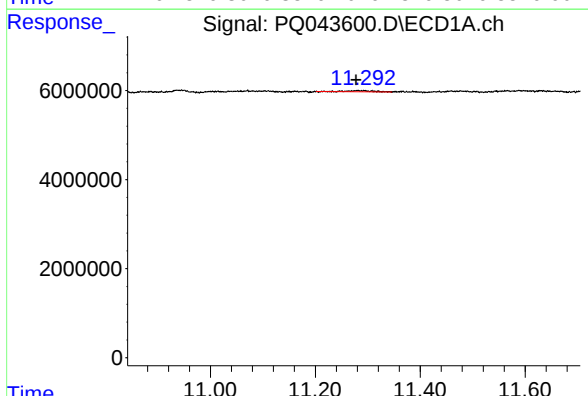


#40 AR-1262-5

R.T.: 11.280 min
Delta R.T.: 0.003 min
Response: 860156
Conc: 2.90 ng/ml

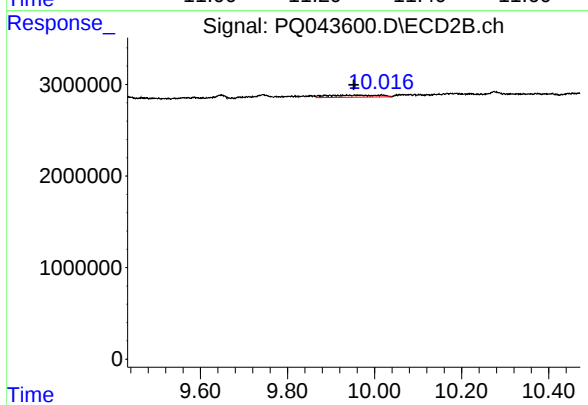

#40 AR-1262-5


R.T.: 10.016 min
Delta R.T.: 0.064 min
Response: 1890624
Conc: 12.93 ng/ml

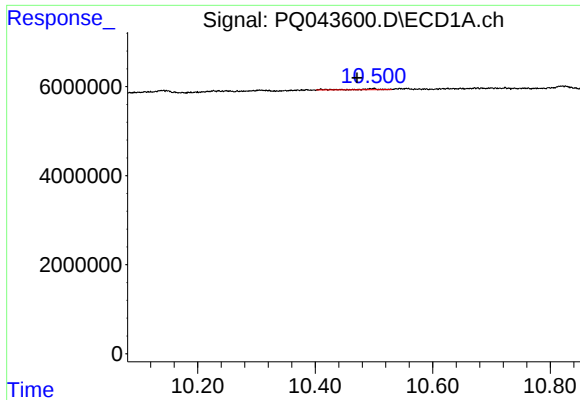

#41 AR-1268-1


R.T.: 10.499 min
Delta R.T.: 0.028 min
Response: 570411
Conc: 0.71 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

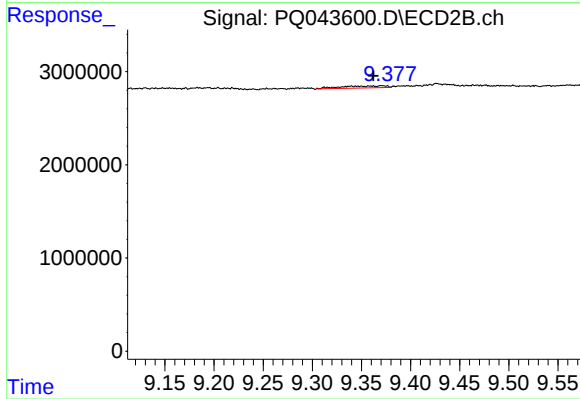


#41 AR-1268-1

R.T.: 9.372 min
Delta R.T.: 0.010 min
Response: 702335
Conc: 2.17 ng/ml

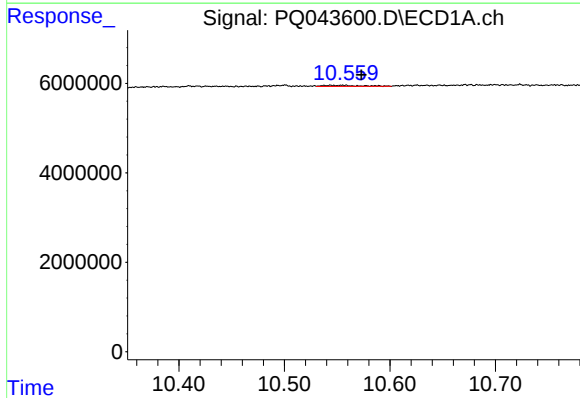


#42 AR-1268-2

R.T.: 10.555 min
Delta R.T.: -0.018 min
Response: 579421
Conc: 0.75 ng/ml

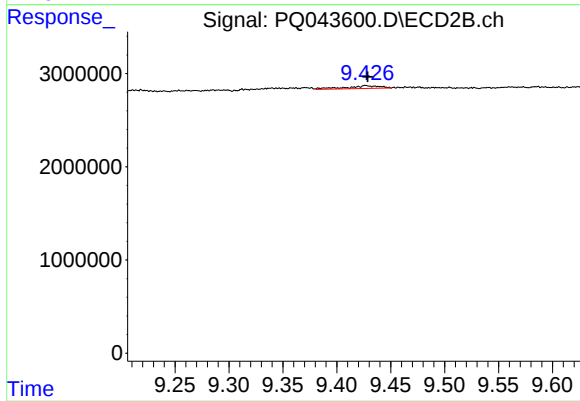

#42 AR-1268-2


R.T.: 9.427 min
Delta R.T.: -0.001 min
Response: 653570
Conc: 2.09 ng/ml

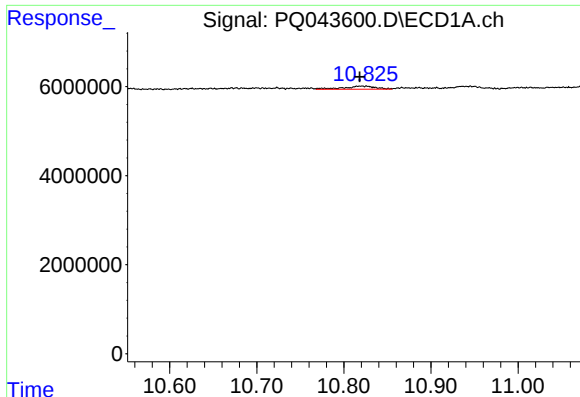

#43 AR-1268-3


R.T.: 10.821 min
Delta R.T.: 0.003 min
Response: 1707759
Conc: 2.59 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

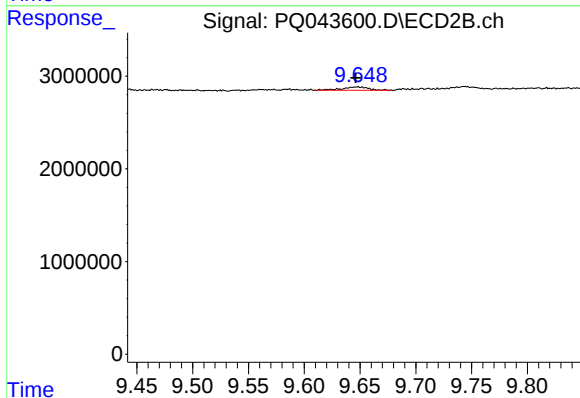


#43 AR-1268-3

R.T.: 9.648 min
Delta R.T.: 0.001 min
Response: 607710
Conc: 2.15 ng/ml

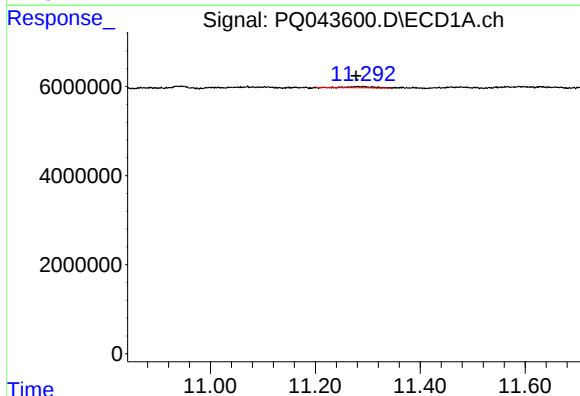


#44 AR-1268-4

R.T.: 11.280 min
Delta R.T.: 0.002 min
Response: 860156
Conc: 2.68 ng/ml

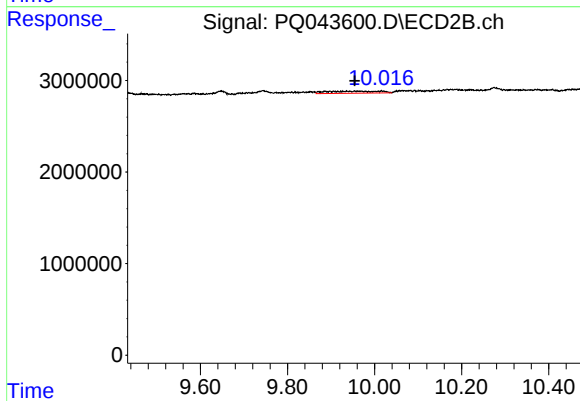

#44 AR-1268-4


R.T.: 10.016 min
Delta R.T.: 0.061 min
Response: 1890624
Conc: 11.98 ng/ml

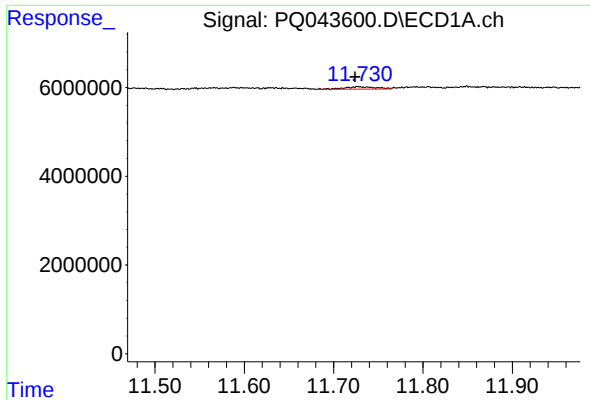

#45 AR-1268-5

R.T.: 11.728 min
Delta R.T.: 0.004 min
Response: 1338789
Conc: 0.50 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

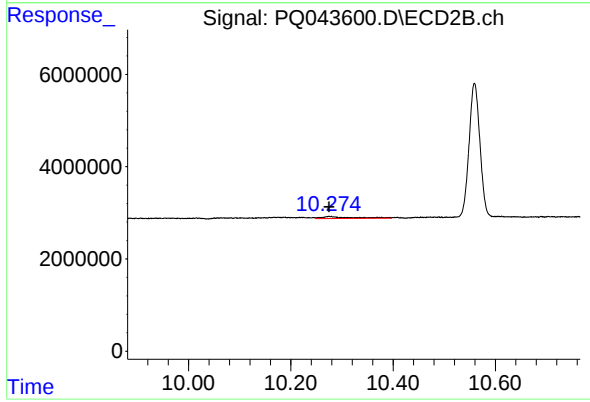

#45 AR-1268-5

R.T.: 10.275 min
Delta R.T.: 0.000 min
Response: 1779965
Conc: 1.46 ng/ml