

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ091619\
 Data File : PQ043601.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Sep 2019 20:12
 Operator : SM\AJ
 Sample : K3591-09
 Misc : AR1262 MDL 25 PPB
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 MDL-MDL-WATER-03-QT3-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 04:51:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ091219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 13 03:48:31 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.701	4.787	27836570	11852222	10.990	11.519
2)	SA Decachlor...	12.094	10.560	127.3E6	50901649	15.381	13.534
Target Compounds							
3)	L1 AR-1016-1	7.152	0.000	762578	0	7.384	N.D. #
4)	L1 AR-1016-2	7.152	6.326	762578	168514	5.200	2.876 #
5)	L1 AR-1016-3	7.243	6.501	493929	-103002	5.382	N.D. #
6)	L1 AR-1016-4	7.361	6.518	429365	135640	5.834	4.982
7)	L1 AR-1016-5	7.724	6.784	3134694	-30587	40.551	N.D. #
8)	L2 AR-1221-1	5.946	0.000	1291085	0	43.925	N.D. #
9)	L2 AR-1221-2	6.091	5.208	1289890	212367	58.937	24.539 #
10)	L2 AR-1221-3	6.166	5.301	1020895	99806	14.663	3.476 #
11)	L3 AR-1232-1	6.166	5.301	1020895	99806	10.405	2.448 #
12)	L3 AR-1232-2	6.816	6.326	2345428	168514	43.468	3.613 #
13)	L3 AR-1232-3	7.152	6.501	762578	-103002	6.691	N.D. #
14)	L3 AR-1232-4	7.361	6.576	429365	335927	7.410	14.330 #
15)	L3 AR-1232-5	7.481	6.784	529702	-30587	13.085	N.D. #
16)	L4 AR-1242-1	7.152	0.000	762578	0	8.565	N.D. #
17)	L4 AR-1242-2	7.152	6.326	762578	168514	5.953	3.355 #
18)	L4 AR-1242-3	7.243	6.501	493929	-103002	6.137	N.D. #
19)	L4 AR-1242-4	7.361	6.576	429365	335927	6.550	11.661 #
20)	L4 AR-1242-5	8.180	7.193	3257472	1235152	35.897	29.397
21)	L5 AR-1248-1	7.152	0.000	762578	0	12.224	N.D. #
22)	L5 AR-1248-2	7.481	6.518	529702	135640	5.813	3.729 #
23)	L5 AR-1248-3	7.724	6.576	3134694	335927	30.216	8.860 #
24)	L5 AR-1248-4	8.140	6.784	2805291	-30587	20.649	N.D. #
25)	L5 AR-1248-5	8.180	7.193	3257472	1235152	24.571	23.921
26)	L6 AR-1254-1	8.103	7.193	2979522	1235152	20.267	13.873 #
27)	L6 AR-1254-2	8.341	7.360	4350304	1661008	17.772	20.428
28)	L6 AR-1254-3	8.735	7.826	4290735	3540471	14.879	25.072 #
29)	L6 AR-1254-4	9.037	8.031	4353886	1675131	18.649	17.179
30)	L6 AR-1254-5	9.472	8.504	5092047	2004829	19.147	14.449
31)	L7 AR-1260-1	8.907	7.951	7445570	2742318	40.165	33.644
32)	L7 AR-1260-2	9.178	8.153	5989271	2173393	25.412	20.484
33)	L7 AR-1260-3	9.553	8.322	6038313	5432777	31.653	56.710 #
34)	L7 AR-1260-4	9.796	8.818	6591487	2517315	28.550	28.770
35)	L7 AR-1260-5	10.141	9.069	13752716	5497935	26.001	25.082
36)	L8 AR-1262-1	9.553	8.545	6038313	2963008	19.103	21.115
37)	L8 AR-1262-2	10.141	9.069	13752716	5497935	20.141	21.185
38)	L8 AR-1262-3	10.477	9.364	8907563	3124495	18.798	26.566 #
39)	L8 AR-1262-4	10.574	9.430	6847005	5343168	19.000	22.520
40)	L8 AR-1262-5	11.282	9.956	6456869	3675591	21.736	25.145
41)	L9 AR-1268-1	10.477	9.364	8907563	3124495	11.095	9.633

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ091619\
 Data File : PQ043601.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Sep 2019 20:12
 Operator : SM\AJ
 Sample : K3591-09
 Misc : AR1262 MDL 25 PPB
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 MDL-MDL-WATER-03-QT3-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 04:51:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ091219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 13 03:48:31 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	10.574	9.430	6847005	5343168	8.885	17.065 #
43) L9	AR-1268-3	10.824	9.648	1263974	982318	1.917	3.475 #
44) L9	AR-1268-4	11.282	9.956	6456869	3675591	20.111	23.287
45) L9	AR-1268-5	11.727	10.277	3169846	2121580	1.192	1.742 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ091619\
Data File : PQ043601.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Sep 2019 20:12
Operator : SM\AJ
Sample : K3591-09
Misc : AR1262 MDL 25 PPB
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 04:51:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ091219.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 13 03:48:31 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

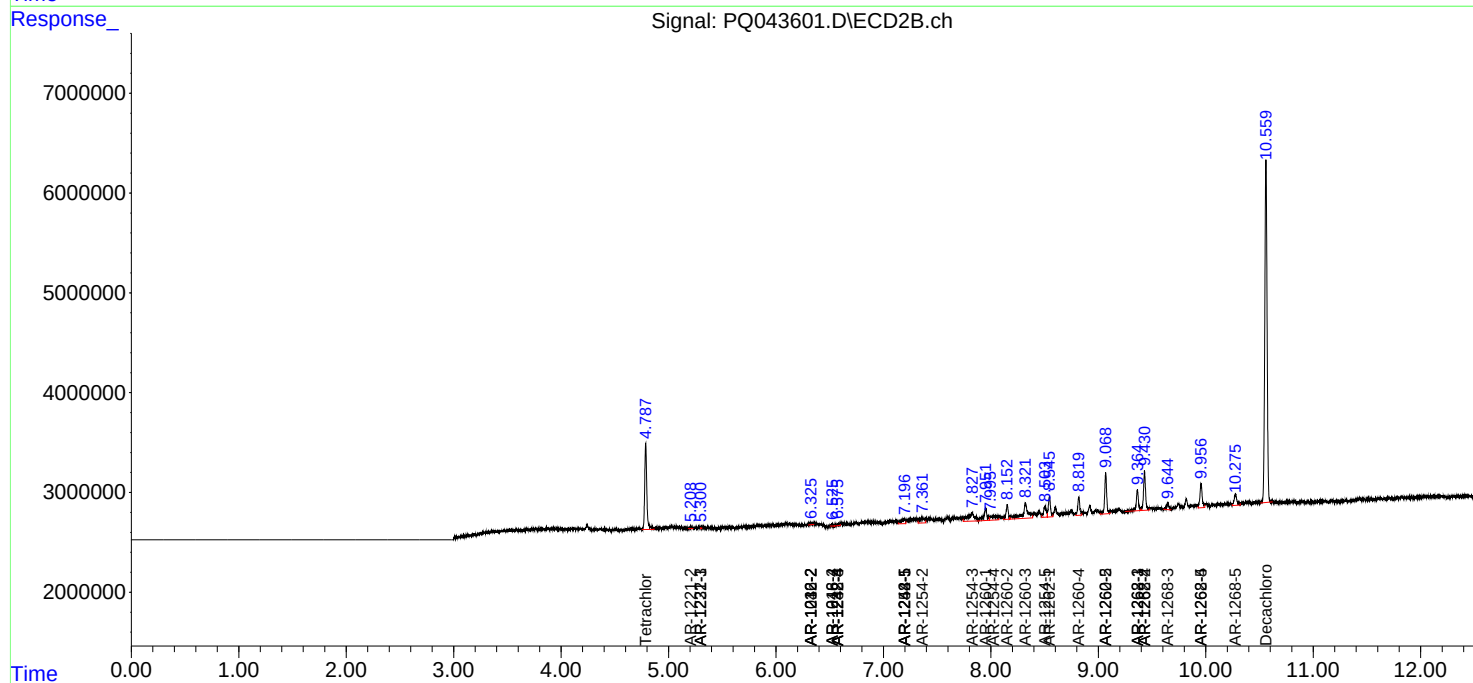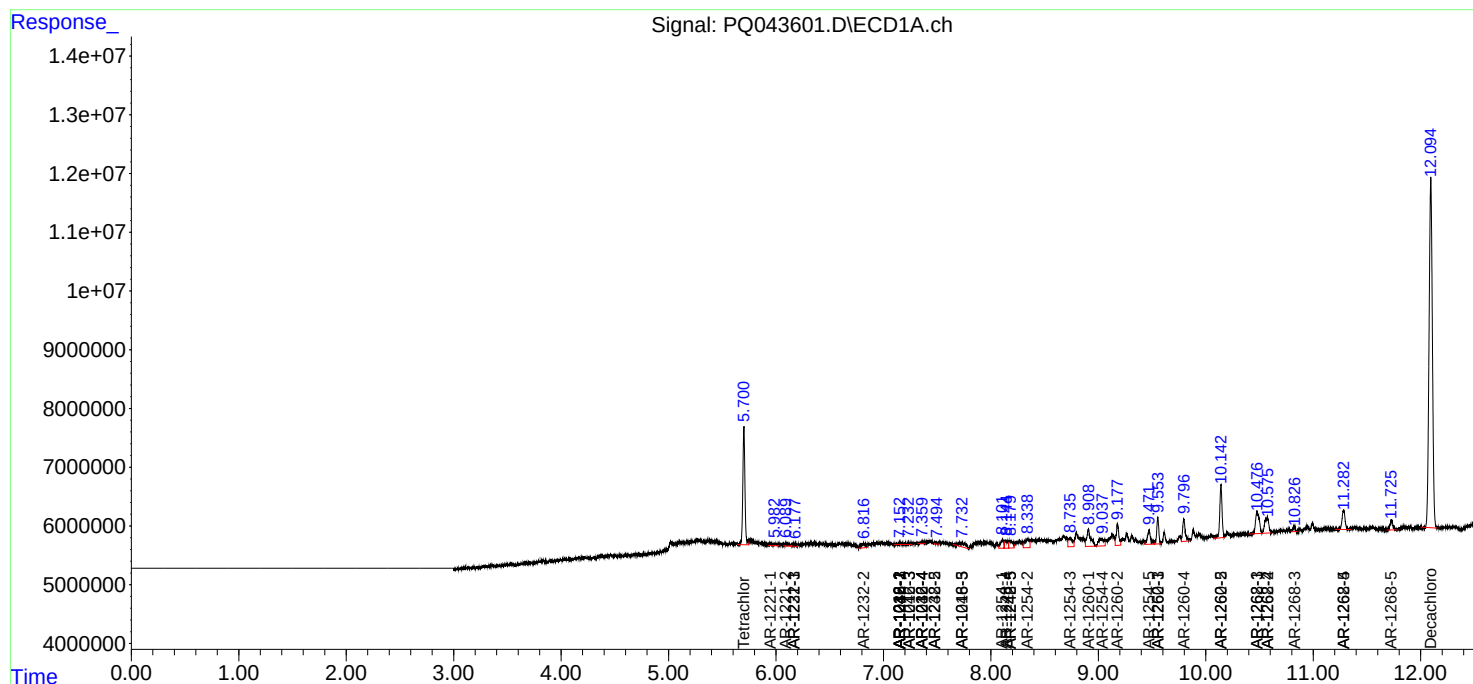


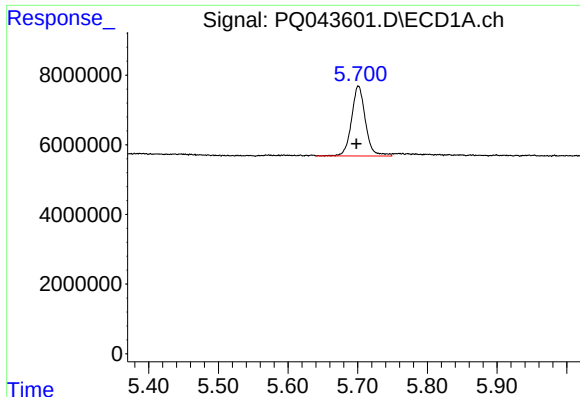

#1 Tetrachloro-m-xylene


R.T.: 5.701 min
Delta R.T.: 0.003 min
Response: 27836570
Conc: 10.99 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

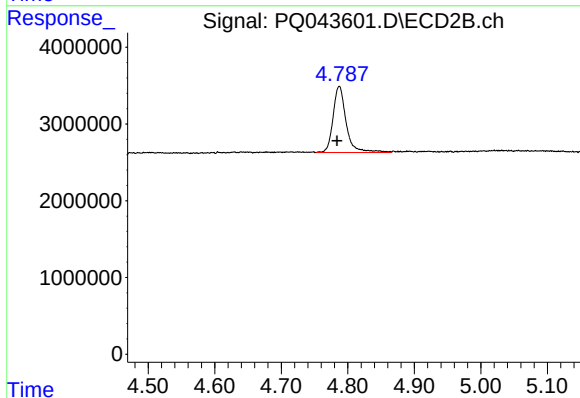


#1 Tetrachloro-m-xylene

R.T.: 4.787 min
Delta R.T.: 0.004 min
Response: 11852222
Conc: 11.52 ng/ml

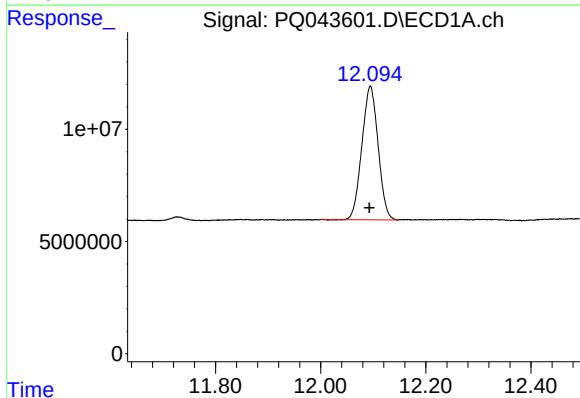


#2 Decachlorobiphenyl

R.T.: 12.094 min
Delta R.T.: 0.002 min
Response: 127349134
Conc: 15.38 ng/ml

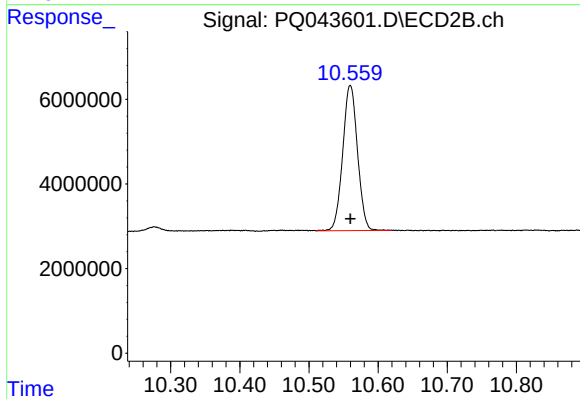

#2 Decachlorobiphenyl


R.T.: 10.560 min
Delta R.T.: 0.000 min
Response: 50901649
Conc: 13.53 ng/ml

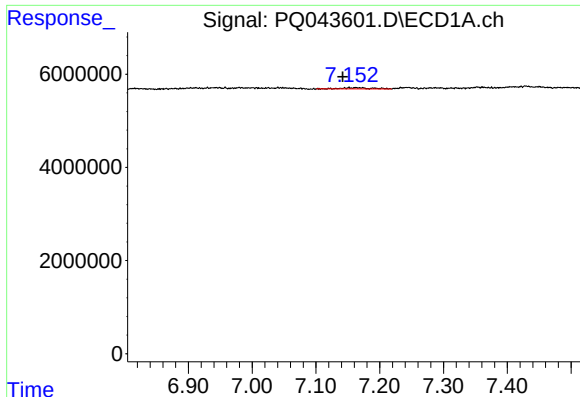

#3 AR-1016-1


R.T.: 7.152 min
Delta R.T.: 0.010 min
Response: 762578
Conc: 7.38 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

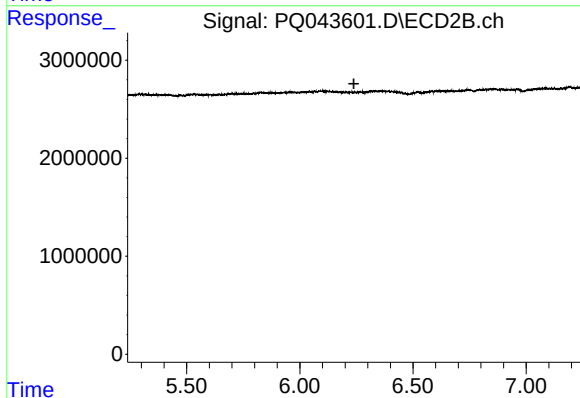


#3 AR-1016-1

R.T.: 0.000 min
Exp R.T. : 6.239 min
Response: 0
Conc: N.D.

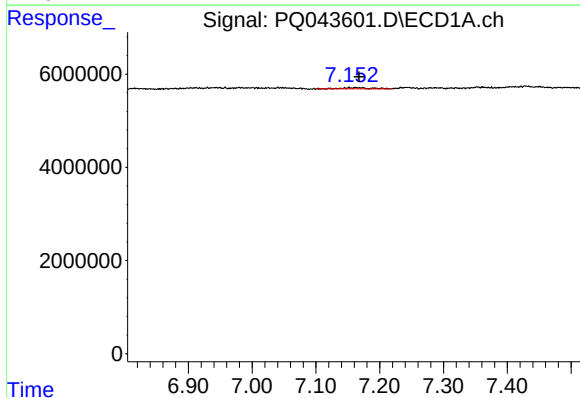


#4 AR-1016-2

R.T.: 7.152 min
Delta R.T.: -0.015 min
Response: 762578
Conc: 5.20 ng/ml

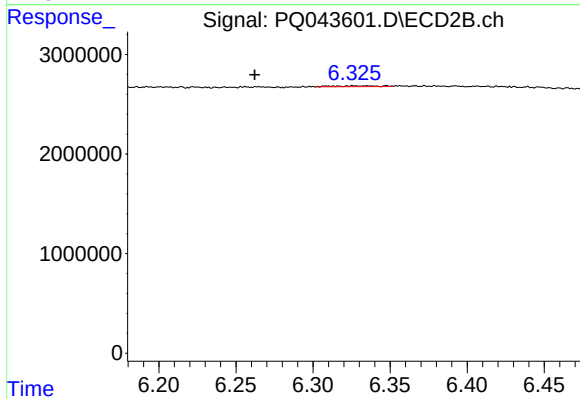

#4 AR-1016-2


R.T.: 6.326 min
Delta R.T.: 0.064 min
Response: 168514
Conc: 2.88 ng/ml

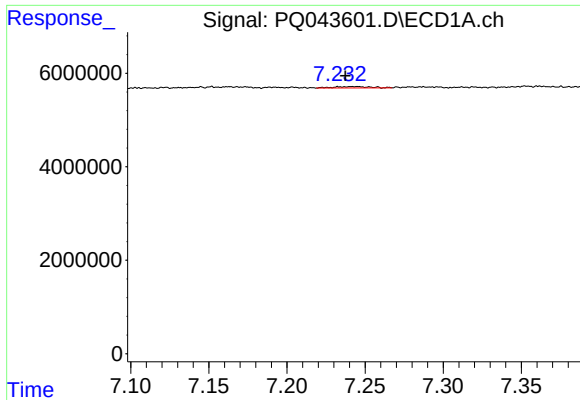

#5 AR-1016-3


R.T.: 7.243 min
Delta R.T.: 0.006 min
Response: 493929
Conc: 5.38 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

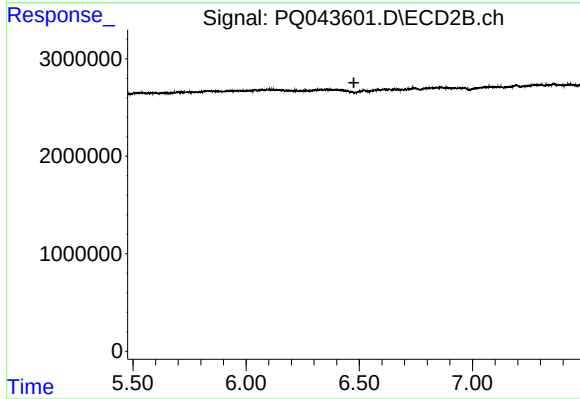


#5 AR-1016-3

R.T.: 6.501 min
Delta R.T.: 0.024 min
Response: -103002
Conc: N.D.

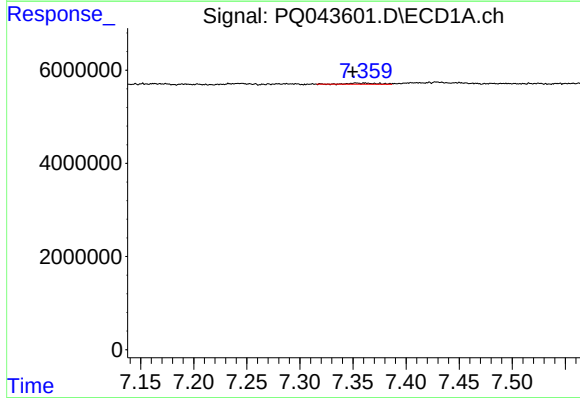


#6 AR-1016-4

R.T.: 7.361 min
Delta R.T.: 0.011 min
Response: 429365
Conc: 5.83 ng/ml

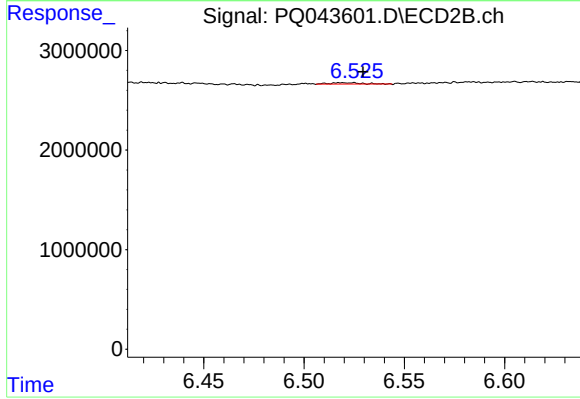

#6 AR-1016-4


R.T.: 6.518 min
Delta R.T.: -0.012 min
Response: 135640
Conc: 4.98 ng/ml

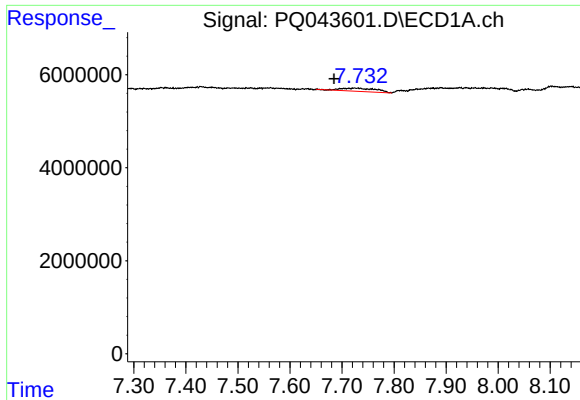

#7 AR-1016-5


R.T.: 7.724 min
Delta R.T.: 0.039 min
Response: 3134694
Conc: 40.55 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

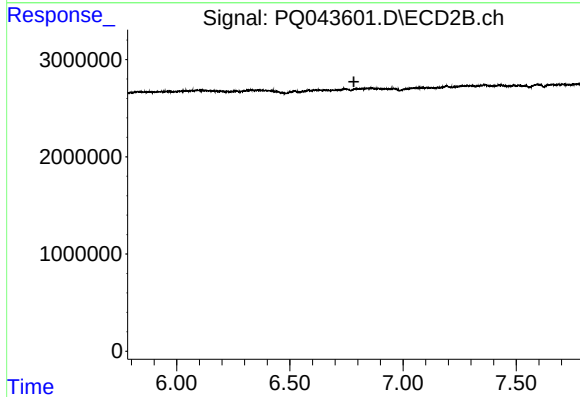


#7 AR-1016-5

R.T.: 6.784 min
Delta R.T.: 0.001 min
Response: -30587
Conc: N.D.

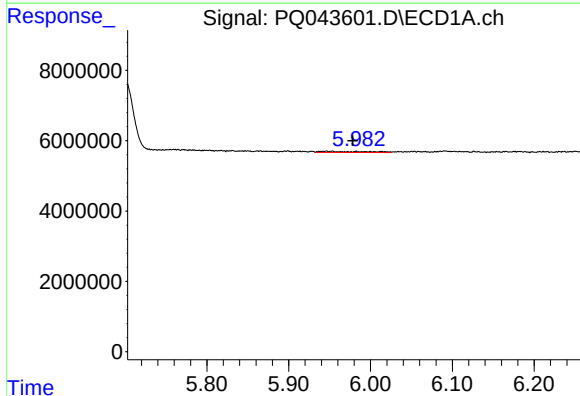


#8 AR-1221-1

R.T.: 5.946 min
Delta R.T.: -0.032 min
Response: 1291085
Conc: 43.92 ng/ml

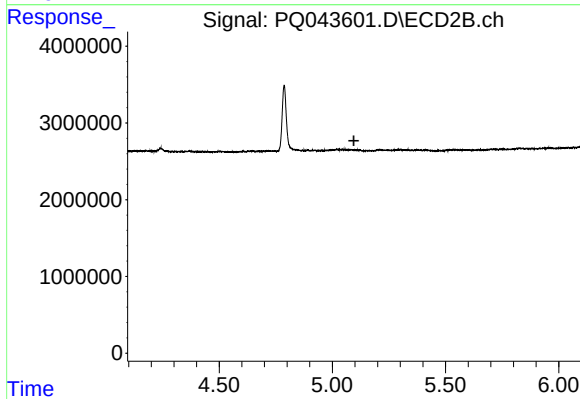

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T.: 5.095 min
Response: 0
Conc: N.D.

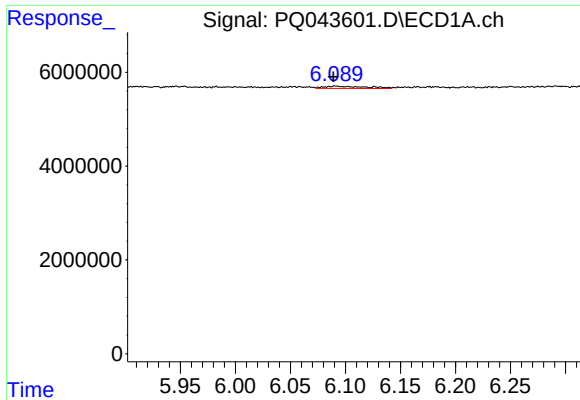

#9 AR-1221-2


R.T.: 6.091 min
Delta R.T.: 0.002 min
Response: 1289890
Conc: 58.94 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

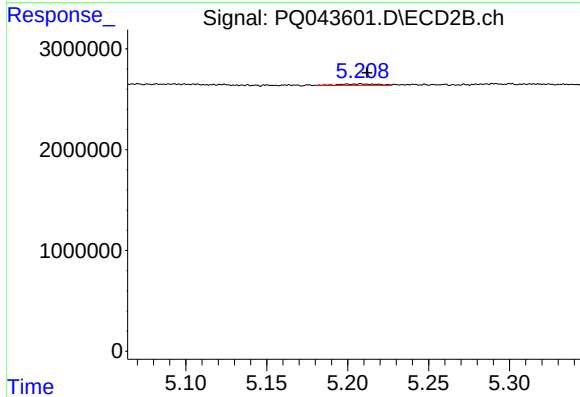


#9 AR-1221-2

R.T.: 5.208 min
Delta R.T.: -0.004 min
Response: 212367
Conc: 24.54 ng/ml

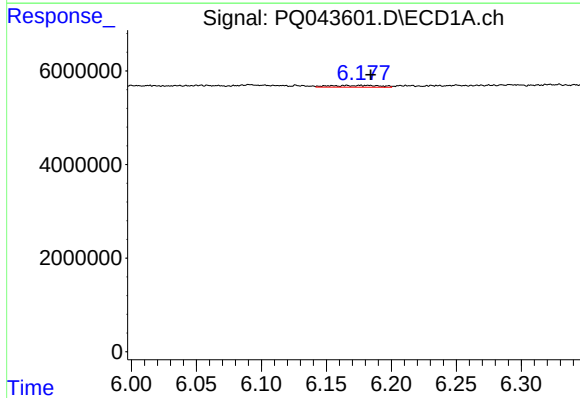


#10 AR-1221-3

R.T.: 6.166 min
Delta R.T.: -0.019 min
Response: 1020895
Conc: 14.66 ng/ml

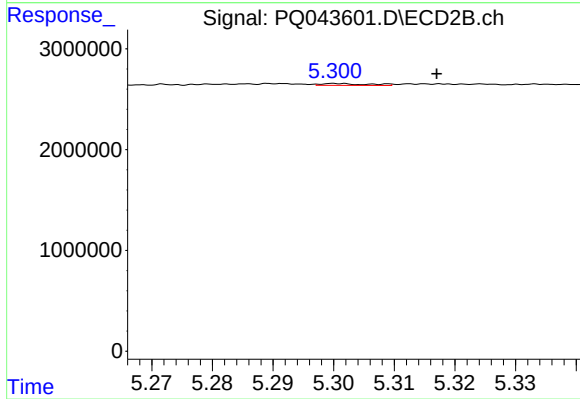

#10 AR-1221-3


R.T.: 5.301 min
Delta R.T.: -0.016 min
Response: 99806
Conc: 3.48 ng/ml

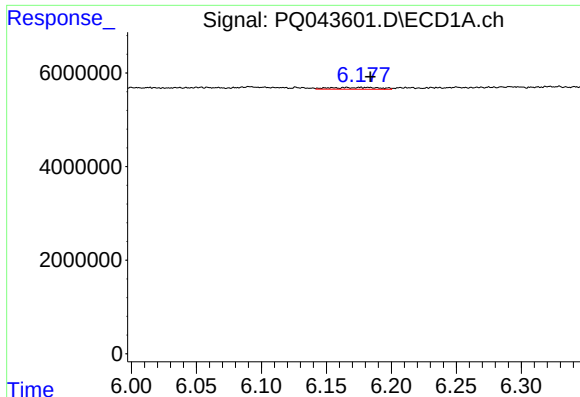

#11 AR-1232-1


R.T.: 6.166 min
Delta R.T.: -0.018 min
Response: 1020895
Conc: 10.40 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

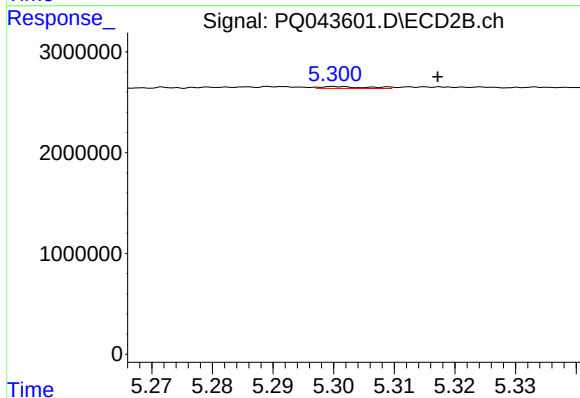


#11 AR-1232-1

R.T.: 5.301 min
Delta R.T.: -0.016 min
Response: 99806
Conc: 2.45 ng/ml

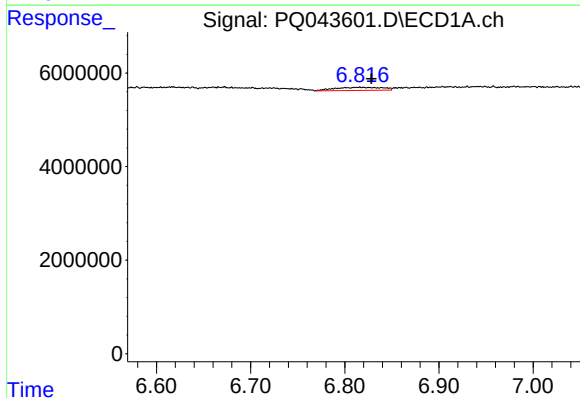


#12 AR-1232-2

R.T.: 6.816 min
Delta R.T.: -0.012 min
Response: 2345428
Conc: 43.47 ng/ml

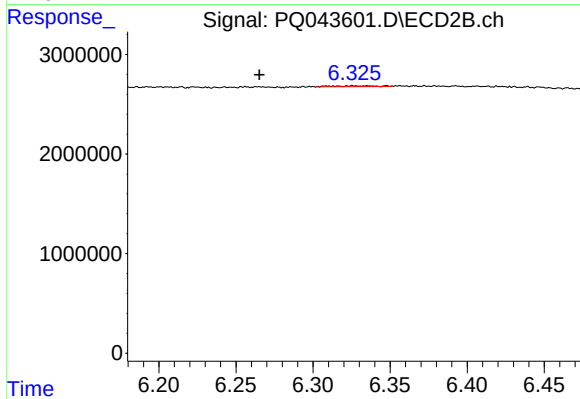

#12 AR-1232-2


R.T.: 6.326 min
Delta R.T.: 0.061 min
Response: 168514
Conc: 3.61 ng/ml

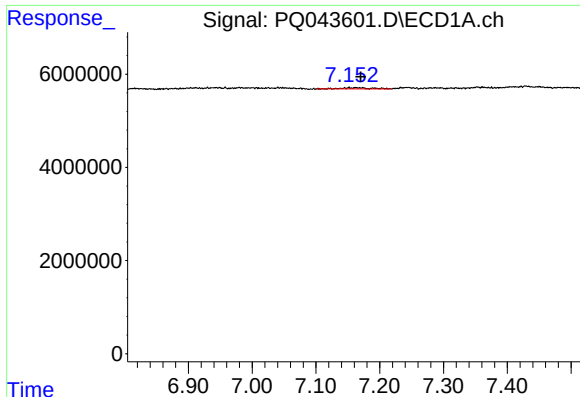

#13 AR-1232-3


R.T.: 7.152 min
Delta R.T.: -0.018 min
Response: 762578
Conc: 6.69 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

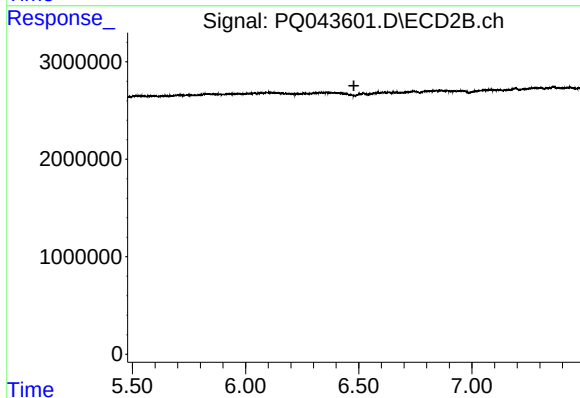


#13 AR-1232-3

R.T.: 6.501 min
Delta R.T.: 0.022 min
Response: -103002
Conc: N.D.

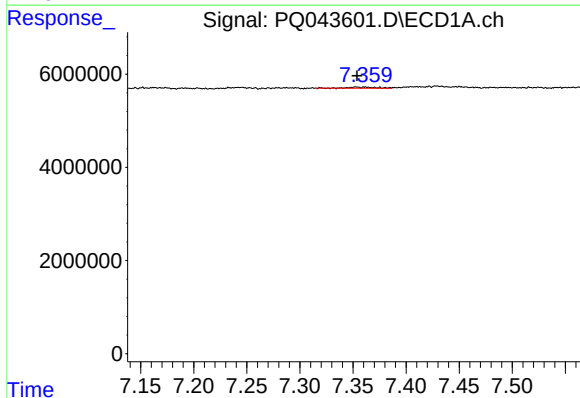


#14 AR-1232-4

R.T.: 7.361 min
Delta R.T.: 0.007 min
Response: 429365
Conc: 7.41 ng/ml

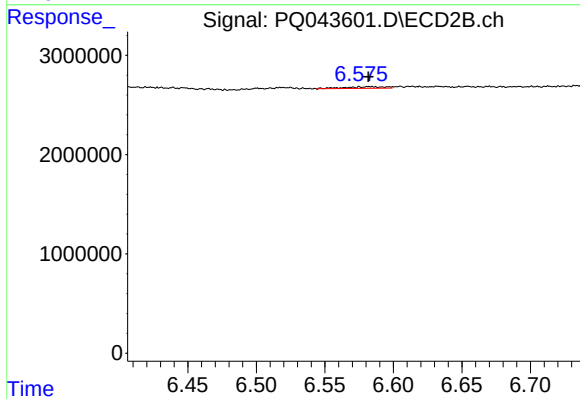

#14 AR-1232-4


R.T.: 6.576 min
Delta R.T.: -0.006 min
Response: 335927
Conc: 14.33 ng/ml

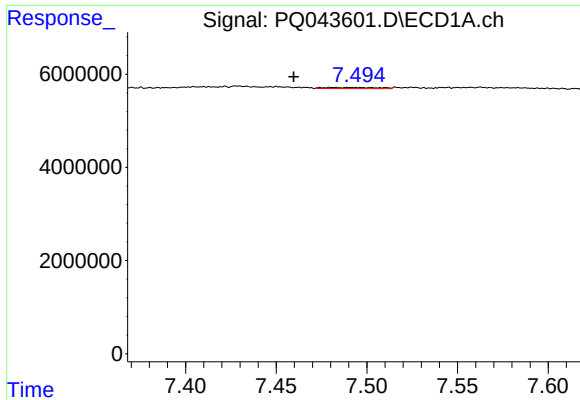

#15 AR-1232-5


R.T.: 7.481 min
Delta R.T.: 0.021 min
Response: 529702
Conc: 13.09 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

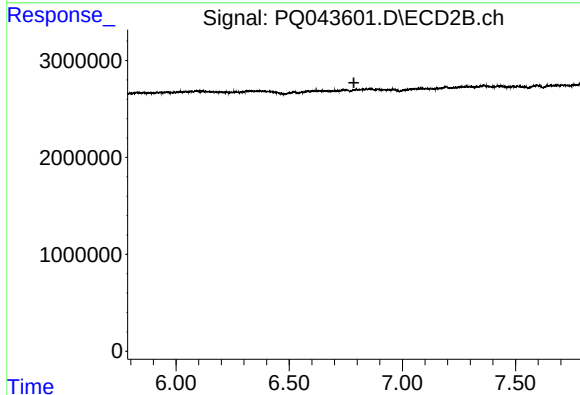


#15 AR-1232-5

R.T.: 6.784 min
Delta R.T.: -0.002 min
Response: -30587
Conc: N.D.

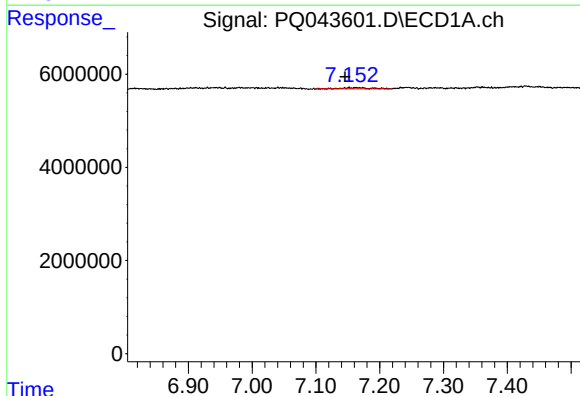


#16 AR-1242-1

R.T.: 7.152 min
Delta R.T.: 0.006 min
Response: 762578
Conc: 8.56 ng/ml

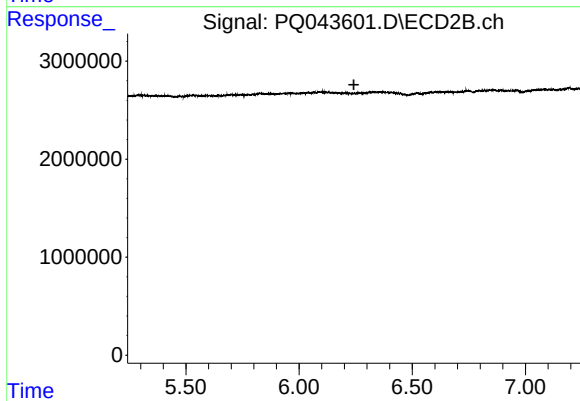

#16 AR-1242-1


R.T.: 0.000 min
Exp R.T.: 6.242 min
Response: 0
Conc: N.D.

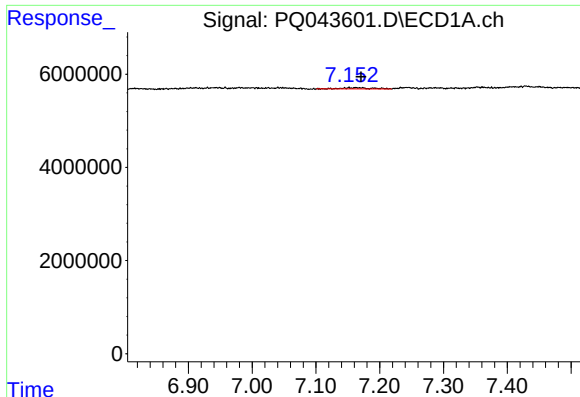

#17 AR-1242-2


R.T.: 7.152 min
Delta R.T.: -0.019 min
Response: 762578
Conc: 5.95 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

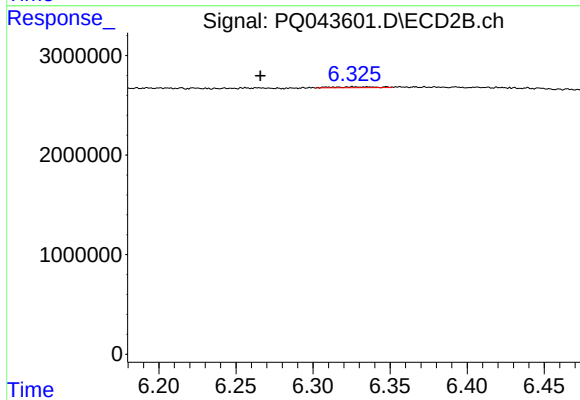


#17 AR-1242-2

R.T.: 6.326 min
Delta R.T.: 0.060 min
Response: 168514
Conc: 3.36 ng/ml

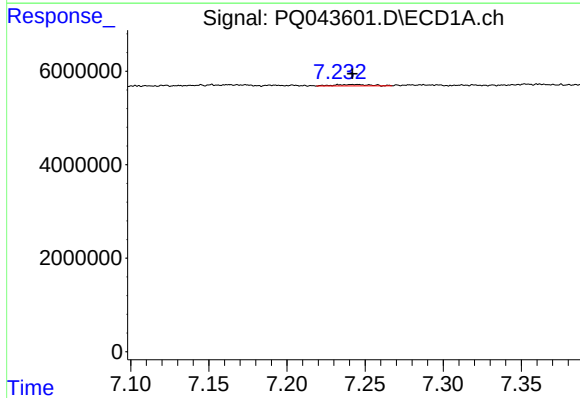


#18 AR-1242-3

R.T.: 7.243 min
Delta R.T.: 0.001 min
Response: 493929
Conc: 6.14 ng/ml

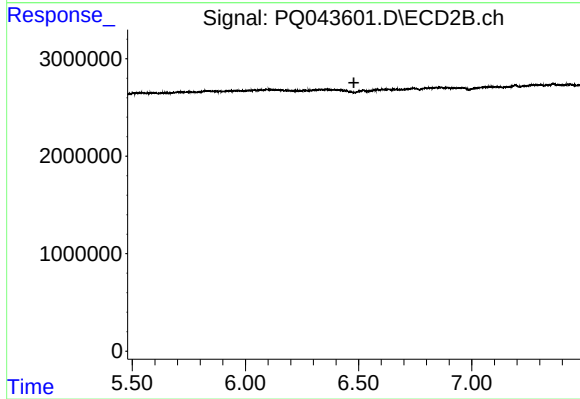

#18 AR-1242-3


R.T.: 6.501 min
Delta R.T.: 0.021 min
Response: -103002
Conc: N.D.

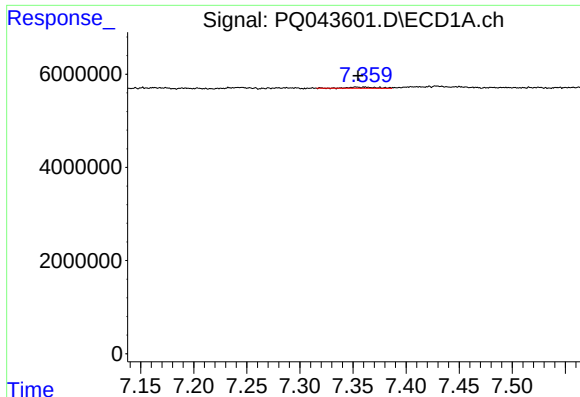

#19 AR-1242-4


R.T.: 7.361 min
Delta R.T.: 0.006 min
Response: 429365
Conc: 6.55 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

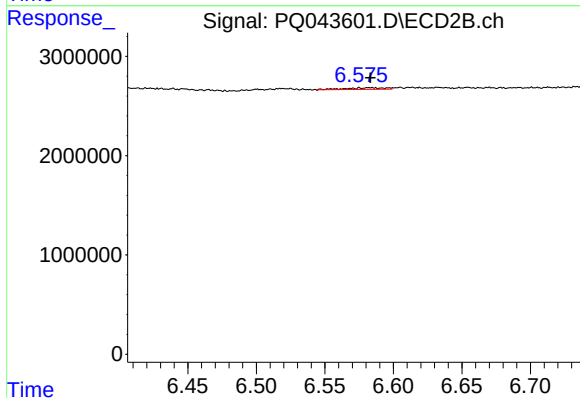


#19 AR-1242-4

R.T.: 6.576 min
Delta R.T.: -0.007 min
Response: 335927
Conc: 11.66 ng/ml

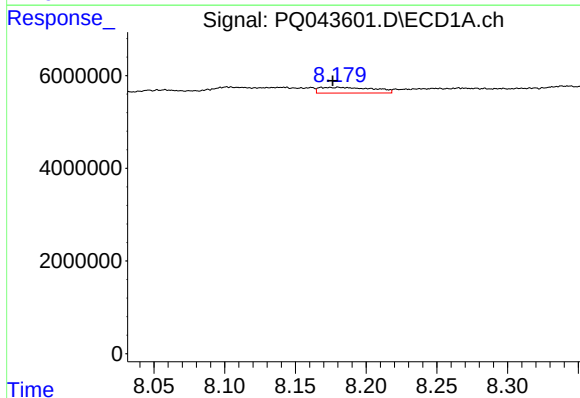


#20 AR-1242-5

R.T.: 8.180 min
Delta R.T.: 0.004 min
Response: 3257472
Conc: 35.90 ng/ml

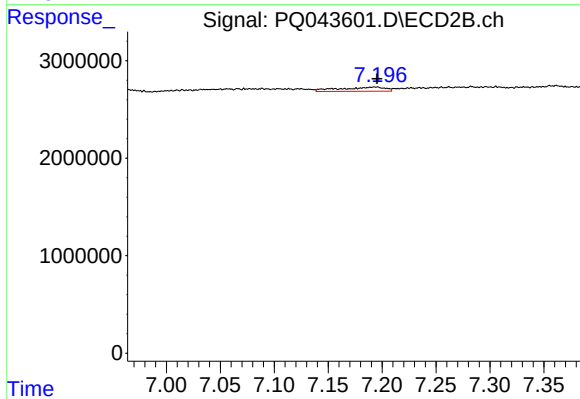

#20 AR-1242-5


R.T.: 7.193 min
Delta R.T.: -0.002 min
Response: 1235152
Conc: 29.40 ng/ml

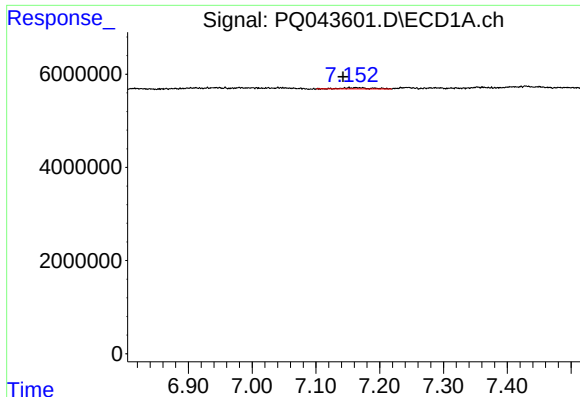

#21 AR-1248-1


R.T.: 7.152 min
Delta R.T.: 0.010 min
Response: 762578
Conc: 12.22 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

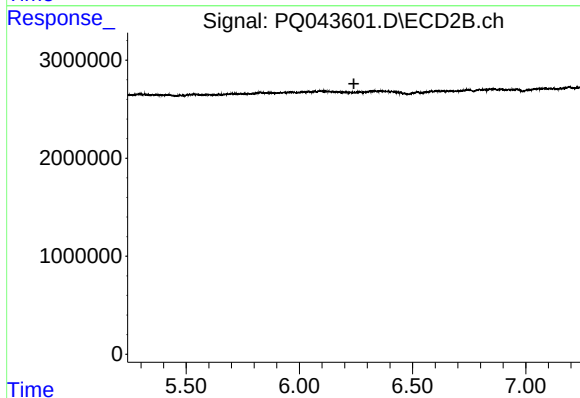


#21 AR-1248-1

R.T.: 0.000 min
Exp R.T. : 6.241 min
Response: 0
Conc: N.D.

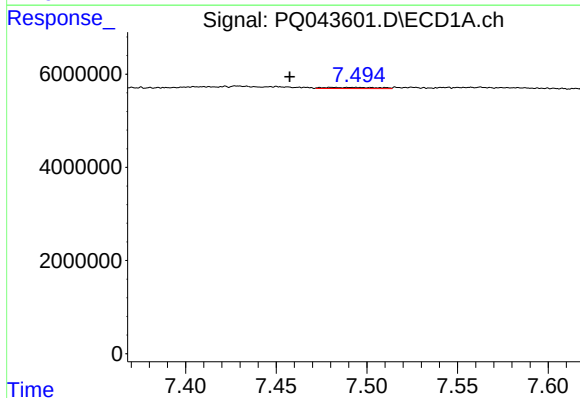


#22 AR-1248-2

R.T.: 7.481 min
Delta R.T.: 0.024 min
Response: 529702
Conc: 5.81 ng/ml

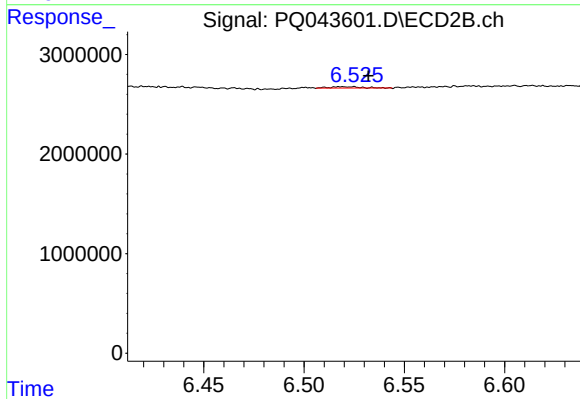

#22 AR-1248-2


R.T.: 6.518 min
Delta R.T.: -0.014 min
Response: 135640
Conc: 3.73 ng/ml

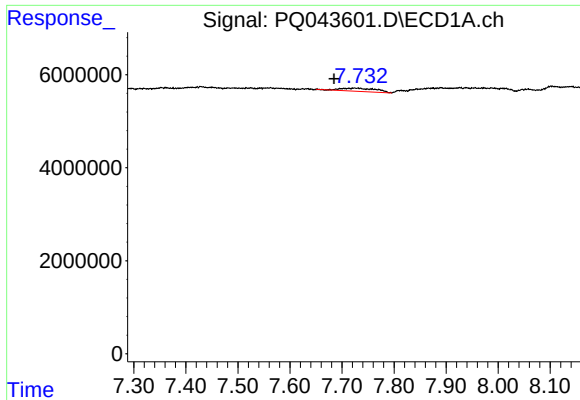

#23 AR-1248-3


R.T.: 7.724 min
Delta R.T.: 0.039 min
Response: 3134694
Conc: 30.22 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

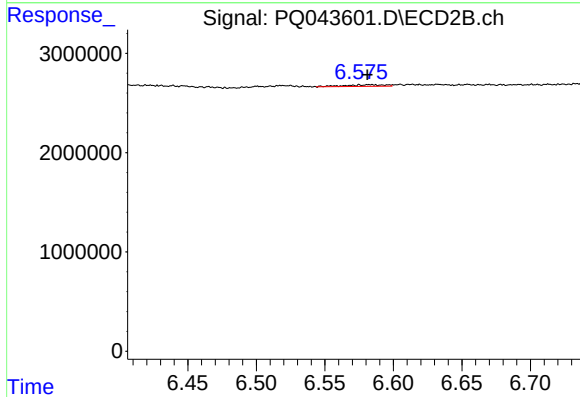


#23 AR-1248-3

R.T.: 6.576 min
Delta R.T.: -0.005 min
Response: 335927
Conc: 8.86 ng/ml

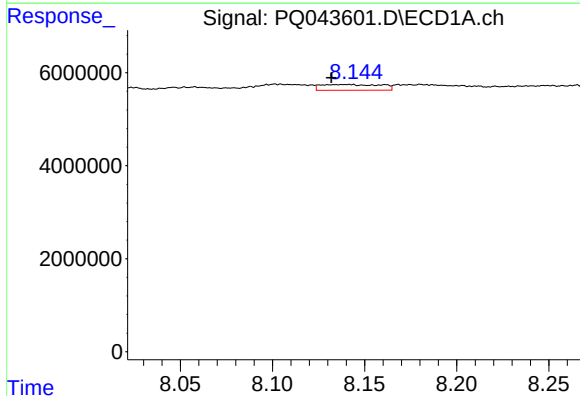


#24 AR-1248-4

R.T.: 8.140 min
Delta R.T.: 0.008 min
Response: 2805291
Conc: 20.65 ng/ml

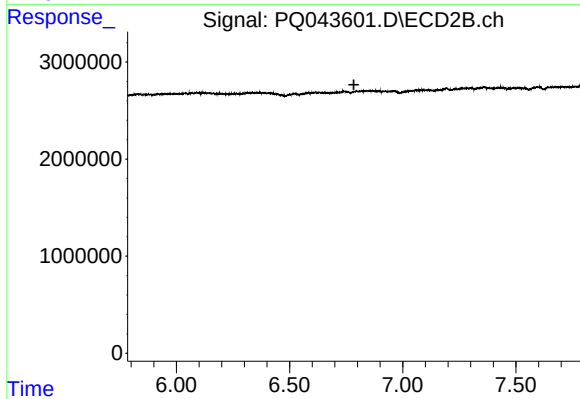

#24 AR-1248-4


R.T.: 6.784 min
Delta R.T.: 0.000 min
Response: -30587
Conc: N.D.

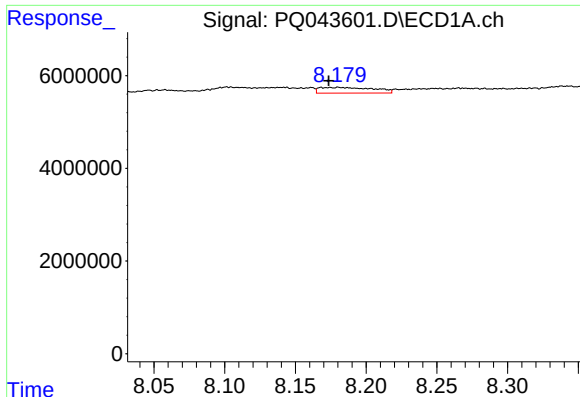

#25 AR-1248-5


R.T.: 8.180 min
Delta R.T.: 0.007 min
Response: 3257472
Conc: 24.57 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

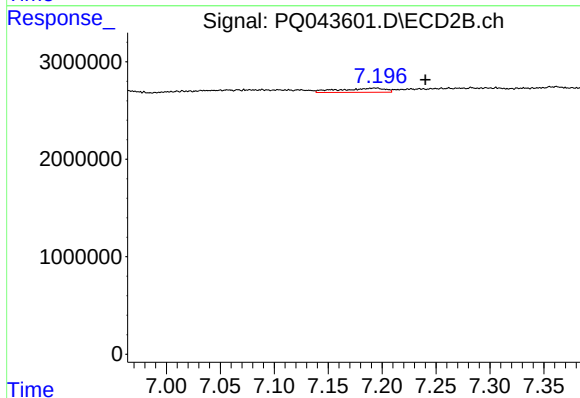


#25 AR-1248-5

R.T.: 7.193 min
Delta R.T.: -0.047 min
Response: 1235152
Conc: 23.92 ng/ml

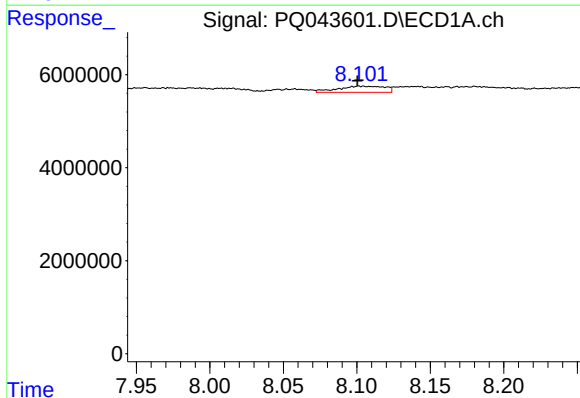


#26 AR-1254-1

R.T.: 8.103 min
Delta R.T.: 0.002 min
Response: 2979522
Conc: 20.27 ng/ml

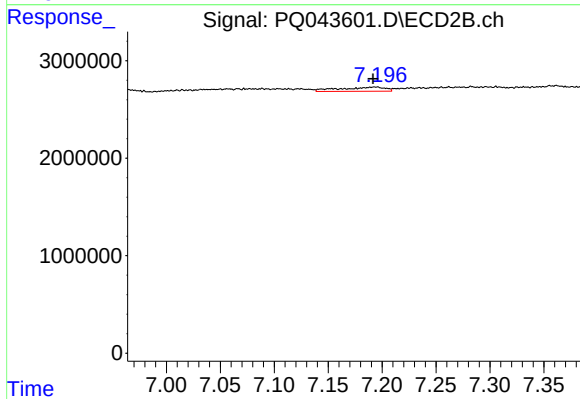

#26 AR-1254-1


R.T.: 7.193 min
Delta R.T.: 0.001 min
Response: 1235152
Conc: 13.87 ng/ml

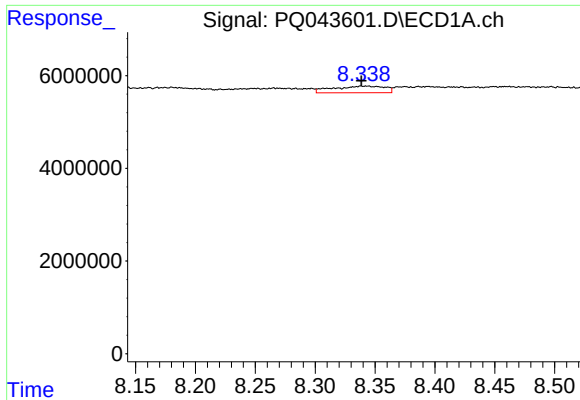

#27 AR-1254-2


R.T.: 8.341 min
Delta R.T.: 0.003 min
Response: 4350304
Conc: 17.77 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

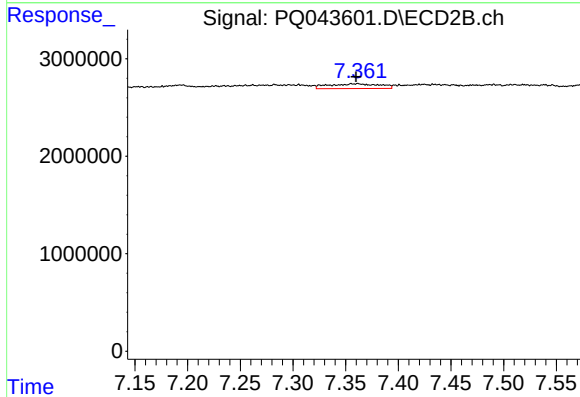


#27 AR-1254-2

R.T.: 7.360 min
Delta R.T.: 0.000 min
Response: 1661008
Conc: 20.43 ng/ml

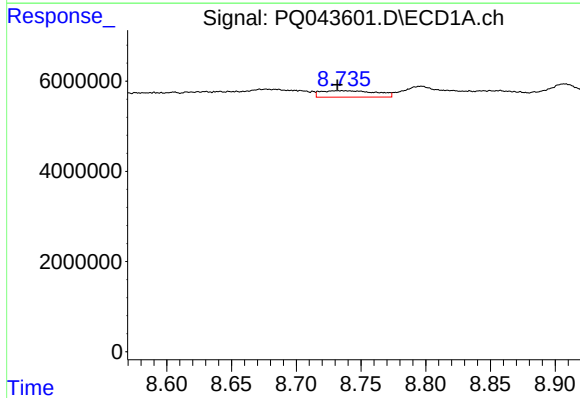


#28 AR-1254-3

R.T.: 8.735 min
Delta R.T.: 0.003 min
Response: 4290735
Conc: 14.88 ng/ml

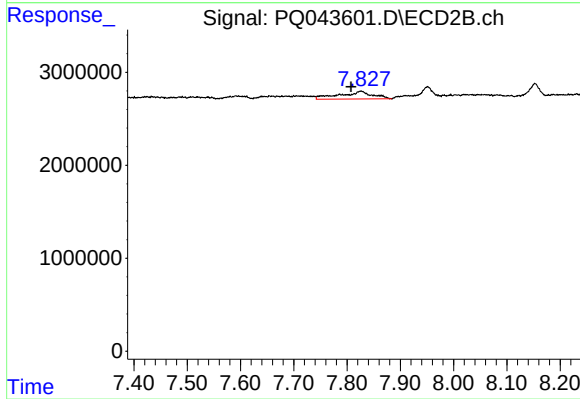

#28 AR-1254-3


R.T.: 7.826 min
Delta R.T.: 0.019 min
Response: 3540471
Conc: 25.07 ng/ml

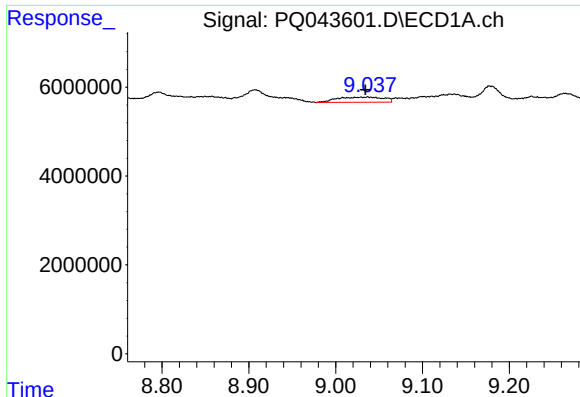

#29 AR-1254-4


R.T.: 9.037 min
Delta R.T.: 0.002 min
Response: 4353886
Conc: 18.65 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

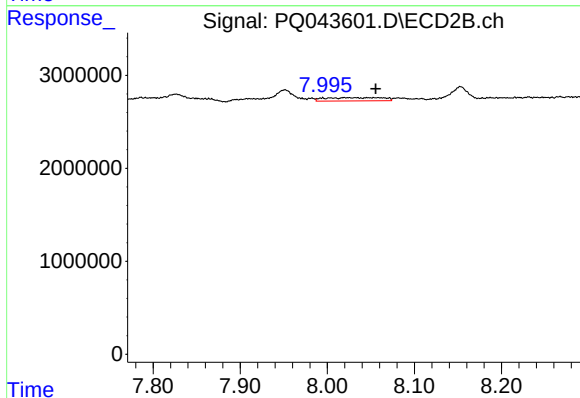


#29 AR-1254-4

R.T.: 8.031 min
Delta R.T.: -0.024 min
Response: 1675131
Conc: 17.18 ng/ml

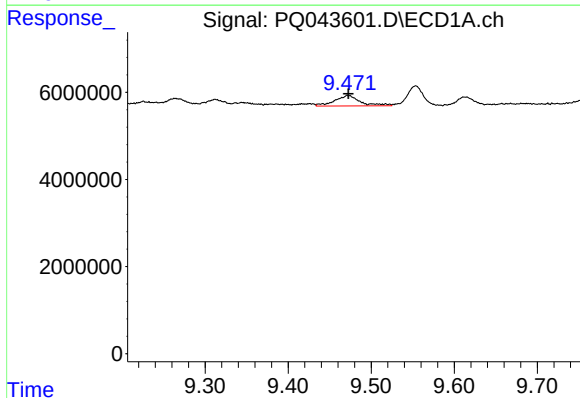


#30 AR-1254-5

R.T.: 9.472 min
Delta R.T.: 0.000 min
Response: 5092047
Conc: 19.15 ng/ml

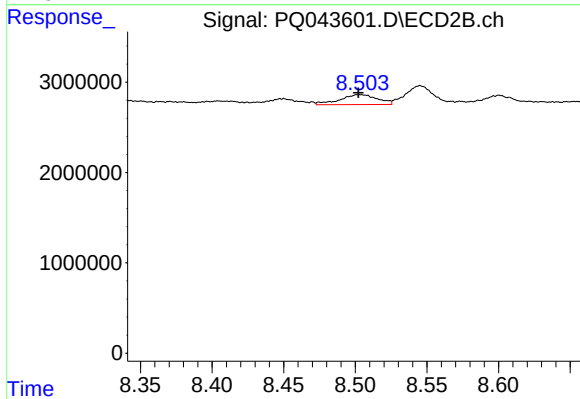

#30 AR-1254-5


R.T.: 8.504 min
Delta R.T.: 0.001 min
Response: 2004829
Conc: 14.45 ng/ml

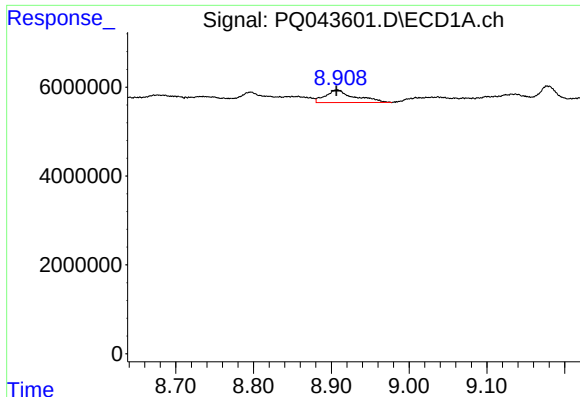

#31 AR-1260-1


R.T.: 8.907 min
Delta R.T.: 0.000 min
Response: 7445570
Conc: 40.17 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

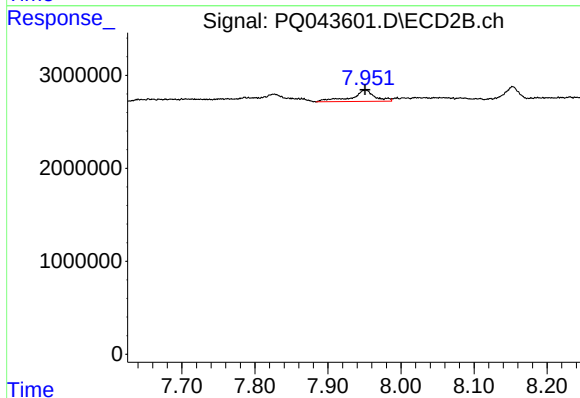


#31 AR-1260-1

R.T.: 7.951 min
Delta R.T.: 0.000 min
Response: 2742318
Conc: 33.64 ng/ml

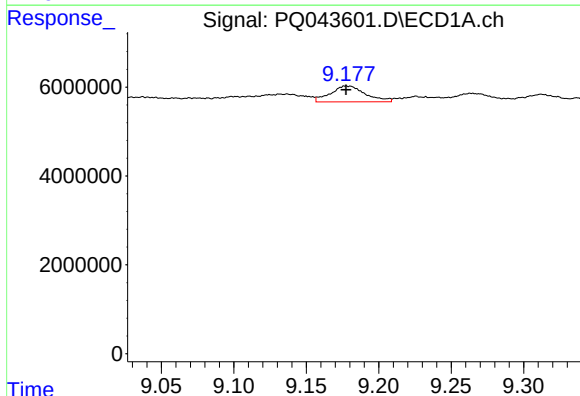


#32 AR-1260-2

R.T.: 9.178 min
Delta R.T.: 0.000 min
Response: 5989271
Conc: 25.41 ng/ml

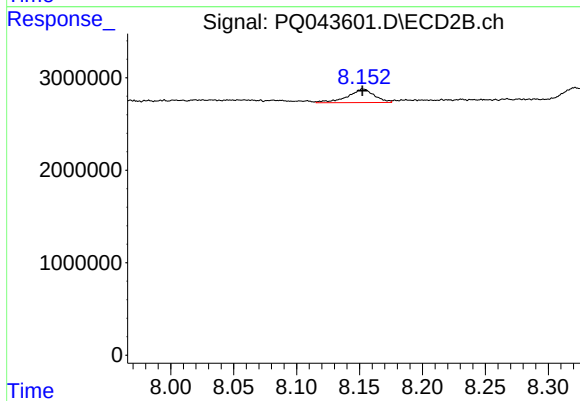

#32 AR-1260-2


R.T.: 8.153 min
Delta R.T.: 0.000 min
Response: 2173393
Conc: 20.48 ng/ml

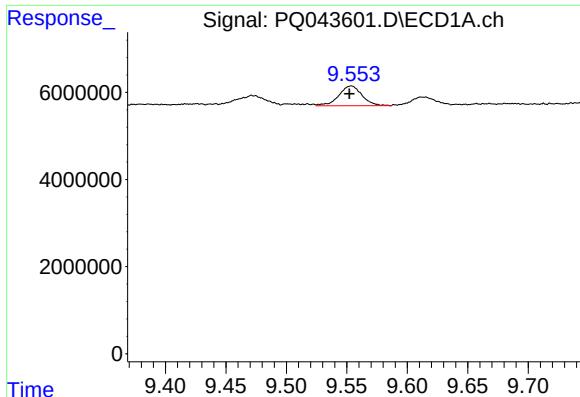

#33 AR-1260-3


R.T.: 9.553 min
Delta R.T.: 0.001 min
Response: 6038313
Conc: 31.65 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

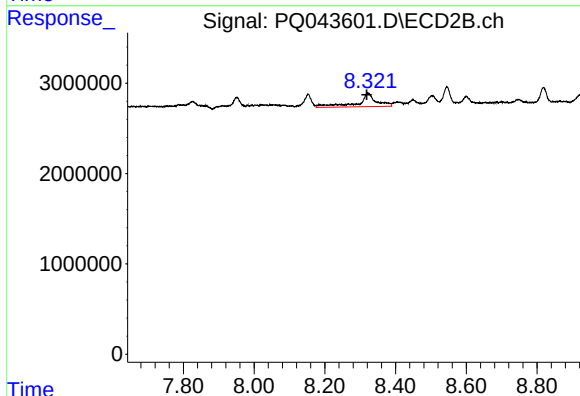


#33 AR-1260-3

R.T.: 8.322 min
Delta R.T.: 0.003 min
Response: 5432777
Conc: 56.71 ng/ml

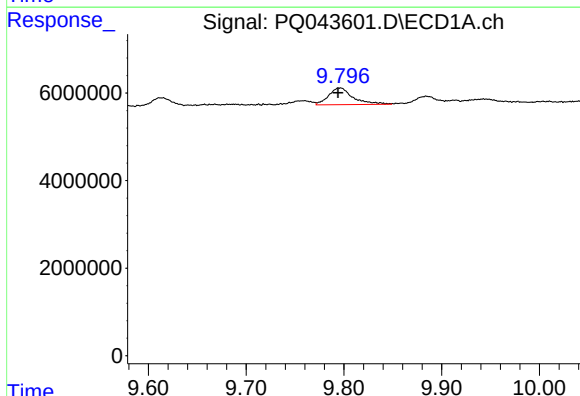


#34 AR-1260-4

R.T.: 9.796 min
Delta R.T.: 0.002 min
Response: 6591487
Conc: 28.55 ng/ml

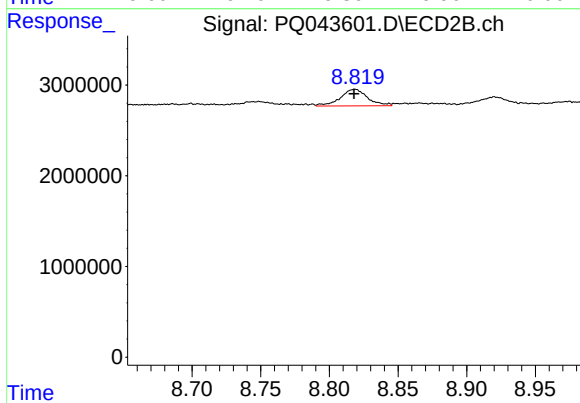

#34 AR-1260-4


R.T.: 8.818 min
Delta R.T.: 0.000 min
Response: 2517315
Conc: 28.77 ng/ml

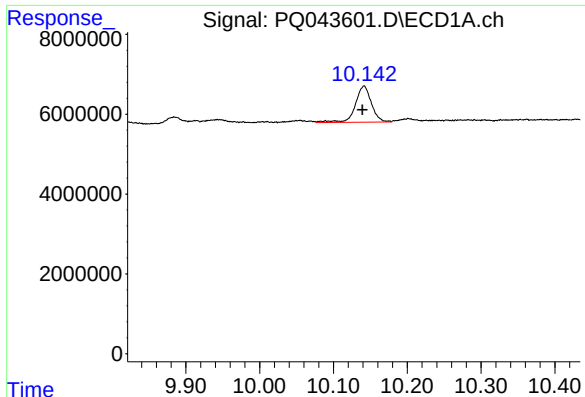

#35 AR-1260-5


R.T.: 10.141 min
Delta R.T.: 0.002 min
Response: 13752716
Conc: 26.00 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

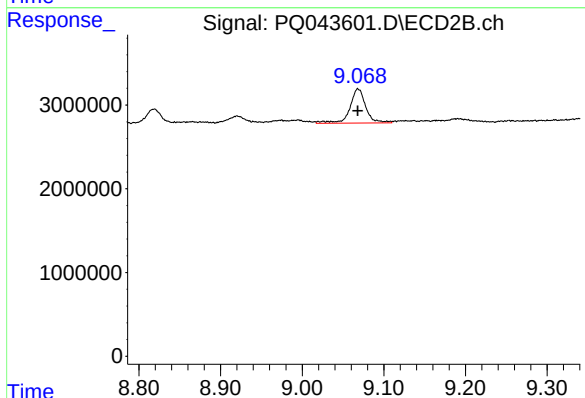


#35 AR-1260-5

R.T.: 9.069 min
Delta R.T.: 0.000 min
Response: 5497935
Conc: 25.08 ng/ml

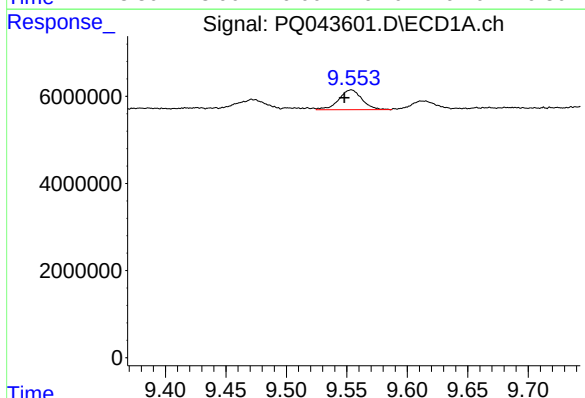


#36 AR-1262-1

R.T.: 9.553 min
Delta R.T.: 0.006 min
Response: 6038313
Conc: 19.10 ng/ml

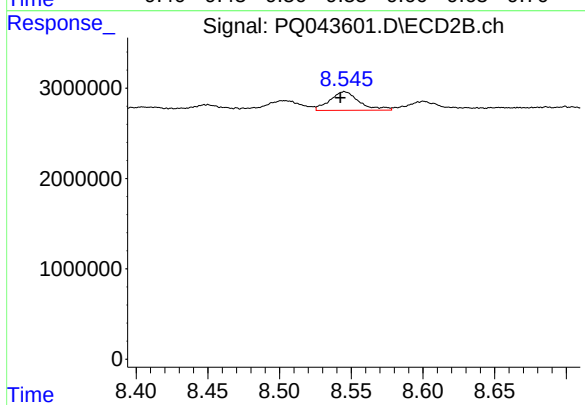

#36 AR-1262-1


R.T.: 8.545 min
Delta R.T.: 0.003 min
Response: 2963008
Conc: 21.12 ng/ml

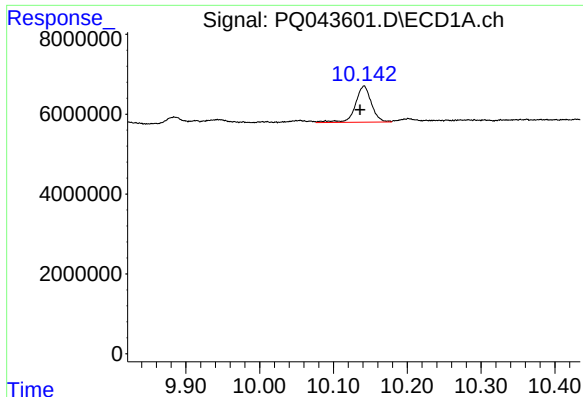

#37 AR-1262-2


R.T.: 10.141 min
Delta R.T.: 0.005 min
Response: 13752716
Conc: 20.14 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

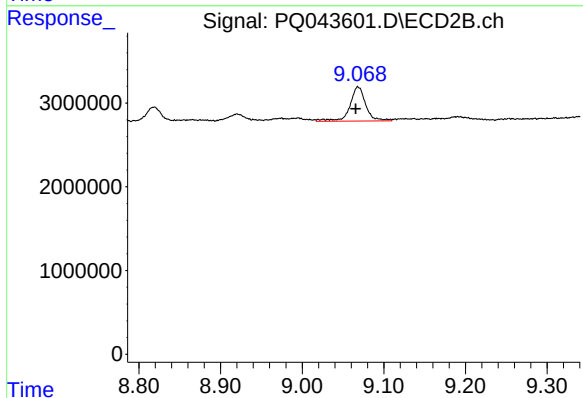


#37 AR-1262-2

R.T.: 9.069 min
Delta R.T.: 0.003 min
Response: 5497935
Conc: 21.18 ng/ml

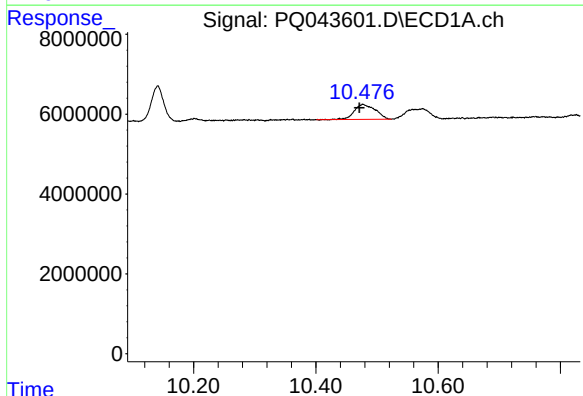


#38 AR-1262-3

R.T.: 10.477 min
Delta R.T.: 0.006 min
Response: 8907563
Conc: 18.80 ng/ml

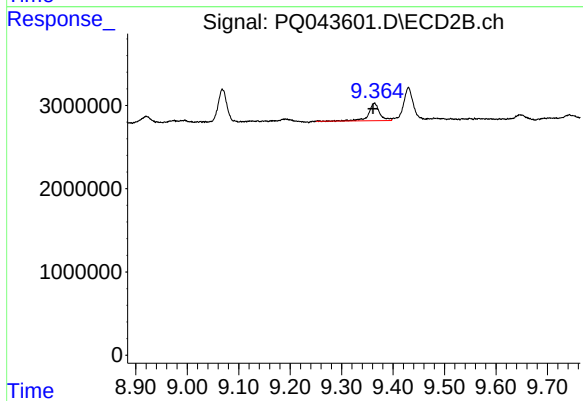

#38 AR-1262-3


R.T.: 9.364 min
Delta R.T.: 0.003 min
Response: 3124495
Conc: 26.57 ng/ml

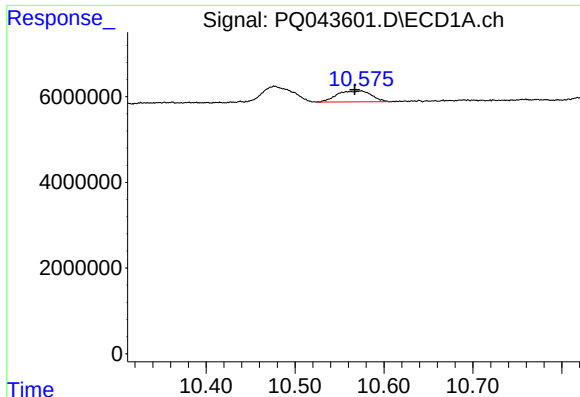

#39 AR-1262-4


R.T.: 10.574 min
Delta R.T.: 0.007 min
Response: 6847005
Conc: 19.00 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

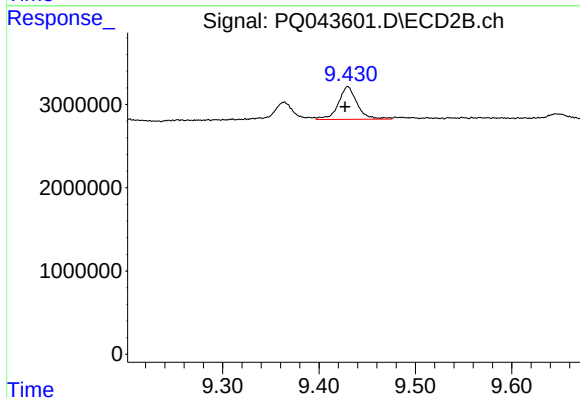


#39 AR-1262-4

R.T.: 9.430 min
Delta R.T.: 0.003 min
Response: 5343168
Conc: 22.52 ng/ml

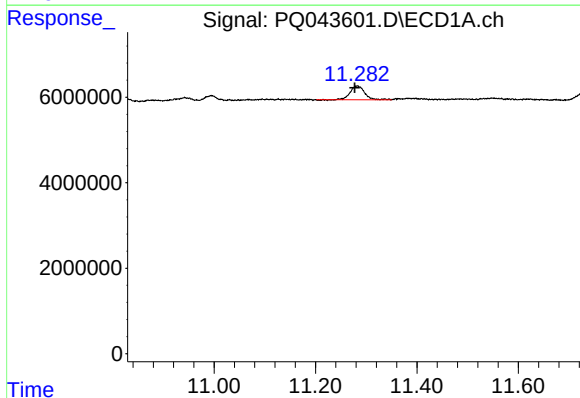


#40 AR-1262-5

R.T.: 11.282 min
Delta R.T.: 0.005 min
Response: 6456869
Conc: 21.74 ng/ml

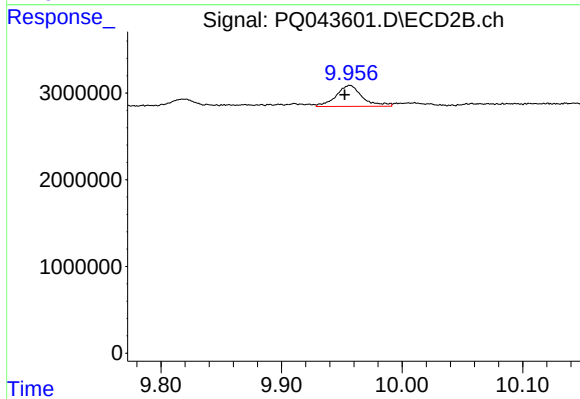

#40 AR-1262-5


R.T.: 9.956 min
Delta R.T.: 0.004 min
Response: 3675591
Conc: 25.14 ng/ml

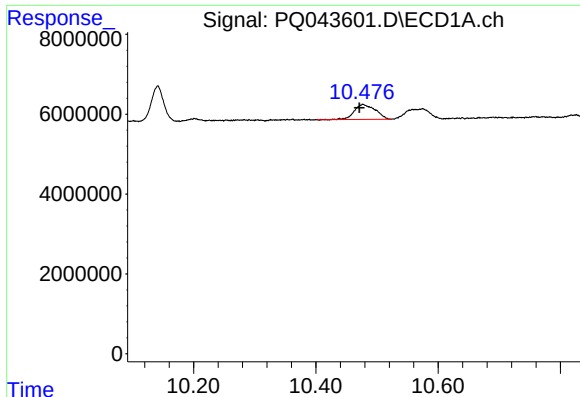

#41 AR-1268-1


R.T.: 10.477 min
Delta R.T.: 0.006 min
Response: 8907563
Conc: 11.09 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

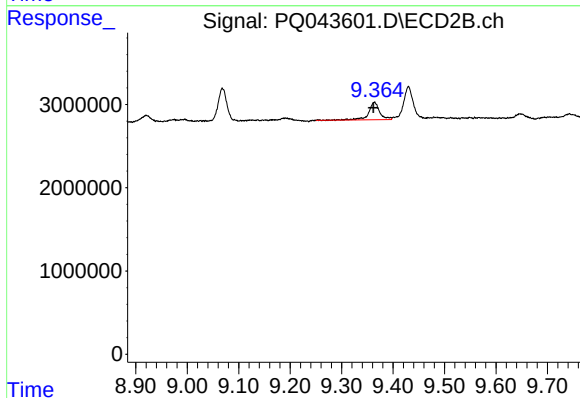


#41 AR-1268-1

R.T.: 9.364 min
Delta R.T.: 0.002 min
Response: 3124495
Conc: 9.63 ng/ml

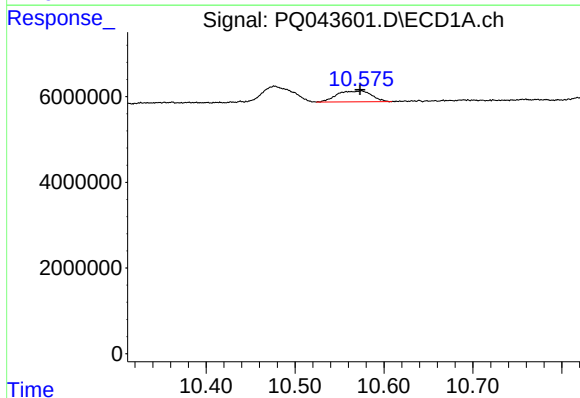


#42 AR-1268-2

R.T.: 10.574 min
Delta R.T.: 0.000 min
Response: 6847005
Conc: 8.88 ng/ml

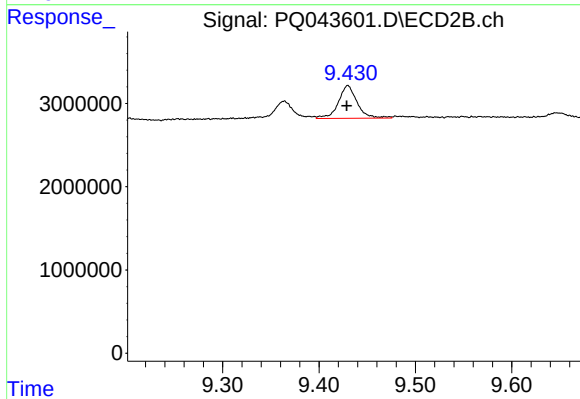

#42 AR-1268-2


R.T.: 9.430 min
Delta R.T.: 0.001 min
Response: 5343168
Conc: 17.06 ng/ml

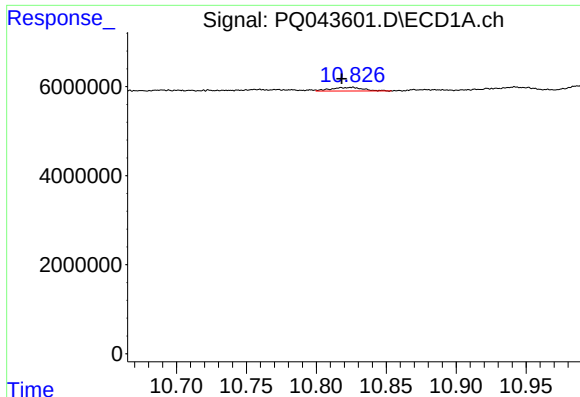

#43 AR-1268-3


R.T.: 10.824 min
Delta R.T.: 0.006 min
Response: 1263974
Conc: 1.92 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

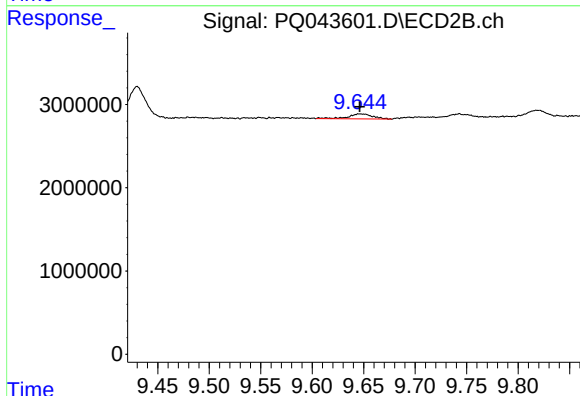


#43 AR-1268-3

R.T.: 9.648 min
Delta R.T.: 0.001 min
Response: 982318
Conc: 3.48 ng/ml

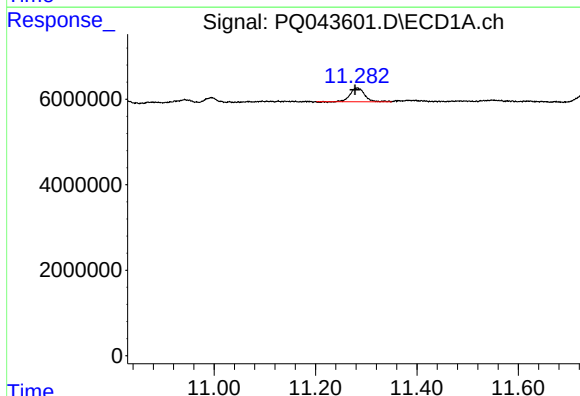


#44 AR-1268-4

R.T.: 11.282 min
Delta R.T.: 0.004 min
Response: 6456869
Conc: 20.11 ng/ml

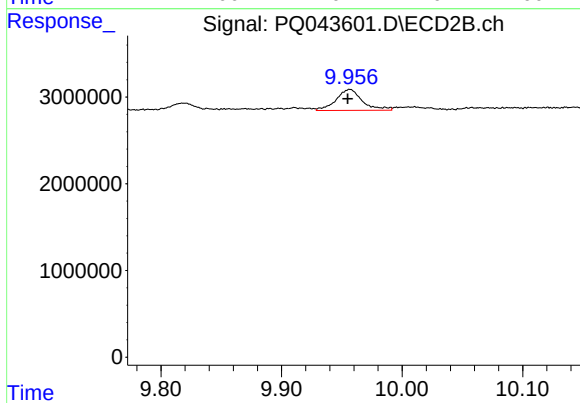

#44 AR-1268-4


R.T.: 9.956 min
Delta R.T.: 0.001 min
Response: 3675591
Conc: 23.29 ng/ml

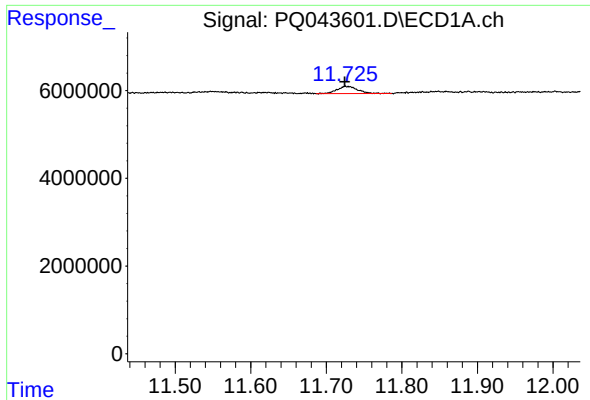

#45 AR-1268-5

R.T.: 11.727 min
Delta R.T.: 0.003 min
Response: 3169846
Conc: 1.19 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

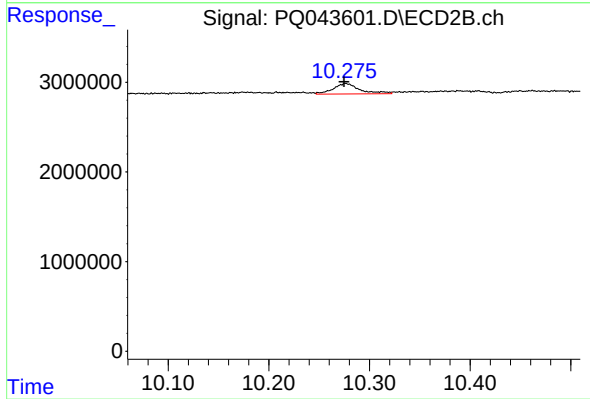

#45 AR-1268-5

R.T.: 10.277 min
Delta R.T.: 0.002 min
Response: 2121580
Conc: 1.74 ng/ml